
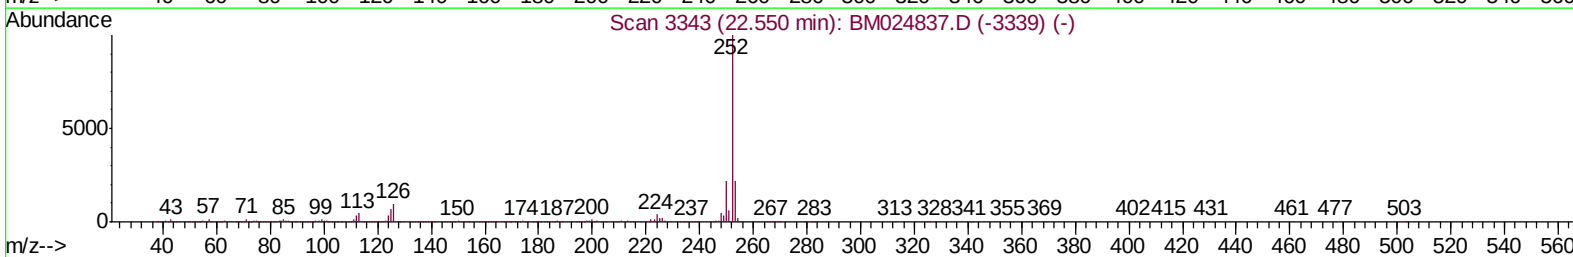
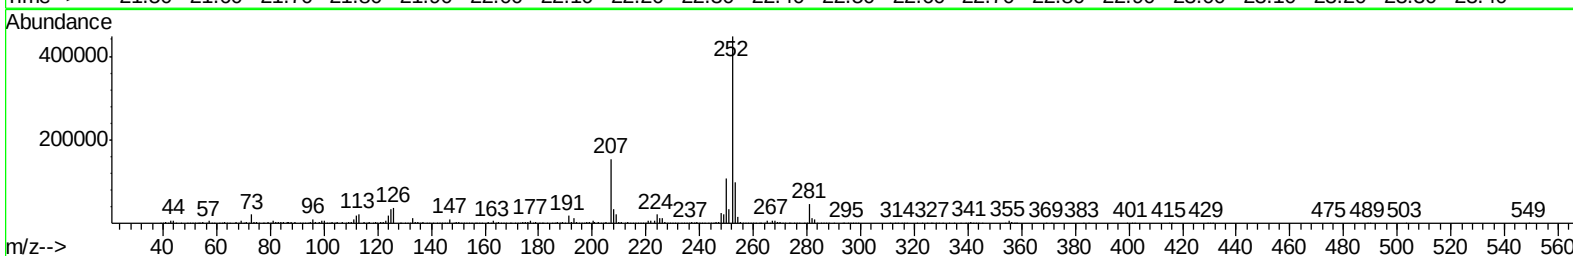


Data File : BM024841.D
Acq On : 11 Feb 2020 19:15
Operator : CG/JU
Sample : L1405-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 12 04:42:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 04:40:07 2020
Response via : Initial Calibration

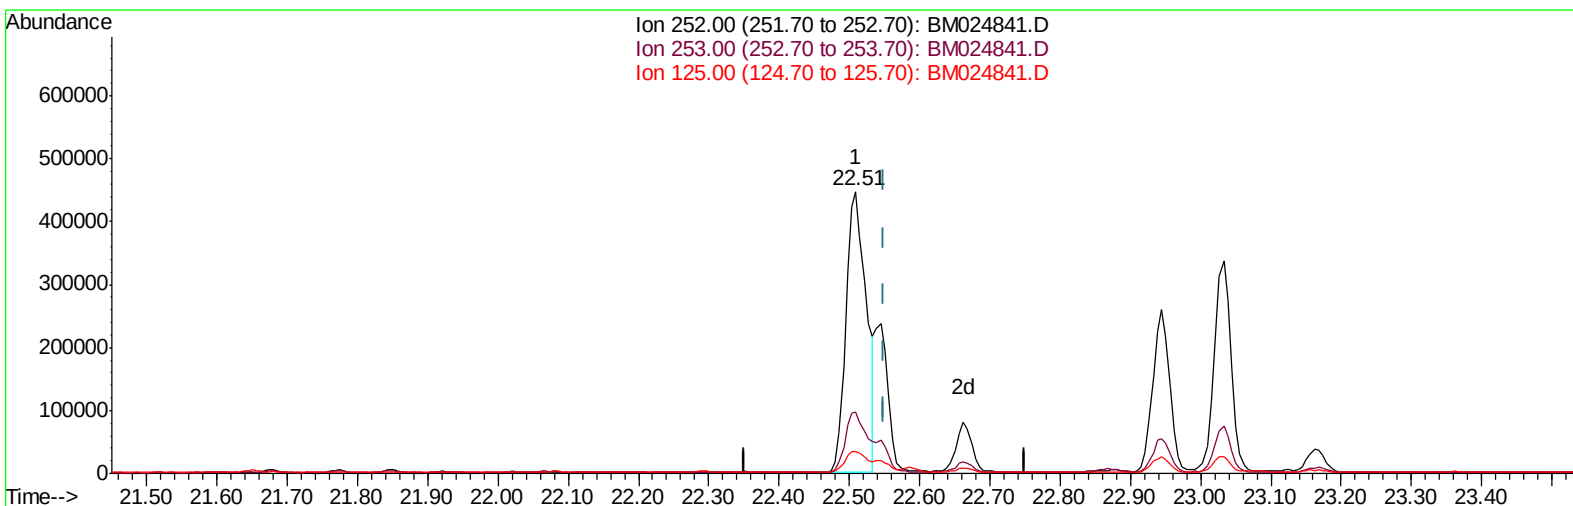

TIC: BM024841.D

(89) Benzo(k)fluoranthene
22.509min (-0.041) 9.35ng/ul
response 908793

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	21.95
125.00	6.40	7.68
0.00	0.00	0.00