
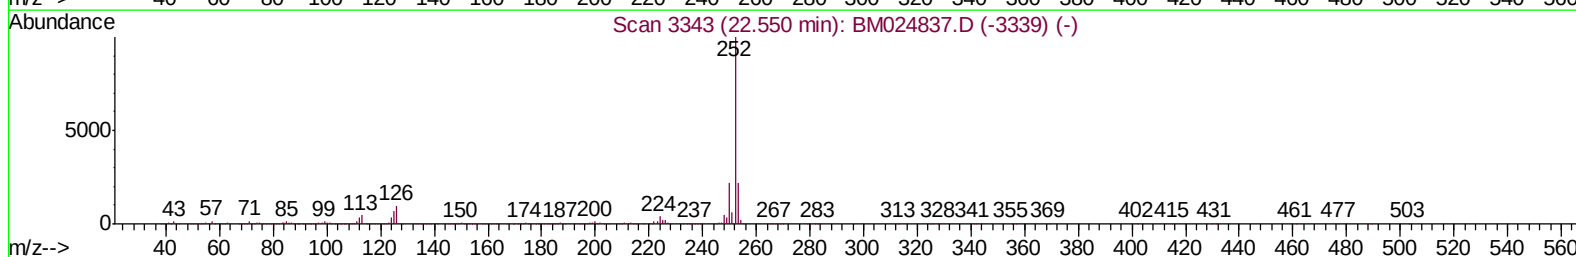
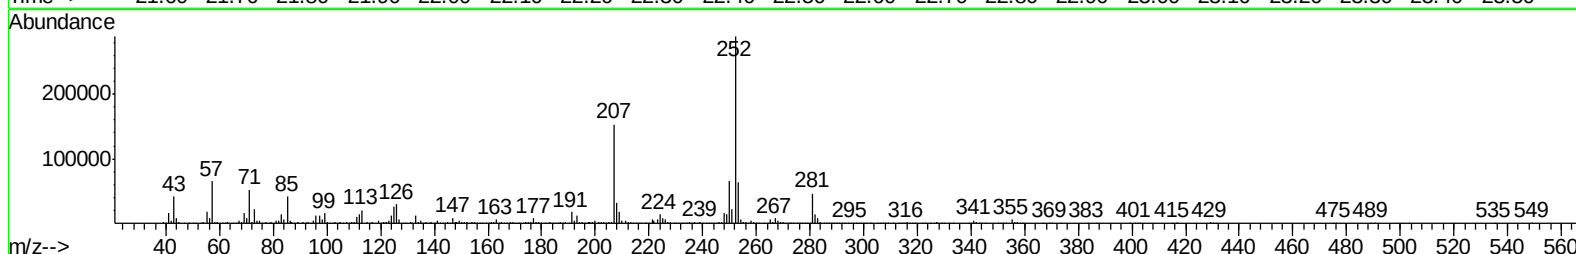


Data File : BM024844.D
Acq On : 11 Feb 2020 21:04
Operator : CG/JU
Sample : L1405-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Feb 12 04:43:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 04:40:07 2020
Response via : Initial Calibration

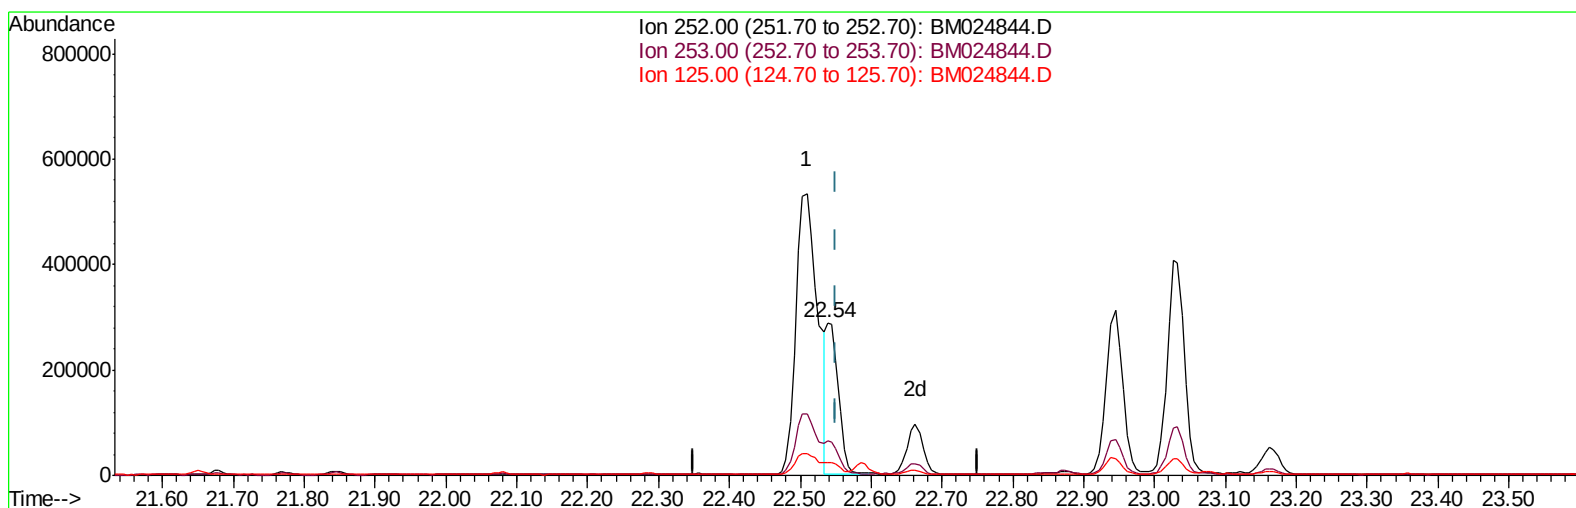

TIC: BM024844.D

(89) Benzo(k)fluoranthene

22.539min (-0.012) 2.93ng/ul m

response 352481

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	22.31
125.00	6.40	8.82#
0.00	0.00	0.00