
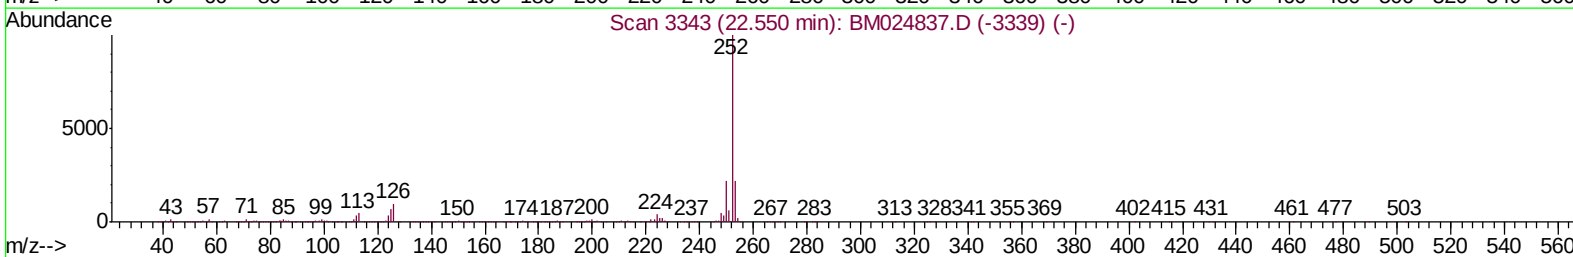
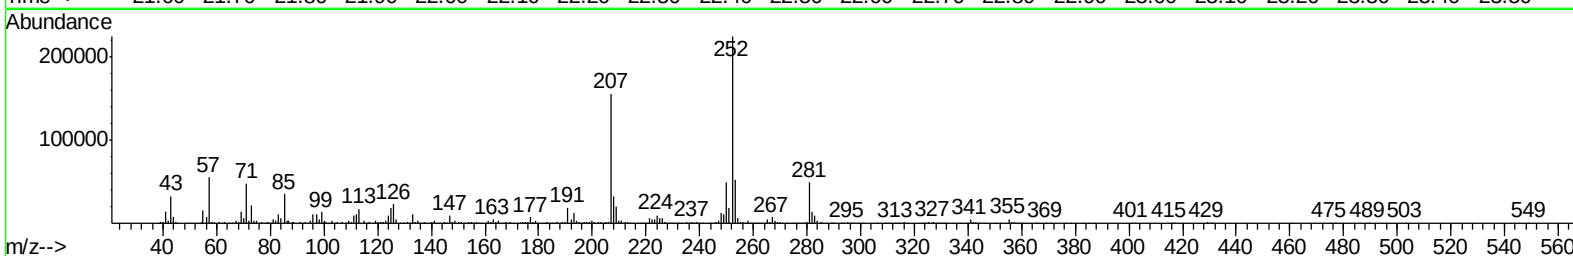


Data File : BM024845.D
Acq On : 11 Feb 2020 21:40
Operator : CG/JU
Sample : L1405-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 12 04:43:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 04:40:07 2020
Response via : Initial Calibration

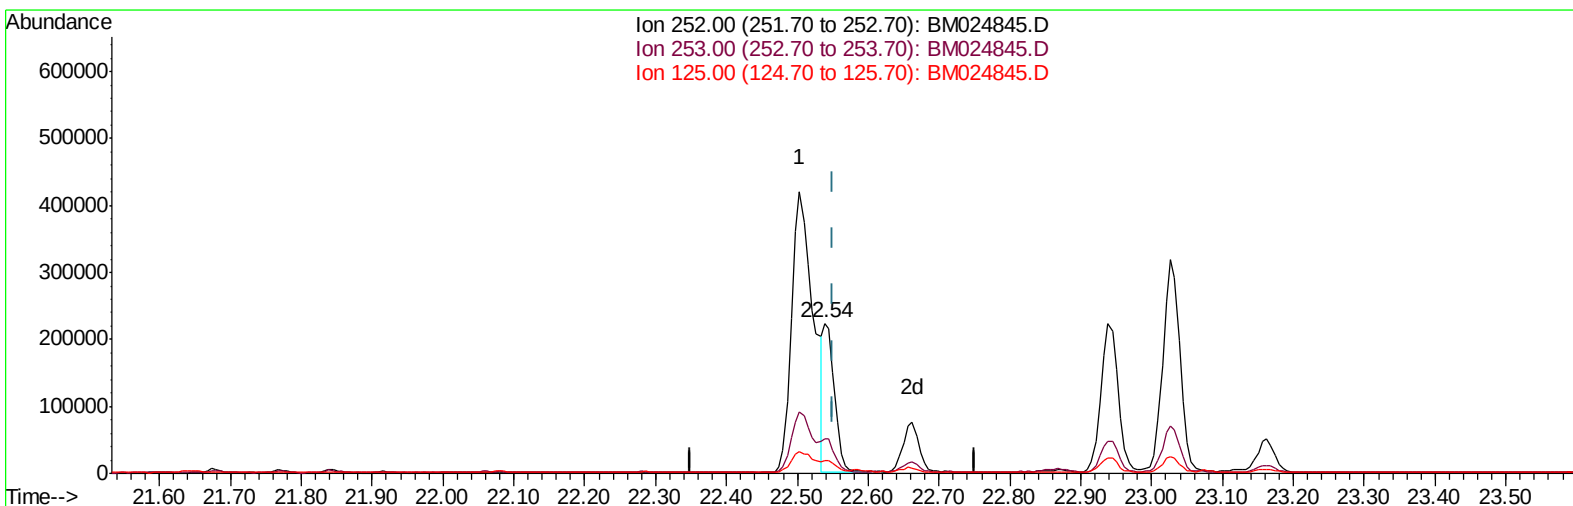

TIC: BM024845.D

(89) Benzo(k)fluoranthene

22.538min (-0.012) 2.45ng/ul m

response 252292

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	23.14
125.00	6.40	8.49#
0.00	0.00	0.00