
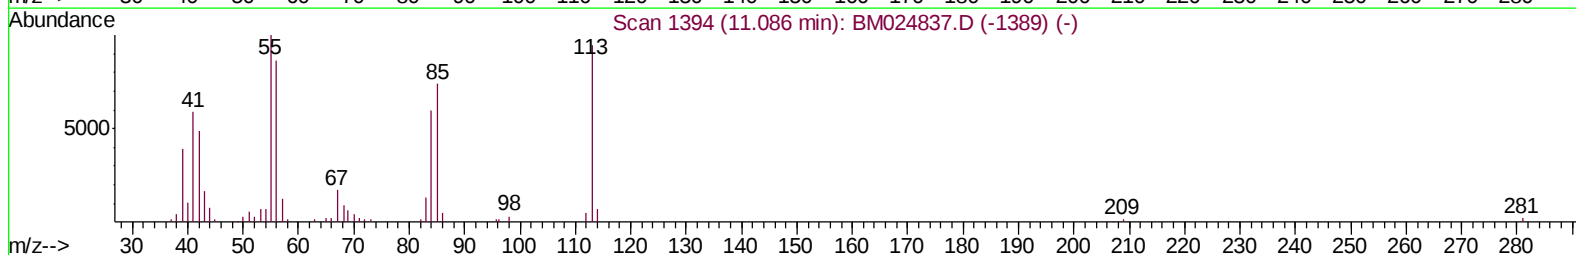
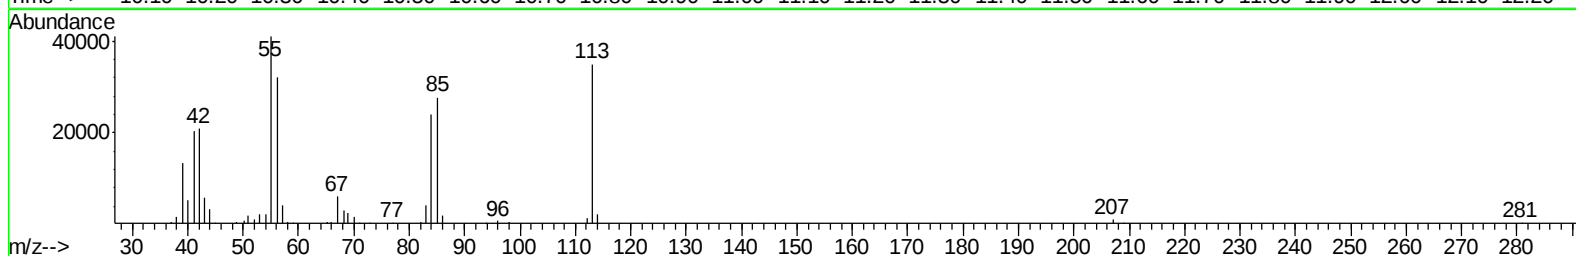


Data File : BM024854.D
Acq On : 12 Feb 2020 03:05
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 12 04:44:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 04:40:07 2020
Response via : Initial Calibration

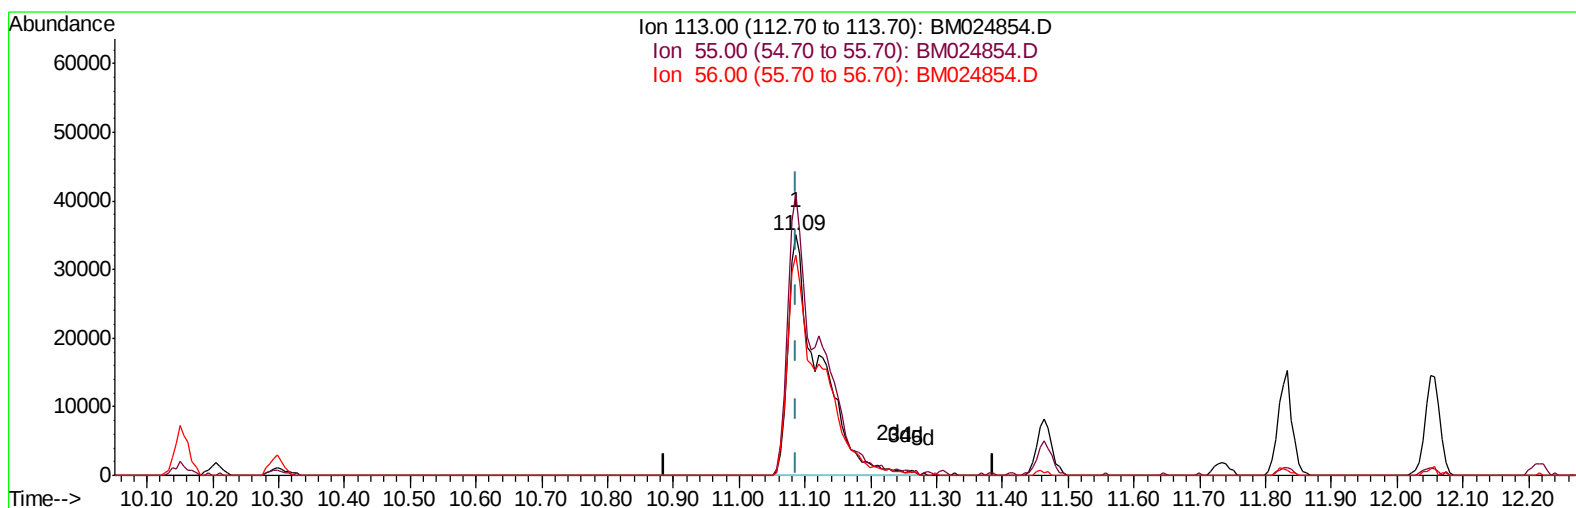

TIC: BM024854.D

(32) Caprolactam

11.086min (+0.000) 21.43ng/ul m

response 116445

Ion	Exp%	Act%
113.00	100	100
55.00	107.70	117.24
56.00	89.90	91.93
0.00	0.00	0.00