

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021120\
 Data File : BM024853.D
 Acq On : 12 Feb 2020 02:29
 Operator : CG/JU
 Sample : L1405-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6Y1

Quant Time: Feb 12 04:44:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 12 04:40:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	327135	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	1272372	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.05	164	816016	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.80	188	1711479	20.00	ng/ul	0.00
78) Chrysene-d12	21.02	240	1671788	20.00	ng/ul	0.00
86) Perylene-d12	23.11	264	1746127	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.01	96	42289	6.22	ng/uL	0.00
5) Phenol-d5	6.59	99	748408	34.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.75	67	447087	36.43	ng/ul	0.00
9) 2-Chlorophenol-d4	6.94	132	679529	34.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.11	113	633410	34.54	ng/ul	0.00
19) Nitrobenzene-d5	8.54	128	335139	36.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.25	143	396560	36.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.79	165	712259	32.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.30	131	905112	44.12	ng/ul	0.00
44) Dimethylphthalate-d6	13.47	166	2130108	34.58	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	2585393	35.94	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	302550	30.23	ng/ul	0.00
58) Fluorene-d10	15.06	176	1858716	34.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	321912	28.86	ng/ul	0.00
71) Anthracene-d10	16.90	188	2783840	35.63	ng/ul	0.00
79) Pyrene-d10	19.21	212	3008991	35.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.99	264	3187035	36.34	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.52	163	122130	1.901	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021120\
Data File : BM024853.D
Acq On : 12 Feb 2020 02:29
Operator : CG/JU
Sample : L1405-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB6Y1

Quant Time: Feb 12 04:44:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 04:40:07 2020
Response via : Initial Calibration

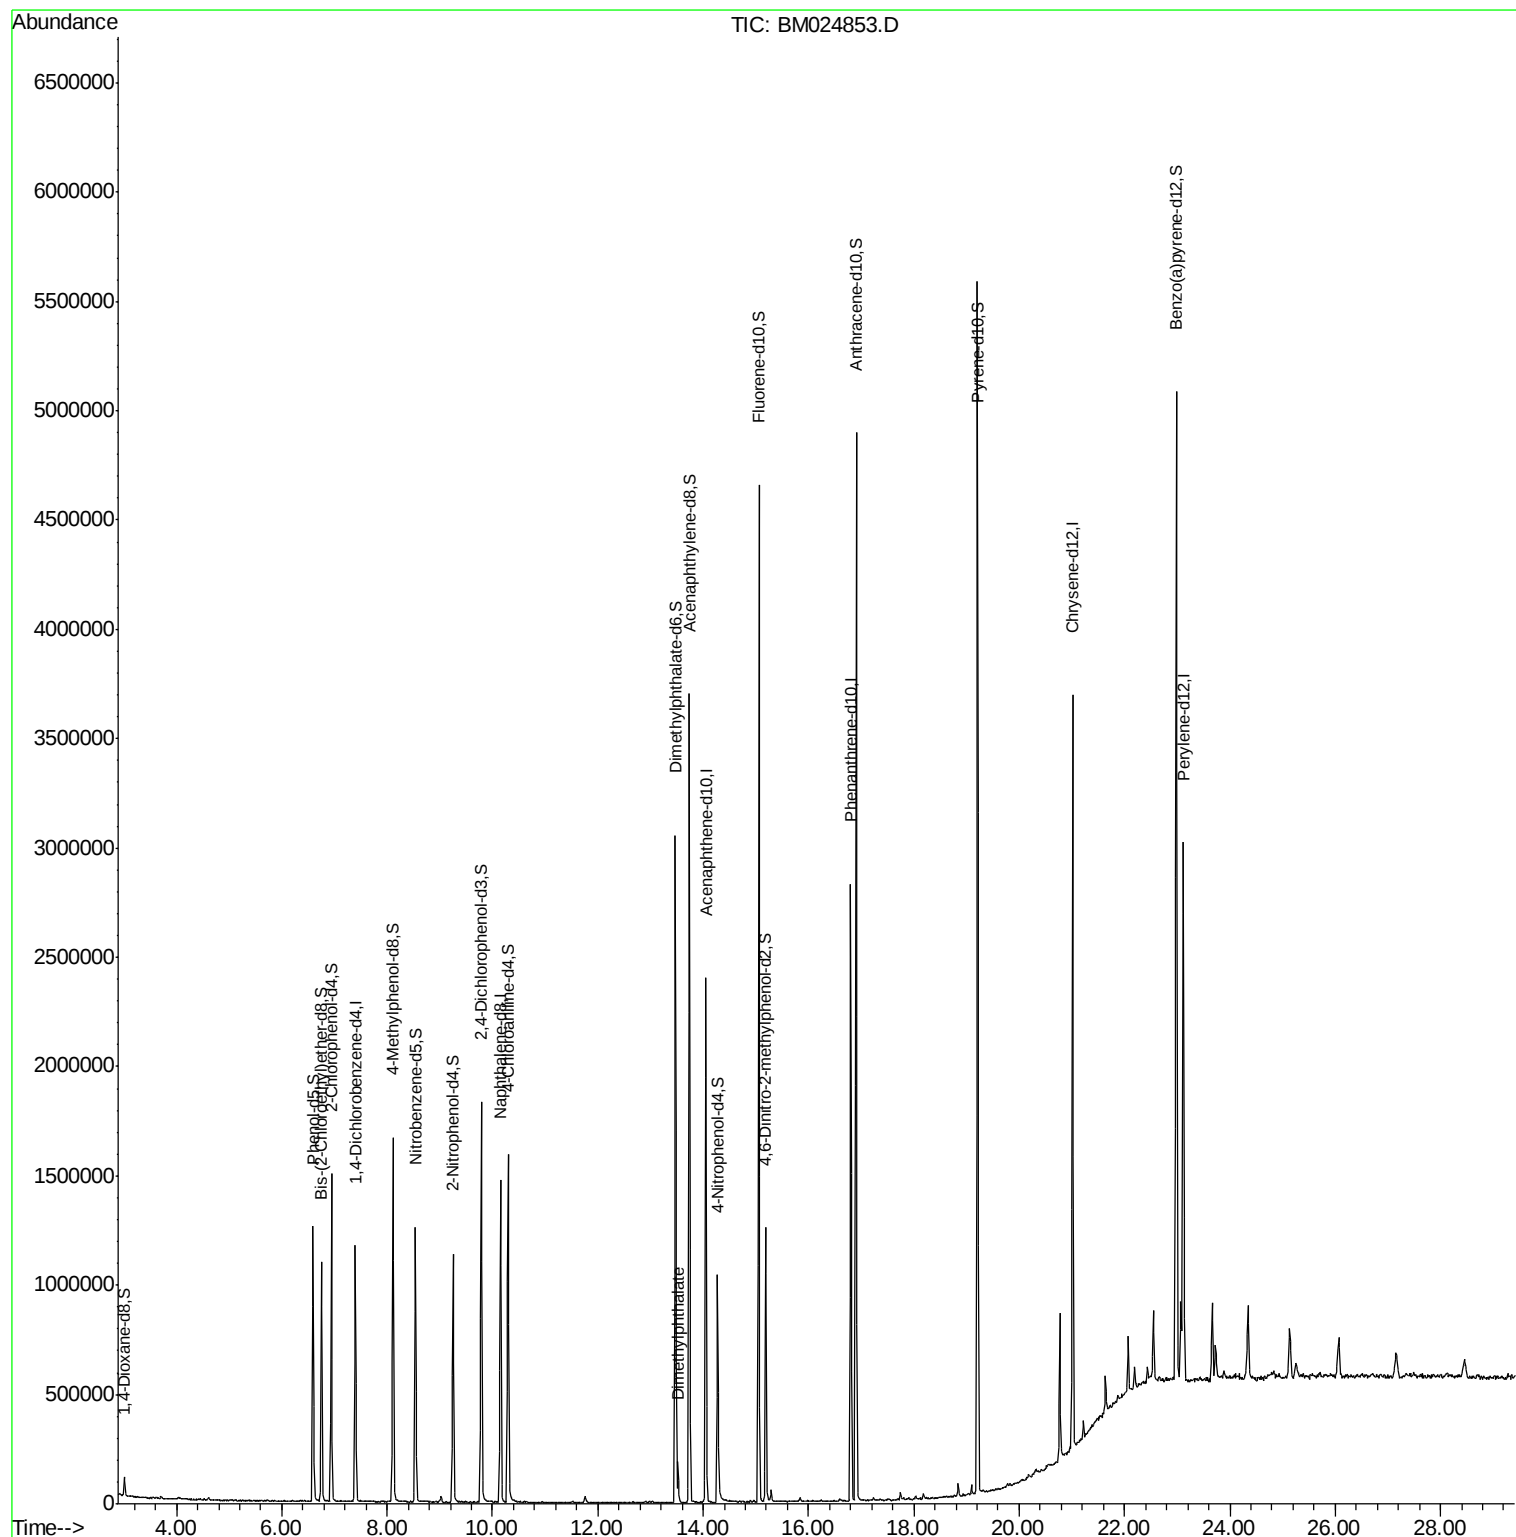

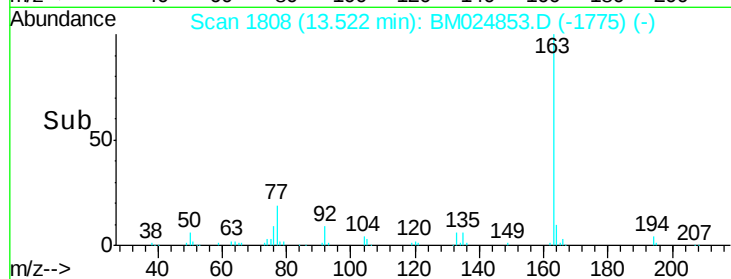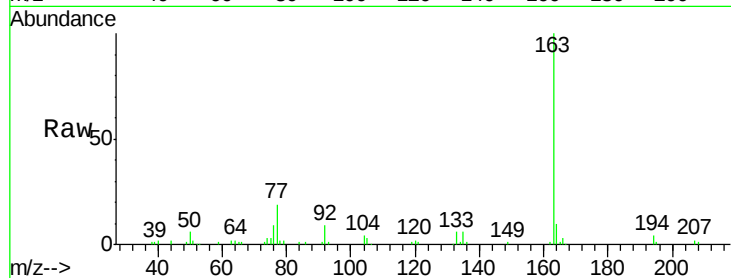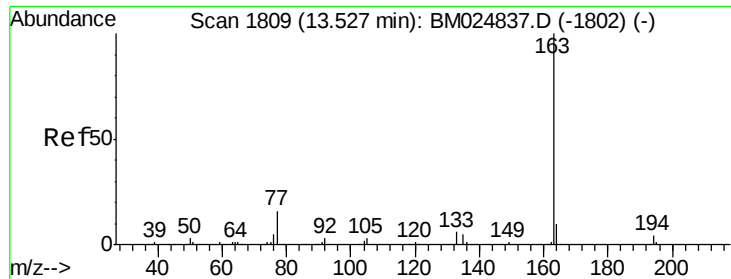

#45

Dimethylphthalate

Concen: 1.901 ng/ul

RT: 13.52 min Scan# 1808

Delta R.T. -0.01 min

Lab File: BM024853.D

Acq: 12 Feb 2020 02:29

Instrument :

BNA_M

ClientSampleId :

CB6Y1

Tot Ion:163 Resp: 122130

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 9.7 8.2 12.2

