

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021216\
 Data File : BM004239.D
 Acq On : 12 Feb 2016 21:50
 Operator : SJ/IZ
 Sample : H1416-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9QD0

Quant Time: Feb 13 01:02:32 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 12 22:29:16 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	25642	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	113424	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	66092	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.06	188	137328	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	127216	20.00	ng/ul	0.00
86) Perylene-d12	23.50	264	123880	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.11	96	775	1.52	ng/uL	0.00
5) Phenol-d5	6.83	99	14431	7.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	37423	33.64	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	50489	27.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	30828	17.57	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	29799	34.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	34027	34.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	54773	31.15	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	210256	38.23	ng/ul	0.00
47) Acenaphthylene-d8	14.00	160	227195	34.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	4958	5.57	ng/ul	0.00
58) Fluorene-d10	15.30	176	176149	38.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.44	200	25368	30.33	ng/ul	0.00
71) Anthracene-d10	17.16	188	252159	37.56	ng/ul	0.00
79) Pyrene-d10	19.47	212	260693	38.61	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	253911	38.41	ng/ul	0.00


Target Compounds					Qvalue
46) 2,6-Dinitrotoluene	13.72	165	1208	1.07 ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021216\
Data File : BM004239.D
Acq On : 12 Feb 2016 21:50
Operator : SJ/IZ
Sample : H1416-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9QD0

Quant Time: Feb 13 01:02:32 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 12 22:29:16 2016
Response via : Initial Calibration

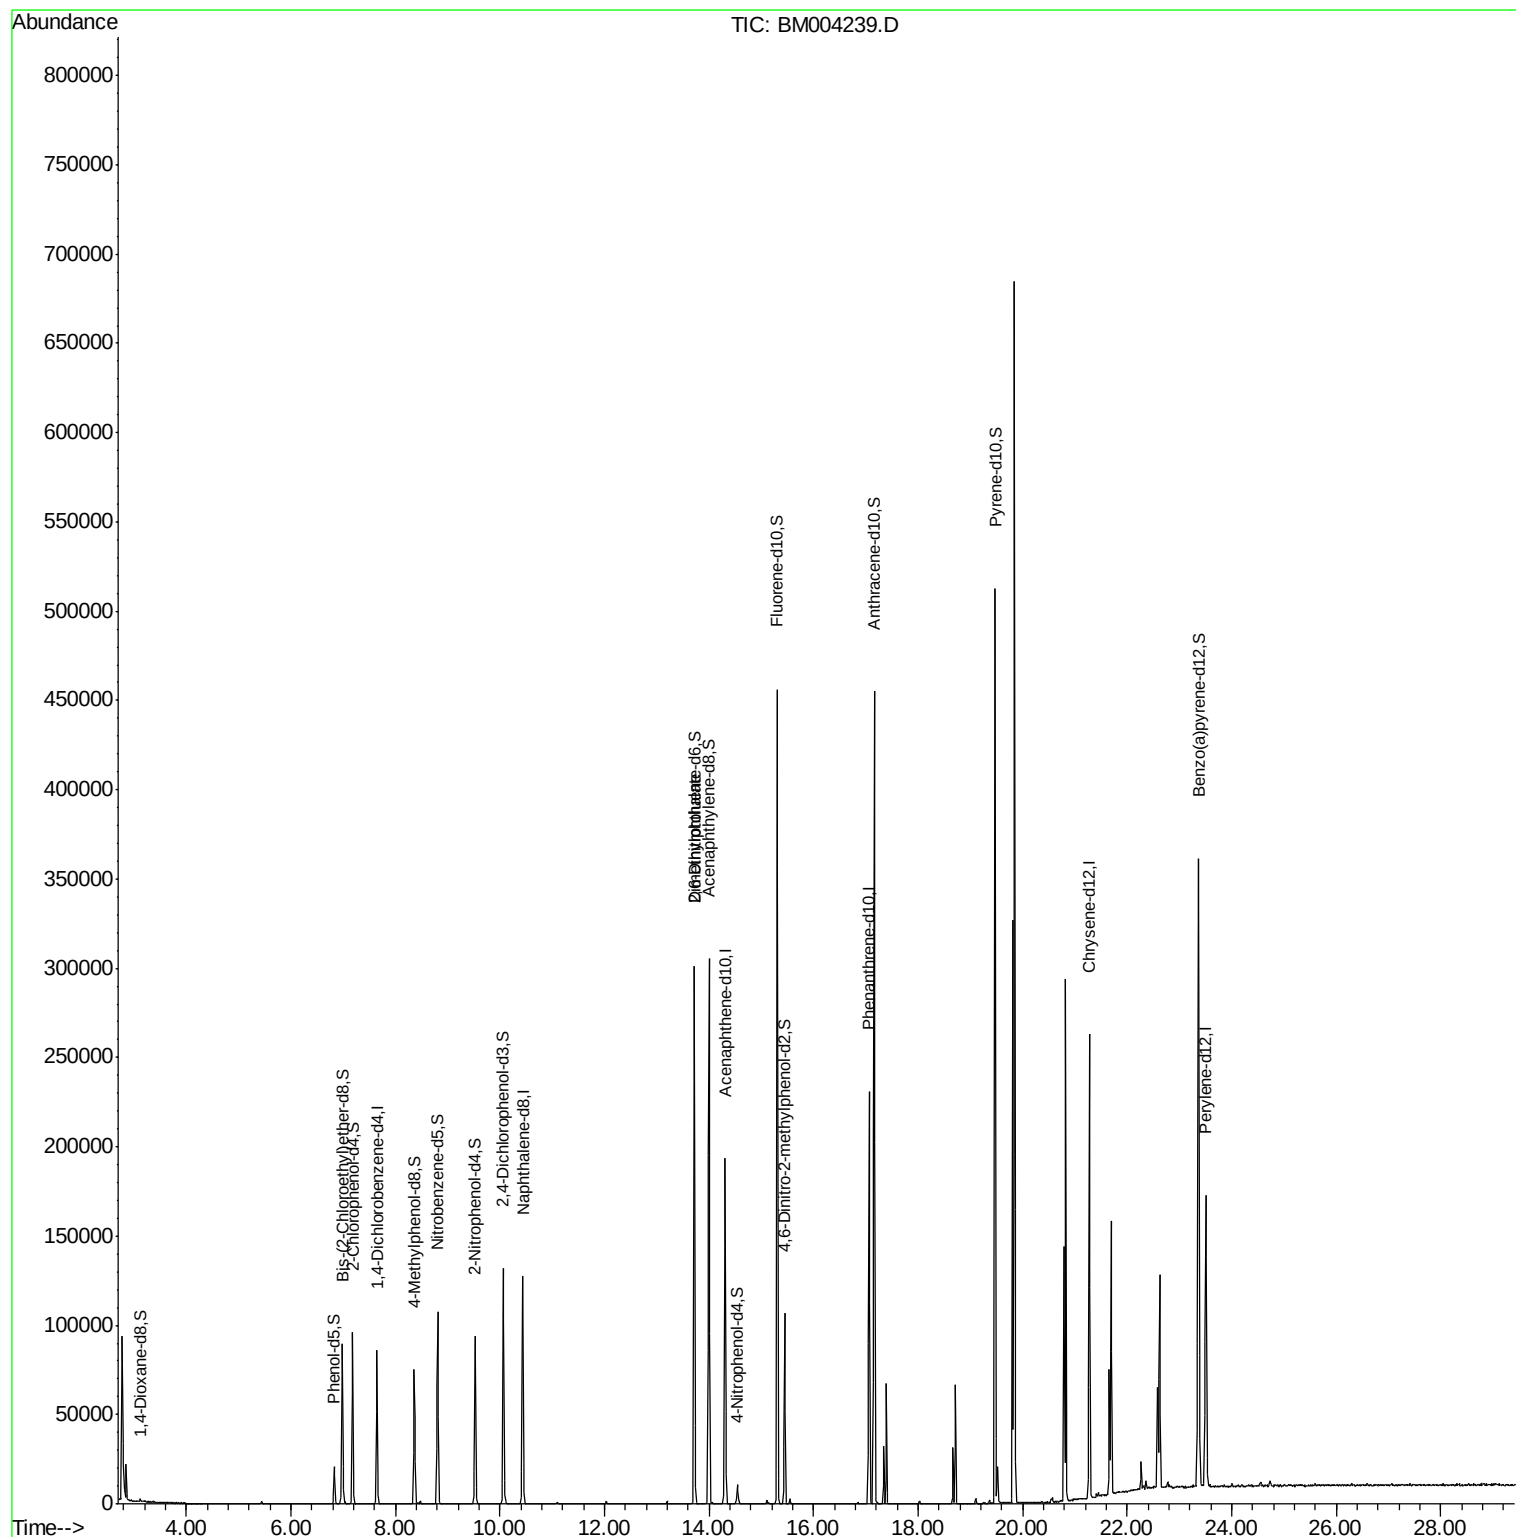

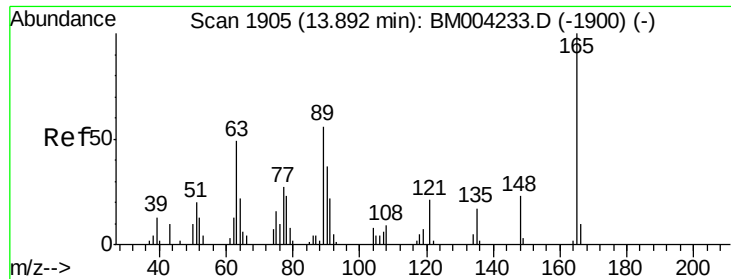

#46
 2,6-Dinitrotoluene
 Concen: 1.07 ng/ul
 RT: 13.72 min Scan# 1876
 Delta R.T. -0.17 min
 Lab File: BM004239.D
 Acq: 12 Feb 2016 21:50

Instrument :
 BNA_M
 ClientSampleId :
 D9QD0

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	42.4	63.6#
121	0.0	16.6	24.8#

