

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021216\
 Data File : BM004241.D
 Acq On : 12 Feb 2016 23:02
 Operator : SJ/IZ
 Sample : H1414-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9QD9

Quant Time: Feb 13 01:02:46 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 12 22:29:16 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	26211	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	117671	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	67812	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.06	188	136702	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	133723	20.00	ng/ul	0.00
86) Perylene-d12	23.50	264	134402	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.11	96	1644	3.16	ng/uL	0.00
5) Phenol-d5	6.82	99	35519	16.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	19916	17.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	32423	17.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	31205	17.40	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	15023	16.60	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	17102	16.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	30228	16.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	41746	19.23	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	104695	18.55	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	126207	18.41	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	12107	13.26	ng/ul	0.00
58) Fluorene-d10	15.30	176	89708	18.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.44	200	10598	12.73	ng/ul	0.00
71) Anthracene-d10	17.16	188	128302	19.20	ng/ul	0.00
79) Pyrene-d10	19.46	212	134723	18.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	137222	19.13	ng/ul	0.00


Target Compounds						Qvalue
2) 1,4-Dioxane	2.85	88	861	1.41	ng/uL#	1
45) Dimethylphthalate	13.76	163	35087	5.95	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021216\
Data File : BM004241.D
Acq On : 12 Feb 2016 23:02
Operator : SJ/IZ
Sample : H1414-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9QD9

Quant Time: Feb 13 01:02:46 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 12 22:29:16 2016
Response via : Initial Calibration

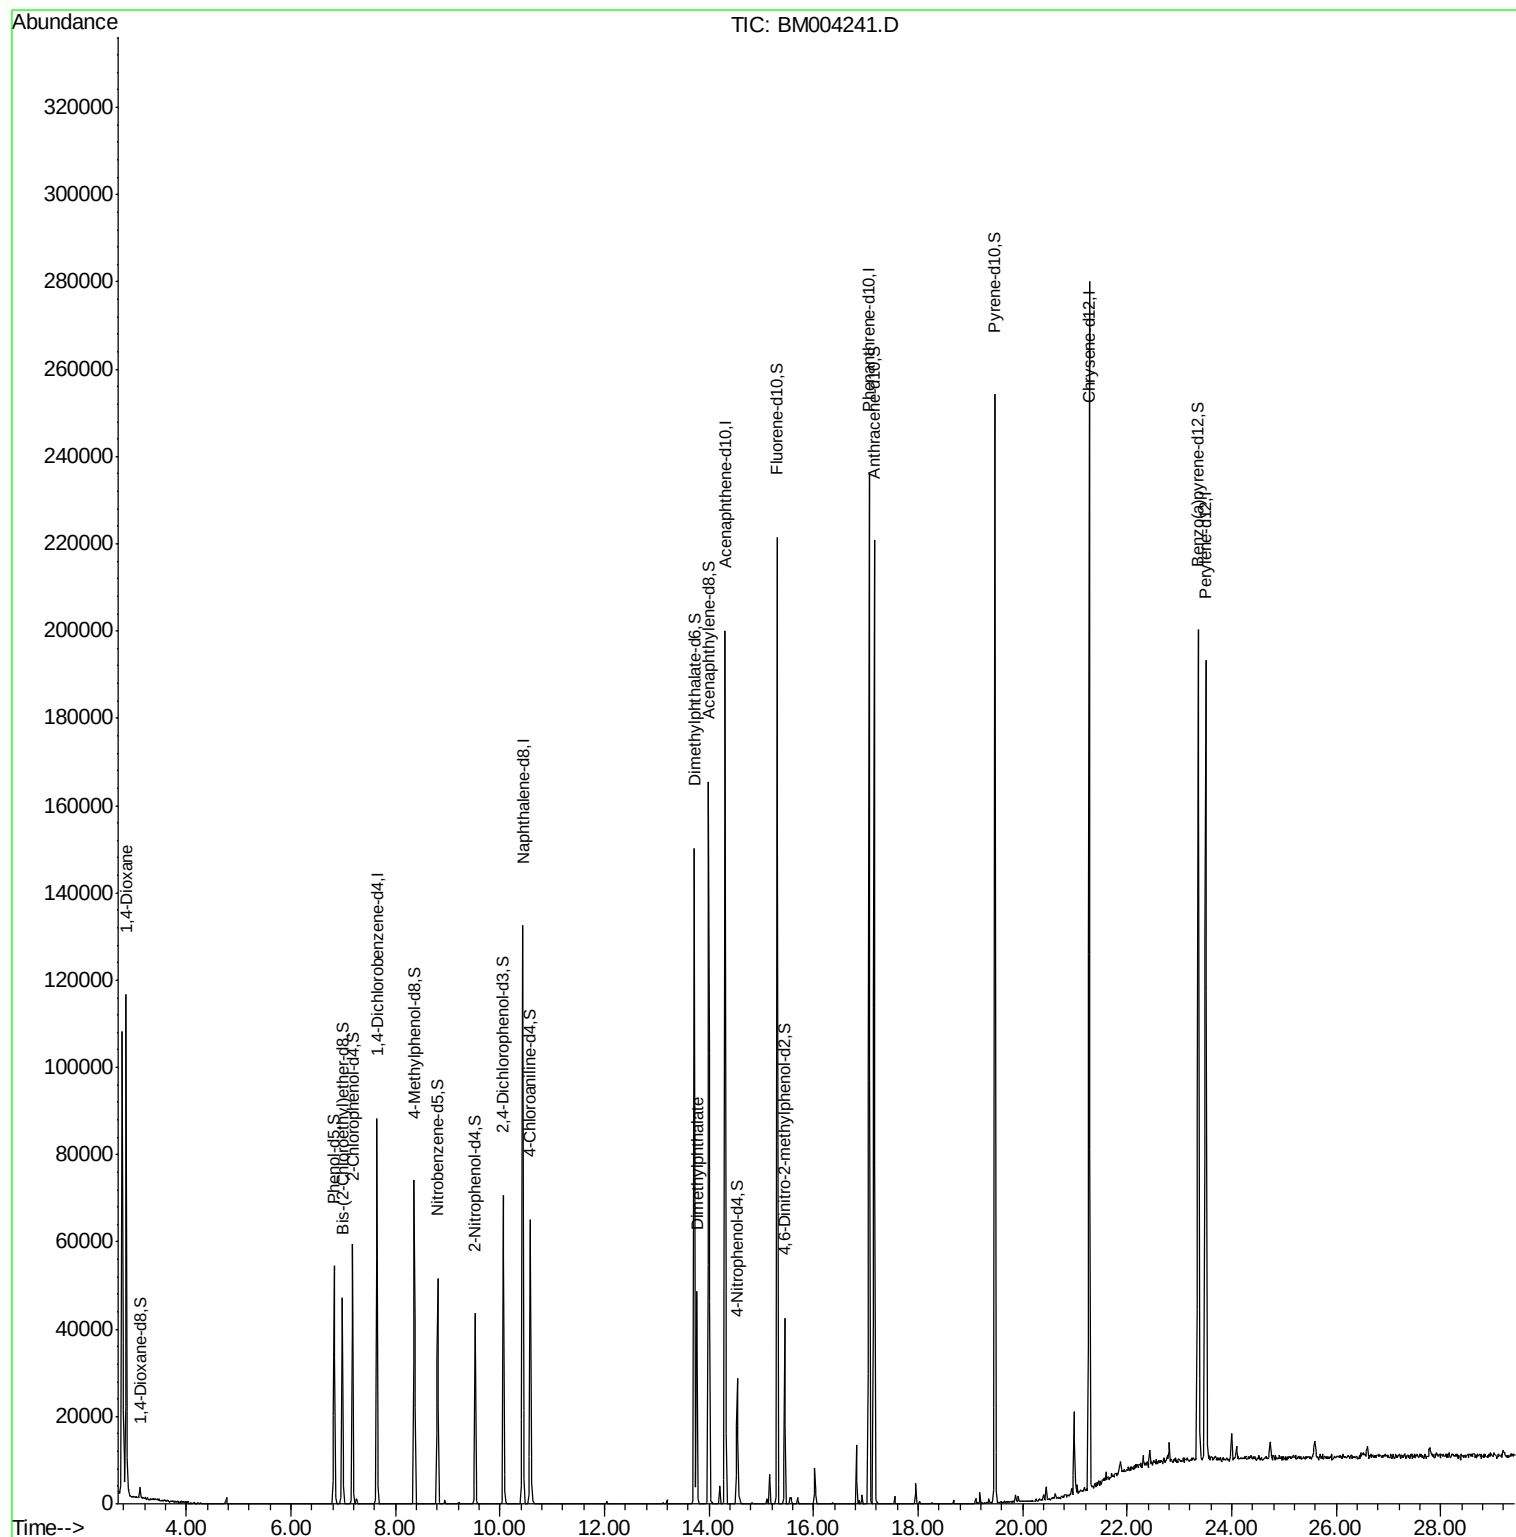

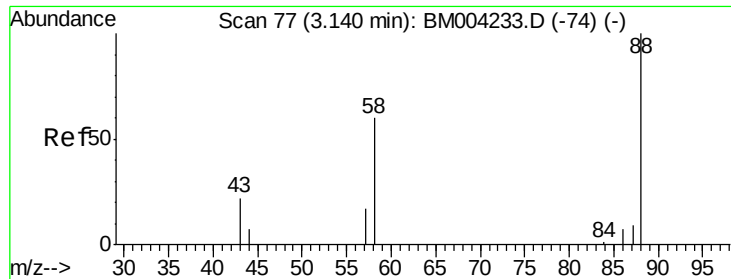

#2

1,4-Dioxane

Concen: 1.41 ng/uL

RT: 2.85 min Scan# 27

Delta R.T. -0.29 min

Lab File: BM004241.D

Acq: 12 Feb 2016 23:02

Instrument :

BNA_M

ClientSampleId :

D9QD9


Tgt Ion: 88 Resp: 861

Ion Ratio Lower Upper

88 100

43 2012.0 21.0 31.6#




58 0.0 47.8 71.8#

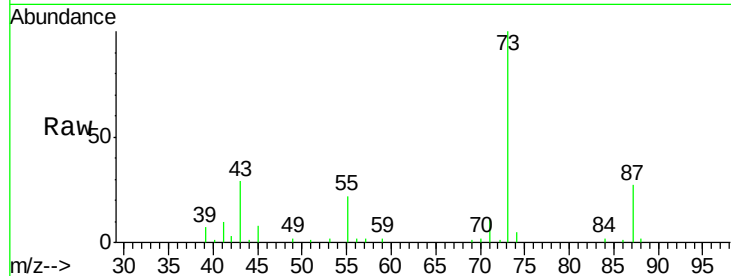

Abundance Ion 88.00 (87.70 to 88.70): BM004233.D (-74) (-)

Ion 43.00 (42.70 to 43.70): BM004233.D (-74) (-)

Ion 58.00 (57.70 to 58.70): BM004233.D (-74) (-)

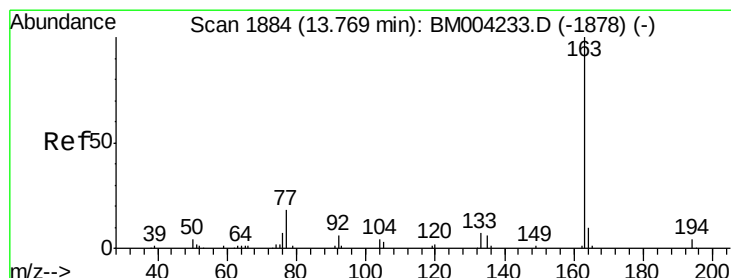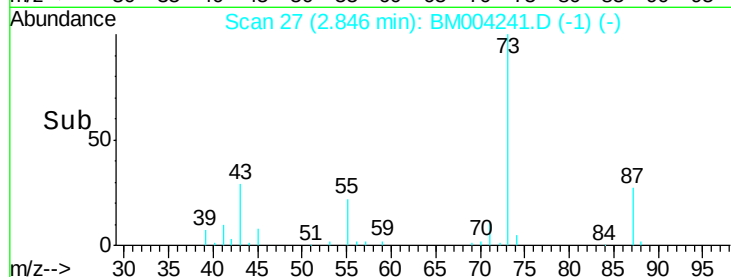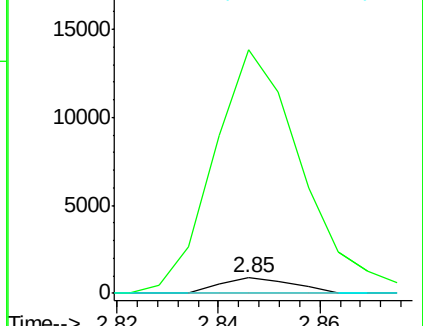

#45

Dimethylphthalate

Concen: 5.95 ng/uL

RT: 13.76 min Scan# 1883

Delta R.T. -0.01 min

Lab File: BM004241.D

Acq: 12 Feb 2016 23:02


Tgt Ion: 163 Resp: 35087

Ion Ratio Lower Upper

163 100

194 3.4 3.2 4.8

164 10.2 7.8 11.8

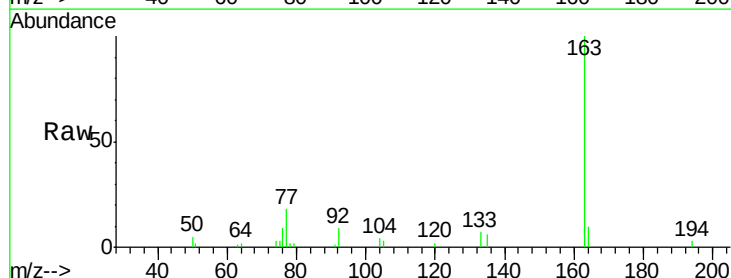

Abundance Ion 163.00 (162.70 to 163.70): BM004233.D (-1878) (-)

Ion 194.00 (193.70 to 194.70): BM004233.D (-1878) (-)

Ion 164.00 (163.70 to 164.70): BM004233.D (-1878) (-)

