

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021216\
 Data File : BM004242.D
 Acq On : 12 Feb 2016 23:38
 Operator : SJ/IZ
 Sample : H1414-17
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9QE0

Quant Time: Feb 13 01:02:52 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 12 22:29:16 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	28622	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	132140	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	81222	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.06	188	178028	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	164541	20.00	ng/ul	0.00
86) Perylene-d12	23.50	264	139494	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.11	96	2612	4.60	ng/uL	0.00
5) Phenol-d5	6.82	99	61136	26.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	33476	26.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	53436	26.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	55251	28.21	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	26883	26.46	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	31491	27.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	54736	26.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	78990	32.40	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	201852	29.86	ng/ul	0.00
47) Acenaphthylene-d8	14.00	160	237124	28.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	30420	27.82	ng/ul	0.00
58) Fluorene-d10	15.30	176	169908	29.82	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.44	200	26367	24.32	ng/ul	0.00
71) Anthracene-d10	17.16	188	257474	29.58	ng/ul	0.00
79) Pyrene-d10	19.46	212	276359	31.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	223342	30.00	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.76	163	80040	11.34	ng/ul	100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021216\
Data File : BM004242.D
Acq On : 12 Feb 2016 23:38
Operator : SJ/IZ
Sample : H1414-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9QE0

Quant Time: Feb 13 01:02:52 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 12 22:29:16 2016
Response via : Initial Calibration

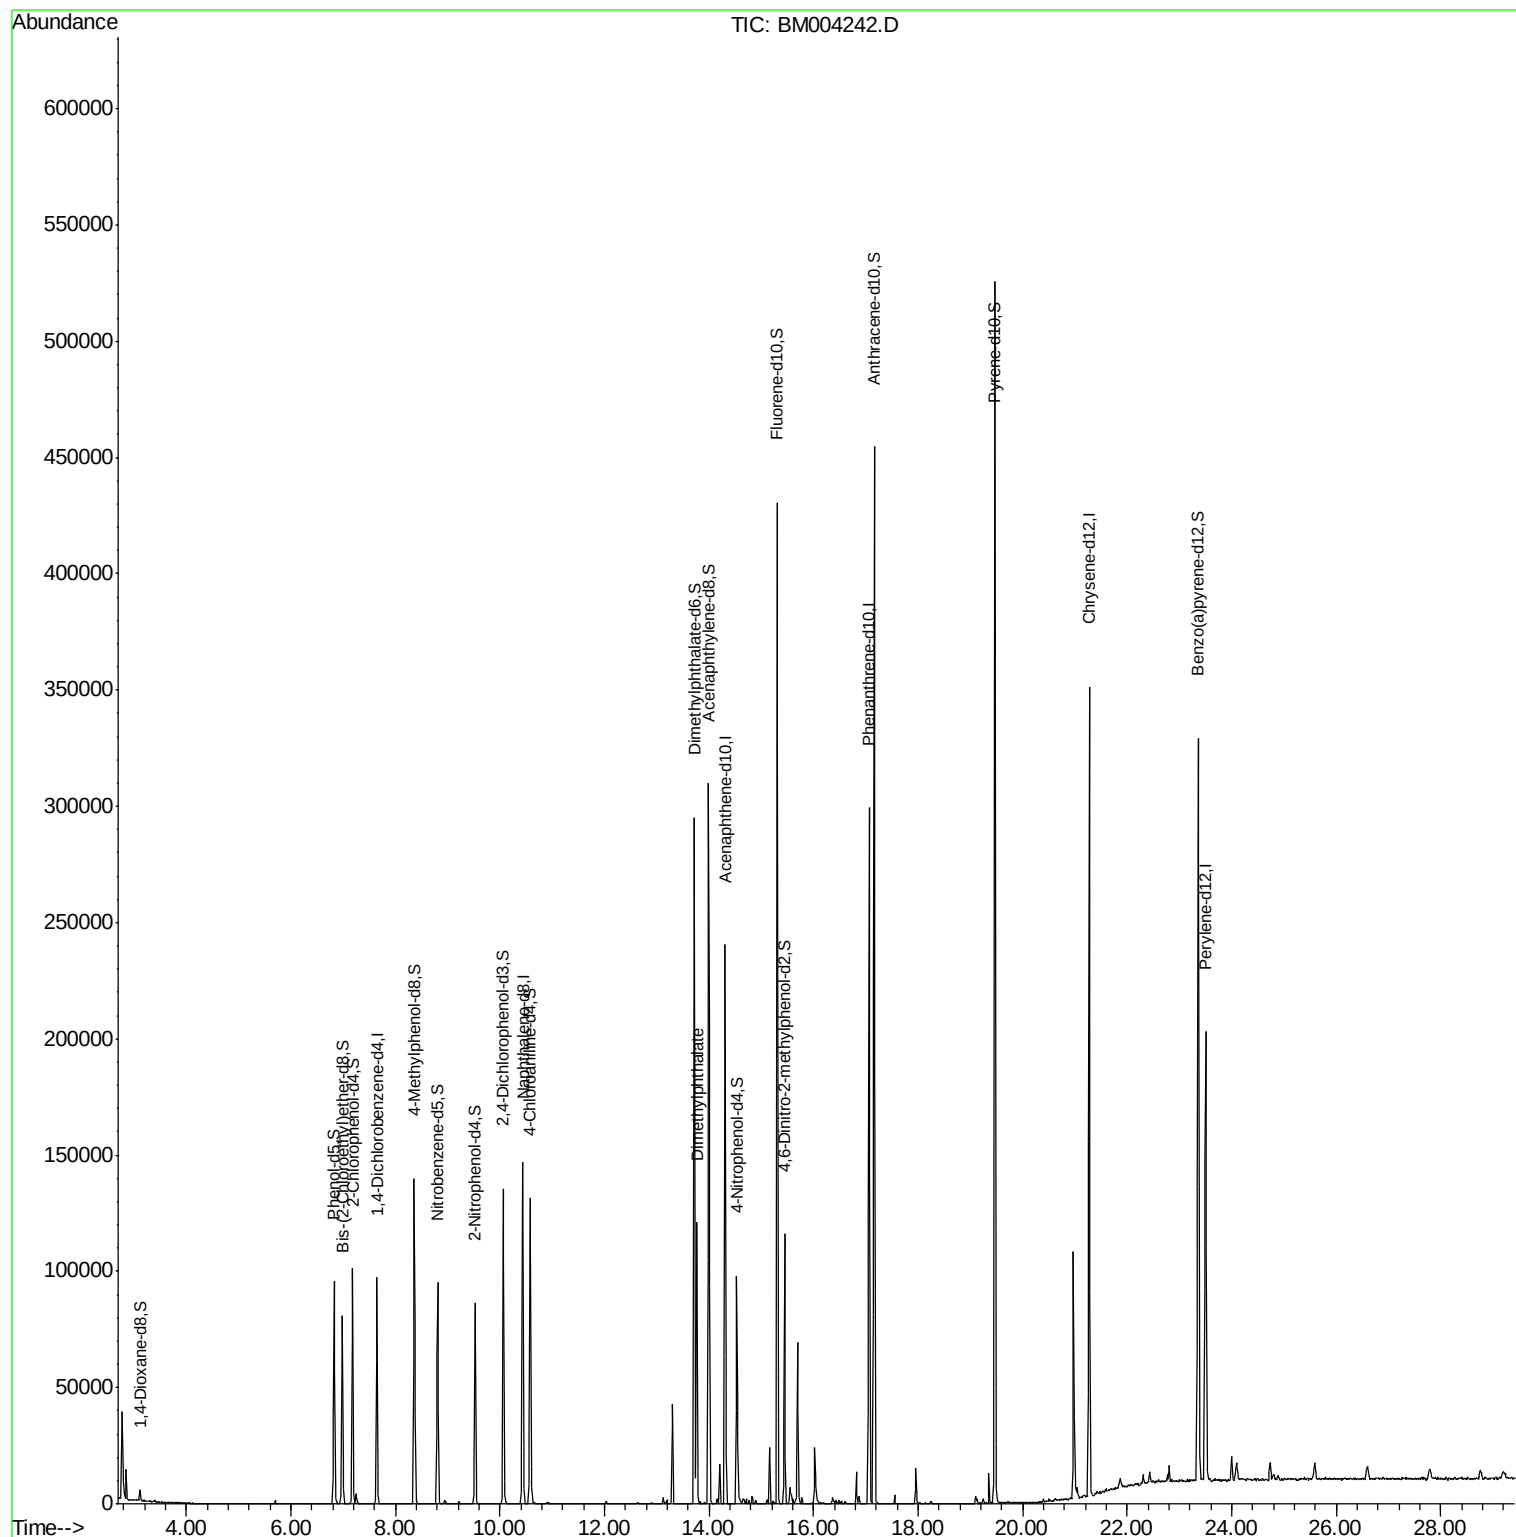

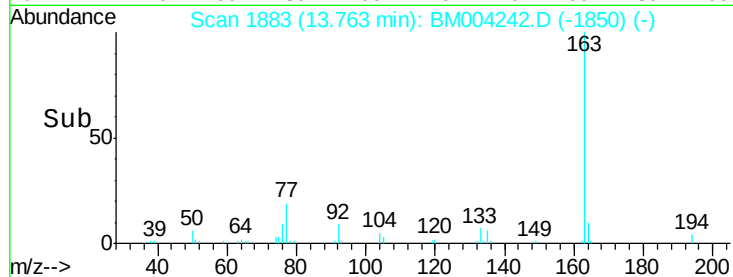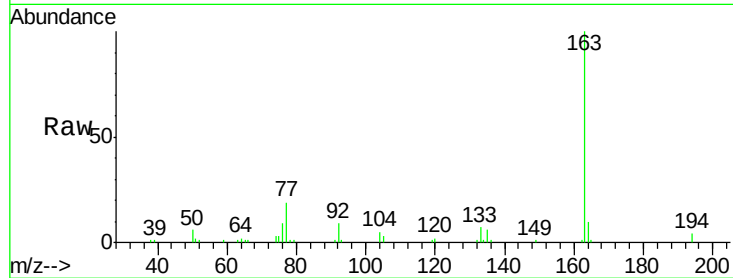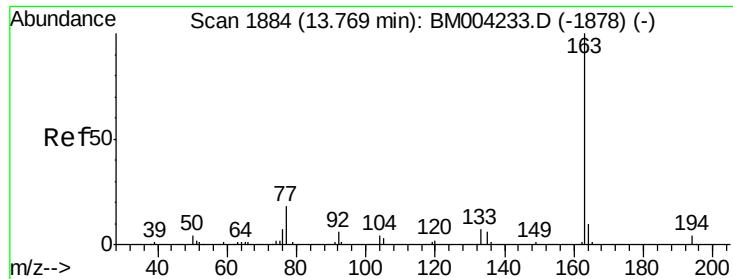

#45

Dimethylphthalate

Concen: 11.34 ng/ul

RT: 13.76 min Scan# 1883

Delta R.T. -0.01 min

Lab File: BM004242.D

Acq: 12 Feb 2016 23:38

Instrument :

BNA_M

ClientSampleId :

D9QE0

Tgt Ion:163 Resp: 80040

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 9.8 7.8 11.8

