

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021216\
 Data File : BM004254.D
 Acq On : 13 Feb 2016 07:27
 Operator : SJ/IZ
 Sample : H1414-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9QE2

Quant Time: Feb 15 00:15:52 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 13 05:01:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	34691	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	159816	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	91407	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.06	188	190220	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	148276	20.00	ng/ul	0.00
86) Perylene-d12	23.50	264	142501	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.11	96	3035	4.41	ng/uL	0.00
5) Phenol-d5	6.83	99	67239	24.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	36845	24.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	60498	24.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	60348	25.43	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	30743	25.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	35197	25.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	59590	24.06	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	86166	29.22	ng/ul	0.00
44) Dimethylphthalate-d6	13.72	166	197832	26.01	ng/ul	0.00
47) Acenaphthylene-d8	14.00	160	241936	26.18	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	30007	24.38	ng/ul	0.00
58) Fluorene-d10	15.30	176	167352	26.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.44	200	26562	22.93	ng/ul	0.00
71) Anthracene-d10	17.16	188	244860	26.33	ng/ul	0.00
79) Pyrene-d10	19.47	212	232584	29.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	198866	26.15	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.76	163	81162	10.21	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021216\
Data File : BM004254.D
Acq On : 13 Feb 2016 07:27
Operator : SJ/IZ
Sample : H1414-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9QE2

Quant Time: Feb 15 00:15:52 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 13 05:01:22 2016
Response via : Initial Calibration

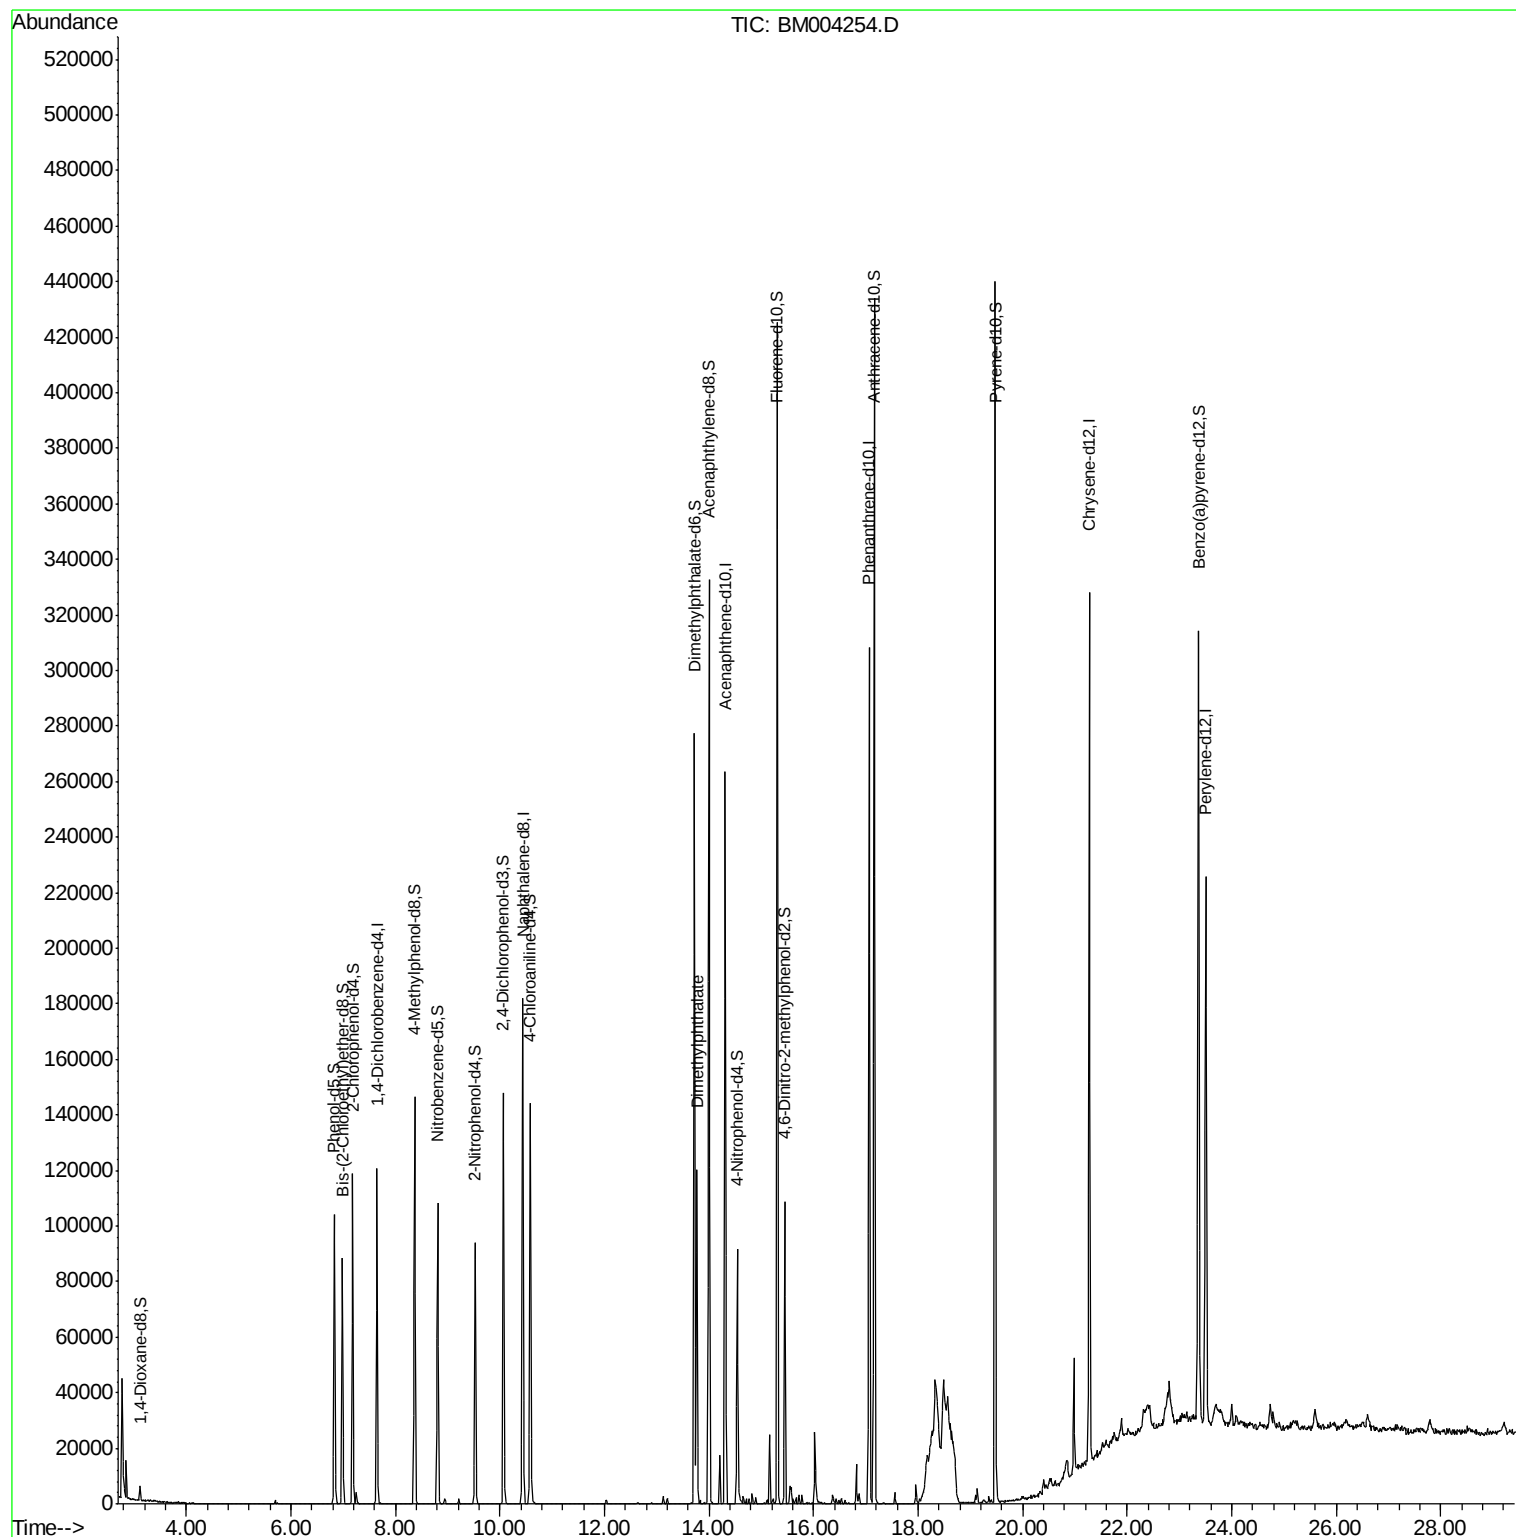

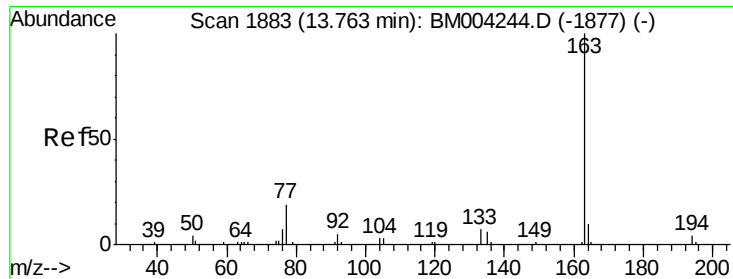

#45

Dimethylphthalate

Concen: 10.21 ng/ul

RT: 13.76 min Scan# 1883

Delta R.T. 0.00 min

Lab File: BM004254.D

Acq: 13 Feb 2016 07:27

Instrument :

BNA_M

ClientSampleId :

D9QE2

Tgt Ion:163 Resp: 81162

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 10.2 7.8 11.8

