


Data Path : Z:\HPCHEM1\BNA M\DATA\BM021216\
Data File : BM004225.D
Acq On : 12 Feb 2016 11:17
Operator : SJ/IZ
Sample : DFTPP50
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP50

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Title : SVOA CALIBRATION
Last Update : Sat Feb 13 05:01:22 2016

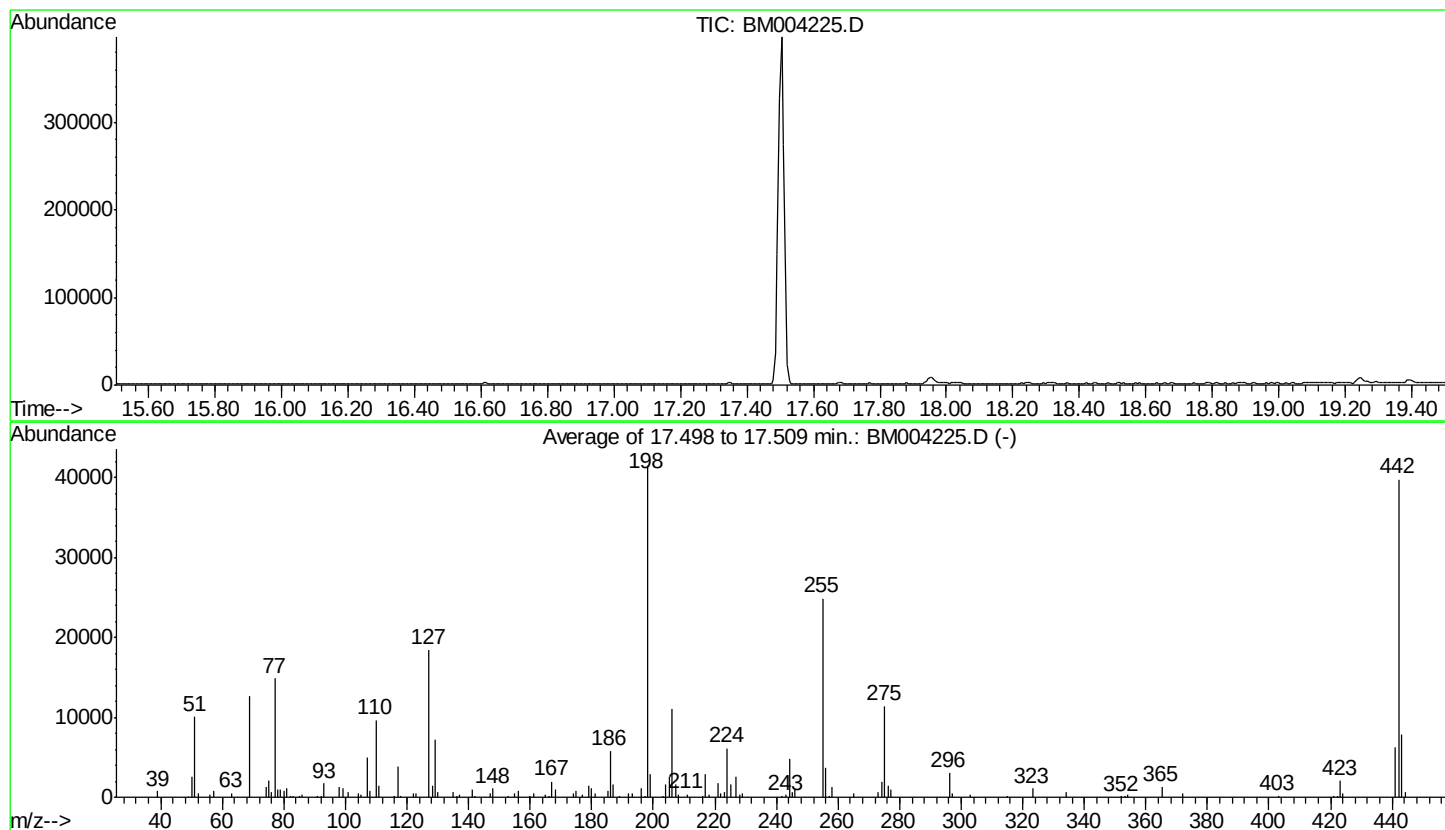

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	10041	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.5	12642	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.4	18443	PASS
197	198	0.00	2	0.3	104	PASS
198	198	100	100	100.0	41509	PASS
199	198	5	9	6.9	2844	PASS
275	198	10	60	27.4	11385	PASS
365	198	1	100	3.3	1365	PASS
441	443	0.01	100	80.4	6267	PASS
442	198	50	100	95.9	39816	PASS
443	442	15	24	19.6	7792	PASS

Scan 2445 (17.468 min): BM004225.D
DFTPP50

m/z	Abundance
43.00	435.0
49.00	558.0
84.00	651.0
85.90	426.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

m/z	Abundance
39.10	868.0
43.00	358.0
49.00	582.0
50.10	2891.0
51.10	11650.0
52.00	600.0
56.00	360.0
57.00	861.0
63.00	585.0
69.00	14221.0
74.00	1490.0
75.00	2344.0
76.10	728.0
77.10	16792.0
78.10	1190.0
79.00	1136.0
80.00	891.0
81.00	1230.0
82.00	321.0
83.00	310.0
84.00	634.0
86.00	741.0
92.00	357.0
93.00	1928.0
98.00	1570.0
99.00	1300.0
101.00	725.0
104.00	405.0
105.00	483.0
107.00	5519.0
108.00	794.0
110.00	10556.0
111.00	1671.0
116.00	324.0
117.00	4068.0
118.00	356.0
122.00	403.0
123.00	569.0
127.10	19776.0
128.10	1663.0
129.00	7697.0
130.00	682.0
135.00	659.0
137.10	395.0
141.00	963.0
141.90	320.0
147.00	515.0
148.00	1064.0
153.00	306.0
155.10	591.0
156.00	813.0
160.00	346.0
161.00	474.0
165.00	373.0
166.00	319.0
167.00	1957.0
168.00	1116.0
174.00	402.0
175.00	812.0
176.90	388.0
179.00	1559.0
180.10	1069.0
181.00	517.0
185.00	781.0
186.10	5673.0
187.10	1743.0
189.00	377.0
192.00	475.0
192.90	529.0
196.00	1177.0
198.00	41512.0
199.00	3053.0
204.00	1648.0
205.10	2595.0
206.10	10927.0
207.10	1559.0
208.00	445.0
210.90	353.0
217.00	2916.0
218.00	372.0
221.10	1680.0
221.90	402.0
223.00	660.0
224.10	5921.0
225.10	1544.0
227.00	2305.0
228.00	435.0
229.10	513.0
242.00	306.0
244.10	4741.0
245.10	628.0
246.00	944.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

255.10	23512.0
256.10	3515.0
258.10	1247.0
265.00	530.0
273.00	667.0
274.10	1731.0
275.10	10354.0
276.10	1277.0
277.00	847.0
296.10	2732.0
297.00	414.0
303.10	327.0
323.10	947.0
334.00	638.0
354.10	326.0
365.10	1150.0
372.10	439.0
423.10	1624.0
424.10	412.0
441.10	4640.0
442.20	30392.0
443.10	6168.0
444.10	547.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

m/z	Abundance
39.10	828.0
43.00	387.0
49.00	622.0
50.10	2968.0
51.10	11590.0
52.00	611.0
56.00	414.0
57.00	876.0
63.00	570.0
69.00	14630.0
74.10	1452.0
75.00	2582.0
76.10	839.0
77.10	17312.0
78.10	1179.0
79.00	1231.0
80.00	937.0
81.00	1348.0
82.10	349.0
83.90	639.0
85.00	300.0
86.00	750.0
91.00	325.0
92.00	313.0
93.00	1977.0
98.00	1610.0
99.00	1255.0
101.00	752.0
104.00	498.0
105.00	503.0
107.00	5928.0
108.10	887.0
110.00	11488.0
111.00	1677.0
116.00	375.0
117.00	4419.0
118.00	379.0
122.00	498.0
123.00	608.0
127.10	22016.0
128.10	1713.0
129.00	8403.0
130.00	681.0
135.00	736.0
136.00	310.0
137.00	390.0
141.00	1149.0
141.90	369.0
147.00	607.0
148.00	1329.0
153.00	343.0
155.10	681.0
156.10	1004.0
160.00	317.0
161.00	495.0
165.00	497.0
166.00	331.0
167.00	2265.0
168.00	1032.0
174.00	509.0
175.10	958.0
177.00	475.0
179.00	1787.0
180.10	1282.0
181.00	575.0
185.10	892.0
186.10	6928.0
187.00	1972.0
189.00	348.0
192.00	558.0
193.00	650.0
196.00	1410.0
197.10	312.0
198.00	49040.0
199.00	3290.0
203.00	371.0
204.10	1697.0
205.10	3024.0
206.10	13100.0
207.10	1784.0
208.00	441.0
211.00	469.0
216.00	323.0
217.00	3481.0
218.00	387.0
221.10	1911.0
221.80	474.0
223.00	778.0
224.10	7358.0
225.10	1797.0
227.00	2913.0
228.00	389.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

229.00	625.0
241.90	327.0
243.10	449.0
244.10	5539.0
245.10	765.0
246.00	1122.0
255.10	29336.0
256.10	4372.0
257.10	319.0
258.00	1609.0
265.00	658.0
273.00	841.0
274.10	2403.0
275.10	13677.0
276.10	1815.0
277.10	1047.0
296.10	3827.0
297.00	486.0
303.00	453.0
315.00	362.0
323.10	1218.0
334.10	770.0
352.10	439.0
353.10	315.0
354.10	398.0
365.10	1729.0
372.10	619.0
403.10	359.0
421.00	337.0
422.10	344.0
423.10	2463.0
424.10	565.0
441.20	7584.0
442.20	47800.0
443.20	9307.0
444.10	952.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

m/z	Abundance
39.10	541.0
43.00	421.0
49.00	582.0
50.00	1632.0
51.10	6884.0
52.00	361.0
57.00	581.0
63.00	323.0
69.00	9077.0
74.00	926.0
75.00	1552.0
76.10	458.0
77.10	10521.0
78.00	747.0
79.00	712.0
80.00	595.0
81.00	783.0
84.00	677.0
86.00	619.0
93.00	1262.0
98.00	921.0
99.00	811.0
101.00	457.0
104.00	338.0
107.00	3690.0
108.00	546.0
110.00	6876.0
111.00	1064.0
117.00	2852.0
122.00	318.0
123.00	358.0
127.10	13538.0
128.00	1064.0
129.00	5716.0
130.00	455.0
135.00	519.0
141.00	738.0
147.00	452.0
148.00	793.0
155.00	383.0
156.00	582.0
161.00	373.0
167.00	1566.0
168.00	773.0
174.00	324.0
175.00	591.0
179.00	1126.0
180.00	946.0
181.10	371.0
185.00	651.0
186.00	4744.0
187.10	1338.0
192.00	355.0
193.00	379.0
196.00	965.0
198.00	33976.0
199.00	2190.0
204.10	1279.0
205.10	2000.0
206.10	9349.0
207.10	1361.0
211.10	341.0
217.00	2312.0
218.00	322.0
221.10	1528.0
221.90	359.0
223.00	553.0
224.10	5228.0
225.10	1386.0
227.00	2292.0
228.00	300.0
229.00	504.0
243.10	301.0
244.10	3973.0
245.10	492.0
246.00	810.0
255.10	21832.0
256.10	2998.0
258.00	1230.0
265.10	509.0
273.10	653.0
274.10	1723.0
275.10	10126.0
276.10	1306.0
277.00	827.0
296.10	2721.0
297.00	412.0
303.00	339.0
315.00	323.0
323.10	1004.0
334.10	640.0
354.10	308.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50

365.10	1218.0
372.10	506.0
403.10	326.0
422.00	322.0
423.10	2005.0
424.10	504.0
441.10	6579.0
442.10	41256.0
443.10	7903.0
444.10	678.0

Instrument :
BNA_M
ClientSampleId :
DFTPP50