
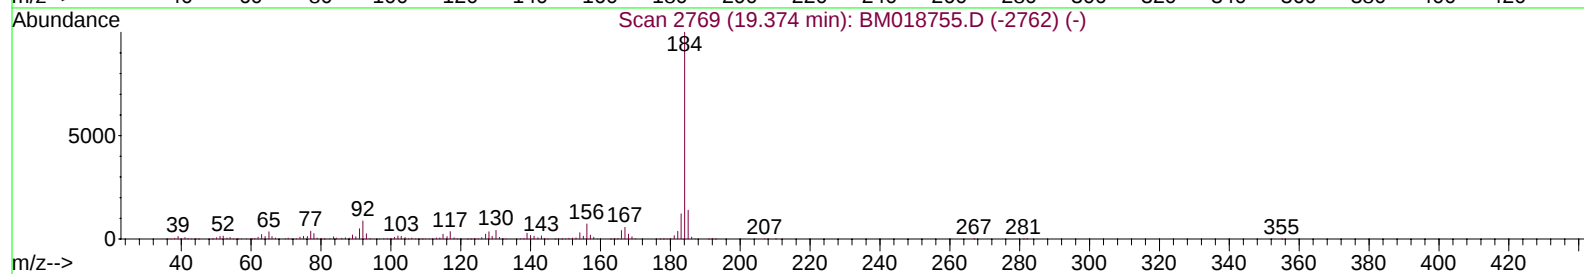
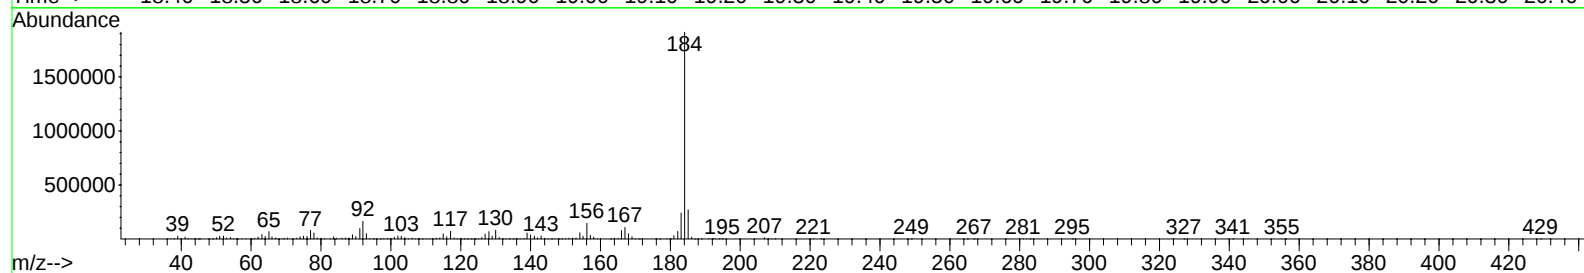


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021219\
Data File : BM018769.D
Acq On : 12 Feb 2019 12:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 10:46:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

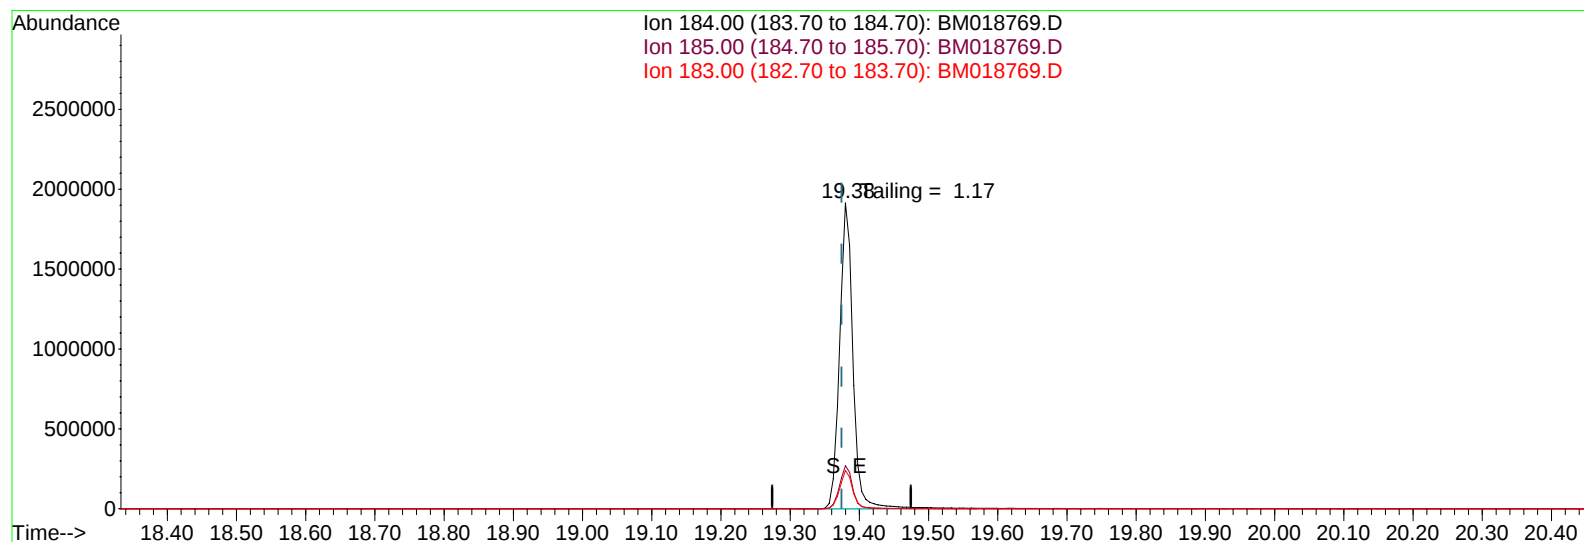

TIC: BM018769.D

(77) Benzidine




19.380min (+0.006) 13238.97ng

response 2521543

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.09
183.00	12.10	12.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021219\
Data File : BM018769.D
Acq On : 12 Feb 2019 12:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 10:46:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

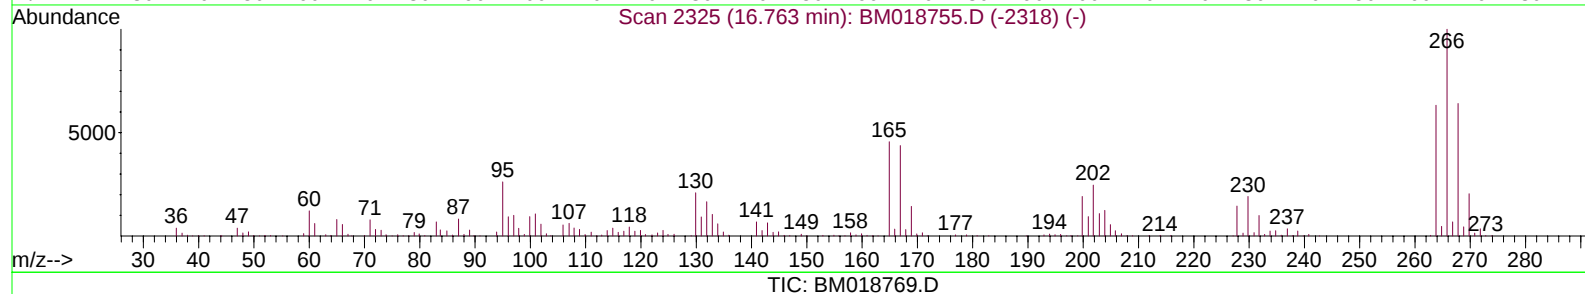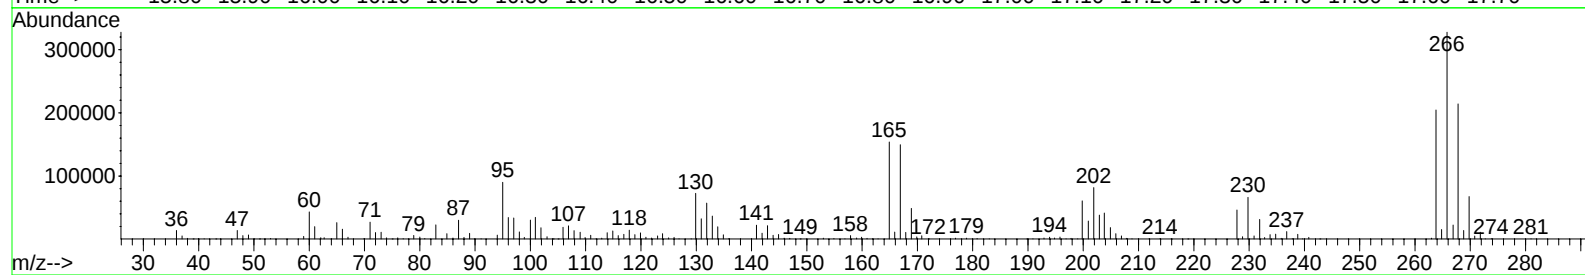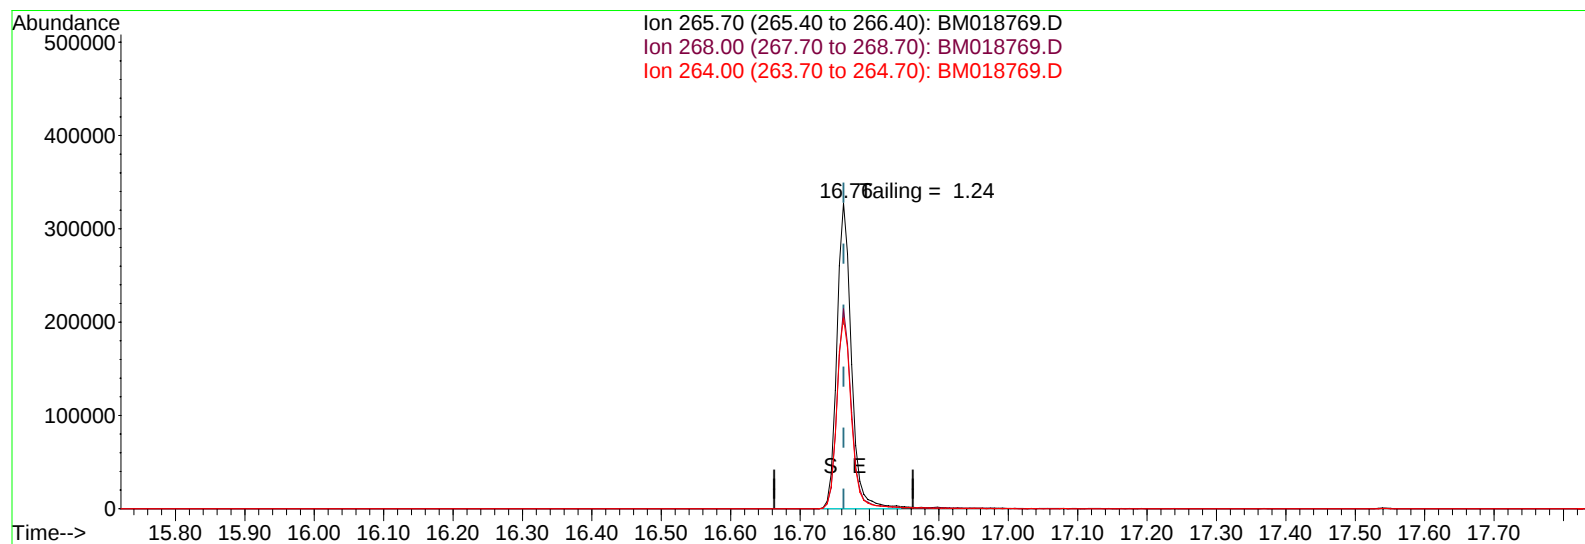

(70) Pentachlorophenol (C)

16.762min (-0.000) 36119.21ng

response 472928

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	65.37
264.00	63.20	62.38
0.00	0.00	0.00