
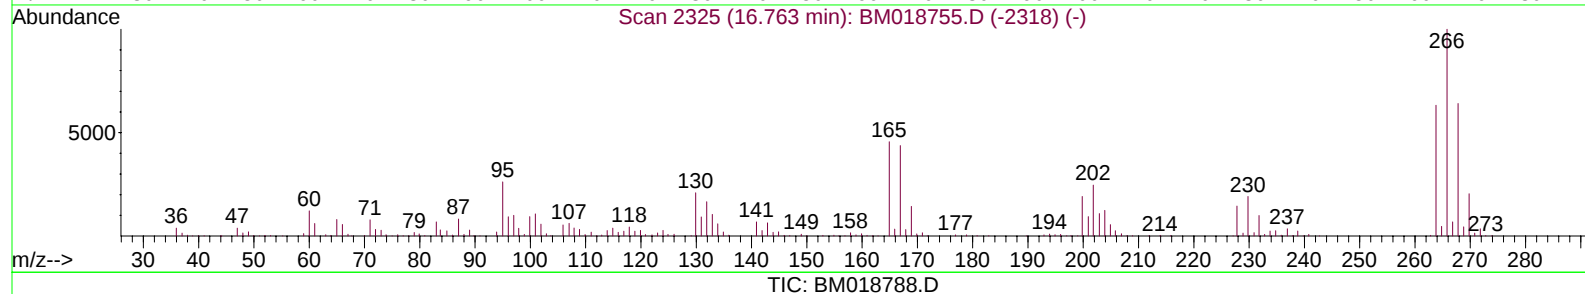
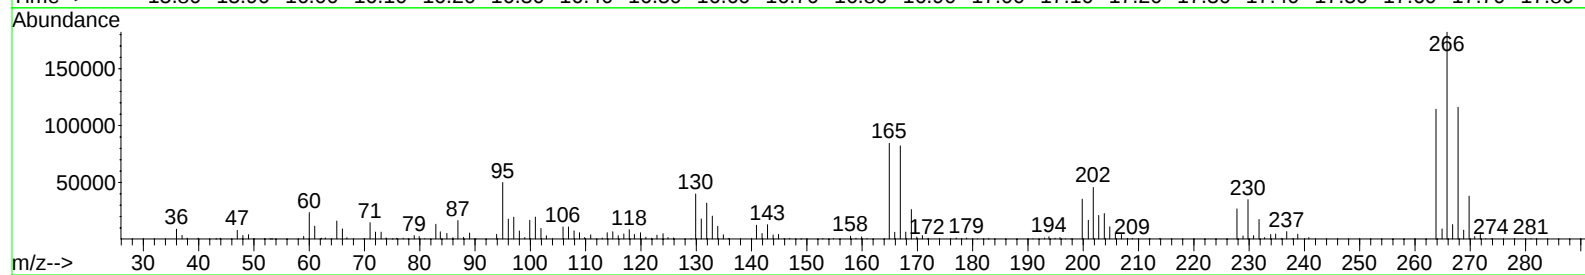


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021219\
Data File : BM018788.D
Acq On : 13 Feb 2019 00:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 10:28:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

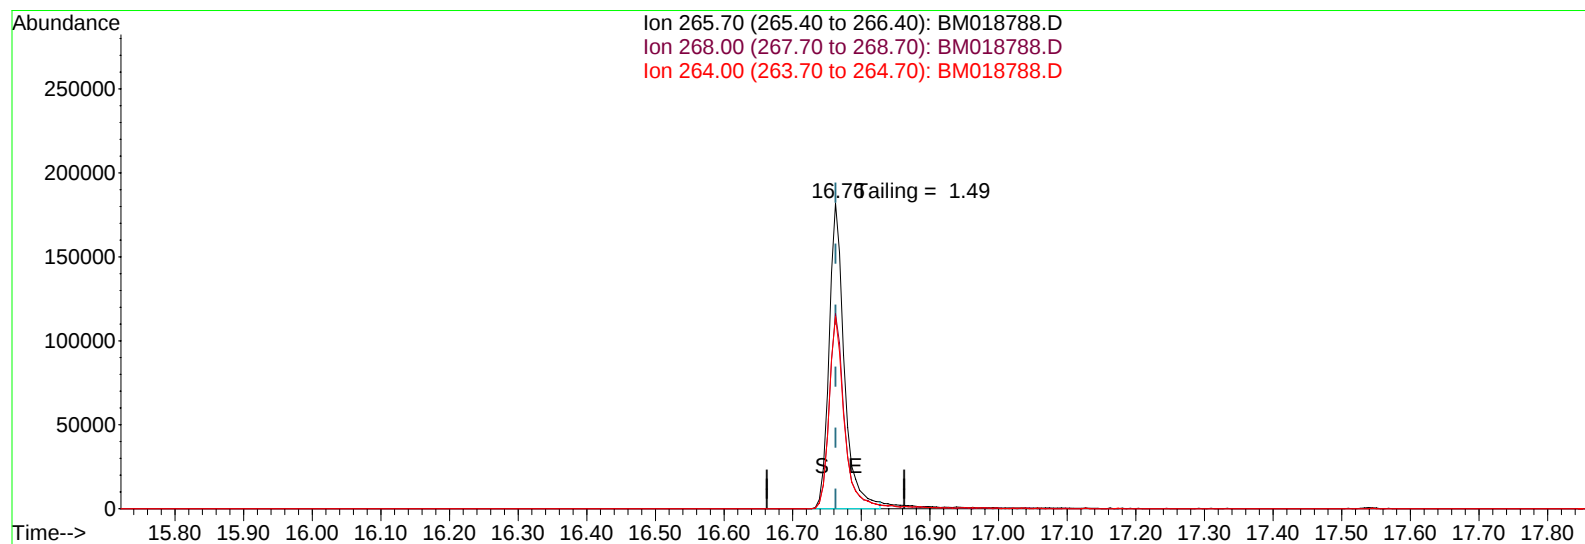

(70) Pentachlorophenol (C)




16.762min (-0.000) 256365.09ng

response 285633

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	63.73
264.00	63.20	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021219\
Data File : BM018788.D
Acq On : 13 Feb 2019 00:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 10:28:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

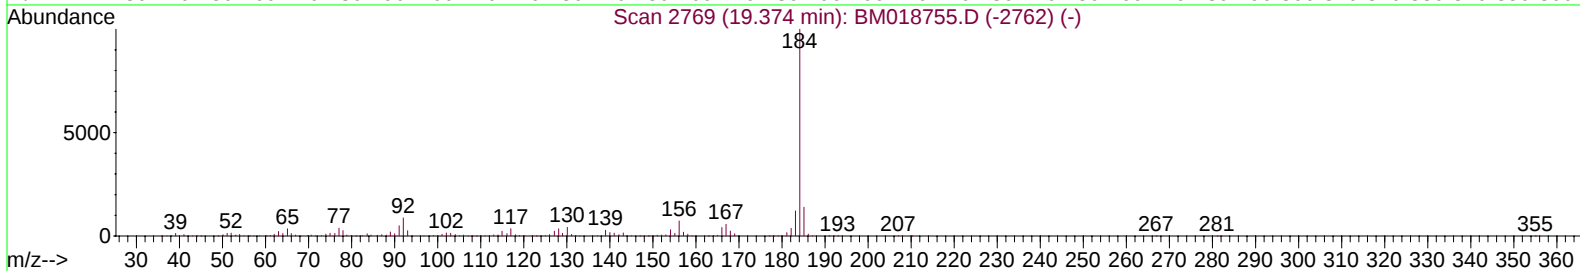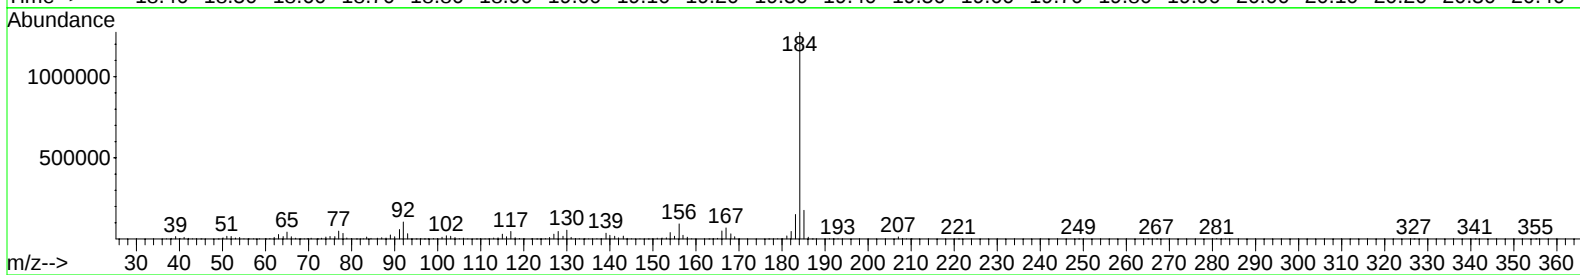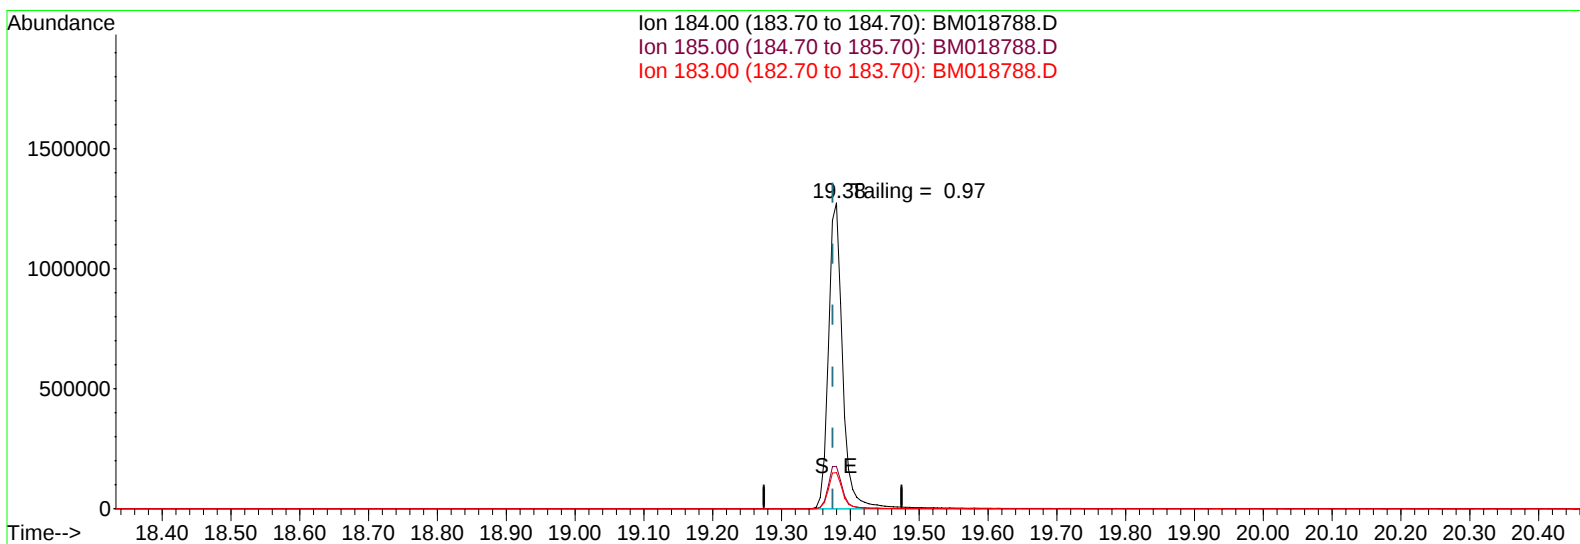

TIC: BM018788.D

(77) Benzidine

19.380min (+0.006) 104445.41ng

response 1799478

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.86
183.00	12.10	11.84
0.00	0.00	0.00