


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021219\
 Data File : BM018769.D
 Acq On : 12 Feb 2019 12:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 11 16:02:12 2019

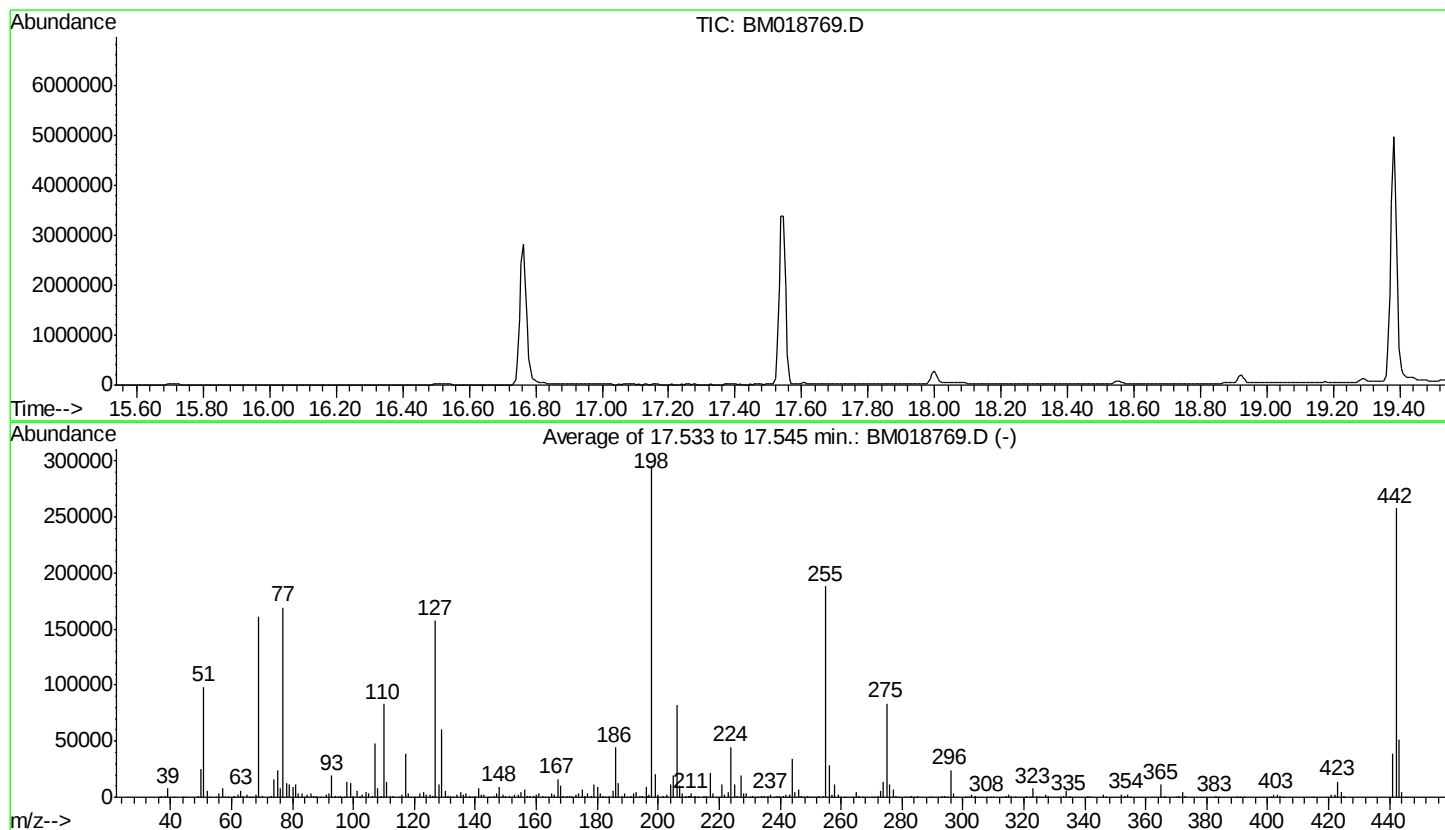

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	98509	PASS
68	69	0.00	2	1.8	2891	PASS
69	198	0.00	100	54.3	160731	PASS
70	69	0.00	2	0.5	874	PASS
127	198	10	80	53.3	157570	PASS
197	198	0.00	2	0.6	1797	PASS
198	198	100	100	100.0	295808	PASS
199	198	5	9	6.9	20374	PASS
275	198	10	60	28.4	83944	PASS
365	198	1	100	3.8	11183	PASS
441	198	0.01	100	13.1	38648	PASS
442	198	50	100	87.1	257706	PASS
443	442	15	24	19.8	51122	PASS