


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021219\
 Data File : BM018788.D
 Acq On : 13 Feb 2019 00:33
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 11 16:02:12 2019

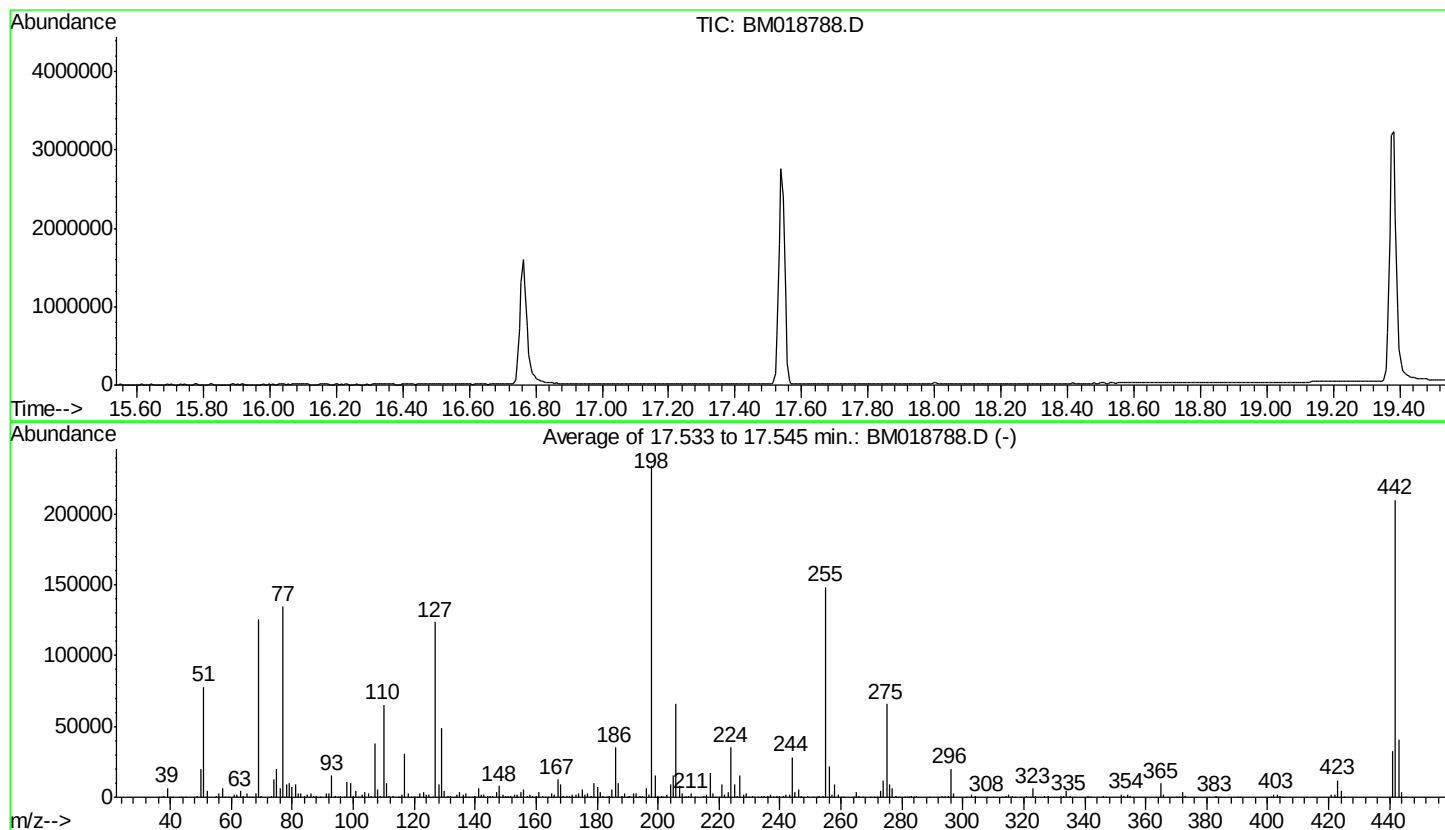

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	77909	PASS
68	69	0.00	2	1.9	2411	PASS
69	198	0.00	100	53.7	125829	PASS
70	69	0.00	2	0.6	786	PASS
127	198	10	80	52.9	123837	PASS
197	198	0.00	2	0.7	1554	PASS
198	198	100	100	100.0	234197	PASS
199	198	5	9	6.6	15490	PASS
275	198	10	60	28.0	65669	PASS
365	198	1	100	4.1	9597	PASS
441	198	0.01	100	13.9	32488	PASS
442	198	50	100	89.8	210216	PASS
443	442	15	24	19.4	40880	PASS