


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021221\
 Data File : BM028725.D
 Acq On : 12 Feb 2021 11:20
 Operator : CG/JU
 Sample : DFTPP28
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP028

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM021221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 12 16:15:08 2021

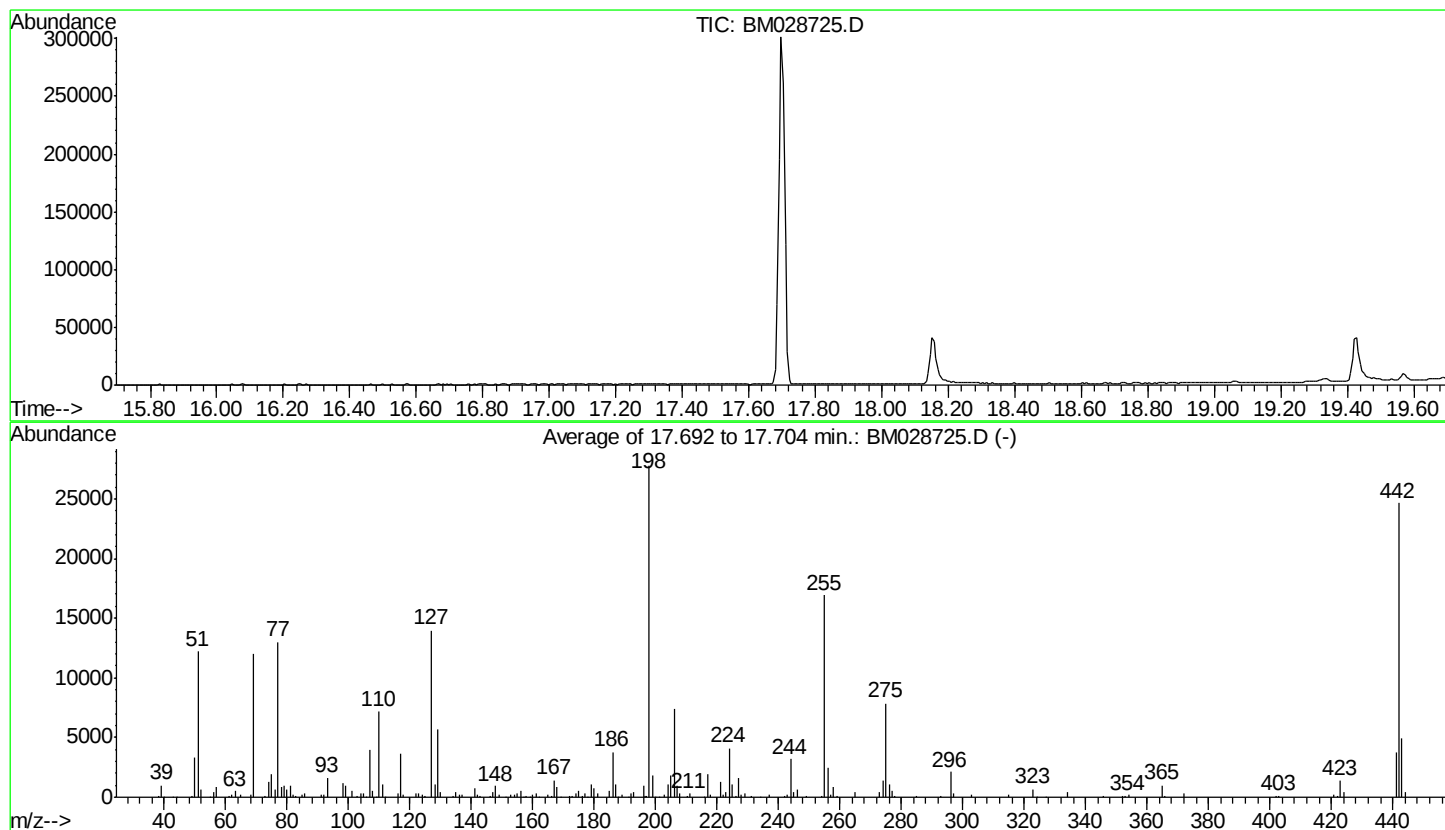

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	12199	PASS
68	69	0.00	2	1.5	179	PASS
69	198	0.00	100	43.1	11977	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	13986	PASS
197	198	0.00	2	0.2	61	PASS
198	198	100	100	100.0	27776	PASS
199	198	5	9	6.6	1838	PASS
275	198	10	60	28.2	7833	PASS
365	198	1	100	3.6	1003	PASS
441	198	0.01	100	13.6	3772	PASS
442	198	50	100	88.6	24615	PASS
443	442	15	24	19.9	4889	PASS

Scan 2494 (17.657 min): BM028725.D
DFTPP28

m/z	Abundance
42.90	168.0
44.00	325.0
72.90	162.0
207.00	284.0

Instrument :
BNA_M
ClientSampleId :
DFTPP028

m/z	Abundance
39.00	839.0
43.00	170.0
44.00	354.0
50.00	3079.0
51.10	10958.0
52.00	556.0
55.90	428.0
57.00	778.0
61.00	154.0
62.00	154.0
63.00	518.0
65.00	232.0
68.10	193.0
69.00	10992.0
73.10	255.0
74.00	1198.0
75.00	1588.0
76.00	522.0
77.10	11678.0
78.10	861.0
79.00	835.0
80.00	666.0
81.00	882.0
82.00	181.0
85.00	162.0
85.90	300.0
90.90	237.0
91.90	250.0
93.00	1492.0
98.00	1074.0
99.00	893.0
101.00	503.0
104.00	312.0
105.00	366.0
107.00	3437.0
107.90	457.0
110.00	6219.0
111.00	1023.0
115.90	218.0
117.00	3207.0
118.00	259.0
122.00	264.0
122.90	290.0
123.90	209.0
127.00	11597.0
128.00	839.0
129.00	4842.0
129.90	445.0
133.90	152.0
135.00	429.0
135.90	157.0
137.00	191.0
141.00	645.0
142.00	219.0
143.00	164.0
147.00	382.0
148.00	750.0
149.00	215.0
152.90	193.0
154.00	153.0
155.00	308.0
156.00	503.0
159.90	172.0
161.00	269.0
164.90	160.0
167.00	1110.0
168.00	702.0
174.00	345.0
174.90	402.0
176.00	166.0
176.90	213.0
178.90	890.0
180.00	638.0
181.00	248.0
185.00	375.0
186.00	2908.0
187.00	871.0
188.90	230.0
192.00	269.0
192.90	375.0
196.00	759.0
198.00	21792.0
198.90	1531.0
204.00	832.0
205.00	1401.0
206.00	5448.0
207.00	1173.0
208.00	263.0
210.90	240.0
216.90	1403.0
218.00	186.0
221.00	978.0

Instrument :
BNA_M
ClientSampleId :
DFTPP028

222.00	183.0
223.00	333.0
224.00	3148.0
225.00	804.0
227.00	1169.0
228.00	186.0
229.00	300.0
237.00	177.0
242.90	177.0
244.00	2513.0
245.00	315.0
246.00	437.0
255.00	12382.0
256.00	1820.0
256.90	166.0
258.00	592.0
265.00	245.0
272.90	323.0
274.00	989.0
275.00	5651.0
276.00	783.0
276.90	401.0
296.00	1378.0
296.90	211.0
314.90	205.0
323.00	406.0
334.00	308.0
365.00	740.0
371.90	206.0
423.00	836.0
424.00	222.0
441.00	2154.0
442.00	13965.0
443.00	2985.0
443.90	227.0

Instrument :
BNA_M
ClientSampleId :
DFTPP028

m/z	Abundance
38.00	216.0
39.10	1232.0
39.90	169.0
43.00	195.0
44.00	406.0
49.10	176.0
50.00	3882.0
51.00	14643.0
52.10	738.0
55.00	157.0
56.00	474.0
57.00	1041.0
61.00	178.0
62.00	208.0
63.00	545.0
65.00	286.0
68.10	344.0
69.00	14164.0
73.00	284.0
74.00	1465.0
75.00	2355.0
76.00	752.0
77.10	15559.0
78.10	991.0
79.00	1104.0
80.00	903.0
81.00	1219.0
82.00	268.0
83.00	245.0
85.00	190.0
85.90	315.0
91.00	253.0
92.00	232.0
93.00	1791.0
98.00	1528.0
99.00	1150.0
100.90	663.0
102.90	195.0
104.00	390.0
105.00	393.0
105.90	152.0
107.00	4825.0
108.00	751.0
109.10	154.0
110.00	8541.0
111.00	1368.0
115.90	377.0
117.00	4444.0
117.90	285.0
122.00	334.0
122.90	425.0
123.90	249.0
125.00	225.0
127.00	16992.0
128.00	1137.0
129.00	6432.0
130.00	569.0
133.90	246.0
134.90	529.0
136.00	174.0
137.00	314.0
140.90	876.0
141.90	255.0
143.00	204.0
146.00	164.0
147.00	516.0
148.00	1145.0
149.00	209.0
151.00	164.0
152.90	246.0
153.90	194.0
154.90	446.0
156.00	648.0
157.10	151.0
158.00	207.0
158.90	166.0
159.90	317.0
160.90	391.0
162.00	166.0
165.00	287.0
166.10	222.0
167.00	1843.0
168.00	961.0
169.00	169.0
172.00	199.0
173.00	207.0
174.00	366.0
175.00	581.0
175.90	195.0
177.00	347.0
179.00	1253.0
180.00	948.0

Instrument :
BNA_M
ClientSampleId :
DFTPP028

180.90	414.0
185.00	671.0
186.00	4651.0
187.00	1280.0
188.00	150.0
189.00	295.0
191.00	169.0
192.00	335.0
193.00	517.0
196.00	1190.0
196.70	183.0
198.00	32592.0
199.00	2149.0
199.90	152.0
201.30	155.0
202.90	281.0
204.00	1218.0
205.00	2138.0
206.00	8917.0
207.00	1486.0
208.00	436.0
210.20	189.0
211.00	358.0
217.00	2346.0
217.90	281.0
221.00	1587.0
222.00	317.0
222.90	498.0
224.00	4878.0
225.00	1308.0
226.00	174.0
227.00	2011.0
228.00	293.0
229.00	458.0
231.00	217.0
233.90	156.0
237.00	228.0
242.00	187.0
243.00	355.0
244.00	3554.0
245.00	539.0
246.00	769.0
248.90	167.0
254.10	196.0
255.00	19680.0
256.00	2930.0
257.00	257.0
258.00	1005.0
259.00	192.0
265.00	585.0
272.90	545.0
274.00	1604.0
275.00	9257.0
276.00	1239.0
277.00	669.0
285.00	158.0
292.90	160.0
296.00	2540.0
297.00	344.0
303.00	282.0
315.00	249.0
323.00	830.0
324.10	159.0
327.00	162.0
334.00	527.0
345.90	153.0
352.00	252.0
354.00	261.0
365.00	1150.0
366.00	181.0
372.00	421.0
401.90	156.0
403.00	268.0
421.00	277.0
422.00	204.0
423.00	1594.0
423.90	514.0
441.00	4239.0
442.00	27992.0
443.00	5429.0
444.00	523.0

Instrument :
BNA_M
ClientSampleId :
DFTPP028

m/z	Abundance
39.00	845.0
43.00	151.0
44.00	310.0
50.10	2988.0
51.10	10998.0
52.00	540.0
55.90	406.0
57.00	707.0
62.00	200.0
63.00	412.0
65.00	270.0
69.00	10775.0
73.00	243.0
74.00	1296.0
75.00	1773.0
76.00	556.0
77.10	11753.0
78.00	808.0
79.00	852.0
80.00	490.0
81.00	843.0
81.90	233.0
82.90	191.0
85.00	197.0
85.90	274.0
91.00	176.0
92.00	251.0
93.00	1553.0
98.00	1098.0
98.90	803.0
101.00	505.0
102.90	230.0
104.00	334.0
105.00	340.0
107.00	3605.0
108.00	559.0
110.00	6696.0
111.00	965.0
112.00	169.0
116.00	250.0
117.00	3373.0
118.00	207.0
121.90	240.0
122.90	412.0
123.90	225.0
124.90	158.0
127.00	13370.0
128.00	1093.0
129.00	5654.0
129.90	382.0
135.00	445.0
135.90	201.0
137.00	210.0
140.90	771.0
141.90	212.0
145.90	201.0
146.90	405.0
148.00	919.0
148.90	208.0
152.90	244.0
154.10	182.0
155.00	360.0
155.90	596.0
160.00	212.0
161.00	361.0
164.90	304.0
166.00	253.0
167.00	1389.0
168.00	764.0
173.90	264.0
175.10	479.0
176.90	314.0
178.00	160.0
179.00	1036.0
180.00	790.0
181.00	288.0
185.00	550.0
186.00	3815.0
187.00	1092.0
189.00	230.0
191.90	425.0
193.00	321.0
196.00	1005.0
197.10	175.0
198.00	28944.0
198.90	1834.0
203.00	241.0
204.00	1116.0
205.00	1781.0
206.00	7780.0
207.00	1202.0
208.00	286.0

Instrument :
BNA_M
ClientSampleId :
DFTPP028

210.90	299.0
215.90	157.0
217.00	2133.0
218.00	212.0
221.00	1414.0
221.90	211.0
223.00	487.0
224.00	4251.0
225.00	1115.0
227.00	1650.0
228.00	269.0
229.00	360.0
231.00	151.0
237.00	242.0
242.00	235.0
243.10	246.0
244.00	3535.0
245.00	379.0
245.90	627.0
249.00	151.0
255.00	18752.0
256.00	2608.0
256.90	204.0
258.00	1022.0
259.00	174.0
265.00	462.0
273.00	542.0
274.00	1471.0
275.00	8592.0
276.00	1255.0
277.00	711.0
278.00	175.0
285.00	167.0
293.00	196.0
296.00	2468.0
297.00	323.0
303.00	303.0
315.00	247.0
323.00	743.0
334.00	446.0
346.00	172.0
352.00	235.0
352.90	185.0
354.00	270.0
364.90	1121.0
365.90	166.0
372.00	436.0
401.90	195.0
403.00	222.0
420.90	259.0
421.90	209.0
423.00	1727.0
424.00	560.0
441.00	4925.0
442.00	31888.0
443.00	6253.0
443.90	523.0

Instrument :
BNA_M
ClientSampleId :
DFTPP028