
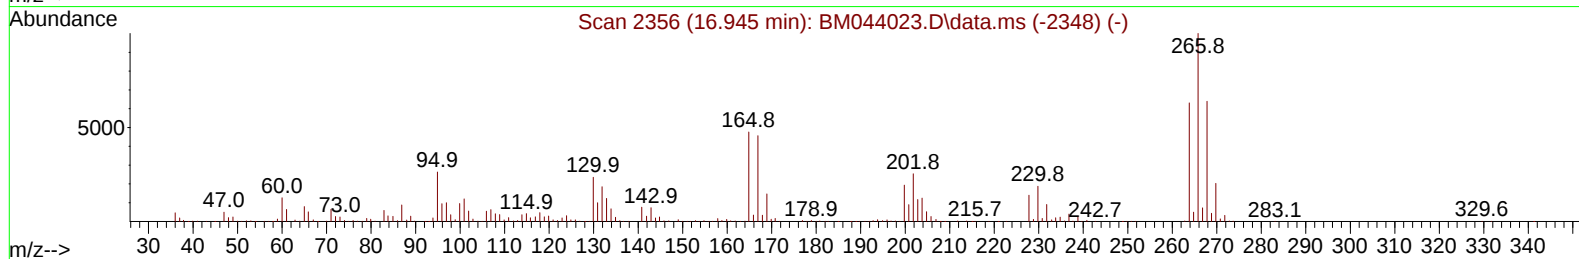
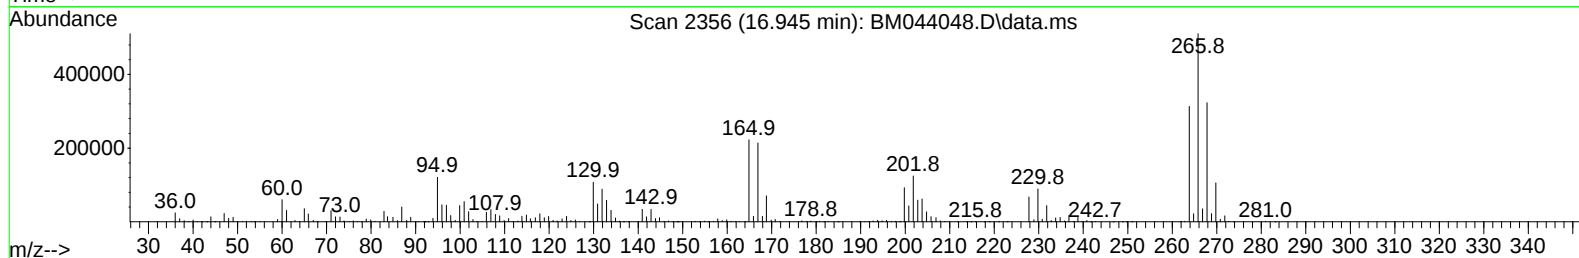


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021224\
Data File : BM044048.D
Acq On : 12 Feb 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 11:30:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

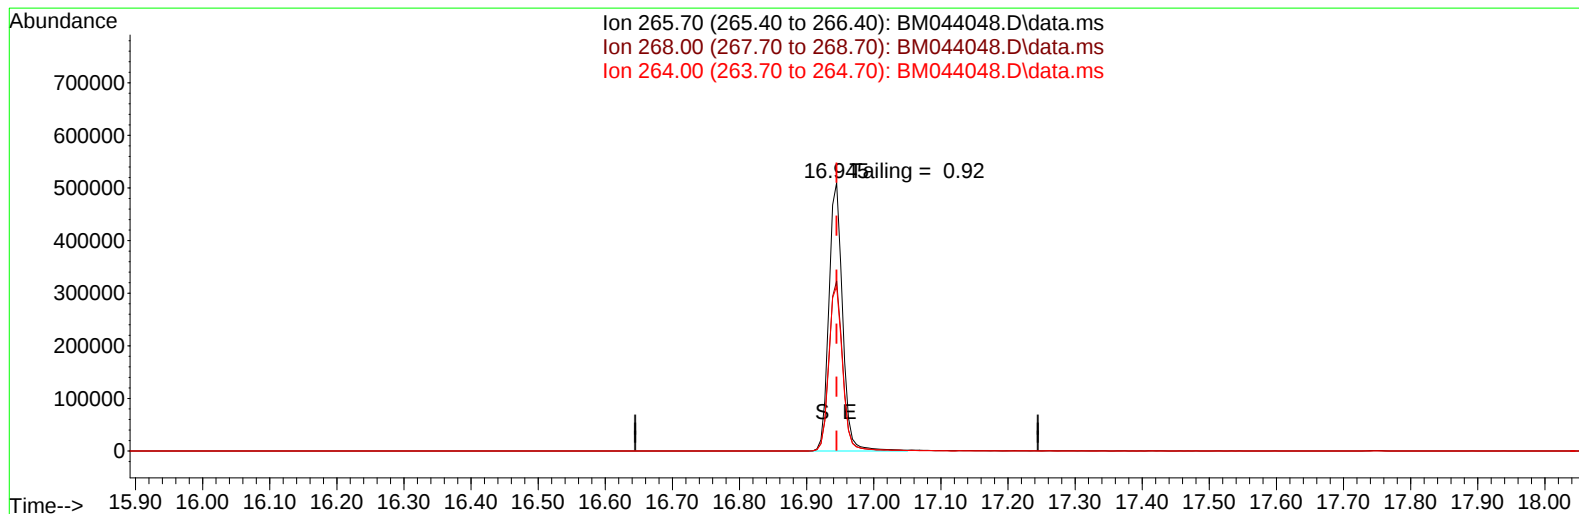

TIC: BM044048.D\data.ms

(70) Pentachlorophenol (C)




16.945min (-0.000) 0.00 ng

response 723381

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.35
264.00	63.10	61.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021224\
Data File : BM044048.D
Acq On : 12 Feb 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 11:30:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

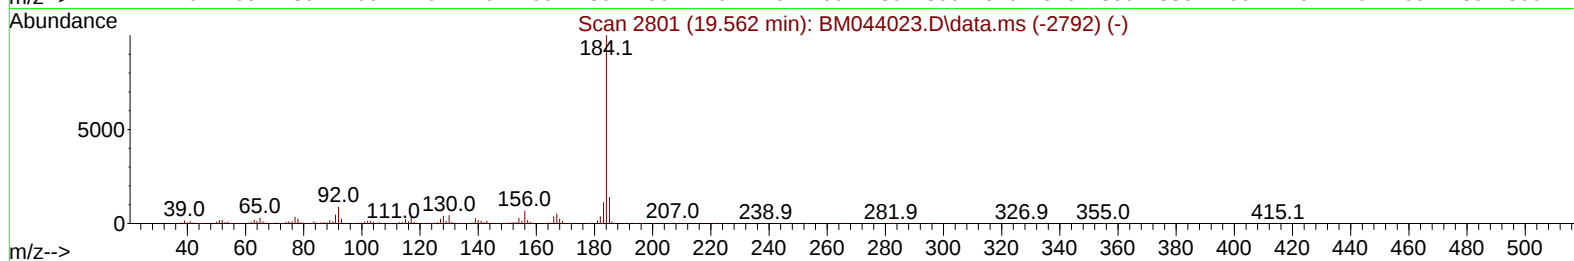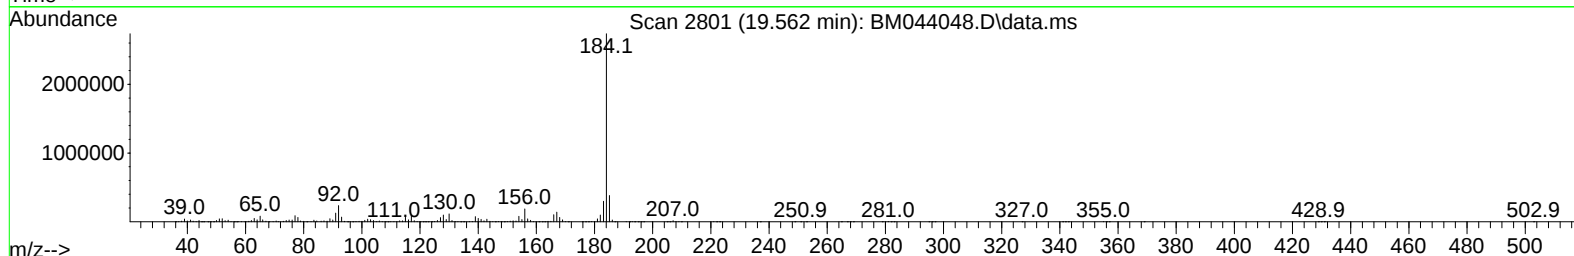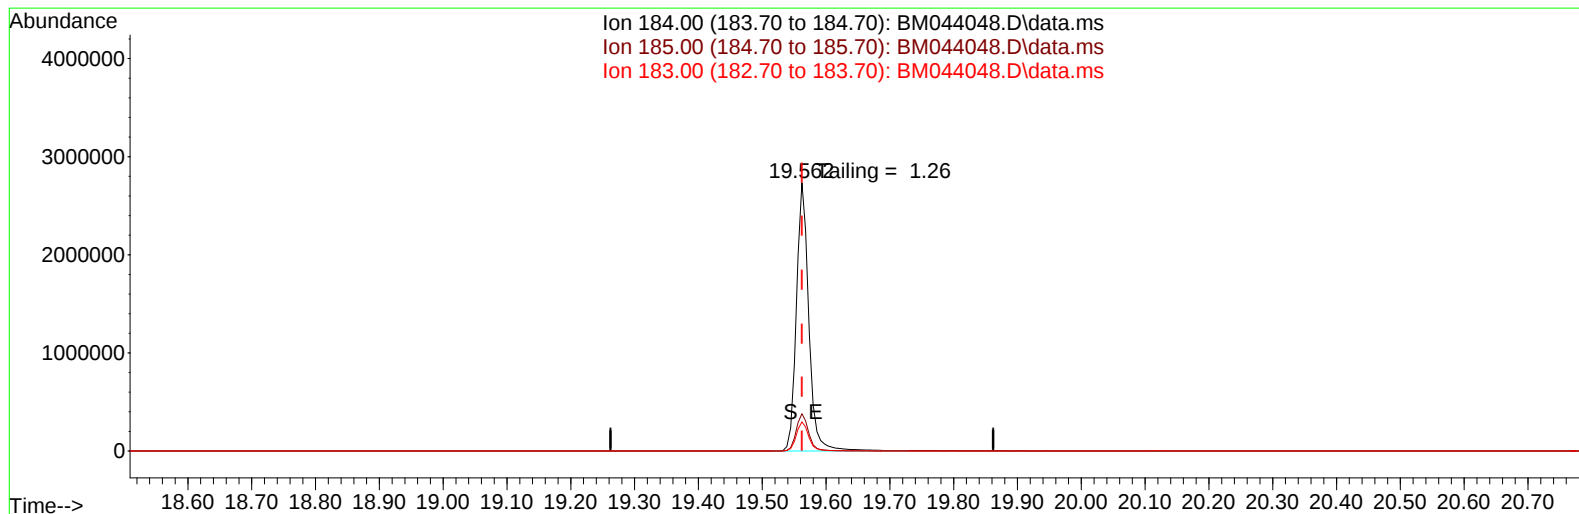

TIC: BM044048.D\data.ms

(77) Benzidine**19.562min (-0.000) 993297.92 ng****response 3720135**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.93
183.00	11.20	10.87
0.00	0.00	0.00