

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021224\
 Data File : BM044056.D
 Acq On : 12 Feb 2024 14:41
 Operator : MA/JU
 Sample : PB158276BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB158276BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM044056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	325	330	338	rBV	205507	290941	1.78%	0.296%
2	5.481	400	407	421	rBV	9260541	13223123	80.92%	13.472%
3	7.075	670	678	693	rBV	8136782	12929857	79.12%	13.173%
4	7.904	811	819	827	rBV	1671713	2614862	16.00%	2.664%
5	9.075	1009	1018	1031	rBV	4904267	8238777	50.42%	8.394%
6	10.710	1287	1296	1305	rBV	2022555	3499540	21.42%	3.565%
7	13.174	1705	1715	1727	rBV	10573466	16282252	99.64%	16.589%
8	14.545	1941	1948	1959	rBV	2636473	4008230	24.53%	4.084%
9	16.039	2194	2202	2234	rBV	6438282	9605265	58.78%	9.786%
10	17.298	2409	2416	2430	rBV	2797529	4116473	25.19%	4.194%
11	19.650	2812	2816	2821	rBV	204970	230441	1.41%	0.235%
12	19.939	2859	2865	2879	rBV	12554063	16341318	100.00%	16.649%
13	21.497	3125	3130	3142	rBV2	2582862	3401710	20.82%	3.466%
14	23.897	3531	3538	3548	rVB	1576124	3370072	20.62%	3.433%




Sum of corrected areas: 98152861

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021224\
Data File : BM044056.D
Acq On : 12 Feb 2024 14:41
Operator : MA/JU
Sample : PB158276BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB158276BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

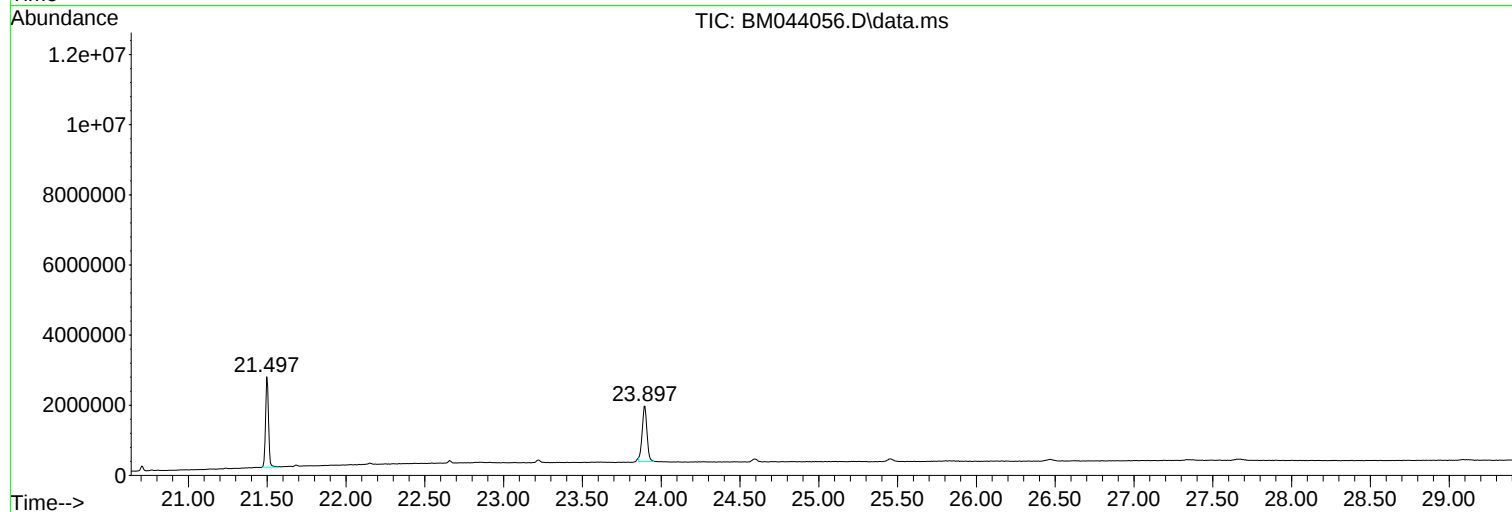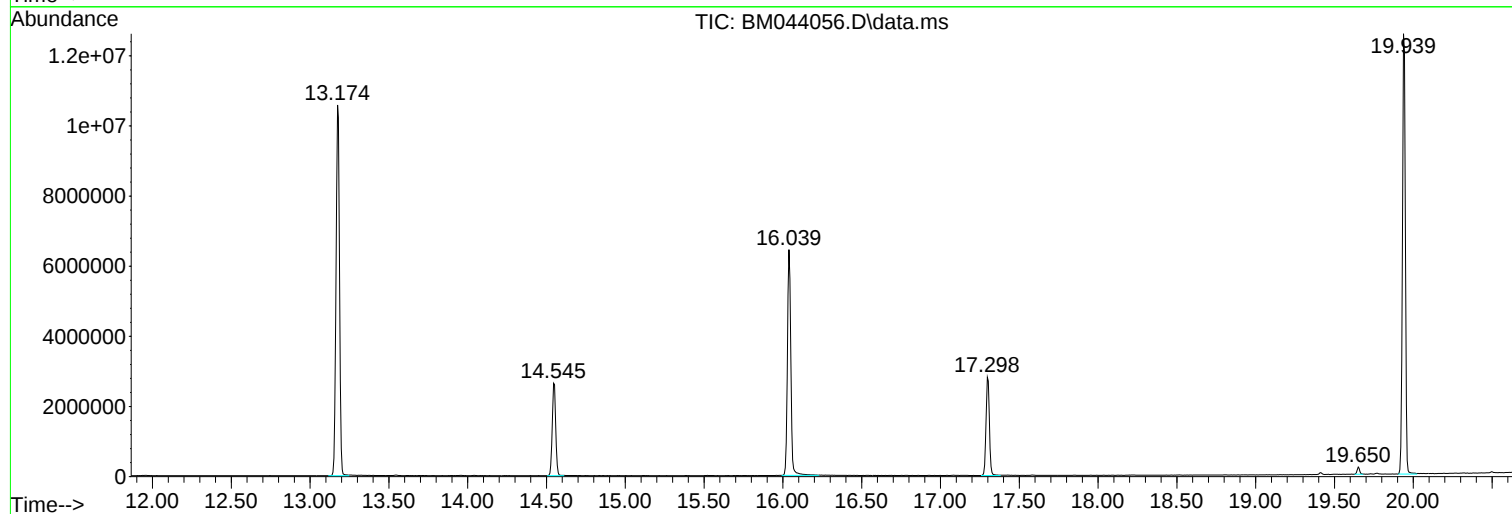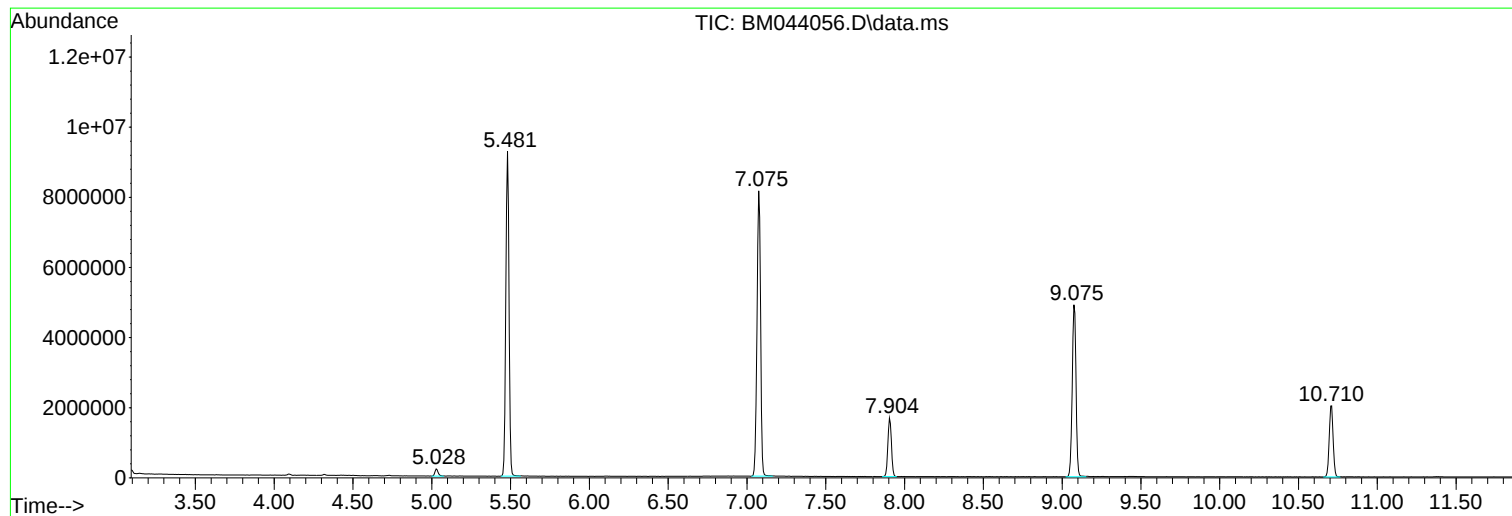

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021224\
Data File : BM044056.D
Acq On : 12 Feb 2024 14:41
Operator : MA/JU
Sample : PB158276BL
Misc :
ALS Vial : 9 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB158276BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.028	2.23 ng	290941	1,4-Dichlorobenzene-d4	7.904	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2	Hexanamide	115	C6H13NO	000628-02-4	25
3	2,5,8,11-Tetraoxadodecane	178	C8H18O4	000112-49-2	23
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
5	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	23

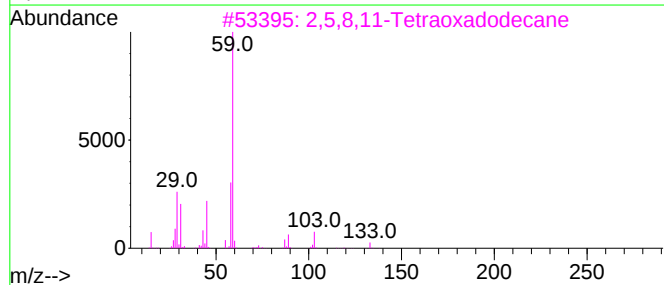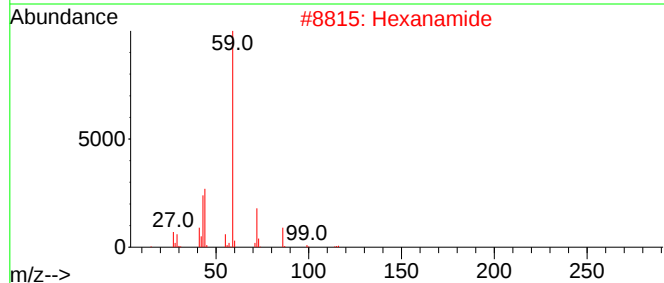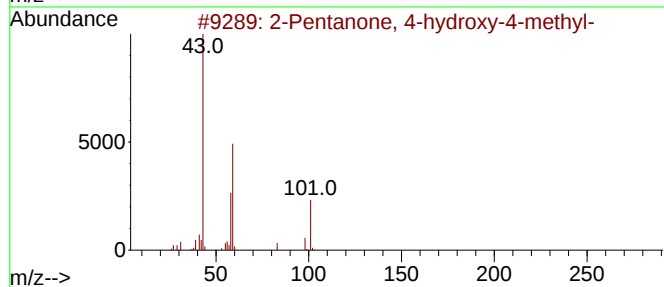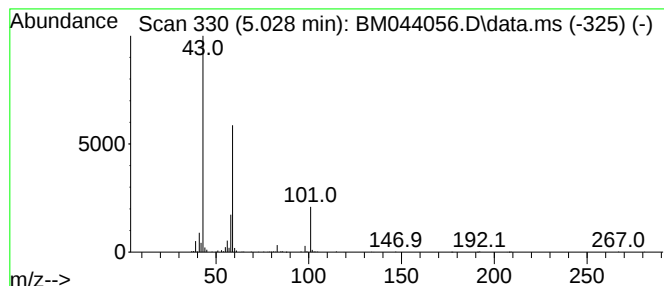

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021224\
Data File : BM044056.D
Acq On : 12 Feb 2024 14:41
Operator : MA/JU
Sample : PB158276BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB158276BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.028	2.2	ng	290941	1	7.904	2614860	20.0