


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021224\
Data File : BM044048.D
Acq On : 12 Feb 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 09 02:42:01 2024

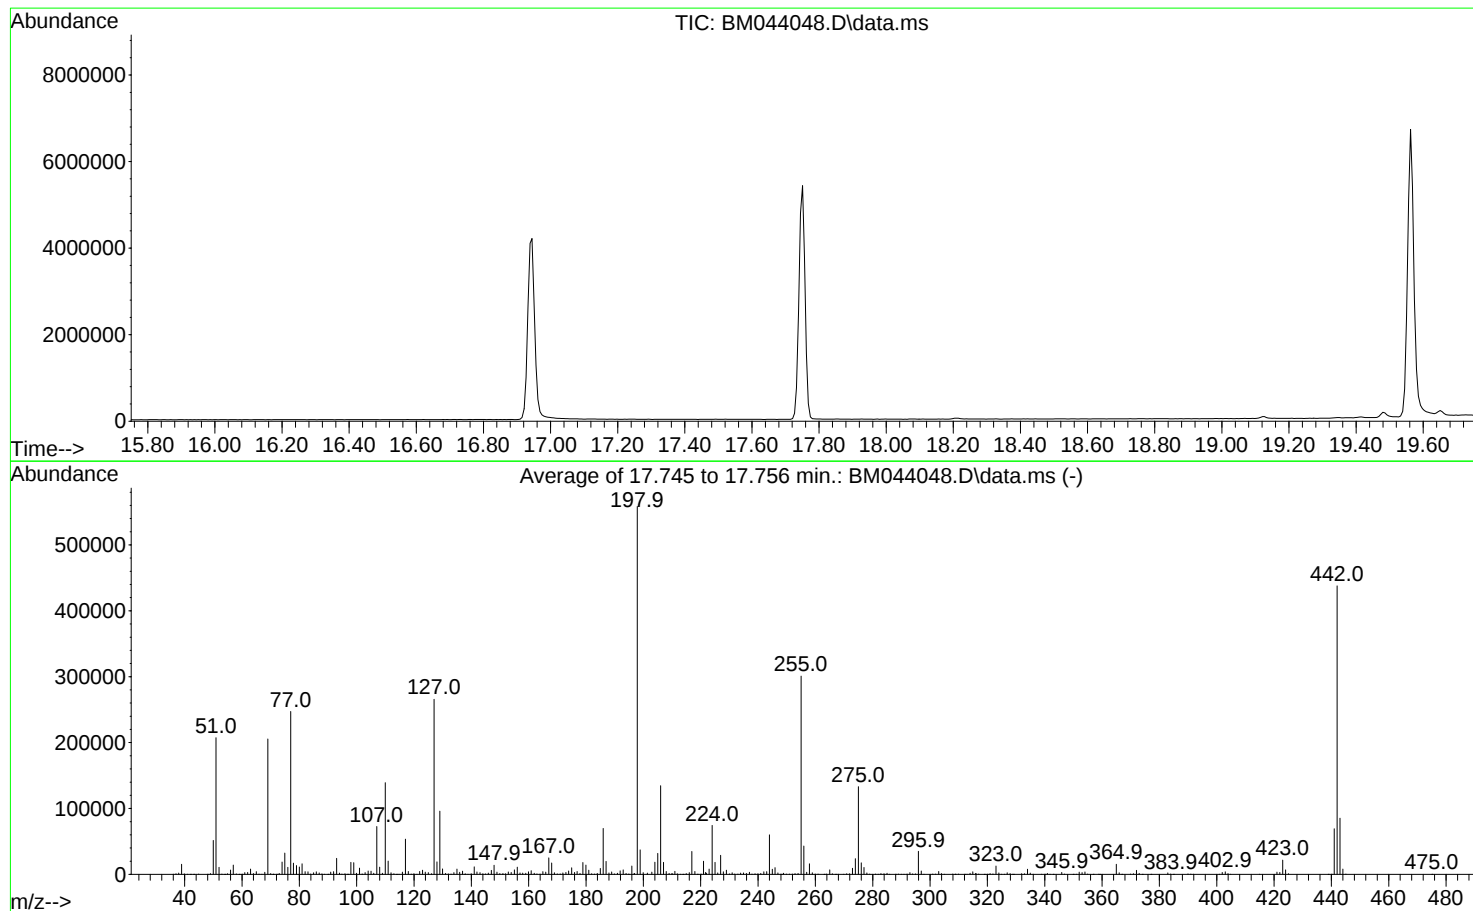




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	207487	PASS
68	69	0.00	2	1.6	3199	PASS
69	198	0.00	100	36.8	205483	PASS
70	69	0.00	2	0.5	1122	PASS
127	198	10	80	47.6	265792	PASS
197	198	0.00	2	0.2	1359	PASS
198	198	100	100	100.0	558315	PASS
199	198	5	9	6.7	37128	PASS
275	198	10	60	23.8	133053	PASS
365	198	1	100	2.7	15252	PASS
441	198	0.01	100	12.4	69243	PASS
442	442	50	100	100.0	437824	PASS
443	442	15	24	19.5	85213	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021224\
Data File : BM044048.D
Acq On : 12 Feb 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 12 11:30:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

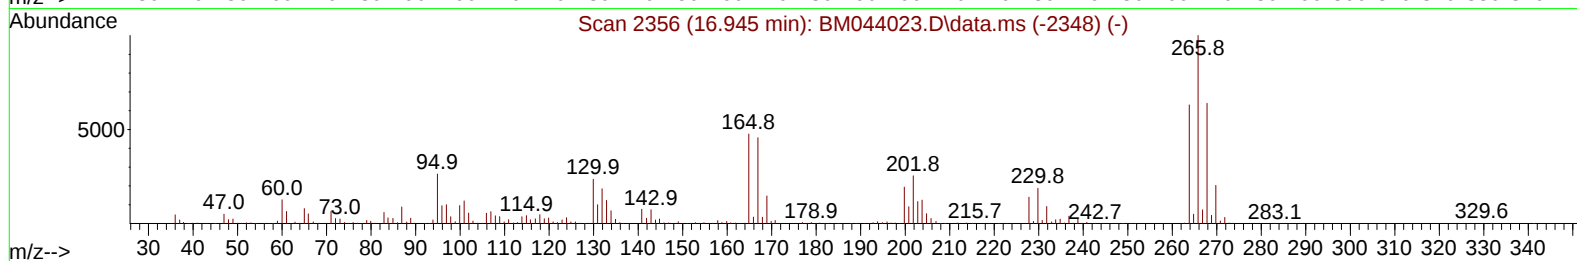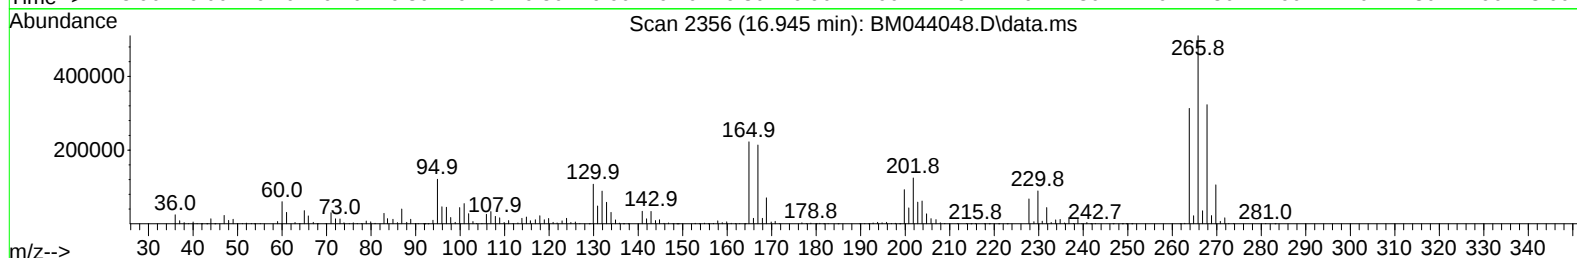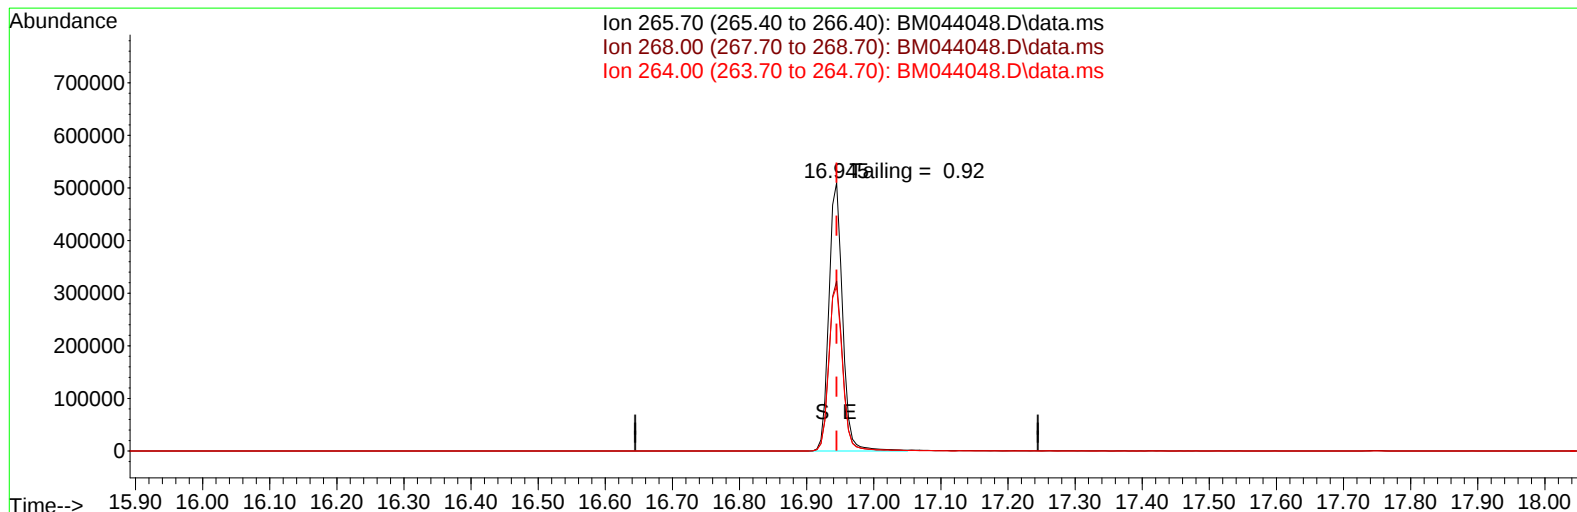

TIC: BM044048.D\data.ms

(70) Pentachlorophenol (C)

16.945min (-0.000) 0.00 ng




response 723381

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.35
264.00	63.10	61.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021224\
Data File : BM044048.D
Acq On : 12 Feb 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 12 11:30:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

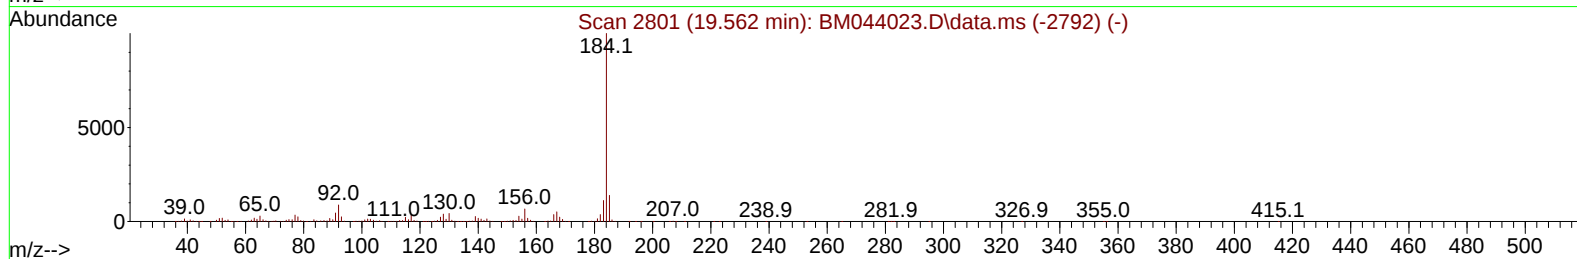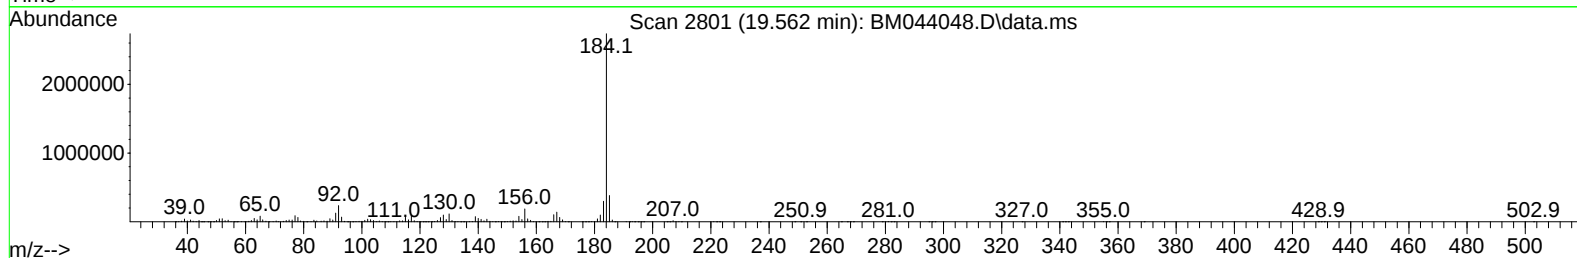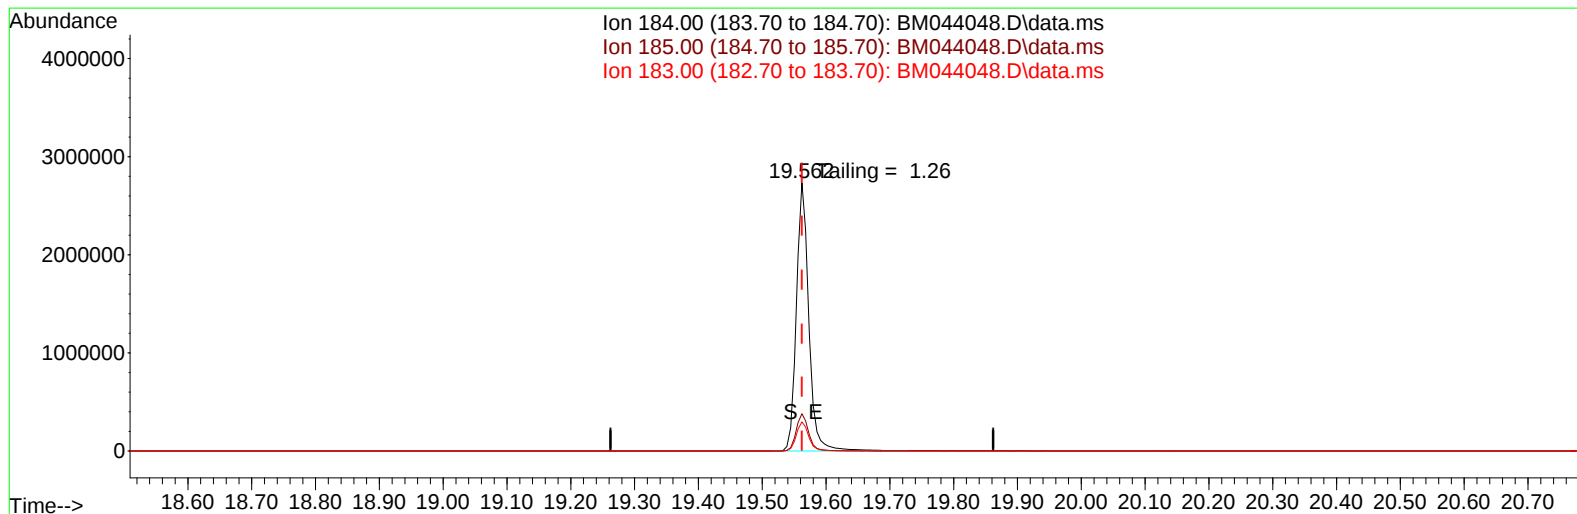

TIC: BM044048.D\data.ms

(77) Benzidine

19.562min (-0.000) 993297.92 ng

response 3720135

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.93
183.00	11.20	10.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/12/2024	BNA_M	<u>BM044048.D</u>
Compound Name	Response	Retention Time
DDT	1897326	20.797
DDD	26451	20.403
DDE	3113	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29564	1926890	1.53

Instrument :
BNA_M
ClientSampleId :
DFTPP