




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049629.D
Acq On : 12 Feb 2025 21:33
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29C6

Manual IntegrationsAPPROVED

Quant Time: Feb 14 16:32:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

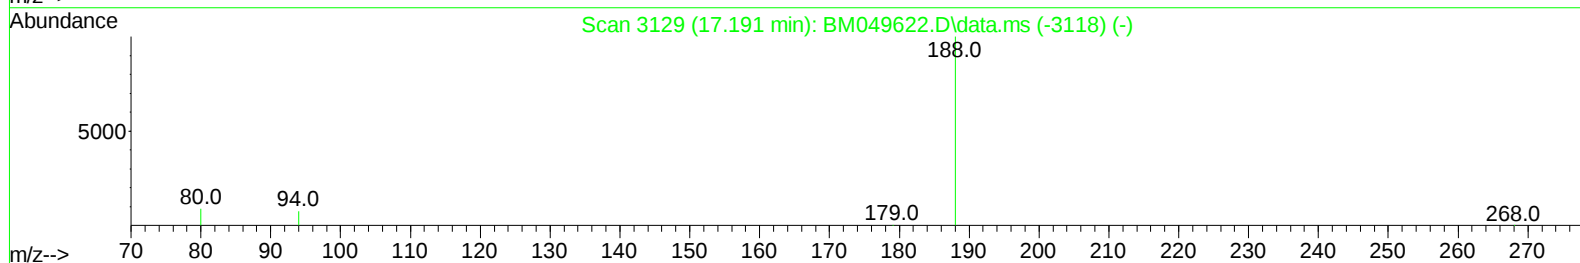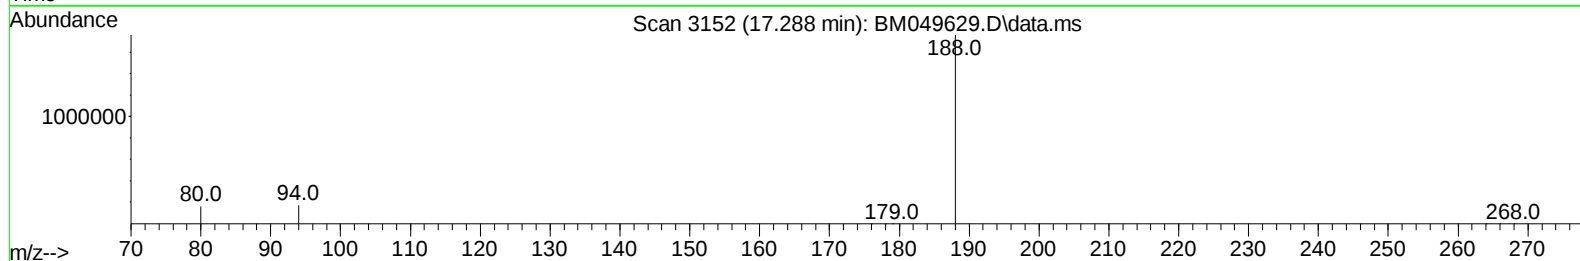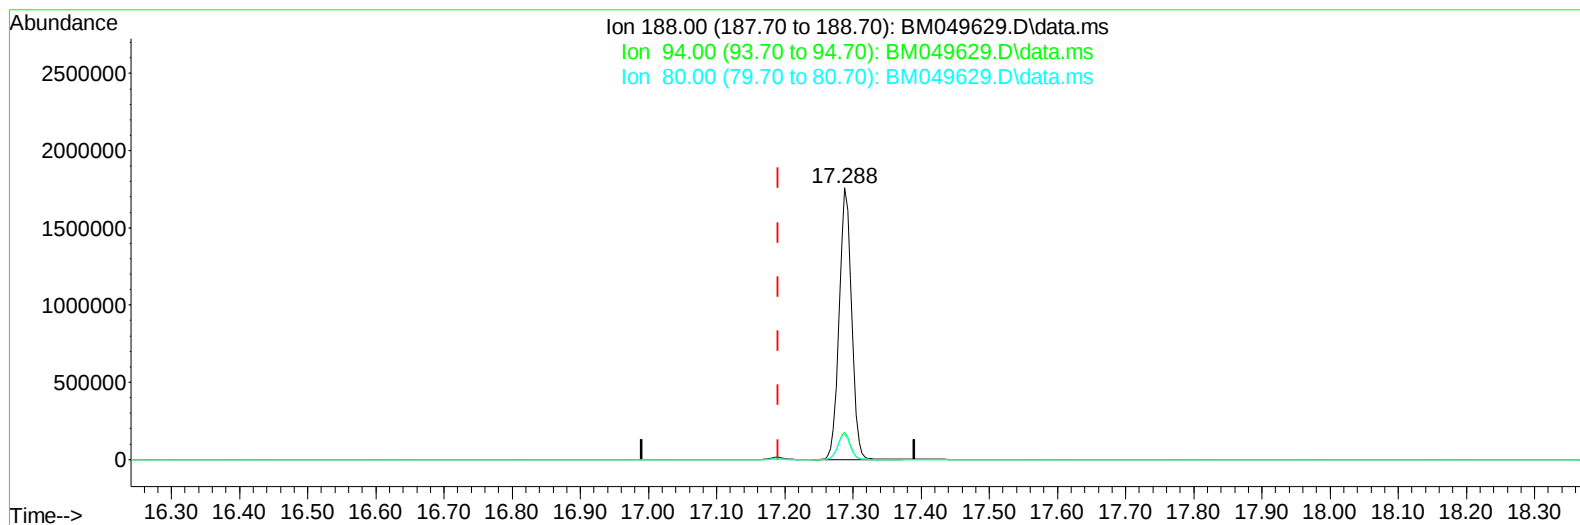

TIC: BM049629.D\data.ms

(13) Phenanthrene-d10 (I)

17.288min (+ 0.097) 0.40 ng/u1

response 2219244

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.50	10.00
80.00	9.30	9.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049629.D
Acq On : 12 Feb 2025 21:33
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29C6

Manual IntegrationsAPPROVED

Quant Time: Feb 14 16:32:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

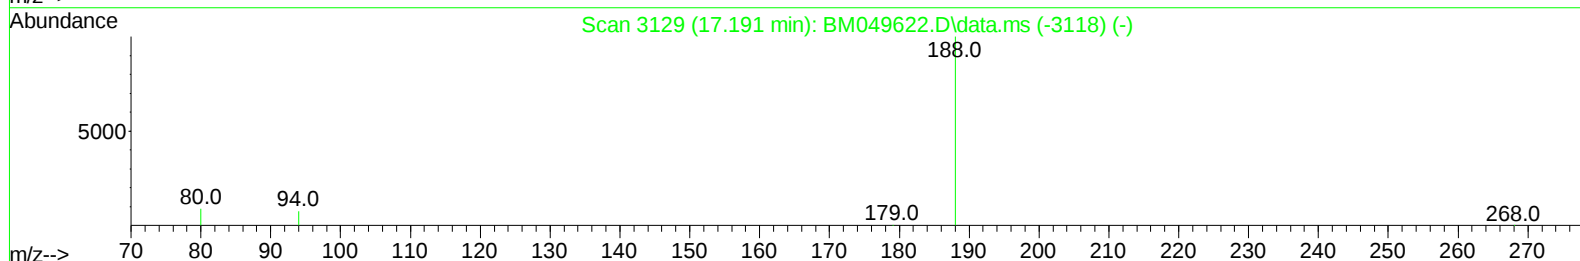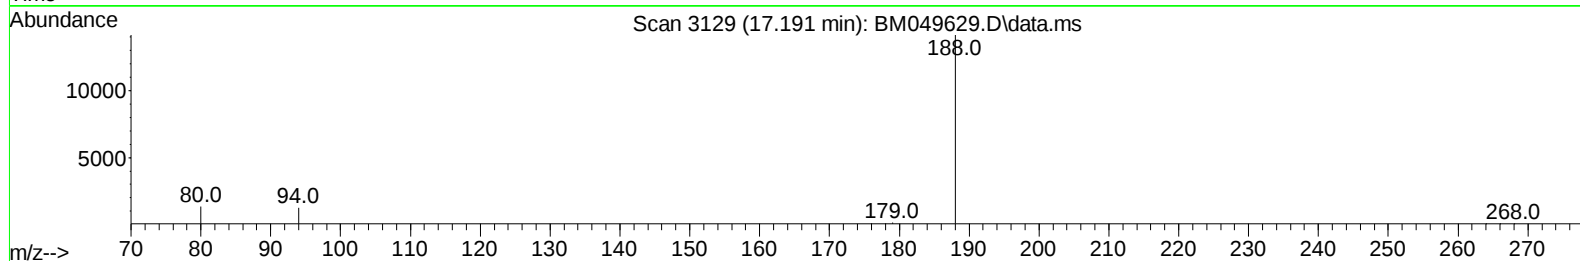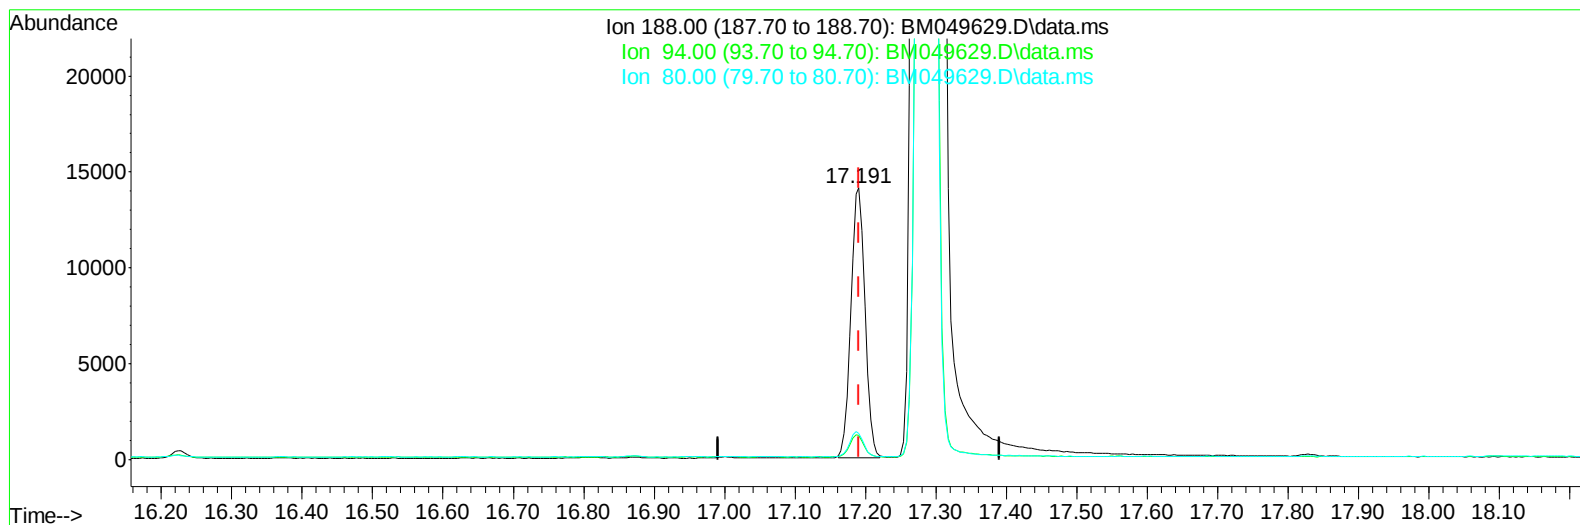

TIC: BM049629.D\data.ms

(13) Phenanthrene-d10 (I)

17.191min (-0.000) 0.40 ng/ul m

response 19420

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.50	8.75
80.00	9.30	9.49
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049629.D
Acq On : 12 Feb 2025 21:33
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29C6

Manual IntegrationsAPPROVED

Quant Time: Feb 14 16:32:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

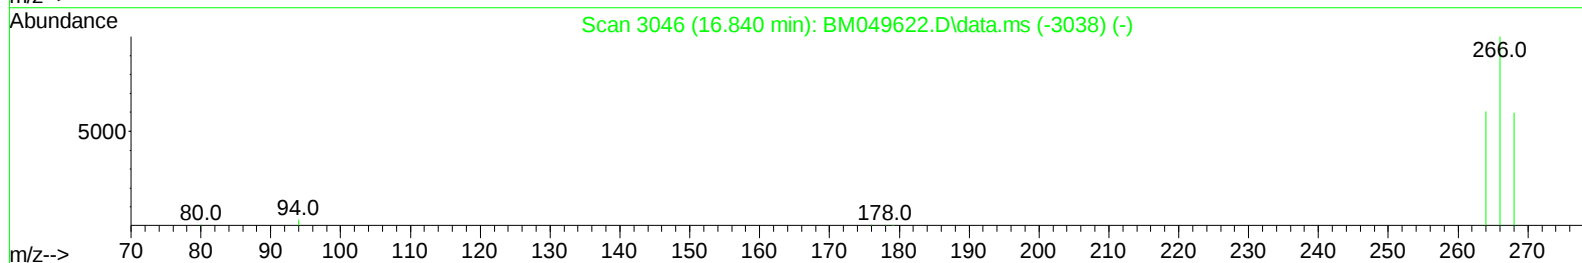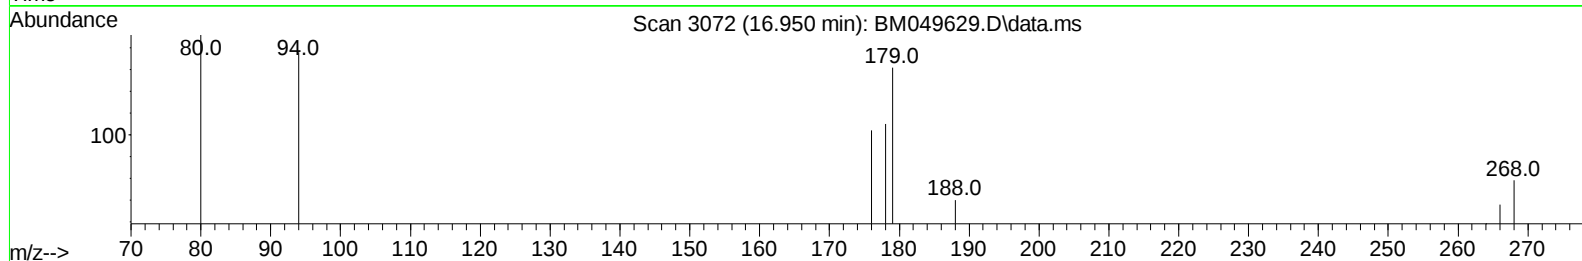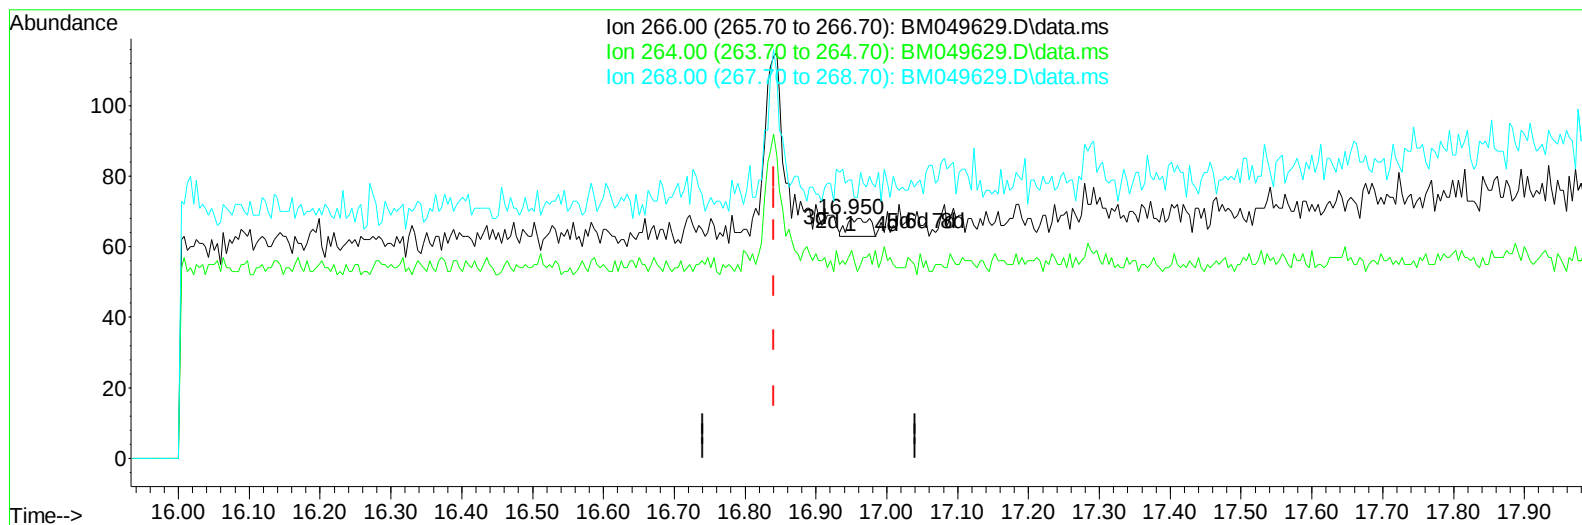

TIC: BM049629.D\data.ms

(14) Pentachloropheno1

16.950min (+ 0.110) 0.00 ng/u1

response 11

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.90	27.27#
268.00	61.50	36.36#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049629.D
Acq On : 12 Feb 2025 21:33
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29C6

Manual IntegrationsAPPROVED

Quant Time: Feb 14 16:32:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

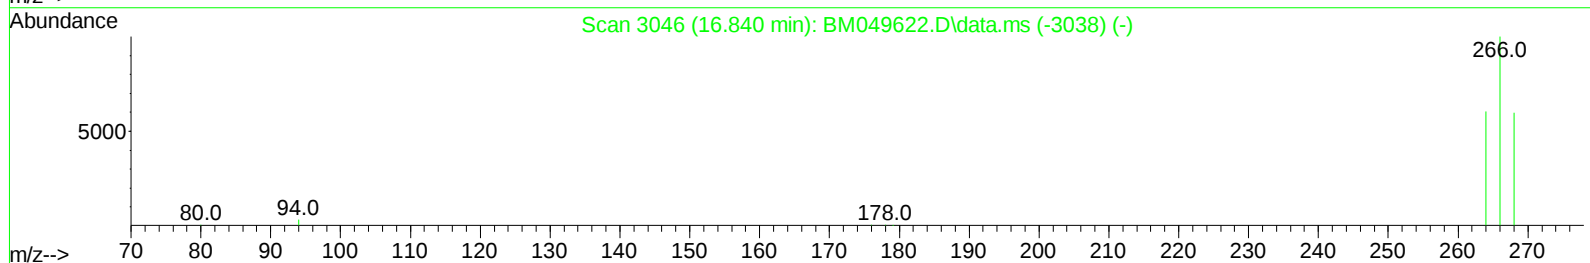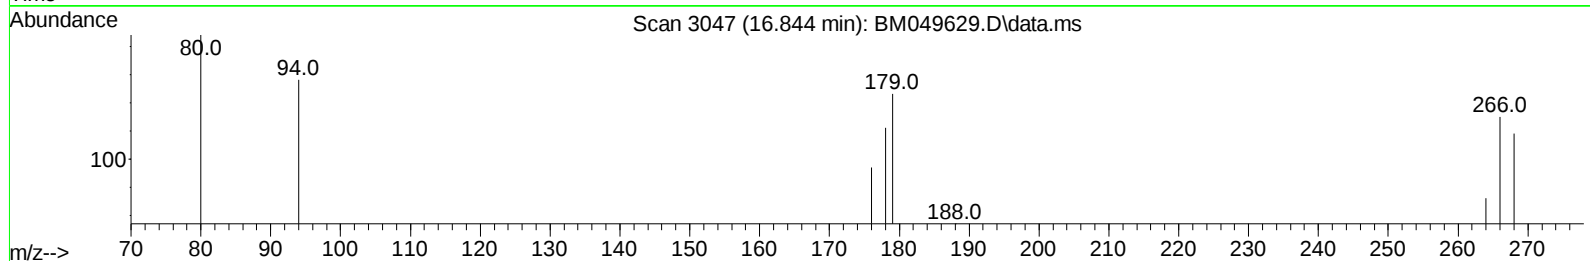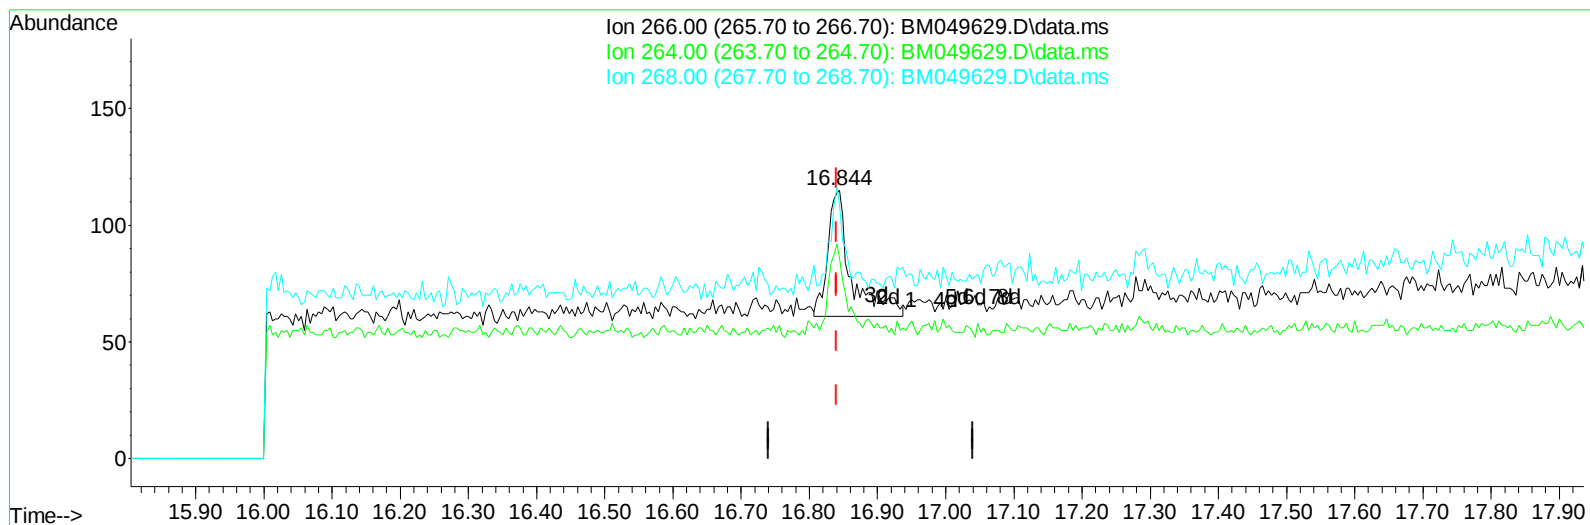

TIC: BM049629.D\data.ms

(14) Pentachloropheno1

16.844min (+ 0.004) 0.03 ng/ul m

response 130

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.90	2.31#
268.00	61.50	3.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049629.D
Acq On : 12 Feb 2025 21:33
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29C6

Manual IntegrationsAPPROVED

Quant Time: Feb 14 16:32:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

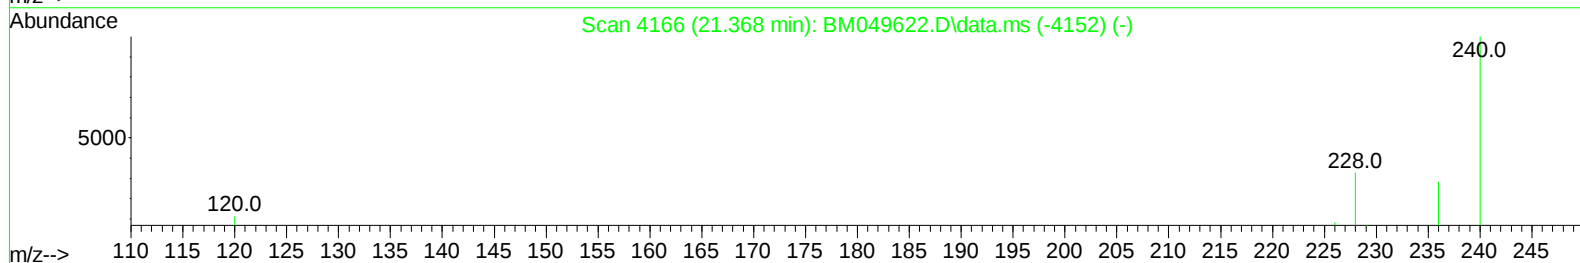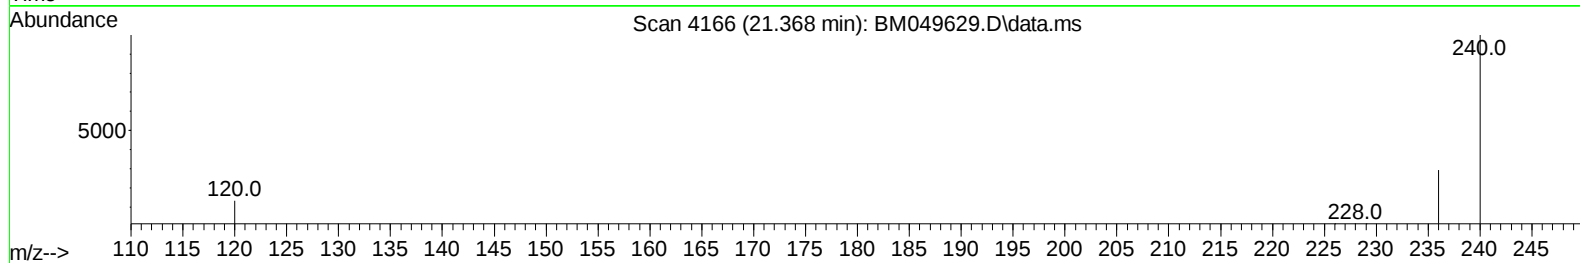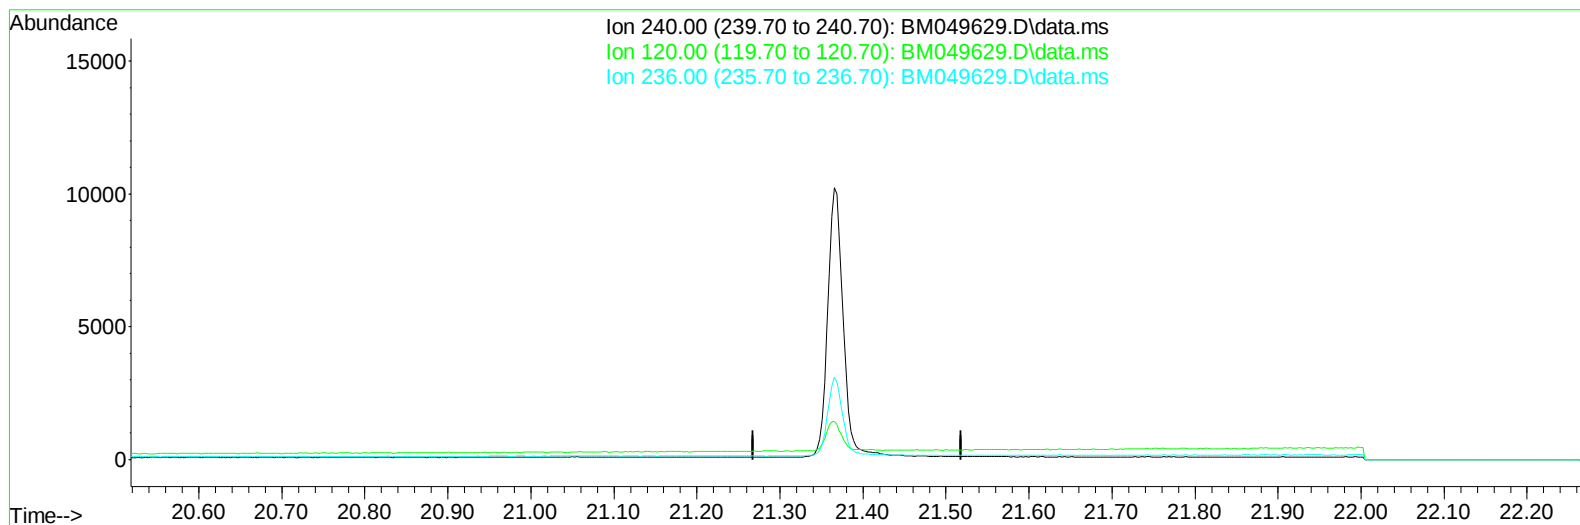

TIC: BM049629.D\data.ms

(17) Chrysene-d12

21.368min (-21.368) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	12.90	0.00#
236.00	29.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049629.D
Acq On : 12 Feb 2025 21:33
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29C6

Manual IntegrationsAPPROVED

Quant Time: Feb 14 16:32:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

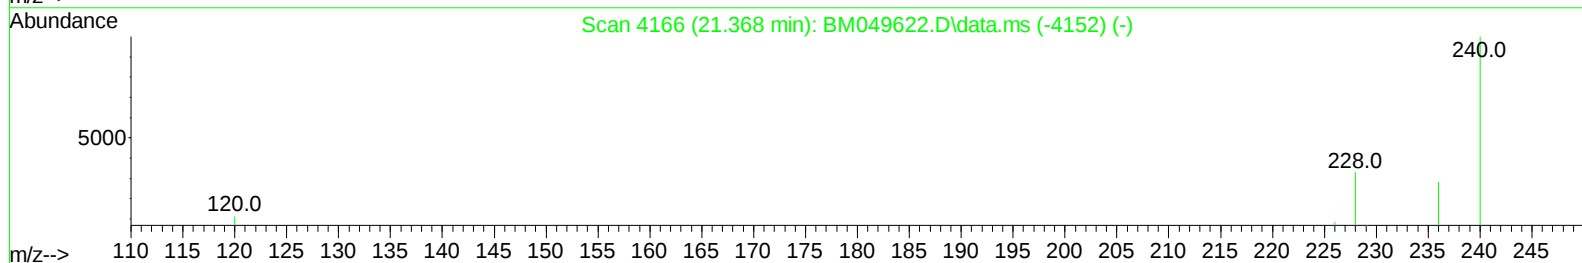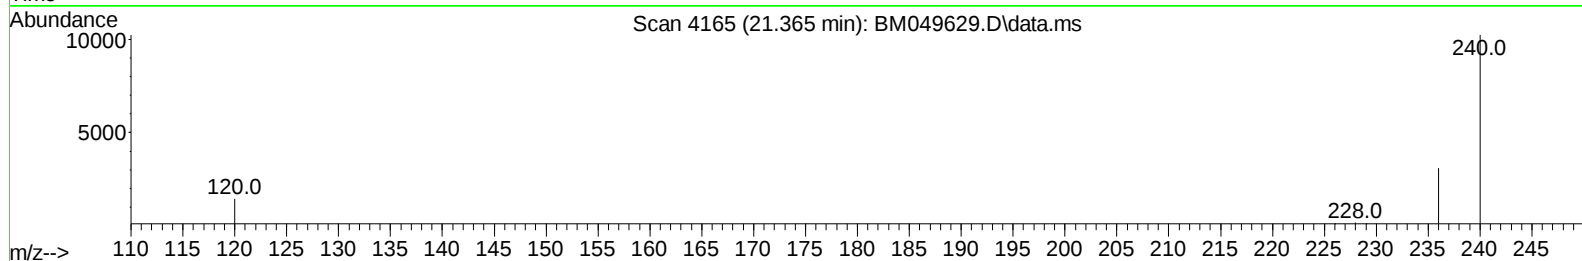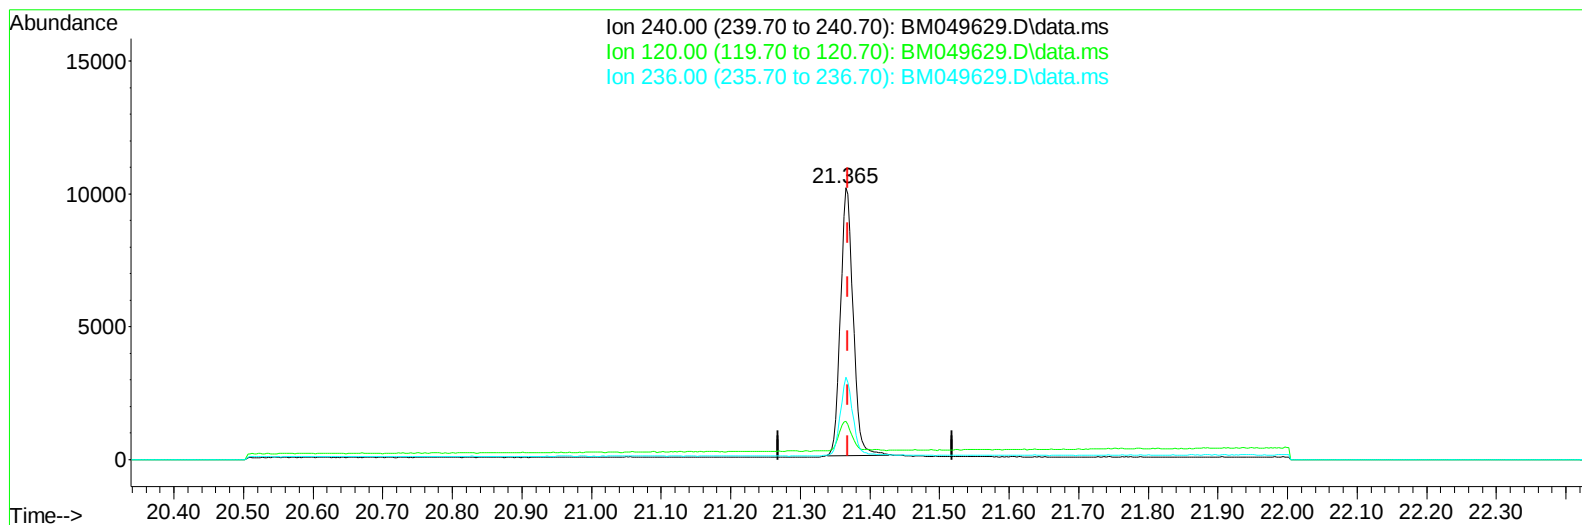

TIC: BM049629.D\data.ms

(17) Chrysene-d12

21.365min (-0.003) 0.40 ng/ul m

response 12808

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	12.90	14.07
236.00	29.30	30.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049629.D
Acq On : 12 Feb 2025 21:33
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29C6

Manual IntegrationsAPPROVED

Quant Time: Feb 14 16:32:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

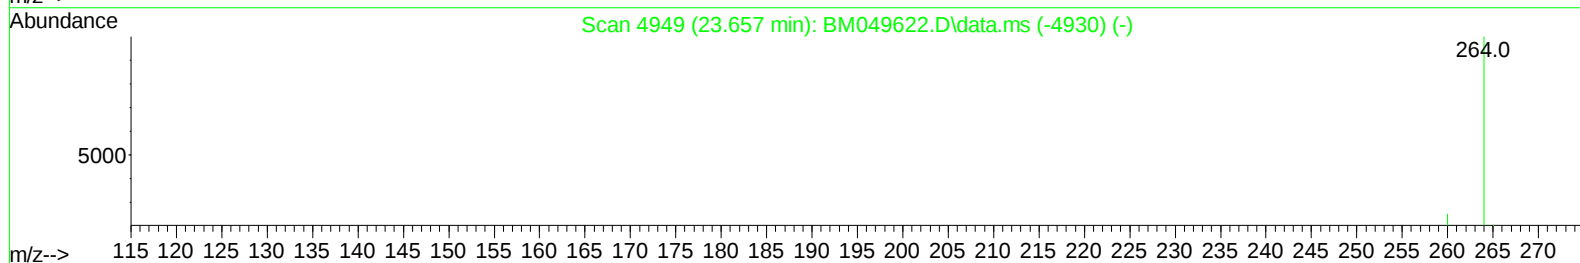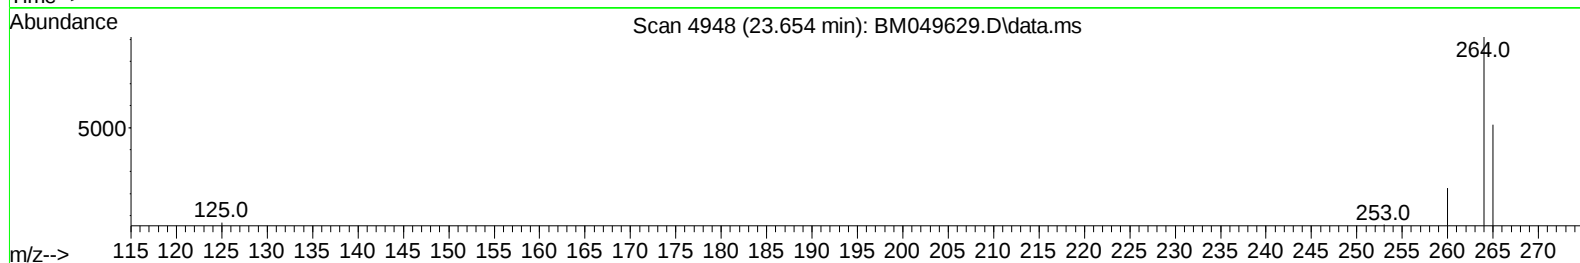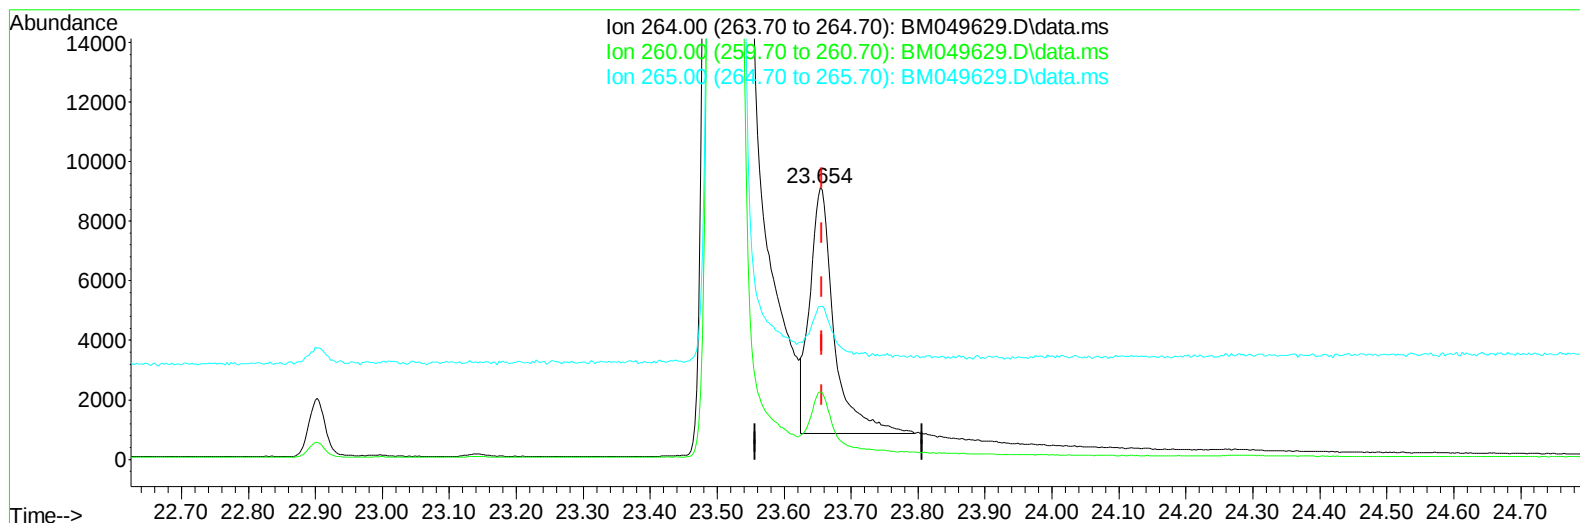

TIC: BM049629.D\data.ms

(23) Perylene-d12 (I)

23.654min (-0.003) 0.40 ng/u1

response 20846

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	24.87
265.00	67.10	56.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049629.D
Acq On : 12 Feb 2025 21:33
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29C6

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

Quant Time: Feb 14 16:32:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

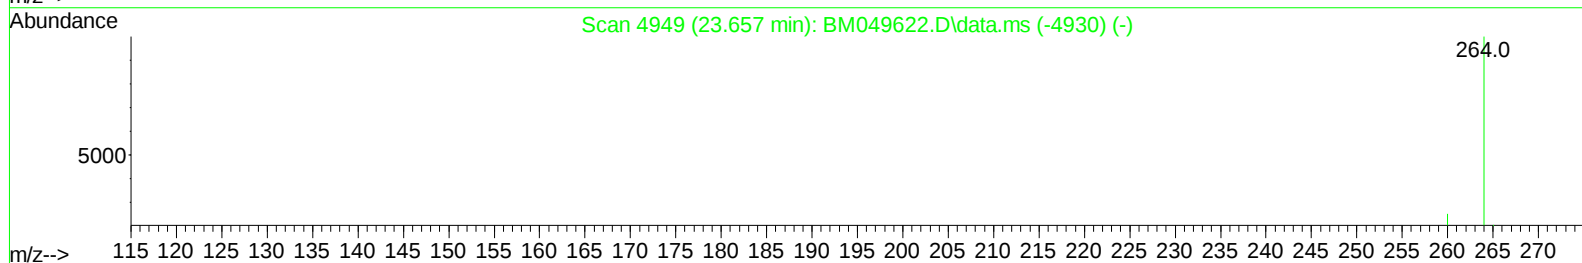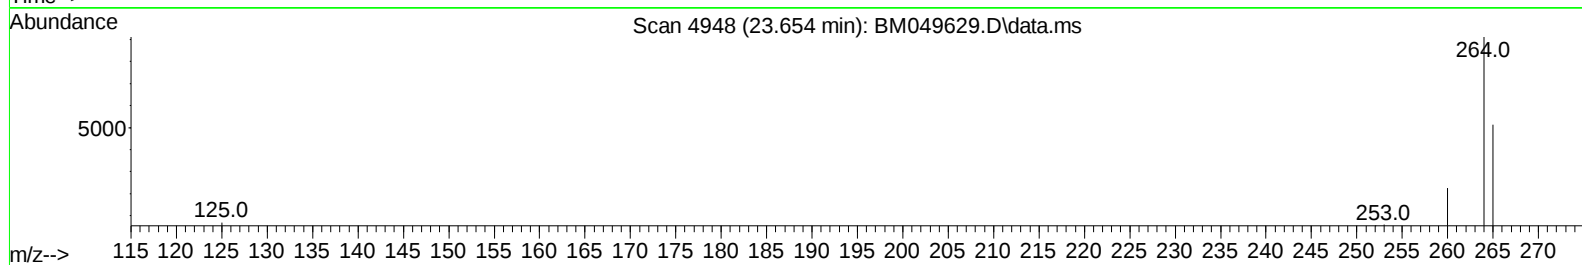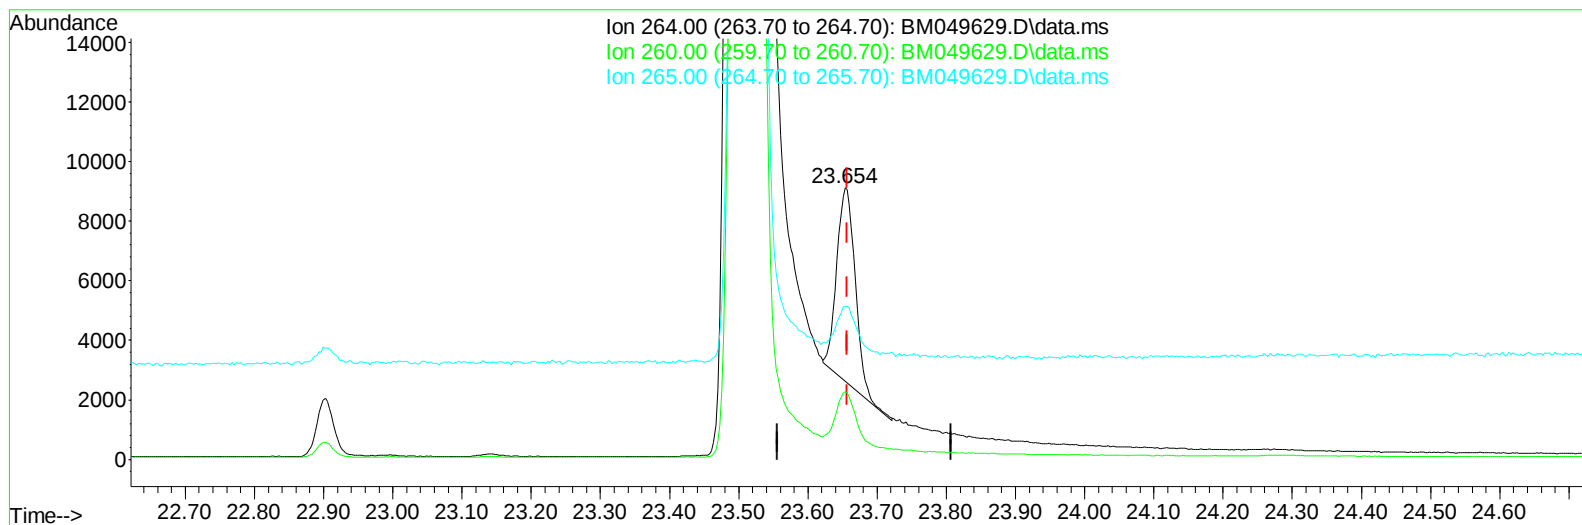

TIC: BM049629.D\data.ms

(23) Perylene-d12 (I)

23.654min (-0.003) 0.40 ng/ul m

response 11984

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	24.87
265.00	67.10	56.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049629.D
Acq On : 12 Feb 2025 21:33
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29C6

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

Quant Time: Feb 14 16:32:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

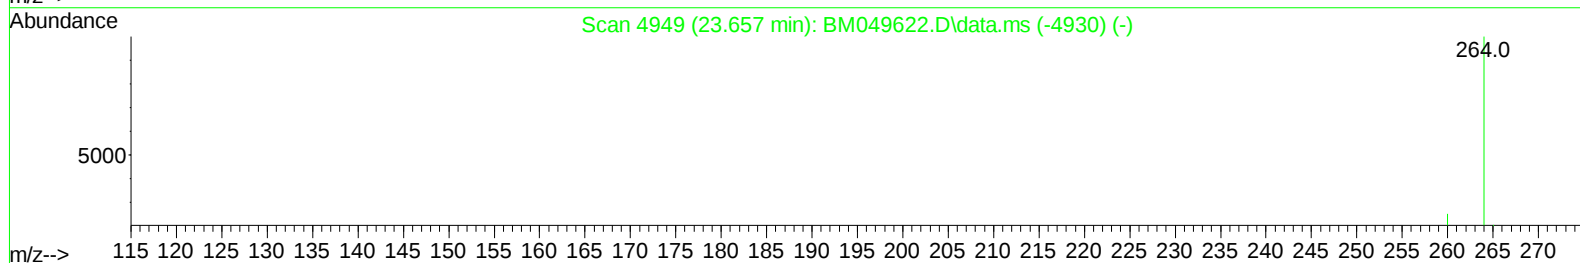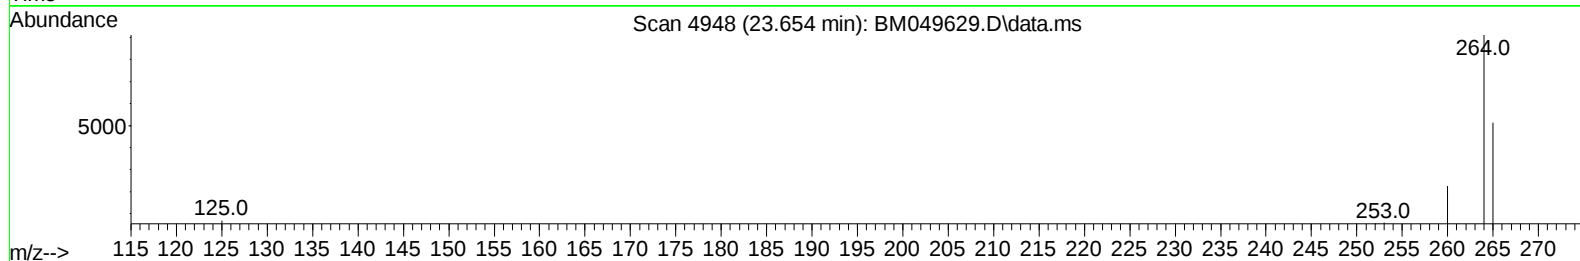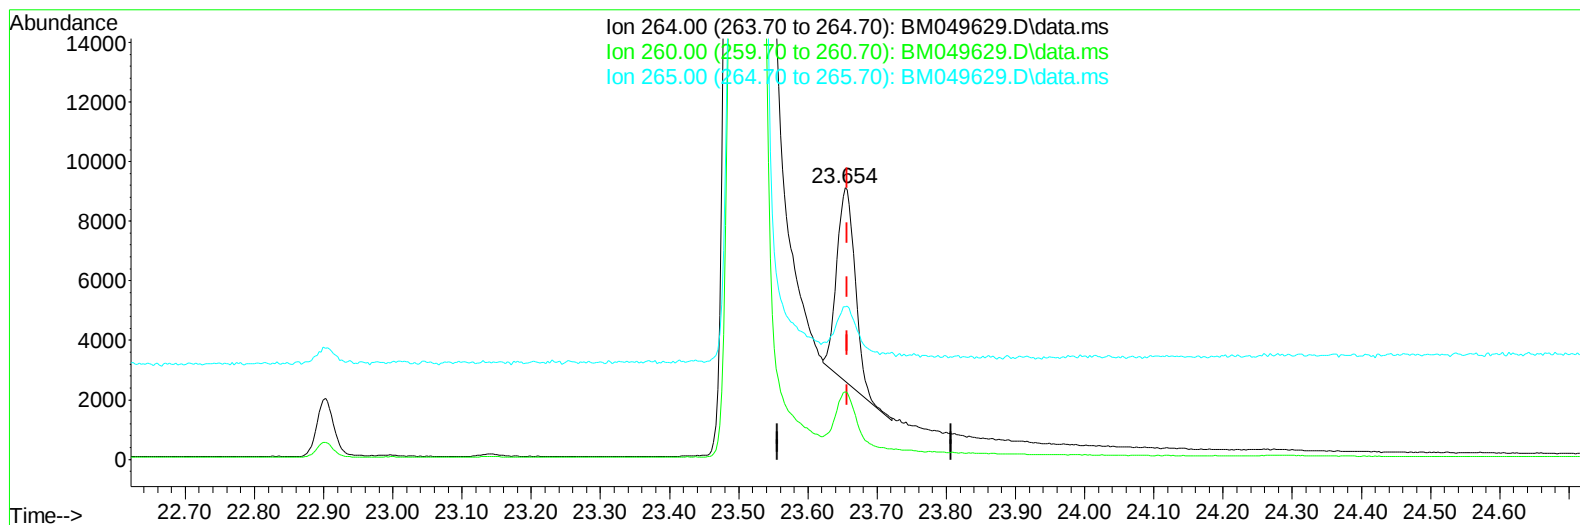

TIC: BM049629.D\data.ms

(23) Perylene-d12 (I)

23.654min (-0.003) 0.40 ng/ul m

response 11984

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	24.87
265.00	67.10	56.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
 Data File : BM049629.D
 Acq On : 12 Feb 2025 21:33
 Operator : RC/JU
 Sample : Q1336-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E29C6

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 02/19/2025
 Supervised By :Jagrut Upadhyay 02/19/2025

Quant Time: Feb 14 16:32:46 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 12 16:40:36 2025
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.813	152		5699	0.400	ng/ul	0.00
4) Naphthalene-d8	10.605	136		15679	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.450	164		9151	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.191	188		19420m	0.400	ng/ul	0.00
17) Chrysene-d12	21.365	240		12808m	0.400	ng/ul	0.00
23) Perylene-d12	23.654	264		11984m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.252	96		39893	6.223	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.200	152		8492	0.394	ng/ul	0.00
18) Fluoranthene-d10	19.215	212		21003	0.538	ng/ul	0.00
Target Compounds							Qvalue
14) Pentachlorophenol	16.844	266		130m	0.033	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049629.D
Acq On : 12 Feb 2025 21:33
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29C6

Manual IntegrationsAPPROVED

Quant Time: Feb 14 16:32:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

