




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

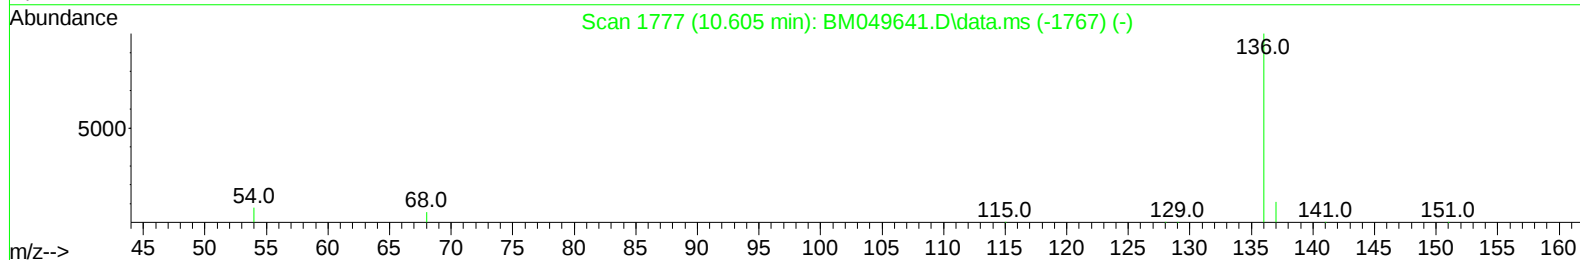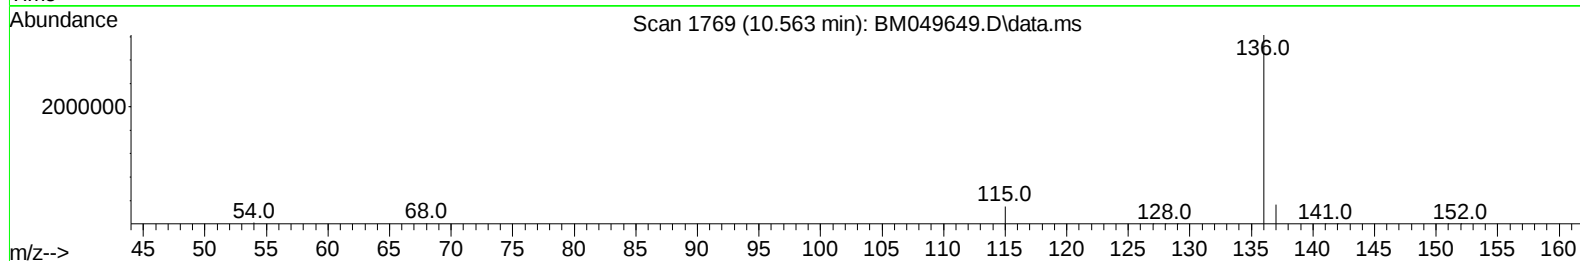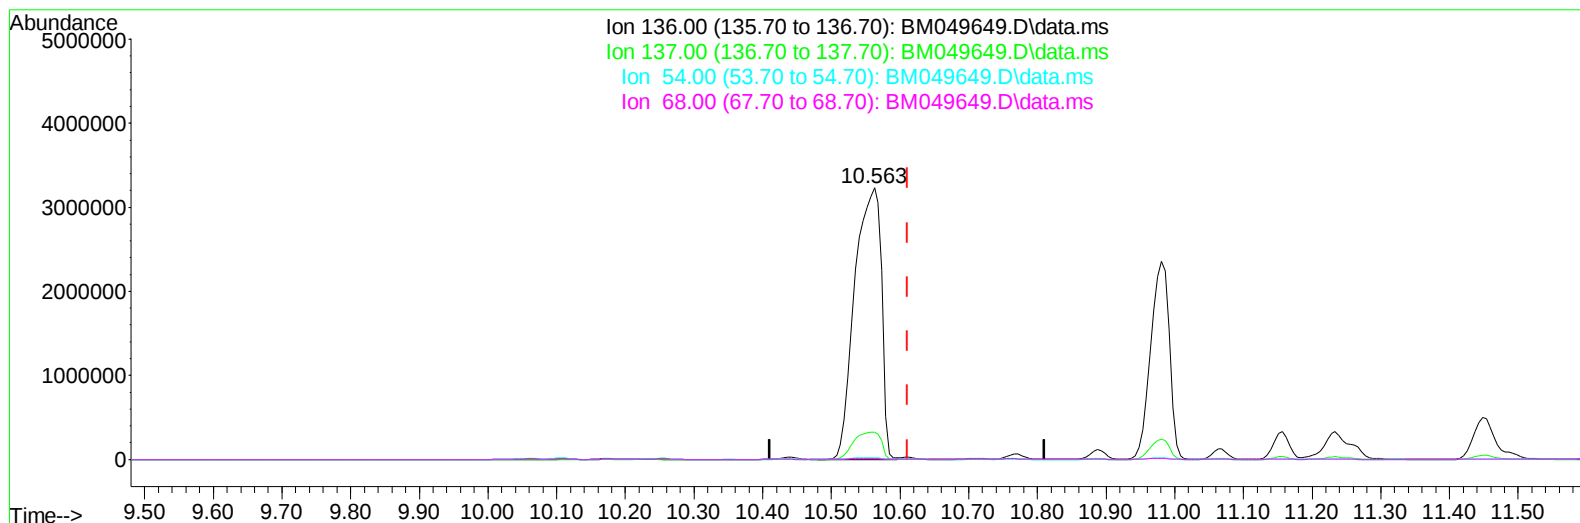

TIC: BM049649.D\data.ms

(4) Naphthalene-d8 (I)

10.563min (-0.048) 0.40 ng/u1

response 8694961

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.70	10.16
54.00	9.30	0.67#
68.00	7.30	0.50#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

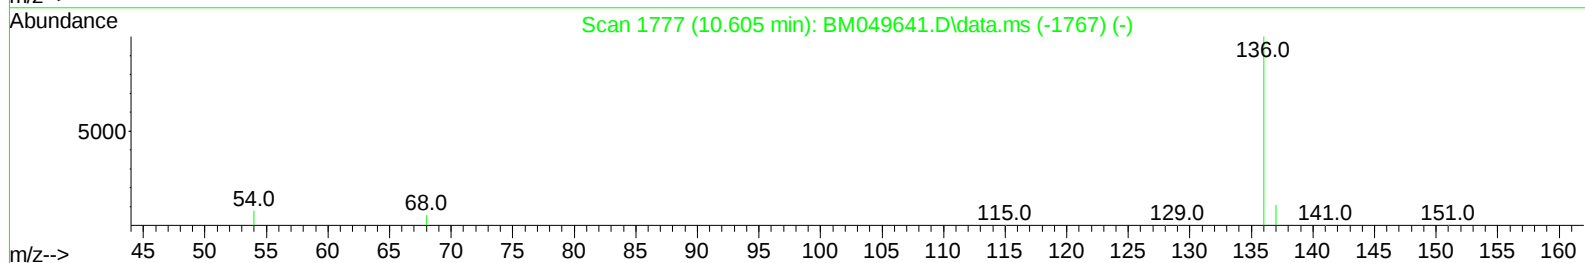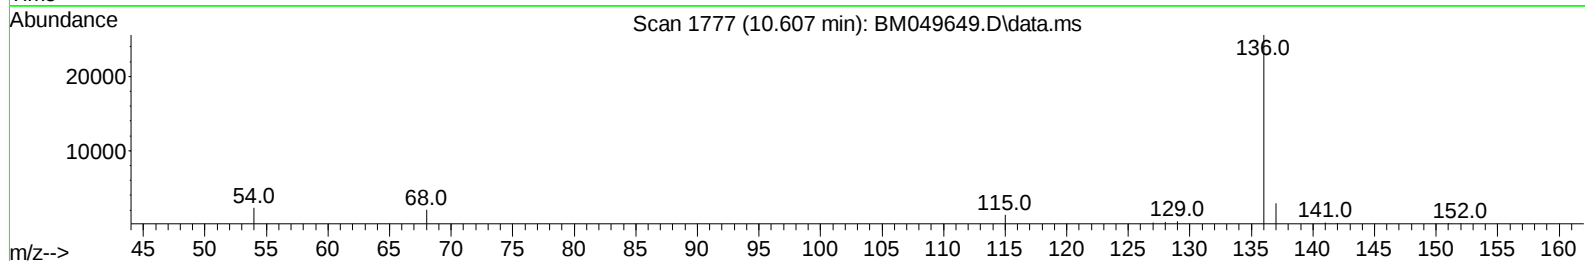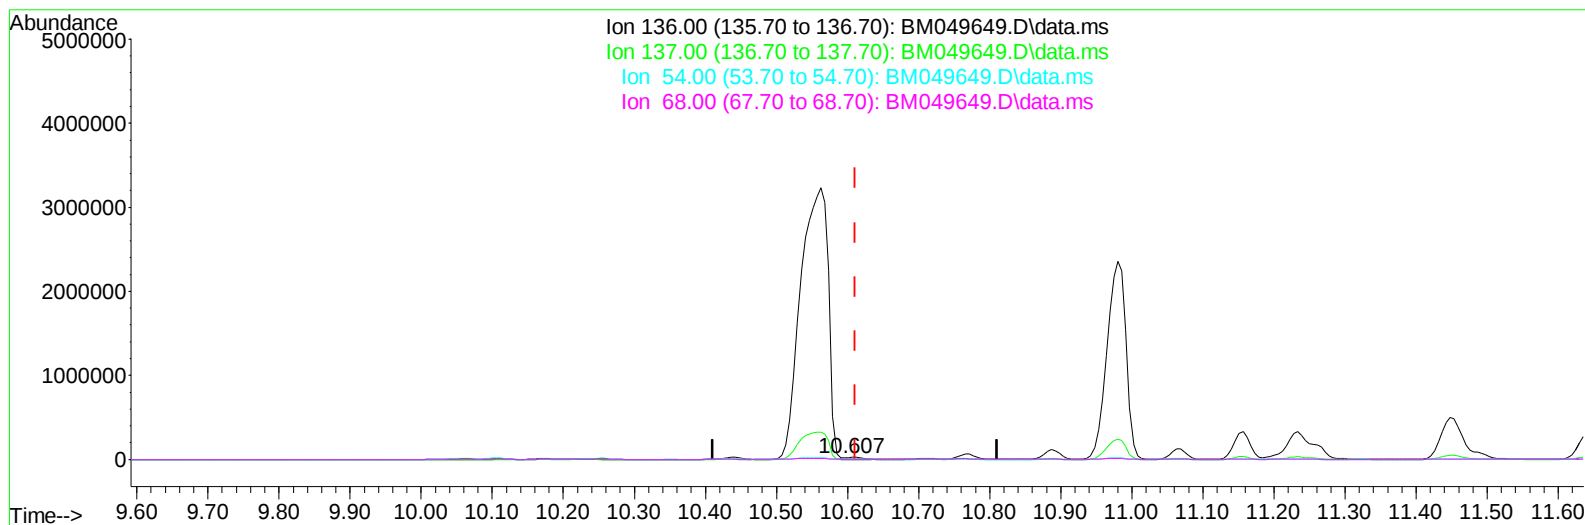

TIC: BM049649.D\data.ms

(4) Naphthalene-d8 (I)

10.607min (-0.004) 0.40 ng/ul m

response 45893

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.70	11.24
54.00	9.30	8.84
68.00	7.30	7.91




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

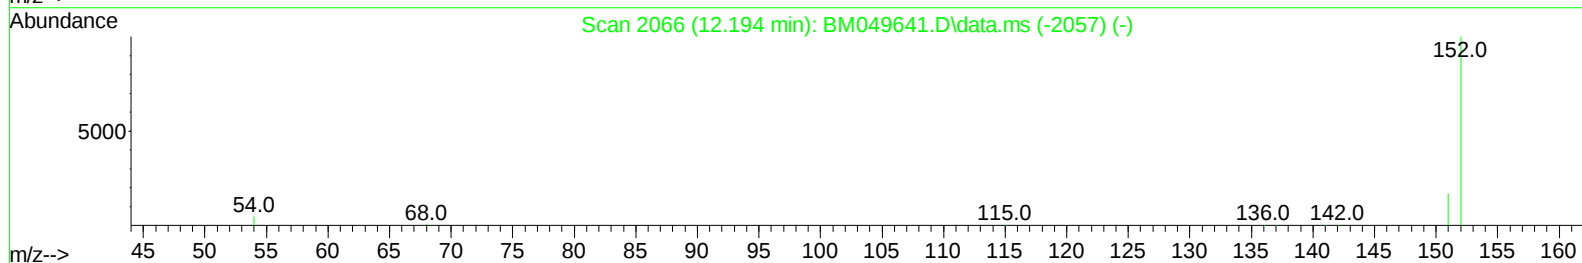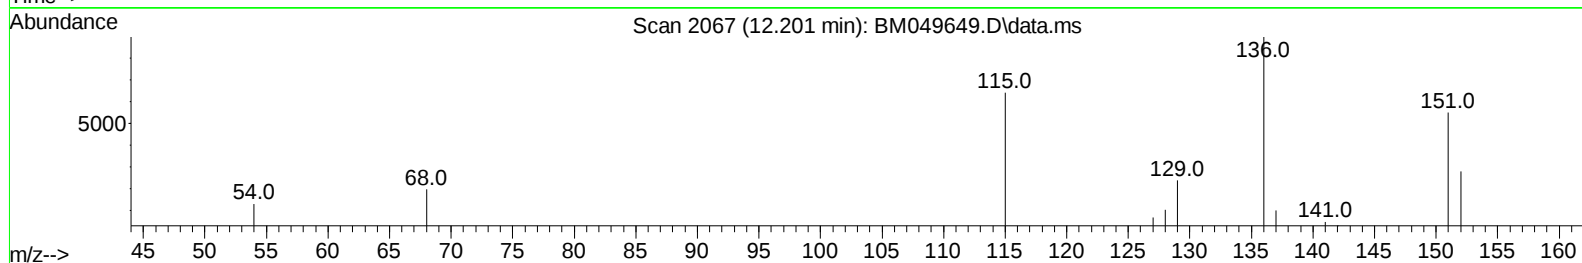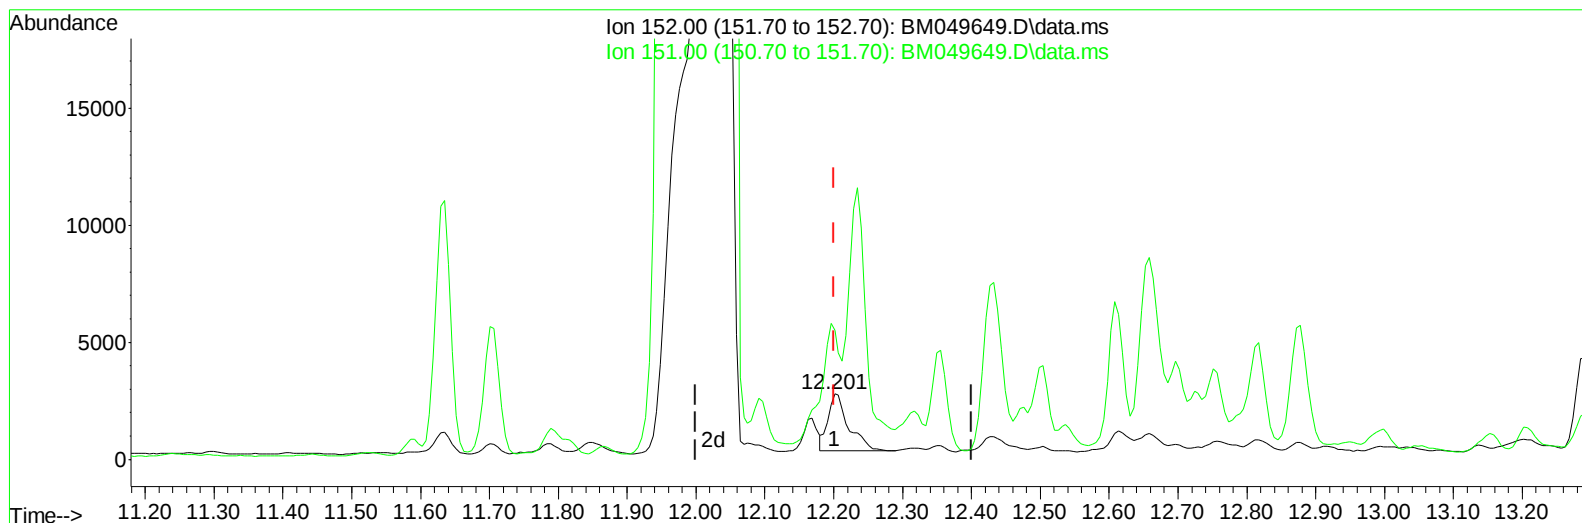

TIC: BM049649.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.201min (+ 0.001) 0.08 ng/u1

response 5123

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.10	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

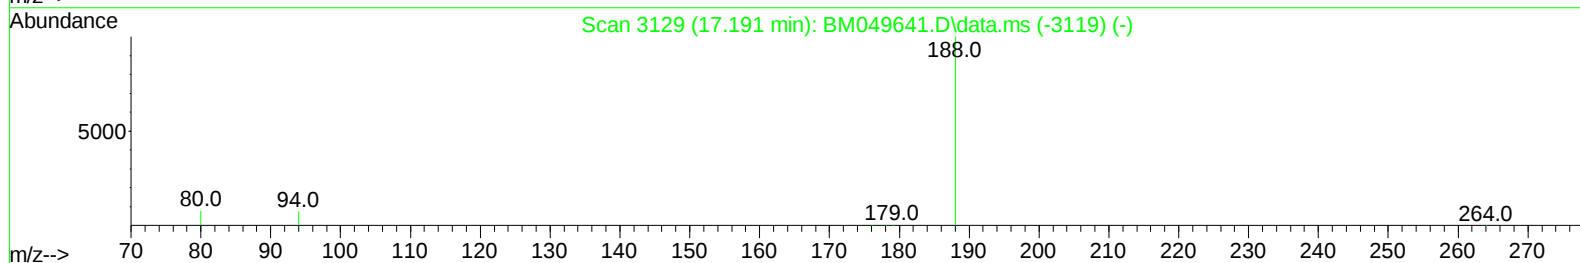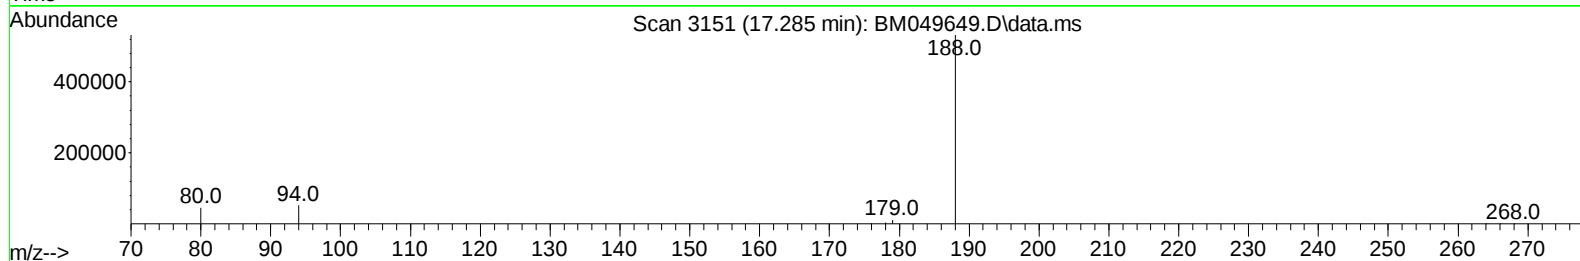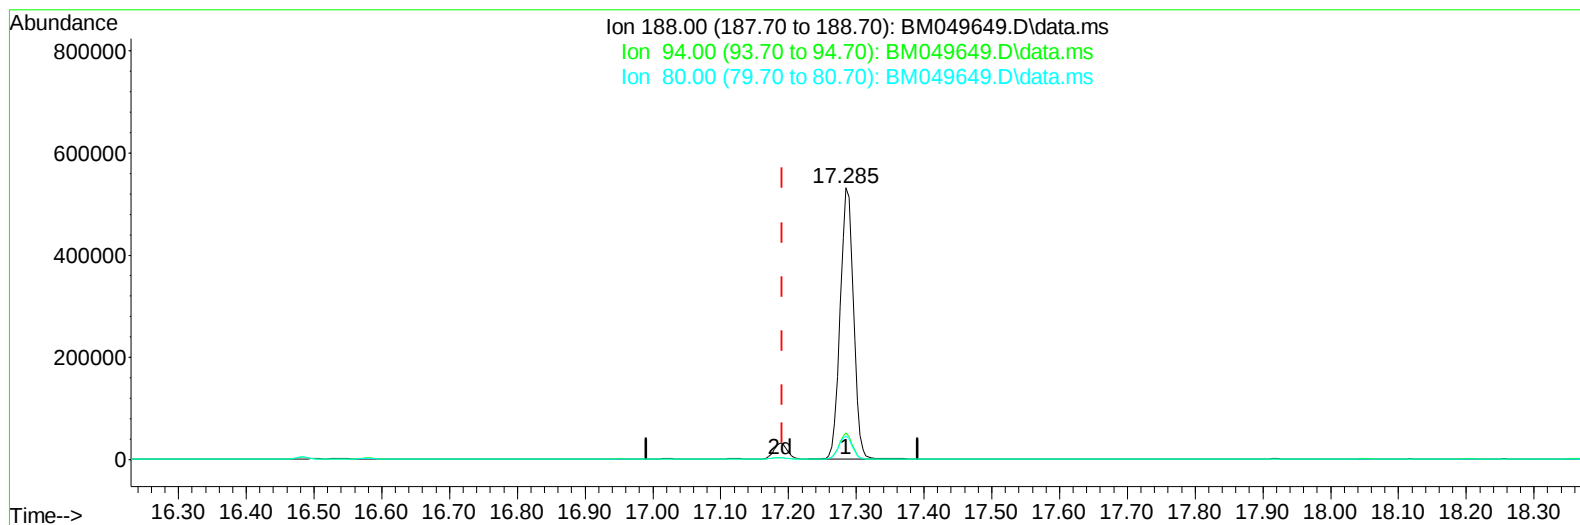

TIC: BM049649.D\data.ms

(13) Phenanthrene-d10 (I)

17.285min (+ 0.094) 0.40 ng/u1

response 725037

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.50	9.71
80.00	9.30	8.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

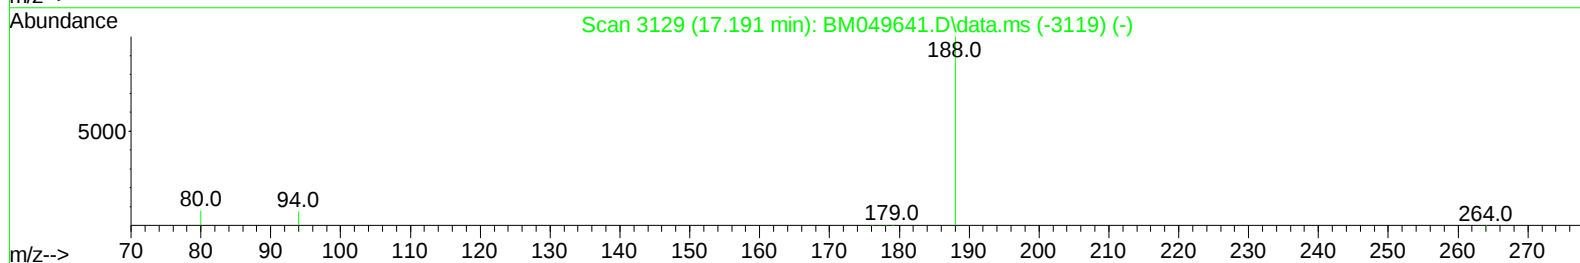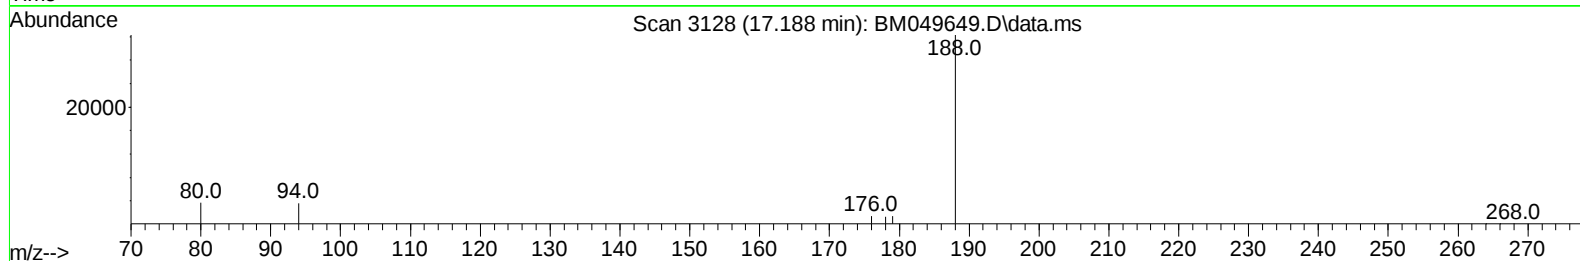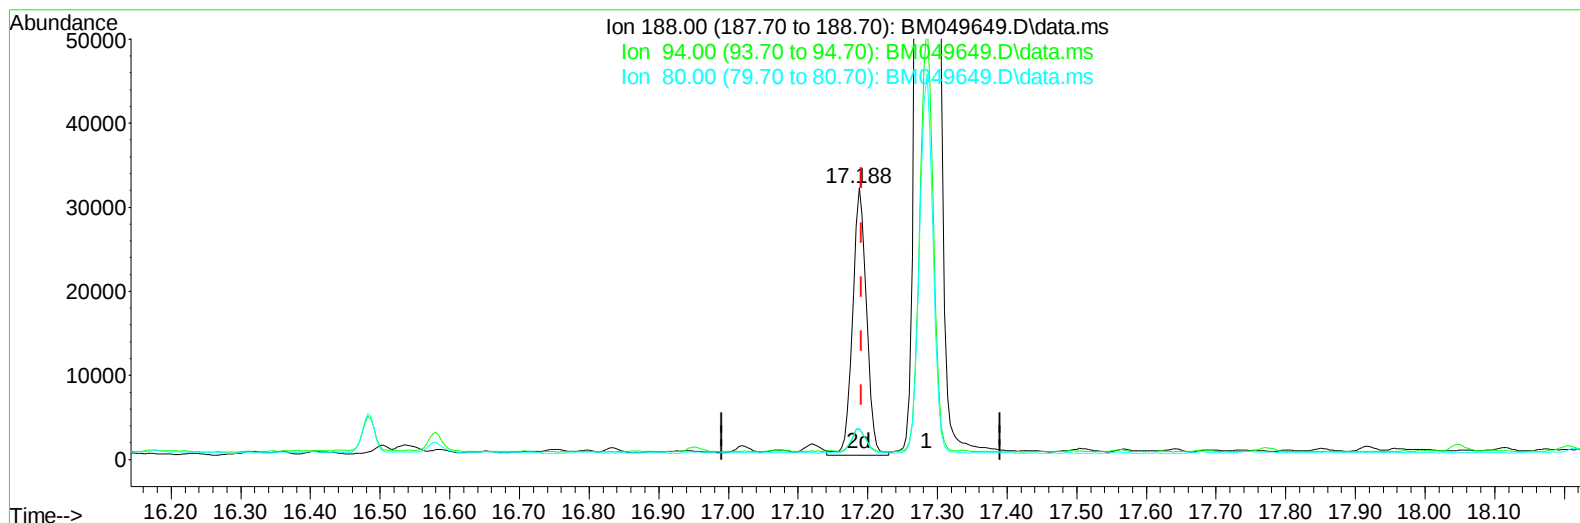

TIC: BM049649.D\data.ms

(13) Phenanthrene-d10 (I)

17.188min (-0.003) 0.40 ng/u1 m

response 44114

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.50	11.24#
80.00	9.30	11.40#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

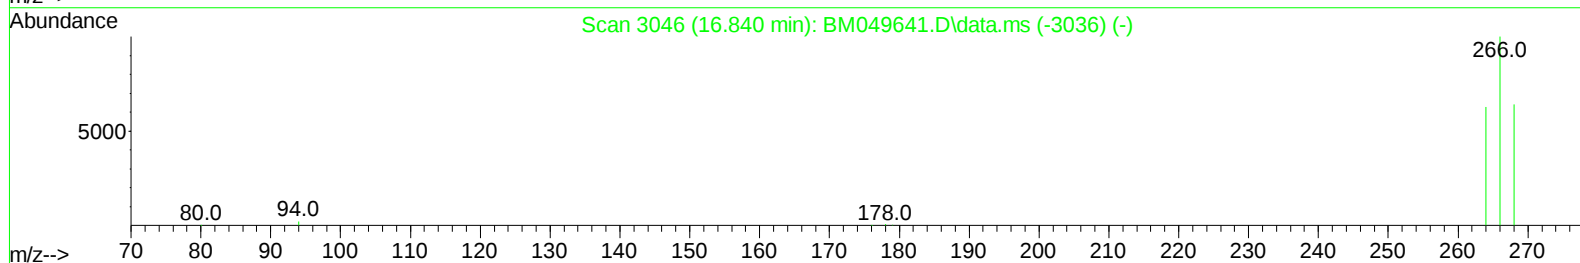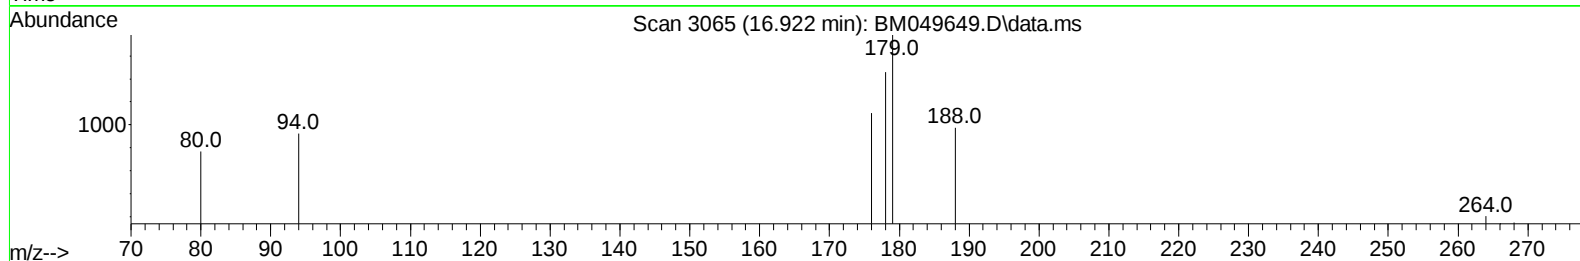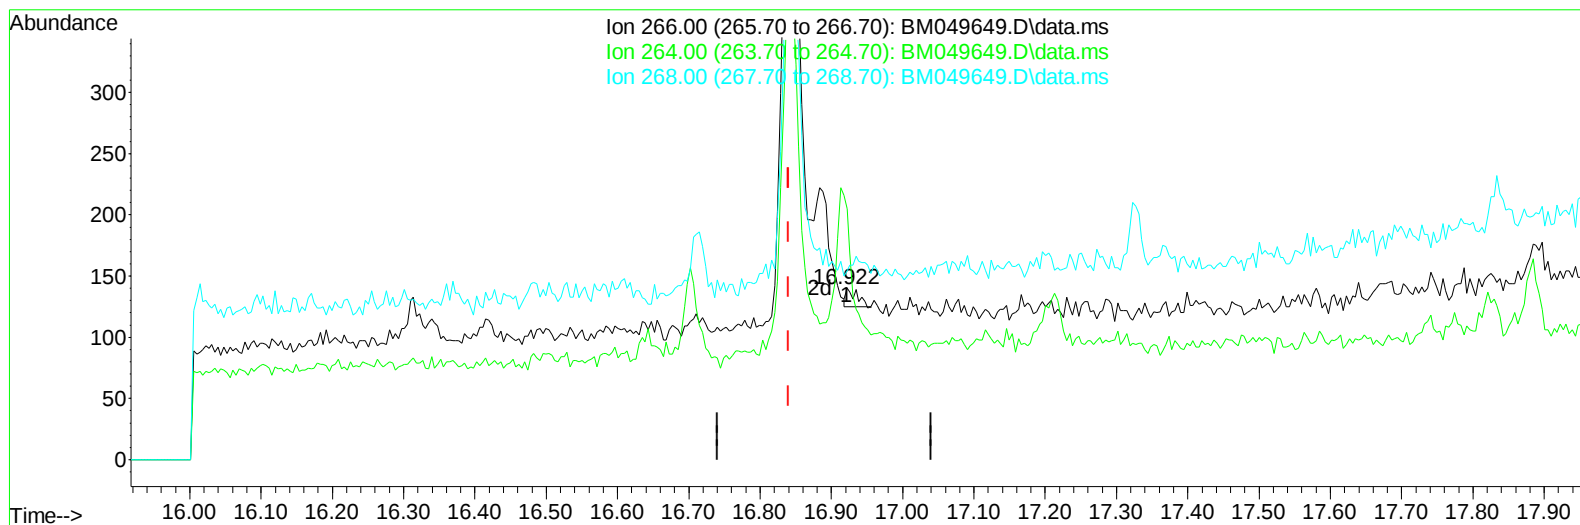

TIC: BM049649.D\data.ms

(14) Pentachlorophenol

16.922min (+ 0.081) 0.00 ng/u1

response 16

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.90	1456.25#
268.00	61.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

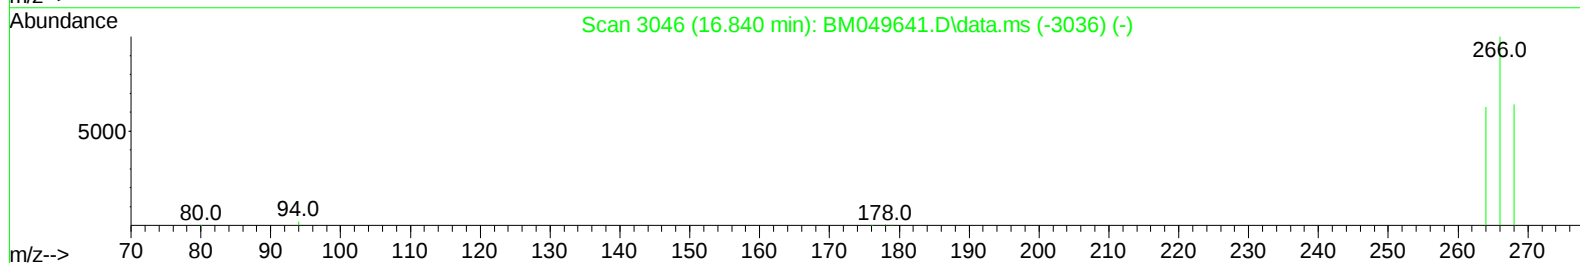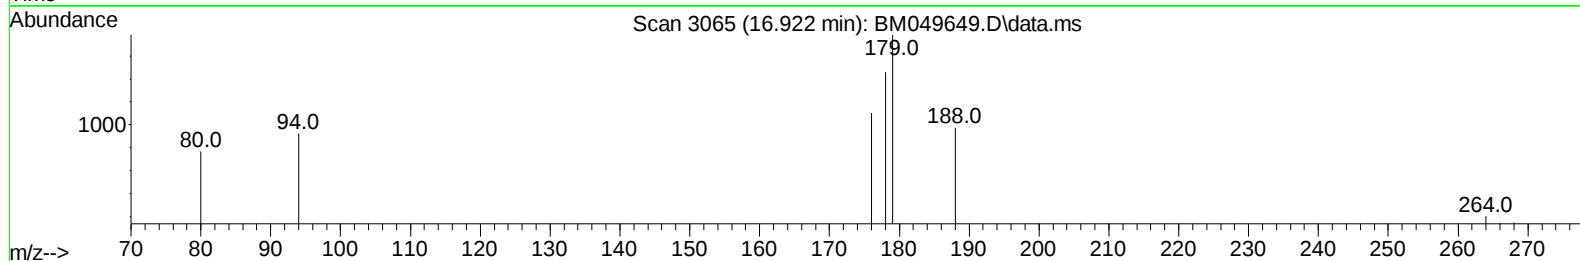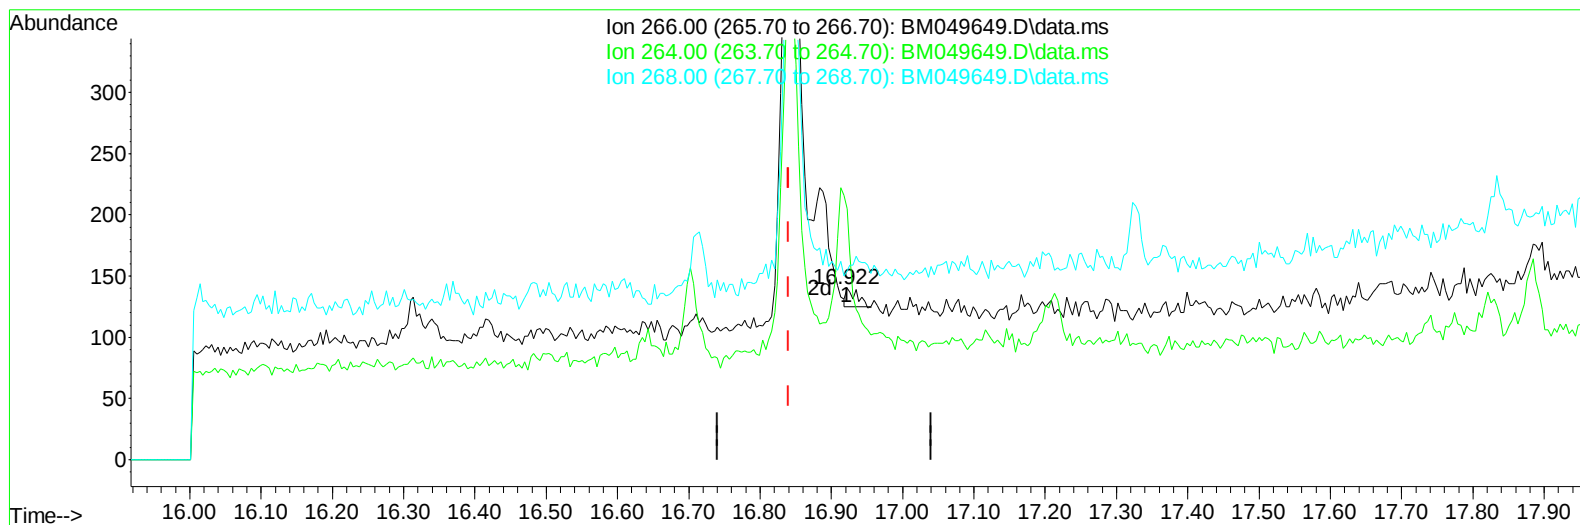

TIC: BM049649.D\data.ms

(14) Pentachlorophenol

16.922min (+ 0.081) 0.00 ng/u1

response 16

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.90	1456.25#
268.00	61.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

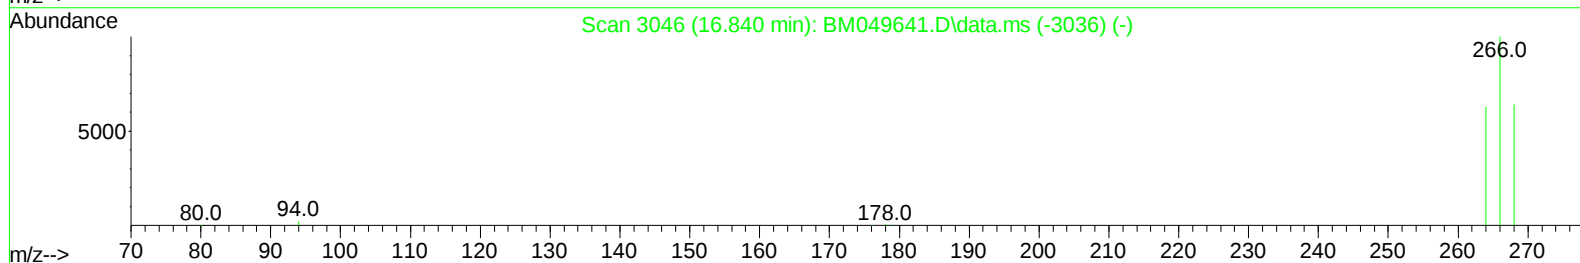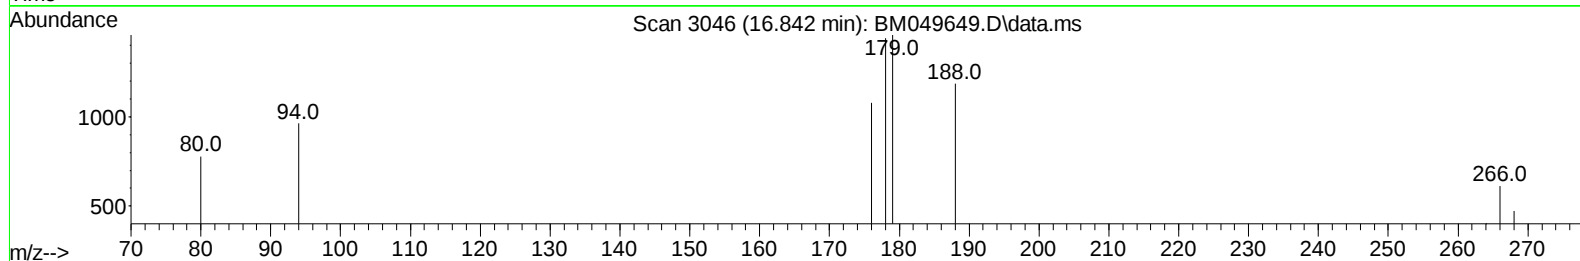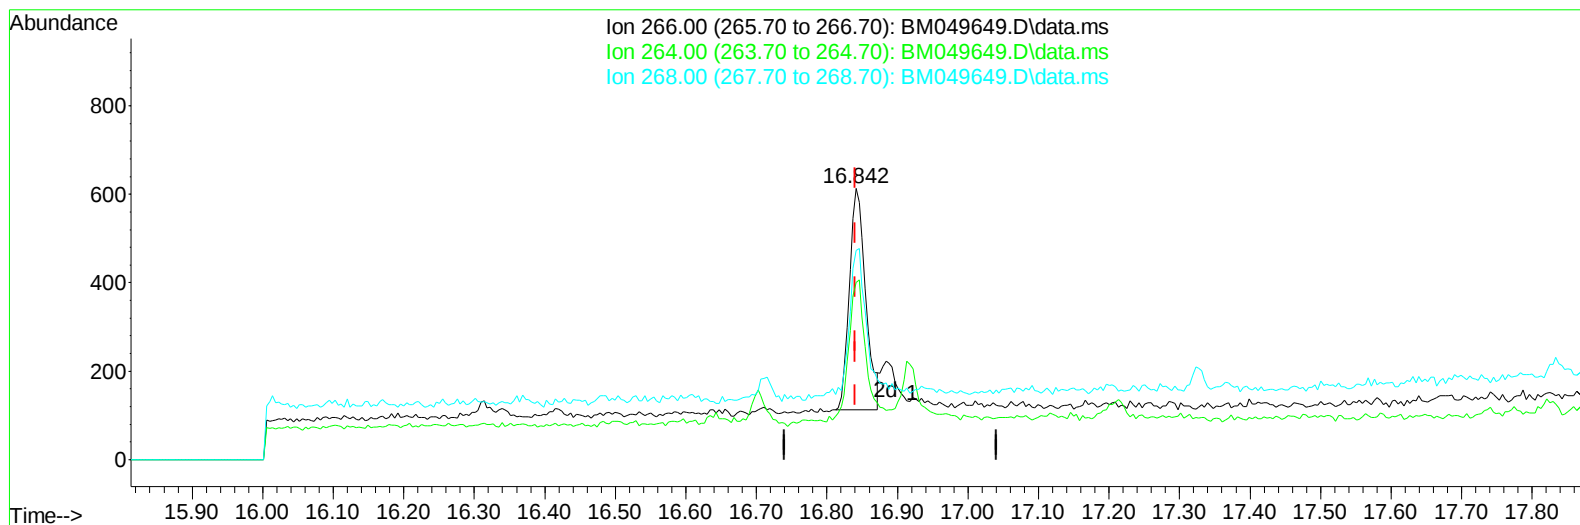

TIC: BM049649.D\data.ms

(14) Pentachloropheno1

16.842min (+ 0.001) 0.09 ng/ul m

response 800

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.90	29.13#
268.00	61.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

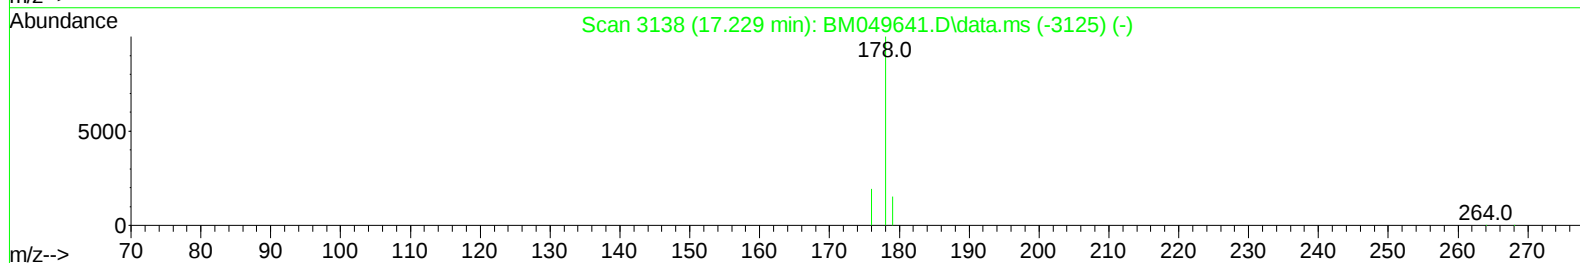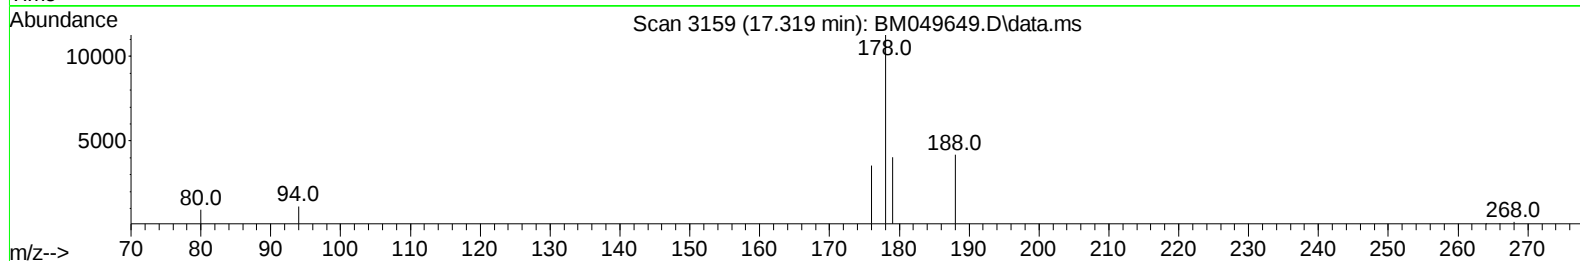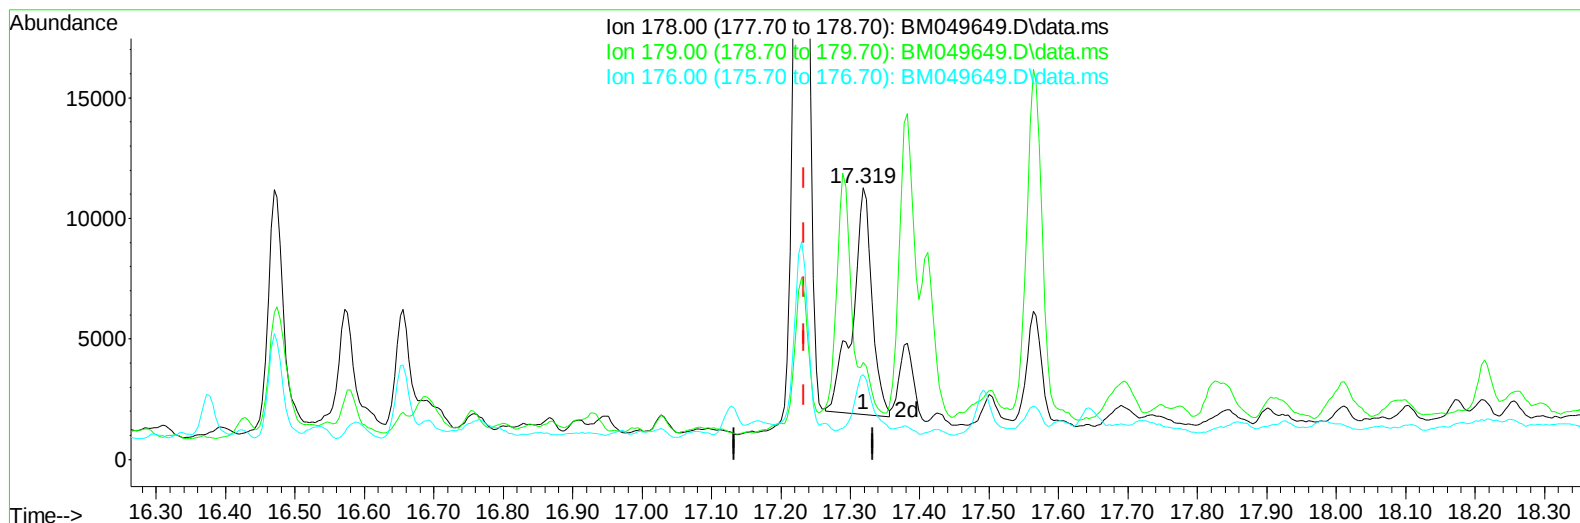

TIC: BM049649.D\data.ms

(15) Phenanthrene

17.319min (+ 0.086) 0.16 ng/u1

response 18441

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.80	35.78#
176.00	20.20	31.35#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

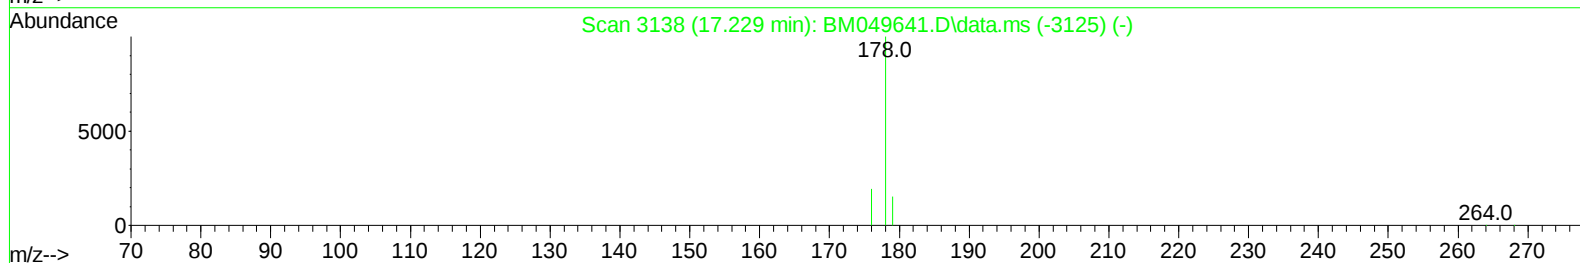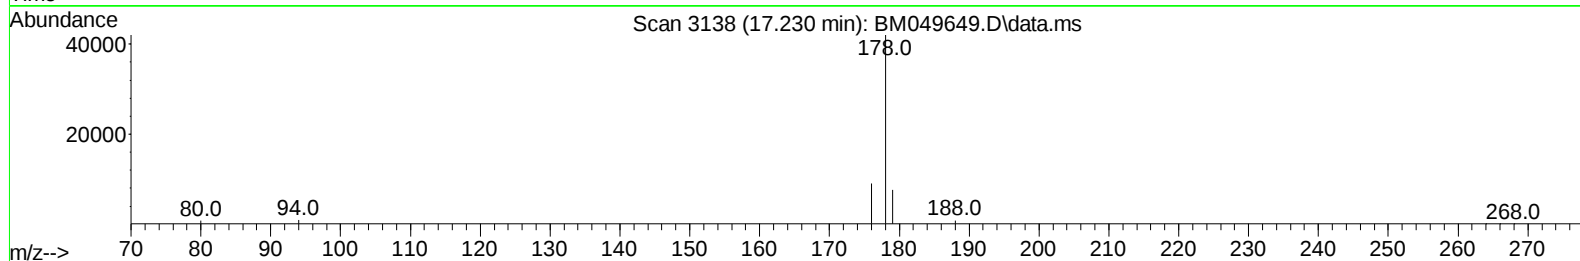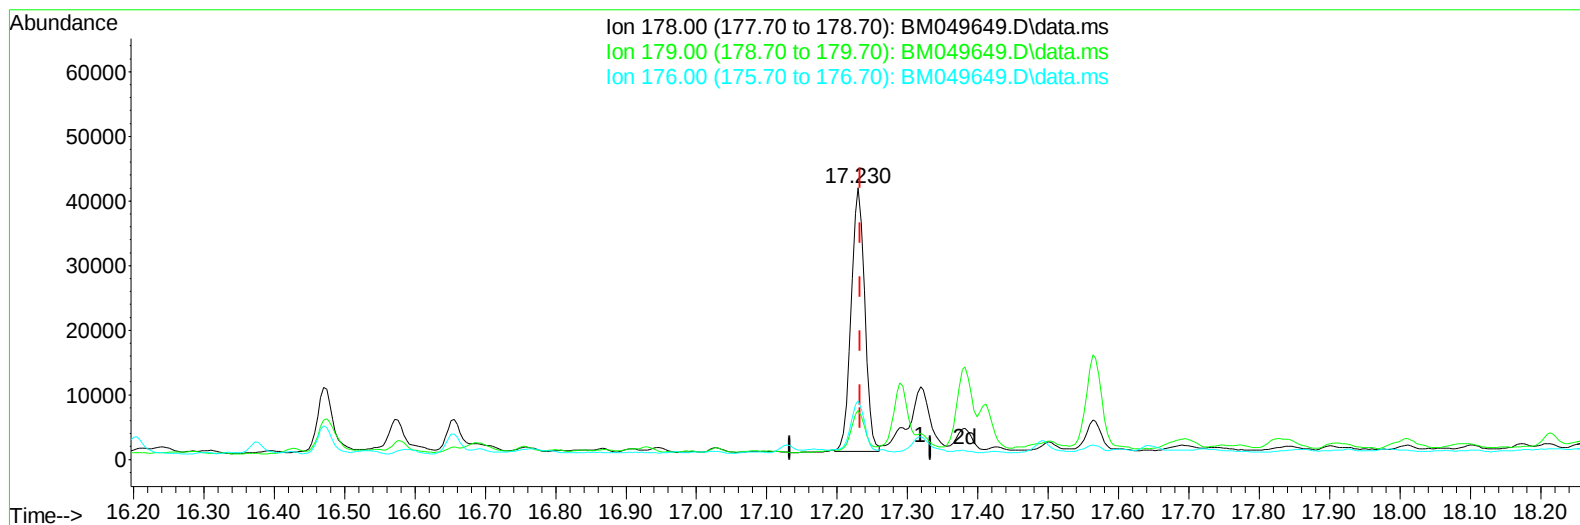

TIC: BM049649.D\data.ms

(15) Phenanthrene

17.230min (-0.003) 0.46 ng/ul m

response 54518

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.80	18.00
176.00	20.20	21.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

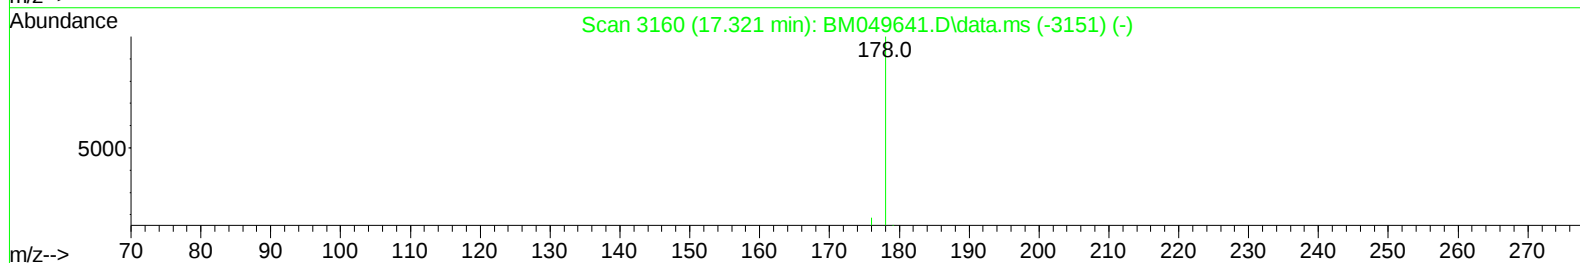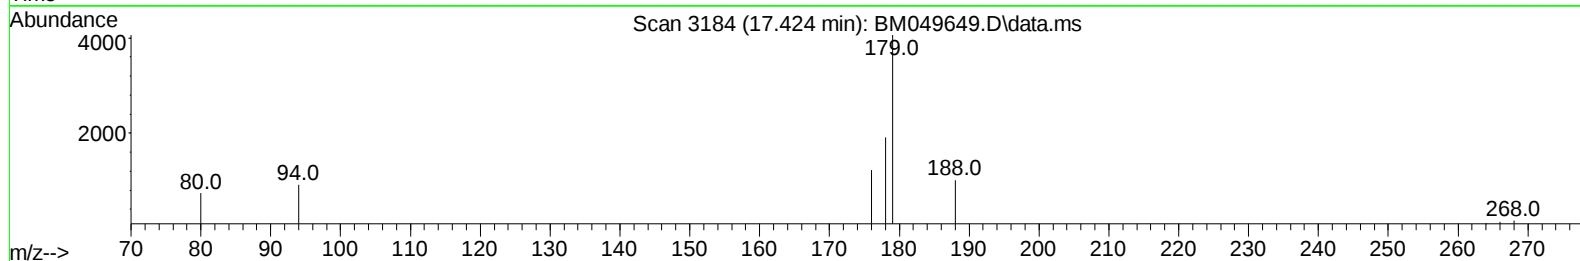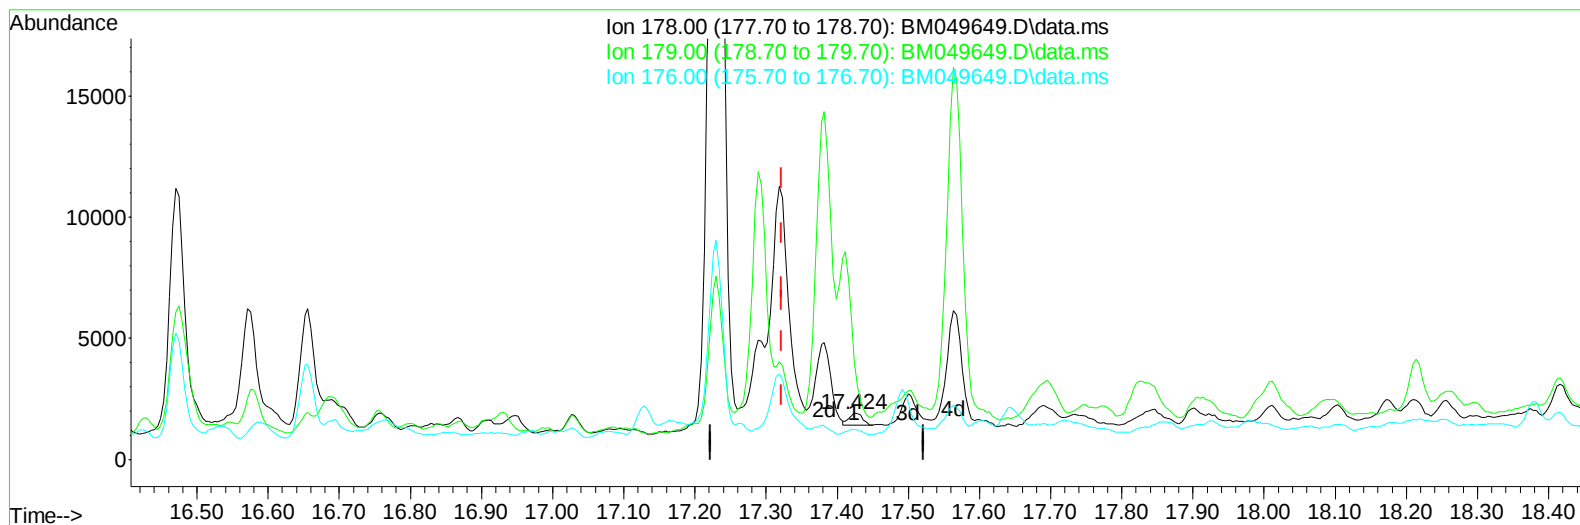

TIC: BM049649.D\data.ms

(16) Anthracene

17.424min (+ 0.103) 0.01 ng/u1

response 660

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.10	212.17#
176.00	19.70	64.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

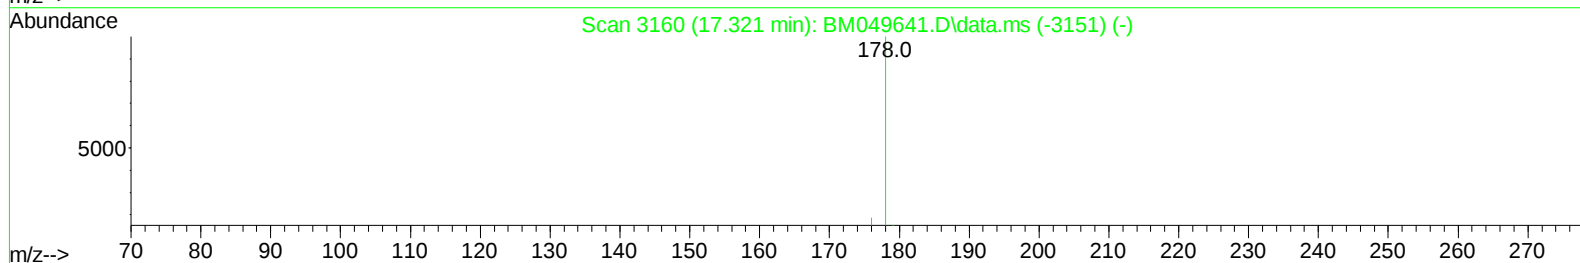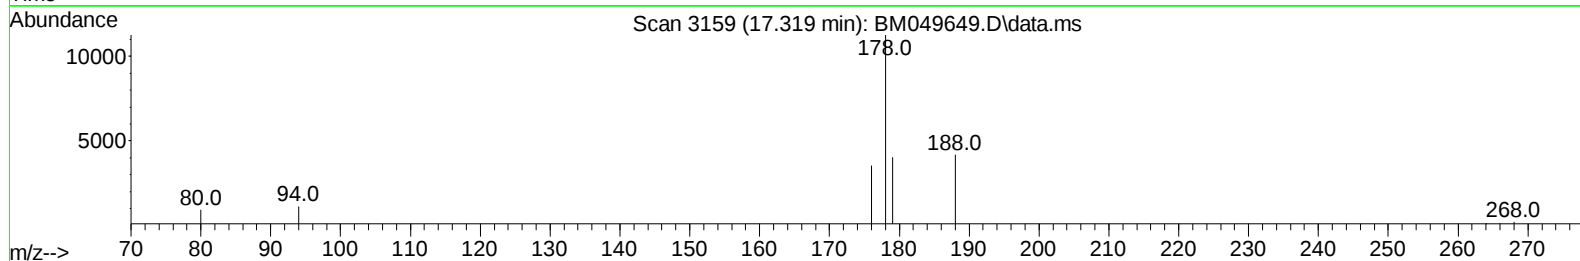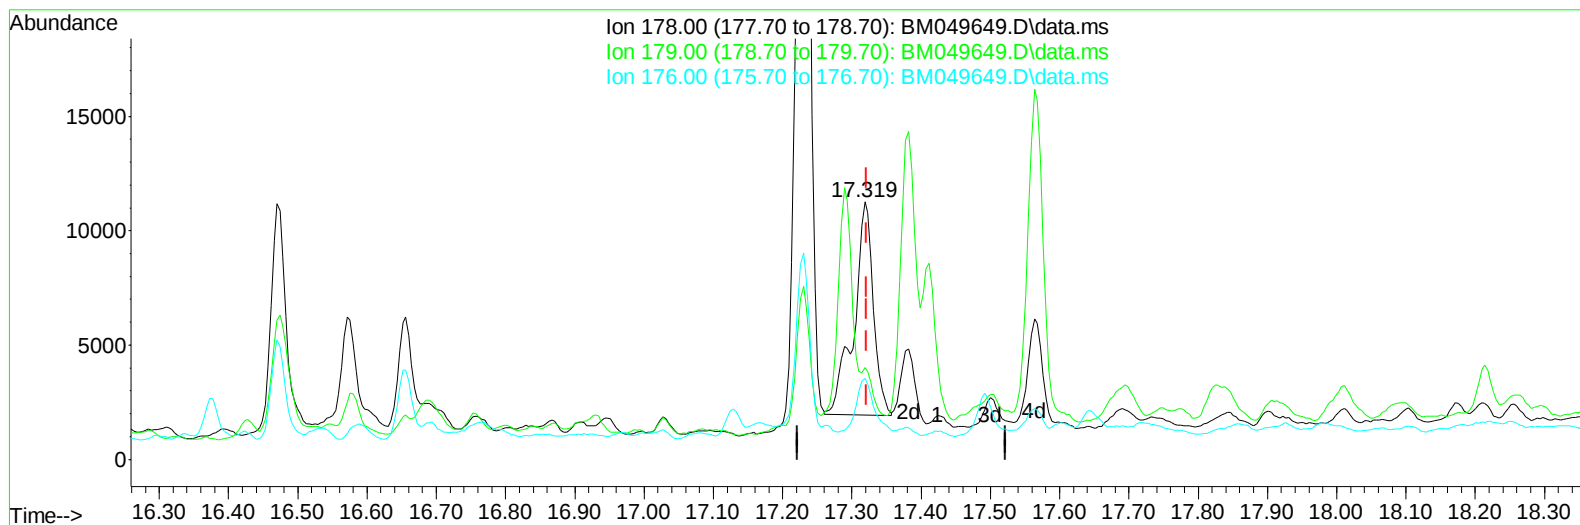

TIC: BM049649.D\data.ms

(16) Anthracene

17.319min (-0.003) 0.17 ng/ul m

response 18165

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.10	35.78#
176.00	19.70	31.35#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

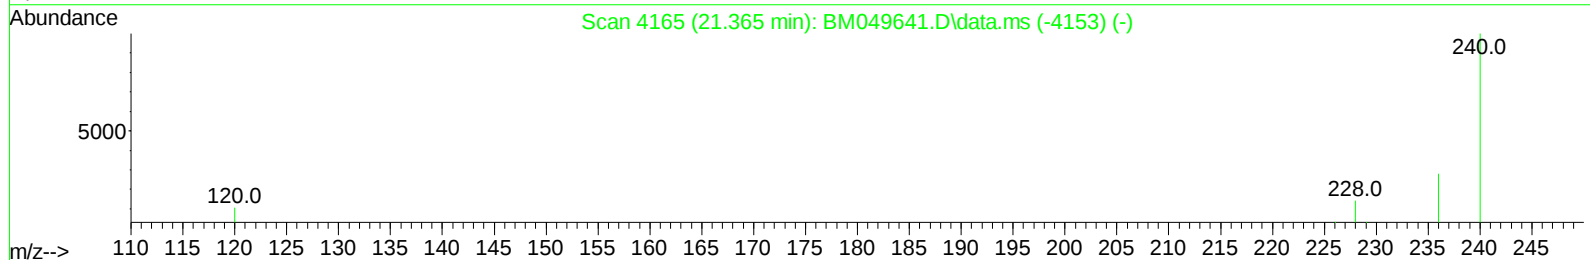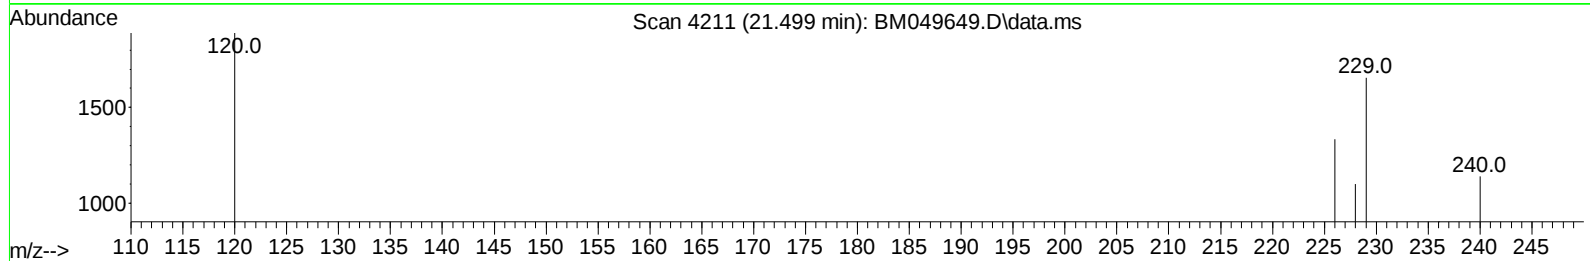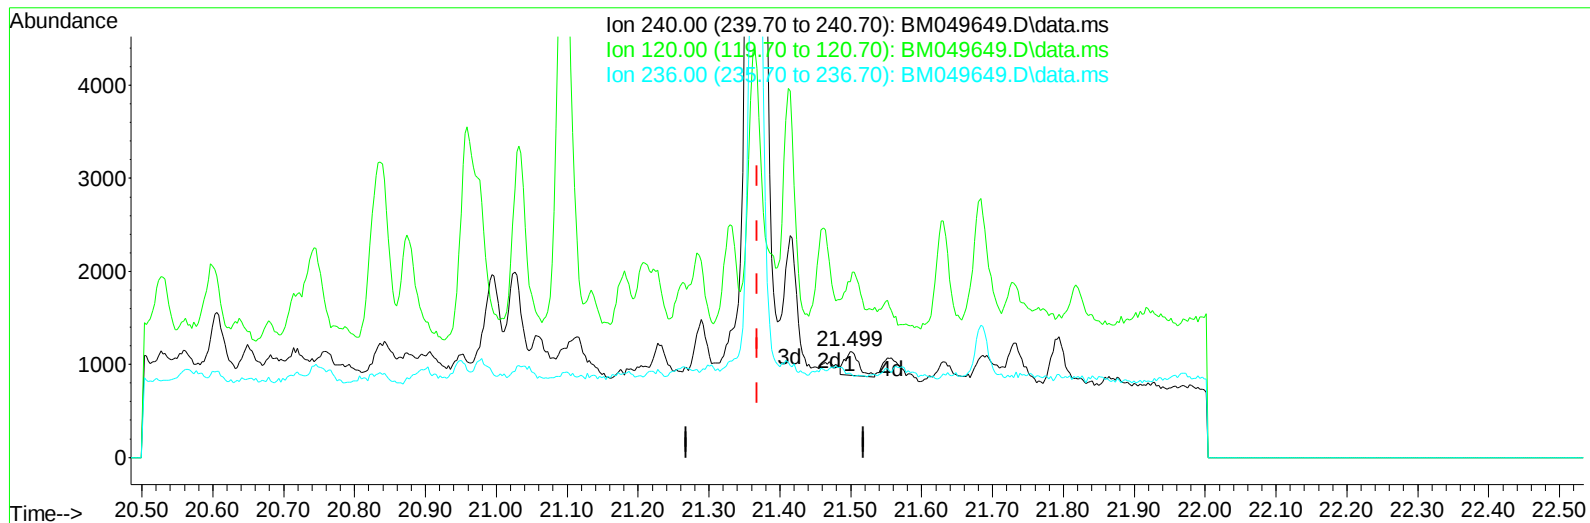

TIC: BM049649.D\data.ms

(17) Chrysene-d12

21.499min (+ 0.131) 0.40 ng/u1

response 354

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	12.90	165.85#
236.00	29.30	79.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

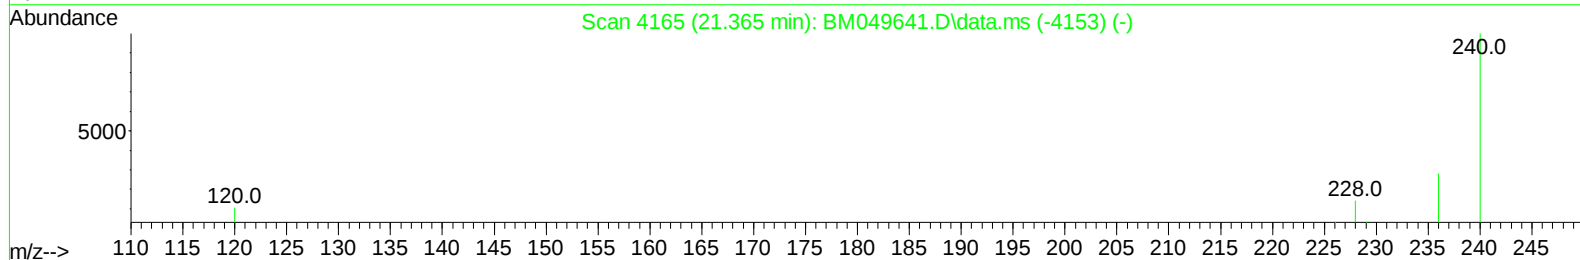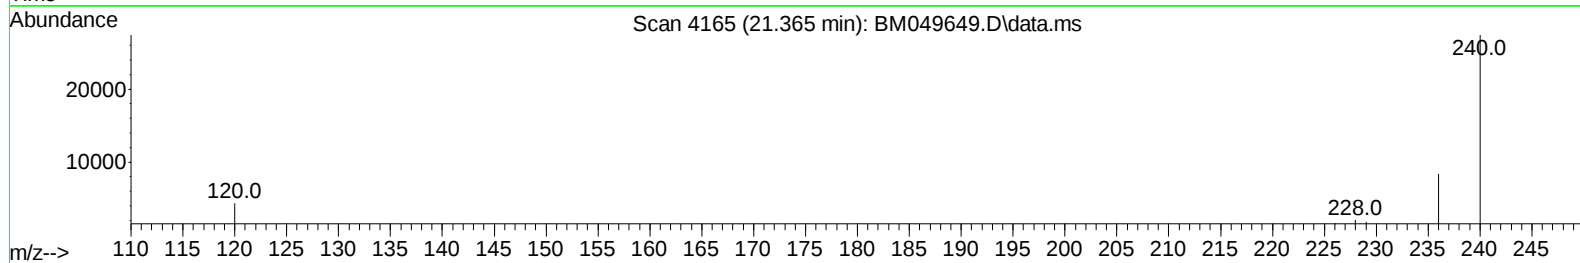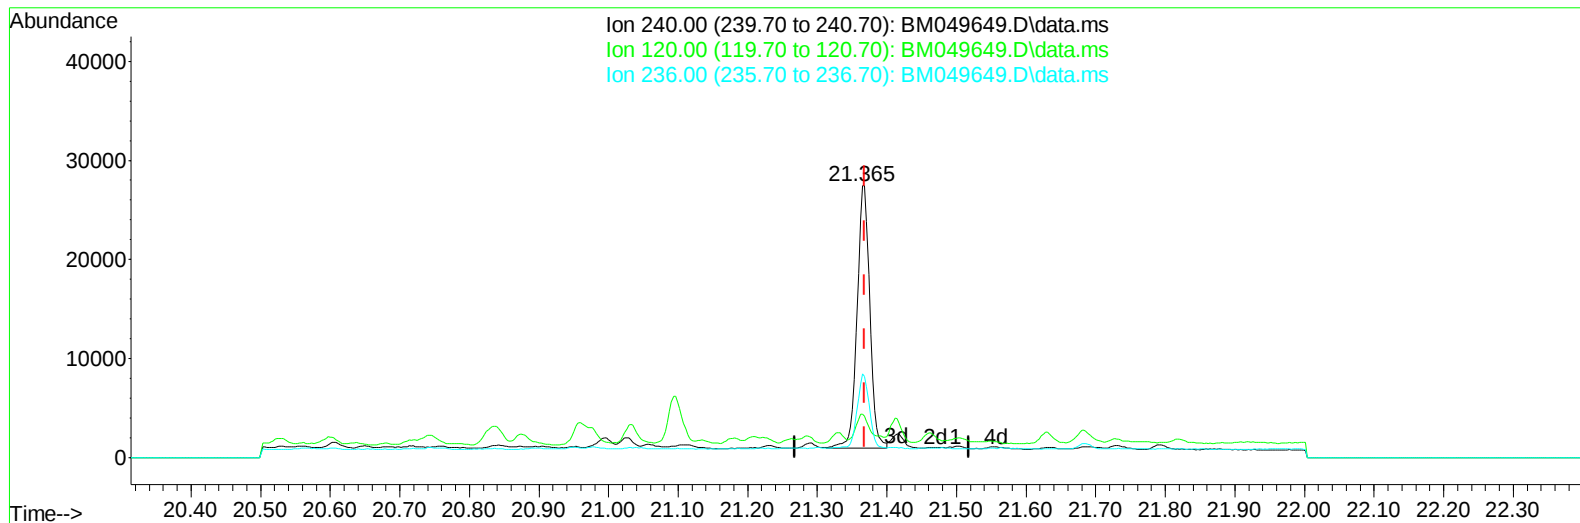

TIC: BM049649.D\data.ms

(17) Chrysene-d12

21.365min (-0.003) 0.40 ng/ul m

response 33412

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	12.90	15.95#
236.00	29.30	30.68
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

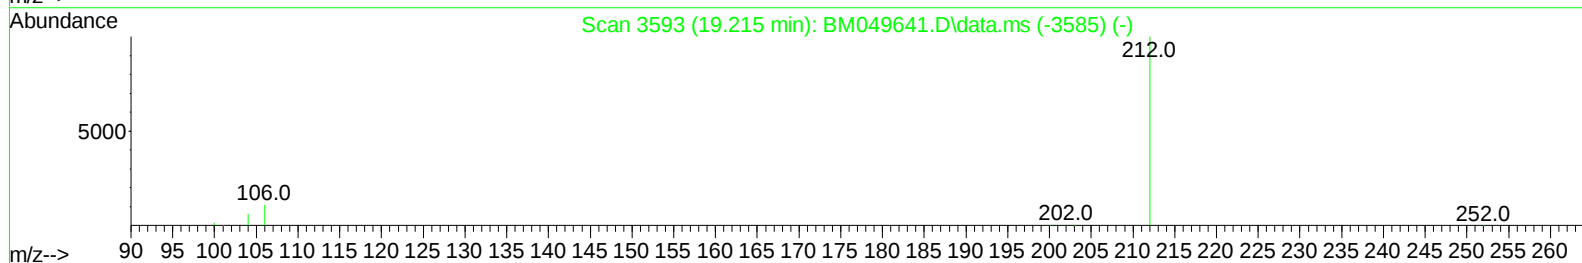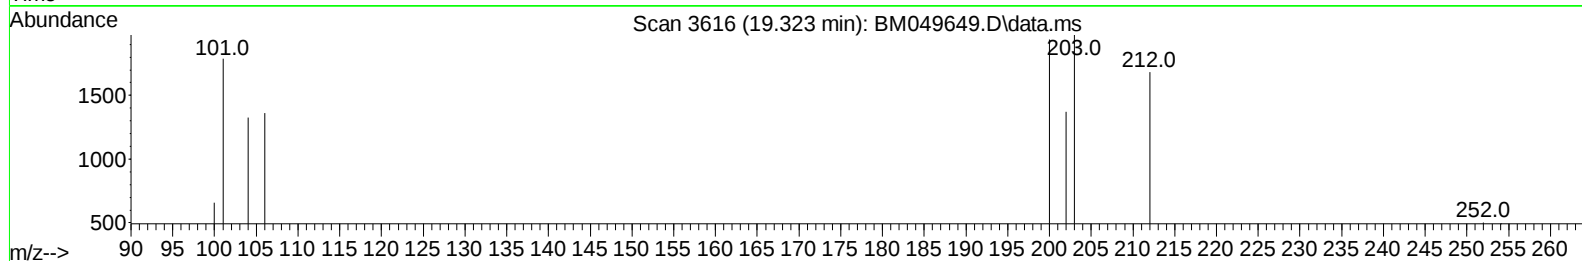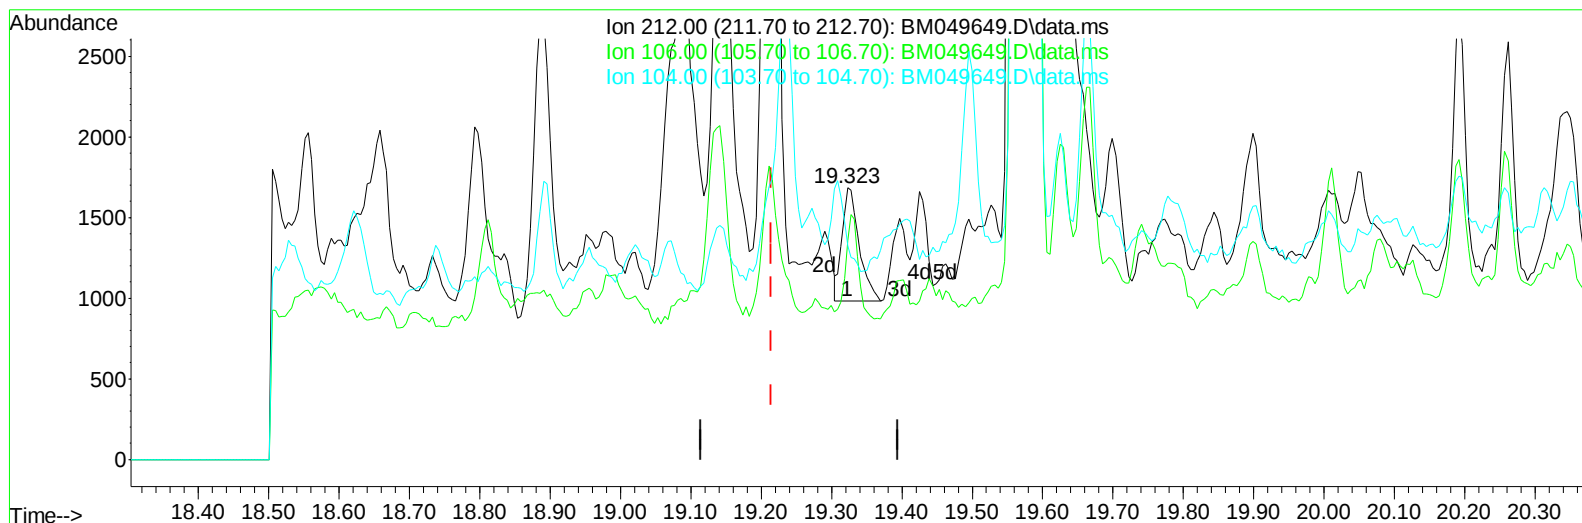

TIC: BM049649.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.323min (+ 0.108) 0.01 ng/u1

response 1175

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	11.30	69.11#
104.00	9.20	65.53#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

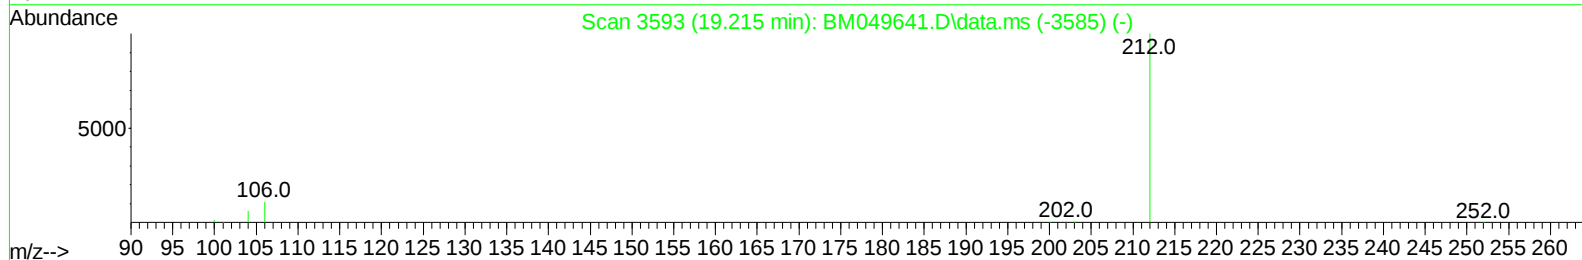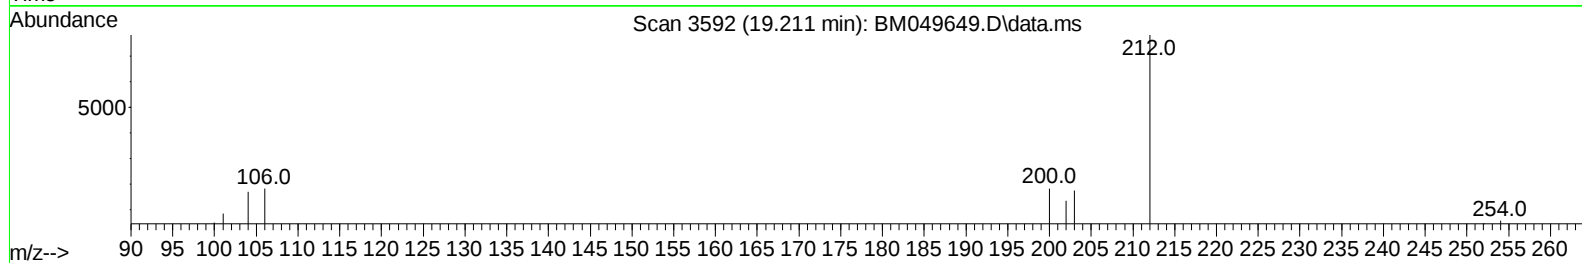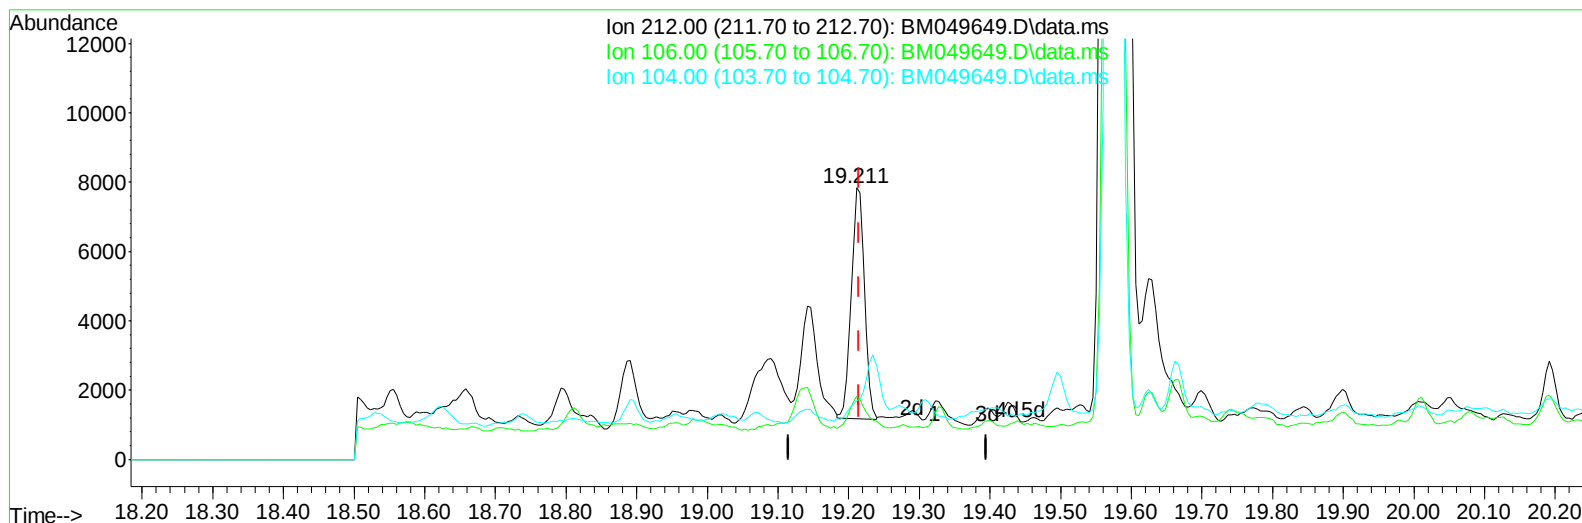

TIC: BM049649.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.211min (-0.003) 0.08 ng/ul m

response 8642

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	11.30	9.40
104.00	9.20	8.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

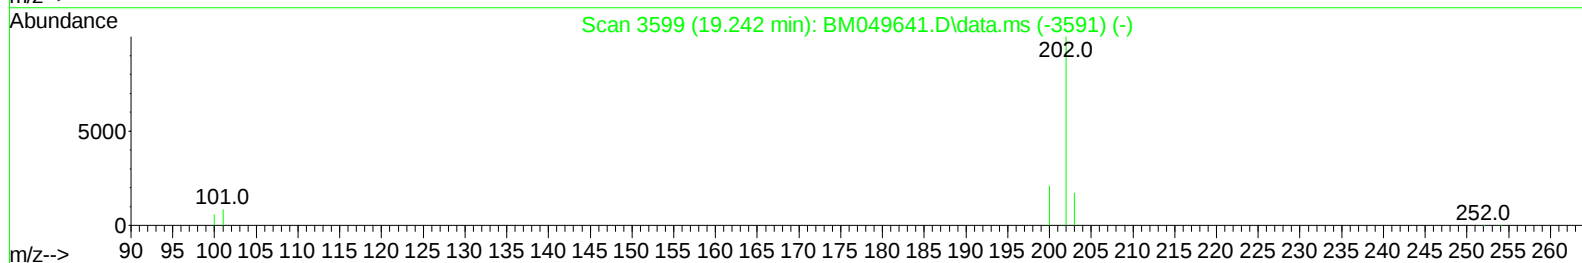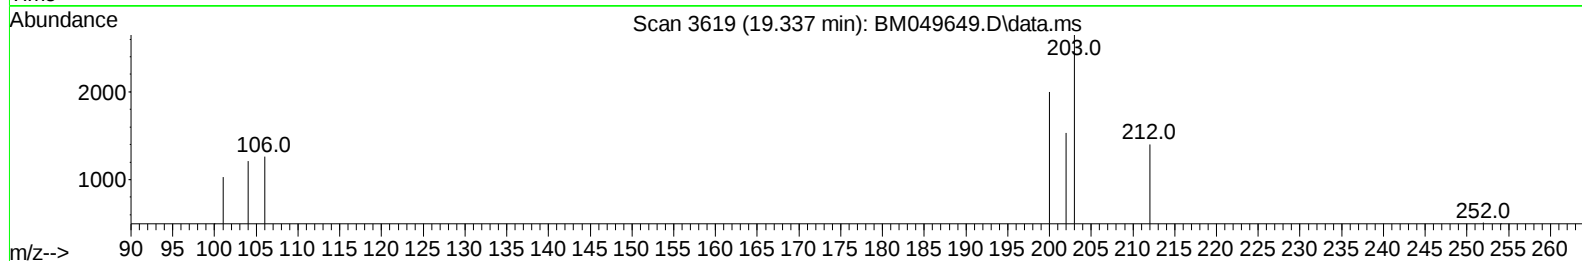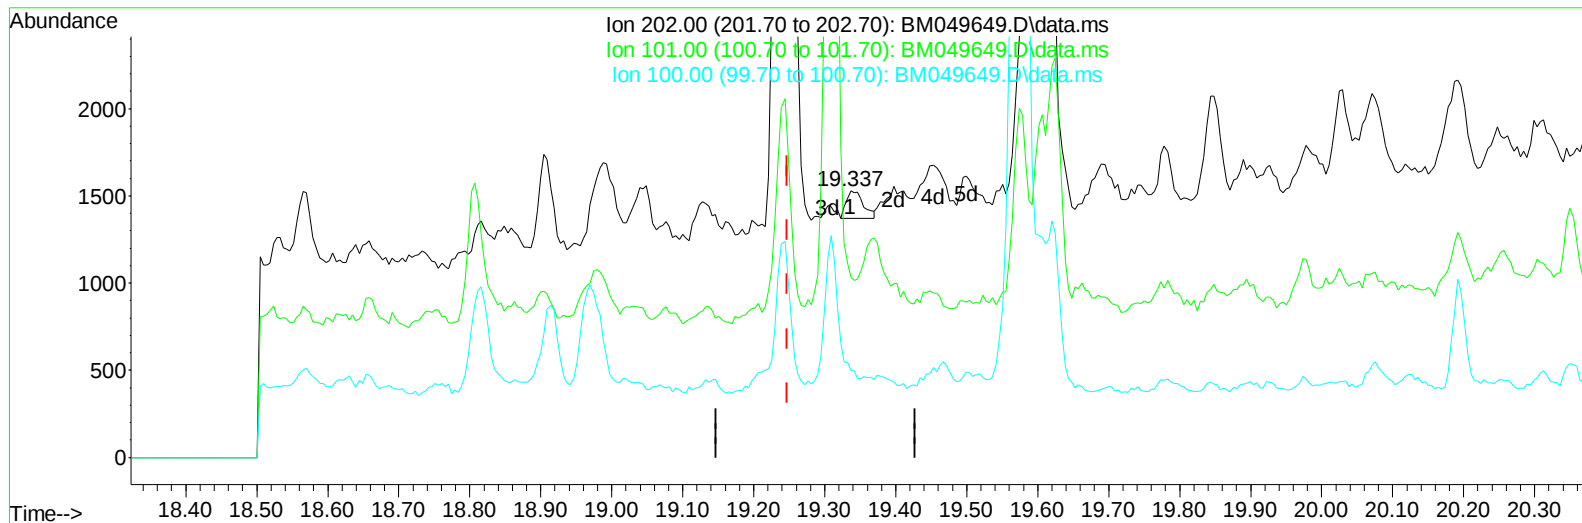

TIC: BM049649.D\data.ms

(19) Fluoranthene (C)

19.337min (+ 0.090) 0.00 ng/u1

response 271

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	8.40	67.50#
100.00	6.20	32.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

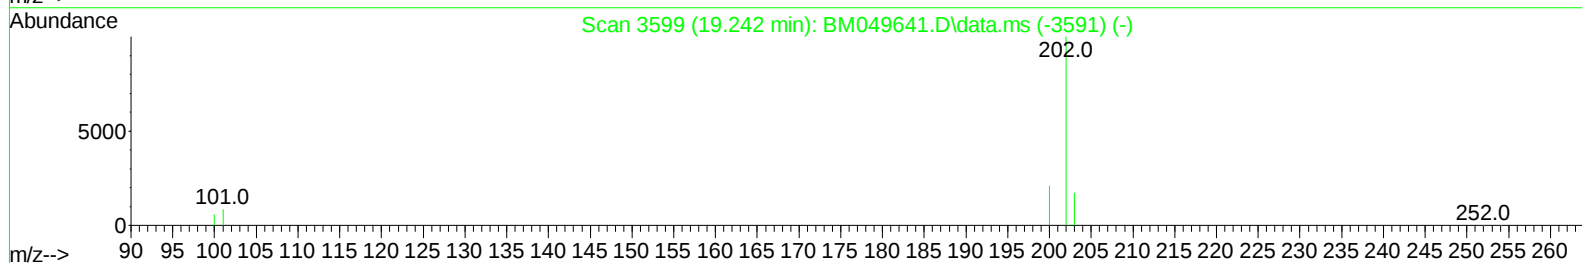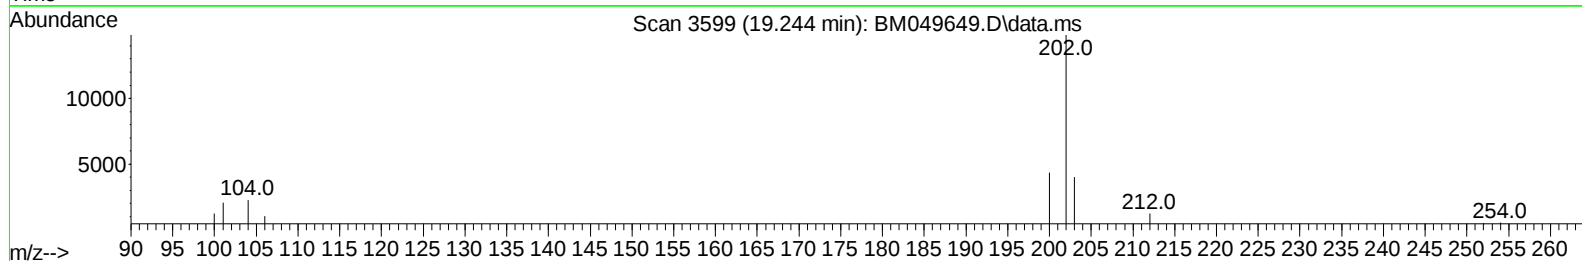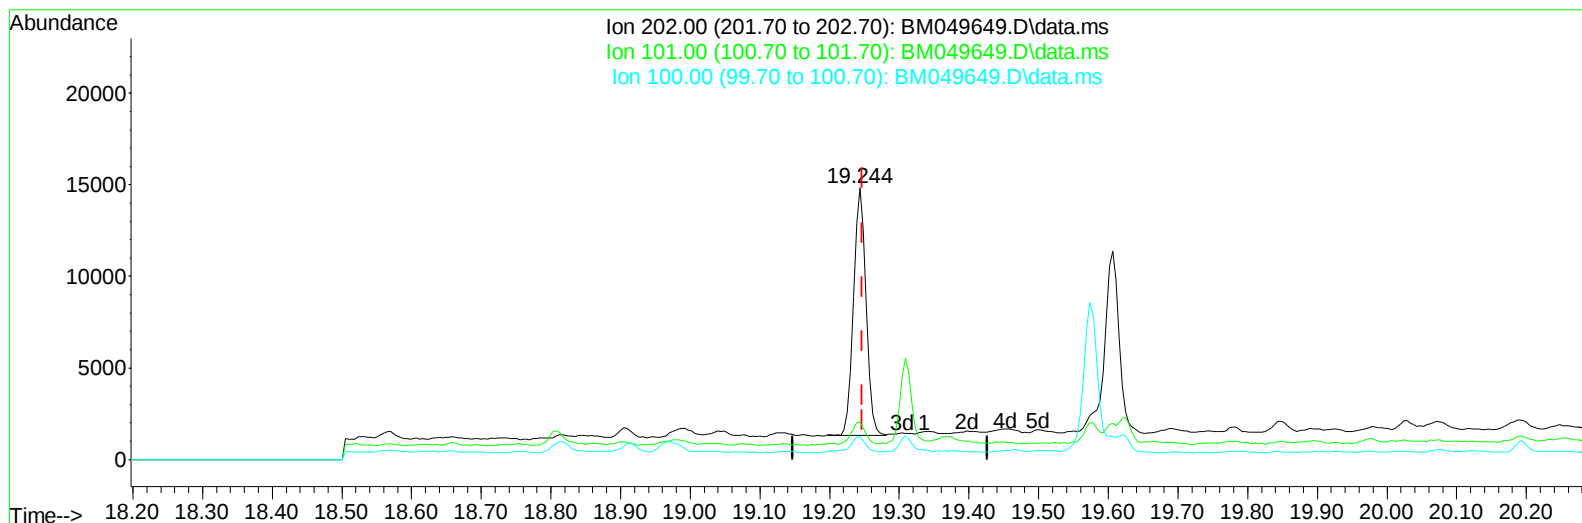

TIC: BM049649.D\data.ms

(19) Fluoranthene (C)

19.244min (-0.003) 0.12 ng/ul m

response 17070

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	8.40	13.87#
100.00	6.20	8.35#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

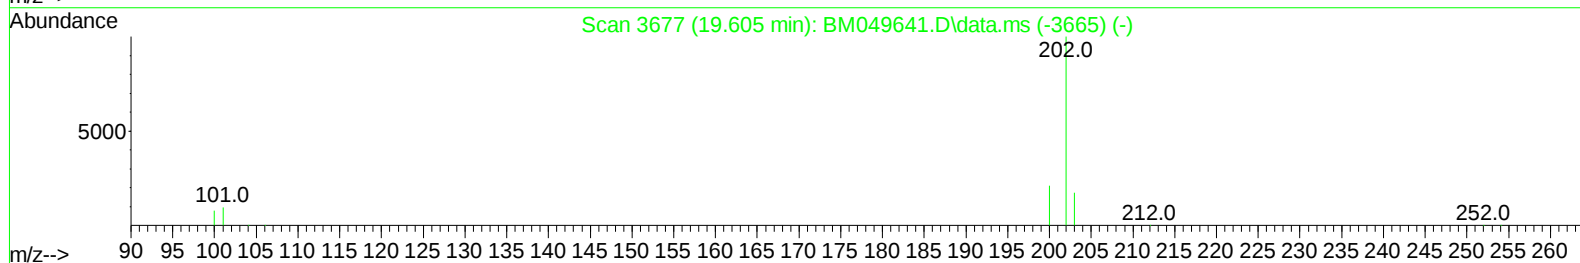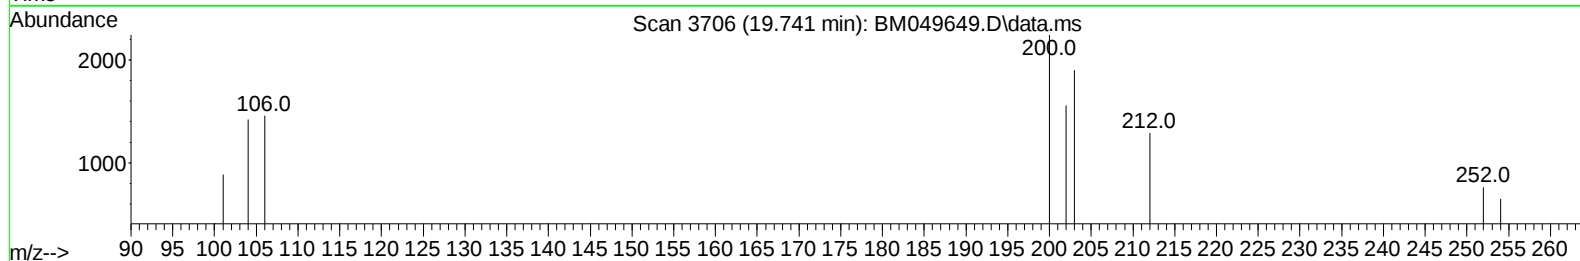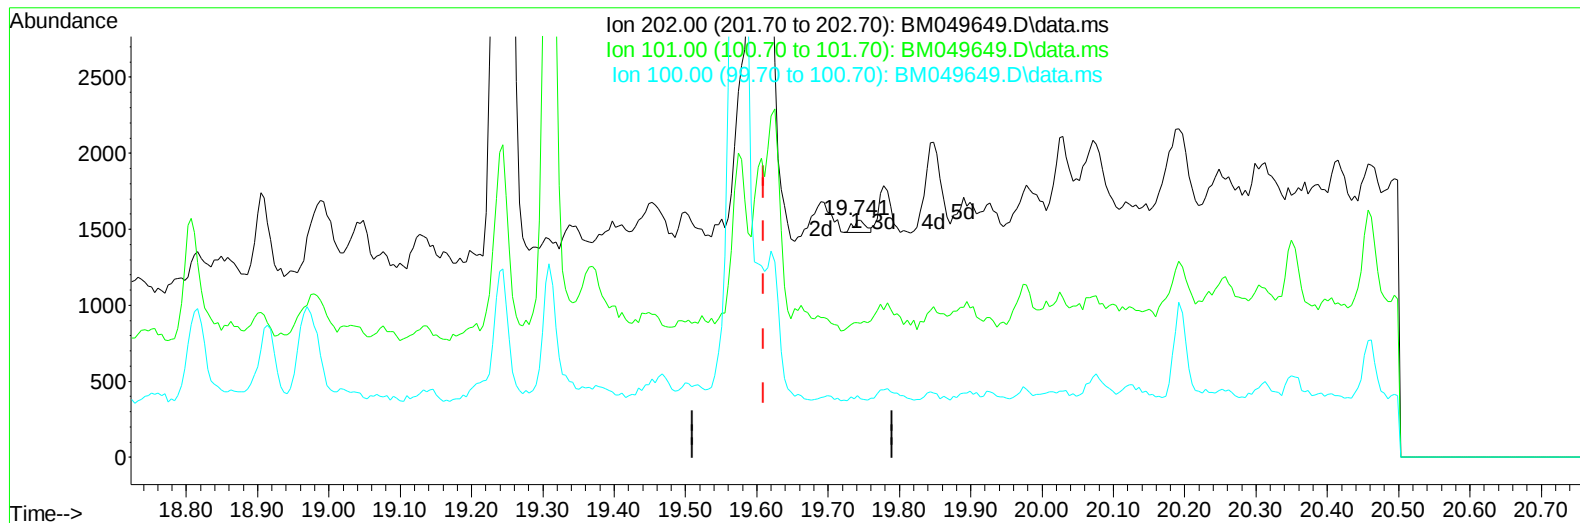

TIC: BM049649.D\data.ms

(20) Pyrene

19.741min (+ 0.131) 0.00 ng/u1

response 105

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	9.40	56.76#
100.00	7.90	26.07#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

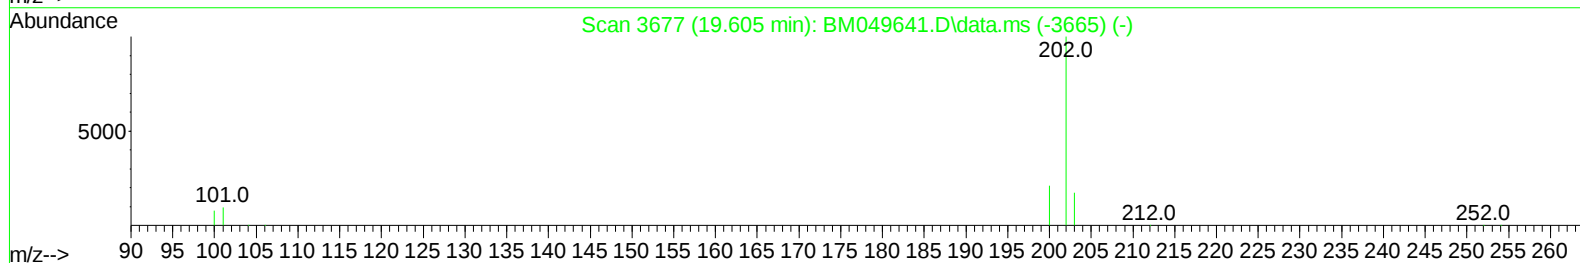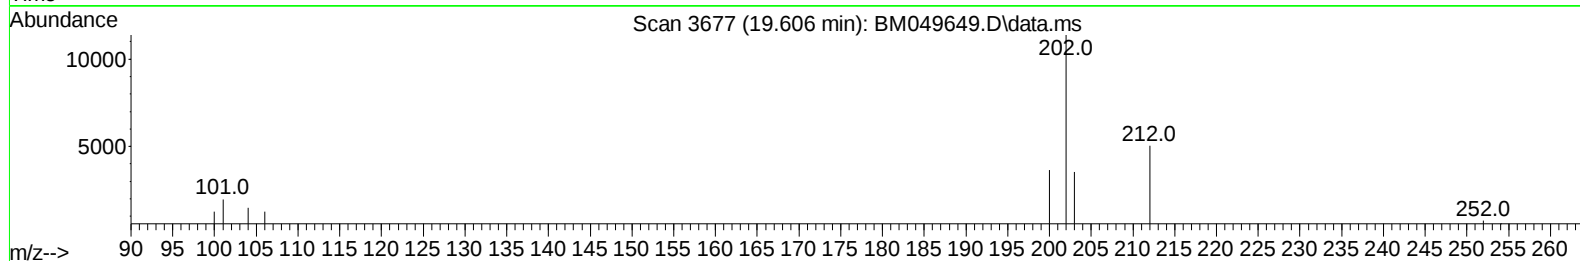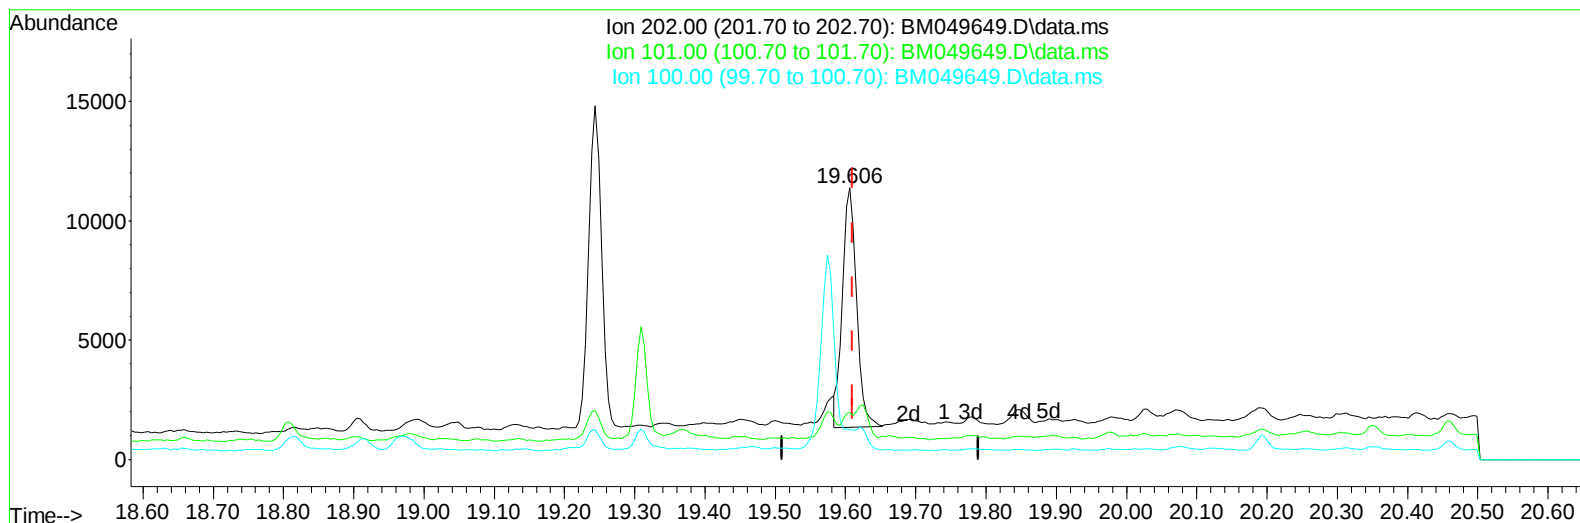

TIC: BM049649.D\data.ms

(20) Pyrene

19.606min (-0.003) 0.10 ng/ul m

response 13963

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	9.40	17.29#
100.00	7.90	11.07#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

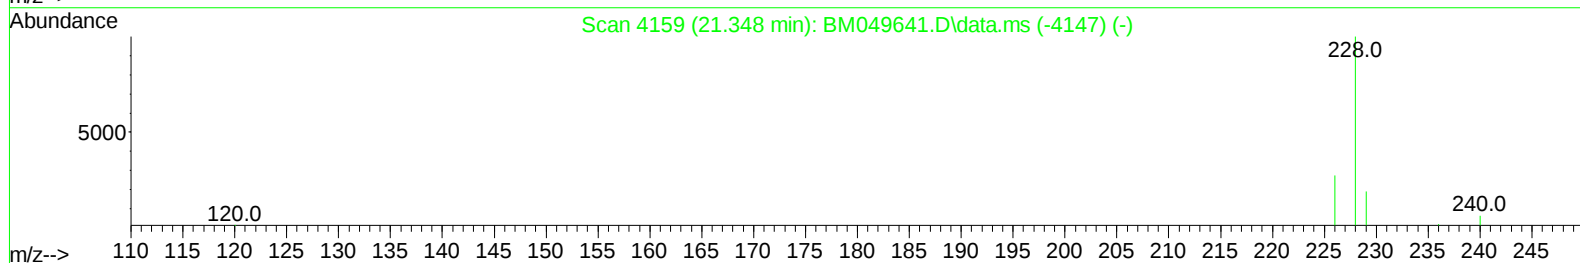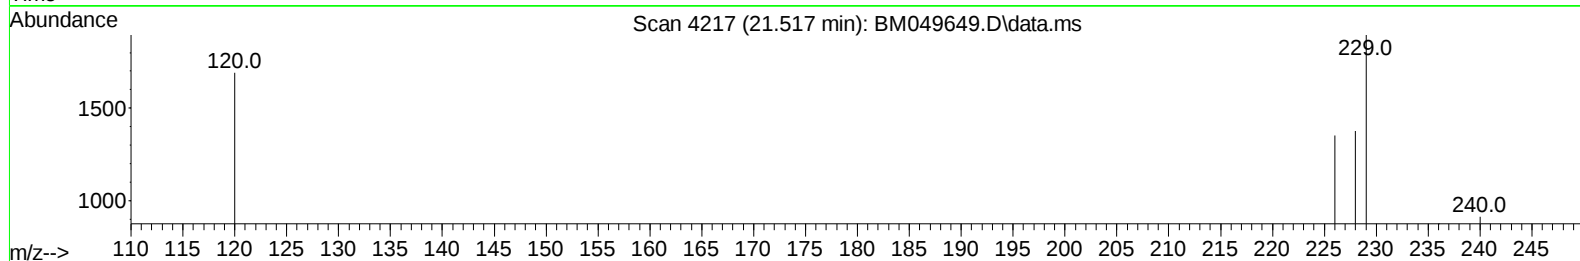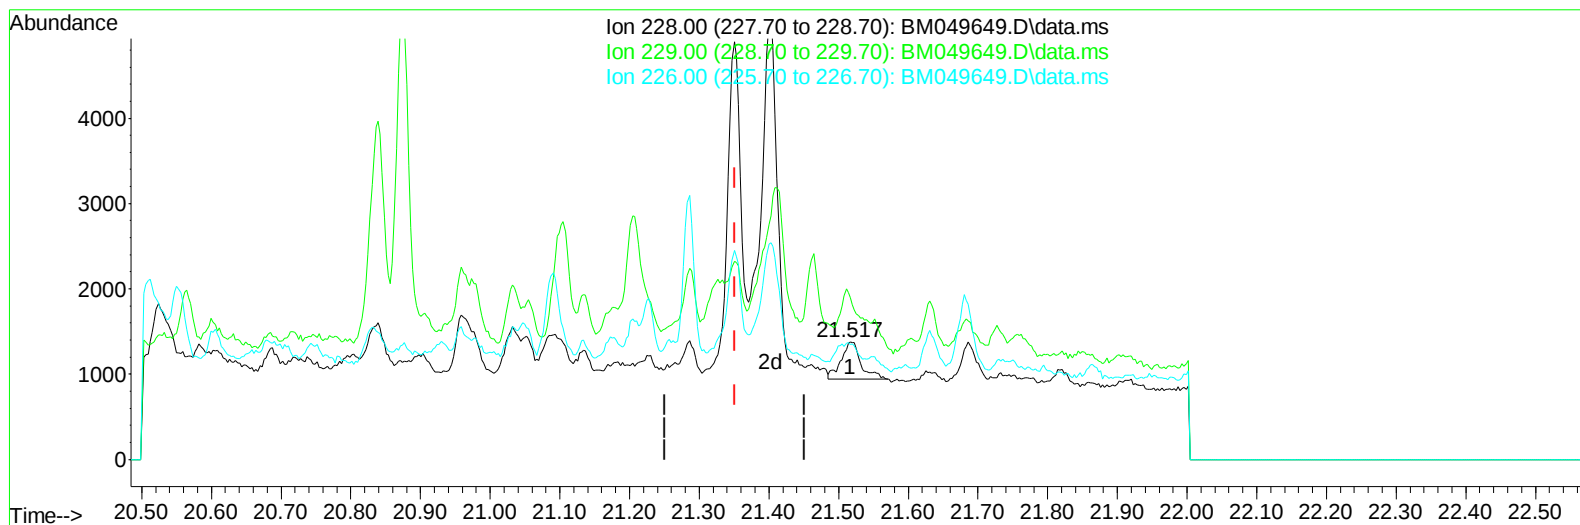

TIC: BM049649.D\data.ms

(21) Benzo(a)anthracene

21.517min (+ 0.166) 0.01 ng/u1

response 851

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.60	137.52#
226.00	27.80	98.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

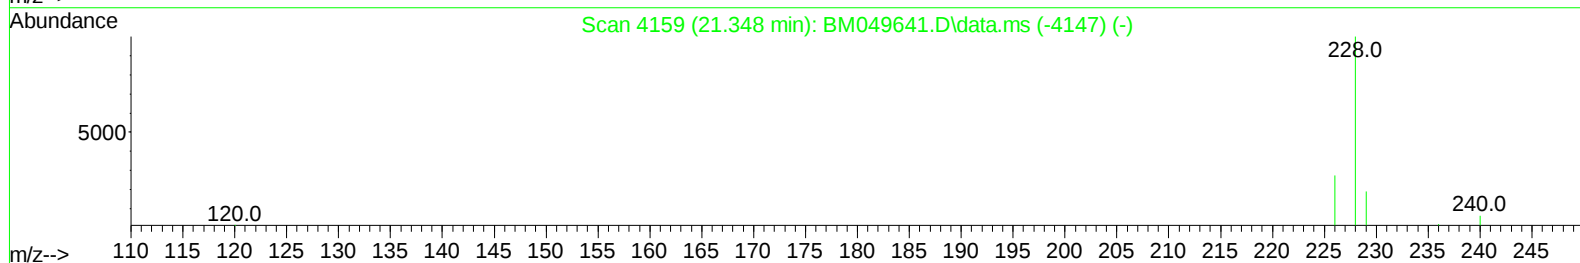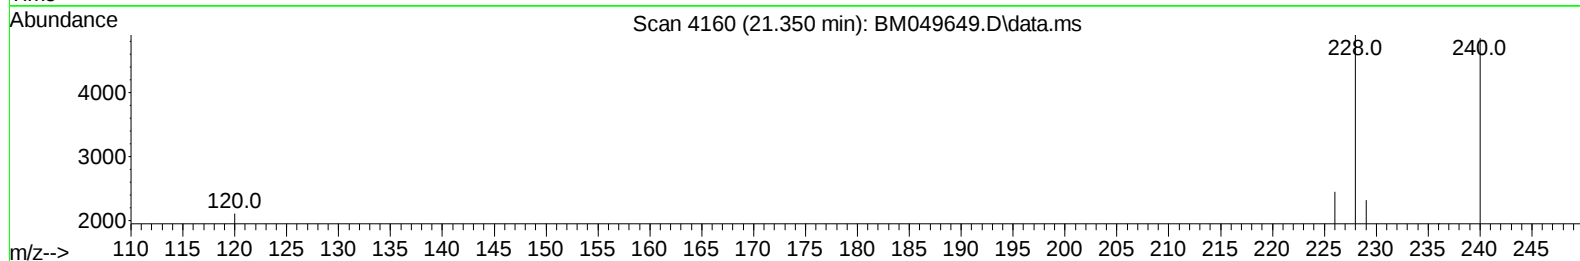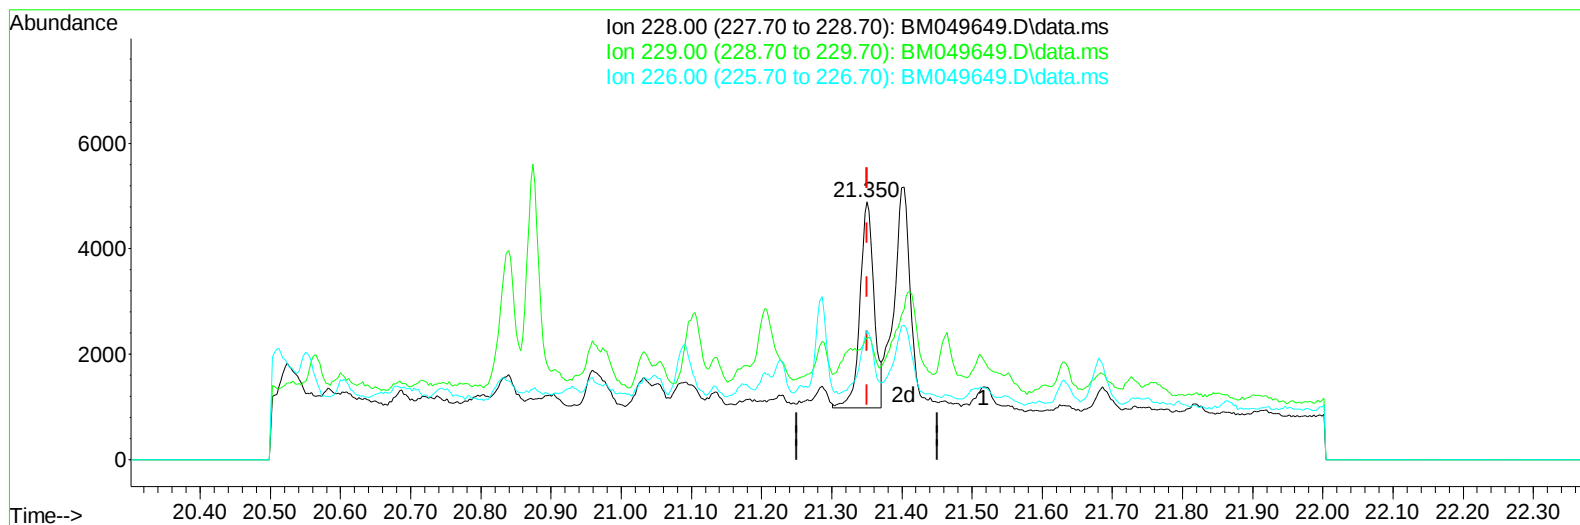

TIC: BM049649.D\data.ms

(21) Benzo(a)anthracene

21.350min (-0.000) 0.05 ng/u1 m

response 5471

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.60	47.43#
226.00	27.80	50.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

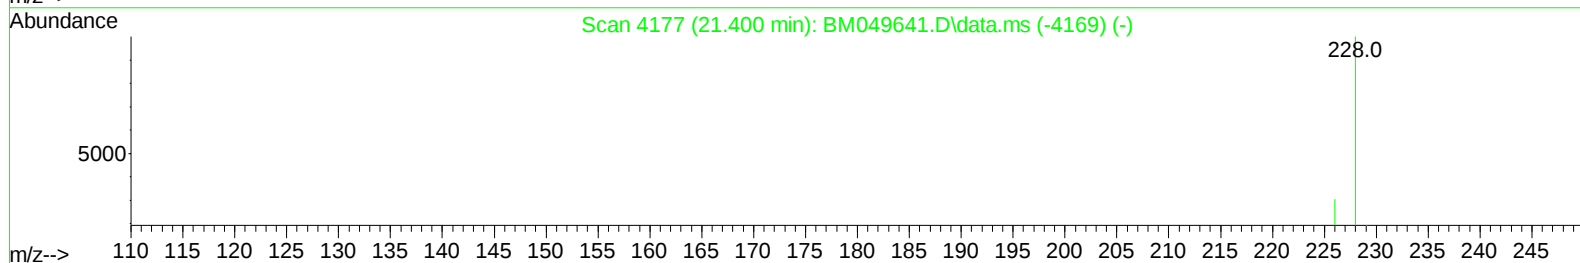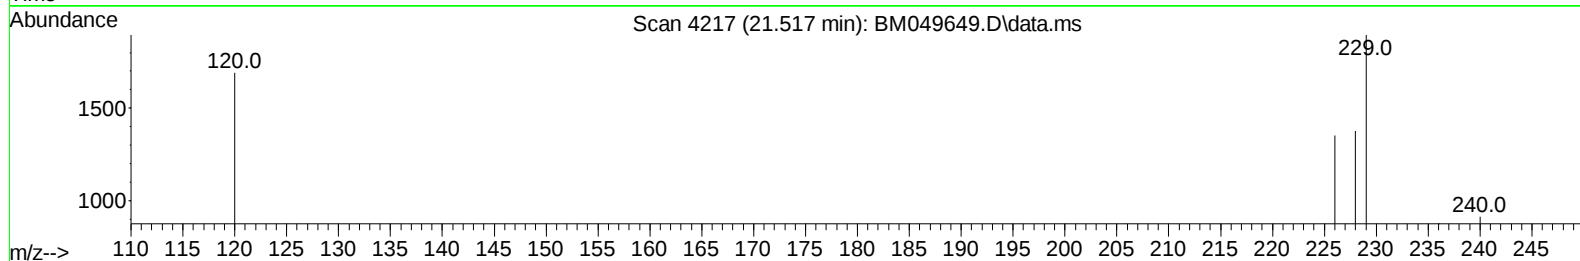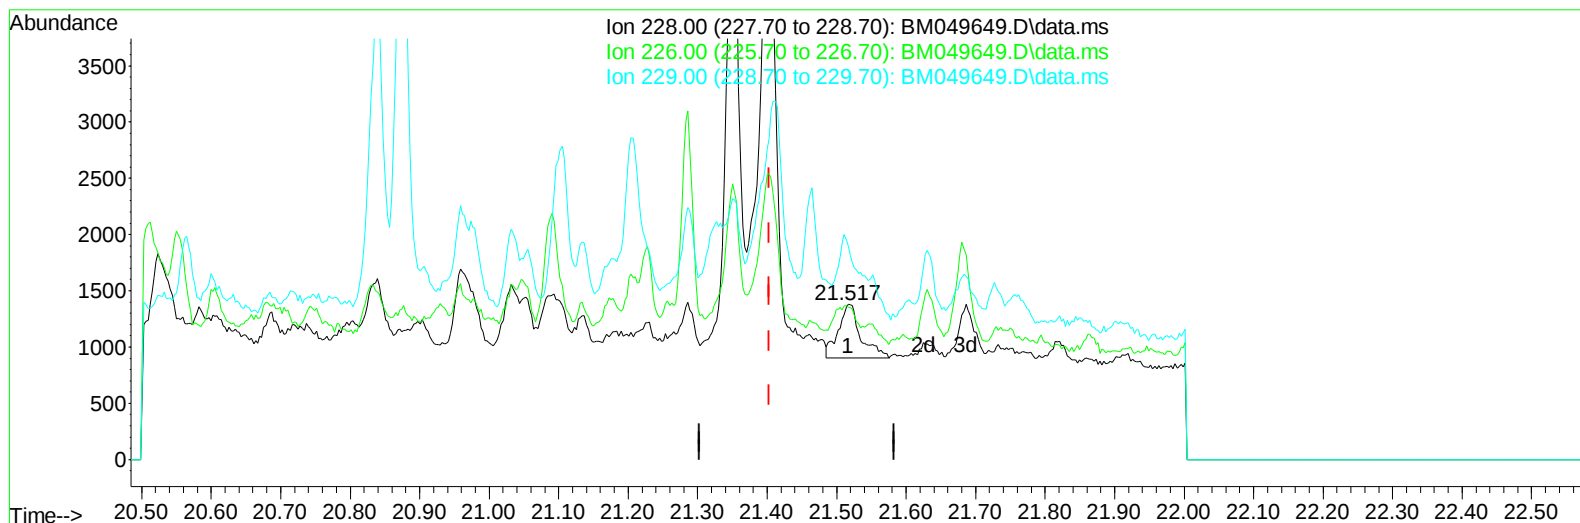

TIC: BM049649.D\data.ms

(22) Chrysene

21.517min (+ 0.113) 0.01 ng/u1

response 1061

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	31.10	98.04#
229.00	19.50	137.52#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

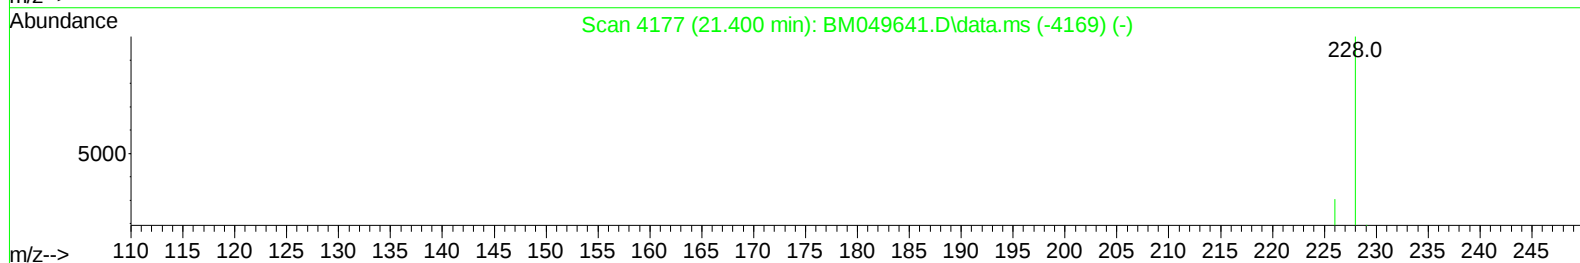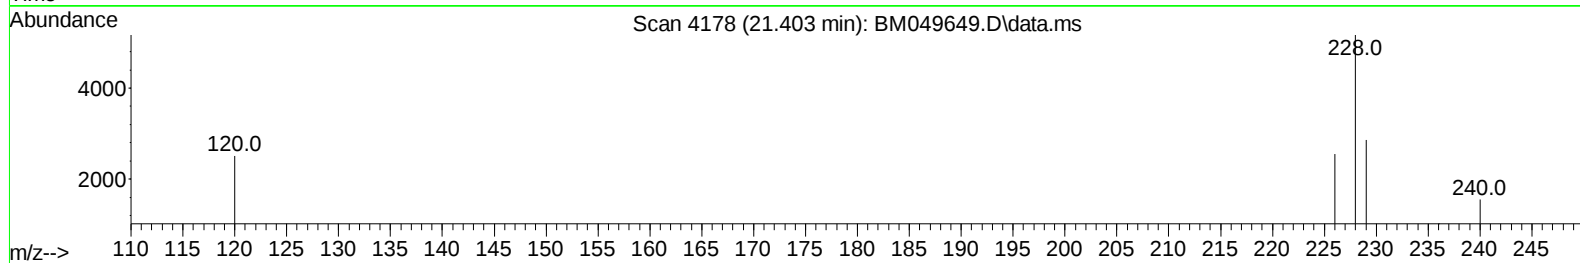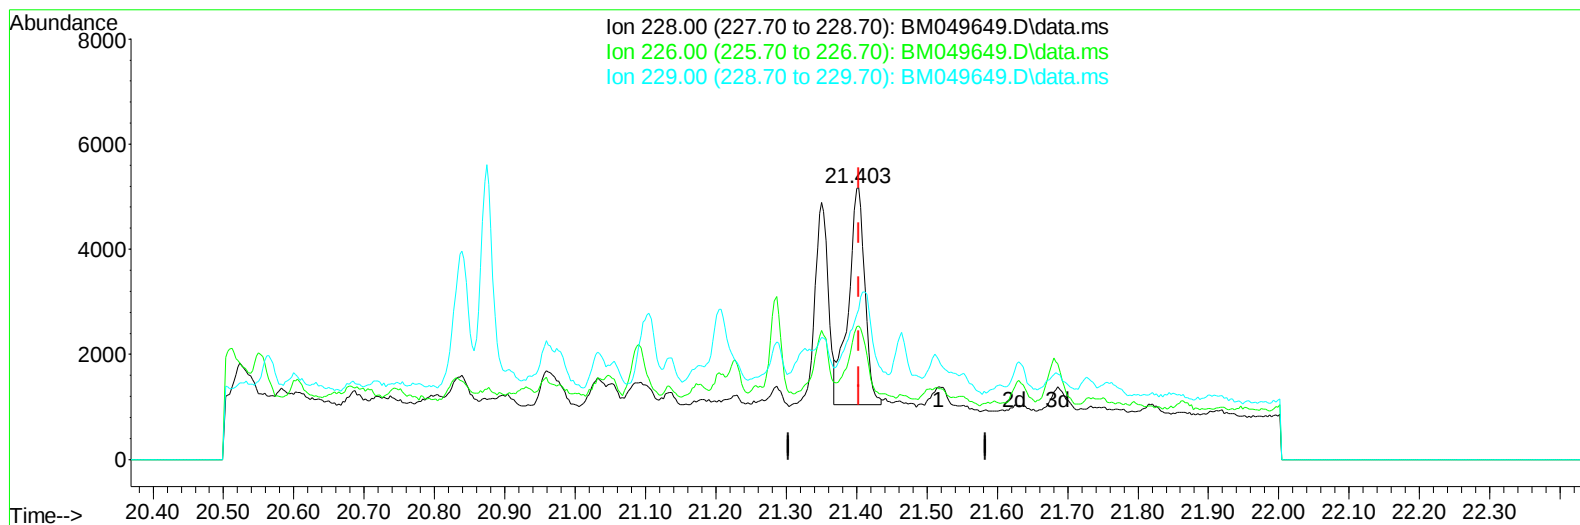

TIC: BM049649.D\data.ms

(22) Chrysene

21.403min (-0.001) 0.06 ng/ul m

response 6720

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	31.10	49.24#
229.00	19.50	55.25#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

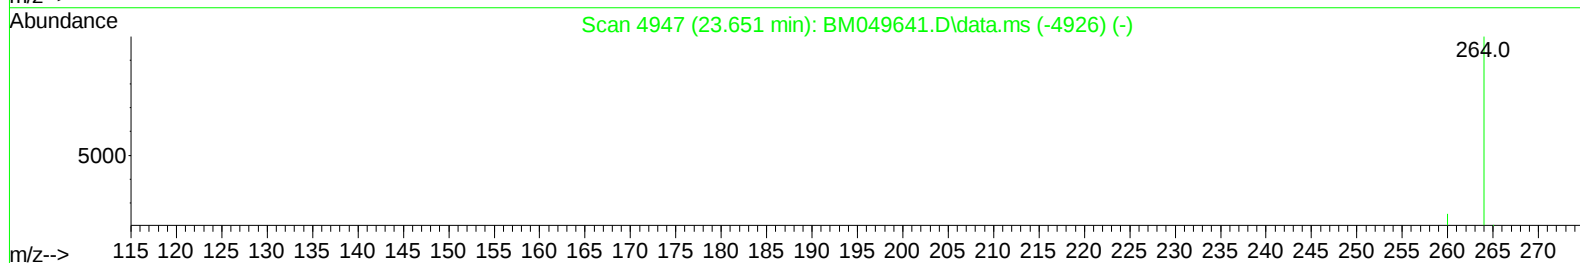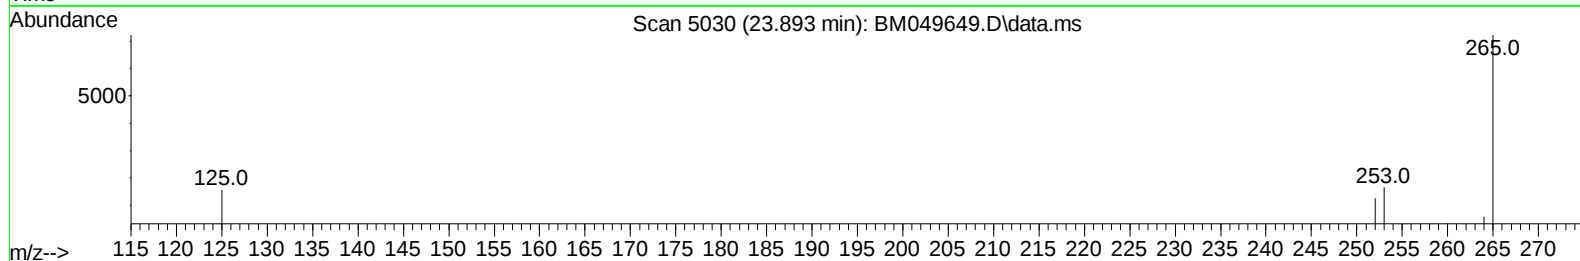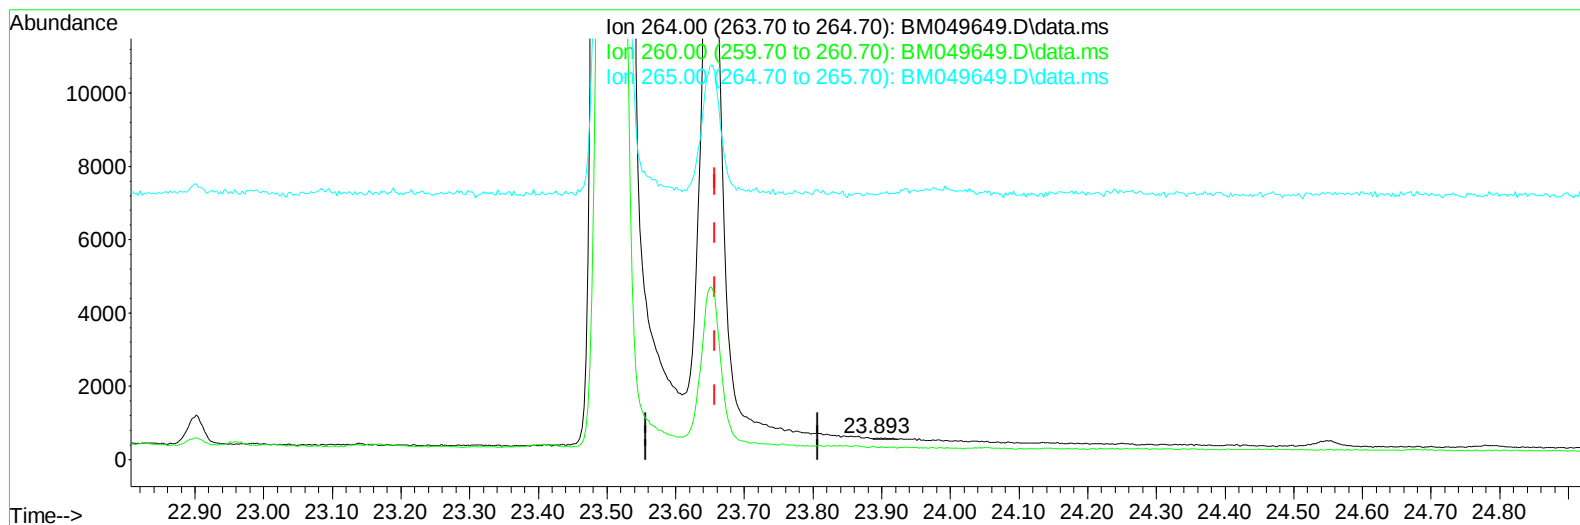

TIC: BM049649.D\data.ms

(23) Perylene-d12 (I)

23.893min (+ 0.236) 0.40 ng/u1

response 50

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	54.50#
265.00	67.10	1226.15#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

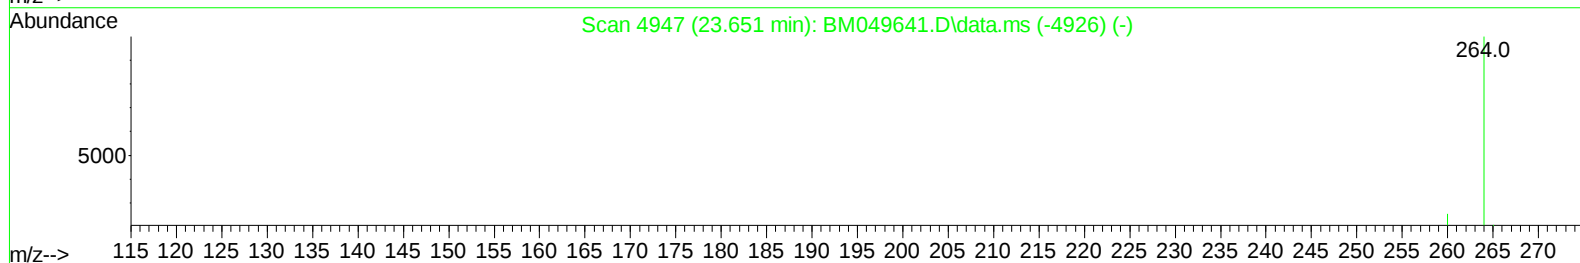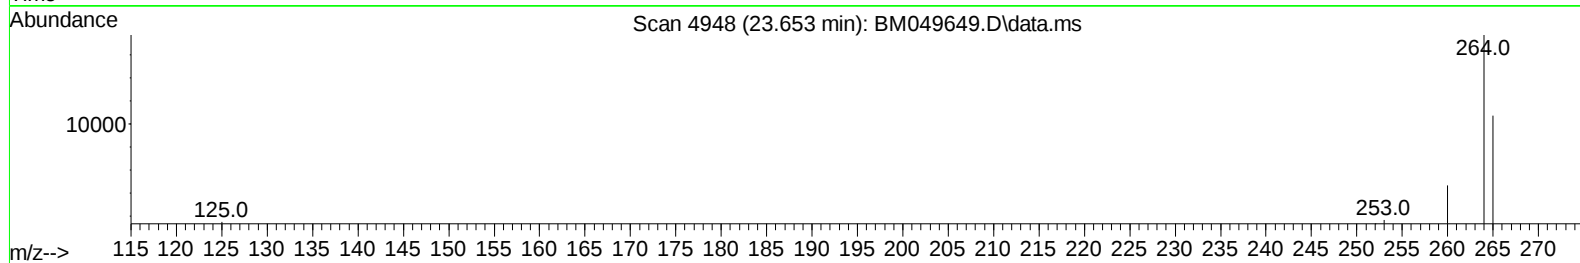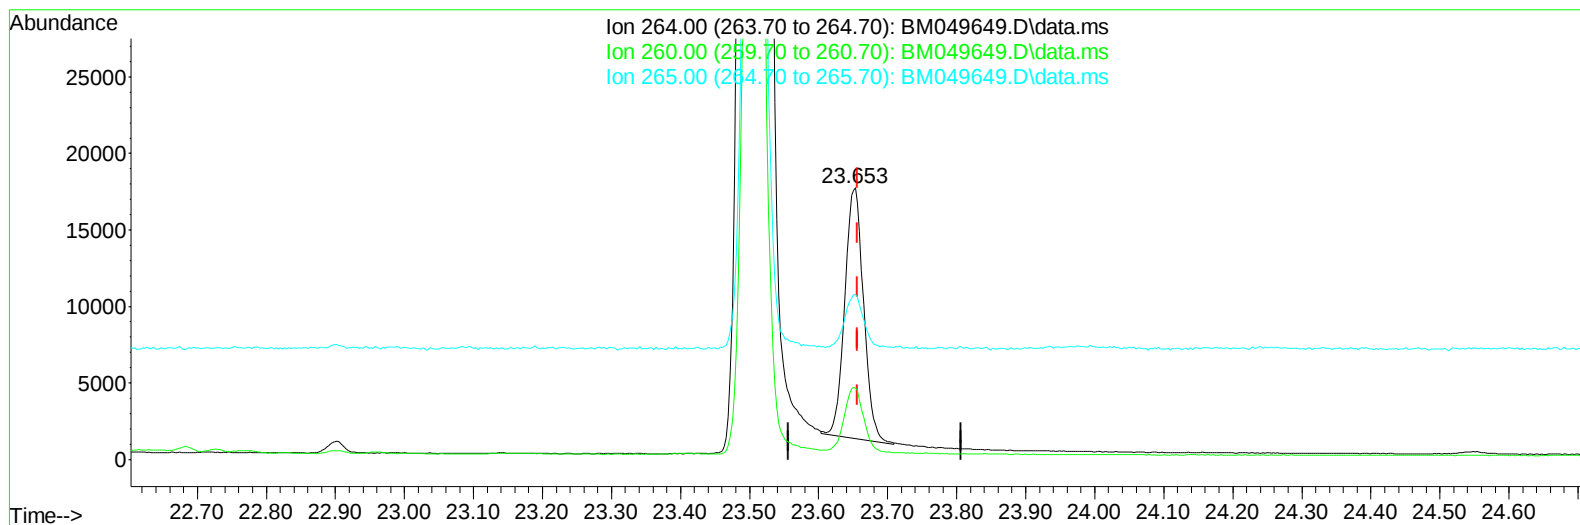

TIC: BM049649.D\data.ms

(23) Perylene-d12 (I)

23.653min (-0.003) 0.40 ng/ul m

response 31007

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	26.35
265.00	67.10	60.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

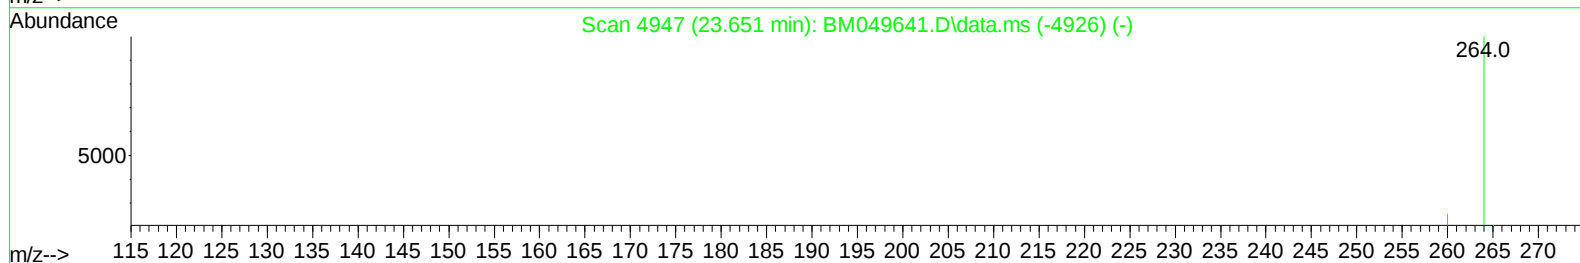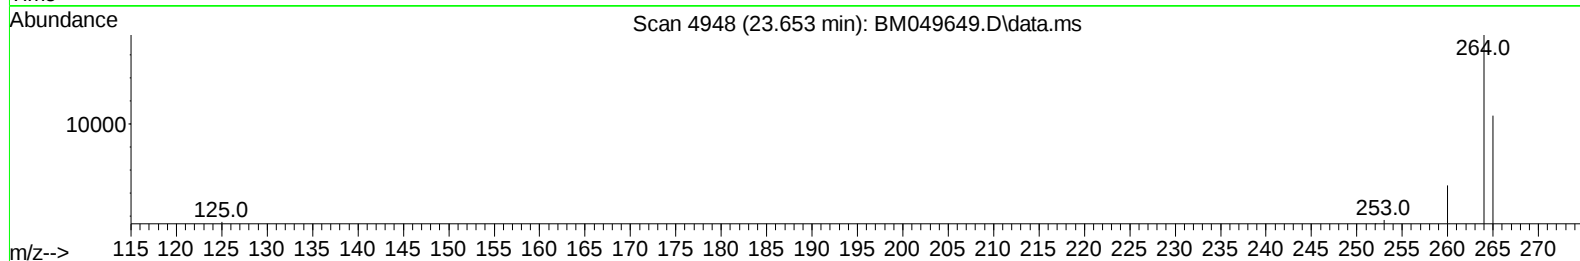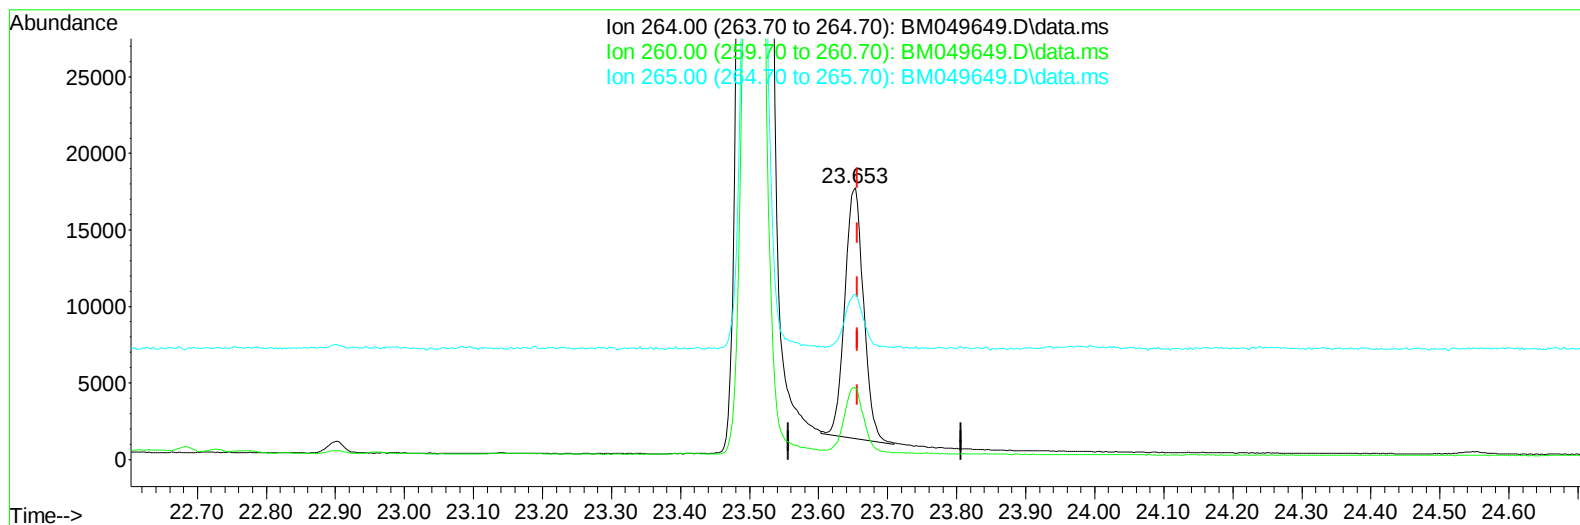

TIC: BM049649.D\data.ms

(23) Perylene-d12 (I)

23.653min (-0.003) 0.40 ng/ul m

response 31007

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	26.35
265.00	67.10	60.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

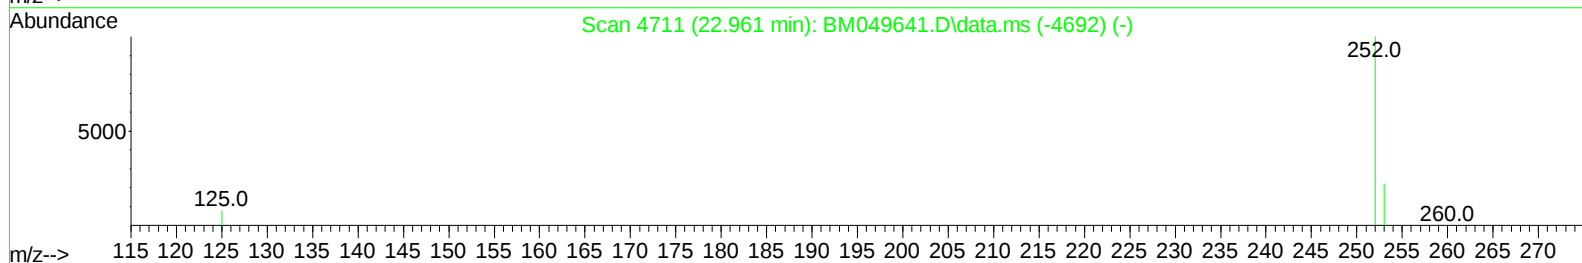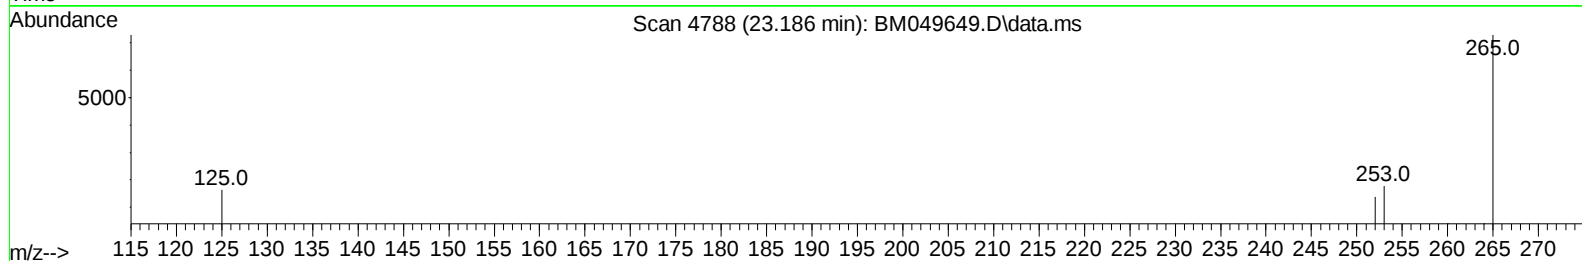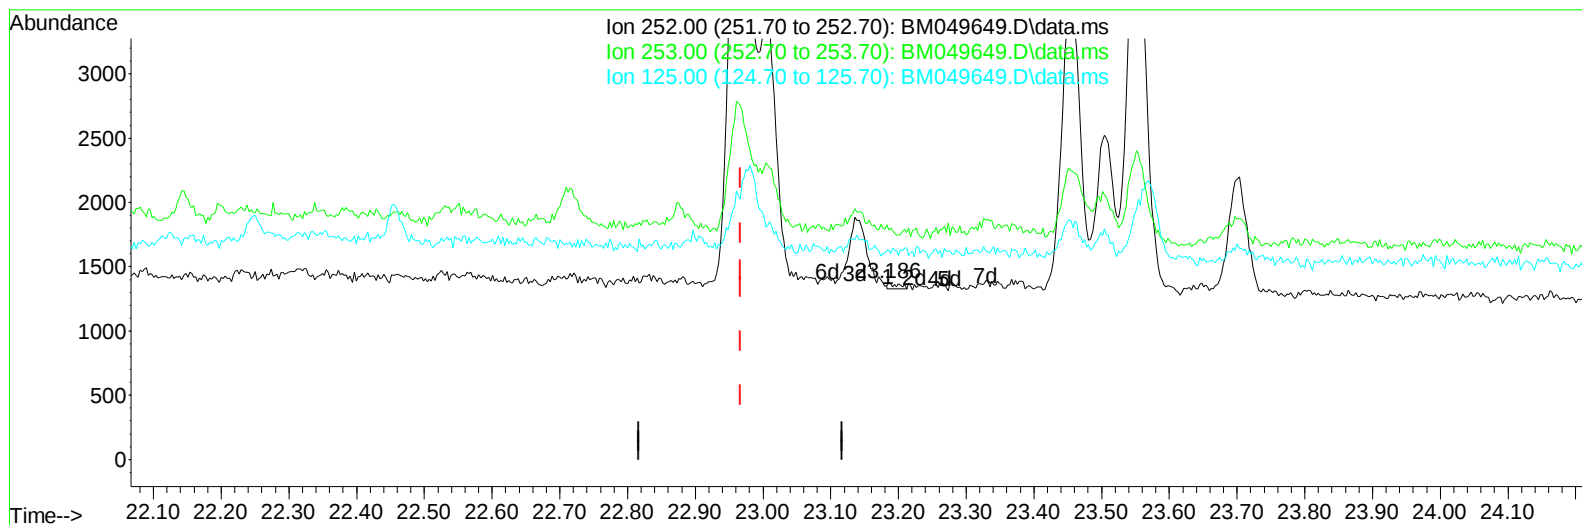

TIC: BM049649.D\data.ms

(24) Benzo(b)fluoranthene

23.186min (+ 0.219) 0.00 ng/u1

response 47

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	129.84#
125.00	12.80	118.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

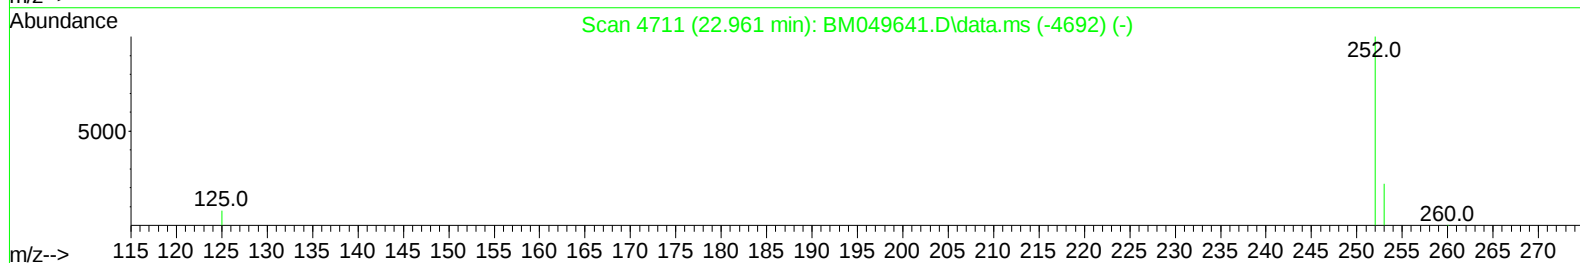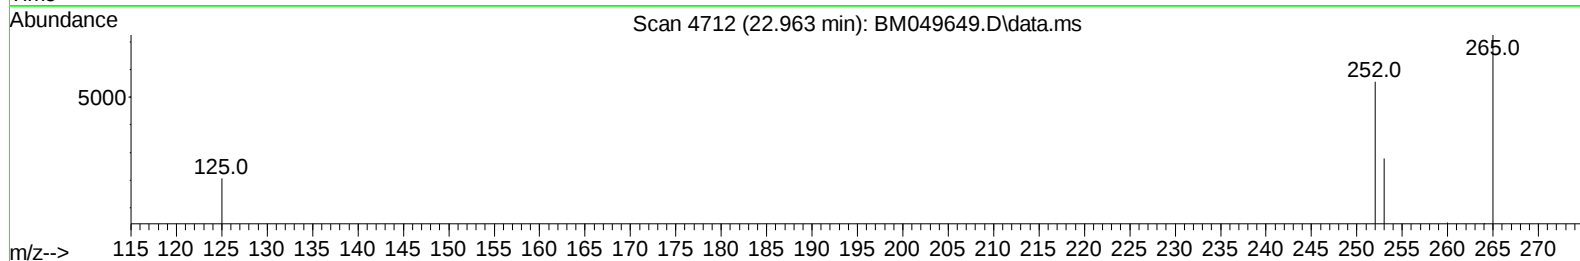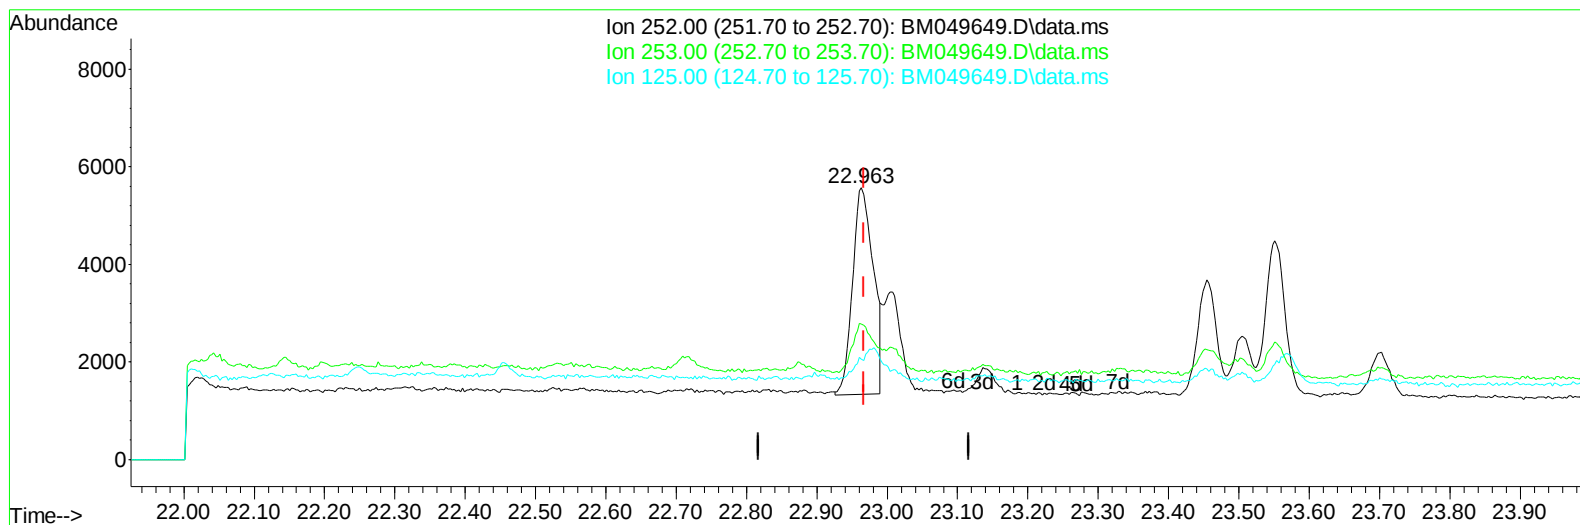

TIC: BM049649.D\data.ms

(24) Benzo(b)fluoranthene

22.963min (-0.003) 0.08 ng/u1 m

response 8717

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	49.92
125.00	12.80	36.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

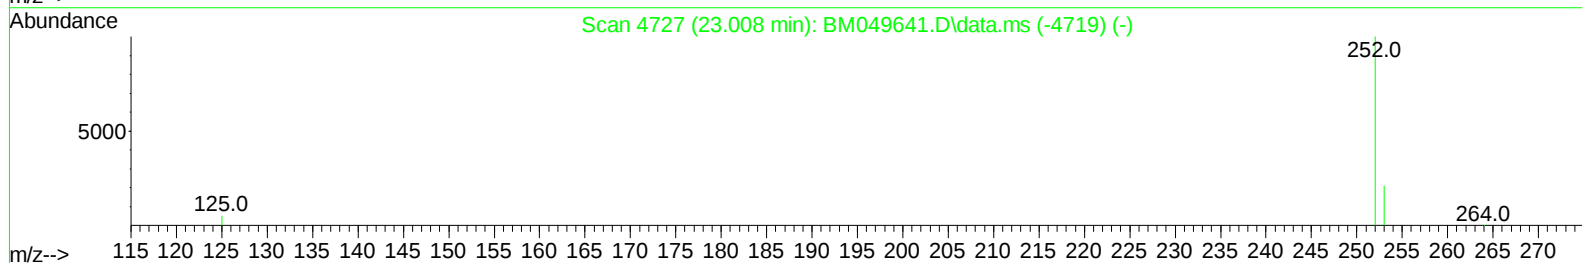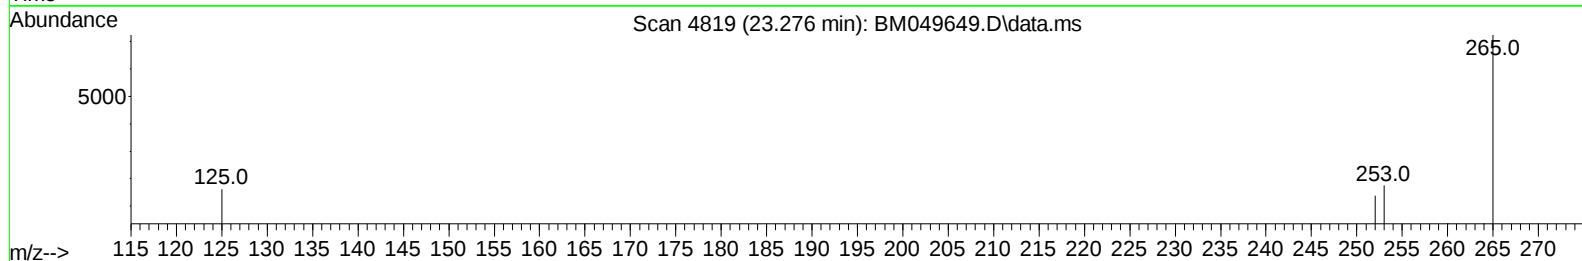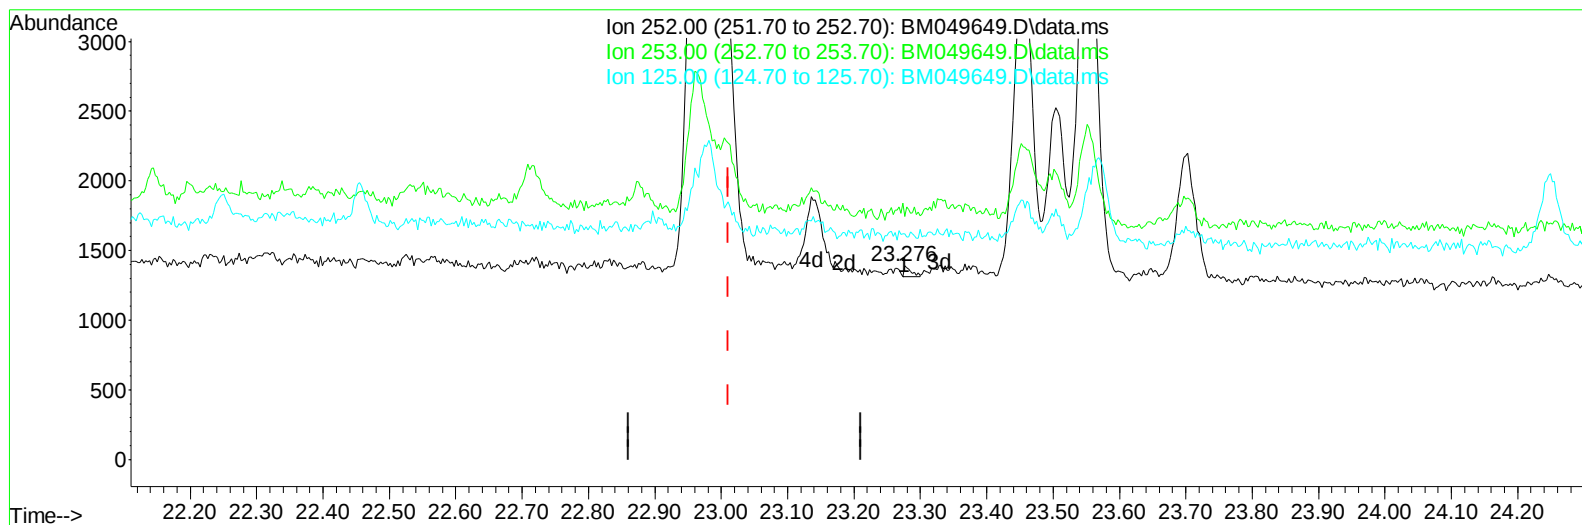

TIC: BM049649.D\data.ms

(25) Benzo(k)fluoranthene

23.276min (+ 0.266) 0.00 ng/u1

response 61

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.30	125.40#
125.00	13.00	116.62#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

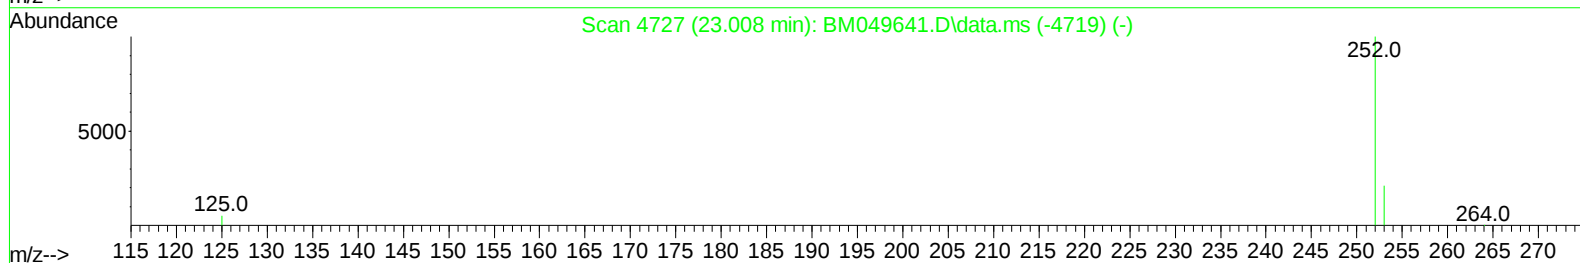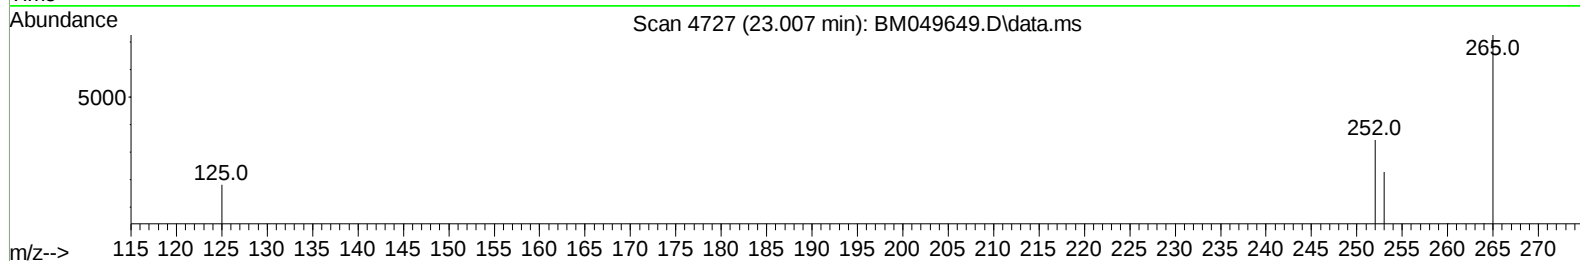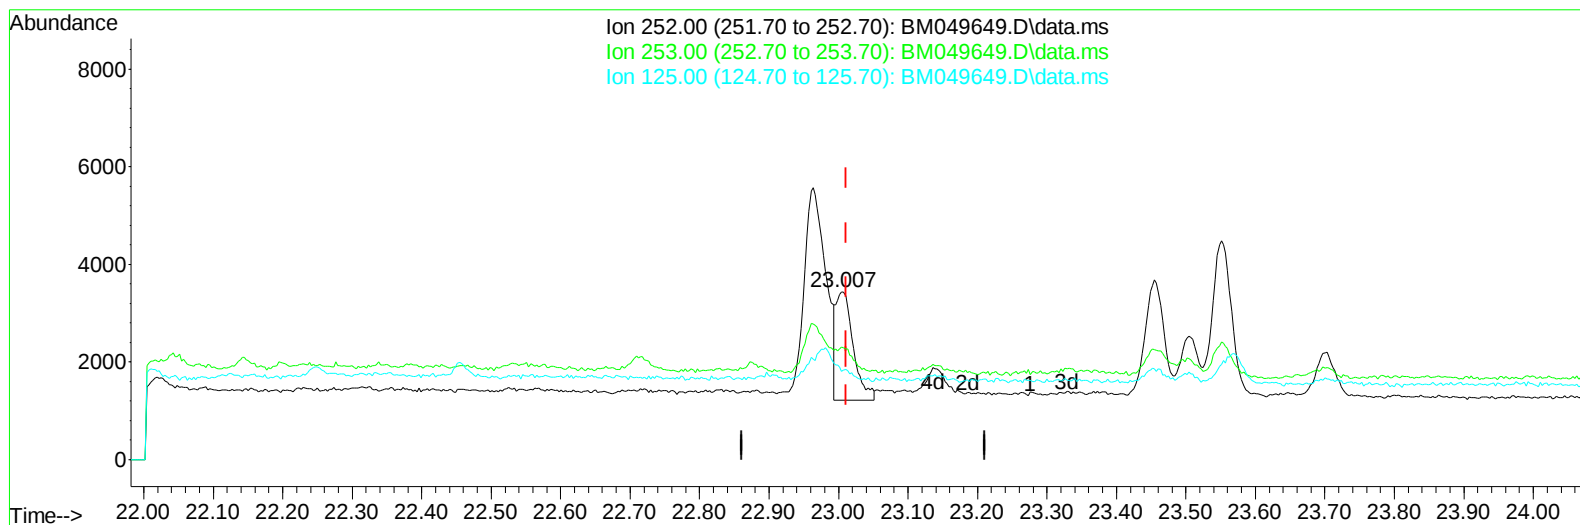

TIC: BM049649.D\data.ms

(25) Benzo(k)fluoranthene

23.007min (-0.003) 0.03 ng/u1 m

response 3905

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.30	66.59#
125.00	13.00	53.11#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

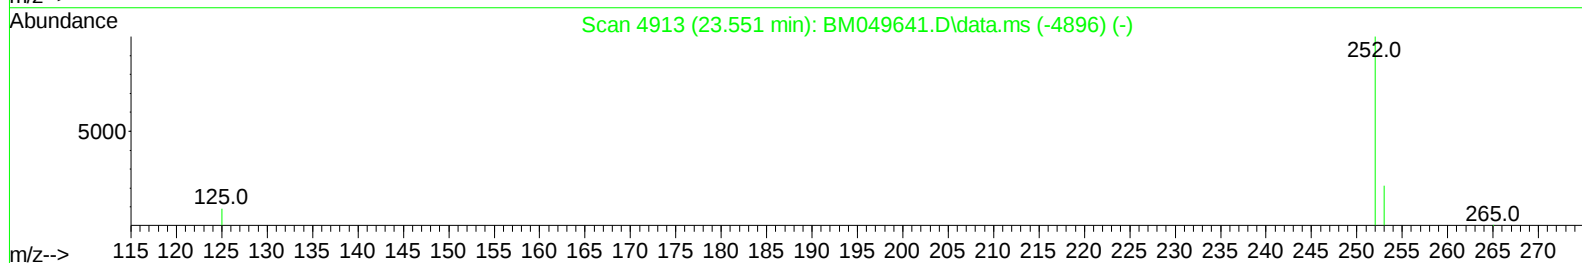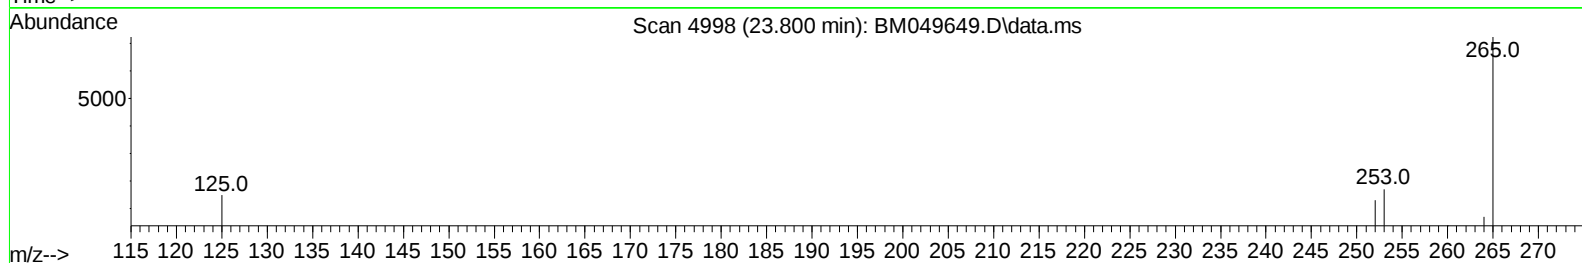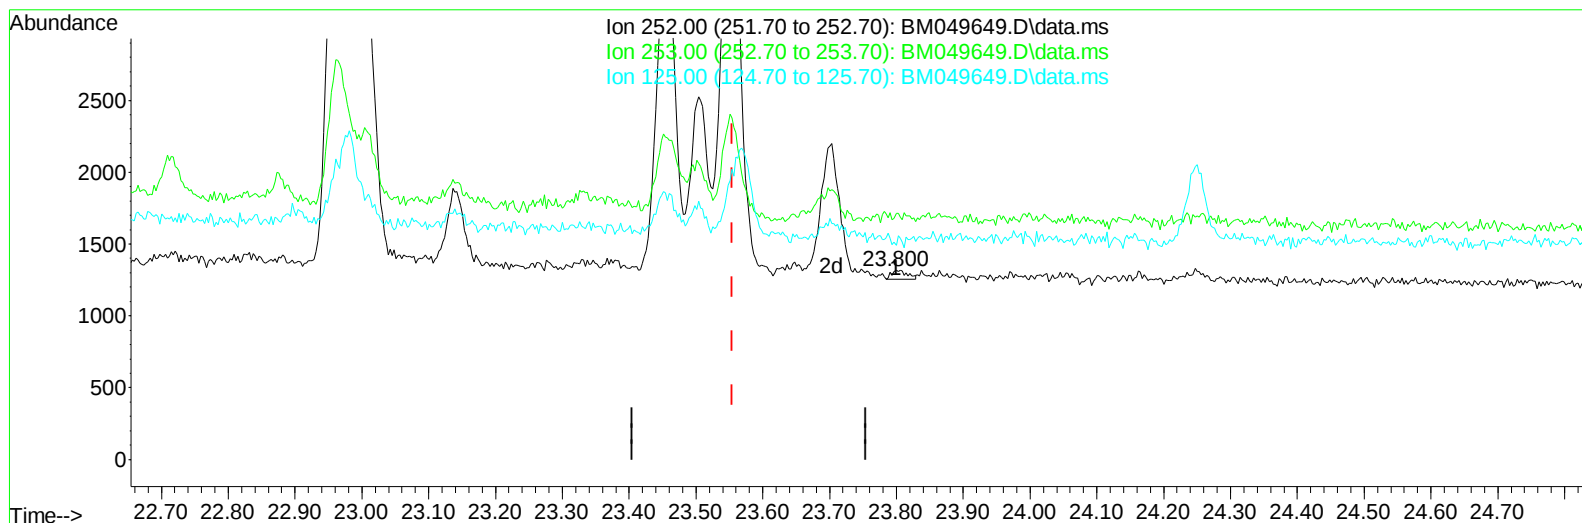

TIC: BM049649.D\data.ms

(26) Benzo(a)pyrene (C)

23.800min (+ 0.245) 0.00 ng/u1

response 105

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	130.24#
125.00	15.70	113.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

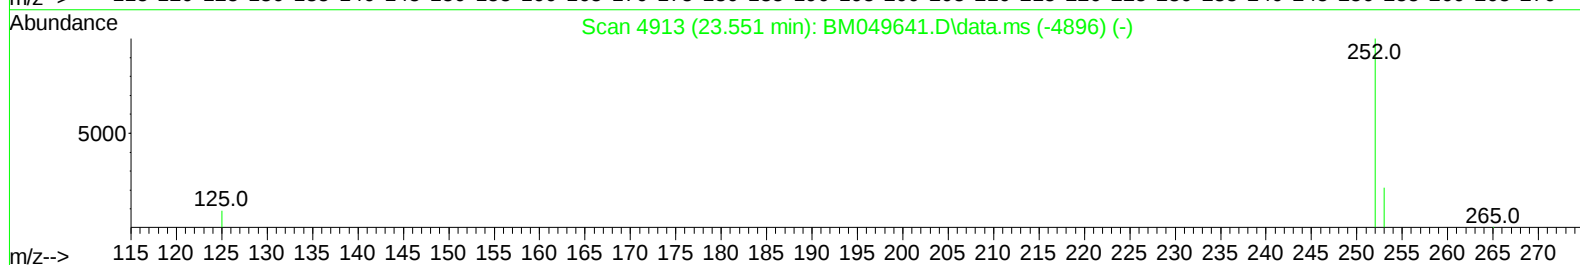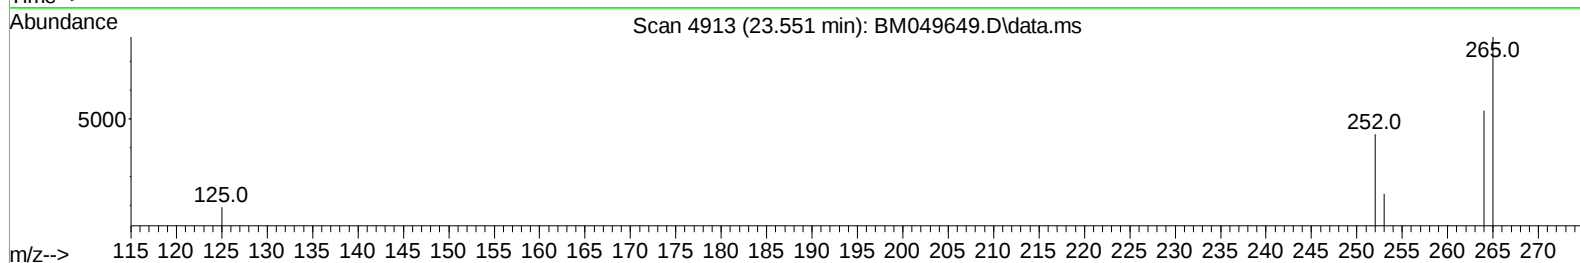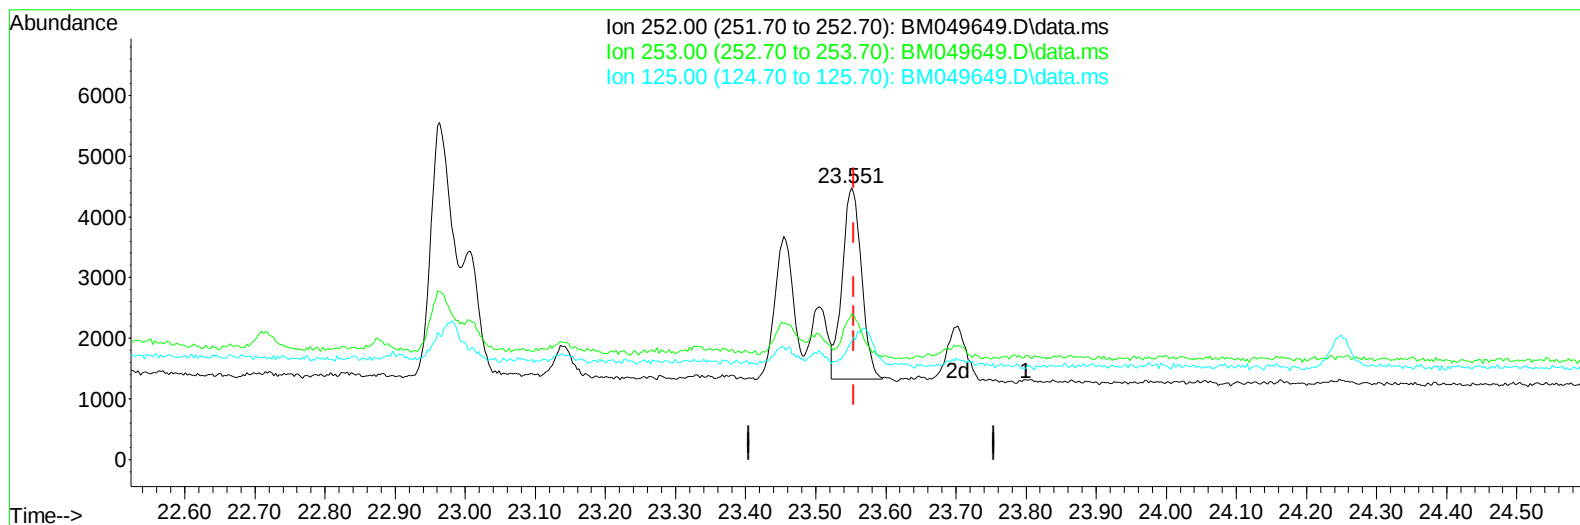

TIC: BM049649.D\data.ms

(26) Benzo(a)pyrene (C)

23.551min (-0.003) 0.06 ng/u1 m

response 6038

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	53.68#
125.00	15.70	43.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

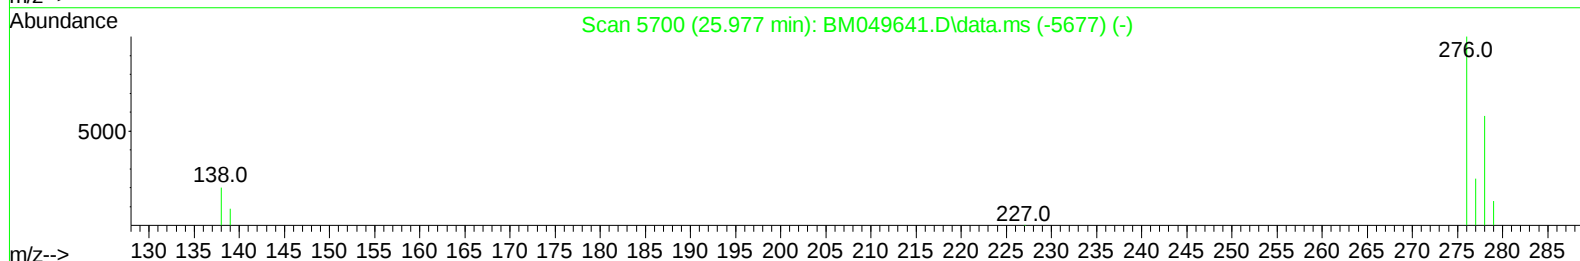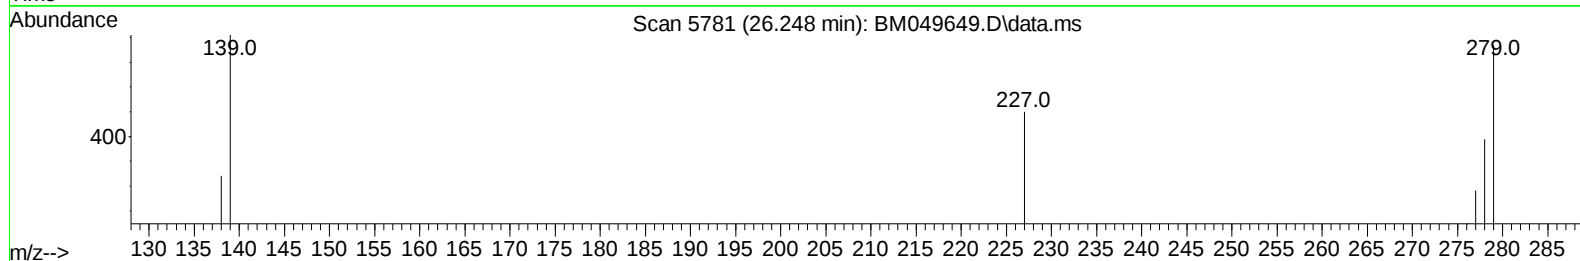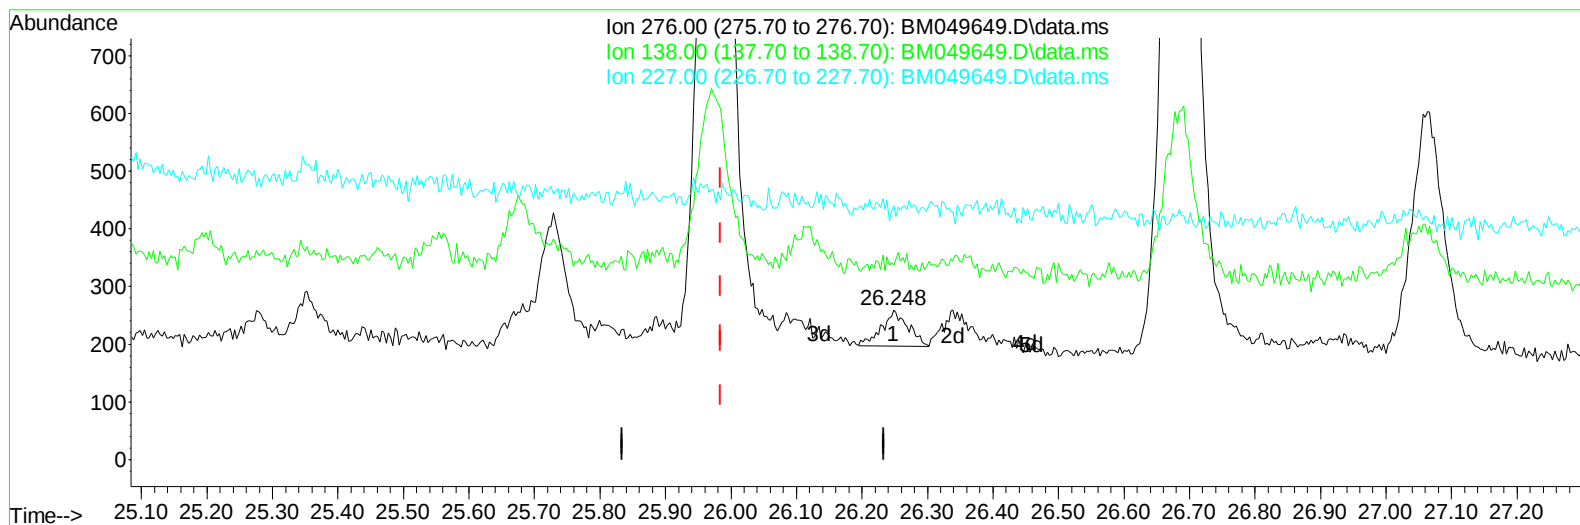

TIC: BM049649.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

26.248min (+ 0.264) 0.00 ng/u1

response 173

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	20.60	18.50
227.00	0.10	2.31#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

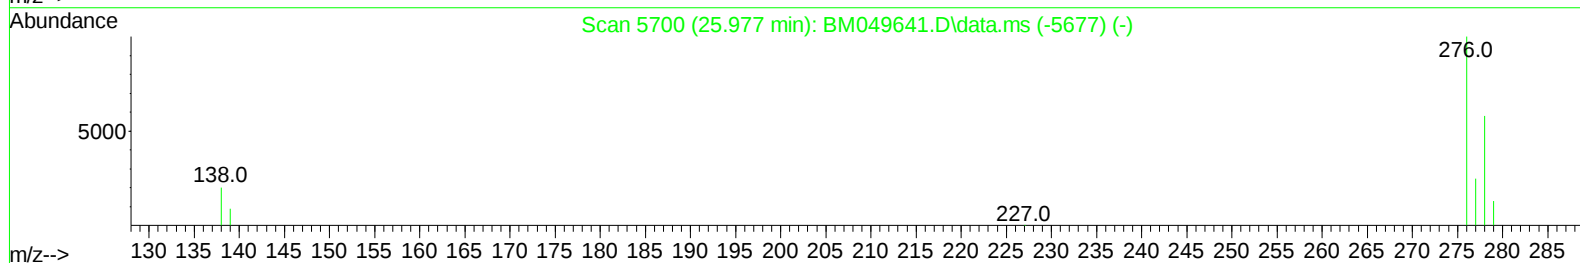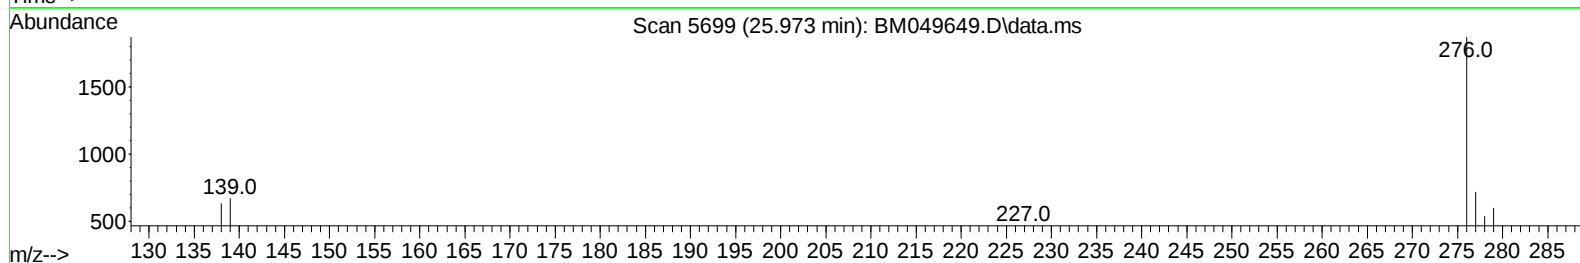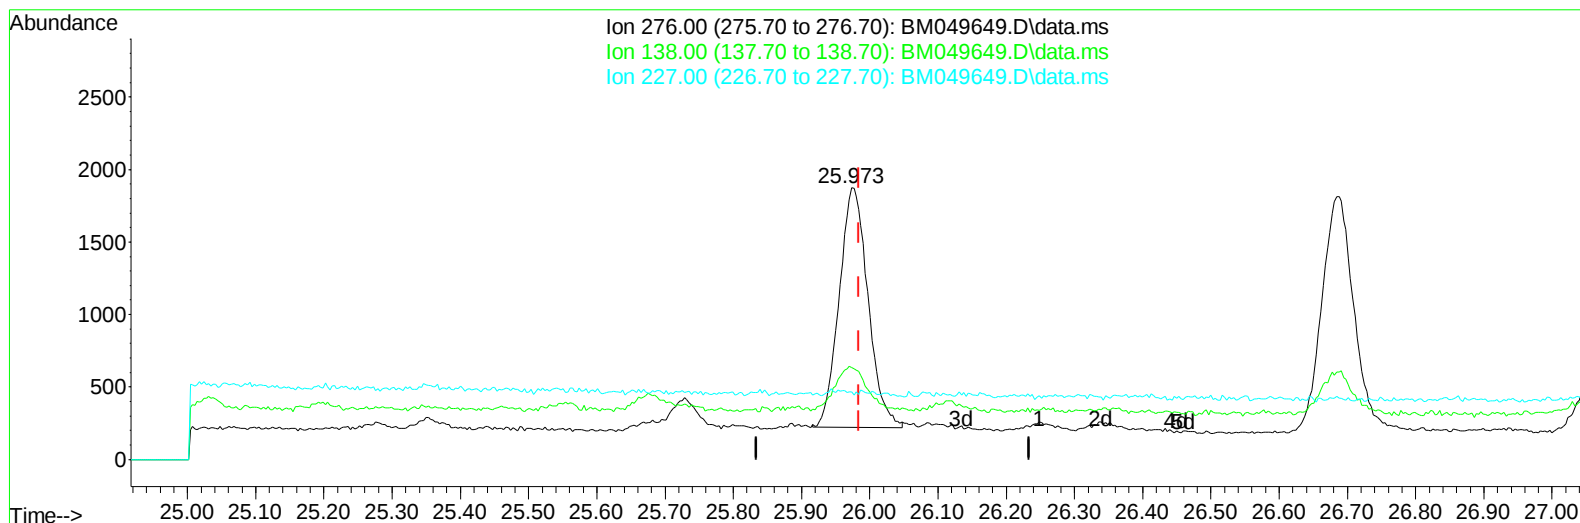

TIC: BM049649.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.973min (-0.011) 0.04 ng/ul m

response 4844

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	20.60	0.66#
227.00	0.10	0.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

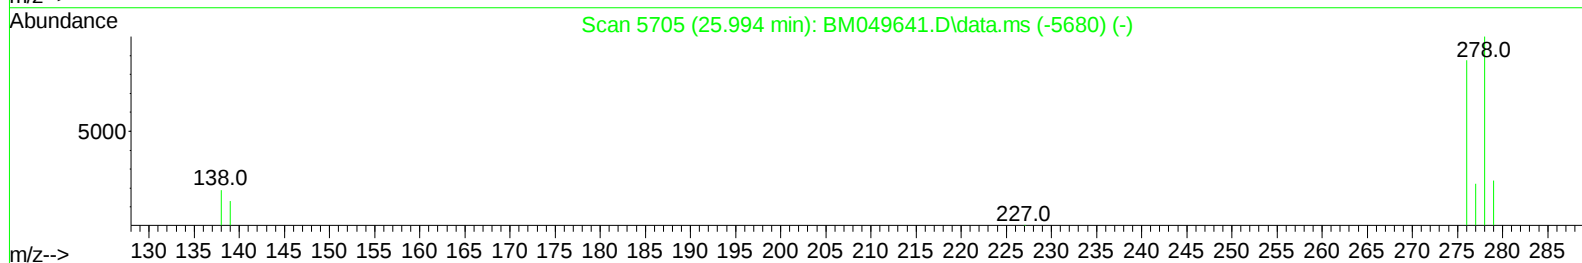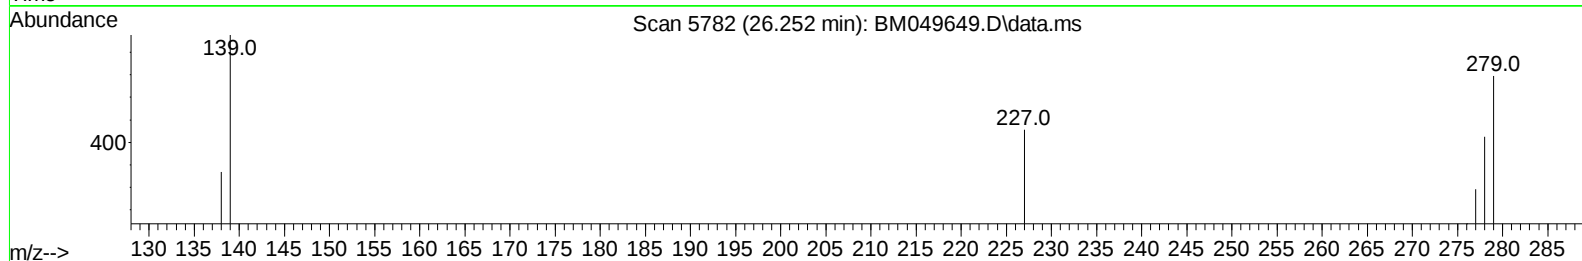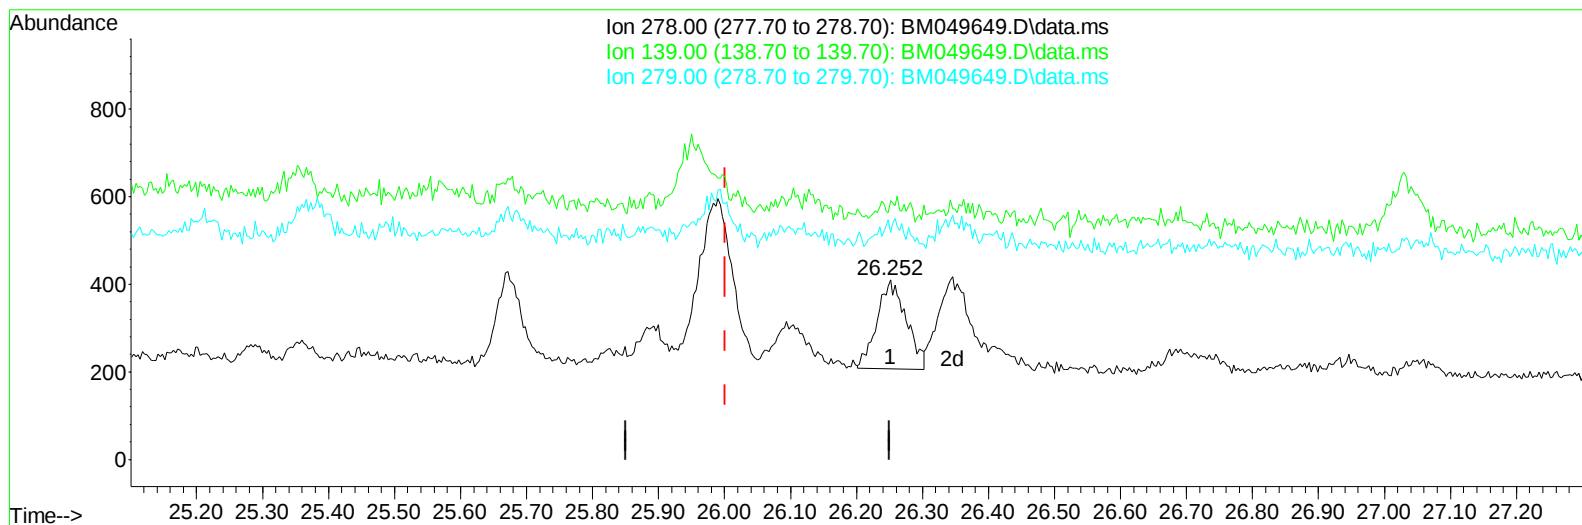

TIC: BM049649.D\data.ms

(28) Dibenzo(a,h)anthracene

26.252min (+ 0.251) 0.01 ng/u1

response 623

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	16.70	144.15#
279.00	26.90	126.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

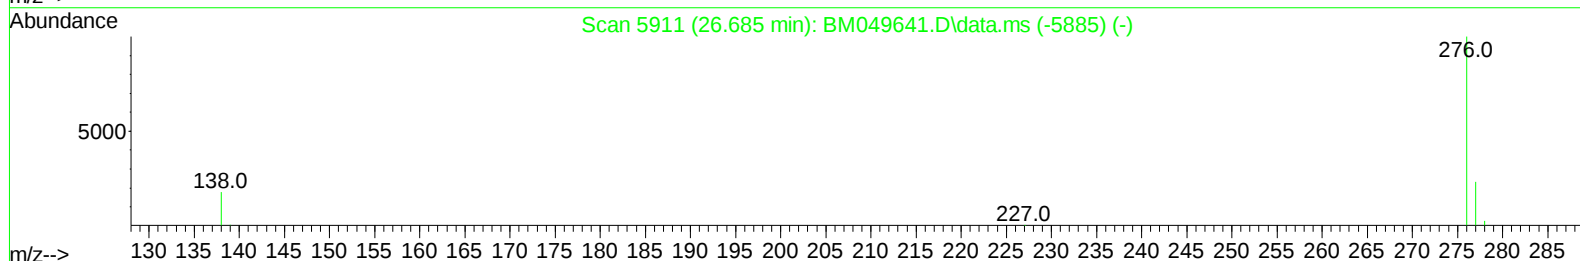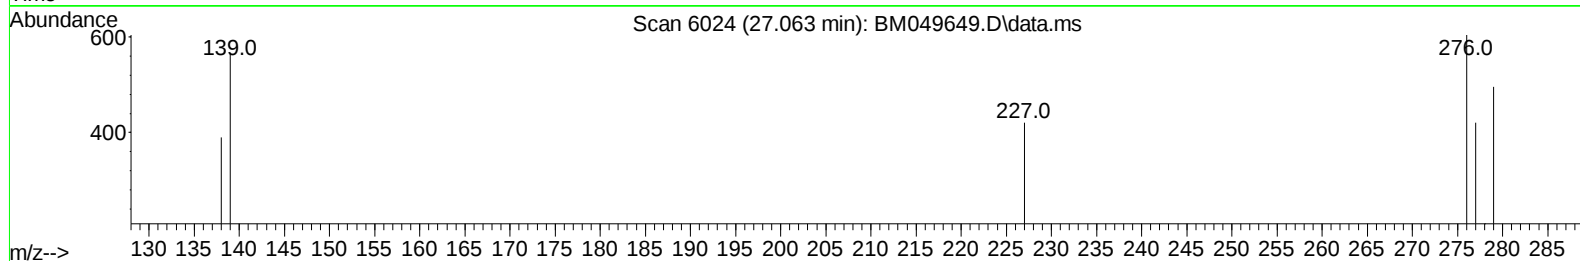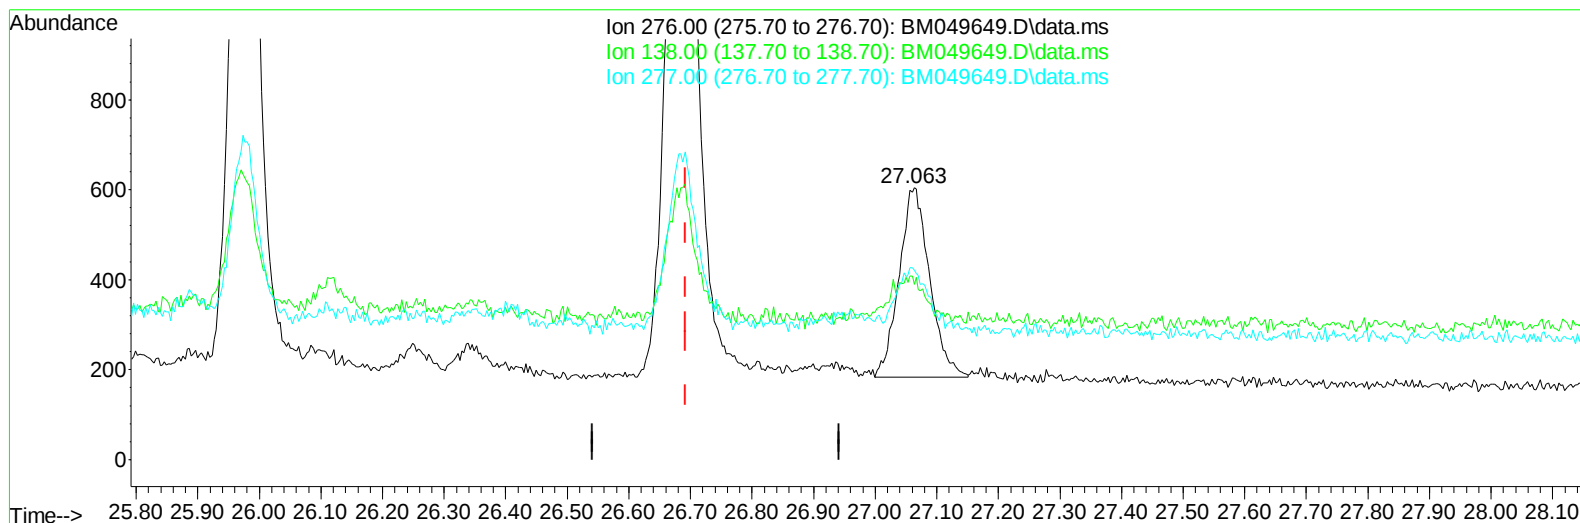

TIC: BM049649.D\data.ms

(29) Benzo(g,h,i)perylene

27.063min (+ 0.372) 0.01 ng/u1

response 1441

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	19.70	64.57#
277.00	24.90	69.70#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

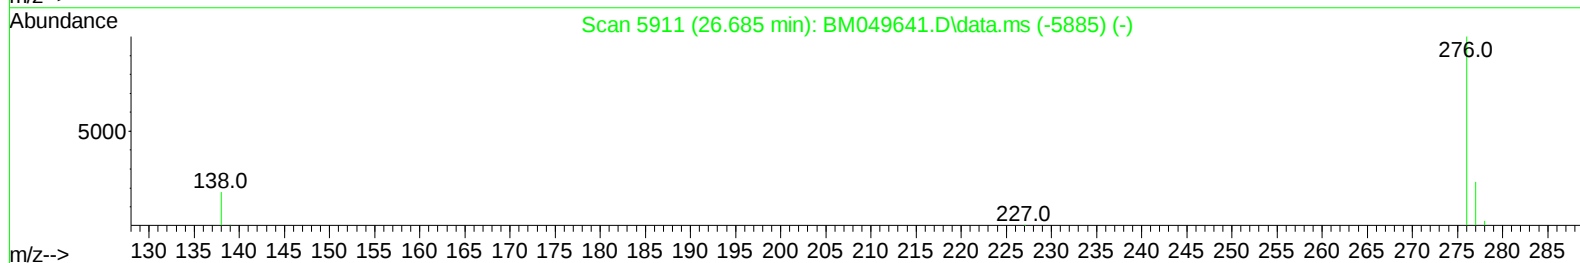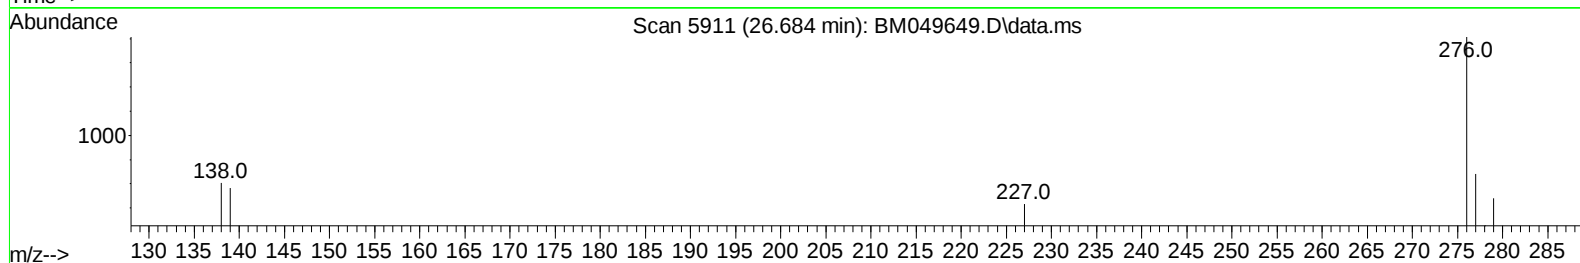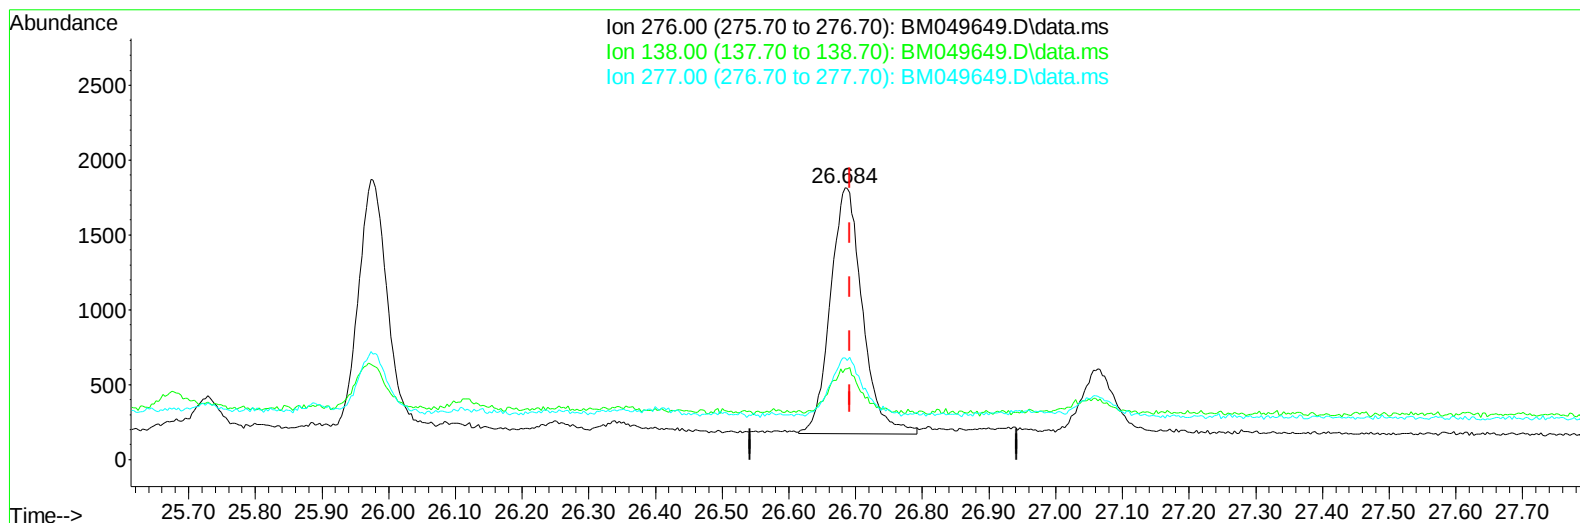

TIC: BM049649.D\data.ms

(29) Benzo(g,h,i)perylene

26.684min (-0.007) 0.05 ng/ul m

response 5518

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	19.70	33.35#
277.00	24.90	37.49#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
 Data File : BM049649.D
 Acq On : 13 Feb 2025 14:50
 Operator : RC/JU
 Sample : Q1202-19DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E29B3DL

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 02/19/2025
 Supervised By :Jagrut Upadhyay 02/19/2025

Quant Time: Feb 17 15:07:46 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 12 16:40:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.809	152	9848	0.400	ng/ul	0.00
4) Naphthalene-d8	10.607	136	45893m	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.451	164	33331	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.188	188	44114m	0.400	ng/ul	0.00
17) Chrysene-d12	21.365	240	33412m	0.400	ng/ul	0.00
23) Perylene-d12	23.653	264	31007m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	6519	0.588	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.201	152	4295m	0.068	ng/ul	0.00
18) Fluoranthene-d10	19.211	212	8642m	0.085	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.656	128	486474	4.277	ng/ul	98
7) 2-Methylnaphthalene	12.278	142	90746	1.225	ng/ul	98
8) 1-Methylnaphthalene	12.498	142	88855	1.184	ng/ul	98
10) Acenaphthylene	14.169	152	7264	0.051	ng/ul#	48
11) Acenaphthene	14.511	153	42784	0.415	ng/ul	87
12) Fluorene	15.497	166	23300	0.198	ng/ul#	99
14) Pentachlorophenol	16.842	266	800m	0.088	ng/ul	
15) Phenanthrene	17.230	178	54518m	0.462	ng/ul	
16) Anthracene	17.319	178	18165m	0.168	ng/ul	
19) Fluoranthene	19.244	202	17070m	0.124	ng/ul	
20) Pyrene	19.606	202	13963m	0.098	ng/ul	
21) Benzo(a)anthracene	21.350	228	5471m	0.048	ng/ul	
22) Chrysene	21.403	228	6720m	0.055	ng/ul	
24) Benzo(b)fluoranthene	22.963	252	8717m	0.084	ng/ul	
25) Benzo(k)fluoranthene	23.007	252	3905m	0.034	ng/ul	
26) Benzo(a)pyrene	23.551	252	6038m	0.065	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.973	276	4844m	0.037	ng/ul	
29) Benzo(g,h,i)perylene	26.684	276	5518m	0.052	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049649.D
Acq On : 13 Feb 2025 14:50
Operator : RC/JU
Sample : Q1202-19DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E29B3DL

Manual IntegrationsAPPROVED

Quant Time: Feb 17 15:07:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

