

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
 Data File : BM049627.D
 Acq On : 12 Feb 2025 20:21
 Operator : RC/JU
 Sample : Q1336-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E29C5

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 02/19/2025
 Supervised By :Jagrut Upadhyay 02/19/2025

Quant Time: Feb 14 16:13:25 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 12 16:40:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	5986	0.400	ng/u1	0.00
4) Naphthalene-d8	10.605	136	16309	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.450	164	9460	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.191	188	20687m	0.400	ng/u1	0.00
17) Chrysene-d12	21.368	240	14075m	0.400	ng/u1	0.00
23) Perylene-d12	23.654	264	13462m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	36781	5.462	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.200	152	8086	0.361	ng/u1	0.00
18) Fluoranthene-d10	19.215	212	18664	0.435	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.840	266	152m	0.036	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049627.D
Acq On : 12 Feb 2025 20:21
Operator : RC/JU
Sample : Q1336-01
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E29C5

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025


Quant Time: Feb 14 16:13:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

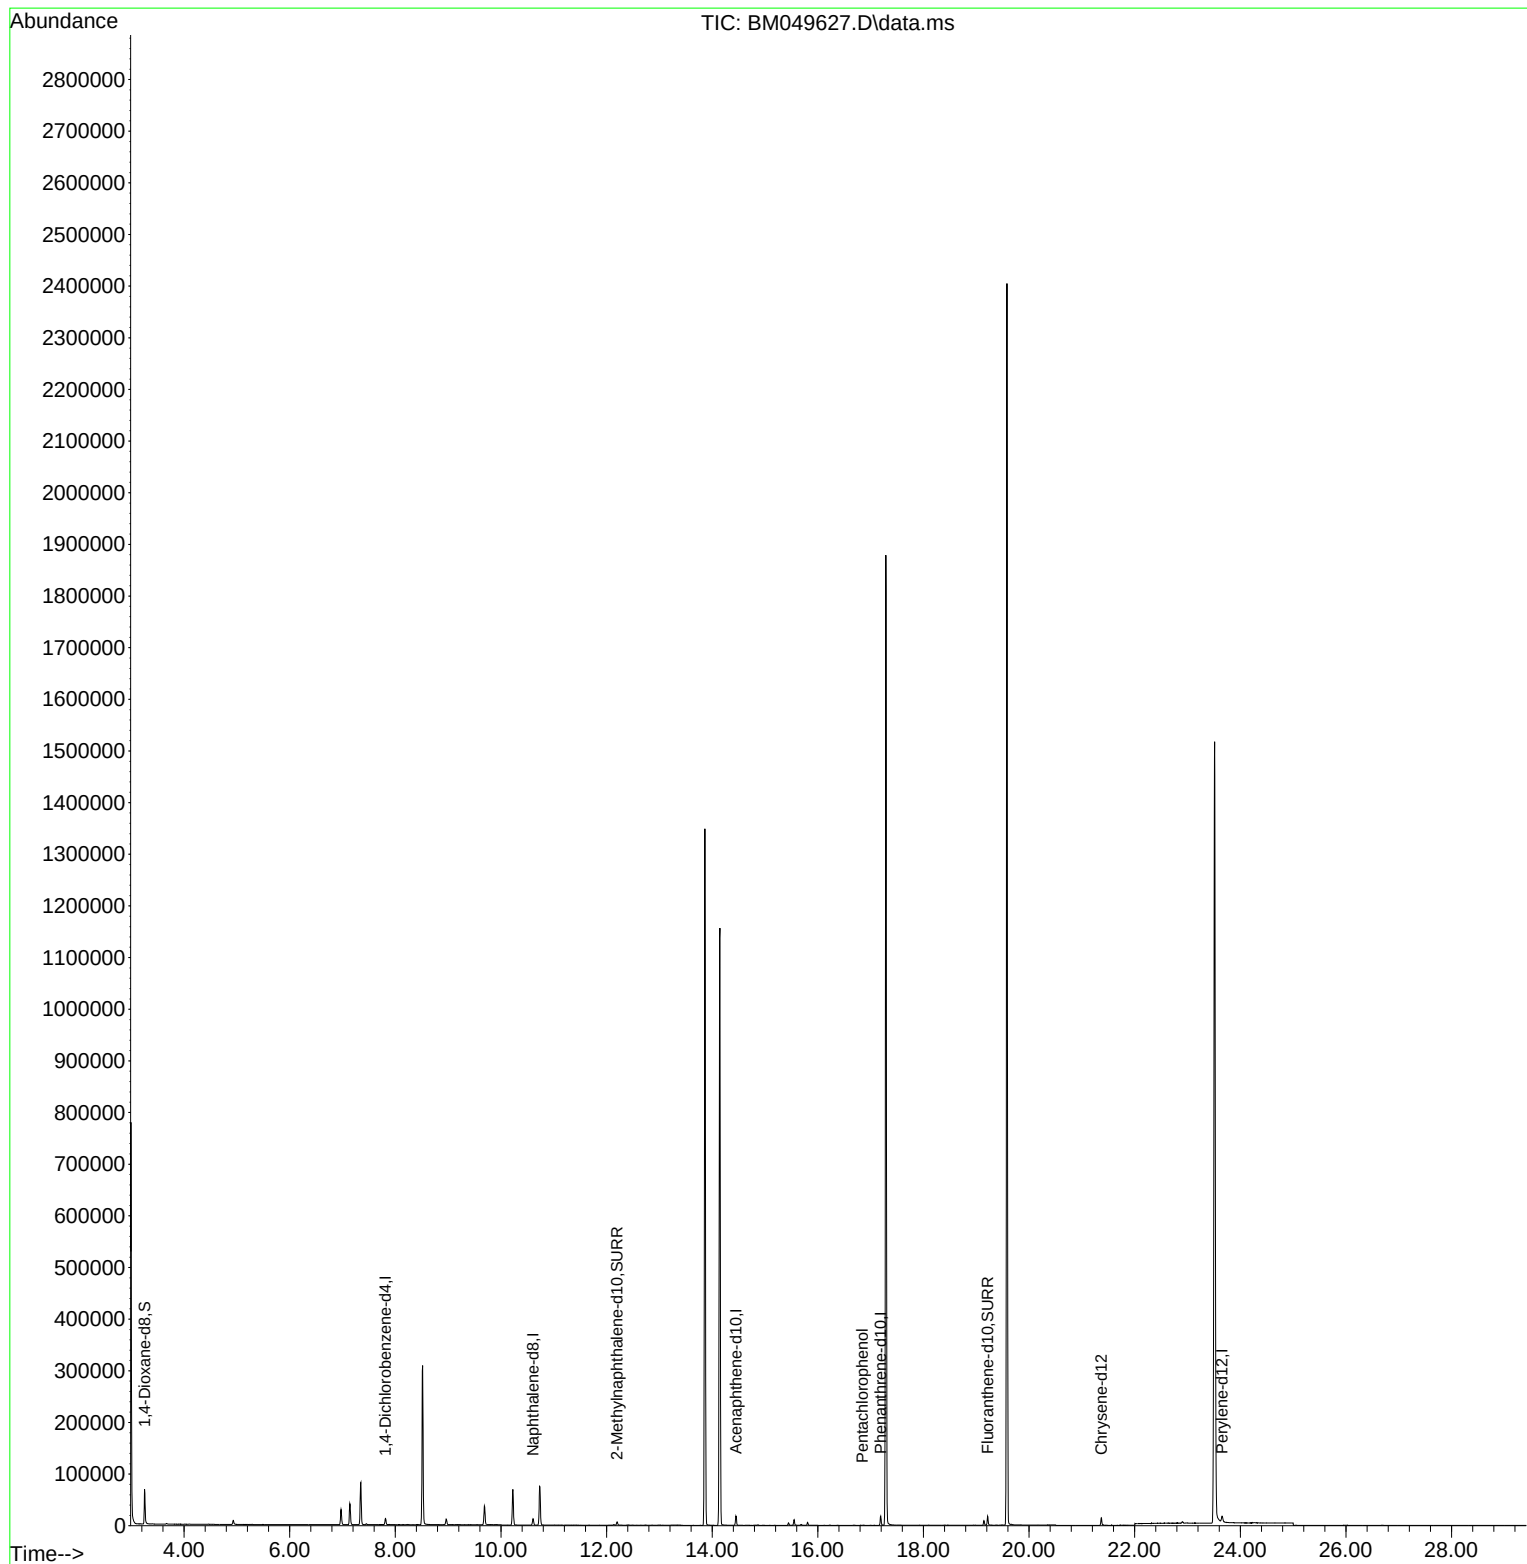

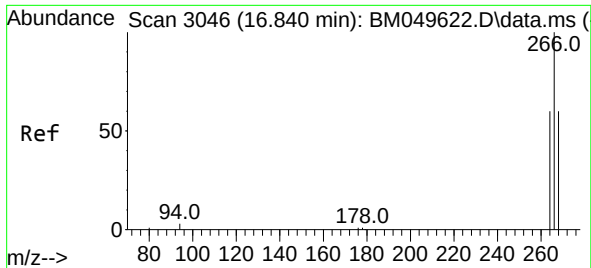

#14
 Pentachlorophenol
 Concen: 0.036 ng/ul m
 RT: 16.840 min Scan# 3046
 Delta R.T. -0.000 min
 Lab File: BM049627.D
 Acq: 12 Feb 2025 20:21

Instrument :
 BNA_M
 ClientSampleId :
 E29C5

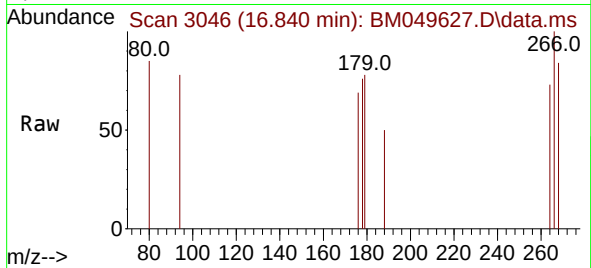

Tgt Ion:	266	Resp:	152
Ion	Ratio	Lower	Upper
266	100		
264	2.6	50.3	75.5
268	1.3	49.2	73.8

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 02/19/2025
 Supervised By :Jagrut Upadhyay 02/19/2025

