

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
 Data File : BM049628.D
 Acq On : 12 Feb 2025 20:57
 Operator : RC/JU
 Sample : Q1336-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E29C7

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 02/19/2025
 Supervised By :Jagrut Upadhyay 02/19/2025

Quant Time: Feb 14 16:24:22 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 12 16:40:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	6979	0.400	ng/ul	0.00
4) Naphthalene-d8	10.605	136	19417	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.450	164	11203	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.191	188	24231m	0.400	ng/ul	0.00
17) Chrysene-d12	21.365	240	16885m	0.400	ng/ul	0.00
23) Perylene-d12	23.654	264	16874m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	43529	5.544	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.200	152	9080	0.340	ng/ul	0.00
18) Fluoranthene-d10	19.215	212	21430	0.417	ng/ul	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.840	266	173m	0.035	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049628.D
Acq On : 12 Feb 2025 20:57
Operator : RC/JU
Sample : Q1336-02
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E29C7

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025


Quant Time: Feb 14 16:24:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

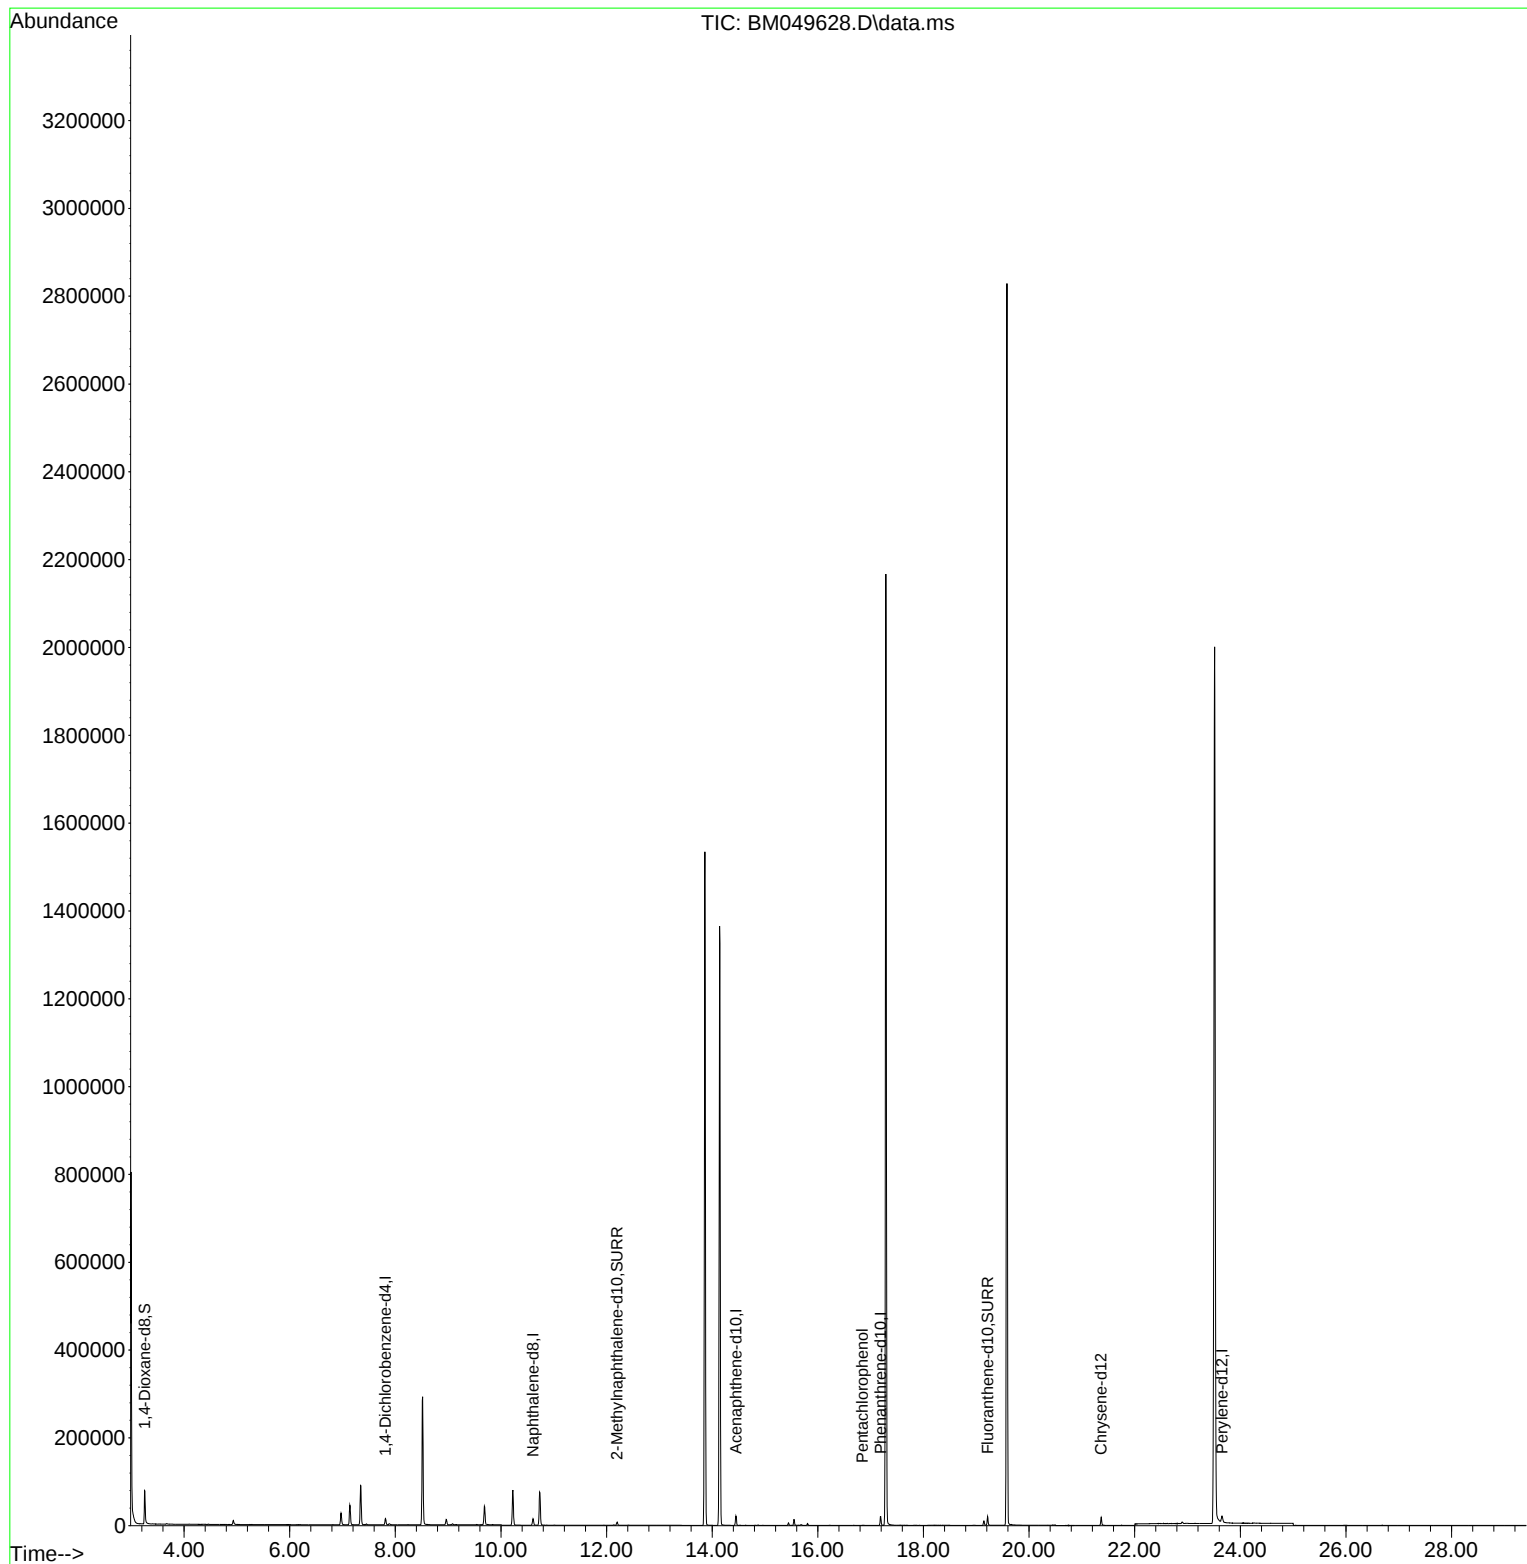

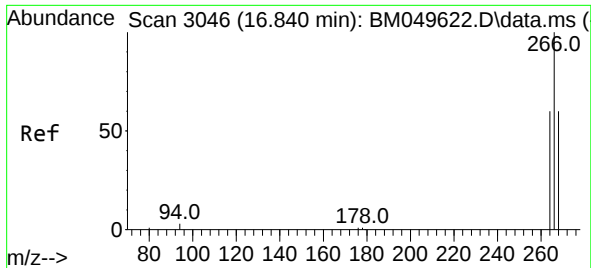

#14
 Pentachlorophenol
 Concen: 0.035 ng/ul m
 RT: 16.840 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BM049628.D
 Acq: 12 Feb 2025 20:57

Instrument :
 BNA_M
 ClientSampleId :
 E29C7

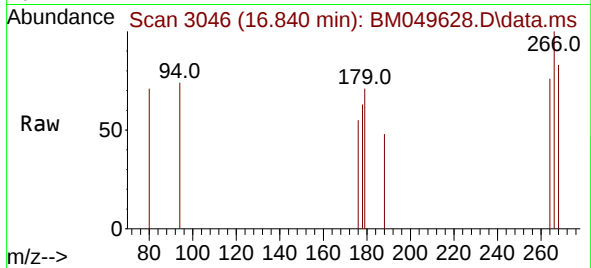

Tgt Ion:	266	Resp:	173
Ion	Ratio	Lower	Upper
266	100		
264	2.3	50.3	75.5
268	0.0	49.2	73.8

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 02/19/2025
 Supervised By :Jagrut Upadhyay 02/19/2025

