

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
 Data File : BM049646.D
 Acq On : 13 Feb 2025 12:58
 Operator : RC/JU
 Sample : Q1229-14
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E29C0

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 02/19/2025
 Supervised By :Jagrut Upadhyay 02/19/2025

Quant Time: Feb 17 14:27:26 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 12 16:40:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	9292	0.400	ng/ul	0.00
4) Naphthalene-d8	10.607	136	28760	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.447	164	17257	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.188	188	36728m	0.400	ng/ul	0.00
17) Chrysene-d12	21.368	240	26141m	0.400	ng/ul	0.00
23) Perylene-d12	23.657	264	25986m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.253	96	52312	5.004	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.196	152	13248	0.335	ng/ul	0.00
18) Fluoranthene-d10	19.216	212	32073m	0.403	ng/ul	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.842	266	6771m	0.899	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021225\
Data File : BM049646.D
Acq On : 13 Feb 2025 12:58
Operator : RC/JU
Sample : Q1229-14
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E29C0

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025


Quant Time: Feb 17 14:27:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

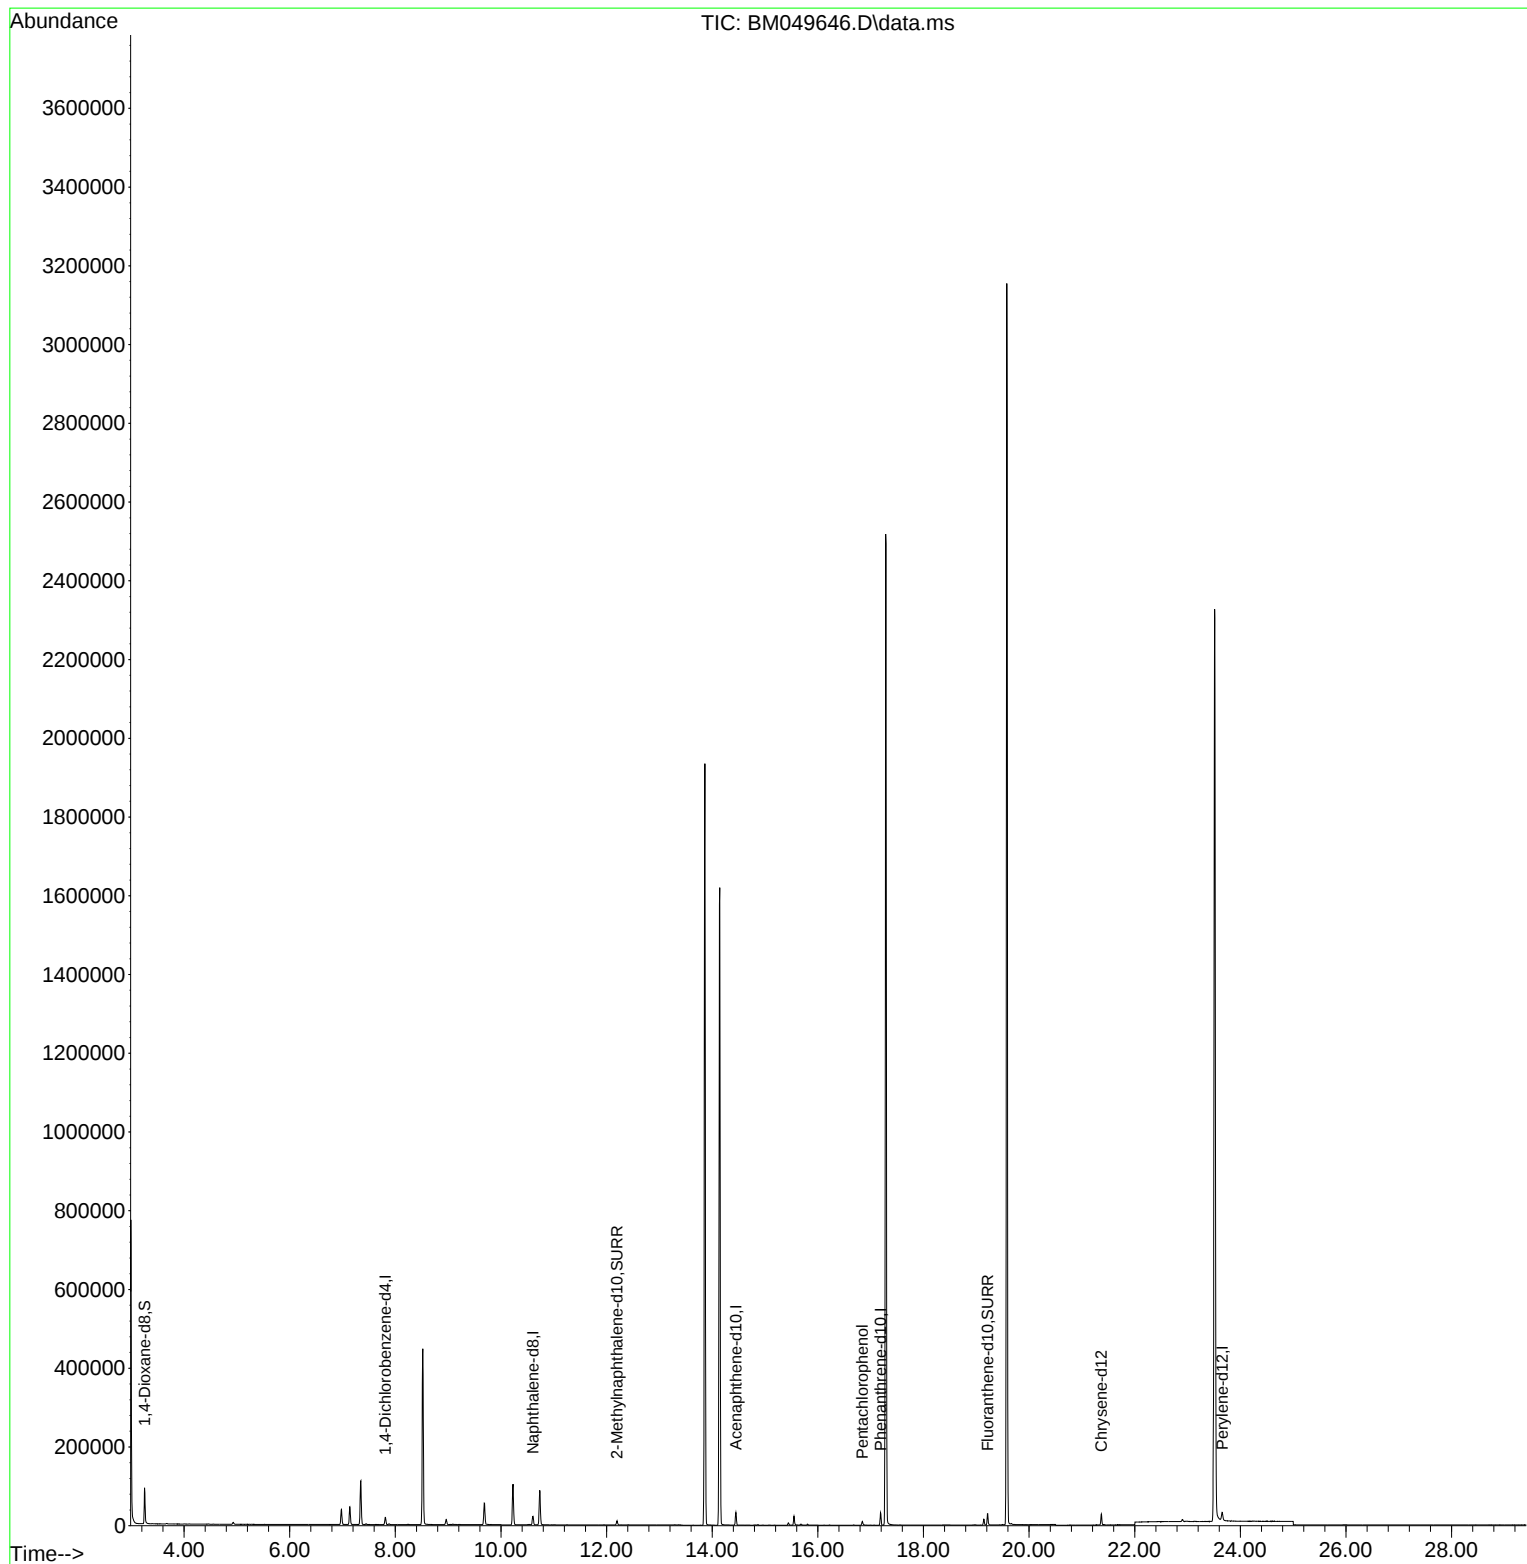

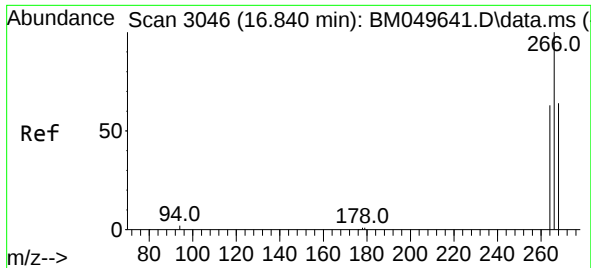

#14
Pentachlorophenol
Concen: 0.899 ng/ul m
RT: 16.842 min Scan# 30
Delta R.T. 0.002 min
Lab File: BM049646.D
Acq: 13 Feb 2025 12:58

Instrument :
BNA_M
ClientSampleId :
E29C0

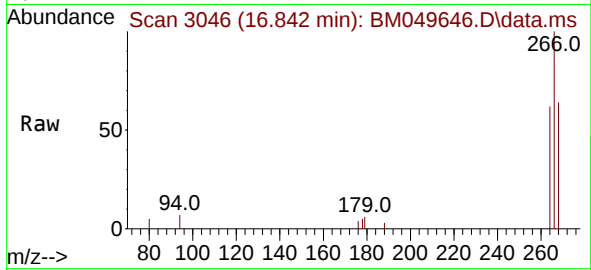

Tgt Ion:	266	Resp:	677
Ion	Ratio	Lower	Upper
266	100		
264	0.0	50.3	75.5
268	0.0	49.2	73.8

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

