


Data Path : Z:\HPCHEM1\BNA_M\Data\BM021315\
 Data File : BM000515.D
 Acq On : 13 Feb 2015 07:29
 Operator : TP/IZ
 Sample : DFTPP22
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP22

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM021215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 12 16:45:55 2015

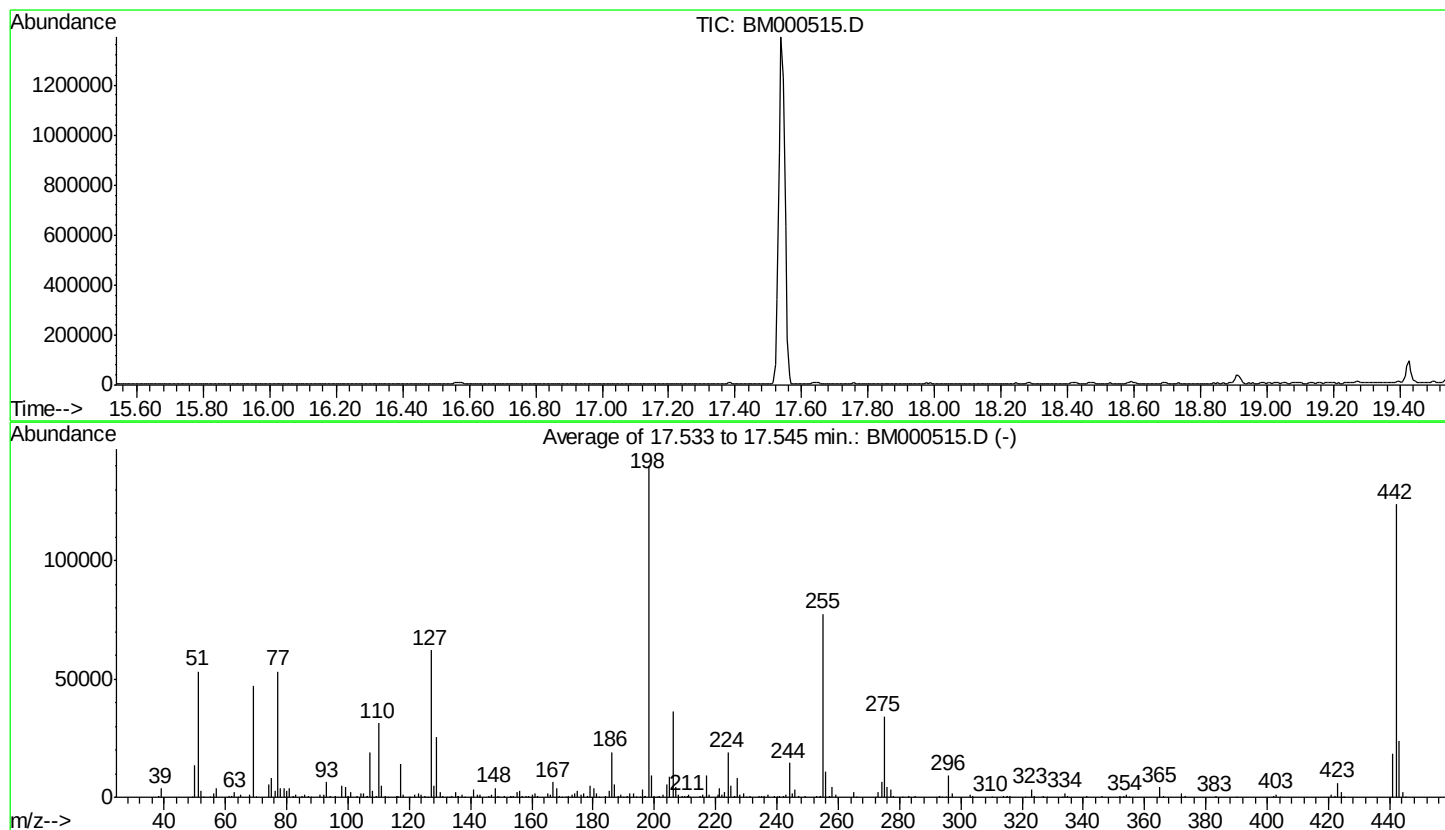

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	53261	PASS
68	69	0.00	2	2.0	920	PASS
69	198	0.00	100	33.7	47173	PASS
70	69	0.00	2	0.2	110	PASS
127	198	10	80	44.3	61997	PASS
197	198	0.00	2	0.5	680	PASS
198	198	100	100	100.0	140045	PASS
199	198	5	9	6.6	9268	PASS
275	198	10	60	24.1	33813	PASS
365	198	1	100	3.0	4253	PASS
441	443	0.01	100	77.6	18498	PASS
442	198	50	100	88.2	123557	PASS
443	442	15	24	19.3	23833	PASS