

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021318\
 Data File : BM014226.D
 Acq On : 13 Feb 2018 18:09
 Operator : SJ/JU
 Sample : J1518-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MW-1

Quant Time: Feb 14 04:58:35 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 07 17:16:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	103201	20.00	ng	0.00
21) Naphthalene-d8	10.31	136	425370	20.00	ng	0.00
38) Acenaphthene-d10	14.19	164	261428	20.00	ng	0.00
63) Phenanthrene-d10	16.95	188	688765	20.00	ng	0.00
75) Chrysene-d12	21.16	240	734797	20.00	ng	0.00
86) Perylene-d12	23.33	264	559340	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	423590	71.54	ng	0.00
7) Phenol-d6	6.73	99	343548	40.97	ng	0.00
23) Nitrobenzene-d5	8.70	82	972712	102.14	ng	0.00
41) 2,4,6-Tribromophenol	15.70	330	545496	147.05	ng	0.00
44) 2-Fluorobiphenyl	12.80	172	2036392	97.24	ng	0.00
78) Terphenyl-d14	19.60	244	3923520	104.33	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021318\
Data File : BM014226.D
Acq On : 13 Feb 2018 18:09
Operator : SJ/JU
Sample : J1518-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-1

Quant Time: Feb 14 04:58:35 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 17:16:49 2018
Response via : Initial Calibration

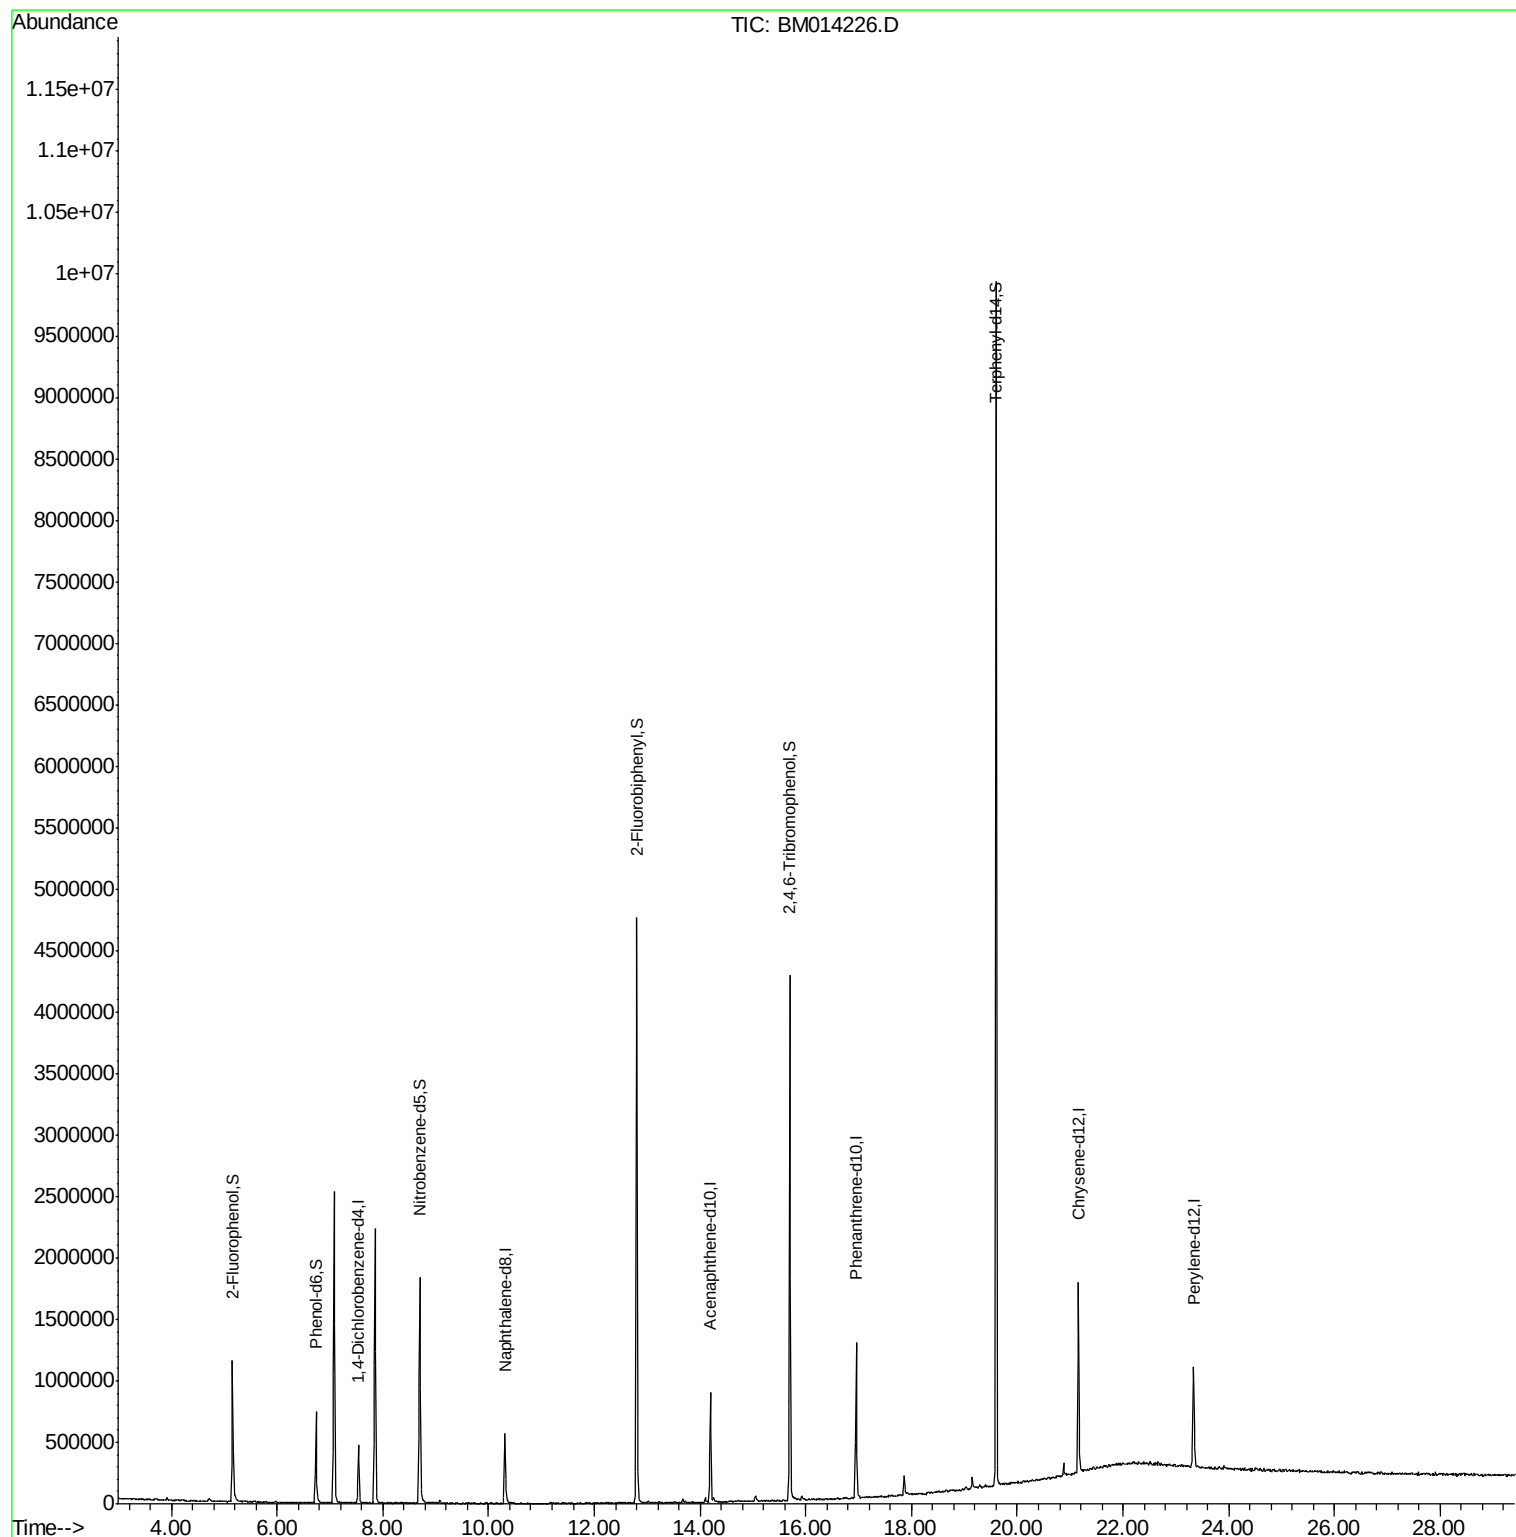

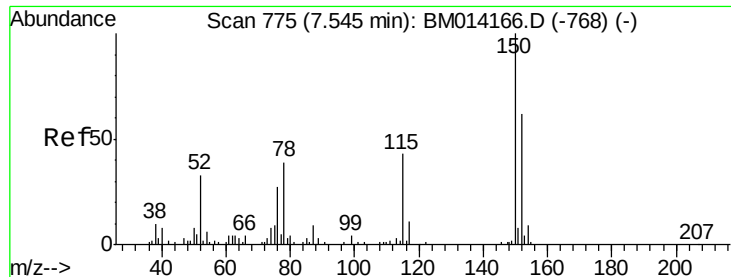


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.54 min Scan# 774
Delta R.T. -0.01 min
Lab File: BM014226.D
Acq: 13 Feb 2018 18:09

Instrument :
BNA_M
ClientSampleId :
MW-1

Tot Ion	Ratio	Lower	Upper
152	100		
150	148.2	119.5	179.3
115	60.8	43.0	64.4

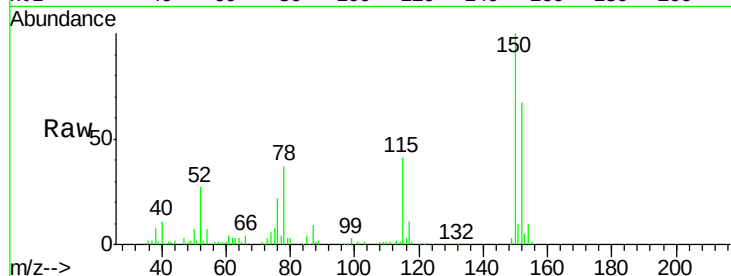


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

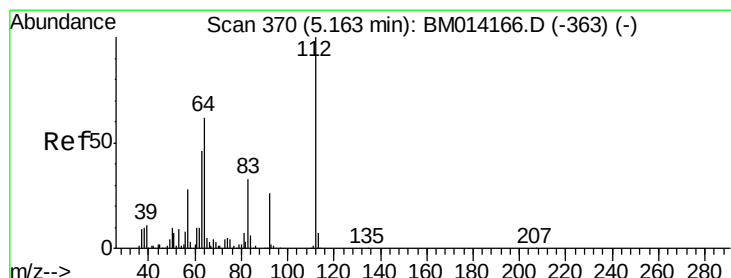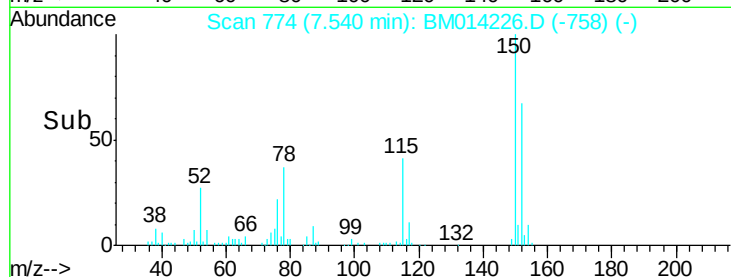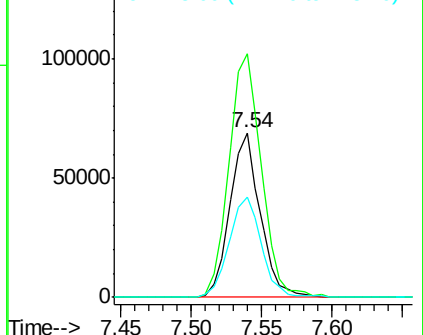



#5


2-Fluorophenol
Concen: 71.541 ng
RT: 5.16 min Scan# 369
Delta R.T. -0.01 min
Lab File: BM014226.D
Acq: 13 Feb 2018 18:09

Tgt Ion	Ratio	Lower	Upper
112	100		
64	62.5	38.6	57.8#
63	39.9	19.3	28.9#

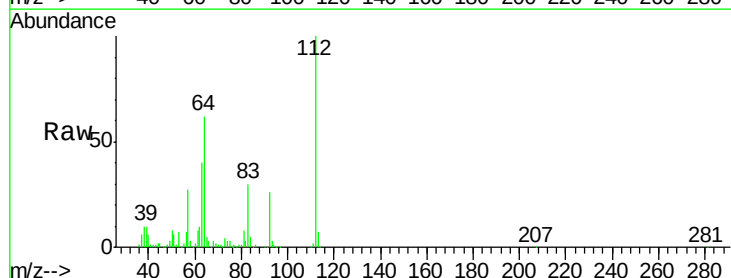

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

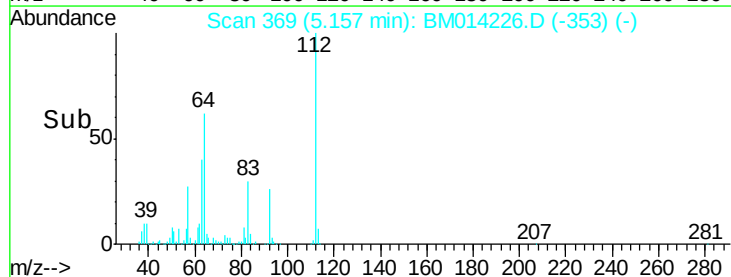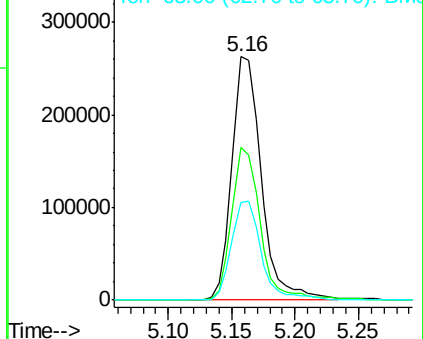

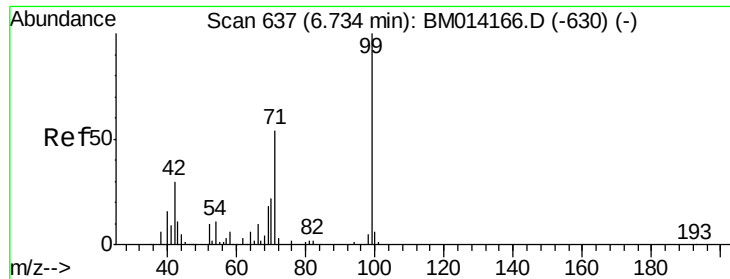

#7

Phenol-d6

Concen: 40.968 ng

RT: 6.73 min Scan# 637

Delta R.T. -0.01 min

Lab File: BM014226.D

Acq: 13 Feb 2018 18:09

Instrument :

BNA_M

ClientSampleId :

MW-1


Tot Ion: 99 Resp: 343548

Ion Ratio Lower Upper

99 100

42 27.3 11.0 16.4#

71 49.7 23.4 35.2#



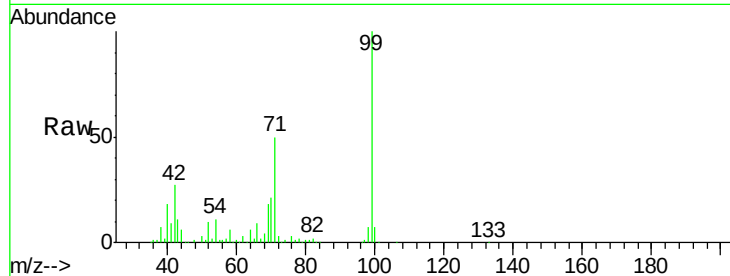


Abundance Ion 99.00 (98.70 to 99.70): BM014166.D (-630) (-)

Ion 42.00 (41.70 to 42.70): BM014166.D (-630) (-)

Ion 71.00 (70.70 to 71.70): BM014166.D (-630) (-)

Time-->

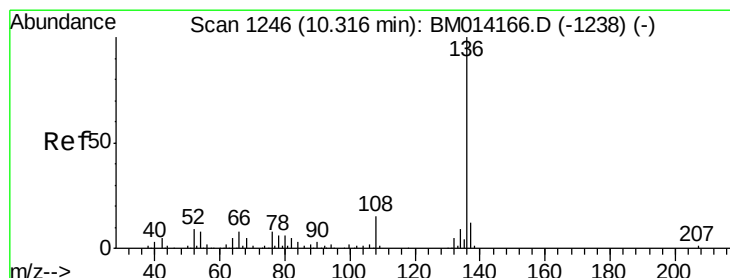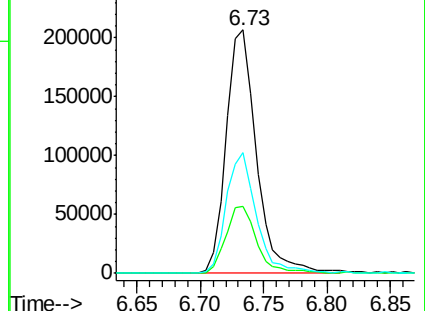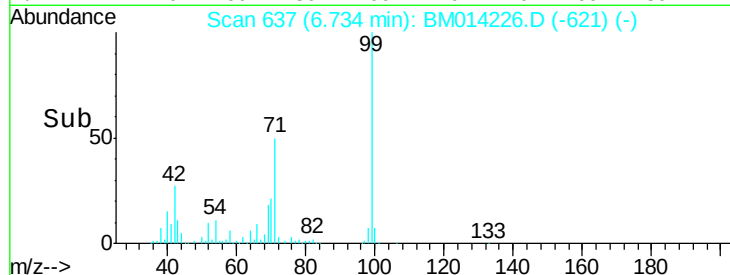

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.31 min Scan# 1245

Delta R.T. -0.01 min

Lab File: BM014226.D

Acq: 13 Feb 2018 18:09

Tgt Ion: 136 Resp: 425370


Ion Ratio Lower Upper

136 100

137 10.6 8.7 13.1

54 8.7 4.6 6.8#

68 5.0 3.7 5.5

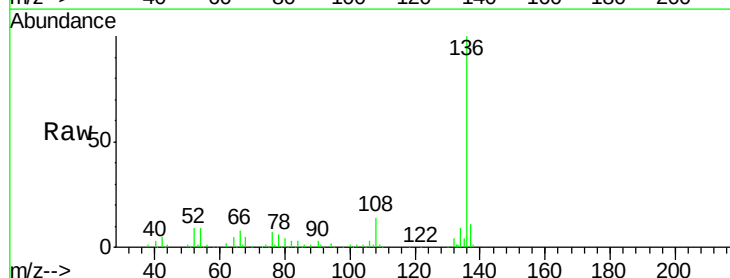



Abundance Ion 136.00 (135.70 to 136.70): BM014166.D (-1238) (-)


Ion 137.00 (136.70 to 137.70): BM014166.D (-1238) (-)

Ion 54.00 (53.70 to 54.70): BM014166.D (-1238) (-)

Ion 68.00 (67.70 to 68.70): BM014166.D (-1238) (-)

Time-->



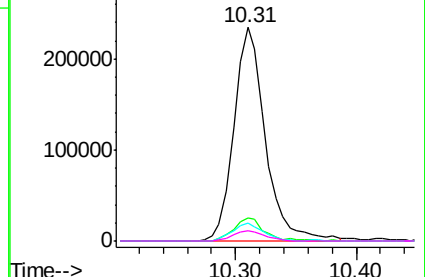
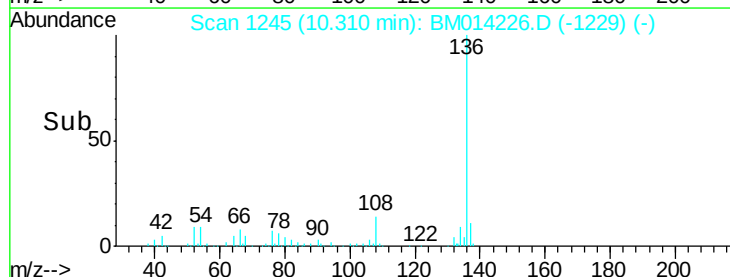


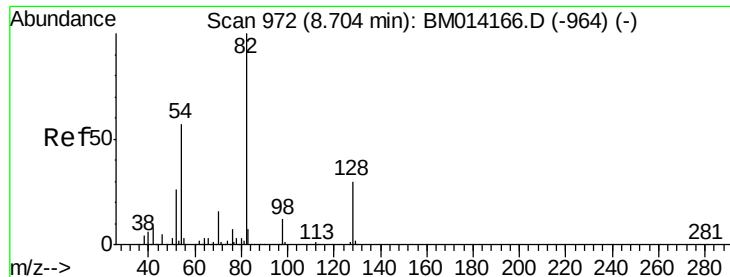

#23
 Nitrobenzene-d5
 Concen: 102.143 ng
 RT: 8.70 min Scan# 971
 Delta R.T. -0.01 min
 Lab File: BM014226.D
 Acq: 13 Feb 2018 18:09




Instrument :
 BNA_M
 ClientSampleId :
 MW-1


Tot Ion	82	Resp	972712
Ion Ratio	Lower	Upper	
82	100		
128	34.5	32.8	49.2
54	54.0	40.6	60.8

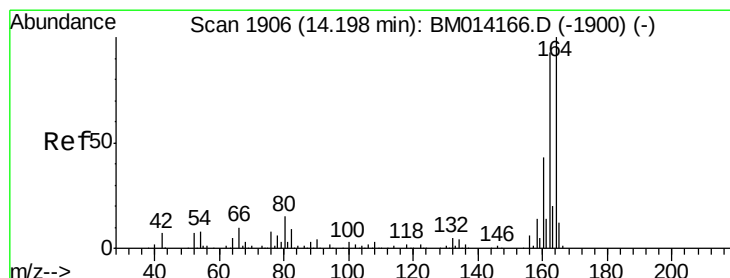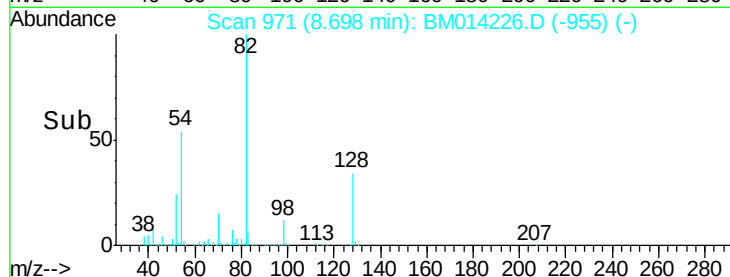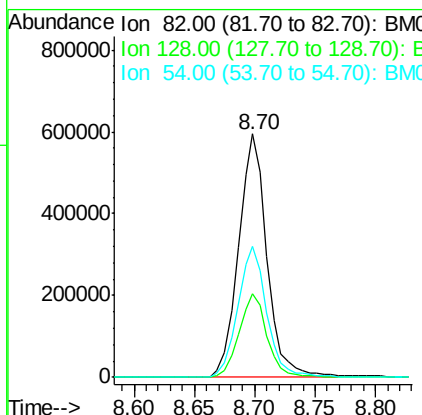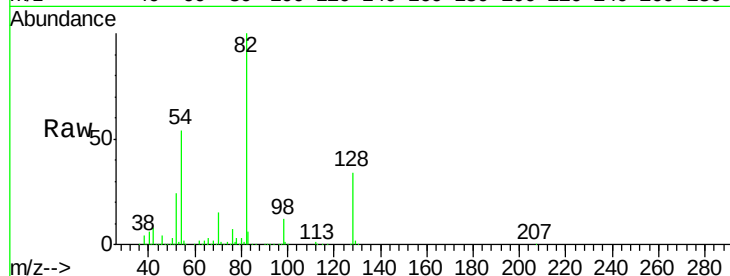

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.19 min Scan# 1905
 Delta R.T. -0.01 min
 Lab File: BM014226.D
 Acq: 13 Feb 2018 18:09

Tgt Ion	164	Resp	261428
Ion Ratio	Lower	Upper	
164	100		
162	109.6	82.4	123.6
160	52.2	35.8	53.6

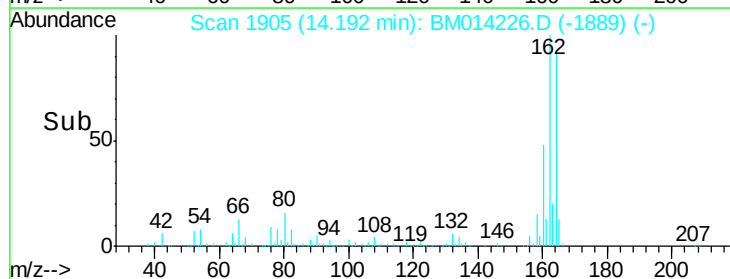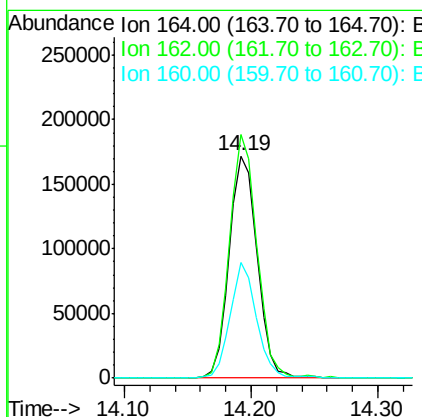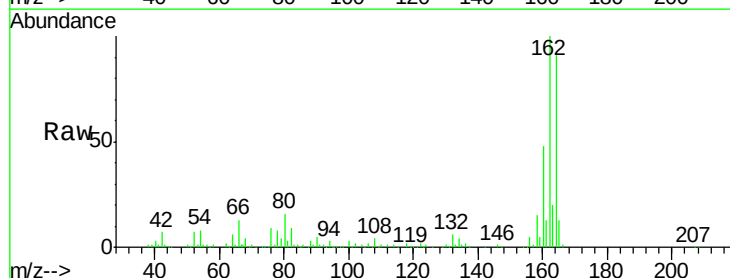


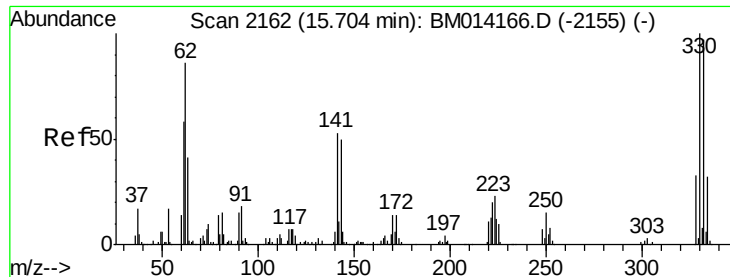




#41
 2,4,6-Tribromophenol
 Concen: 147.050 ng
 RT: 15.70 min Scan# 2161
 Delta R.T. -0.01 min
 Lab File: BM014226.D
 Acq: 13 Feb 2018 18:09

Instrument :
 BNA_M
 ClientSampled :
 MW-1

Tot Ion:330 Resp: 545496
 Ion Ratio Lower Upper
 330 100
 332 96.7 0.0 0.0#
 141 54.4 0.0 0.0#

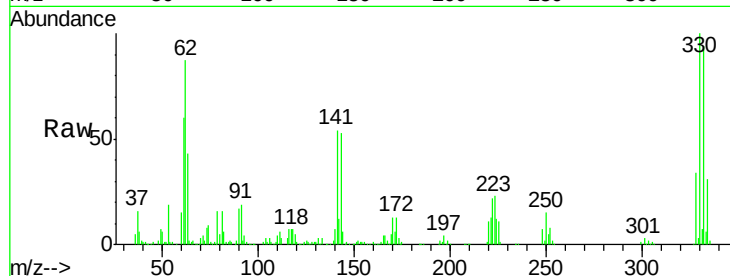


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

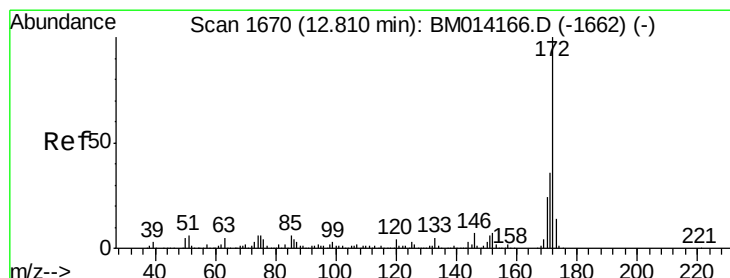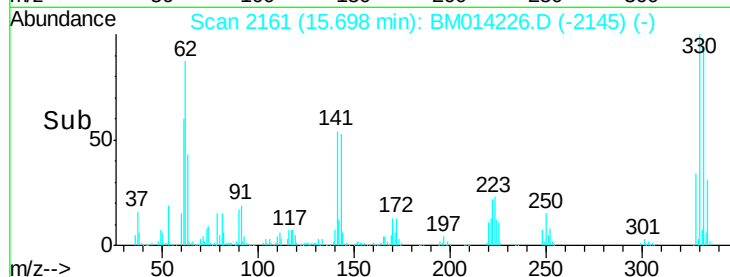
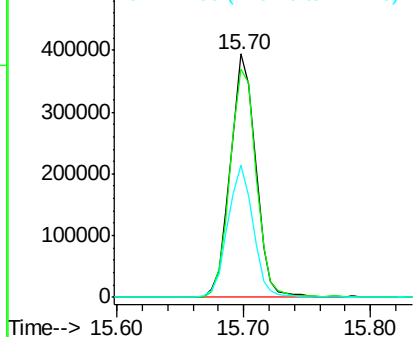



#44
 2-Fluorobiphenyl
 Concen: 97.237 ng
 RT: 12.80 min Scan# 1669
 Delta R.T. -0.01 min
 Lab File: BM014226.D
 Acq: 13 Feb 2018 18:09

Tgt Ion:172 Resp: 2036392
 Ion Ratio Lower Upper
 172 100
 171 34.3 28.5 42.7
 170 23.2 18.8 28.2

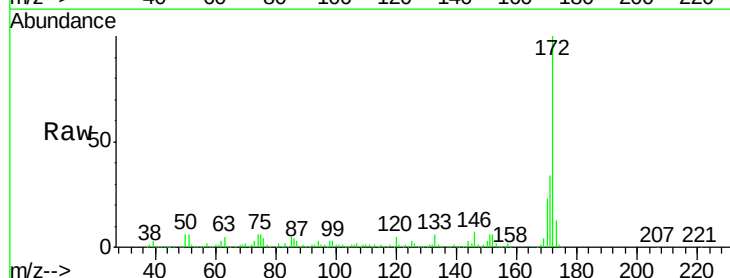

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



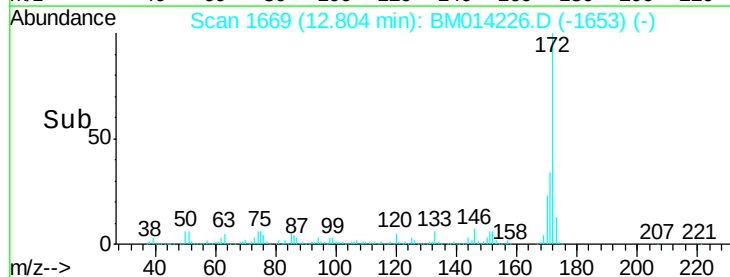
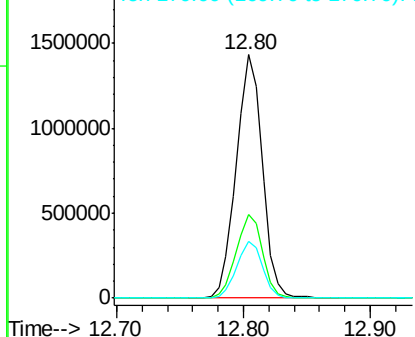


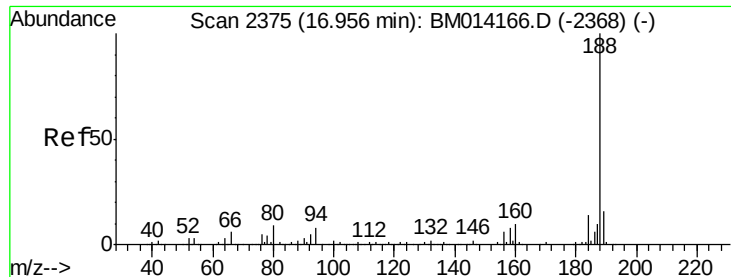

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.95 min Scan# 2374
Delta R.T. -0.01 min
Lab File: BM014226.D
Acq: 13 Feb 2018 18:09




Instrument :
BNA_M
ClientSampled :
MW-1


Tot Ion:188 Resp: 688765
Ion Ratio Lower Upper
188 100
94 7.7 8.7 13.1#
80 8.4 9.3 13.9#

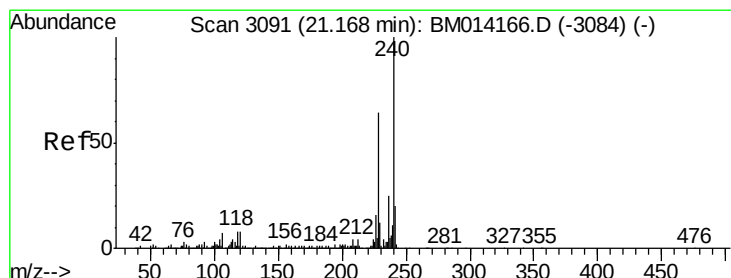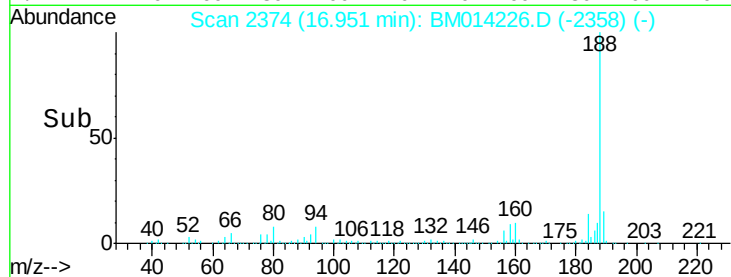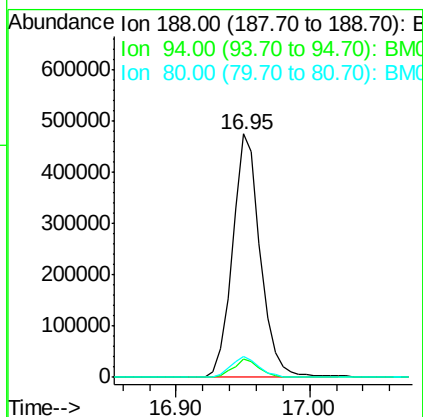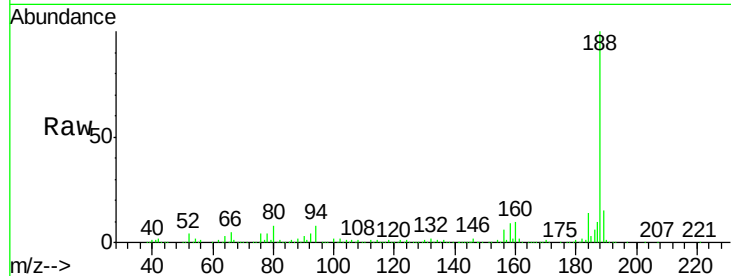

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.16 min Scan# 3090
Delta R.T. -0.01 min
Lab File: BM014226.D
Acq: 13 Feb 2018 18:09

Tgt Ion:240 Resp: 734797
Ion Ratio Lower Upper
240 100
120 7.2 8.2 12.2#
236 24.7 20.0 30.0

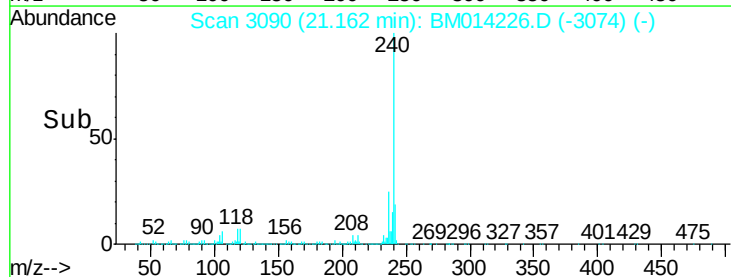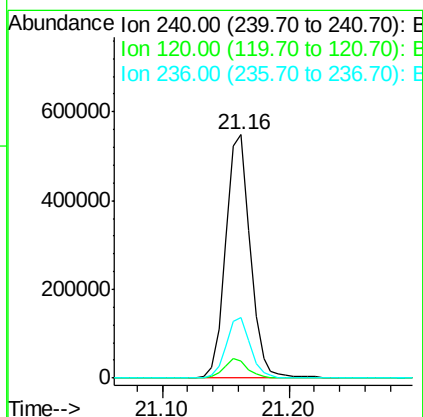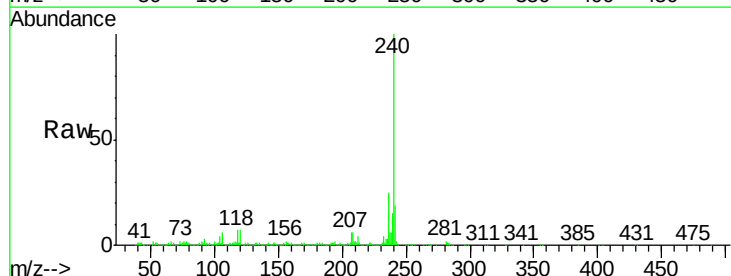

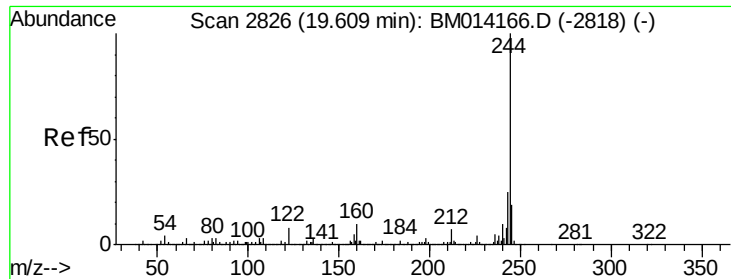

#78

Terphenyl-d14

Concen: 104.333 ng

RT: 19.60 min Scan# 2824

Delta R.T. -0.01 min

Lab File: BM014226.D

Acq: 13 Feb 2018 18:09

Instrument :

BNA_M

ClientSampleId :

MW-1


Tot Ion:244 Resp: 3923520

Ion Ratio Lower Upper

244 100

212 8.1 4.9 7.3#




122 9.5 6.2 9.4#

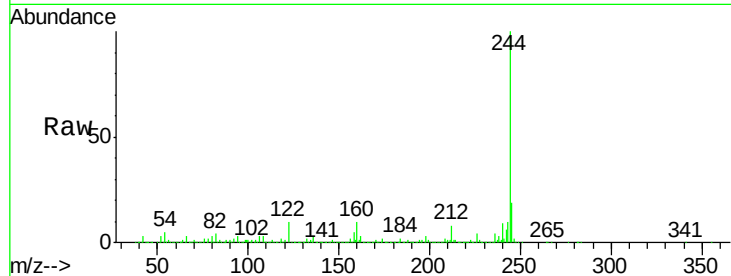

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

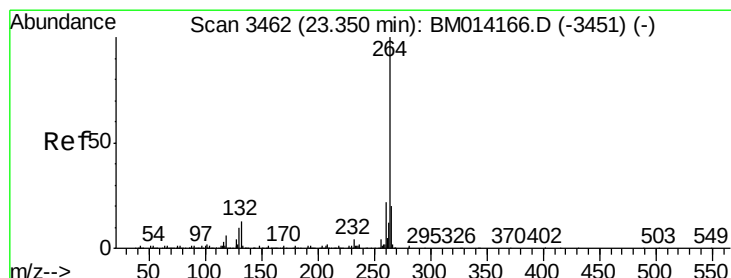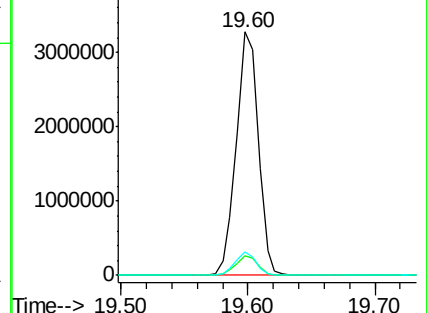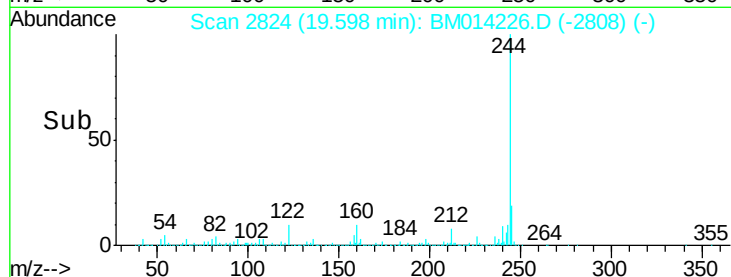

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.33 min Scan# 3459

Delta R.T. -0.01 min

Lab File: BM014226.D

Acq: 13 Feb 2018 18:09


Tgt Ion:264 Resp: 559340

Ion Ratio Lower Upper

264 100

260 22.3 18.6 27.8

265 20.6 17.3 25.9

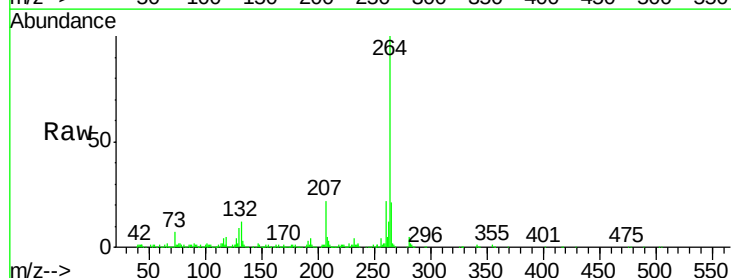

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

