

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021318\
Data File : BM014221.D
Acq On : 13 Feb 2018 15:09
Operator : SJ/JU
Sample : J1518-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-2A

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.163	365	370	377	rBV	209104	343920	30.69%	4.247%
2	6.734	632	637	653	rBV2	167836	351213	31.34%	4.337%
3	7.081	690	696	708	rBV	228404	405022	36.15%	5.002%
4	7.539	767	774	788	rBV	227341	397739	35.50%	4.912%
5	7.851	821	827	842	rVB2	168022	318355	28.41%	3.931%
6	8.716	967	974	986	rBV2	76671	200665	17.91%	2.478%
7	10.316	1236	1246	1263	rBV	222091	499669	44.59%	6.170%
8	12.810	1663	1670	1681	rBV	234422	484644	43.25%	5.985%
9	14.198	1898	1906	1918	rBV2	376053	685337	61.16%	8.463%
10	15.704	2156	2162	2177	rBV2	259636	534871	47.73%	6.605%
11	16.957	2368	2375	2391	rBV	492213	869493	77.60%	10.737%
12	19.598	2819	2824	2835	rBV	673930	917268	81.86%	11.327%
13	21.162	3084	3090	3100	rBV	717174	1120536	100.00%	13.838%
14	23.333	3453	3459	3470	rBV2	447705	969036	86.48%	11.967%


Sum of corrected areas: 8097768

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021318\
Data File : BM014221.D
Acq On : 13 Feb 2018 15:09
Operator : SJ/JU
Sample : J1518-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-2A

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

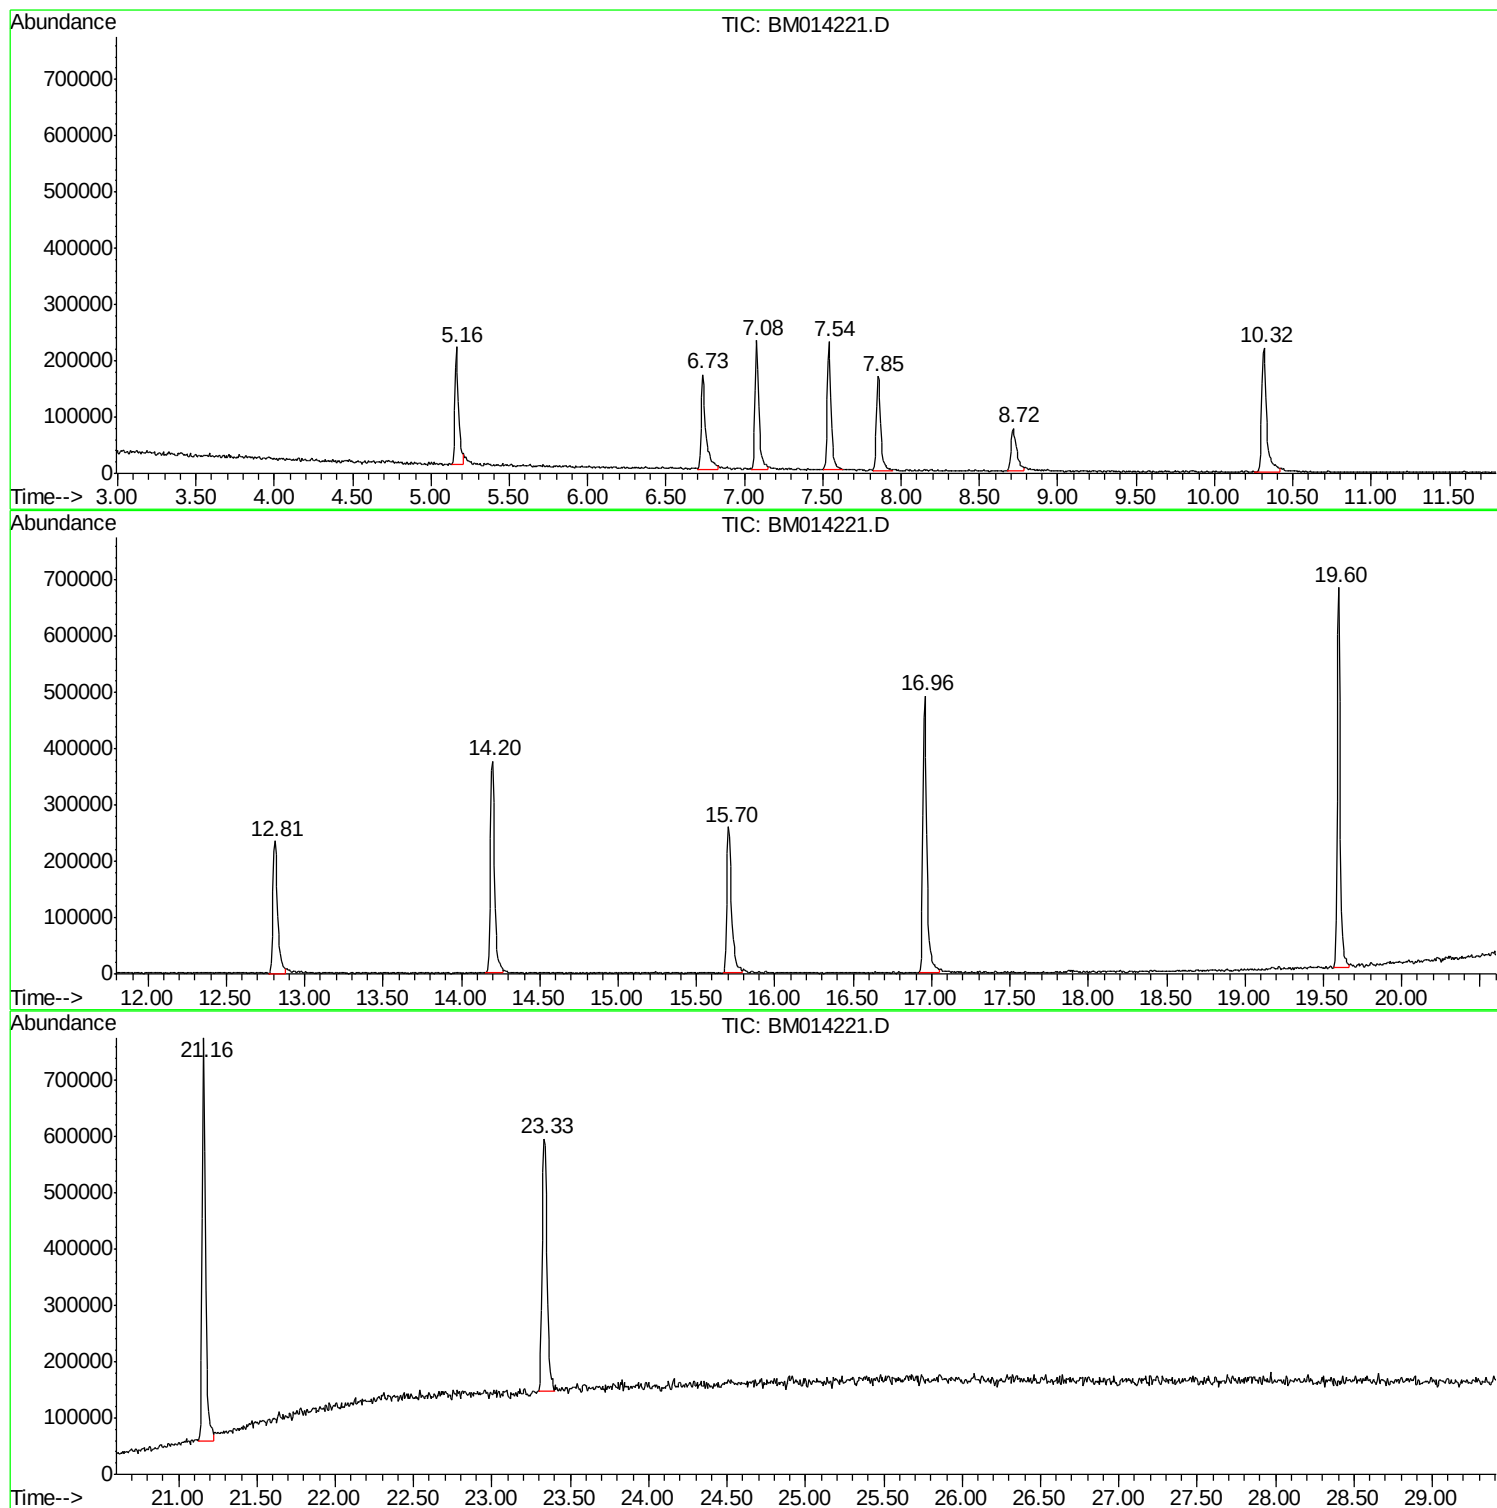

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021318\
Data File : BM014221.D
Acq On : 13 Feb 2018 15:09
Operator : SJ/JU
Sample : J1518-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-2A










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.08 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.08	20.37 ng	405022	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Acetic acid, trifluoro-, bicyclo...	208	C9H11F3O2	054934-98-4	25
2		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	22
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
4		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	10

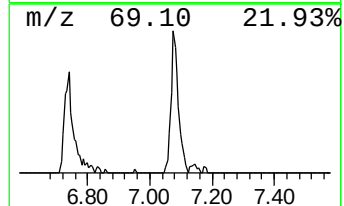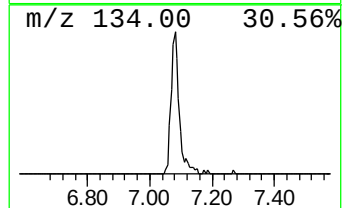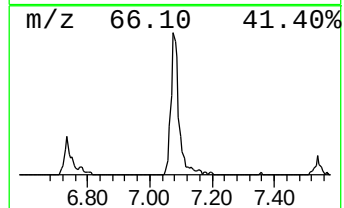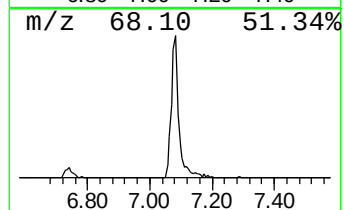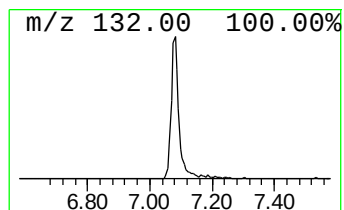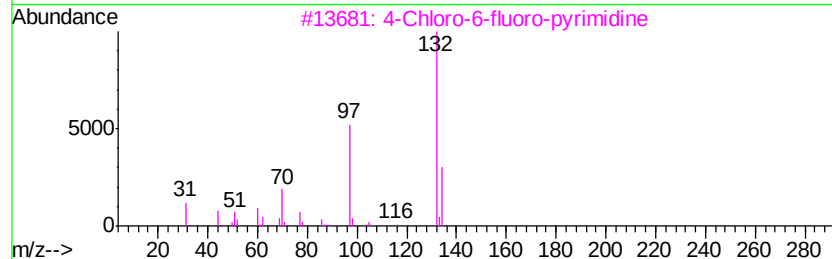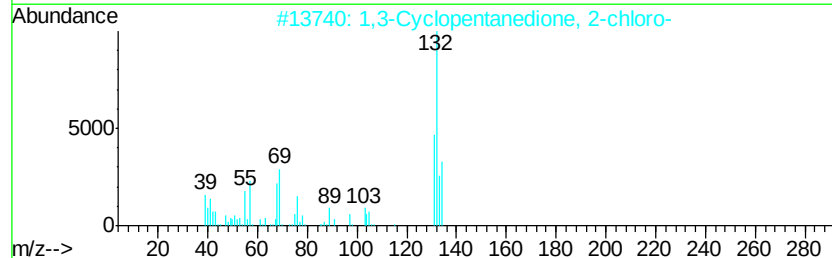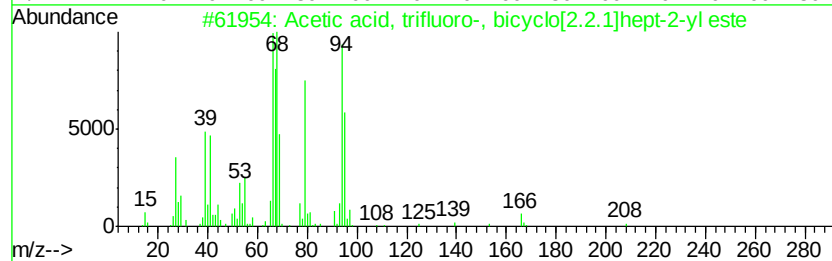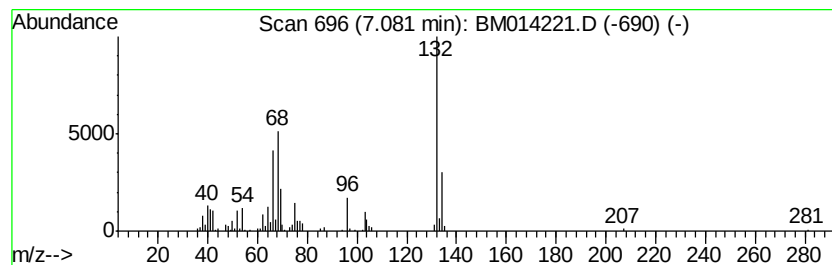

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021318\
Data File : BM014221.D
Acq On : 13 Feb 2018 15:09
Operator : SJ/JU
Sample : J1518-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-2A

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.08	7.08	20.4	ng	405022	1	7.54	397739	20.0