


Data Path : Z:\HPCHEM1\BNA M\Data\BM021318\
 Data File : BM014217.D
 Acq On : 13 Feb 2018 10:52
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 17:16:49 2018

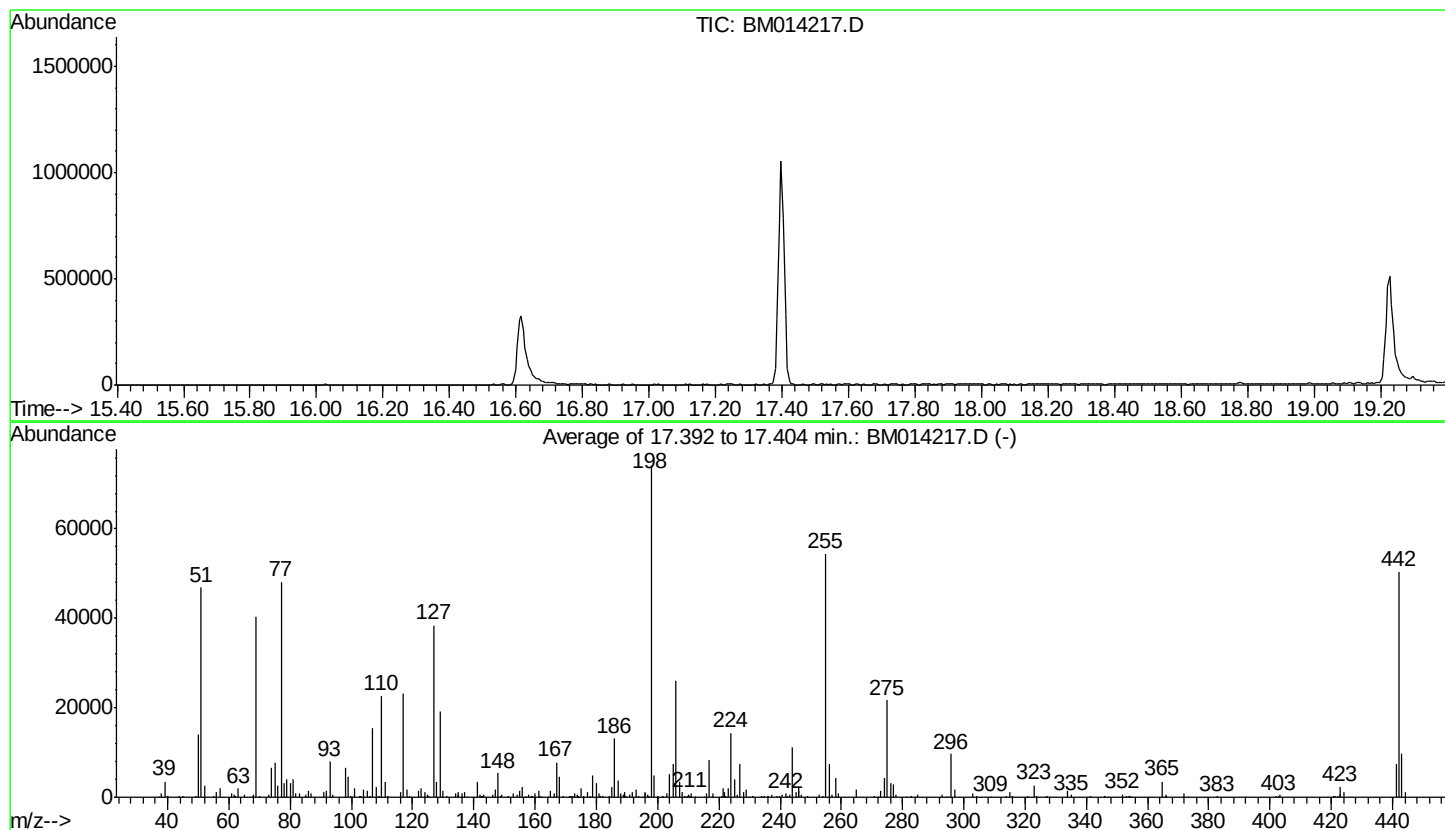

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.1	46842	PASS
68	69	0.00	2	1.8	727	PASS
69	198	0.00	100	54.6	40501	PASS
70	69	0.00	2	0.9	383	PASS
127	198	10	80	51.9	38514	PASS
197	198	0.00	2	0.7	496	PASS
198	198	100	100	100.0	74178	PASS
199	198	5	9	6.5	4785	PASS
275	198	10	60	29.2	21677	PASS
365	198	1	100	4.8	3572	PASS
441	443	0.01	100	76.6	7377	PASS
442	198	50	100	68.0	50405	PASS
443	442	15	24	19.1	9629	PASS