
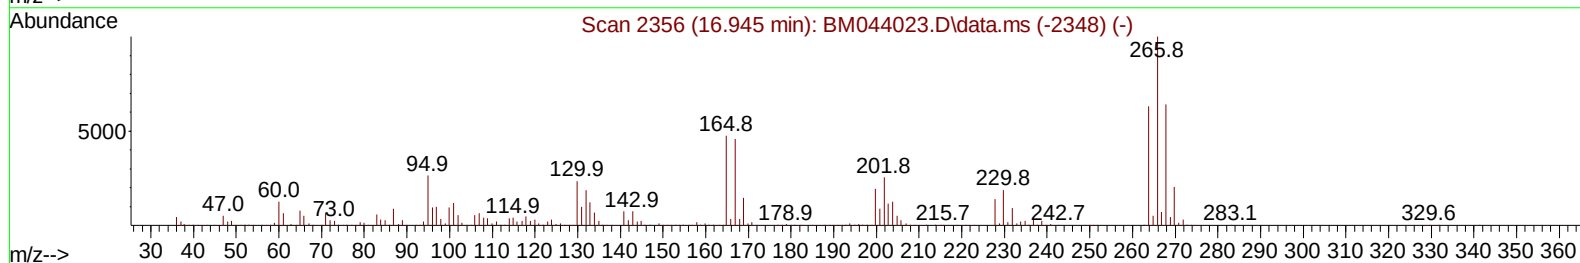
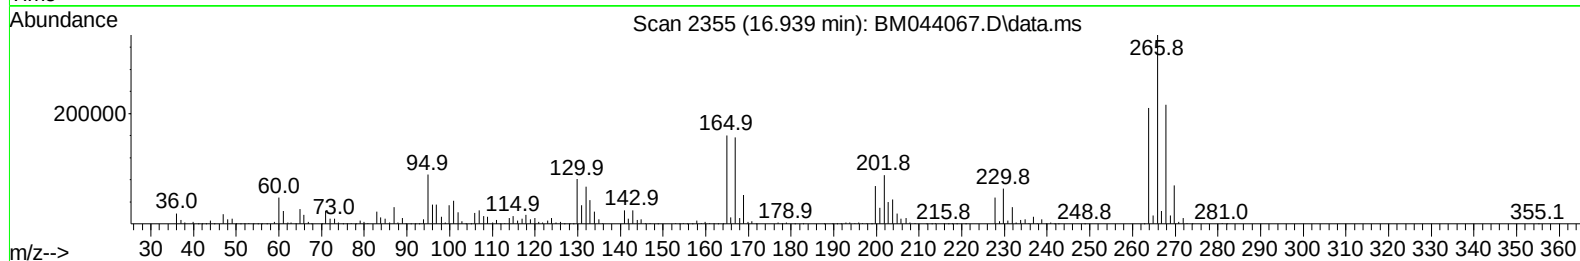


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021324\
Data File : BM044067.D
Acq On : 13 Feb 2024 14:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 01:08:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

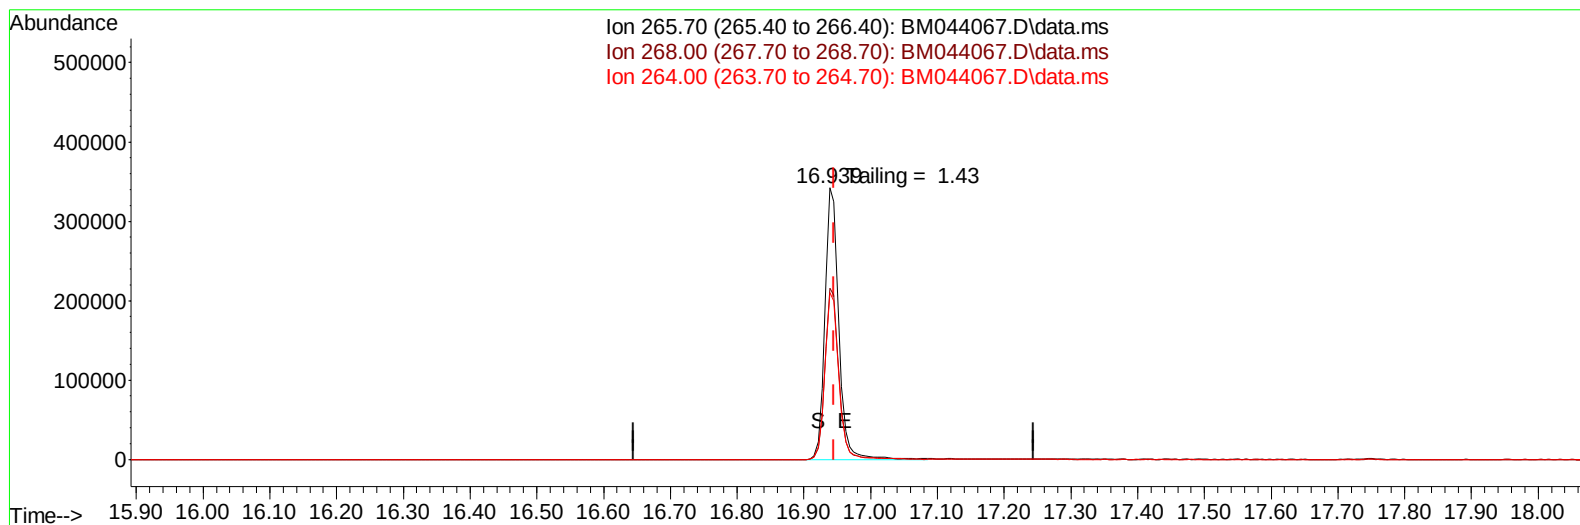

TIC: BM044067.D\data.ms

(70) Pentachlorophenol (C)




16.939min (-0.006) 146312.37 ng

response 500296

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.03
264.00	63.10	61.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021324\
Data File : BM044067.D
Acq On : 13 Feb 2024 14:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 01:08:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

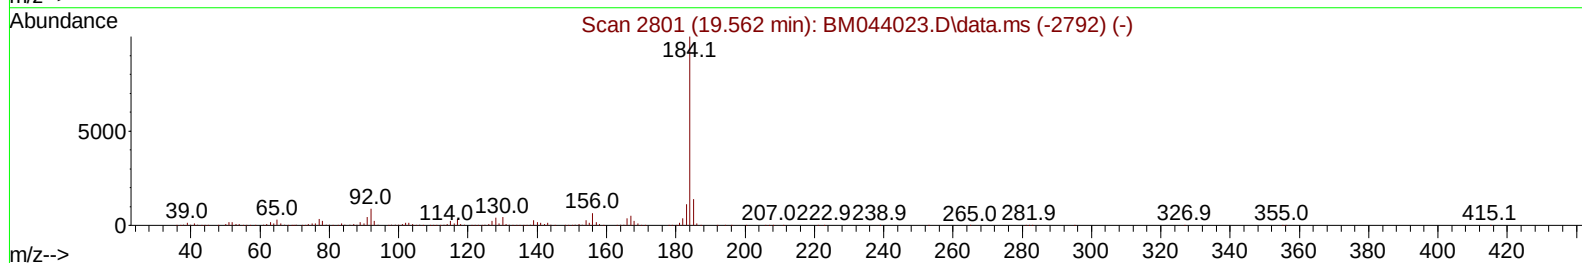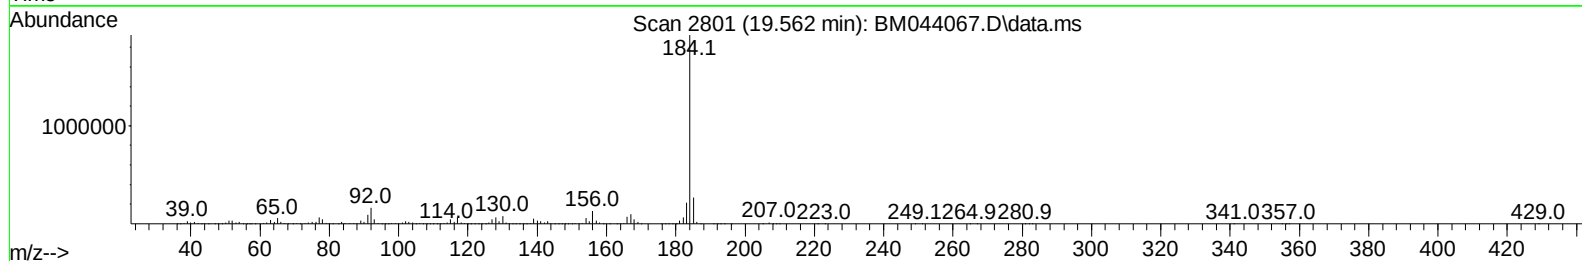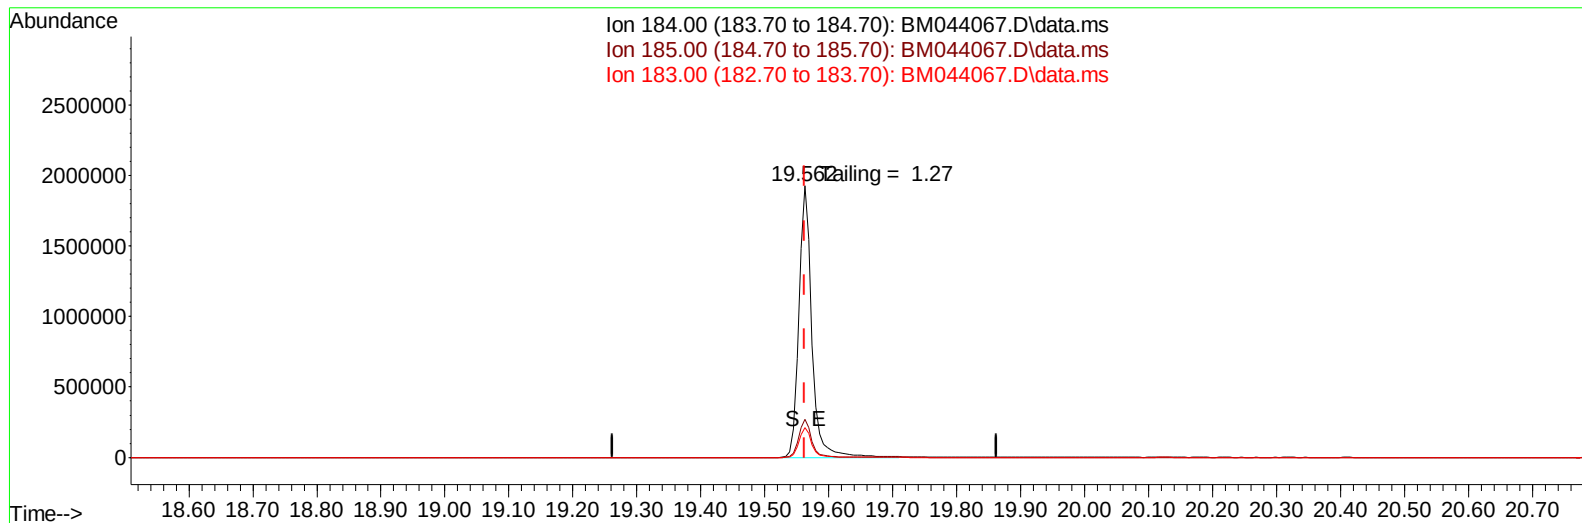

TIC: BM044067.D\data.ms

(77) Benzidine**19.562min (+ 0.000) 96798.96 ng****response 2743833**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.04
183.00	11.20	11.04
0.00	0.00	0.00