


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021324\
Data File : BM044067.D
Acq On : 13 Feb 2024 14:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 09 02:42:01 2024

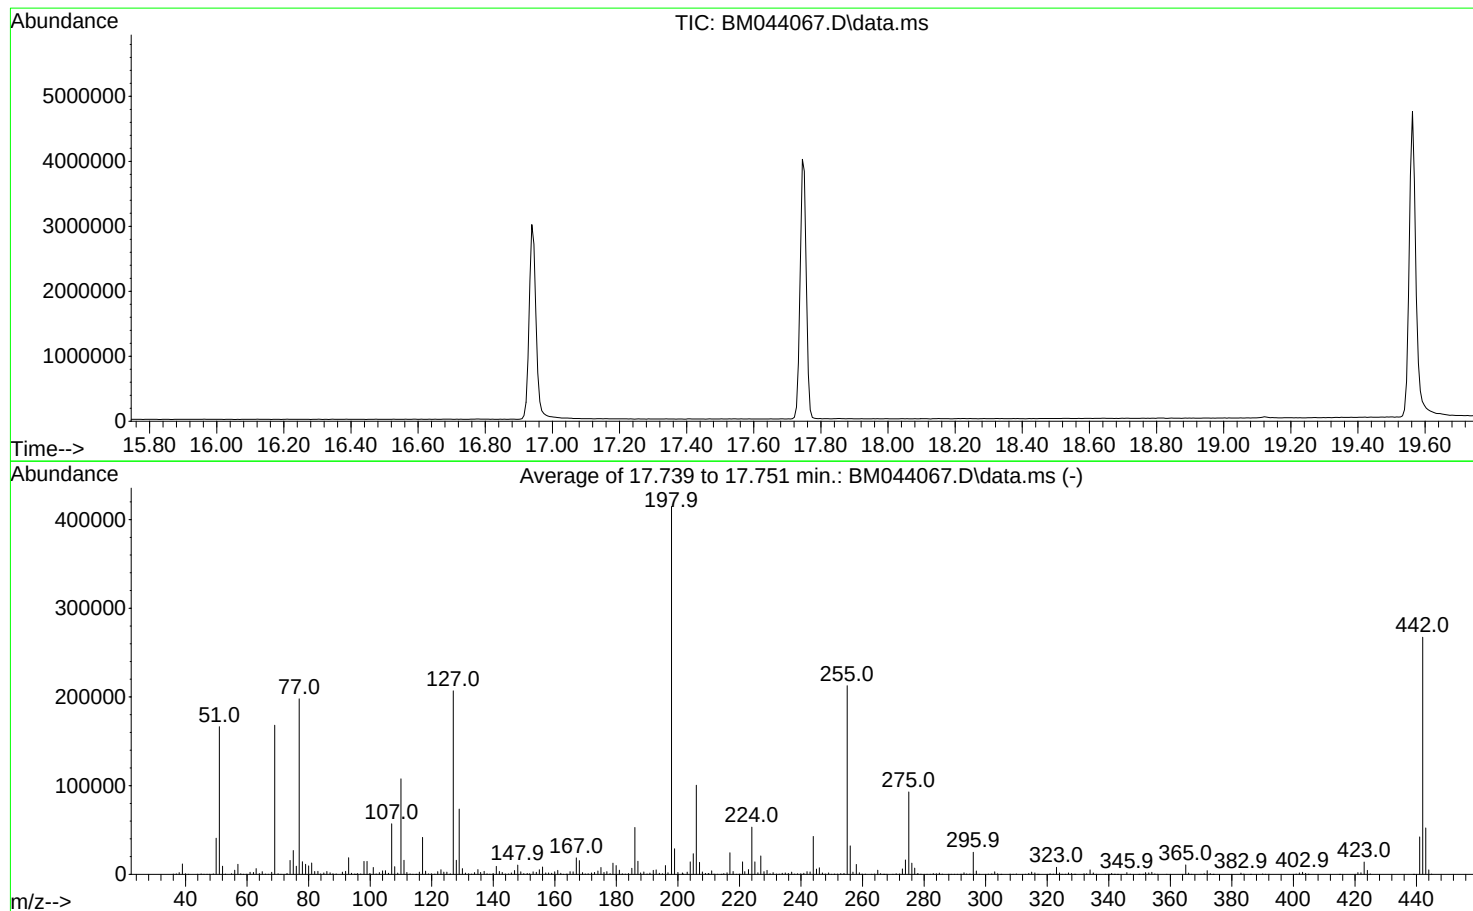




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	166484	PASS
68	69	0.00	2	1.4	2423	PASS
69	198	0.00	100	40.5	168149	PASS
70	69	0.00	2	0.5	816	PASS
127	198	10	80	49.9	206955	PASS
197	198	0.00	2	0.4	1751	PASS
198	198	100	100	100.0	414741	PASS
199	198	5	9	6.9	28811	PASS
275	198	10	60	22.4	92909	PASS
365	198	1	100	2.5	10571	PASS
441	198	0.01	100	10.2	42240	PASS
442	442	50	100	100.0	267435	PASS
443	442	15	24	19.6	52341	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021324\
Data File : BM044067.D
Acq On : 13 Feb 2024 14:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 14 01:08:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

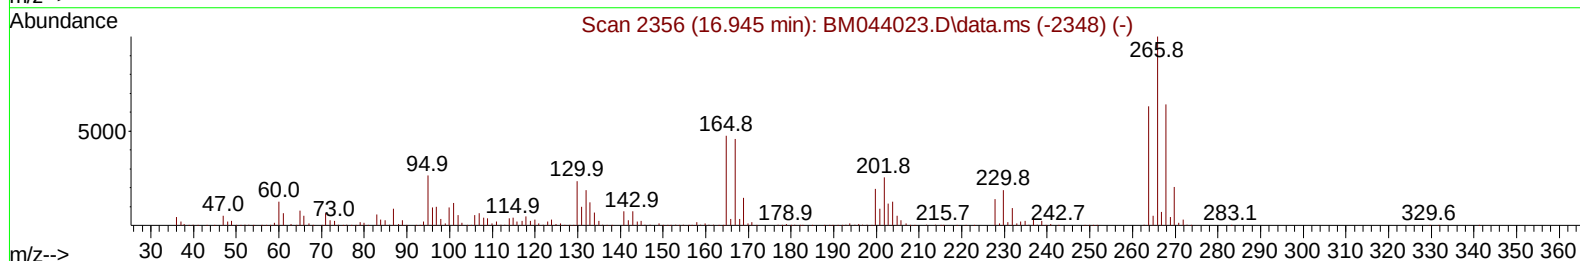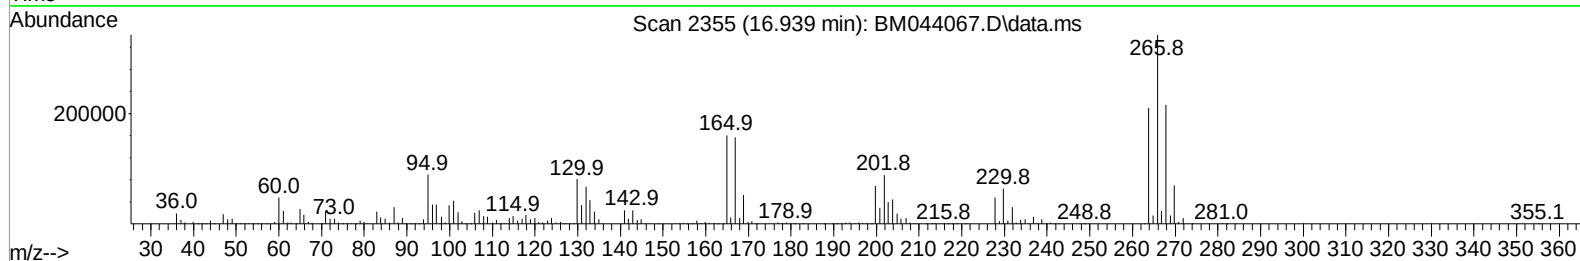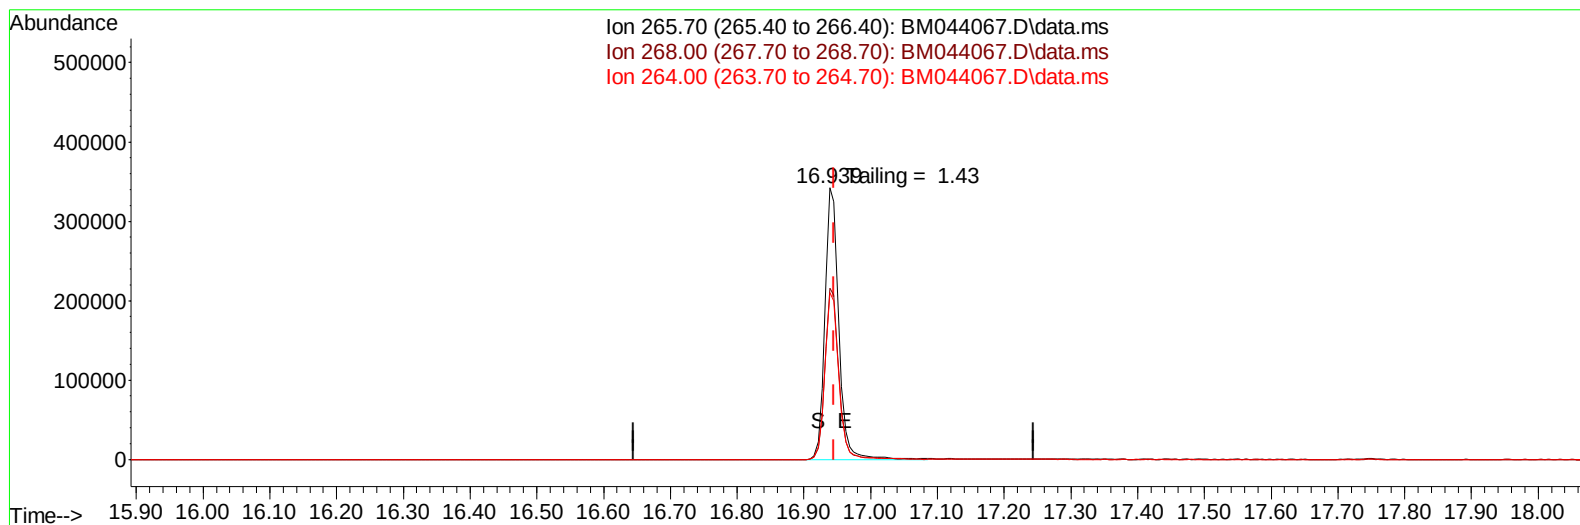

TIC: BM044067.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.006) 146312.37 ng




response 500296

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.03
264.00	63.10	61.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021324\
Data File : BM044067.D
Acq On : 13 Feb 2024 14:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 14 01:08:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

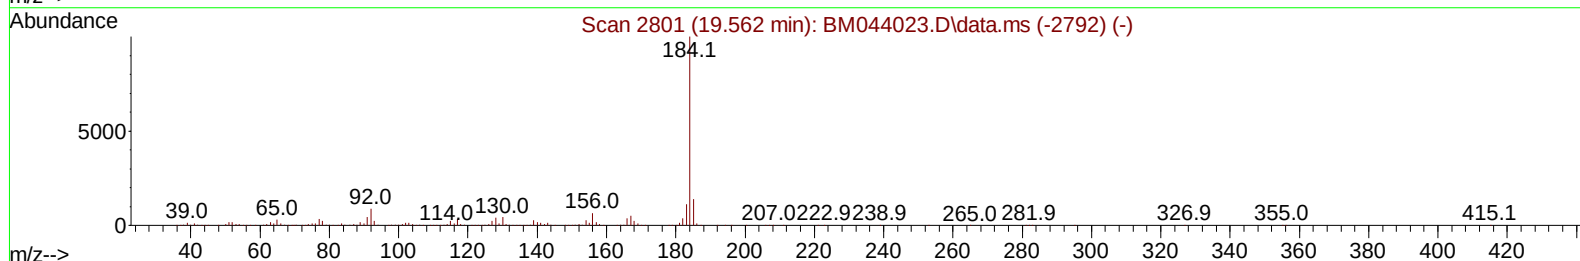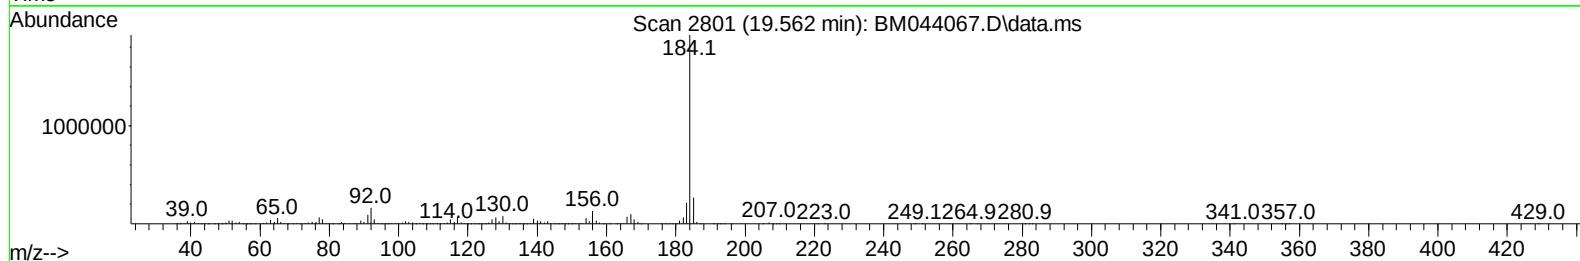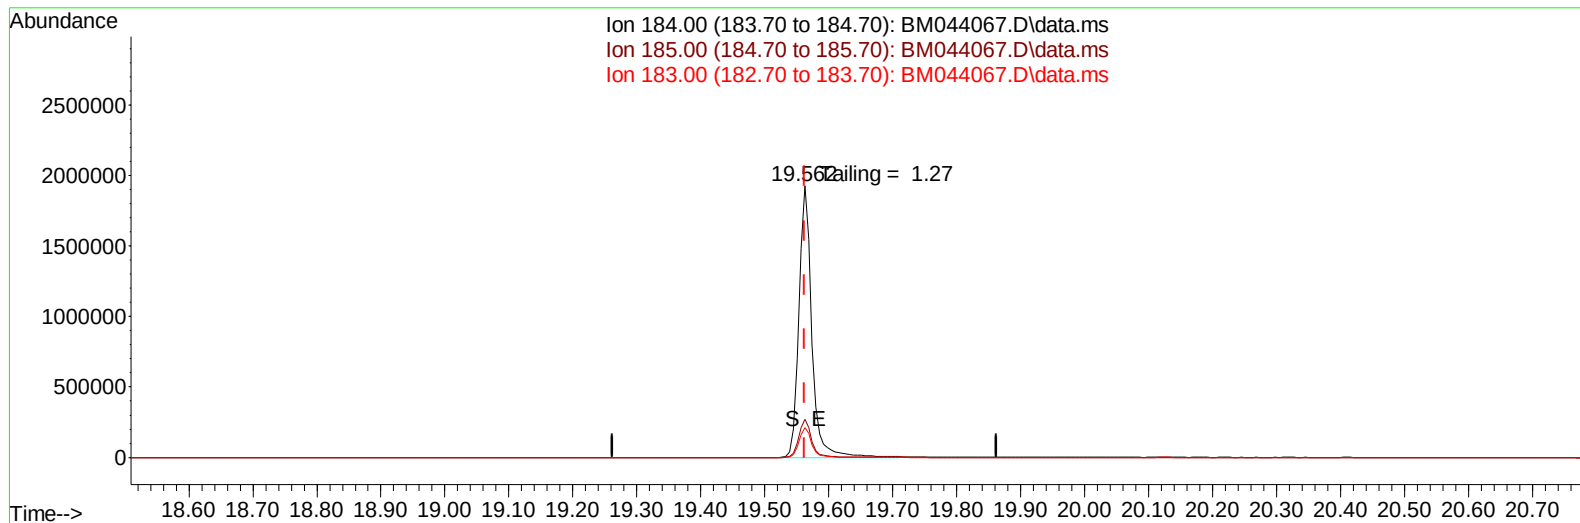

TIC: BM044067.D\data.ms

(77) Benzidine**19.562min (+ 0.000) 96798.96 ng****response 2743833**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.04
183.00	11.20	11.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/13/2024	BNA_M	<u>BM044067.D</u>
Compound Name	Response	Retention Time
DDT	1289562	20.797
DDD	19720	20.356
DDE	1242	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20962	1310524	1.60

Instrument :
BNA_M
ClientSampleId :
DFTPP