

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021418\
 Data File : BM014246.D
 Acq On : 14 Feb 2018 20:51
 Operator : SJ/JU
 Sample : J1553-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 15 01:14:07 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 15 01:12:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	70762	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	306954	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.19	164	204485	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.95	188	483095	20.00	ng/ul	0.00
75) Chrysene-d12	21.16	240	464611	20.00	ng/ul	0.00
83) Perylene-d12	23.33	264	420559	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.11	96	9768	5.91	ng/uL	0.00
5) Phenol-d5	6.73	99	32285	5.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	109968	30.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.07	132	110902	24.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	75409	14.41	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	75852	33.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	80497	34.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	107897	22.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.30	131	252	0.05	ng/ul	-0.16
43) Dimethylphthalate-d6	13.62	166	548926	32.51	ng/ul	0.00
46) Acenaphthylene-d8	13.88	160	702818	33.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	3128	1.34	ng/ul	0.07
57) Fluorene-d10	15.20	176	493073	32.59	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	71883	24.80	ng/ul	0.00
70) Anthracene-d10	16.95	188	483095	20.73	ng/ul	-0.10
76) Pyrene-d10	19.36	212	900954	37.60	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.33	264	407694	19.92	ng/ul	0.14
Target Compounds						
2) 1,4-Dioxane	3.15	88	5812	3.164	ng/uL#	72
21) Isophorone	9.41	82	12996	1.133	ng/ul#	77
45) 2,6-Dinitrotoluene	13.62	165	4115	1.301	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021418\
Data File : BM014246.D
Acq On : 14 Feb 2018 20:51
Operator : SJ/JU
Sample : J1553-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 15 01:14:07 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 15 01:12:03 2018
Response via : Initial Calibration

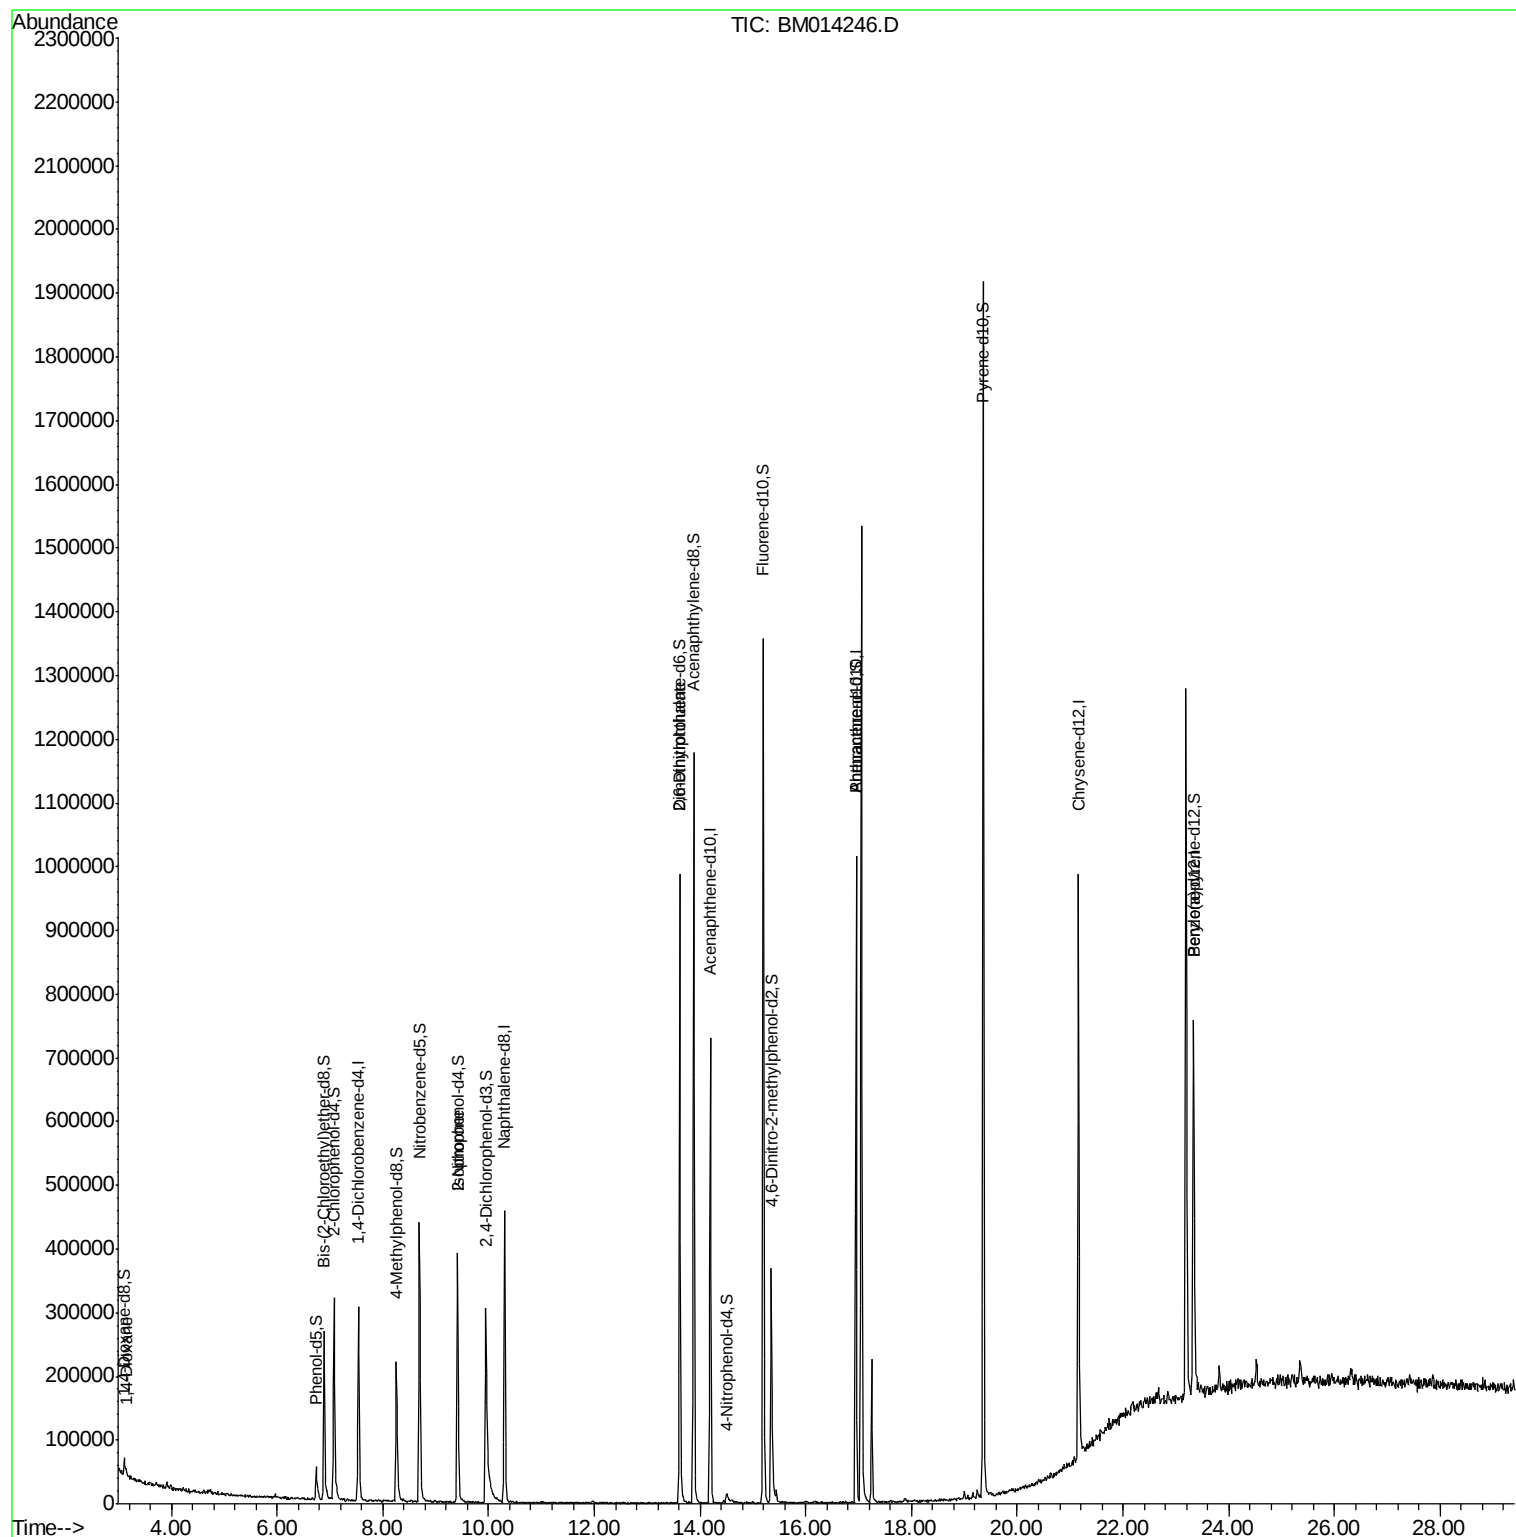

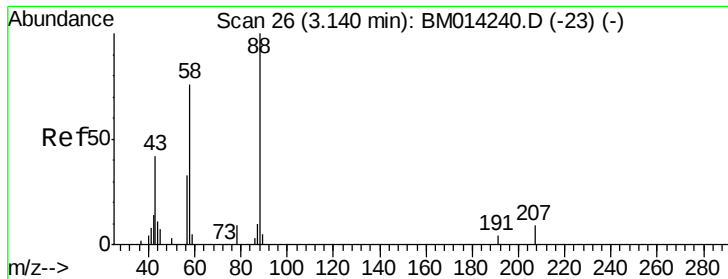

#2

1,4-Dioxane

Concen: 3.164 ng/uL

RT: 3.15 min Scan# 27

Delta R.T. 0.01 min

Lab File: BM014246.D

Acq: 14 Feb 2018 20:51

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 88 Resp: 5812

Ion Ratio Lower Upper

88 100

43 47.3 48.0 72.0#




58 65.1 80.0 120.0#

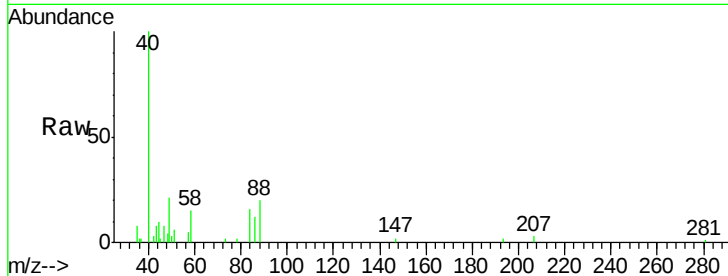

Abundance Ion 88.00 (87.70 to 88.70): BM014246.D (-23) (-)

Ion 43.00 (42.70 to 43.70): BM014246.D (-23) (-)

Ion 58.00 (57.70 to 58.70): BM014246.D (-23) (-)

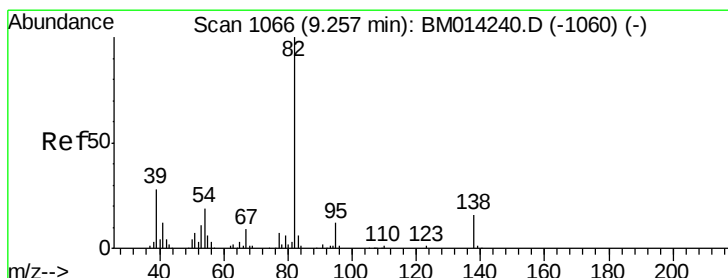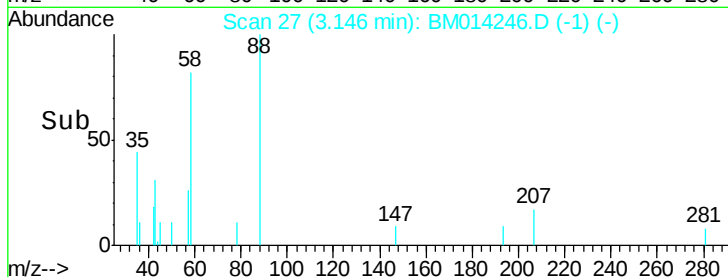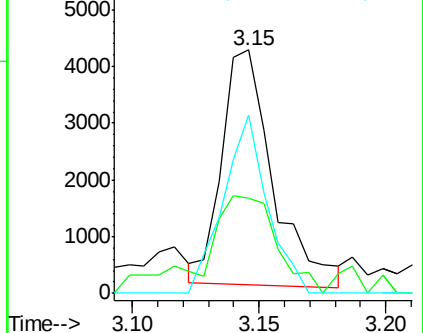

#21

Isophorone

Concen: 1.133 ng/uL

RT: 9.41 min Scan# 1092

Delta R.T. 0.15 min

Lab File: BM014246.D

Acq: 14 Feb 2018 20:51


Tgt Ion: 82 Resp: 12996

Ion Ratio Lower Upper

82 100

95 8.9 7.8 11.8



138 0.0 11.9 17.9#



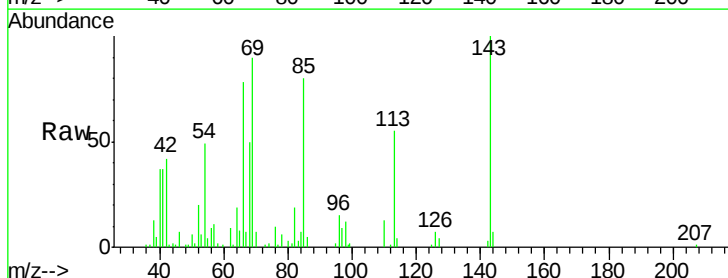


Abundance Ion 82.00 (81.70 to 82.70): BM014246.D (-1060) (-)

Ion 95.00 (94.70 to 95.70): BM014246.D (-1060) (-)

Ion 138.00 (137.70 to 138.70): BM014246.D (-1060) (-)

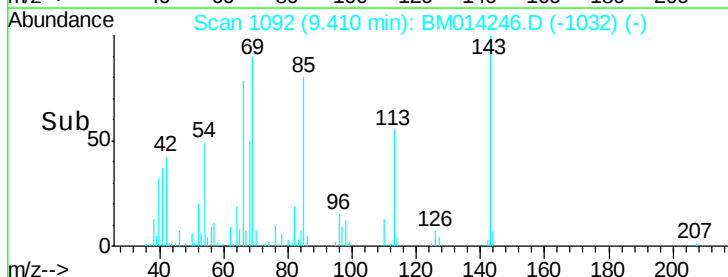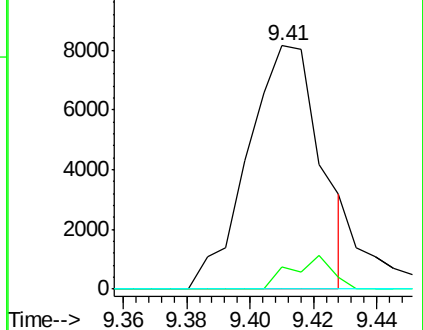

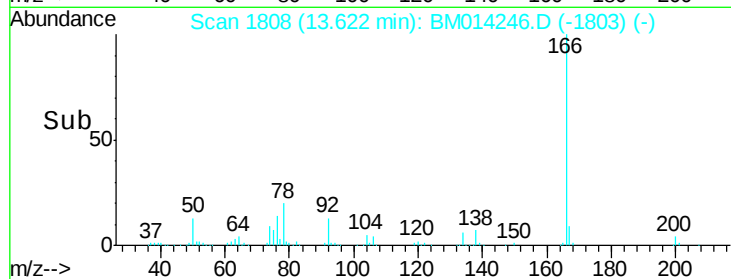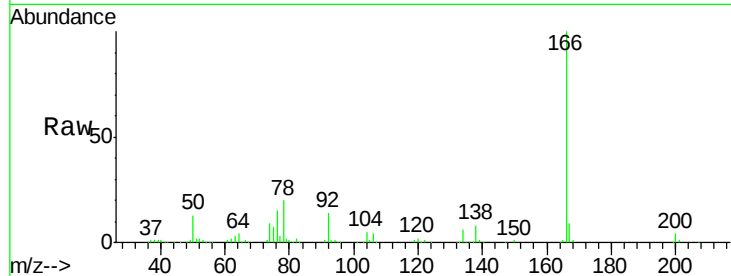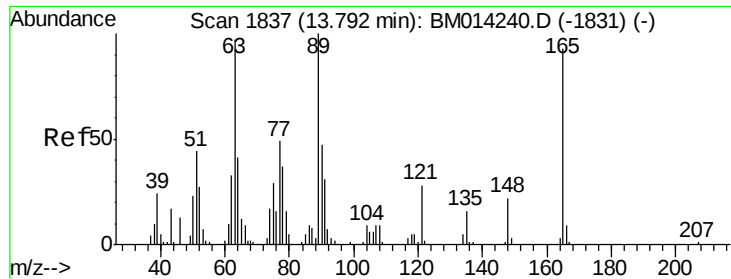

#45

2,6-Dinitrotoluene

Concen: 1.301 ng/ul

RT: 13.62 min Scan# 1808

Delta R.T. -0.17 min

Lab File: BM014246.D

Acq: 14 Feb 2018 20:51

Instrument :

BNA_M

ClientSampleId :

Tot Ion:165 Resp: 4115

Ion Ratio Lower Upper

165 100

89 0.0 52.6 79.0#

121 15.5 14.6 22.0

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

