


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021423\
Data File : BM038723.D
Acq On : 14 Feb 2023 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 15 02:07:17 2023

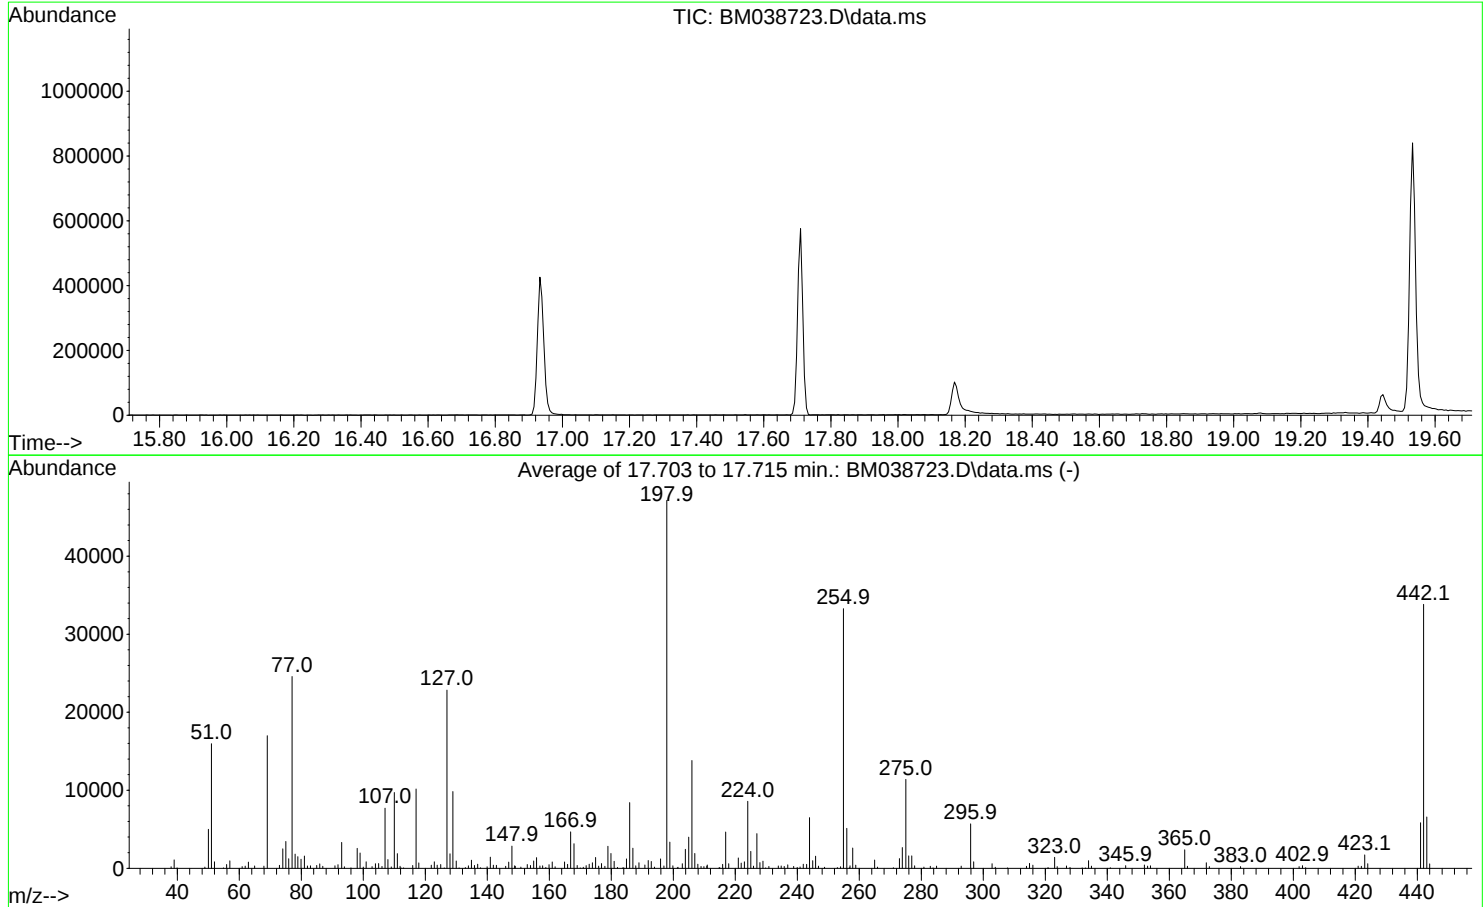




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	15971	PASS
68	69	0.00	2	1.6	280	PASS
69	198	0.00	100	36.0	16986	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.4	22841	PASS
197	198	0.00	2	0.6	293	PASS
198	198	100	100	100.0	47147	PASS
199	198	5	9	7.1	3359	PASS
275	198	10	60	24.2	11400	PASS
365	198	1	100	5.0	2374	PASS
441	198	0.01	100	12.4	5827	PASS
442	442	50	100	100.0	33827	PASS
443	442	15	24	19.4	6575	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021423\
Data File : BM038723.D
Acq On : 14 Feb 2023 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 15 04:39:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 15 02:07:17 2023
Response via : Initial Calibration

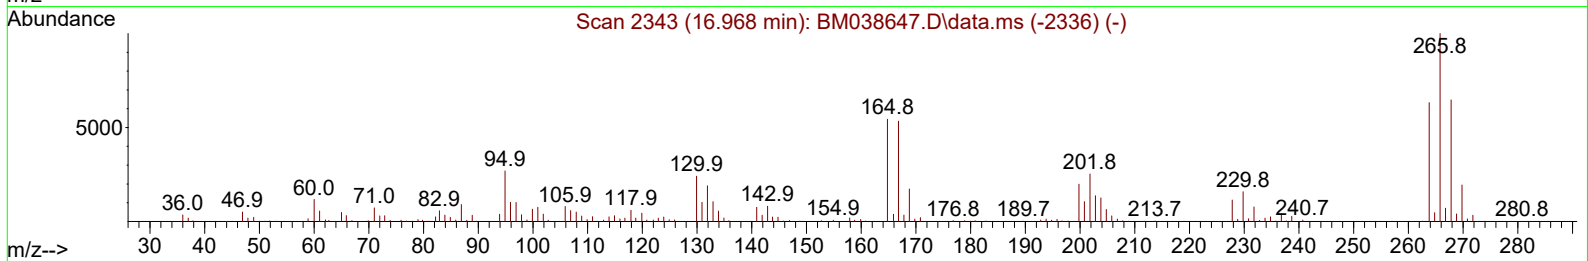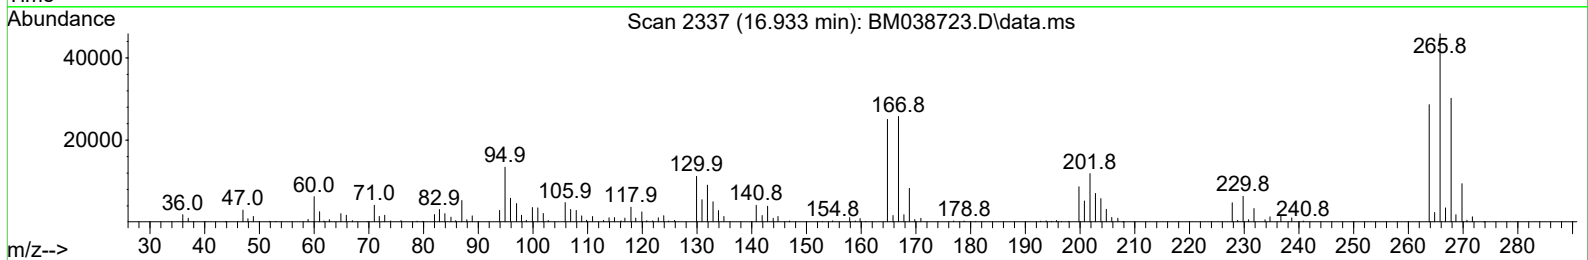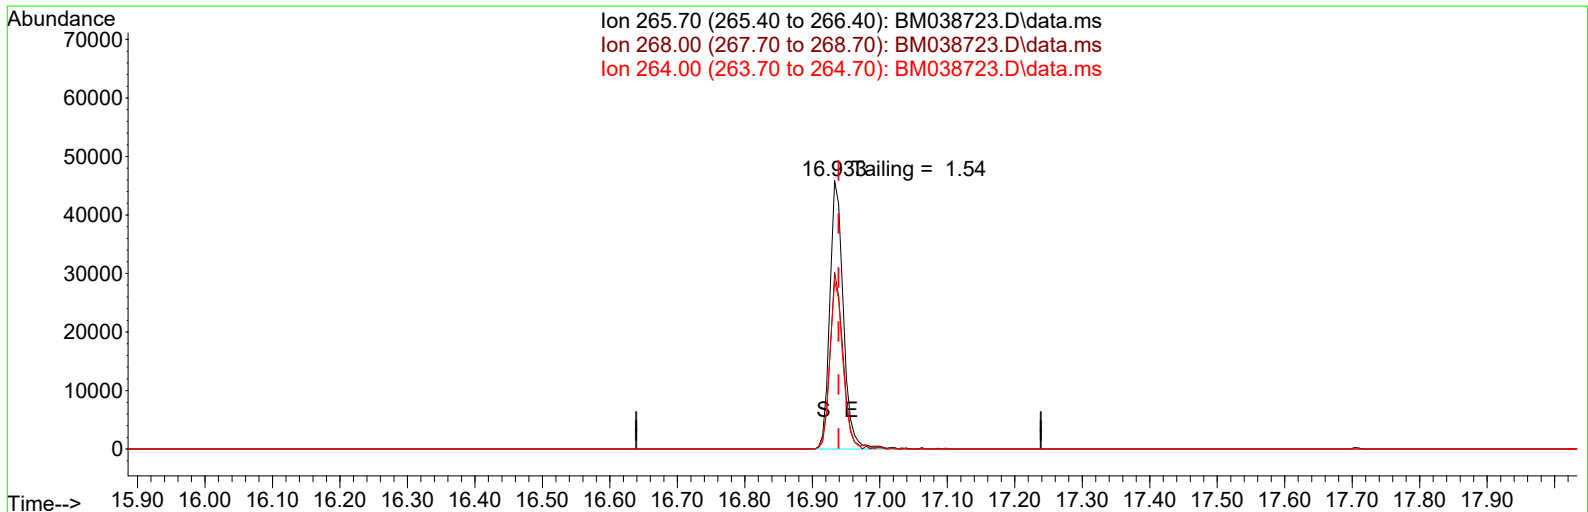

TIC: BM038723.D\data.ms

(70) Pentachlorophenol (C)

16.933min (-0.006) 0.00 ng




response 64218

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	69.90
264.00	63.30	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021423\
Data File : BM038723.D
Acq On : 14 Feb 2023 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 15 04:39:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 15 02:07:17 2023
Response via : Initial Calibration

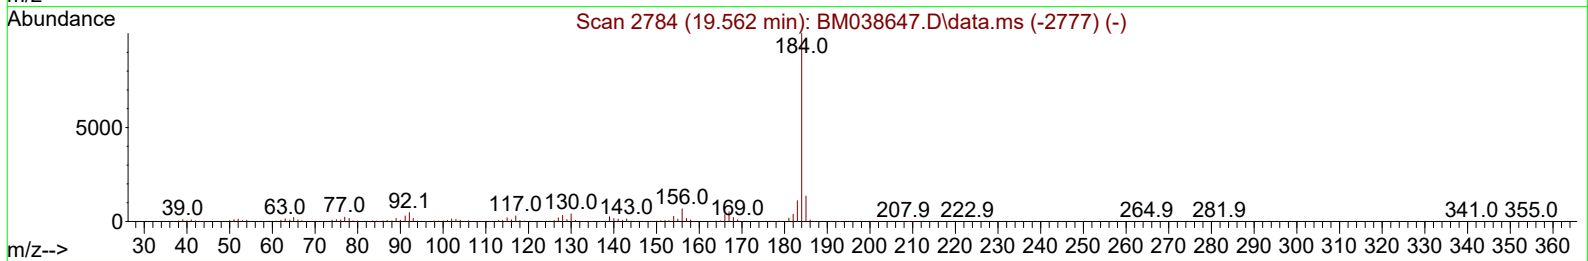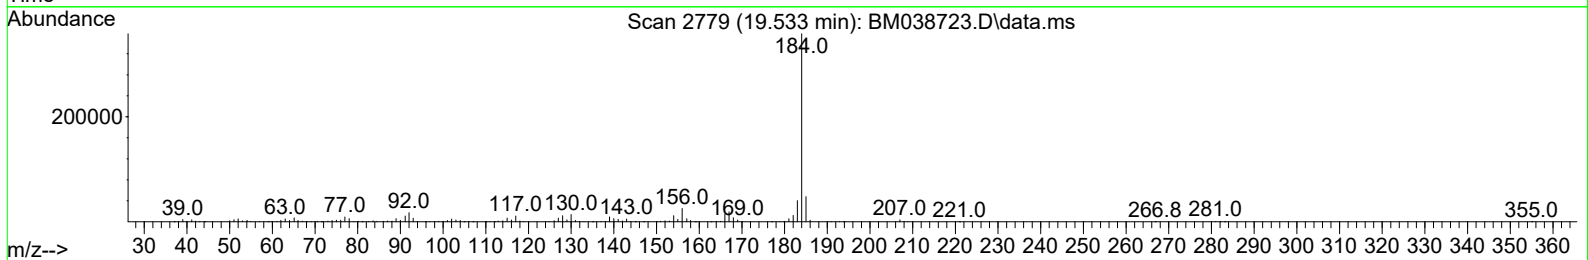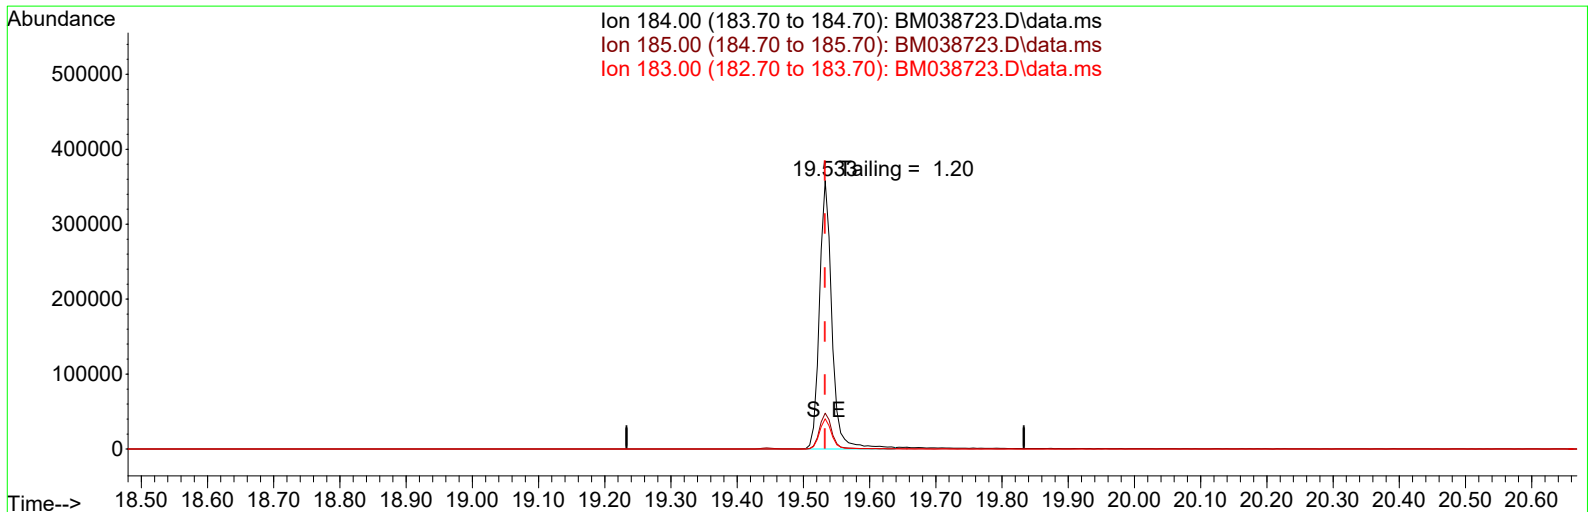

TIC: BM038723.D\data.ms

(77) Benzidine

19.533min (0.000) 0.00 ng

response 472621

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.39
183.00	11.00	11.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/14/2023	BNA_M	<u>BM038723.D</u>
Compound Name	Response	Retention Time
DDT	193620	20.75
DDD	3486	20.315
DDE	144	19.803
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3630	197250	1.84

Instrument :
BNA_M
ClientSampleId :
DFTPP