
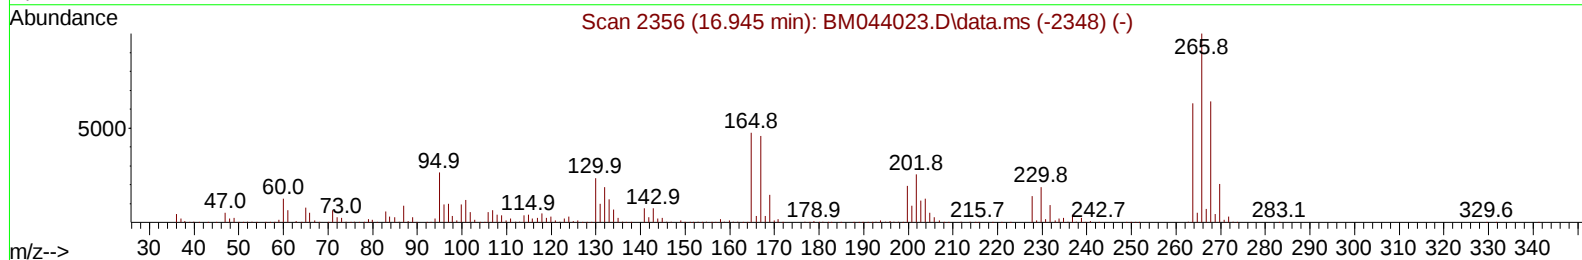
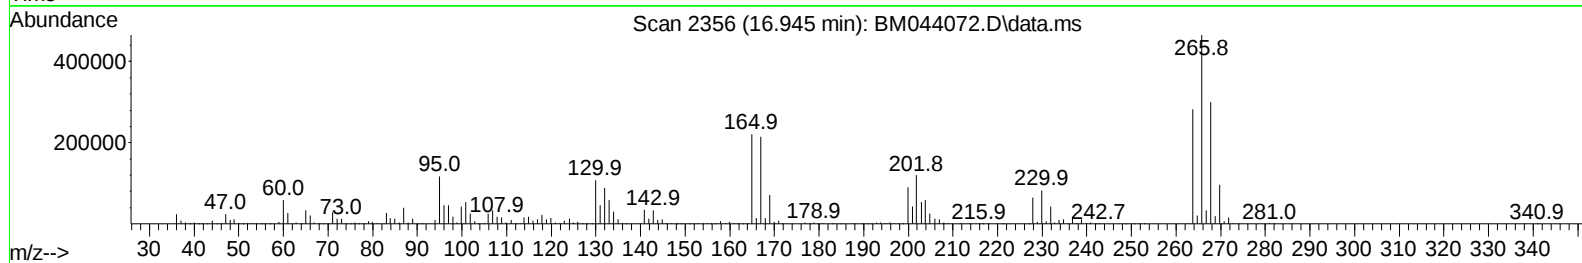


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021424\
Data File : BM044072.D
Acq On : 14 Feb 2024 08:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 02:34:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

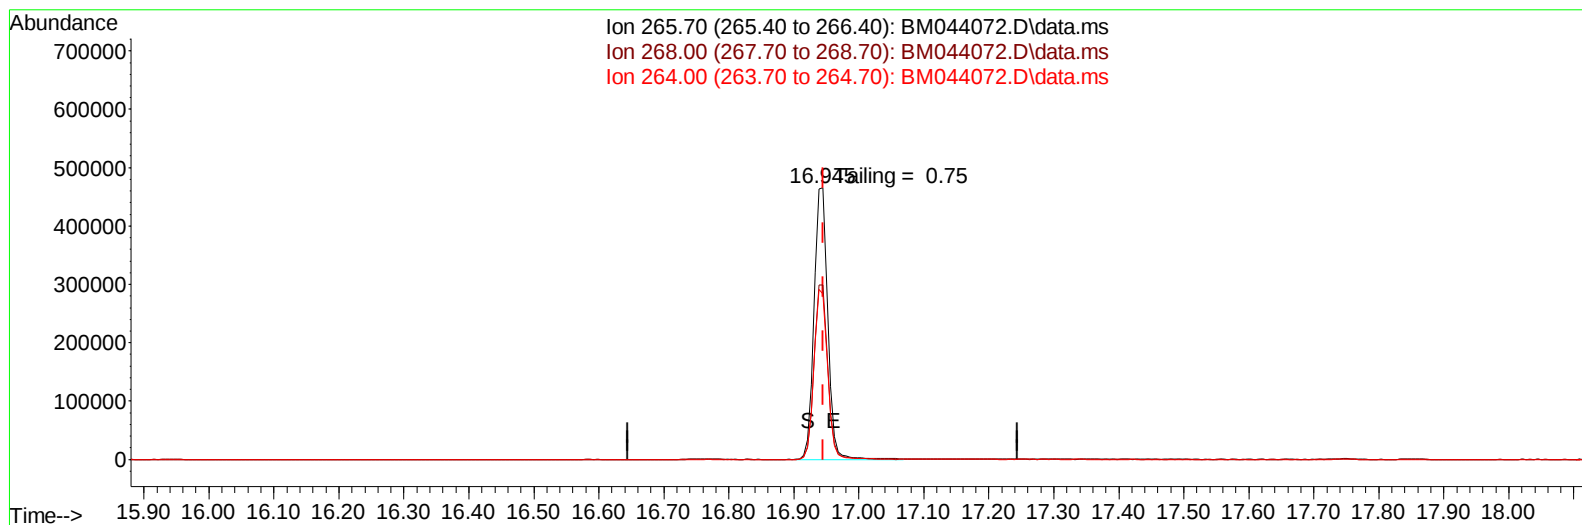




TIC: BM044072.D\data.ms

(70) Pentachlorophenol (C)**16.945min (+ 0.000) 111748.26 ng****response 684978**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.27
264.00	63.10	60.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021424\
Data File : BM044072.D
Acq On : 14 Feb 2024 08:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 02:34:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

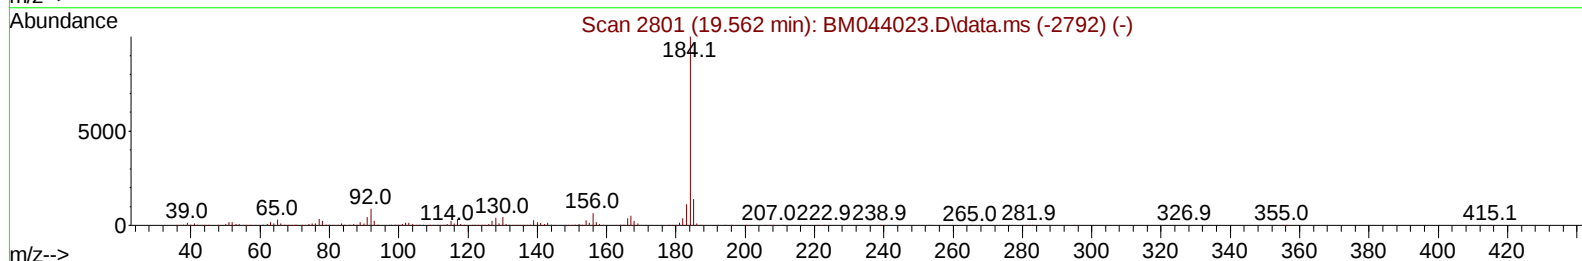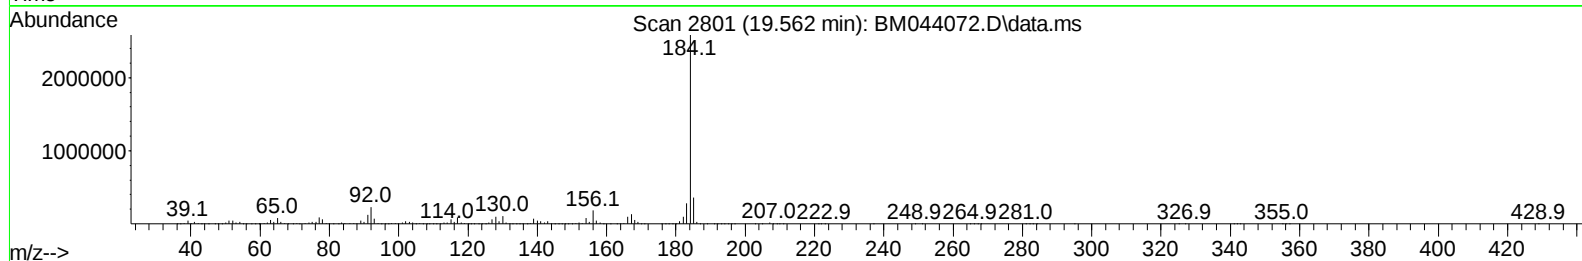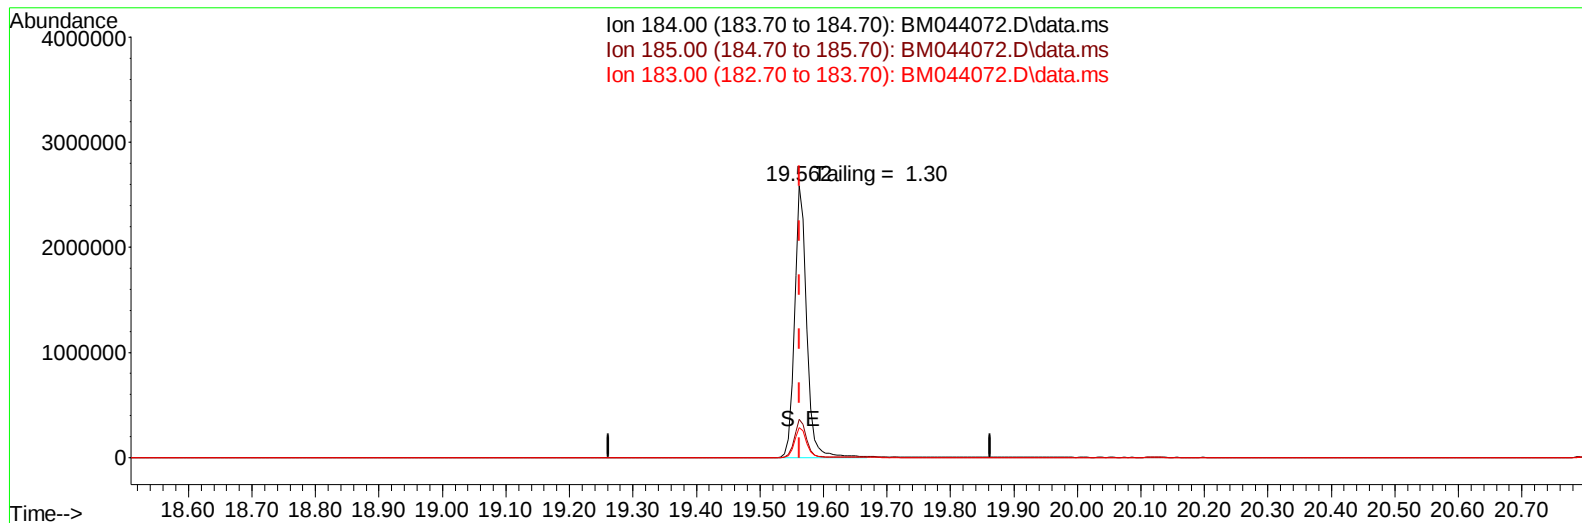

TIC: BM044072.D\data.ms

(77) Benzidine**19.562min (+ 0.000) 15890.00 ng****response 3478847**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.95
183.00	11.20	11.03
0.00	0.00	0.00