

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021424\
 Data File : BM044074.D
 Acq On : 14 Feb 2024 09:55
 Operator : MA/JU
 Sample : PB158892BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB158892BL

Quant Time: Feb 14 10:57:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 02:42:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	408112	20.000	ng	0.00
21) Naphthalene-d8	10.704	136	1620025	20.000	ng	-0.01
39) Acenaphthene-d10	14.545	164	877125	20.000	ng	-0.01
64) Phenanthrene-d10	17.298	188	1665945	20.000	ng	0.00
76) Chrysene-d12	21.497	240	1177591	20.000	ng	0.00
86) Perylene-d12	23.891	264	1233443	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	3771710	134.416	ng	0.00
7) Phenol-d6	7.075	99	4603979	128.956	ng	0.00
23) Nitrobenzene-d5	9.075	82	2723583	89.210	ng	0.00
42) 2,4,6-Tribromophenol	16.039	330	1033295	108.804	ng	0.00
45) 2-Fluorobiphenyl	13.174	172	5387336	86.684	ng	0.00
79) Terphenyl-d14	19.939	244	6291957	93.666	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021424\
Data File : BM044074.D
Acq On : 14 Feb 2024 09:55
Operator : MA/JU
Sample : PB158892BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB158892BL

Quant Time: Feb 14 10:57:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration




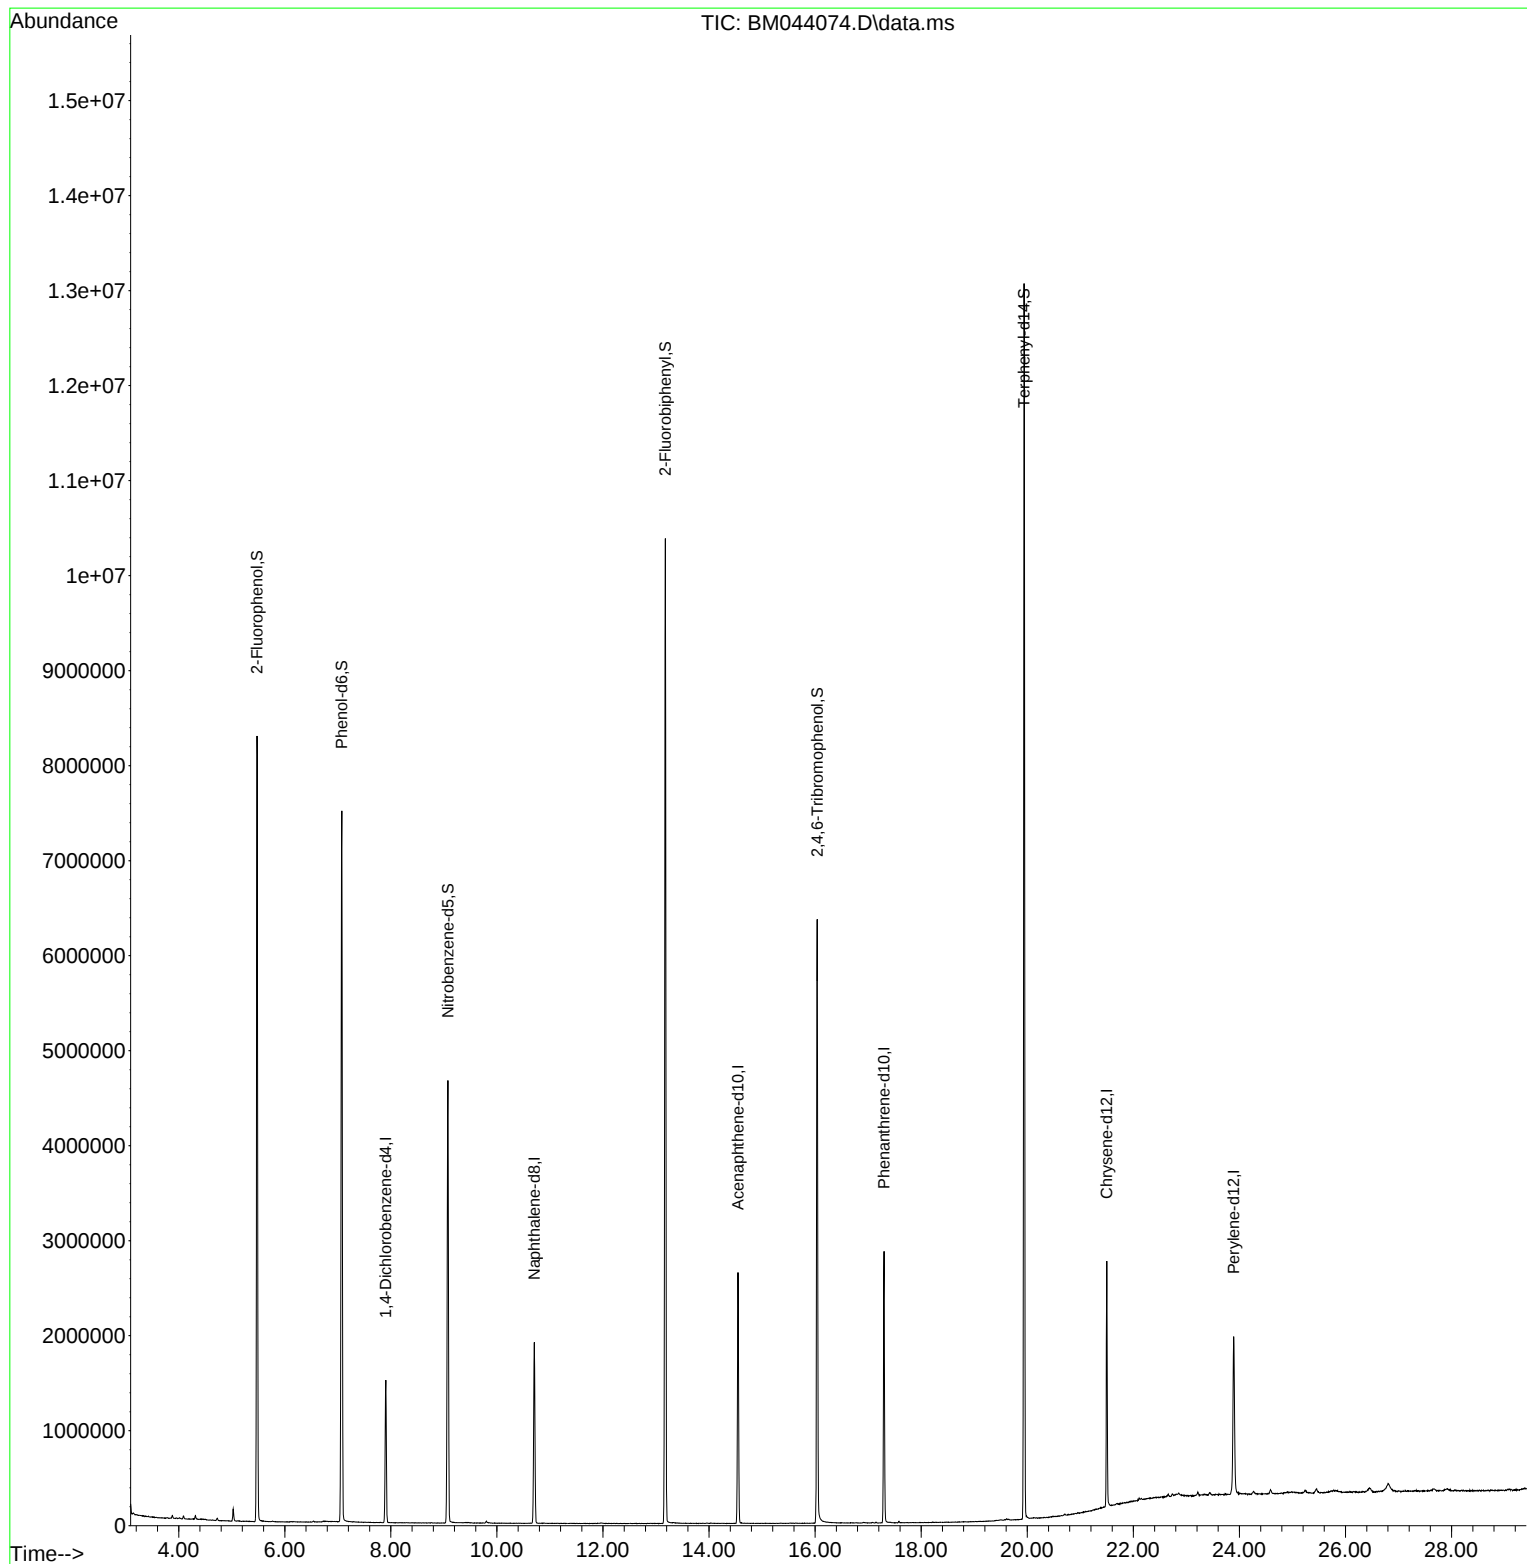


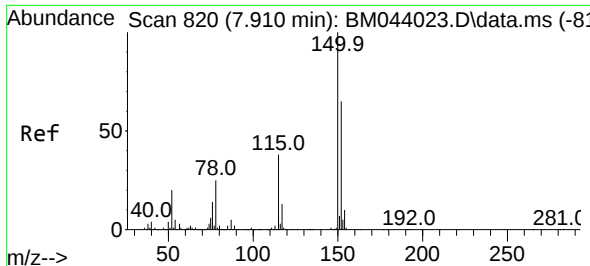

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.904 min Scan# 81
 Delta R.T. -0.006 min
 Lab File: BM044074.D
 Acq: 14 Feb 2024 09:55




Instrument :
 BNA_M
 ClientSampleId :
 PB158892BL


Tgt Ion:152 Resp: 408112
 Ion Ratio Lower Upper
 152 100
 150 157.7 122.7 184.1
 115 61.4 47.0 70.6

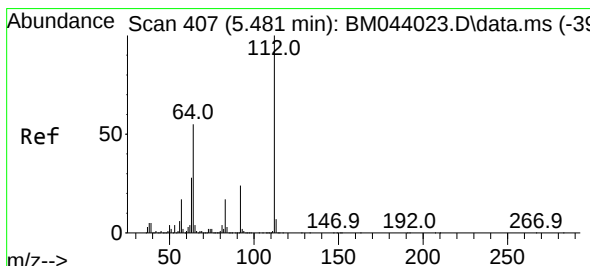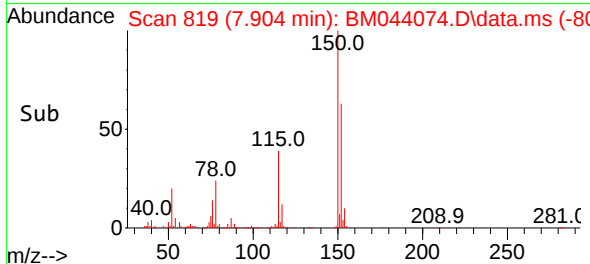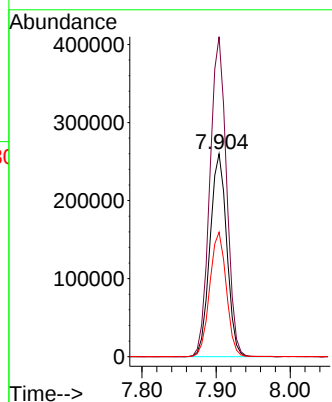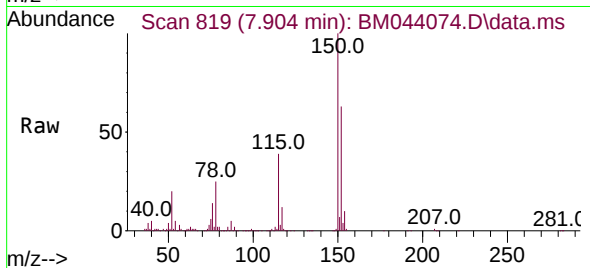

#5
 2-Fluorophenol
 Concen: 134.416 ng
 RT: 5.475 min Scan# 406
 Delta R.T. -0.006 min
 Lab File: BM044074.D
 Acq: 14 Feb 2024 09:55

Tgt Ion:112 Resp: 3771710
 Ion Ratio Lower Upper
 112 100
 64 56.2 44.2 66.4
 63 28.5 22.6 34.0

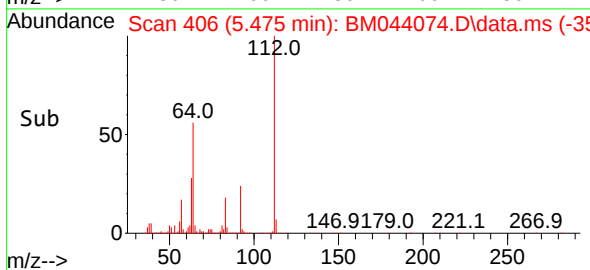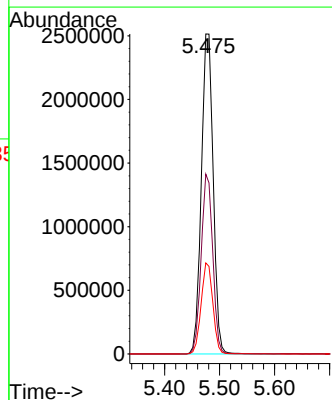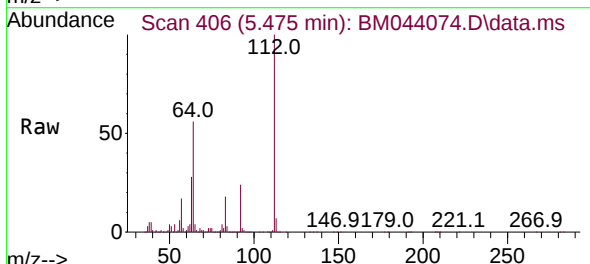







#7
Phenol-d6
Concen: 128.956 ng
RT: 7.075 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM044074.D
Acq: 14 Feb 2024 09:55

Instrument :
BNA_M
ClientSampleId :
PB158892BL

Tgt Ion: 99 Resp: 4603979




Ion	Ratio	Lower	Upper
99	100		
42	16.2	12.9	19.3
71	30.2	23.9	35.9

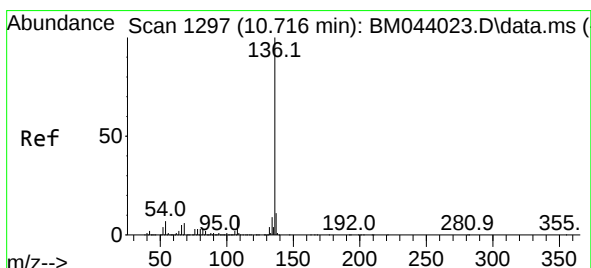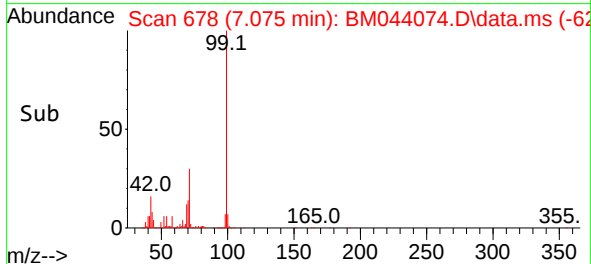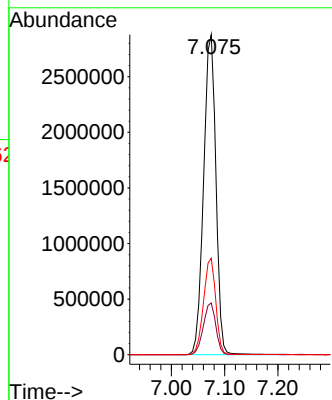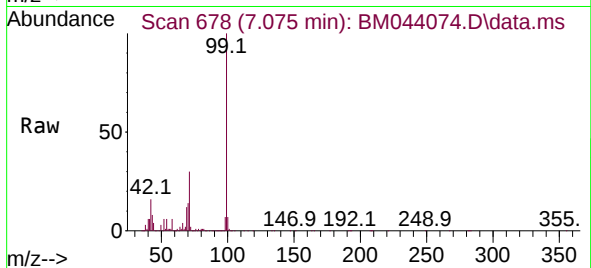


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.704 min Scan# 1295
Delta R.T. -0.012 min
Lab File: BM044074.D
Acq: 14 Feb 2024 09:55

Tgt Ion: 136 Resp: 1620025

Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.9	13.3
54	7.5	5.9	8.9
68	5.8	4.8	7.2


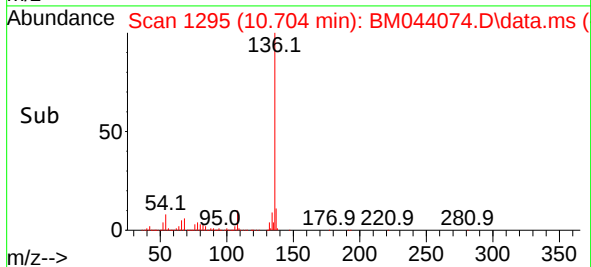
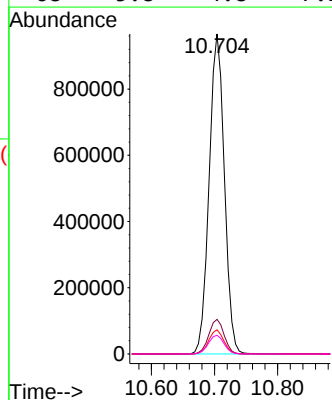
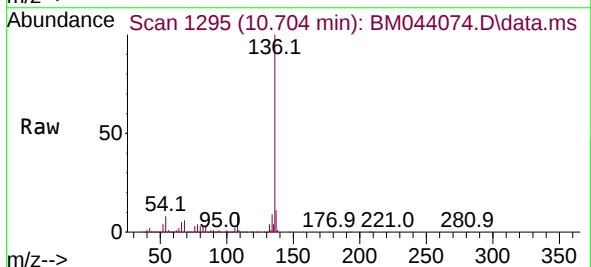




#23
Nitrobenzene-d5
Concen: 89.210 ng
RT: 9.075 min Scan# 1018
Delta R.T. -0.006 min
Lab File: BM044074.D
Acq: 14 Feb 2024 09:55




Instrument :
BNA_M
ClientSampleId :
PB158892BL


Tgt Ion: 82 Resp: 2723583
Ion Ratio Lower Upper
82 100
128 45.0 37.1 55.7
54 47.3 38.9 58.3

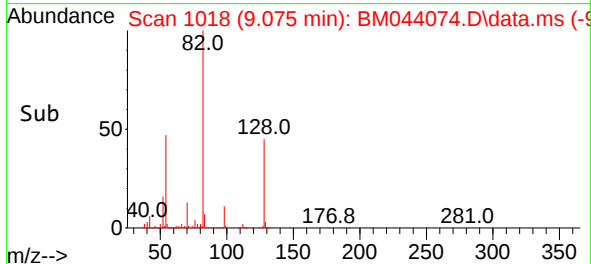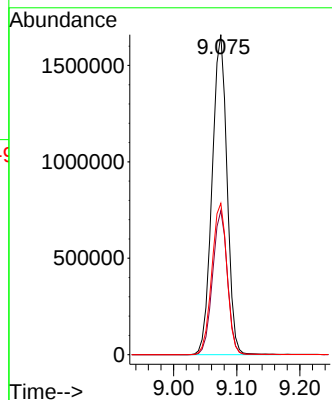

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.545 min Scan# 1948
Delta R.T. -0.012 min
Lab File: BM044074.D
Acq: 14 Feb 2024 09:55

Tgt Ion: 164 Resp: 877125
Ion Ratio Lower Upper
164 100
162 99.5 78.4 117.6
160 45.1 34.6 51.8


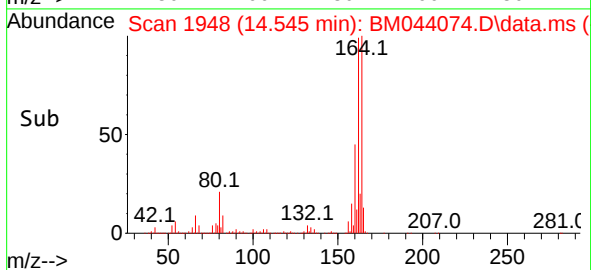
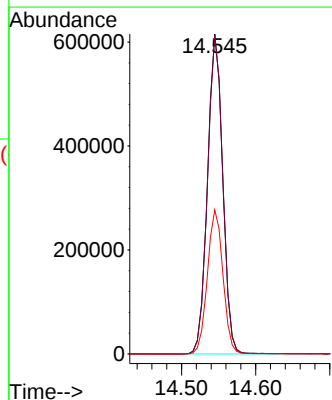
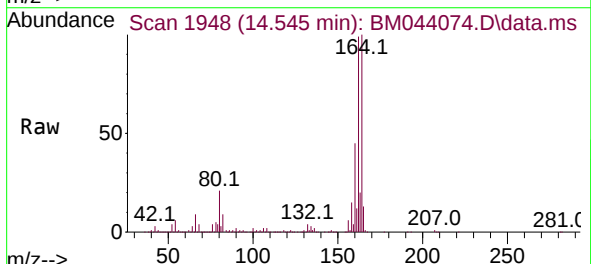




#42
2,4,6-Tribromophenol
Concen: 108.804 ng
RT: 16.039 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM044074.D
Acq: 14 Feb 2024 09:55




Instrument :
BNA_M
ClientSampleId :
PB158892BL


Tgt Ion:330 Resp: 1033295
Ion Ratio Lower Upper
330 100
332 96.1 77.7 116.5
141 43.9 31.0 46.4

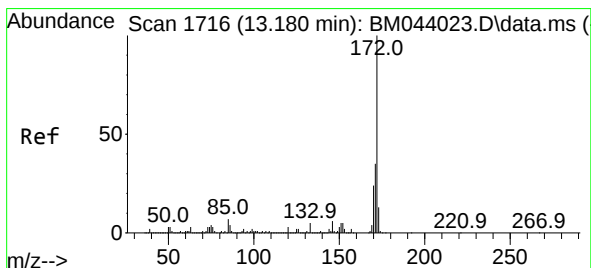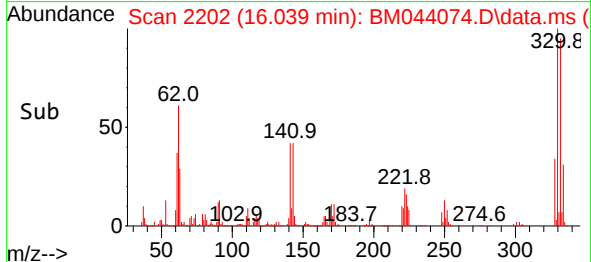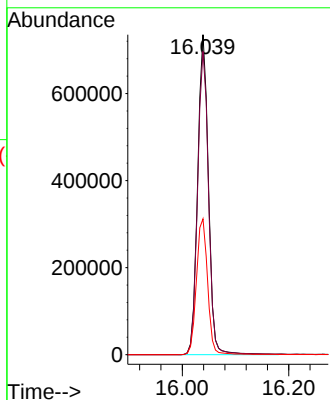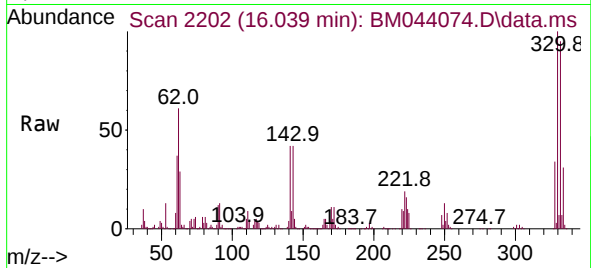

#45
2-Fluorobiphenyl
Concen: 86.684 ng
RT: 13.174 min Scan# 1715
Delta R.T. -0.006 min
Lab File: BM044074.D
Acq: 14 Feb 2024 09:55

Tgt Ion:172 Resp: 5387336
Ion Ratio Lower Upper
172 100
171 34.8 27.9 41.9
170 23.4 19.0 28.4


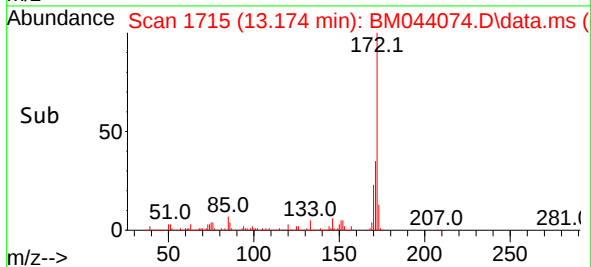
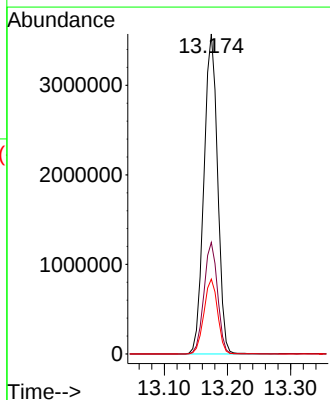
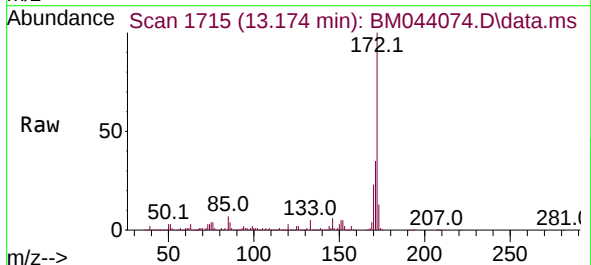




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.298 min Scan# 2417
Delta R.T. -0.006 min
Lab File: BM044074.D
Acq: 14 Feb 2024 09:55




Instrument :
BNA_M
ClientSampleId :
PB158892BL


Tgt Ion:188 Resp: 1665945
Ion Ratio Lower Upper
188 100
94 10.7 8.2 12.2
80 11.3 8.8 13.2

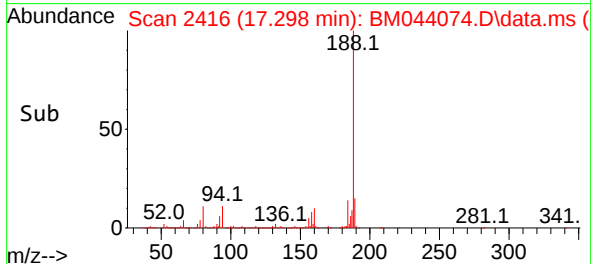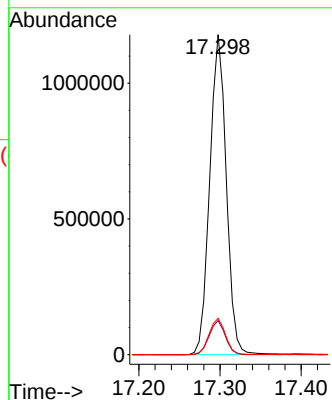

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.497 min Scan# 3130
Delta R.T. -0.006 min
Lab File: BM044074.D
Acq: 14 Feb 2024 09:55

Tgt Ion:240 Resp: 1177591
Ion Ratio Lower Upper
240 100
120 13.5 10.1 15.1
236 26.1 20.6 31.0


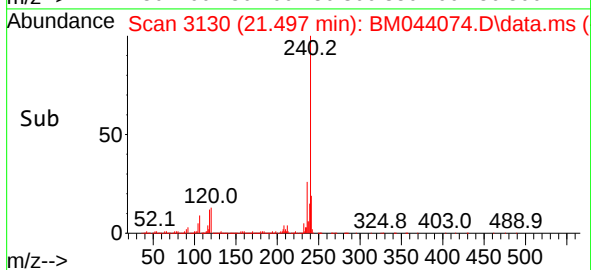
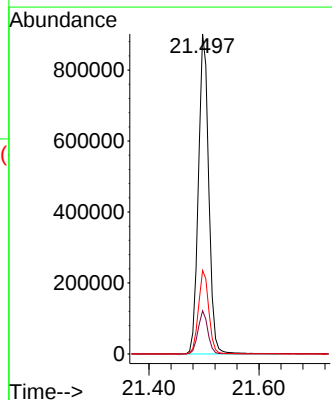
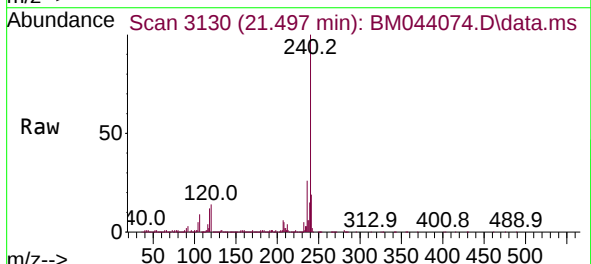




#79
 Terphenyl-d14
 Concen: 93.666 ng
 RT: 19.939 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM044074.D
 Acq: 14 Feb 2024 09:55

Instrument :
 BNA_M
 ClientSampleId :
 PB158892BL

Tgt Ion:244 Resp: 6291957
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.4 8.2
 122 13.8 9.5 14.3

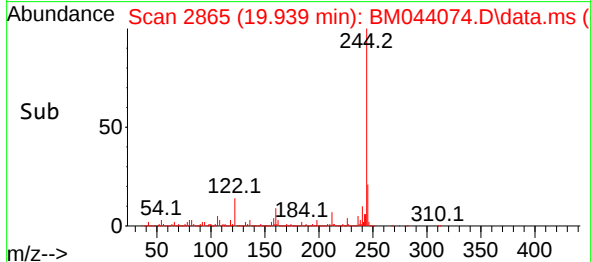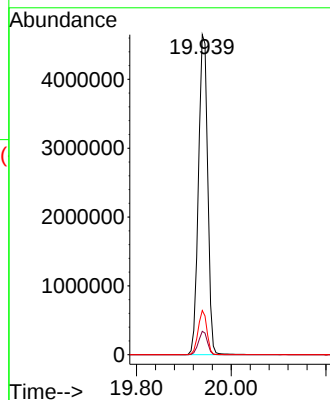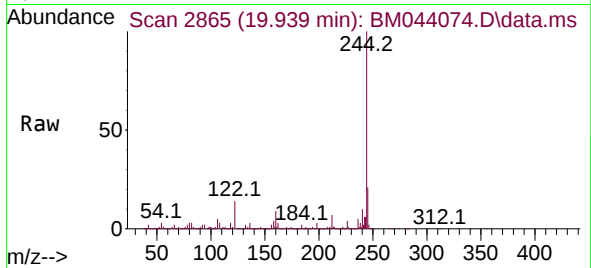

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.891 min Scan# 3537
 Delta R.T. -0.006 min
 Lab File: BM044074.D
 Acq: 14 Feb 2024 09:55

Tgt Ion:264 Resp: 1233443
 Ion Ratio Lower Upper
 264 100
 260 24.2 18.8 28.2
 265 21.9 17.3 25.9

