
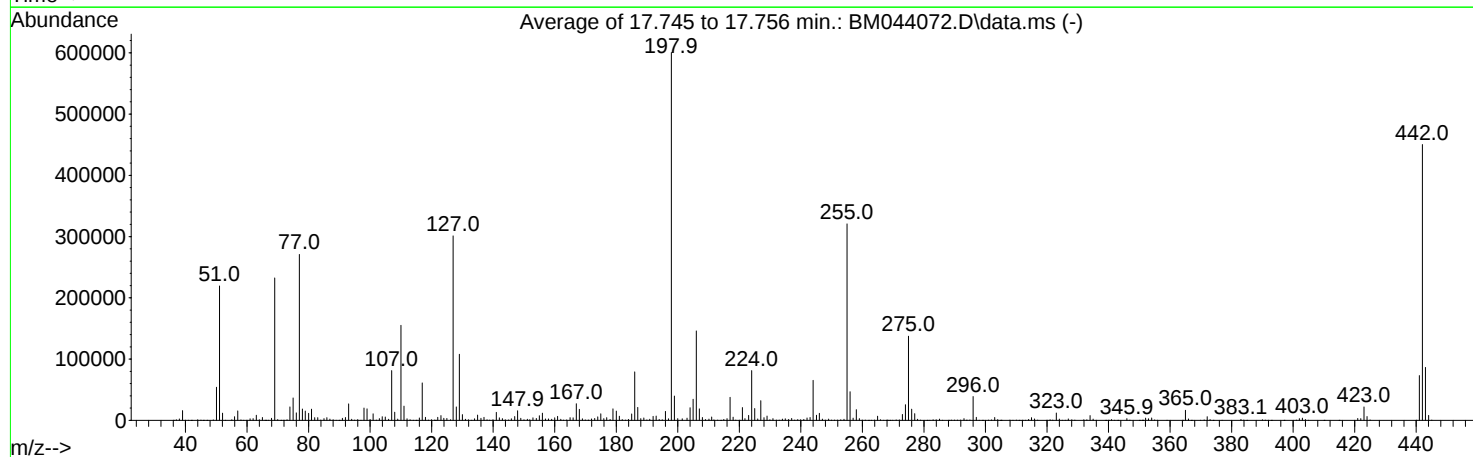


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021424\
Data File : BM044072.D
Acq On : 14 Feb 2024 08:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 09 02:42:01 2024

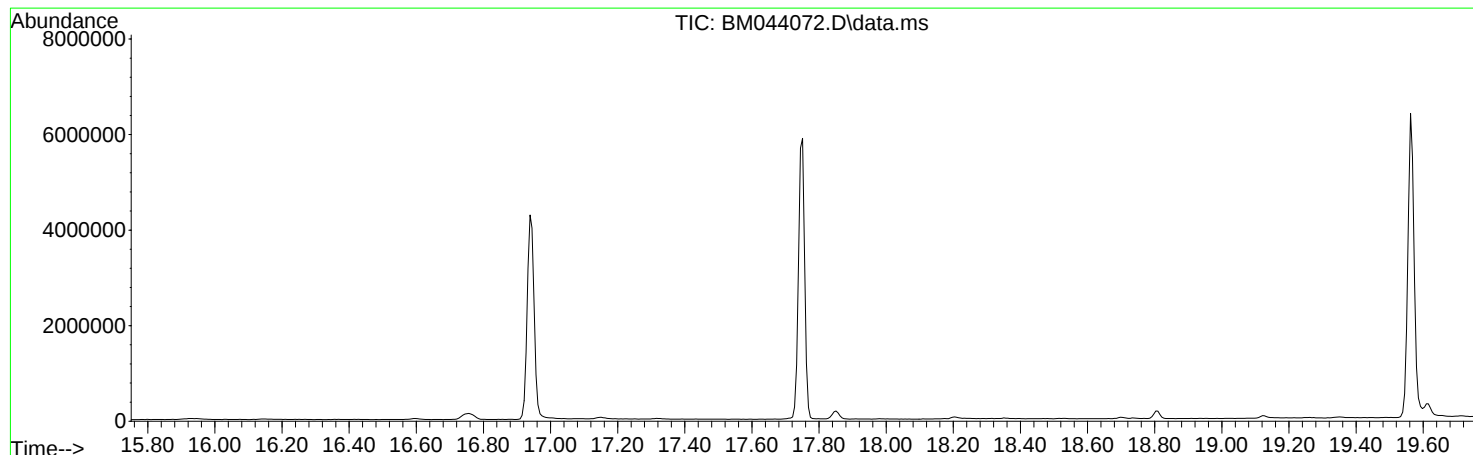

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	219517	PASS
68	69	0.00	2	1.4	3304	PASS
69	198	0.00	100	38.7	232556	PASS
70	69	0.00	2	0.6	1293	PASS
127	198	10	80	50.1	301077	PASS
197	198	0.00	2	0.4	2608	PASS
198	198	100	100	100.0	600555	PASS
199	198	5	9	6.6	39755	PASS
275	198	10	60	22.9	137384	PASS
365	198	1	100	2.7	16446	PASS
441	198	0.01	100	12.2	73069	PASS
442	442	50	100	100.0	450411	PASS
443	442	15	24	19.2	86477	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/14/2024	BNA_M	<u>BM044072.D</u>
Compound Name	Response	Retention Time
DDT	1822641	20.803
DDD	28154	20.409
DDE	2238	19.85
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30392	1853033	1.64

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021424\
Data File : BM044072.D
Acq On : 14 Feb 2024 08:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 15 02:34:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

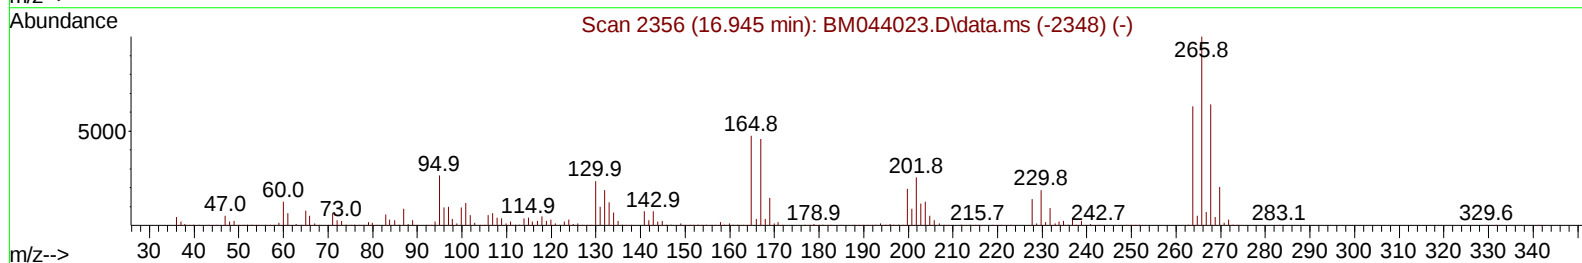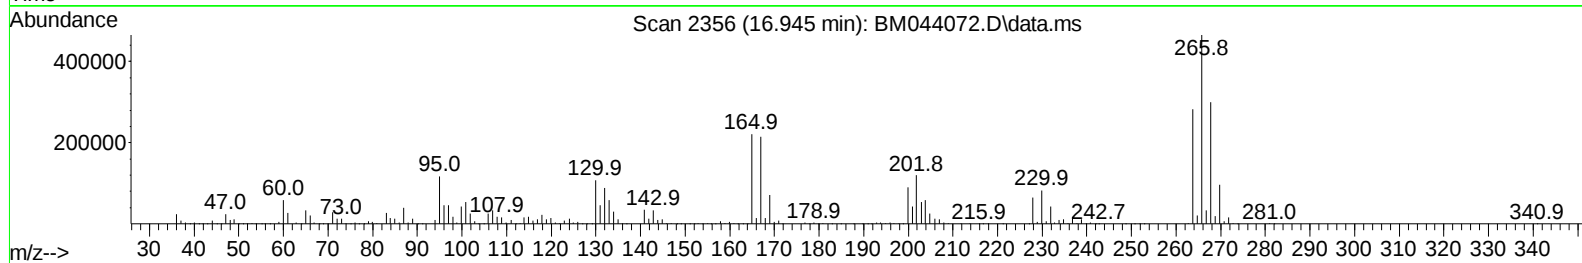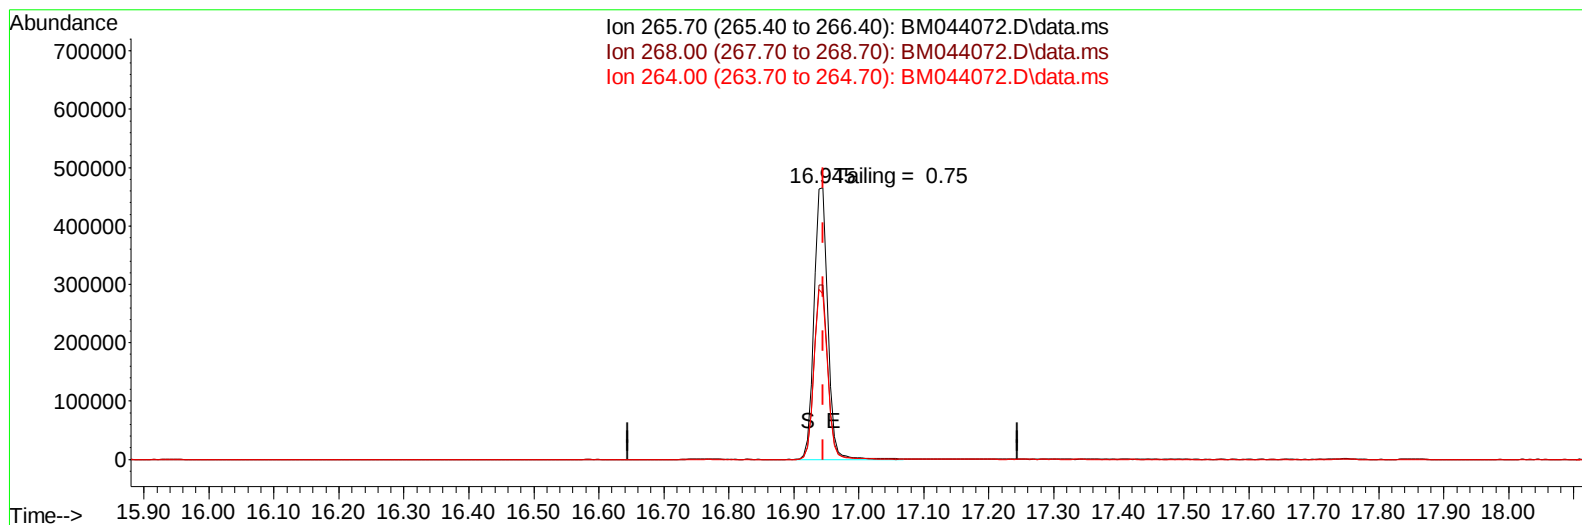

TIC: BM044072.D\data.ms

(70) Pentachlorophenol (C)

16.945min (+ 0.000) 111748.26 ng




response 684978

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.27
264.00	63.10	60.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021424\
Data File : BM044072.D
Acq On : 14 Feb 2024 08:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 15 02:34:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

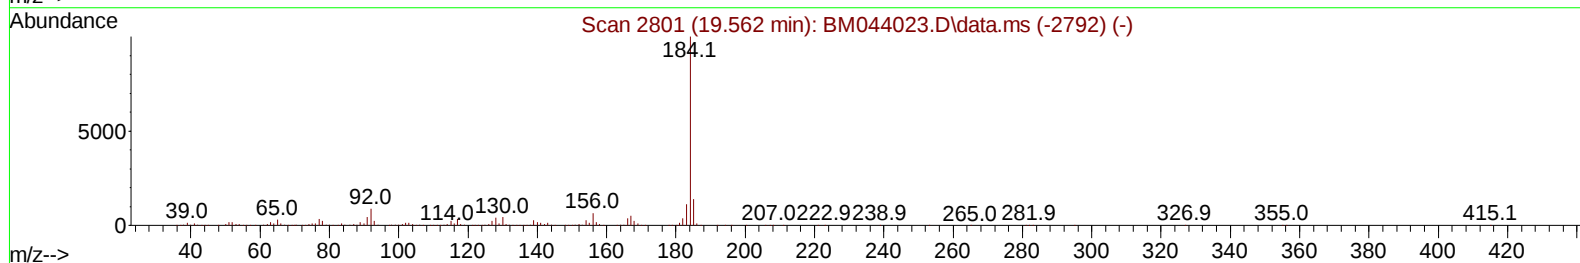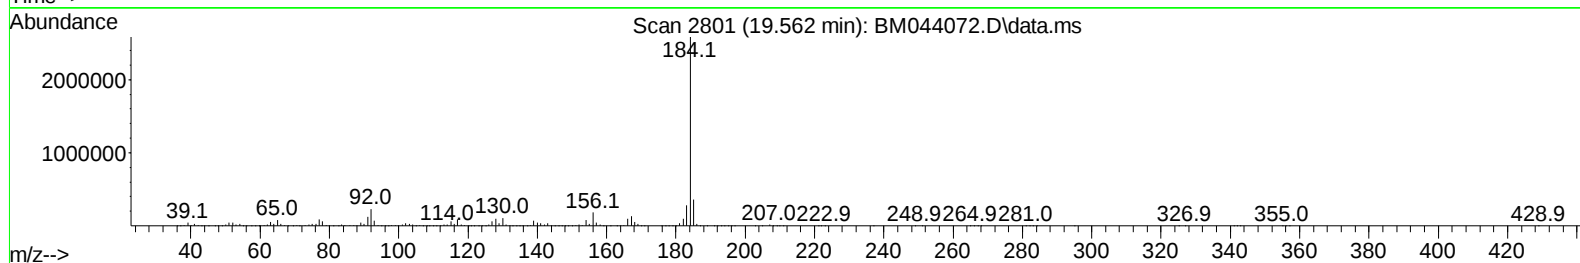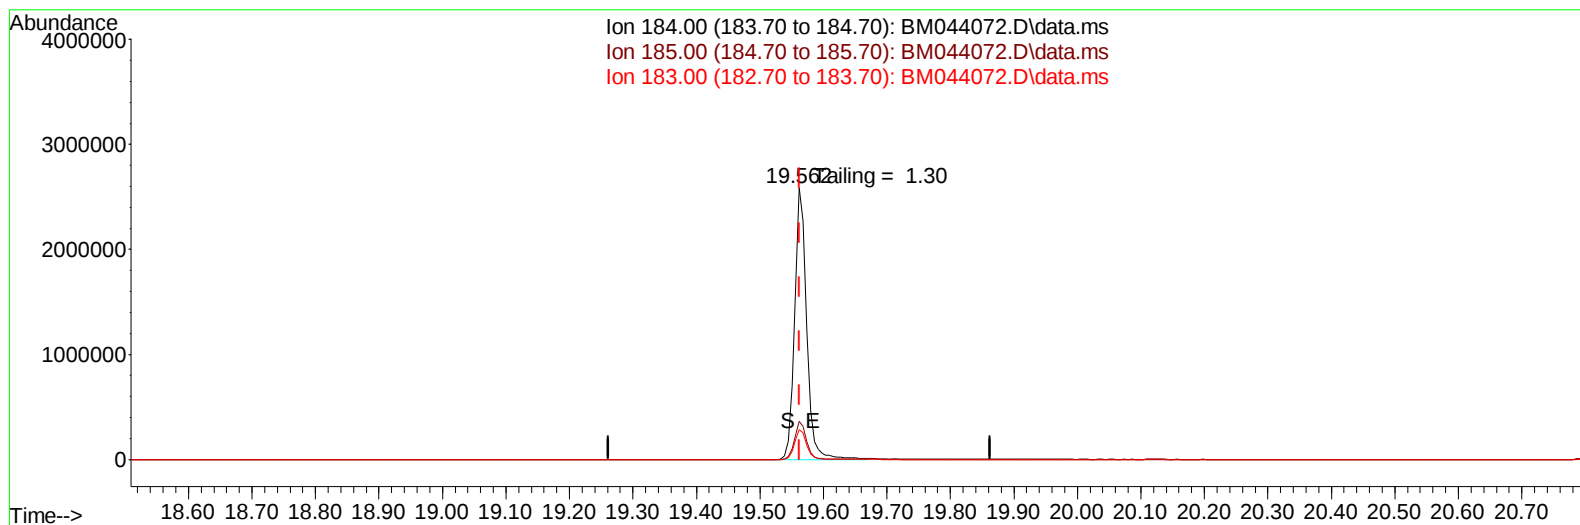

TIC: BM044072.D\data.ms

(77) Benzidine

19.562min (+ 0.000) 15890.00 ng

response 3478847

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.95
183.00	11.20	11.03
0.00	0.00	0.00