

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021516\
 Data File : BM004260.D
 Acq On : 15 Feb 2016 15:41
 Operator : SJ/UM
 Sample : H1449-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.763	9	13	21	rVB	12555	19819	6.15%	1.382%
2	3.275	99	100	103	rVV	460	422	0.13%	0.029%
3	3.322	107	108	111	rVB2	371	346	0.11%	0.024%
4	3.616	157	158	162	rBV2	363	578	0.18%	0.040%
5	3.763	182	183	188	rBV	701	1067	0.33%	0.074%
6	3.899	204	206	207	rBB	677	348	0.11%	0.024%
7	3.910	207	208	211	rBB	626	441	0.14%	0.031%
8	3.940	211	213	216	rBV	341	567	0.18%	0.040%
9	3.981	219	220	222	rBB	619	325	0.10%	0.023%
10	7.640	837	842	850	rBB	68873	108806	33.78%	7.589%
11	10.434	1310	1317	1330	rBB	97558	164829	51.18%	11.497%
12	14.304	1970	1975	1983	rBB2	152582	228520	70.96%	15.939%
13	17.057	2438	2443	2458	rBB2	188975	265466	82.43%	18.516%
14	18.833	2743	2745	2747	rBV	368	465	0.14%	0.032%
15	18.915	2756	2759	2760	rBB	373	355	0.11%	0.025%
16	20.362	3003	3005	3007	rBV	1174	1013	0.31%	0.071%
17	20.386	3007	3009	3010	rVB	714	376	0.12%	0.026%
18	20.398	3010	3011	3012	rBV	642	354	0.11%	0.025%
19	20.439	3015	3018	3020	rVB3	508	522	0.16%	0.036%
20	20.468	3020	3023	3024	rBV	414	373	0.12%	0.026%
21	20.545	3034	3036	3037	rVB	644	443	0.14%	0.031%
22	20.568	3037	3040	3042	rBV2	750	979	0.30%	0.068%
23	20.651	3050	3054	3057	rBV3	678	1284	0.40%	0.090%
24	20.945	3102	3104	3105	rBV2	562	323	0.10%	0.023%
25	21.098	3128	3130	3133	rBV3	806	769	0.24%	0.054%
26	21.274	3154	3160	3166	rBV	247103	322059	100.00%	22.463%
27	23.503	3532	3539	3546	rBV	174048	312863	97.14%	21.822%


Sum of corrected areas: 1433712

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021516\
Data File : BM004260.D
Acq On : 15 Feb 2016 15:41
Operator : SJ/UM
Sample : H1449-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

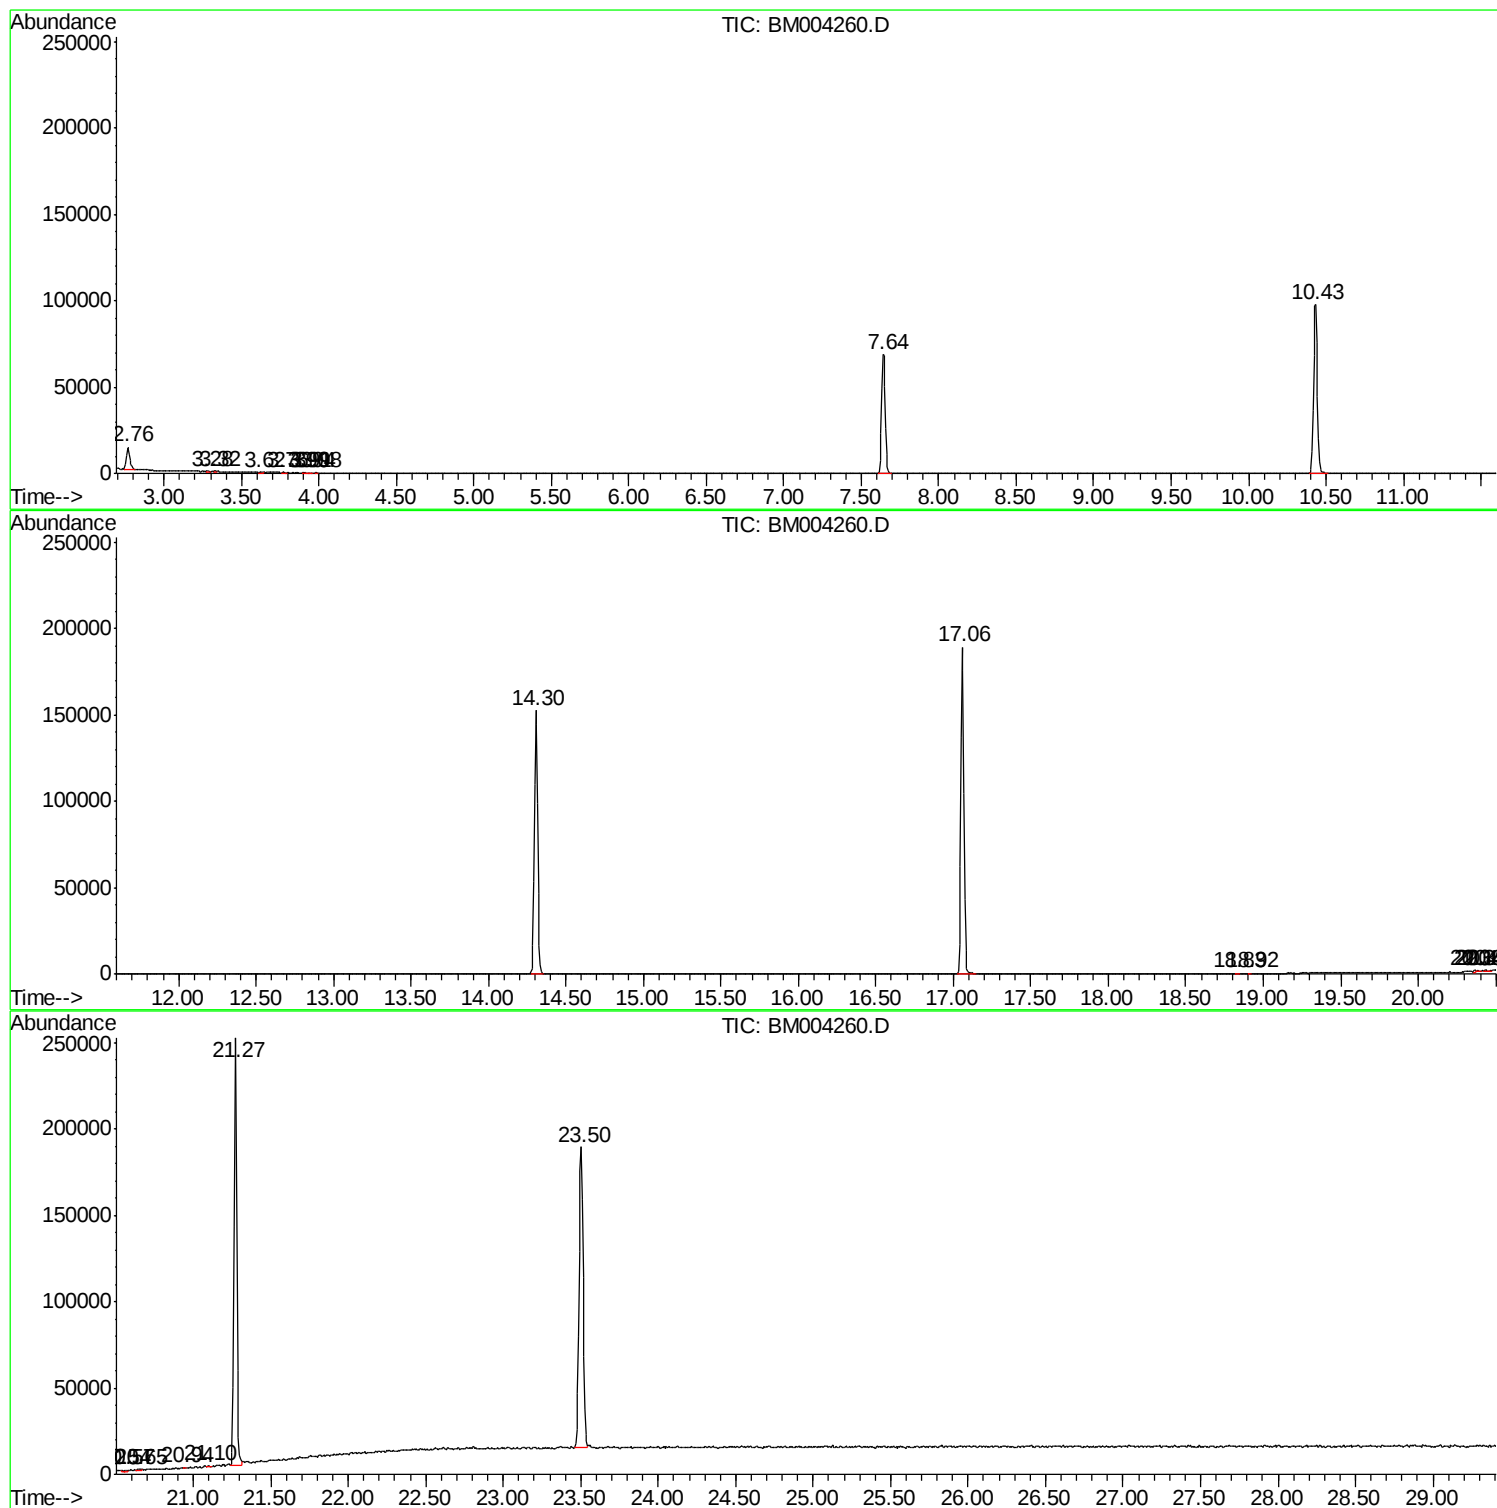

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021516\
Data File : BM004260.D
Acq On : 15 Feb 2016 15:41
Operator : SJ/UM
Sample : H1449-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021516\
Data File : BM004260.D
Acq On : 15 Feb 2016 15:41
Operator : SJ/UM
Sample : H1449-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc