


Data Path : Z:\HPCHEM1\BNA M\DATA\BM021516\
Data File : BM004256.D
Acq On : 15 Feb 2016 08:57
Operator : SJ/UM
Sample : DFTPP51
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP51

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Title : SVOA CALIBRATION
Last Update : Tue Feb 16 02:45:44 2016

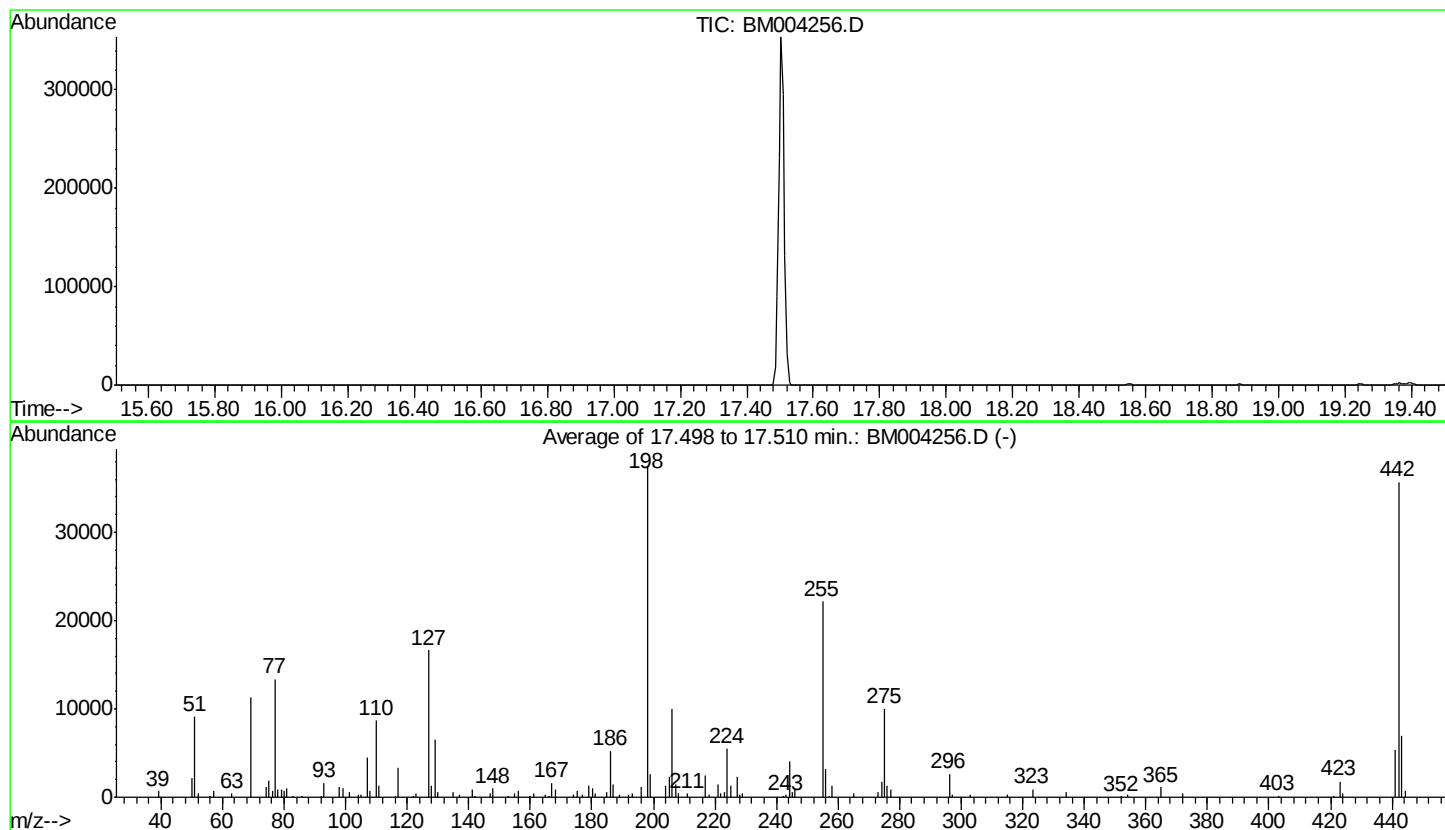

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	9086	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.1	11304	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.4	16661	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37533	PASS
199	198	5	9	7.1	2655	PASS
275	198	10	60	26.7	10031	PASS
365	198	1	100	3.1	1148	PASS
441	443	0.01	100	76.7	5350	PASS
442	198	50	100	95.2	35714	PASS
443	442	15	24	19.5	6976	PASS

m/z	Abundance
39.10	676.0
50.10	2093.0
51.10	8434.0
52.10	454.0
56.00	312.0
57.00	688.0
63.00	362.0
69.00	10554.0
74.10	1079.0
75.00	1708.0
76.10	561.0
77.10	12164.0
78.10	904.0
79.00	843.0
80.00	640.0
81.00	966.0
93.00	1485.0
98.00	1034.0
99.00	866.0
101.10	497.0
104.00	300.0
105.00	367.0
107.10	4063.0
108.00	658.0
110.00	7710.0
111.00	1186.0
117.00	2827.0
122.90	386.0
127.10	15006.0
128.00	1134.0
129.00	5772.0
130.00	492.0
134.90	463.0
141.00	734.0
147.00	434.0
148.00	867.0
155.00	472.0
156.00	654.0
161.00	349.0
167.00	1496.0
168.00	816.0
175.00	556.0
179.00	1205.0
180.10	919.0
181.00	344.0
185.00	589.0
186.10	4248.0
187.00	1244.0
193.00	422.0
196.10	953.0
198.00	31136.0
199.00	2271.0
204.10	1074.0
205.10	1849.0
206.10	8196.0
207.10	1224.0
208.00	322.0
211.10	301.0
217.00	1913.0
221.00	1062.0
221.80	328.0
223.10	512.0
224.10	4259.0
225.10	1113.0
227.10	1862.0
229.00	335.0
244.10	3194.0
245.10	487.0
246.00	636.0
255.10	17008.0
256.10	2524.0
258.00	968.0
265.00	435.0
273.00	464.0
274.10	1269.0
275.10	7431.0
276.10	1072.0
277.00	615.0
296.10	1969.0
323.10	635.0
334.10	368.0
365.10	793.0
372.10	320.0
423.10	1075.0
424.10	359.0
441.10	3248.0
442.20	21152.0
443.10	4244.0
444.10	525.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

m/z	Abundance
39.10	837.0
50.10	2593.0
51.10	11221.0
52.10	591.0
56.00	335.0
57.00	824.0
63.00	473.0
69.00	13841.0
74.10	1379.0
75.00	2259.0
76.10	834.0
77.10	16326.0
78.10	1061.0
79.00	1157.0
80.00	869.0
81.00	1156.0
83.00	304.0
86.00	310.0
92.00	322.0
93.00	1917.0
98.00	1382.0
99.00	1197.0
101.00	711.0
104.00	441.0
105.00	428.0
107.00	5314.0
108.00	816.0
110.00	10400.0
111.00	1607.0
116.00	361.0
117.10	4036.0
122.00	374.0
123.00	599.0
127.10	19992.0
128.00	1587.0
129.00	7776.0
130.00	670.0
135.00	639.0
137.00	390.0
141.00	1001.0
142.00	350.0
147.00	623.0
148.00	1122.0
153.00	405.0
155.00	655.0
156.00	813.0
160.00	314.0
161.00	514.0
165.00	407.0
166.00	343.0
167.00	1859.0
168.00	1071.0
174.00	400.0
175.10	837.0
177.00	413.0
179.00	1536.0
180.00	1193.0
181.00	526.0
185.00	796.0
186.10	6297.0
187.00	1793.0
189.00	381.0
192.00	516.0
193.00	586.0
196.10	1259.0
198.00	44912.0
199.00	3172.0
204.10	1562.0
205.10	2680.0
206.10	12001.0
207.10	1732.0
208.00	430.0
211.00	484.0
217.00	3050.0
218.00	384.0
221.00	1894.0
221.80	446.0
223.00	752.0
224.10	6495.0
225.10	1590.0
227.00	2659.0
228.00	351.0
229.00	501.0
242.10	313.0
243.10	359.0
244.10	4817.0
245.10	628.0
246.00	974.0
255.10	26536.0
256.10	3792.0
257.00	321.0
258.00	1513.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

265.00	556.0
273.10	760.0
274.10	2041.0
275.10	12080.0
276.10	1615.0
277.10	1019.0
296.10	3191.0
297.00	333.0
303.10	424.0
315.10	350.0
323.10	1052.0
334.10	669.0
354.10	380.0
365.10	1393.0
372.10	604.0
403.10	326.0
421.00	324.0
423.10	2112.0
424.10	568.0
441.20	6381.0
442.20	41120.0
443.20	8090.0
444.20	709.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

m/z	Abundance
39.10	610.0
50.10	1921.0
51.10	7603.0
52.00	400.0
57.00	612.0
63.00	357.0
69.00	9519.0
74.10	992.0
75.00	1605.0
76.10	609.0
77.10	11577.0
78.10	826.0
79.00	810.0
80.00	597.0
81.00	1020.0
93.00	1455.0
98.00	1209.0
99.00	865.0
101.00	532.0
104.00	332.0
105.00	308.0
107.00	4068.0
108.00	642.0
110.00	7811.0
111.00	1123.0
117.00	3113.0
123.00	418.0
127.10	14986.0
128.00	1169.0
129.00	5984.0
130.00	468.0
135.00	475.0
137.00	309.0
141.00	750.0
147.10	417.0
148.00	856.0
155.00	396.0
156.10	604.0
161.00	454.0
165.00	341.0
167.10	1660.0
168.00	793.0
173.90	365.0
175.10	608.0
177.00	335.0
179.00	1207.0
180.00	870.0
181.00	446.0
185.00	587.0
186.10	5177.0
187.00	1419.0
189.00	326.0
192.00	440.0
193.00	496.0
196.10	1142.0
198.00	36552.0
199.00	2524.0
204.00	1400.0
205.10	2264.0
206.10	9995.0
207.10	1244.0
208.00	395.0
211.00	424.0
217.00	2346.0
218.00	338.0
221.10	1497.0
221.90	349.0
223.00	525.0
224.10	5708.0
225.10	1355.0
227.10	2261.0
228.00	334.0
229.00	428.0
243.10	321.0
244.10	4146.0
245.10	615.0
246.00	796.0
255.10	22864.0
256.10	3388.0
258.00	1240.0
265.00	537.0
273.00	699.0
274.10	1773.0
275.10	10583.0
276.00	1390.0
277.00	888.0
296.10	2862.0
297.00	438.0
303.10	345.0
315.00	322.0
323.10	967.0
334.10	602.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

352.10	300.0
354.10	359.0
365.10	1258.0
372.10	570.0
403.10	337.0
421.10	308.0
423.10	2176.0
424.10	545.0
441.10	6422.0
442.20	44872.0
443.20	8596.0
444.10	750.0

Instrument :
BNA_M
ClientSampleId :
DFTPP51

m/z

Abundance

Instrument :
BNA_M
ClientSampleId :
DFTPP51