


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021521\
 Data File : BM028733.D
 Acq On : 15 Feb 2021 09:41
 Operator : CG/JU
 Sample : DFTPP29
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP029

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM021221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 15 11:26:28 2021

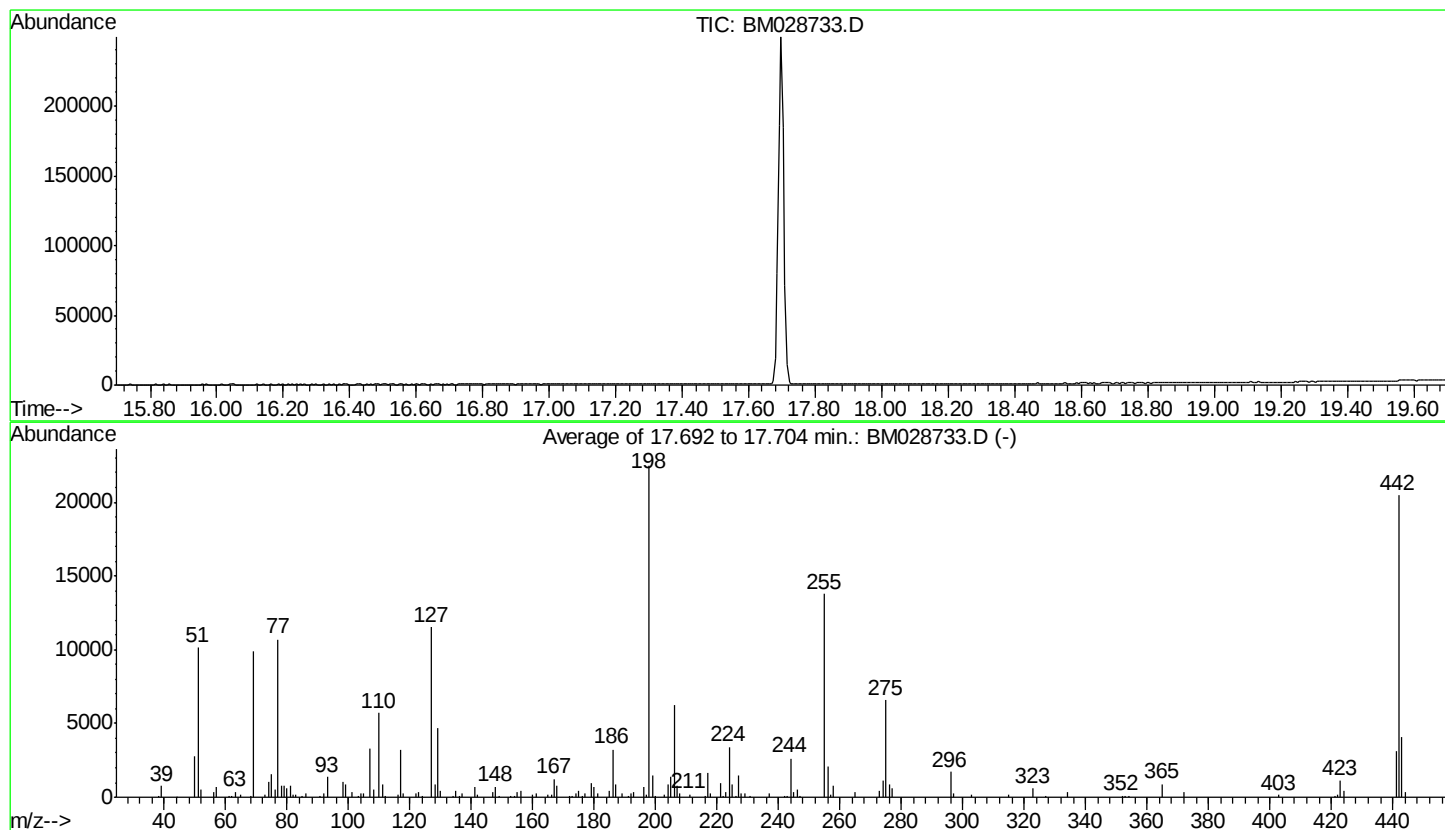

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	10128	PASS
68	69	0.00	2	1.3	132	PASS
69	198	0.00	100	44.2	9934	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	11516	PASS
197	198	0.00	2	0.8	170	PASS
198	198	100	100	100.0	22474	PASS
199	198	5	9	6.7	1495	PASS
275	198	10	60	29.2	6559	PASS
365	198	1	100	3.9	876	PASS
441	198	0.01	100	13.8	3109	PASS
442	198	50	100	90.9	20438	PASS
443	442	15	24	19.9	4071	PASS

Scan 2494 (17.656 min): BM028733.D
DFTPP29

m/z	Abundance
44.00	420.0
207.00	284.0

Instrument :
BNA_M
ClientSampleId :
DFTPP029

m/z	Abundance
39.00	815.0
43.90	380.0
50.10	2819.0
51.10	10492.0
52.00	500.0
56.00	319.0
57.00	769.0
60.90	185.0
63.00	340.0
65.00	196.0
68.10	221.0
69.00	10453.0
73.00	219.0
74.00	1151.0
75.00	1644.0
76.10	572.0
77.10	11150.0
78.10	779.0
79.00	790.0
80.00	632.0
81.00	785.0
82.00	191.0
82.90	155.0
85.00	180.0
86.00	239.0
90.90	199.0
92.00	299.0
93.00	1317.0
98.00	1091.0
99.00	933.0
101.00	373.0
104.00	331.0
105.00	272.0
107.00	3201.0
108.00	496.0
110.00	5582.0
111.00	909.0
116.10	234.0
117.00	3188.0
117.90	258.0
121.90	250.0
123.00	381.0
123.90	179.0
127.00	11026.0
128.00	825.0
129.00	4699.0
130.00	414.0
133.90	150.0
135.00	383.0
137.00	251.0
140.90	643.0
141.90	201.0
146.90	344.0
147.90	555.0
149.00	157.0
152.90	177.0
153.90	163.0
155.00	284.0
156.00	345.0
159.90	225.0
161.00	260.0
165.00	192.0
166.00	181.0
167.00	1106.0
168.00	778.0
174.00	261.0
175.00	384.0
176.90	193.0
179.00	909.0
180.00	600.0
181.00	214.0
184.90	404.0
186.00	2931.0
187.00	845.0
188.90	205.0
191.90	243.0
193.00	348.0
196.00	615.0
197.00	176.0
198.00	20104.0
198.90	1345.0
203.00	209.0
204.00	675.0
205.00	1299.0
206.00	5606.0
207.00	980.0
208.00	243.0
210.90	169.0
217.00	1425.0
218.00	229.0
221.00	748.0
222.90	325.0

Instrument :
BNA_M
ClientSampleId :
DFTPP029

224.00	3043.0
225.00	829.0
227.00	1318.0
227.90	189.0
229.00	229.0
237.00	197.0
242.00	196.0
243.00	182.0
244.00	2334.0
245.00	328.0
246.00	475.0
255.00	11851.0
256.00	1691.0
258.00	636.0
265.00	248.0
273.00	361.0
274.00	889.0
275.00	5598.0
276.00	754.0
276.90	514.0
296.00	1399.0
297.00	161.0
303.00	209.0
314.90	176.0
323.00	392.0
334.00	267.0
365.00	570.0
372.00	221.0
423.00	810.0
424.00	398.0
441.00	2178.0
442.00	13858.0
443.00	2978.0
443.90	264.0

Instrument :
BNA_M
ClientSampleId :
DFTPP029

m/z	Abundance
38.00	171.0
39.00	893.0
44.00	457.0
50.00	3230.0
51.10	12396.0
52.00	748.0
55.90	415.0
57.00	796.0
61.00	162.0
62.00	188.0
63.00	510.0
64.90	207.0
69.00	11834.0
73.00	223.0
74.00	1244.0
75.00	2037.0
76.00	552.0
77.10	12937.0
78.00	886.0
79.00	853.0
80.00	731.0
81.00	964.0
82.00	218.0
83.00	240.0
85.00	189.0
86.00	359.0
92.00	279.0
93.00	1742.0
98.00	1324.0
99.00	928.0
100.90	493.0
103.00	242.0
103.90	326.0
104.90	368.0
107.00	3956.0
108.00	617.0
110.00	6830.0
111.00	1097.0
112.00	173.0
116.00	239.0
117.00	3901.0
117.90	269.0
121.90	267.0
123.00	406.0
124.00	205.0
127.00	13845.0
128.00	994.0
129.00	5541.0
130.00	505.0
133.90	175.0
135.00	446.0
136.00	202.0
136.90	301.0
141.00	781.0
141.90	239.0
147.00	412.0
148.00	952.0
149.00	205.0
152.90	199.0
153.90	188.0
154.90	494.0
156.00	627.0
159.90	199.0
161.00	385.0
165.00	248.0
165.90	174.0
167.00	1579.0
168.00	872.0
171.90	152.0
173.00	161.0
173.90	357.0
175.00	577.0
176.00	176.0
176.90	291.0
178.90	1178.0
180.00	884.0
181.00	333.0
185.00	620.0
186.00	4095.0
187.00	1098.0
188.90	270.0
191.00	194.0
192.00	318.0
193.00	391.0
196.00	720.0
197.10	168.0
198.00	27464.0
198.90	1969.0
199.90	163.0
202.90	194.0
204.00	1075.0
205.00	1542.0

Instrument :
BNA_M
ClientSampleId :
DFTPP029

206.00	7564.0
207.00	1340.0
208.00	276.0
211.00	228.0
216.00	155.0
217.00	1962.0
217.90	287.0
221.00	1143.0
221.90	220.0
222.90	417.0
224.00	3898.0
225.00	976.0
226.00	151.0
227.00	1797.0
228.00	298.0
229.00	348.0
230.90	163.0
236.90	279.0
243.00	204.0
244.00	3159.0
245.00	387.0
246.00	595.0
247.00	169.0
255.00	16194.0
256.00	2516.0
257.00	266.0
258.00	993.0
265.00	374.0
273.00	597.0
274.00	1375.0
275.00	7634.0
276.00	1067.0
277.00	737.0
296.00	2079.0
296.90	225.0
302.90	203.0
314.90	177.0
323.00	709.0
326.90	154.0
334.00	361.0
352.00	197.0
353.00	182.0
354.00	191.0
365.00	1137.0
372.00	362.0
403.00	288.0
421.90	210.0
423.00	1175.0
424.00	503.0
441.00	3504.0
442.00	23848.0
443.00	4742.0
444.00	380.0

Instrument :
BNA_M
ClientSampleId :
DFTPP029

m/z	Abundance
39.10	577.0
44.00	465.0
50.10	2225.0
51.10	7496.0
52.10	361.0
56.00	233.0
56.90	498.0
63.00	321.0
68.00	176.0
69.00	7516.0
72.90	159.0
74.00	775.0
75.10	1138.0
76.10	488.0
77.10	7938.0
78.00	568.0
79.00	625.0
79.90	384.0
81.00	554.0
82.00	160.0
83.00	152.0
85.90	209.0
91.90	171.0
93.00	1092.0
98.00	836.0
99.00	640.0
100.90	250.0
104.00	218.0
104.90	215.0
107.00	2802.0
108.00	383.0
110.00	4727.0
111.00	605.0
115.90	154.0
117.00	2588.0
117.90	240.0
121.90	186.0
122.90	353.0
127.00	9678.0
128.00	695.0
129.00	3865.0
130.00	362.0
135.00	366.0
137.00	159.0
141.00	568.0
146.90	304.0
147.90	656.0
155.00	220.0
156.00	453.0
161.00	260.0
164.90	182.0
166.00	166.0
167.00	1021.0
168.00	625.0
174.00	249.0
174.90	372.0
176.90	208.0
178.90	714.0
180.00	601.0
180.90	220.0
185.00	374.0
186.00	2711.0
187.00	765.0
188.90	242.0
192.00	248.0
192.90	250.0
196.00	654.0
197.00	166.0
198.00	19856.0
199.00	1172.0
202.90	179.0
204.00	804.0
205.00	1332.0
206.00	5639.0
207.00	931.0
208.00	221.0
211.00	235.0
217.00	1510.0
218.00	183.0
221.00	1042.0
221.90	170.0
222.90	319.0
224.00	3257.0
225.00	825.0
227.00	1403.0
227.90	182.0
229.00	305.0
236.90	186.0
241.90	185.0
244.00	2412.0
245.00	374.0
246.00	433.0

Instrument :
BNA_M
ClientSampleId :
DFTPP029

255.00	13284.0
256.00	1934.0
256.90	152.0
258.00	695.0
265.00	383.0
273.00	439.0
274.00	1084.0
275.00	6445.0
276.00	833.0
276.90	530.0
296.00	1715.0
296.90	319.0
303.00	200.0
314.90	212.0
323.00	664.0
333.90	344.0
352.00	181.0
354.00	160.0
364.90	923.0
372.00	362.0
403.00	181.0
421.00	176.0
421.90	194.0
423.00	1377.0
423.90	361.0
441.00	3646.0
442.00	23608.0
443.00	4493.0
444.00	318.0

Instrument :
BNA_M
ClientSampleId :
DFTPP029