

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044133.D
 Acq On : 16 Feb 2024 11:31
 Operator : MA/JU
 Sample : P1305-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FQ1

Quant Time: Feb 16 22:38:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.901	152	8298	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	28721	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	15324	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.398	188	2016599	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.50
23) Perylene-d12	23.891	264	22548	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	53142	4.522	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	12925	0.321	ng/ul	0.00
18) Fluoranthene-d10	19.331	212	23951	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
25) Benzo(k)fluoranthene	23.166	252	2634	0.026	ng/ul#	1
26) Benzo(a)pyrene	23.739	252	6277	0.073	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044133.D
Acq On : 16 Feb 2024 11:31
Operator : MA/JU
Sample : P1305-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FQ1


Quant Time: Feb 16 22:38:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

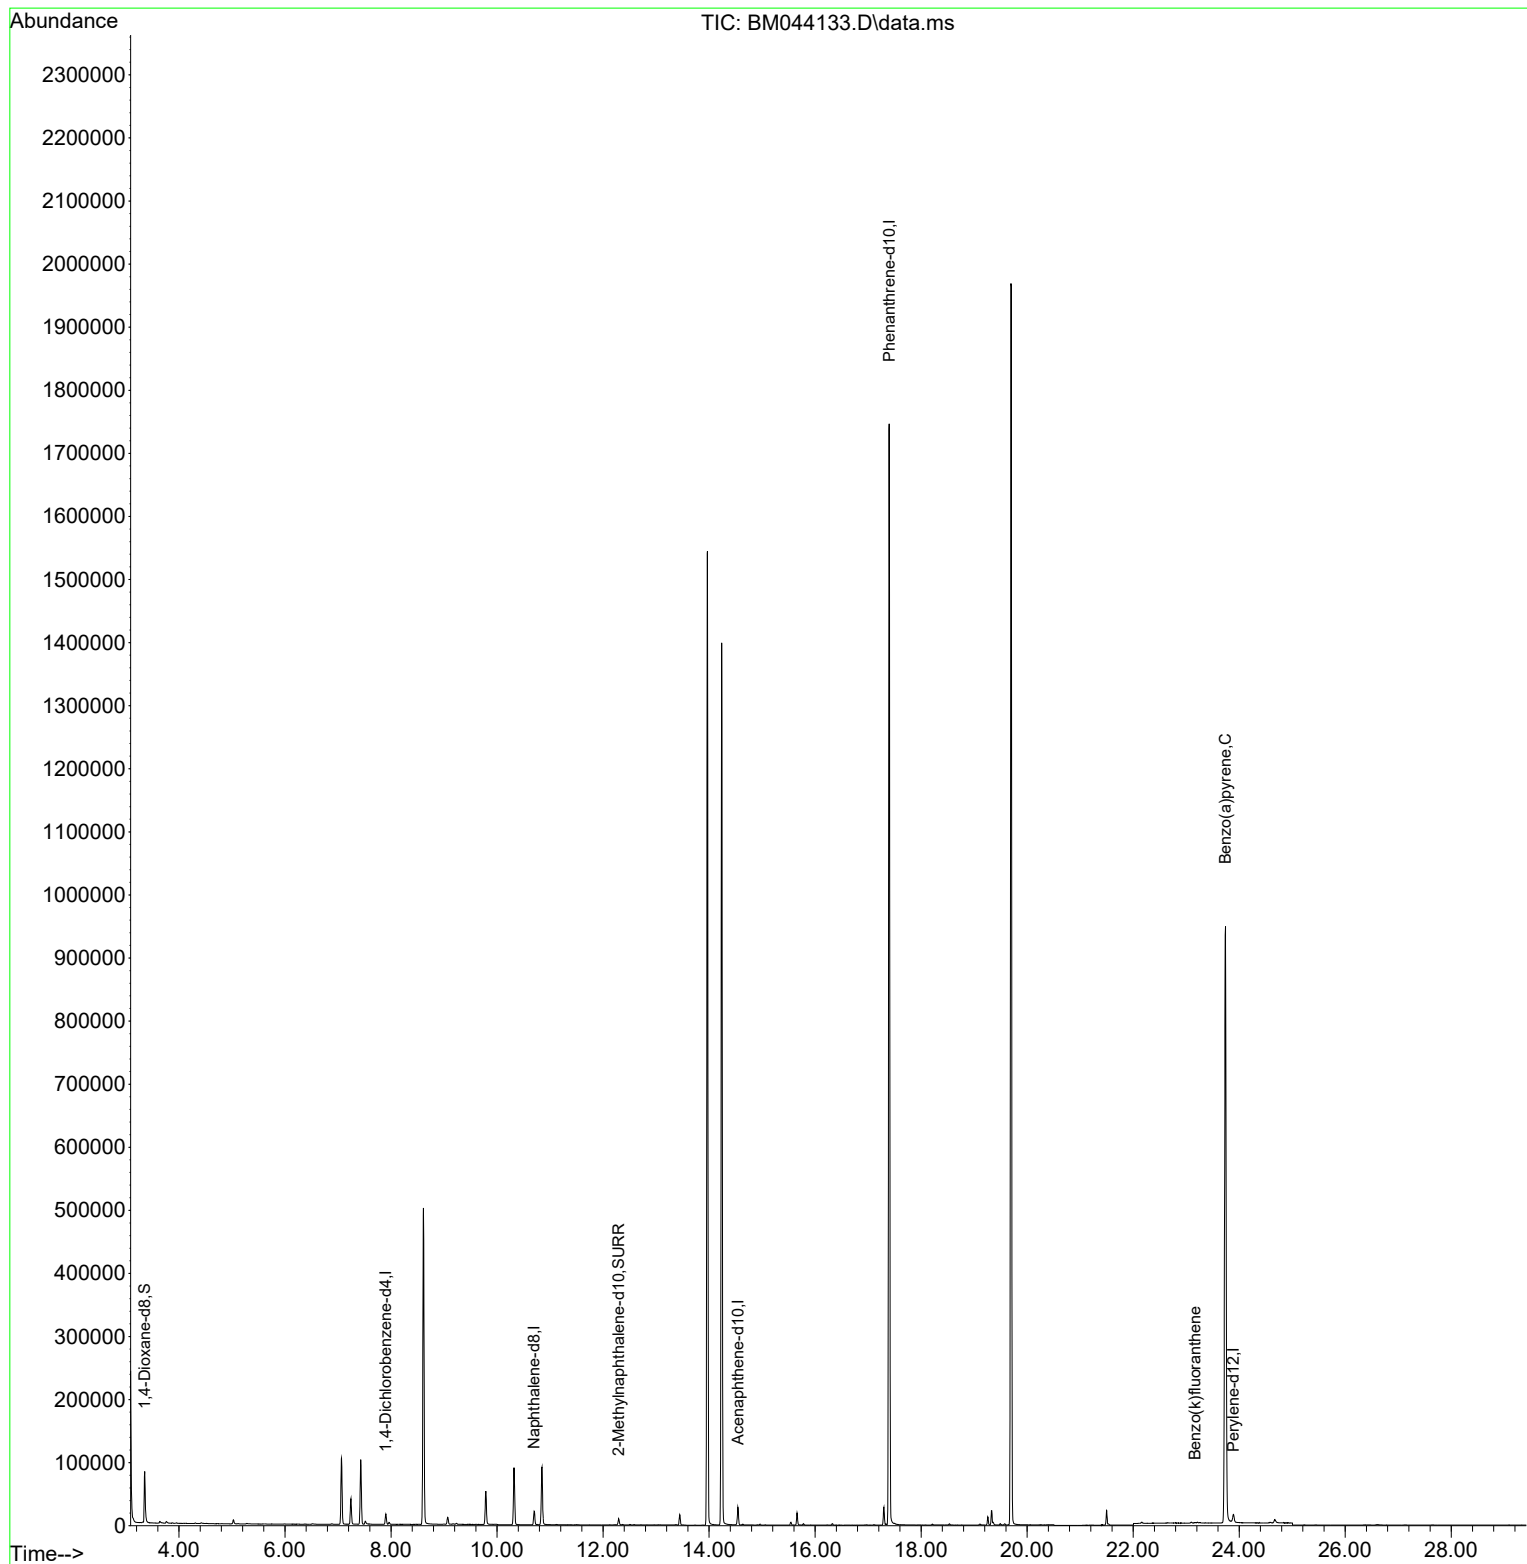



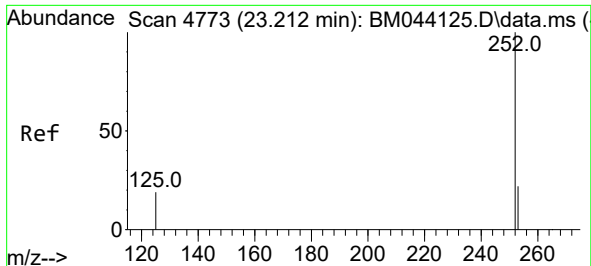


#25
Benzo(k)fluoranthene
Concen: 0.026 ng/ul
RT: 23.166 min Scan# 41
Delta R.T. -0.047 min
Lab File: BM044133.D
Acq: 16 Feb 2024 11:31

Instrument :
BNA_M
ClientSampleId :
C0FQ1

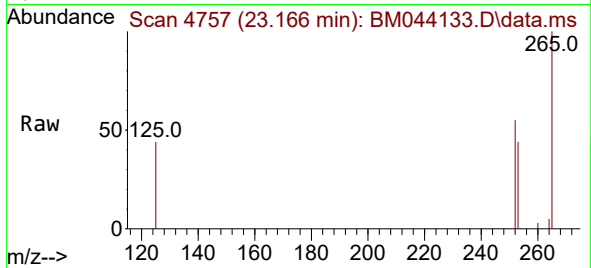

Tgt Ion:252 Resp: 2634
Ion Ratio Lower Upper
252 100
253 79.4 20.1 30.1#
125 79.0 12.3 18.5#

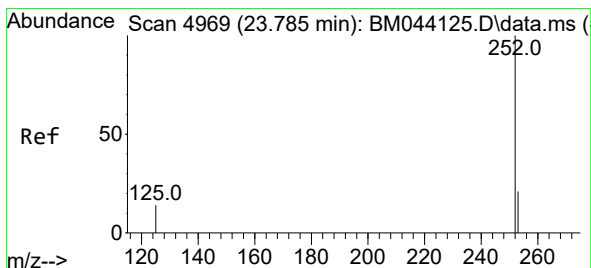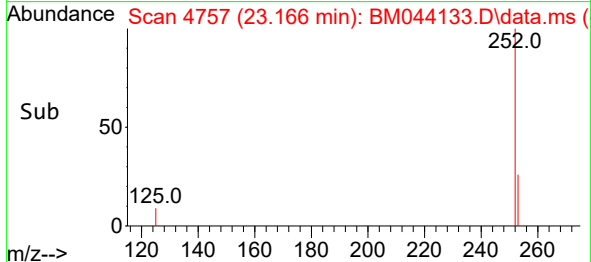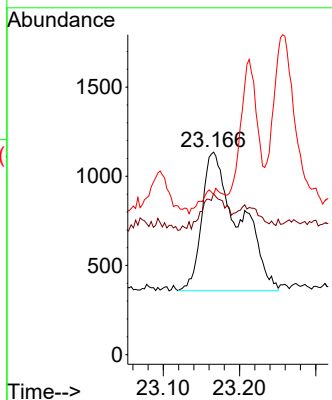

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.739 min Scan# 4953
Delta R.T. -0.047 min
Lab File: BM044133.D
Acq: 16 Feb 2024 11:31

Tgt Ion:252 Resp: 6277
Ion Ratio Lower Upper
252 100
253 48.8 21.4 32.2#
125 42.6 13.3 19.9#

