

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044142.D
 Acq On : 16 Feb 2024 17:35
 Operator : MA/JU
 Sample : PB158870BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK870

Quant Time: Feb 16 22:39:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.901	152	9347	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	31952	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	17227	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.394	188	2494268	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.50
23) Perylene-d12	23.891	264	34282	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	83004	6.271	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	16063	0.359	ng/ul	0.00
18) Fluoranthene-d10	19.331	212	28242	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.542	166	5169	0.067	ng/ul#	12
26) Benzo(a)pyrene	23.739	252	6407	0.049	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044142.D
Acq On : 16 Feb 2024 17:35
Operator : MA/JU
Sample : PB158870BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK870

Quant Time: Feb 16 22:39:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration




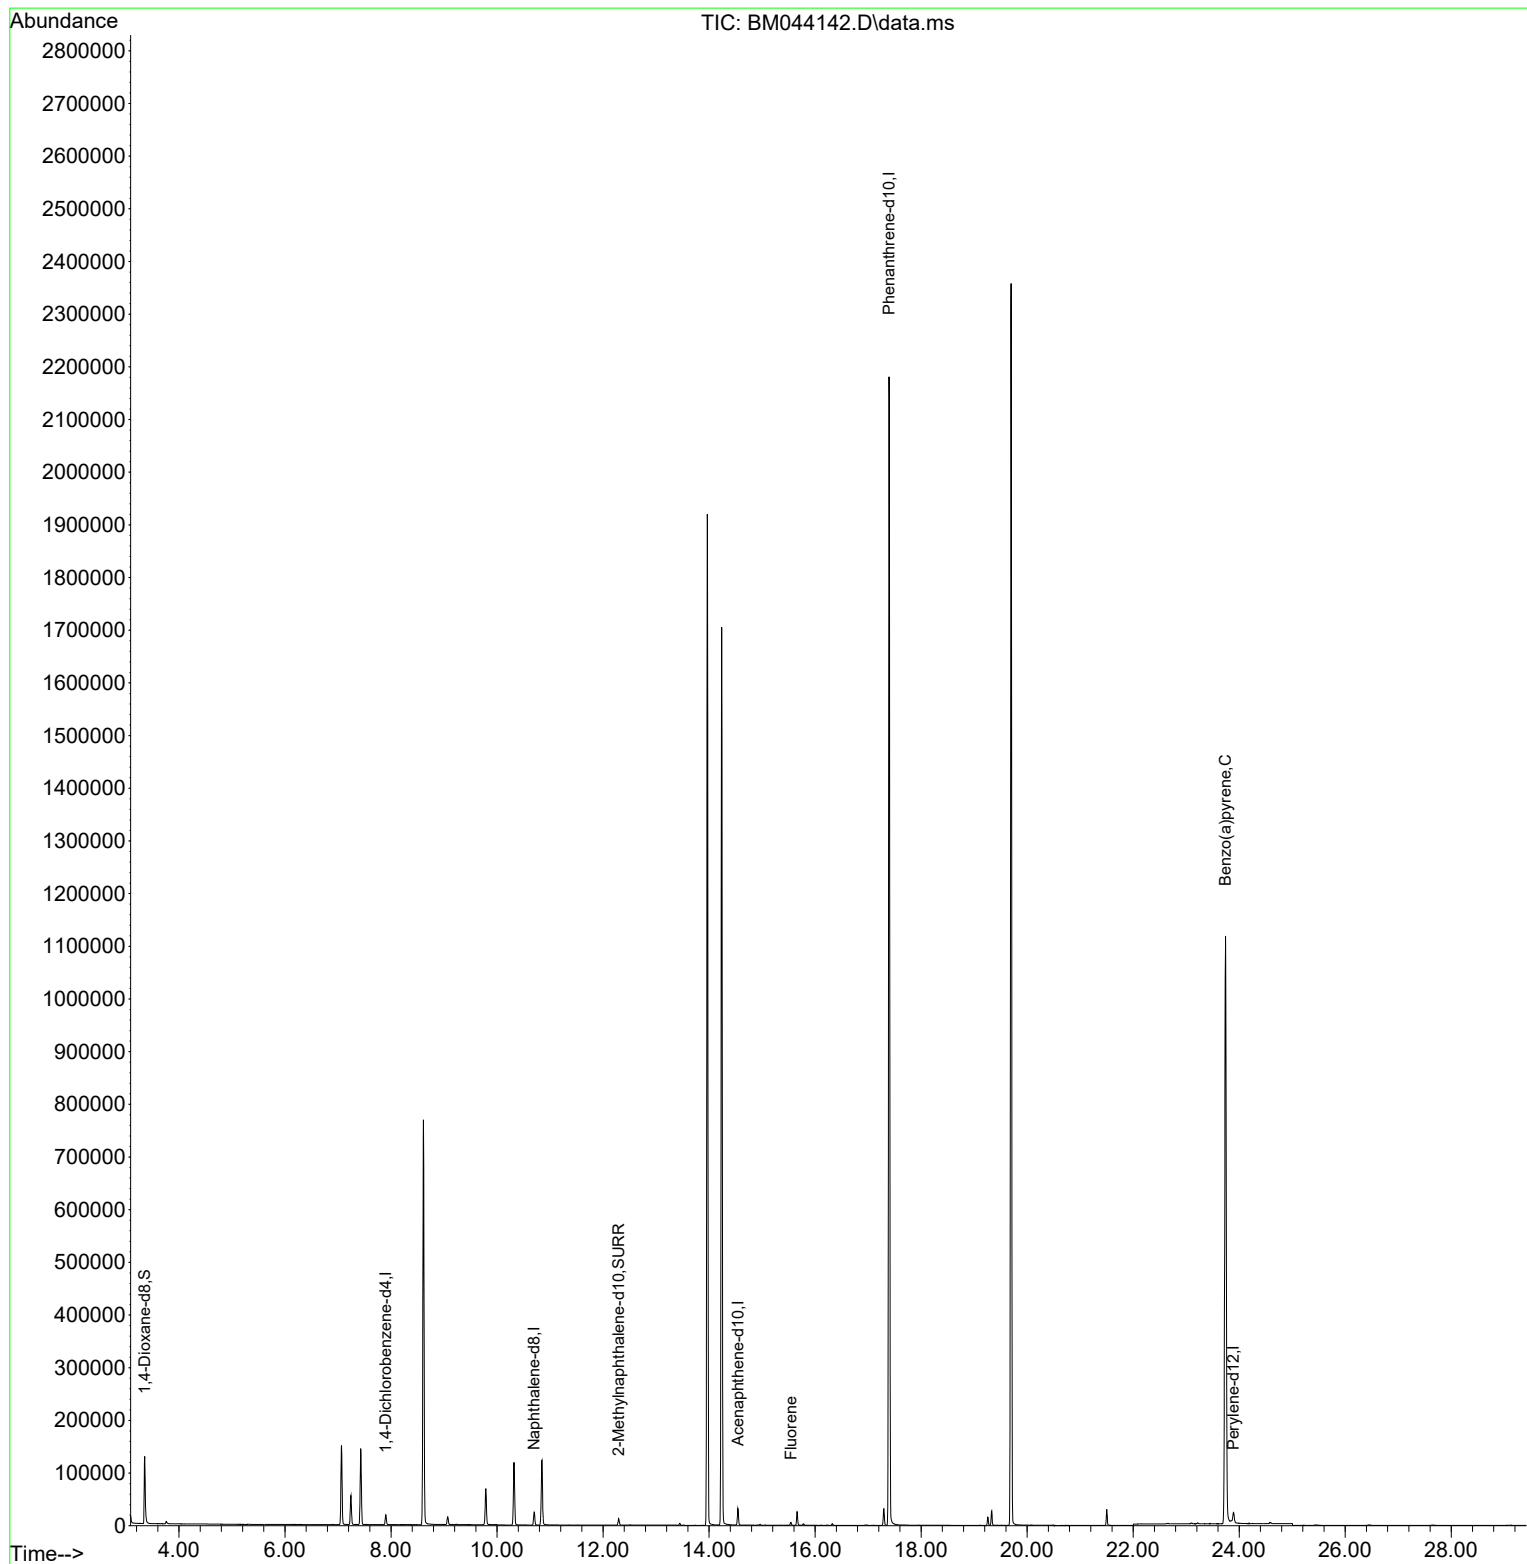


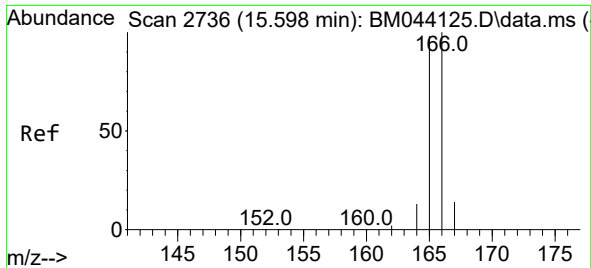

#12
Fluorene
Concen: 0.067 ng/ul
RT: 15.542 min Scan# 21
Delta R.T. -0.055 min
Lab File: BM044142.D
Acq: 16 Feb 2024 17:35

Instrument :
BNA_M
ClientSampleId :
SBLK870

Tgt Ion:166 Resp: 5169
Ion Ratio Lower Upper
166 100
165 6.8 79.8 119.6#
167 35.2 11.1 16.7#

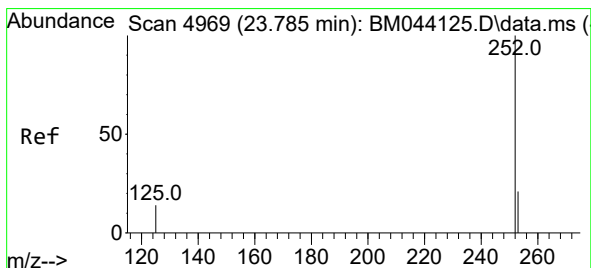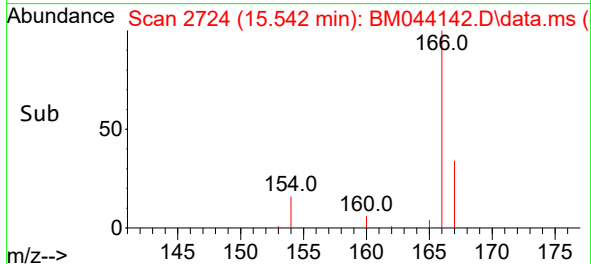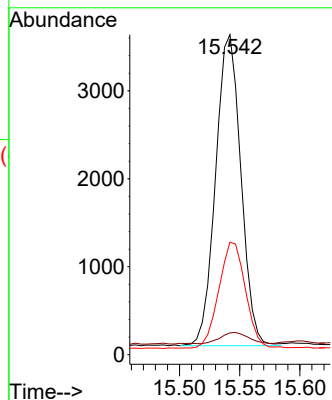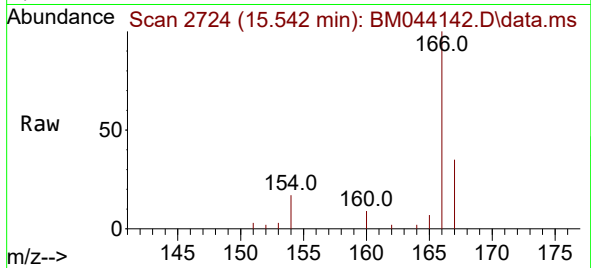

#26
Benzo(a)pyrene
Concen: 0.049 ng/ul
RT: 23.739 min Scan# 4953
Delta R.T. -0.047 min
Lab File: BM044142.D
Acq: 16 Feb 2024 17:35

Tgt Ion:252 Resp: 6407
Ion Ratio Lower Upper
252 100
253 43.0 21.4 32.2#
125 37.3 13.3 19.9#

