

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044148.D
 Acq On : 16 Feb 2024 21:13
 Operator : MA/JU
 Sample : P1352-04
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FN7

Quant Time: Feb 16 22:40:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.901	152	8754	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	29308	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	15538	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.398	188	2668247	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.50
23) Perylene-d12	23.888	264	19766	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	57337	4.625	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	16355	0.399	ng/ul	0.00
18) Fluoranthene-d10	19.331	212	32528	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.542	166	5790	0.083	ng/ul#	12
26) Benzo(a)pyrene	23.738	252	6727	0.089	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044148.D
Acq On : 16 Feb 2024 21:13
Operator : MA/JU
Sample : P1352-04
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FN7

Quant Time: Feb 16 22:40:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration




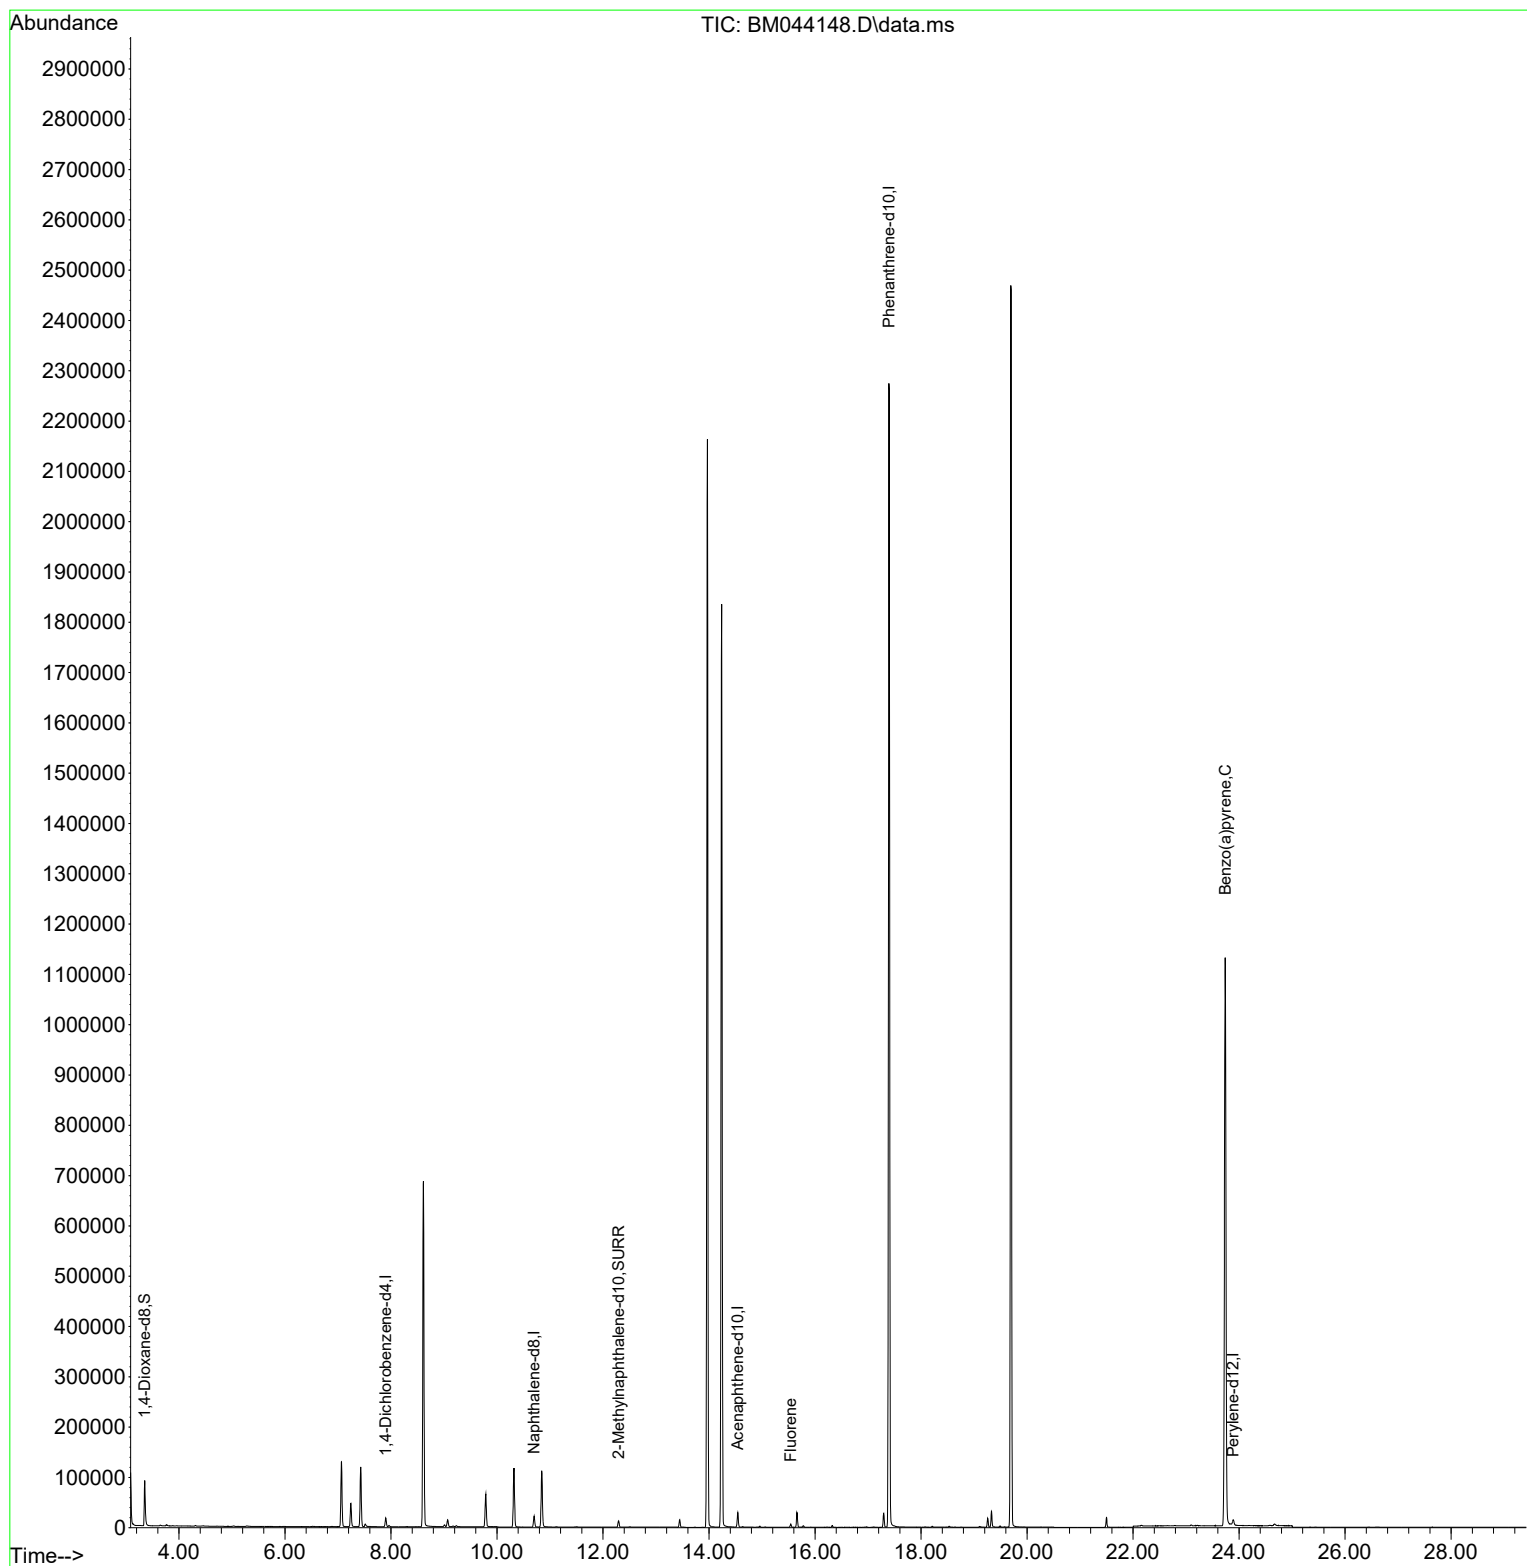


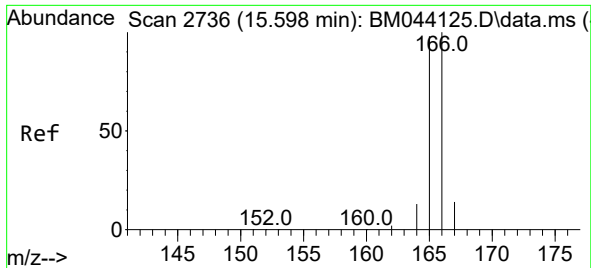

#12
Fluorene
Concen: 0.083 ng/u1
RT: 15.542 min Scan# 21
Delta R.T. -0.055 min
Lab File: BM044148.D
Acq: 16 Feb 2024 21:13

Instrument :
BNA_M
ClientSampleId :
C0FN7

Tgt Ion:166 Resp: 5790
Ion Ratio Lower Upper
166 100
165 6.5 79.8 119.6#
167 33.5 11.1 16.7#

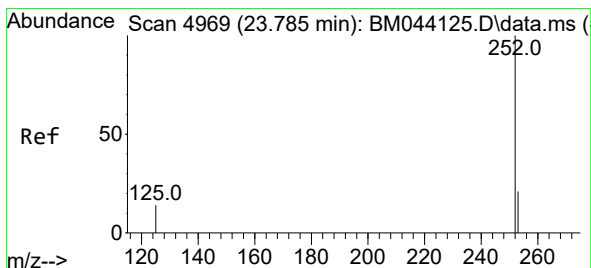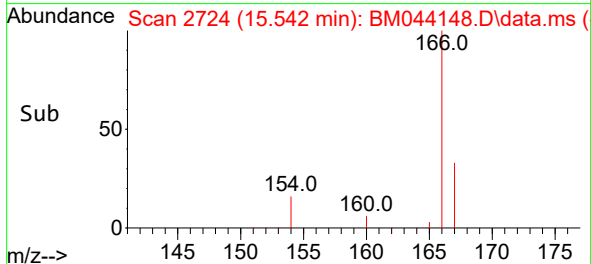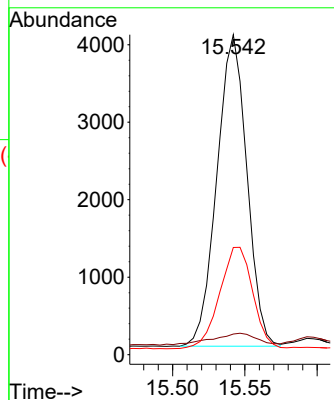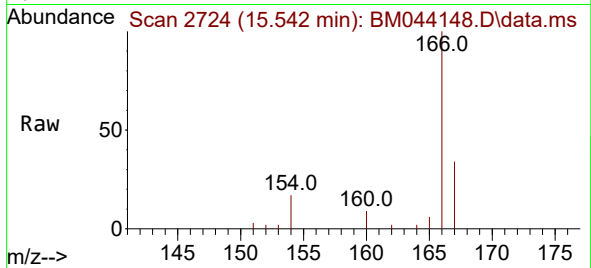

#26
Benzo(a)pyrene
Concen: 0.089 ng/u1
RT: 23.738 min Scan# 4953
Delta R.T. -0.047 min
Lab File: BM044148.D
Acq: 16 Feb 2024 21:13

Tgt Ion:252 Resp: 6727
Ion Ratio Lower Upper
252 100
253 41.7 21.4 32.2#
125 39.4 13.3 19.9#

