

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044162.D
 Acq On : 17 Feb 2024 06:17
 Operator : MA/JU
 Sample : P1436-01
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7G5

Quant Time: Feb 18 23:55:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	7896	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	25359	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	13406	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.393	188	2692957	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.50
23) Perylene-d12	23.885	264	19997	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	43928	3.928	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.288	152	17176	0.484	ng/ul	-0.01
18) Fluoranthene-d10	19.326	212	31567	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.390	88	8024	0.718	ng/ul#	86
26) Benzo(a)pyrene	23.736	252	7086	0.092	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044162.D
Acq On : 17 Feb 2024 06:17
Operator : MA/JU
Sample : P1436-01
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G5


Quant Time: Feb 18 23:55:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

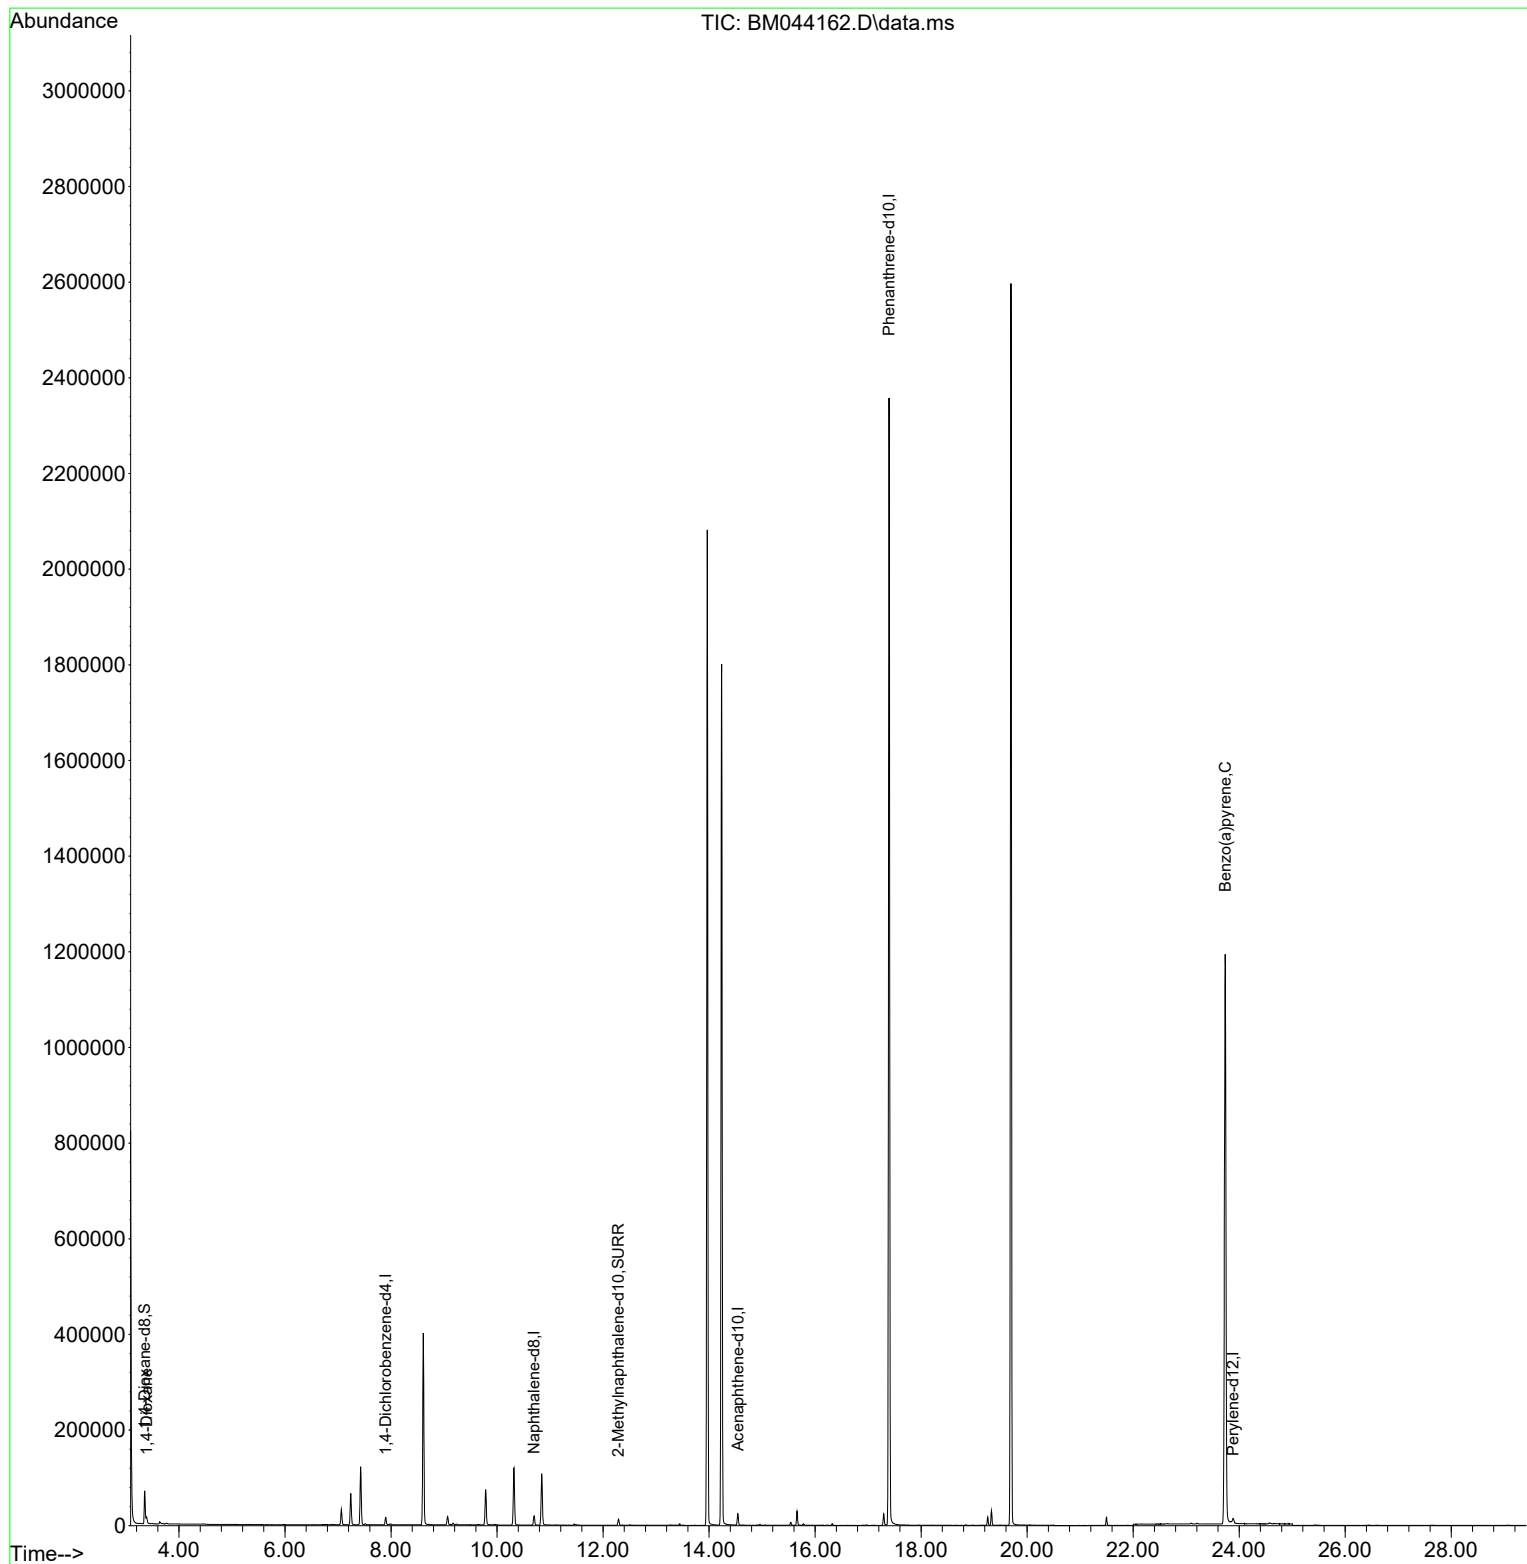



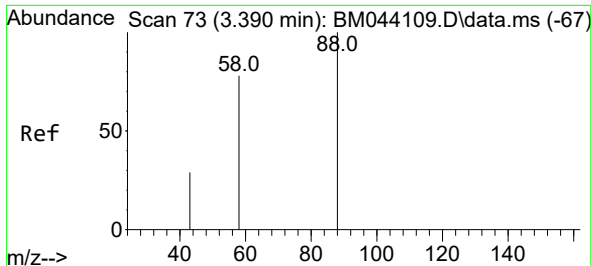


#2
1,4-Dioxane
Concen: 0.718 ng/ul
RT: 3.390 min Scan# 71
Delta R.T. 0.000 min
Lab File: BM044162.D
Acq: 17 Feb 2024 06:17

Instrument :
BNA_M
ClientSampleId :
BH7G5

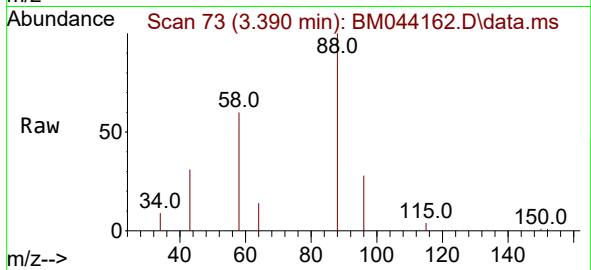

Tgt Ion: 88 Resp: 8024
Ion Ratio Lower Upper
88 100
43 30.8 32.2 48.2#
58 60.3 40.6 60.8

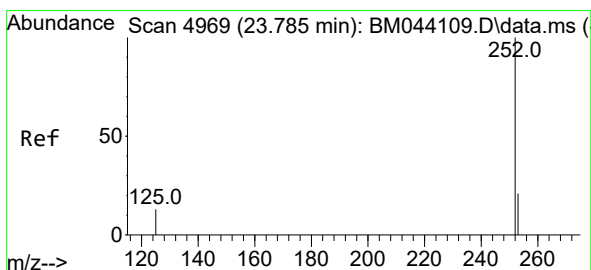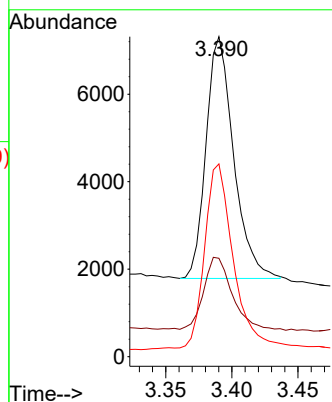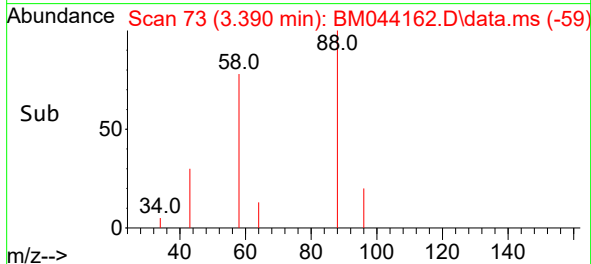

#26
Benzo(a)pyrene
Concen: 0.092 ng/ul
RT: 23.736 min Scan# 4952
Delta R.T. -0.050 min
Lab File: BM044162.D
Acq: 17 Feb 2024 06:17

Tgt Ion: 252 Resp: 7086
Ion Ratio Lower Upper
252 100
253 44.1 21.4 32.2#
125 35.3 13.3 19.9#

