

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044163.D
 Acq On : 17 Feb 2024 06:53
 Operator : MA/JU
 Sample : P1436-02
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7G6

Quant Time: Feb 18 23:55:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	8330	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	27051	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	13927	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.394	188	2710526	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.50
23) Perylene-d12	23.885	264	20567	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	50771	4.304	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.288	152	17514	0.462	ng/ul	-0.01
18) Fluoranthene-d10	19.326	212	32183	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.390	88	8865	0.752	ng/ul#	83
12) Fluorene	15.537	166	5759	0.092	ng/ul#	12
26) Benzo(a)pyrene	23.736	252	7271	0.092	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044163.D
Acq On : 17 Feb 2024 06:53
Operator : MA/JU
Sample : P1436-02
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G6

Quant Time: Feb 18 23:55:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration




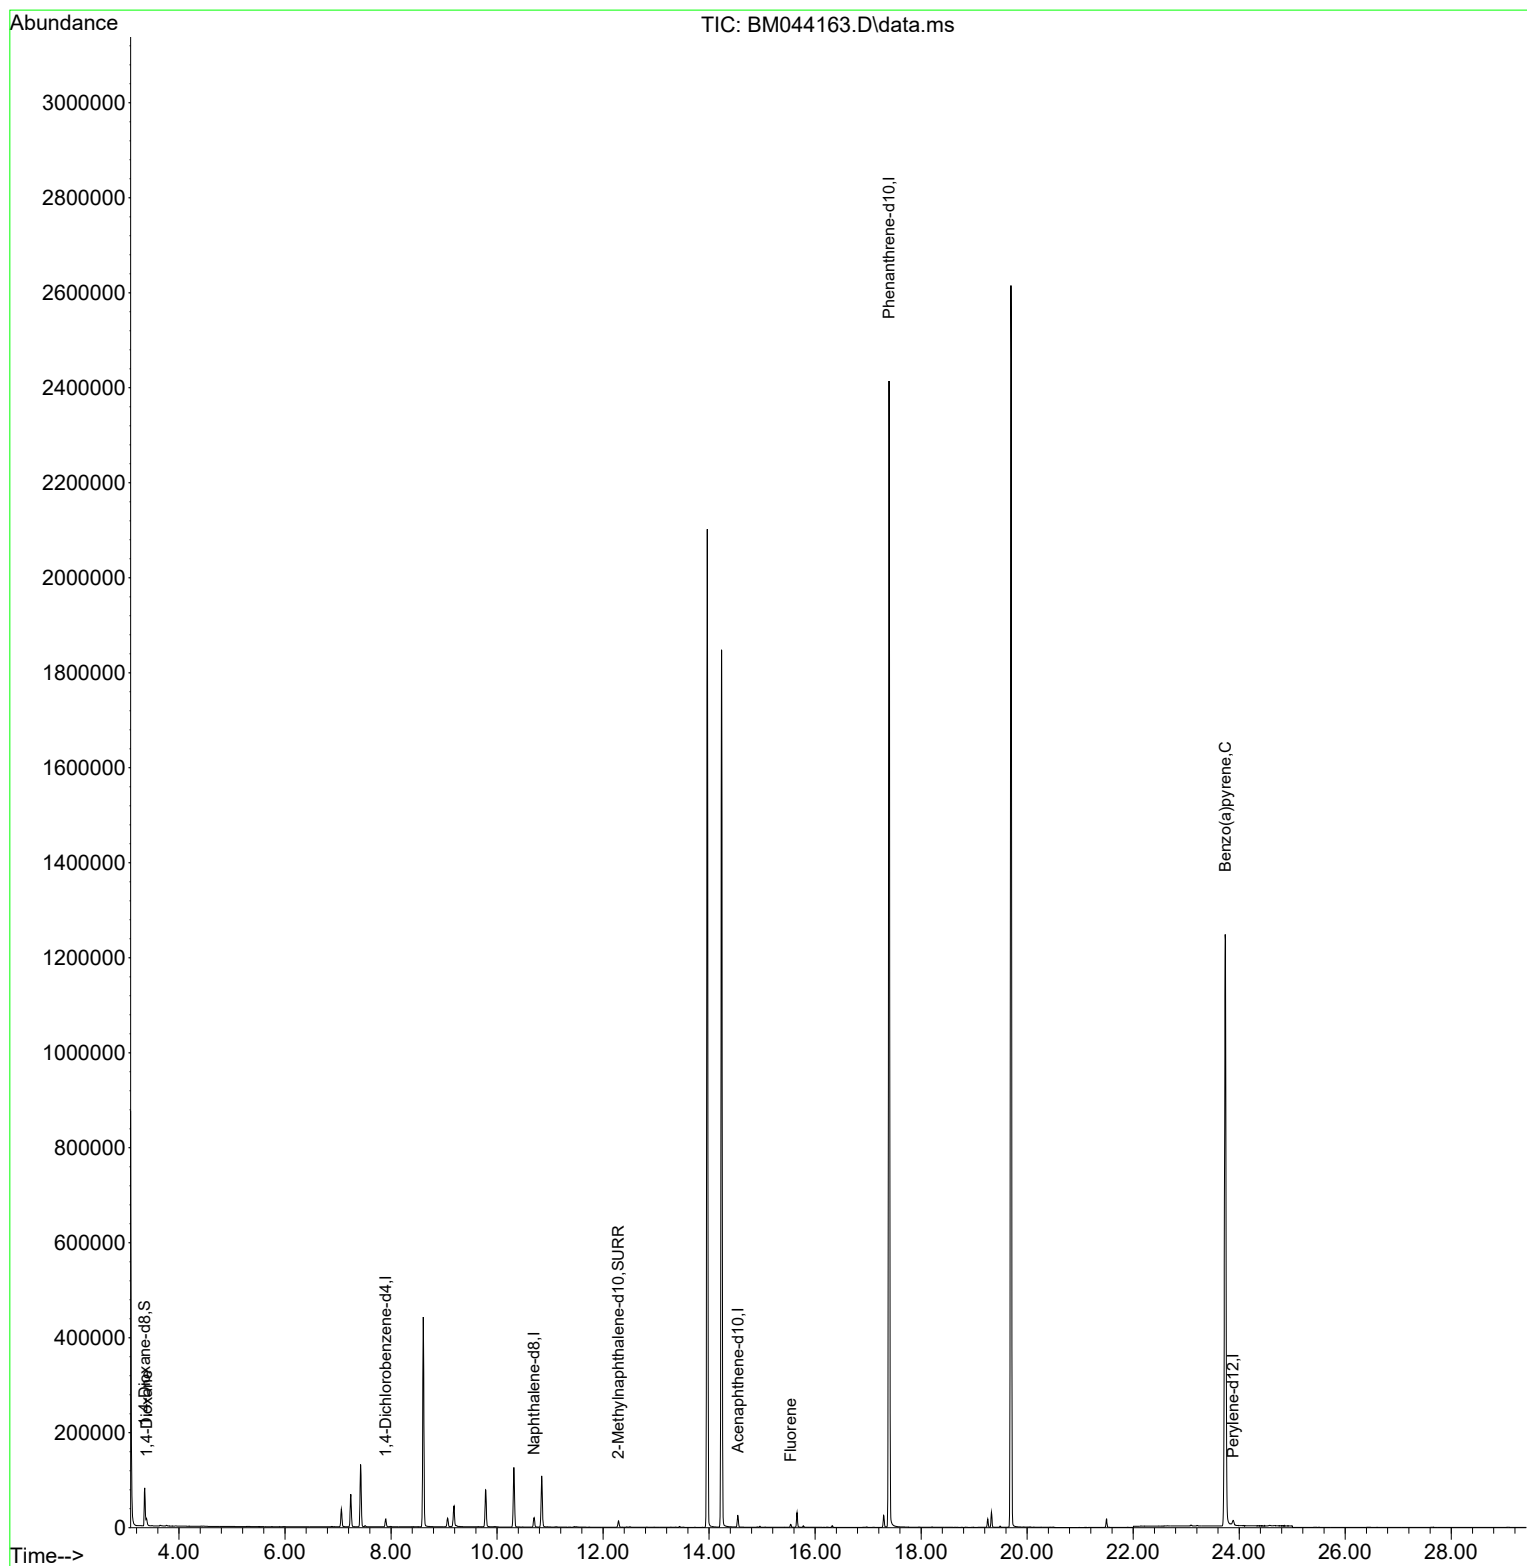


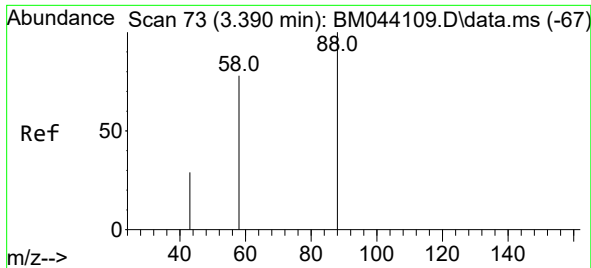

#2
1,4-Dioxane
Concen: 0.752 ng/ul
RT: 3.390 min Scan# 71
Delta R.T. 0.000 min
Lab File: BM044163.D
Acq: 17 Feb 2024 06:53




Instrument :
BNA_M
ClientSampleId :
BH7G6


Tgt Ion: 88 Resp: 8865
Ion Ratio Lower Upper
88 100
43 31.3 32.2 48.2#
58 63.4 40.6 60.8#

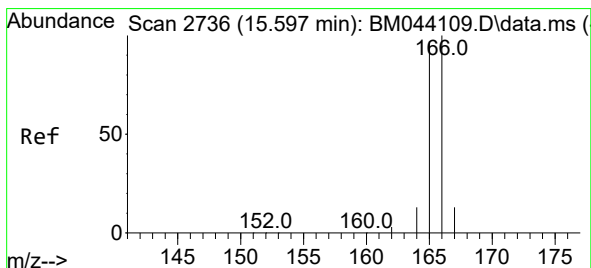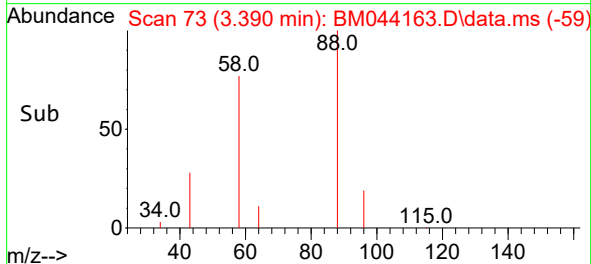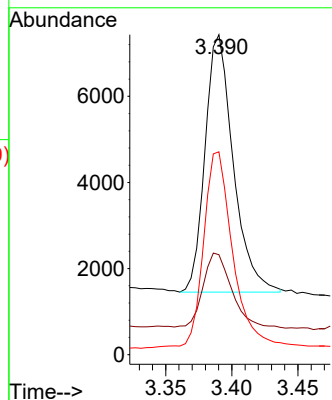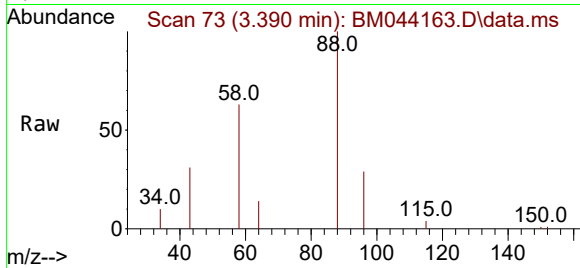

#12
Fluorene
Concen: 0.092 ng/ul
RT: 15.537 min Scan# 2723
Delta R.T. -0.060 min
Lab File: BM044163.D
Acq: 17 Feb 2024 06:53


Tgt Ion: 166 Resp: 5759
Ion Ratio Lower Upper
166 100
165 6.1 79.8 119.6#
167 32.2 11.1 16.7#

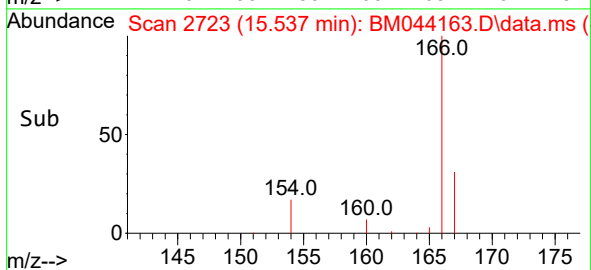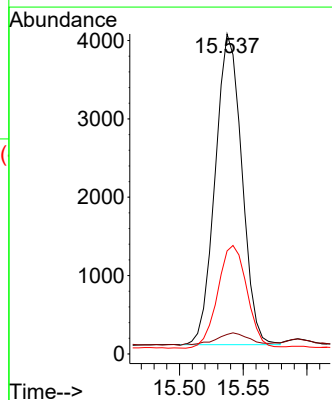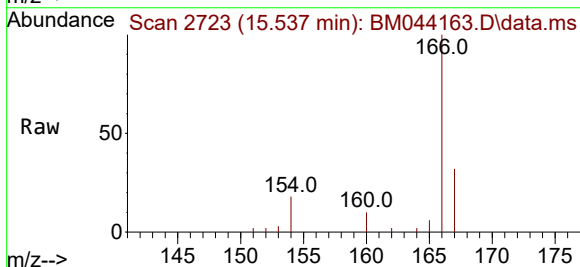

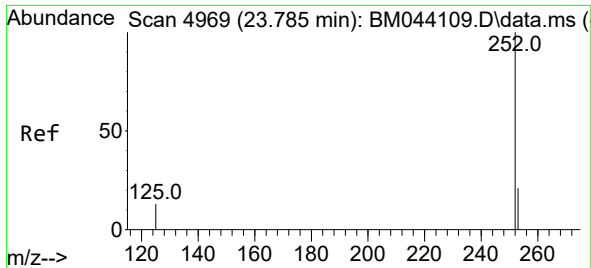

#26
Benzo(a)pyrene
Concen: 0.092 ng/ul
RT: 23.736 min Scan# 4969
Delta R.T. -0.050 min
Lab File: BM044163.D
Acq: 17 Feb 2024 06:53

Instrument :
BNA_M
ClientSampleId :
BH7G6

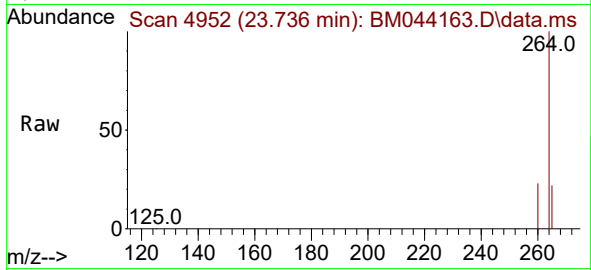

Tgt Ion:252 Resp: 7271
Ion Ratio Lower Upper
252 100
253 42.5 21.4 32.2#
125 35.4 13.3 19.9#

