

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044167.D
 Acq On : 17 Feb 2024 09:18
 Operator : MA/JU
 Sample : P1402-15
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD4

Quant Time: Feb 18 23:55:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.901	152	7960	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	26131	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	13628	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.394	188	2575641	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.50
23) Perylene-d12	23.888	264	22288	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	46018	4.082	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	14612	0.399	ng/ul	0.00
18) Fluoranthene-d10	19.326	212	31141	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.390	88	4143	0.368	ng/ul	96
12) Fluorene	15.537	166	5156	0.084	ng/ul#	13
26) Benzo(a)pyrene	23.739	252	7737	0.090	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044167.D
Acq On : 17 Feb 2024 09:18
Operator : MA/JU
Sample : P1402-15
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD4

Quant Time: Feb 18 23:55:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration




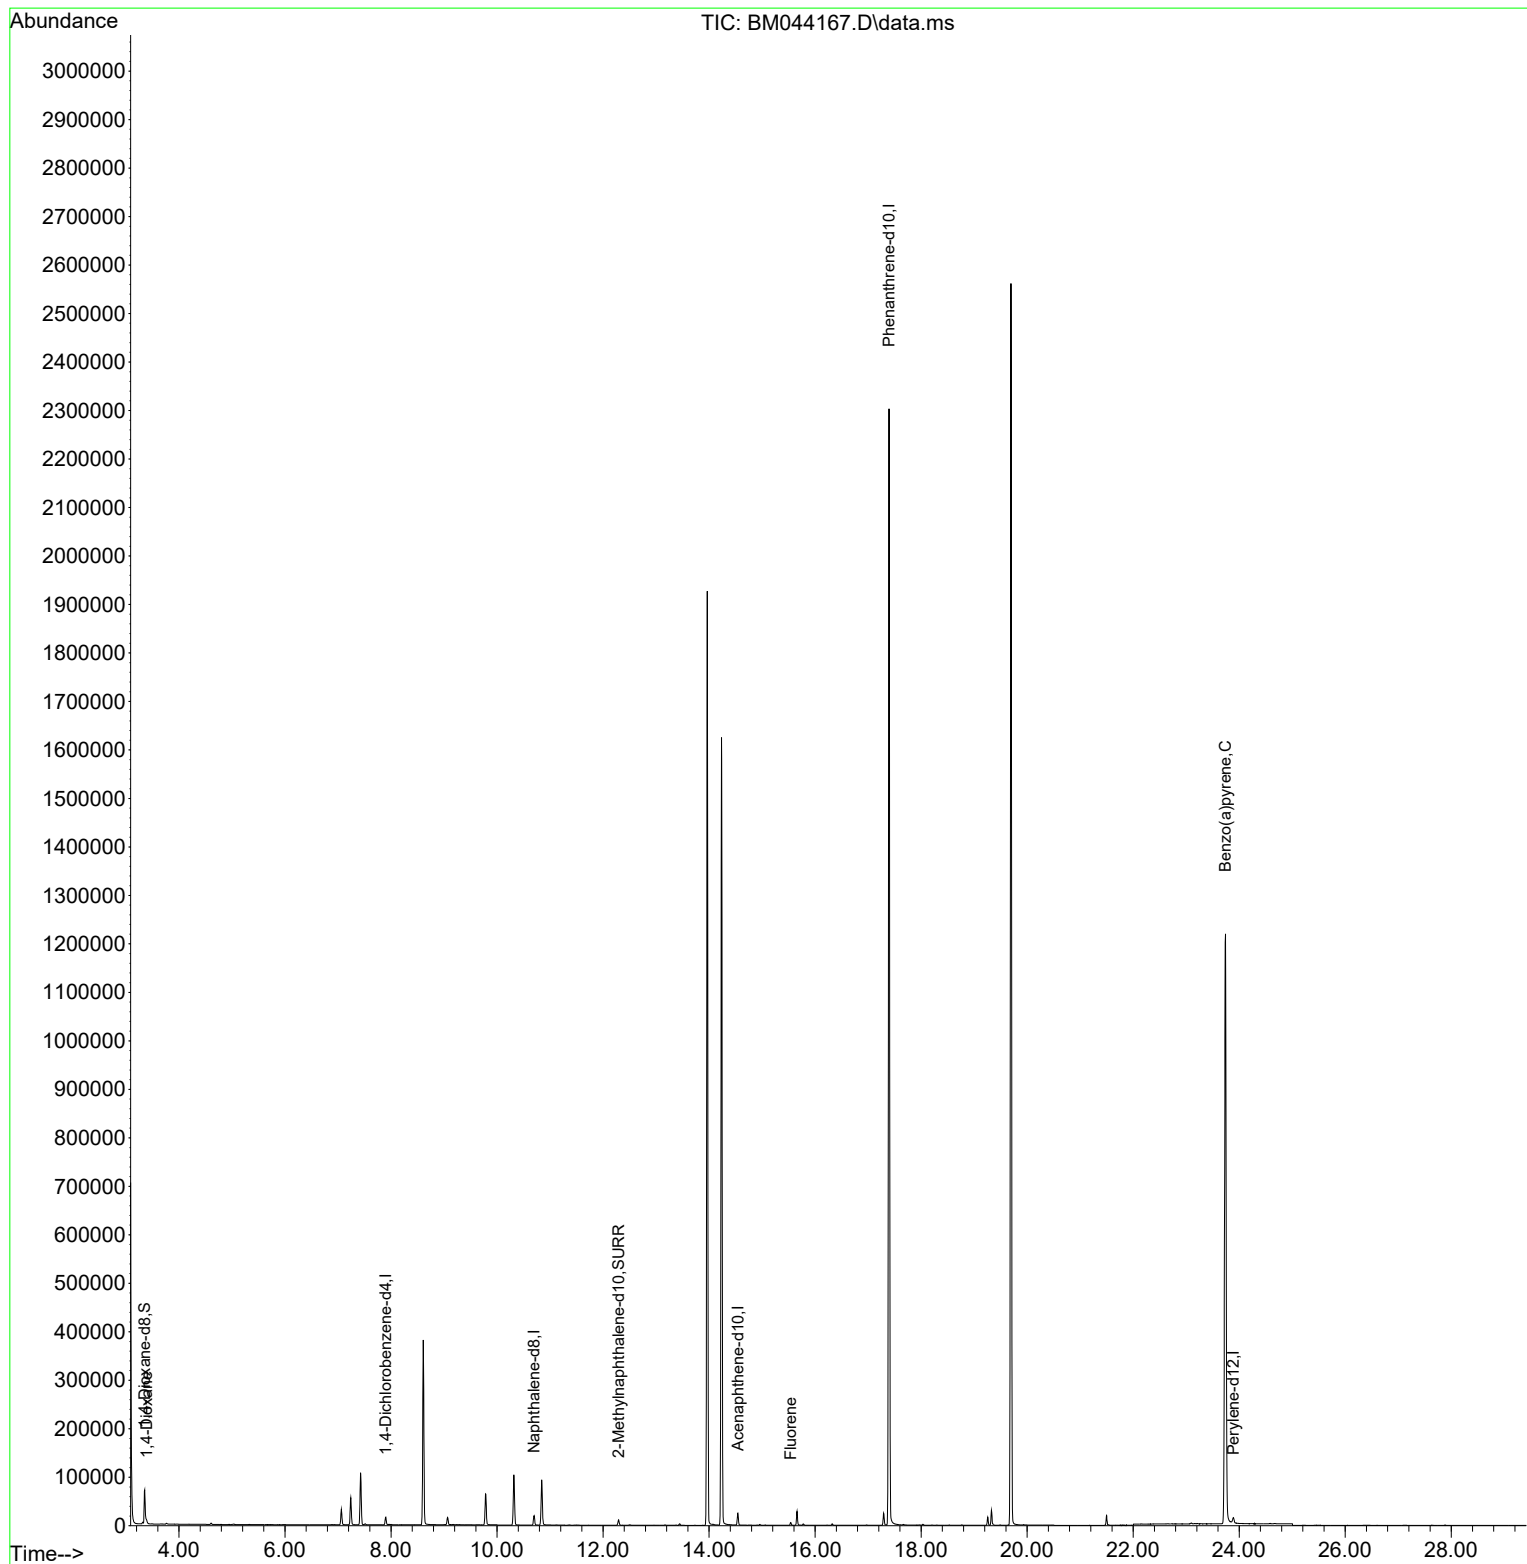


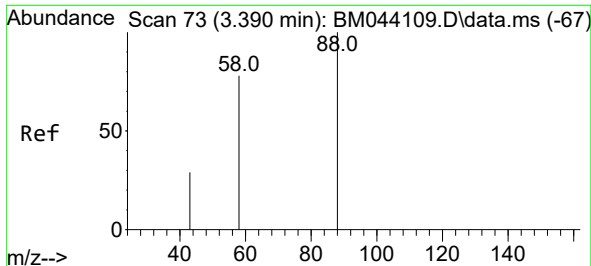

#2
1,4-Dioxane
Concen: 0.368 ng/ul
RT: 3.390 min Scan# 71
Delta R.T. 0.000 min
Lab File: BM044167.D
Acq: 17 Feb 2024 09:18




Instrument :
BNA_M
ClientSampleId :
C0AD4


Tgt Ion: 88 Resp: 4143
Ion Ratio Lower Upper
88 100
43 35.8 32.2 48.2
58 51.5 40.6 60.8

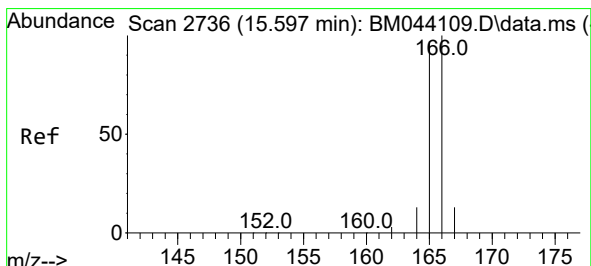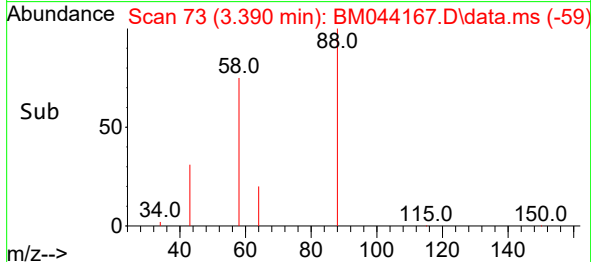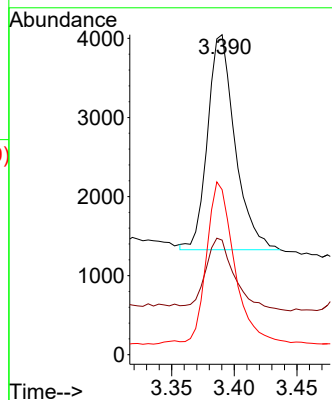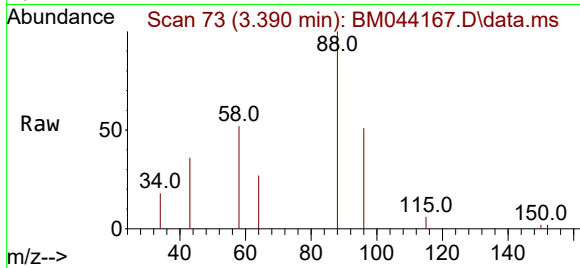

#12
Fluorene
Concen: 0.084 ng/ul
RT: 15.537 min Scan# 2723
Delta R.T. -0.060 min
Lab File: BM044167.D
Acq: 17 Feb 2024 09:18


Tgt Ion: 166 Resp: 5156
Ion Ratio Lower Upper
166 100
165 6.9 79.8 119.6#
167 33.0 11.1 16.7#

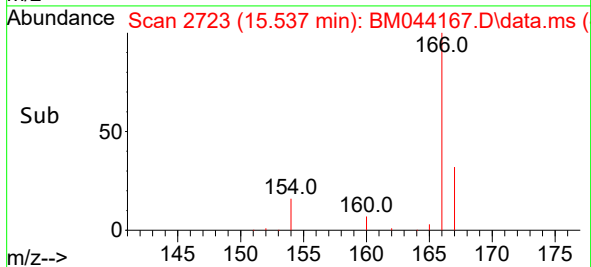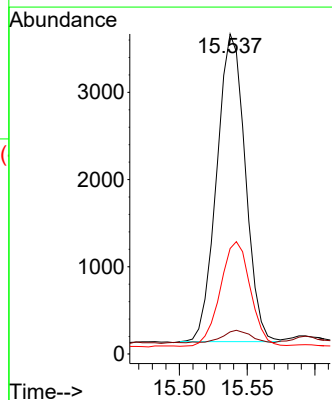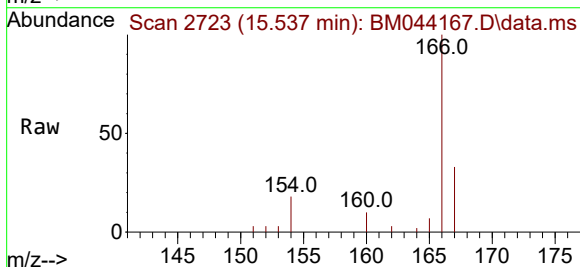

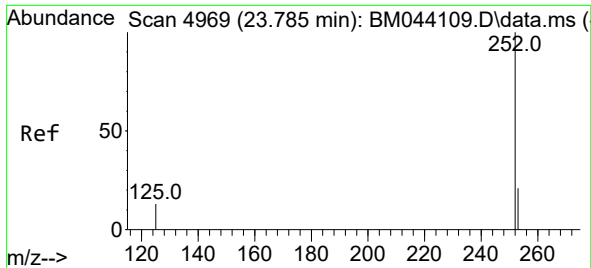

#26
Benzo(a)pyrene
Concen: 0.090 ng/ul
RT: 23.739 min Scan# 4953
Delta R.T. -0.047 min
Lab File: BM044167.D
Acq: 17 Feb 2024 09:18

Instrument :
BNA_M
ClientSampleId :
C0AD4

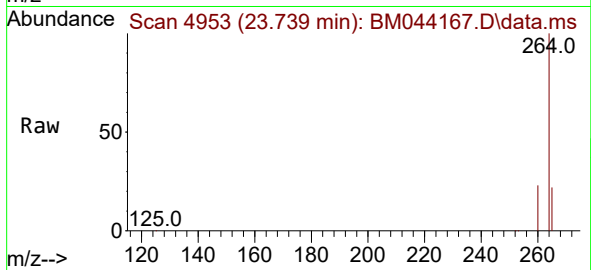

Tgt Ion:252 Resp: 7737
Ion Ratio Lower Upper
252 100
253 46.0 21.4 32.2#
125 35.6 13.3 19.9#

