

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044169.D
 Acq On : 17 Feb 2024 10:30
 Operator : MA/JU
 Sample : PB159059BL
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK059

Quant Time: Feb 18 23:56:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	6201	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	20350	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	10812	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.394	188	2132722	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.50
23) Perylene-d12	23.885	264	16521	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	71103	8.097	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	13291	0.466	ng/ul	0.00
18) Fluoranthene-d10	19.326	212	22901	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.537	166	4446	0.092	ng/ul#	13
26) Benzo(a)pyrene	23.736	252	5098	0.080	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044169.D
Acq On : 17 Feb 2024 10:30
Operator : MA/JU
Sample : PB159059BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK059

Quant Time: Feb 18 23:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration




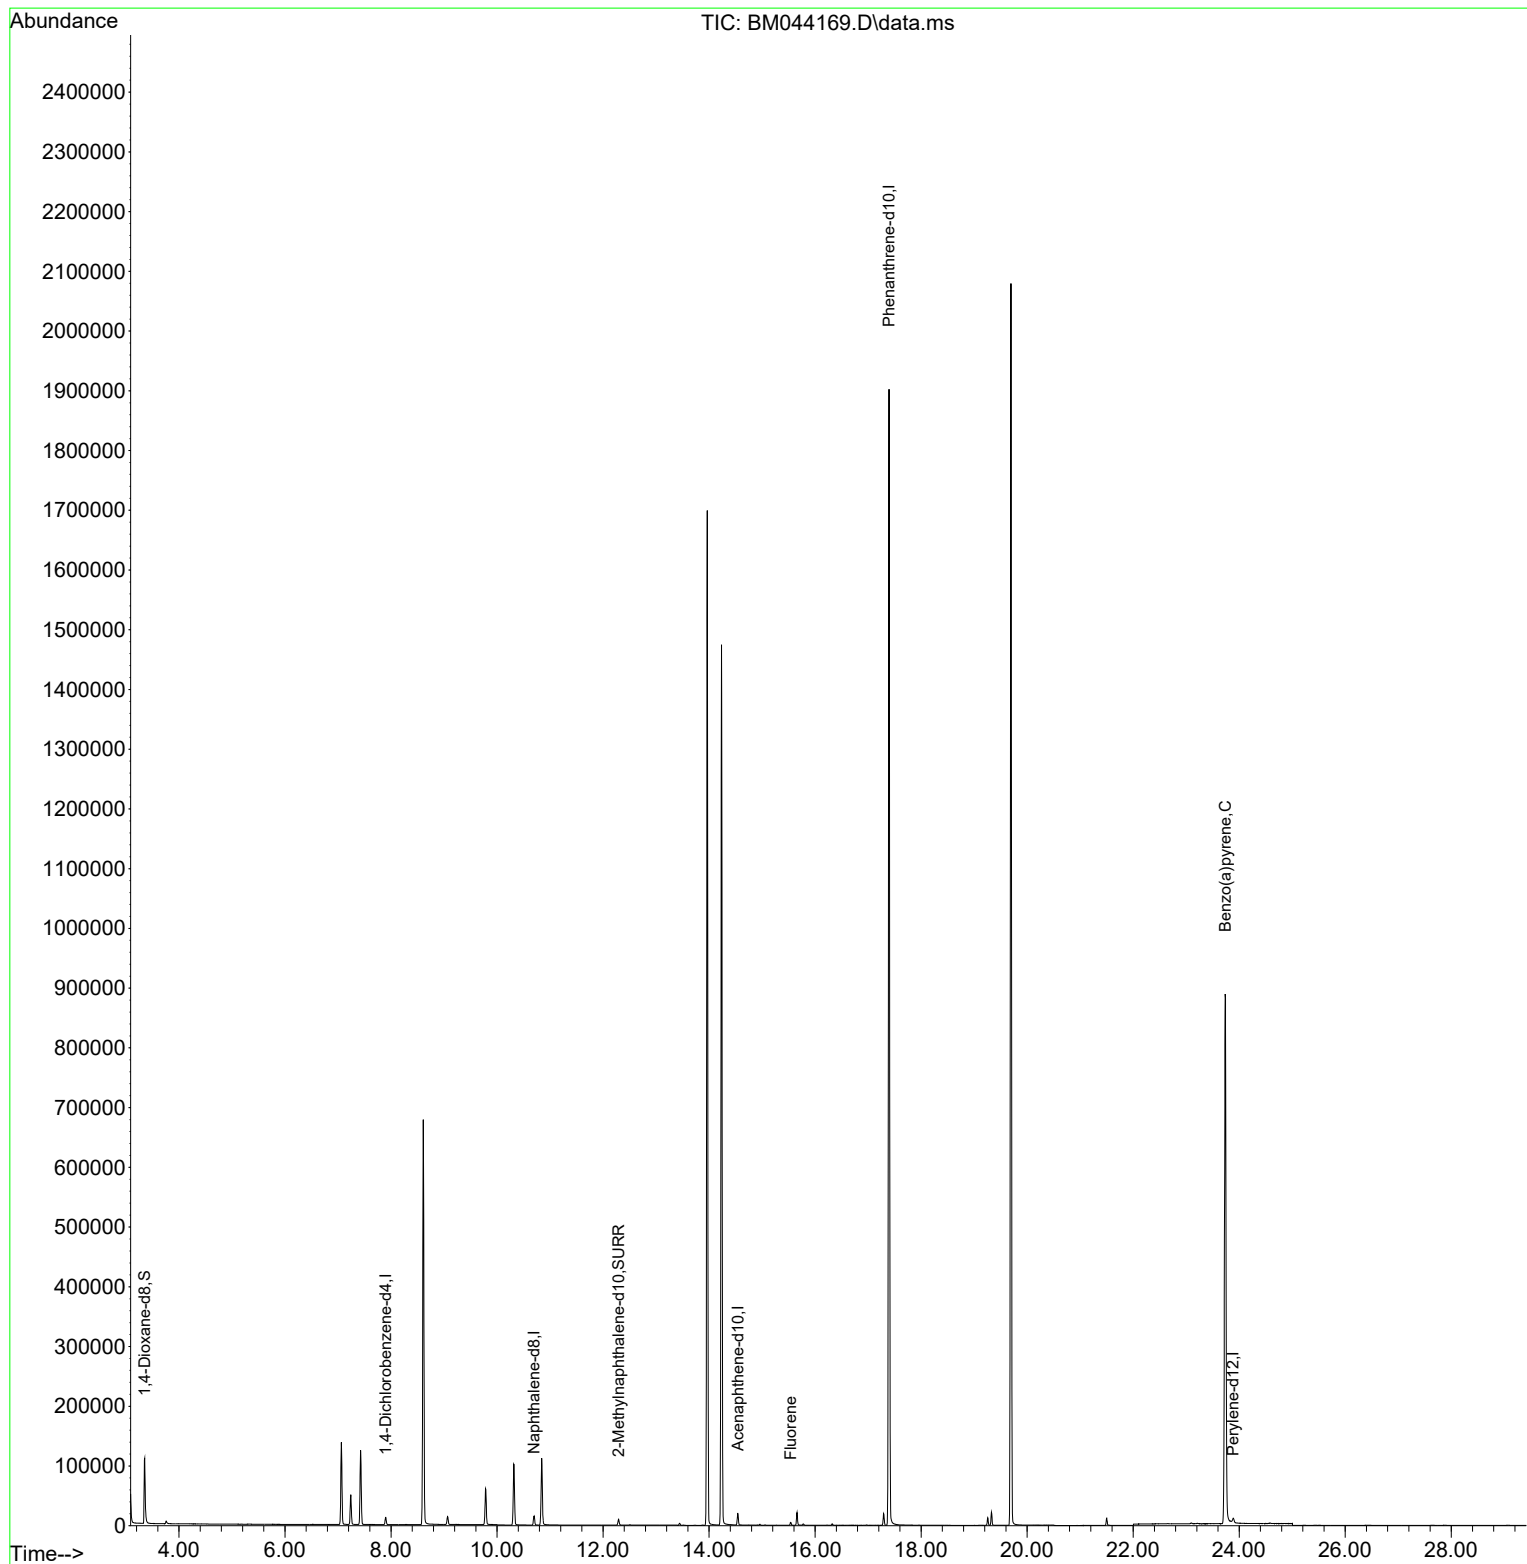


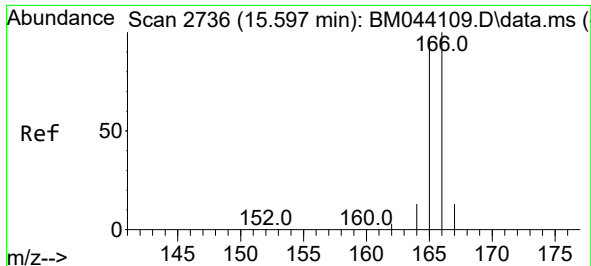

#12
Fluorene
Concen: 0.092 ng/ul
RT: 15.537 min Scan# 21
Delta R.T. -0.060 min
Lab File: BM044169.D
Acq: 17 Feb 2024 10:30

Instrument :
BNA_M
ClientSampleId :
SBLK059

Tgt Ion:166 Resp: 4446
Ion Ratio Lower Upper
166 100
165 6.9 79.8 119.6#
167 32.2 11.1 16.7#

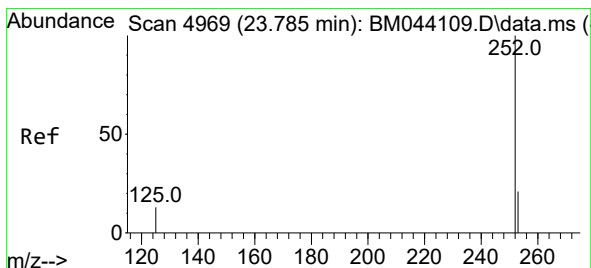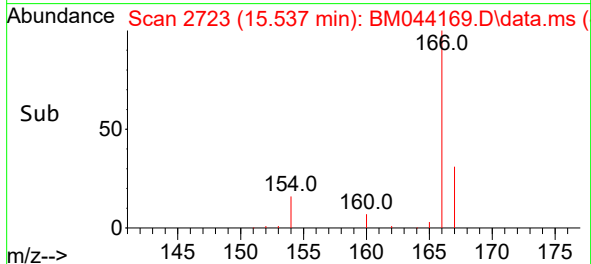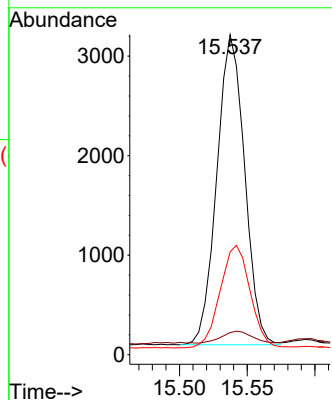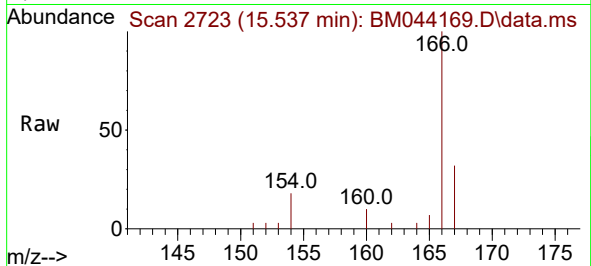

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.736 min Scan# 4952
Delta R.T. -0.050 min
Lab File: BM044169.D
Acq: 17 Feb 2024 10:30

Tgt Ion:252 Resp: 5098
Ion Ratio Lower Upper
252 100
253 47.0 21.4 32.2#
125 37.0 13.3 19.9#

