




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

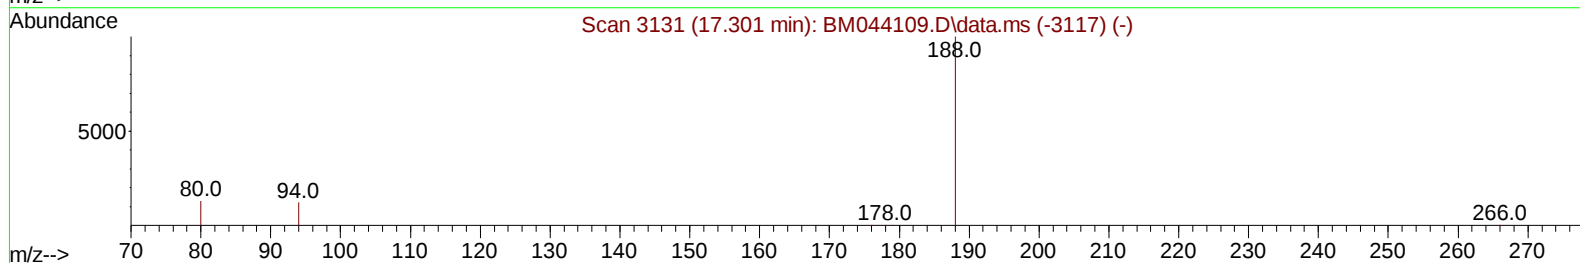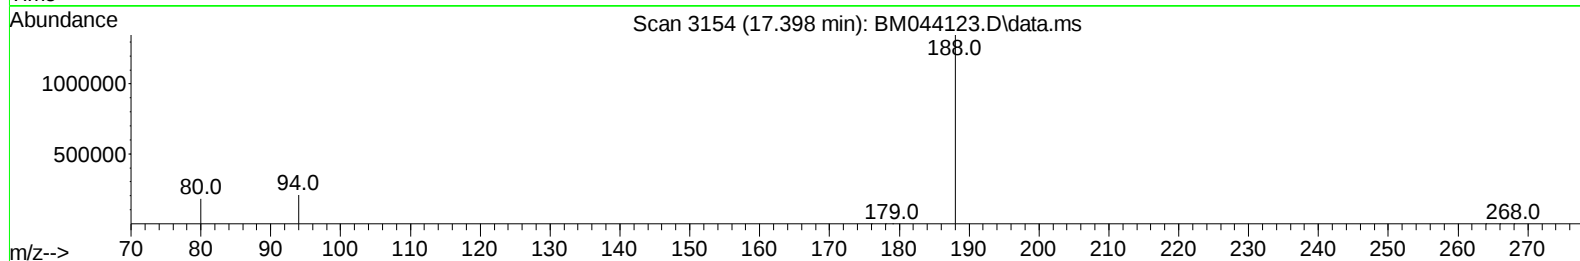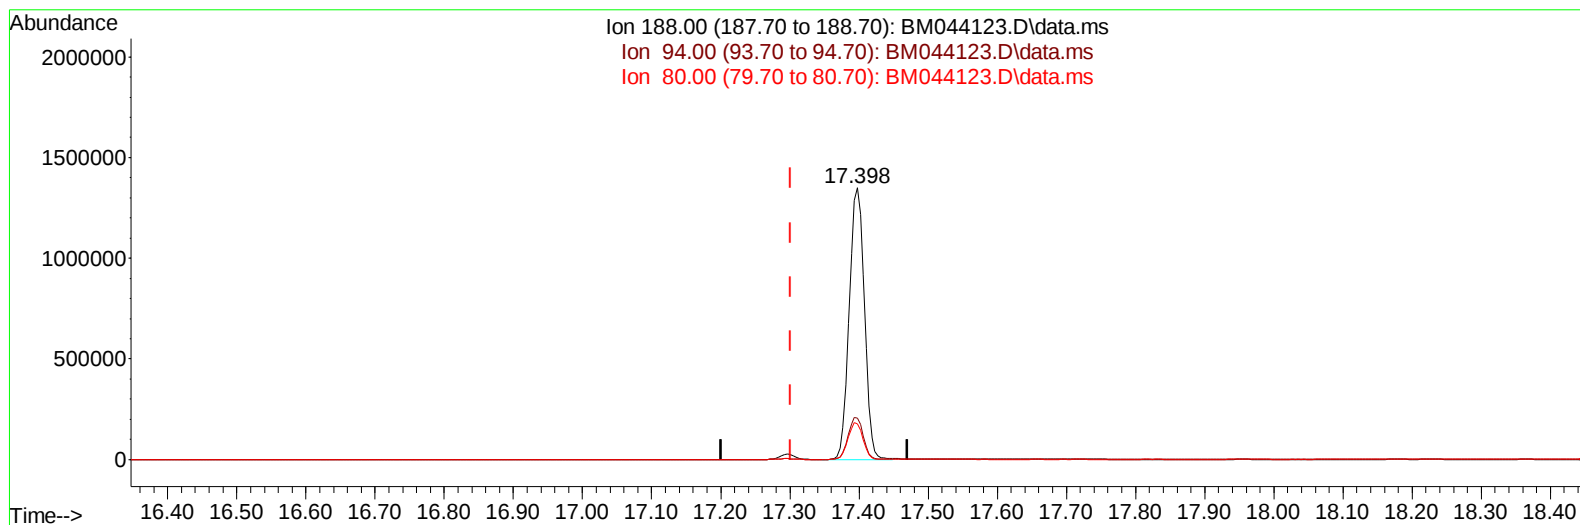

TIC: BM044123.D\data.ms

(13) Phenanthrene-d10 (I)

17.398min (+ 0.097) 0.40 ng/u1

response 2048090

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	15.30#
80.00	13.40	13.13
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

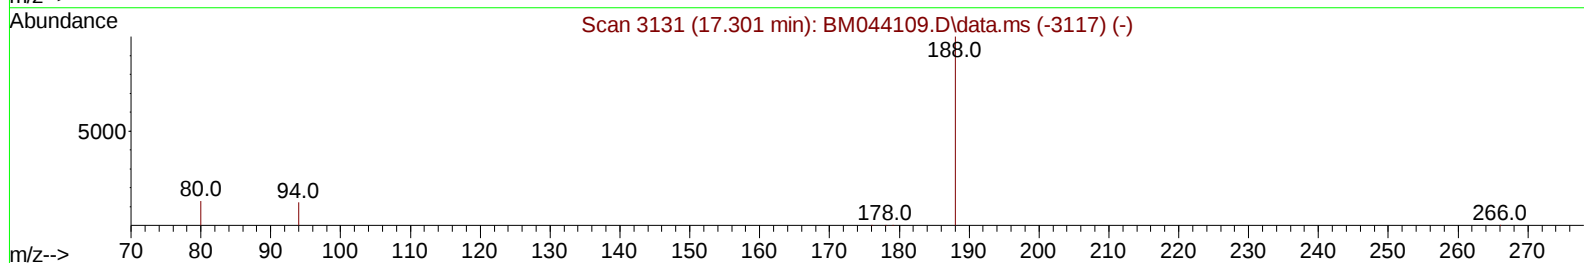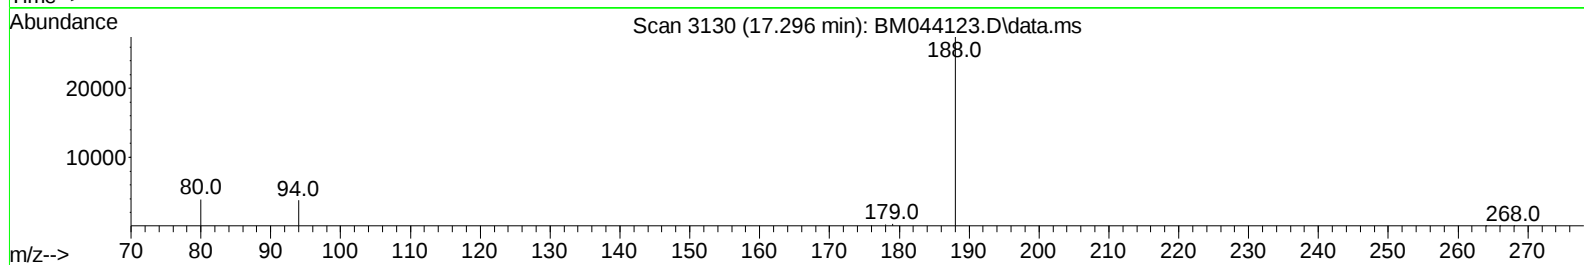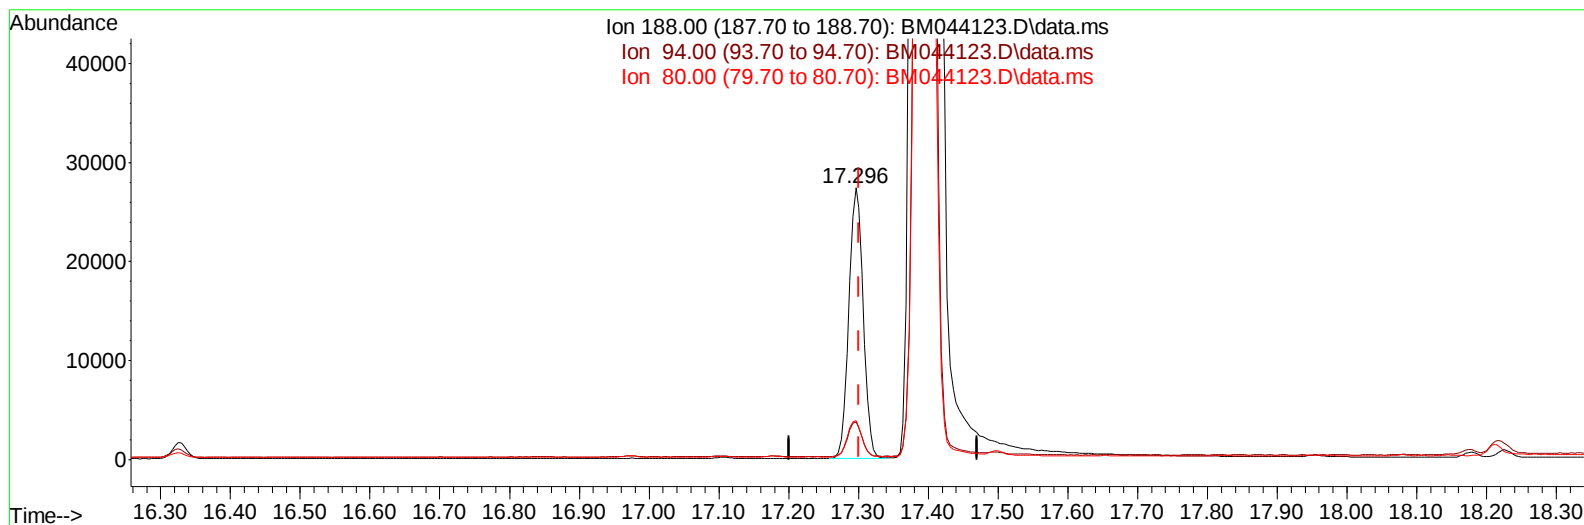

TIC: BM044123.D\data.ms

(13) Phenanthrene-d10 (I)

17.296min (-0.004) 0.40 ng/ul m

response 39101

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	13.76
80.00	13.40	14.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

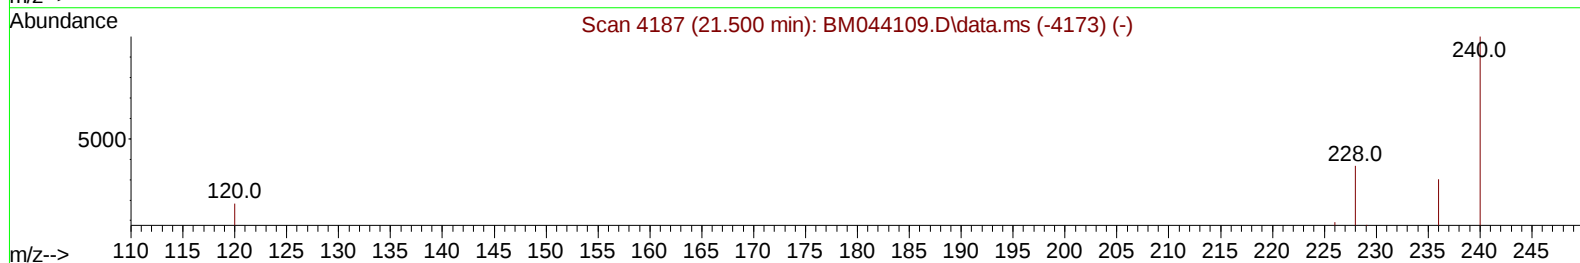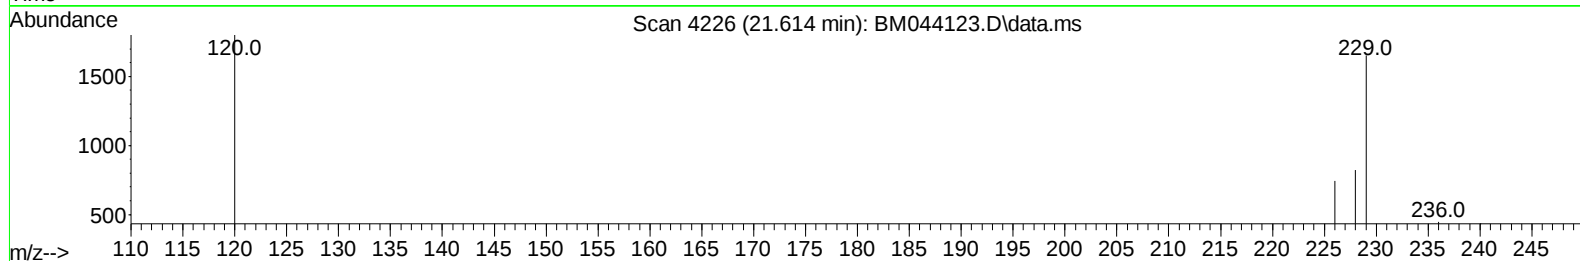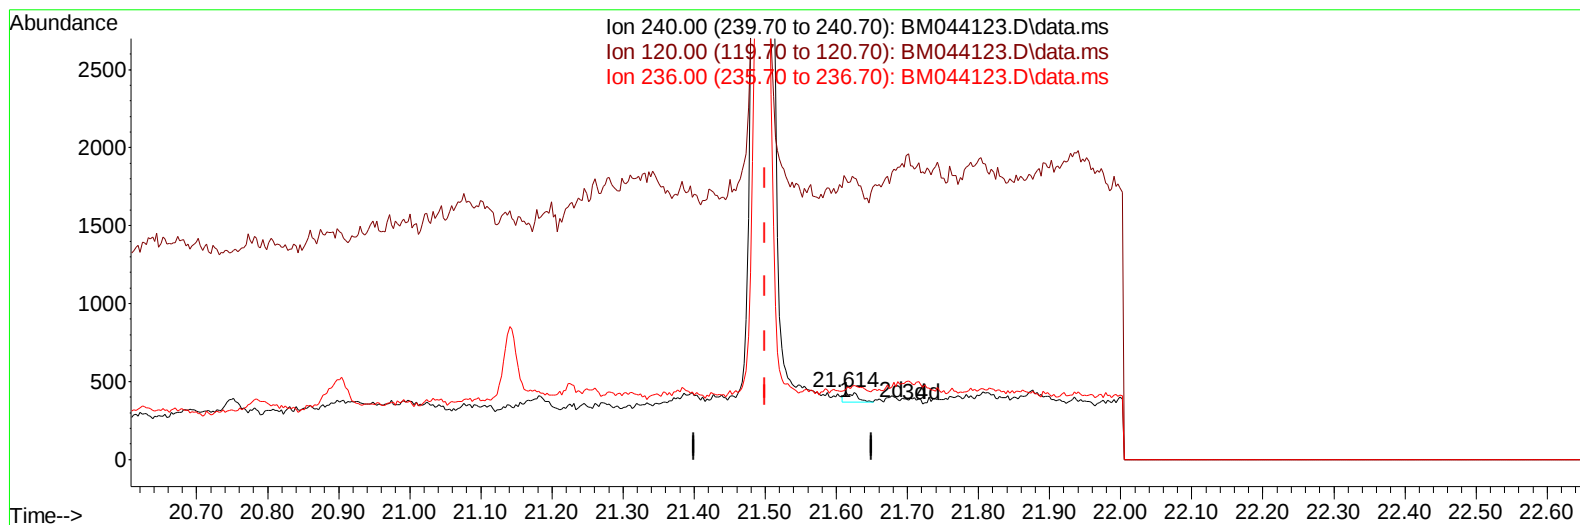

TIC: BM044123.D\data.ms

(17) Chrysene-d12

21.614min (+ 0.114) 0.40 ng/u1

response 76

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.50	415.70#
236.00	30.60	103.70#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

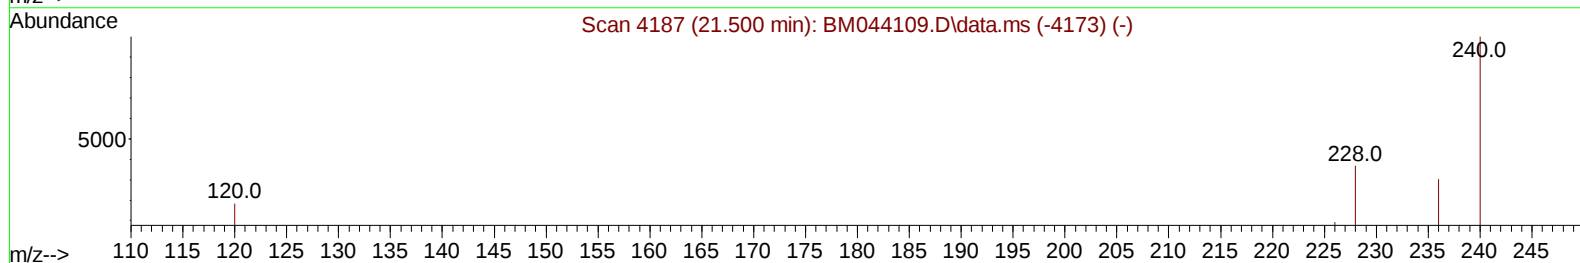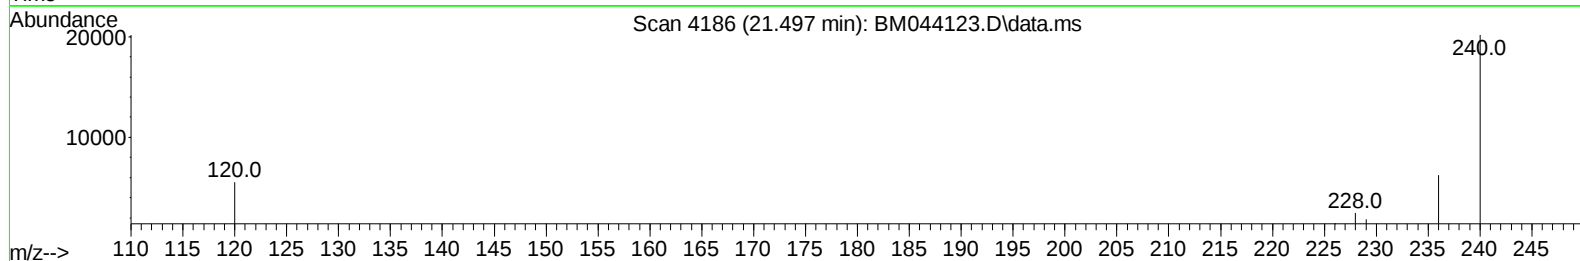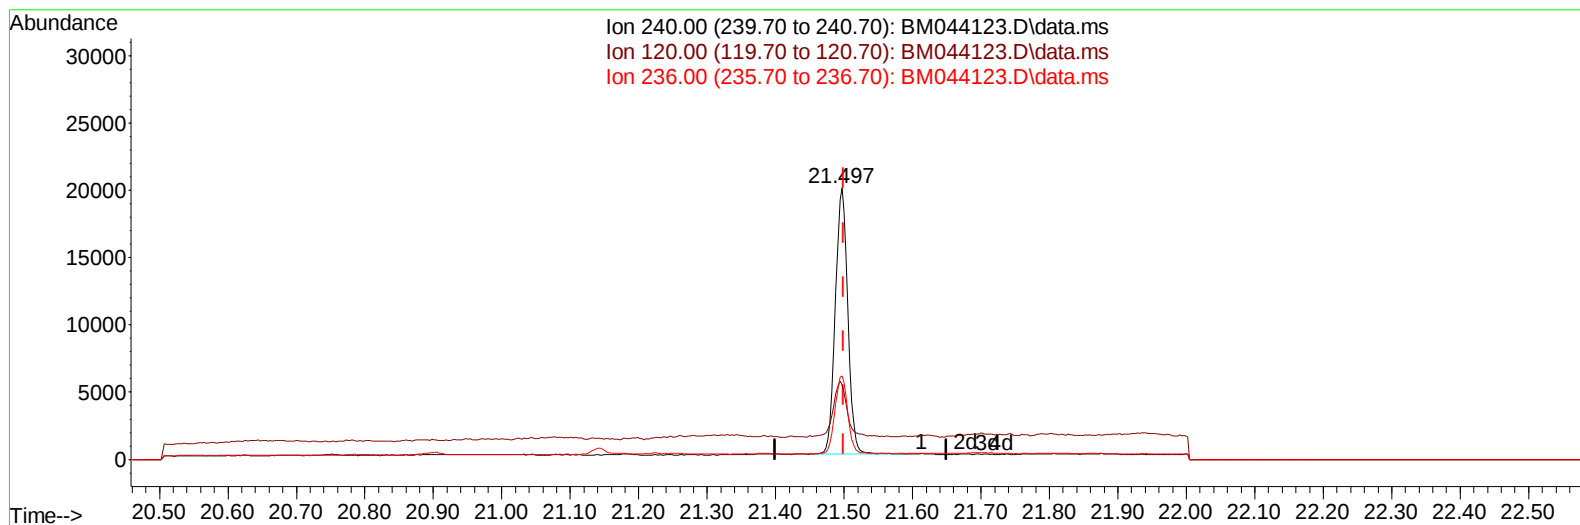

TIC: BM044123.D\data.ms

(17) Chrysene-d12

21.497min (-0.003) 0.40 ng/u1 m

response 25180

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.50	27.53#
236.00	30.60	30.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

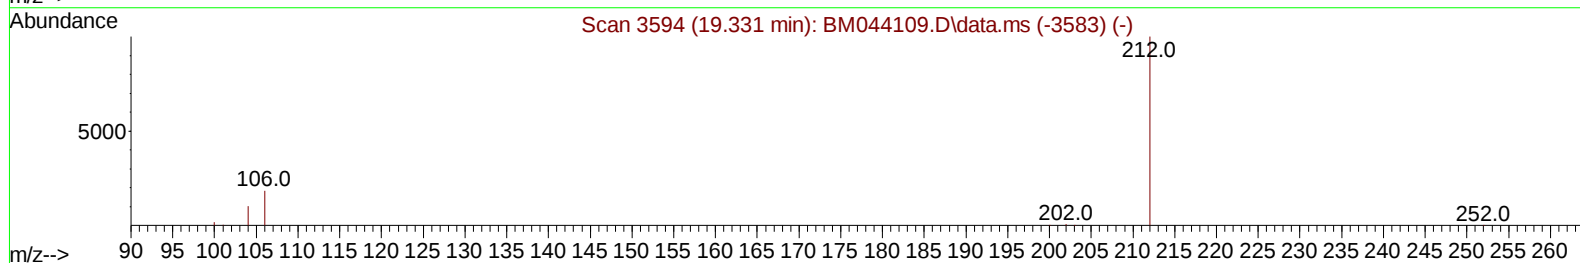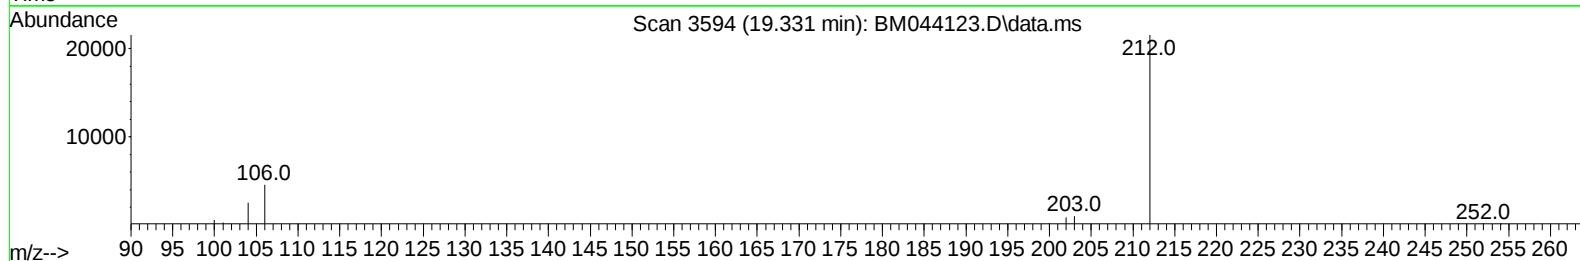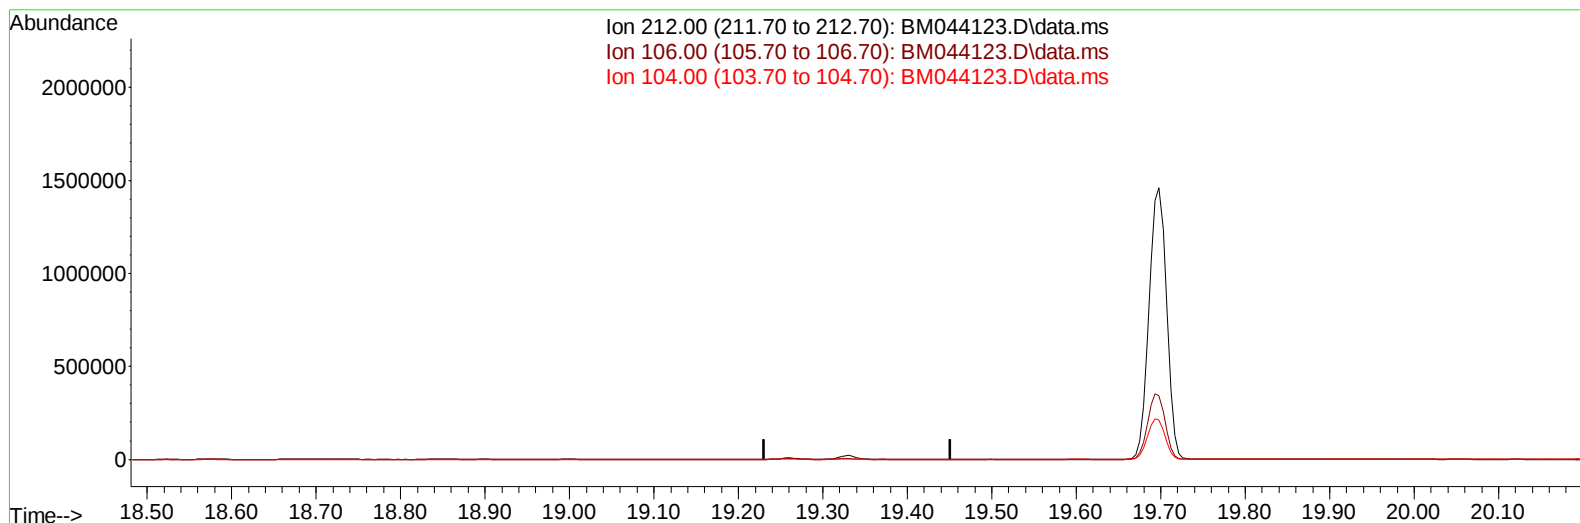

TIC: BM044123.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.331min (-19.331) 0.00 ng/u1

response 0

Ion	Exp%	Act%
212.00	100.00	0.00
106.00	18.40	0.00#
104.00	10.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

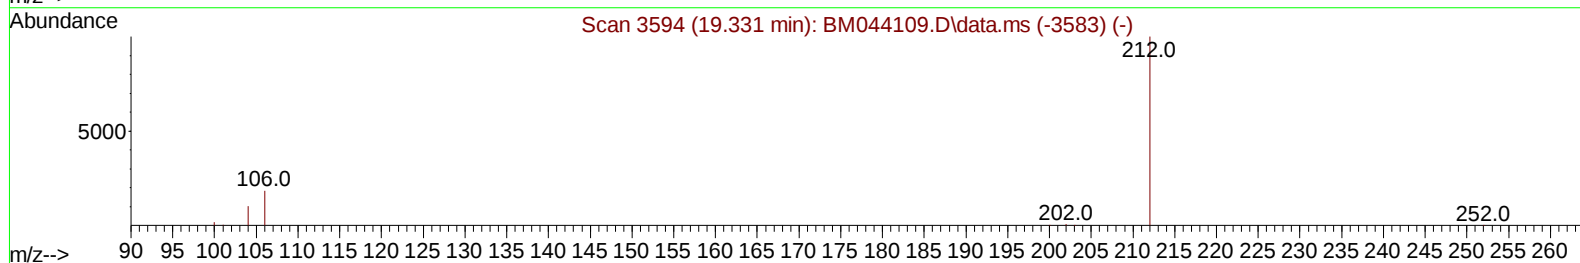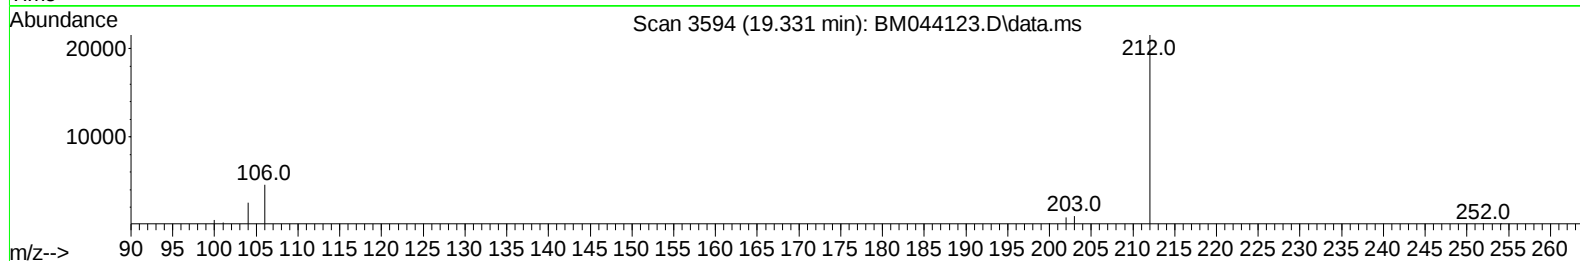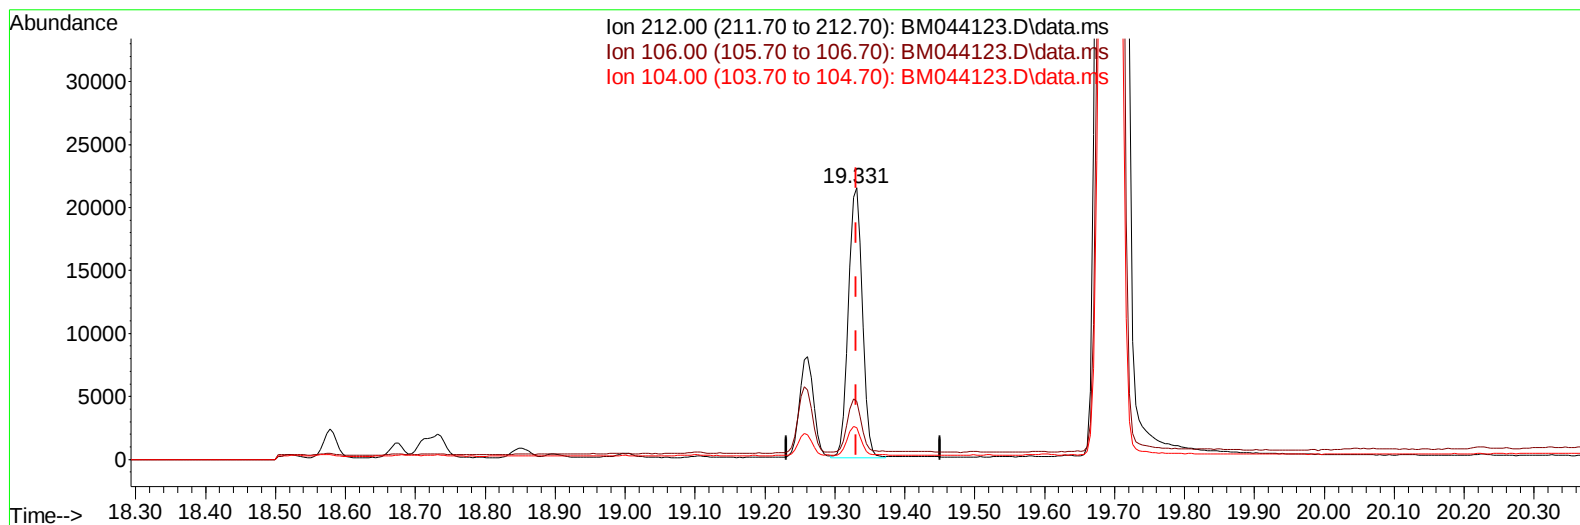

TIC: BM044123.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.331min (+ 0.000) 0.39 ng/ul m

response 29269

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	18.40	0.00#
104.00	10.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

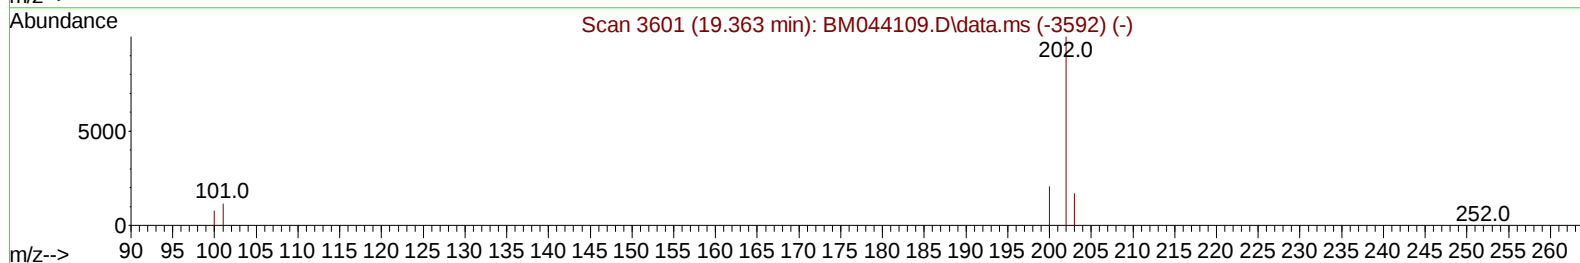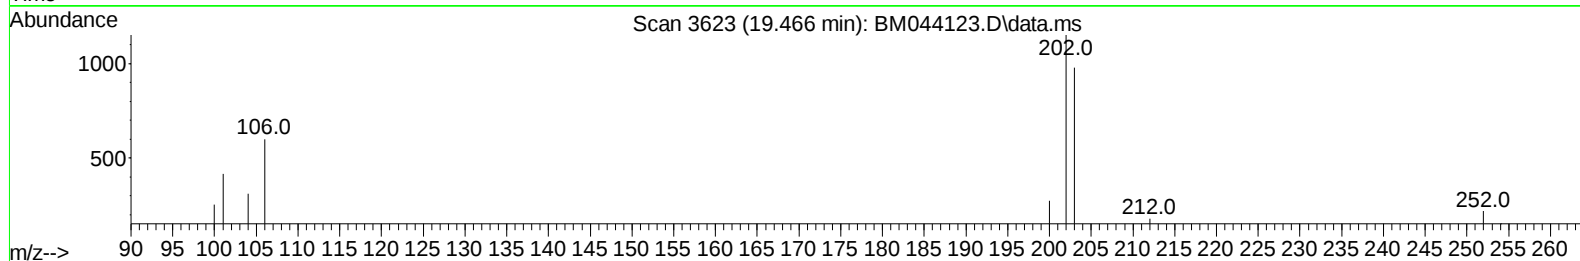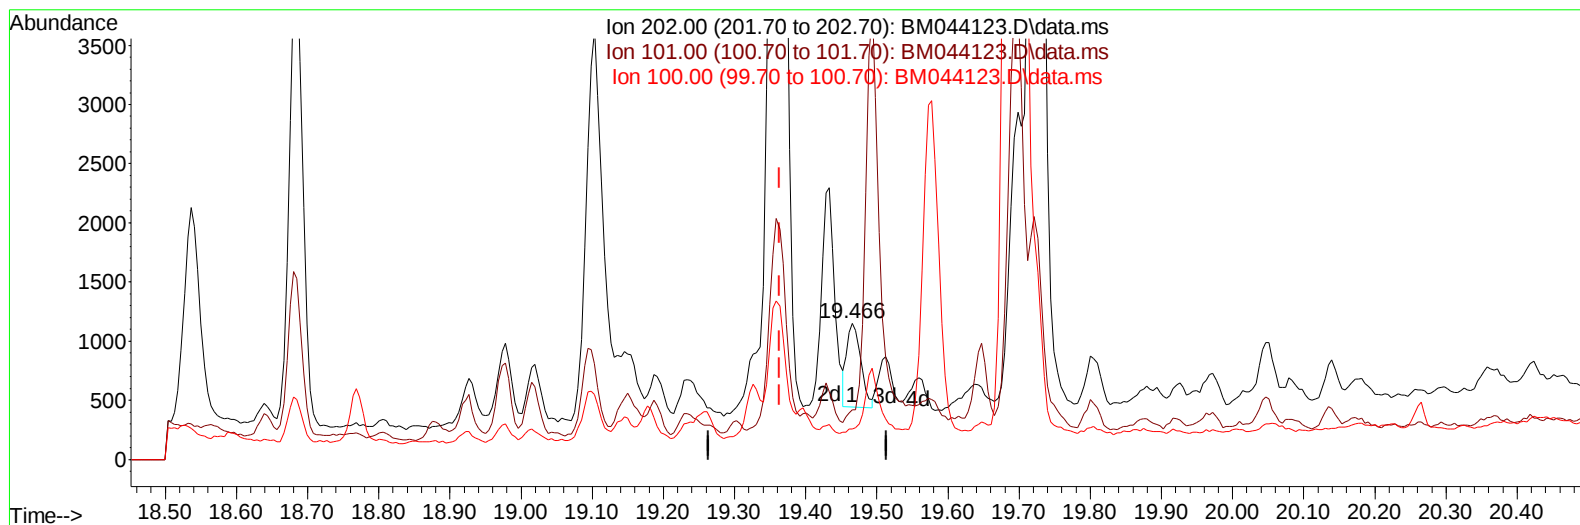

TIC: BM044123.D\data.ms

(19) Fluoranthene (C)

19.466min (+ 0.102) 0.01 ng/u1

response 975

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.20	36.28#
100.00	8.70	22.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

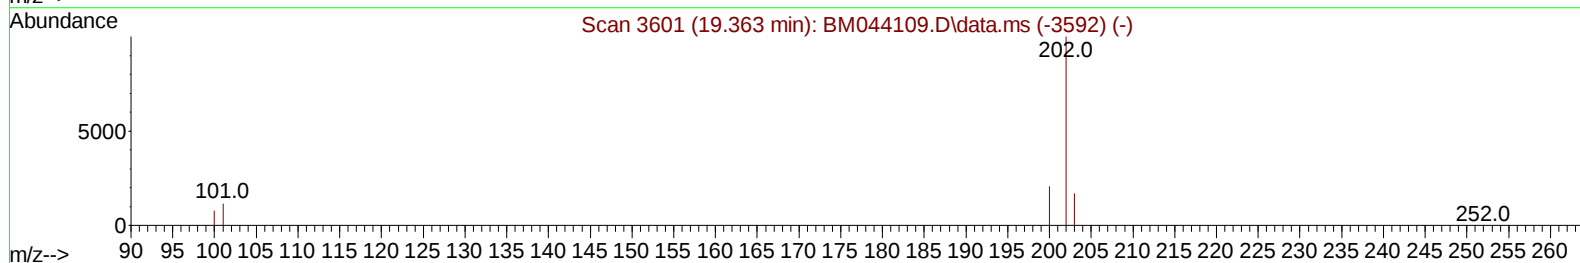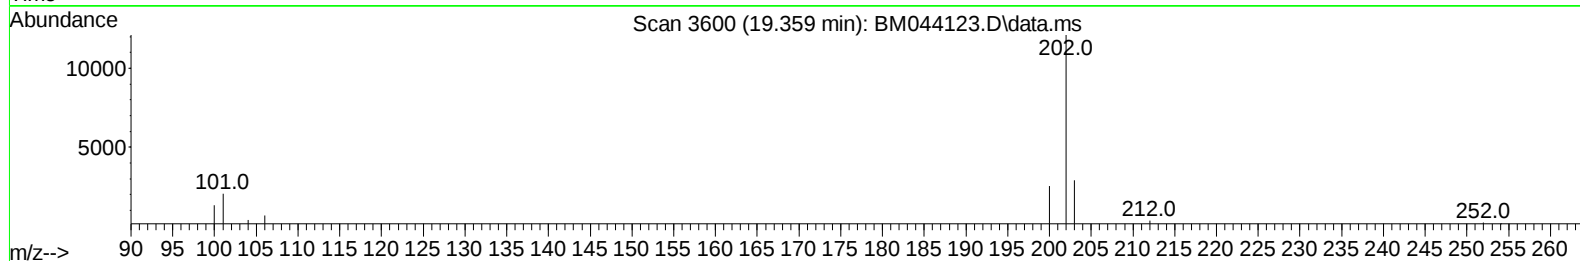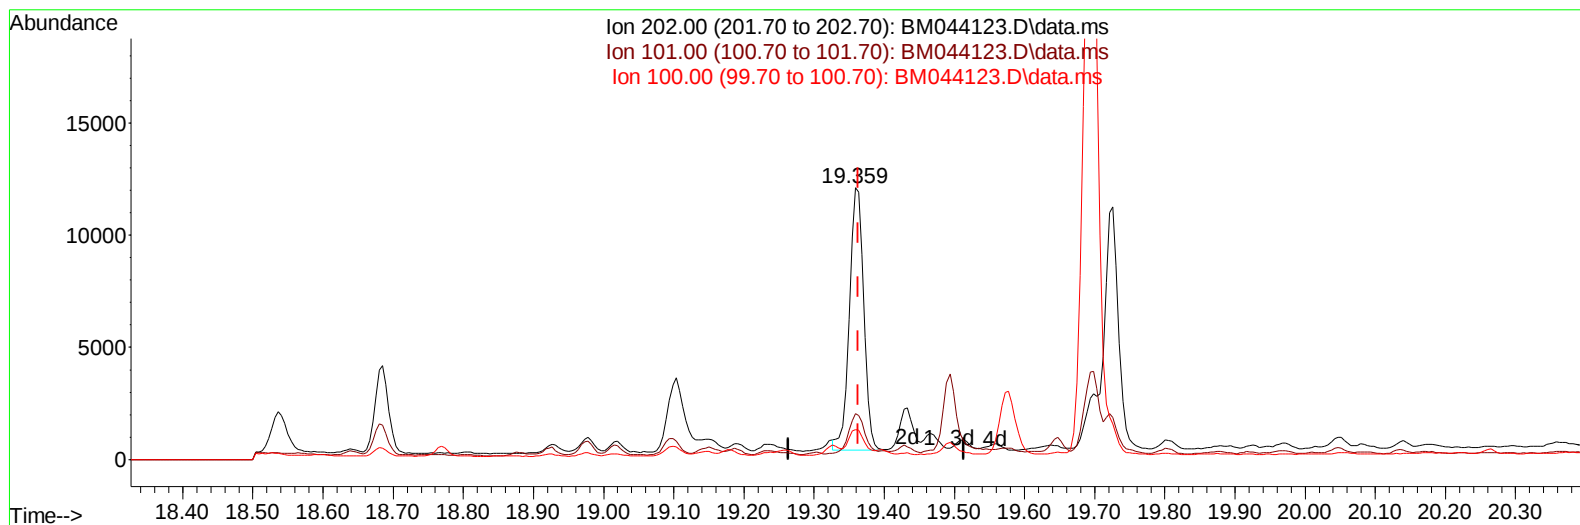

TIC: BM044123.D\data.ms

(19) Fluoranthene (C)

19.359min (-0.005) 0.15 ng/ul m

response 16888

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.20	16.81#
100.00	8.70	11.07#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

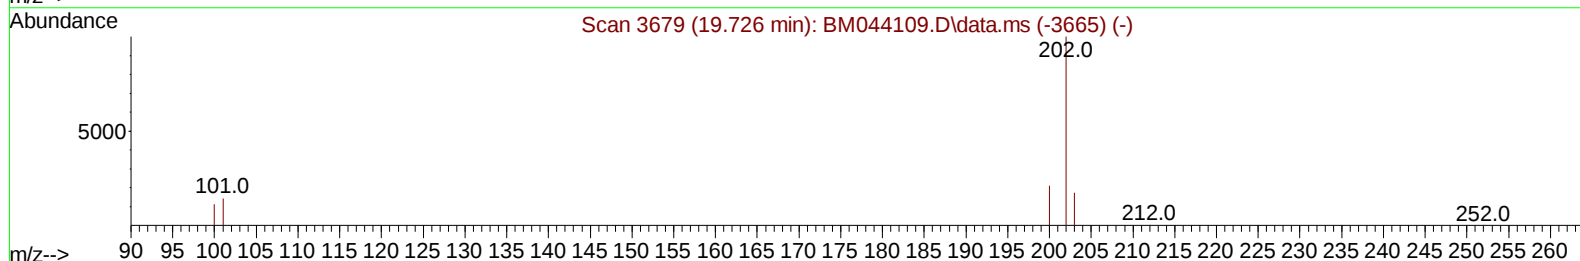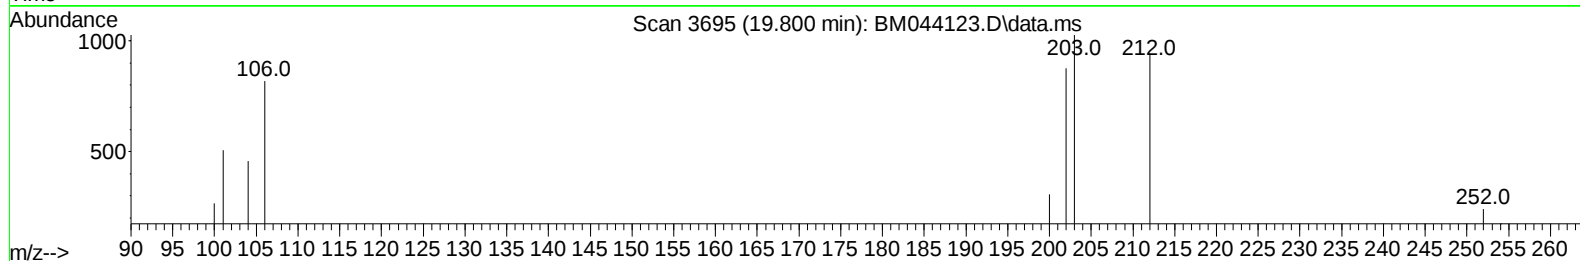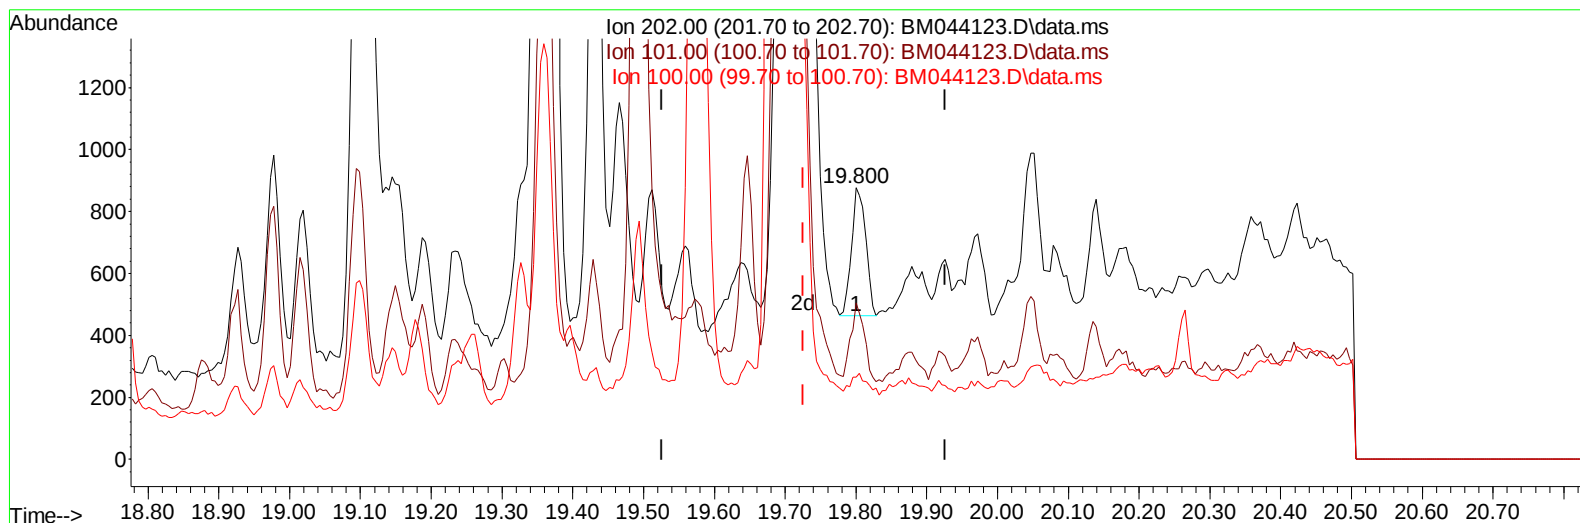

TIC: BM044123.D\data.ms

(20) Pyrene

19.800min (+ 0.074) 0.00 ng/u1

response 572

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.00	57.65#
100.00	10.80	30.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

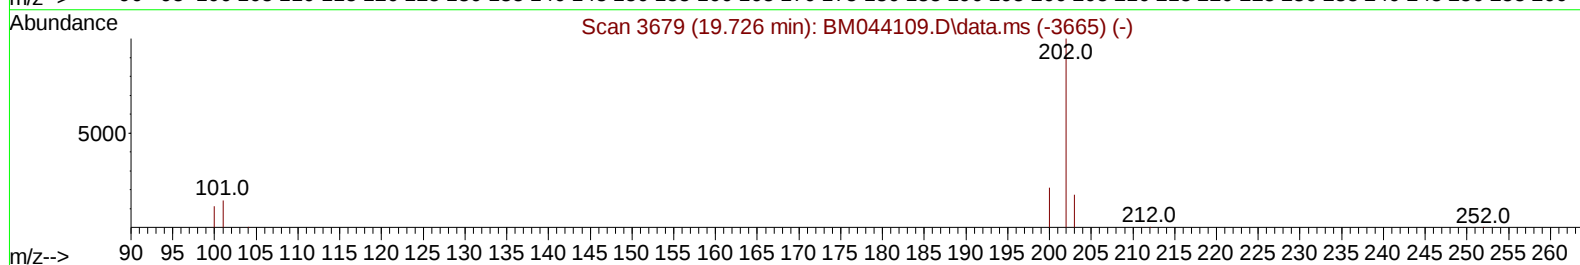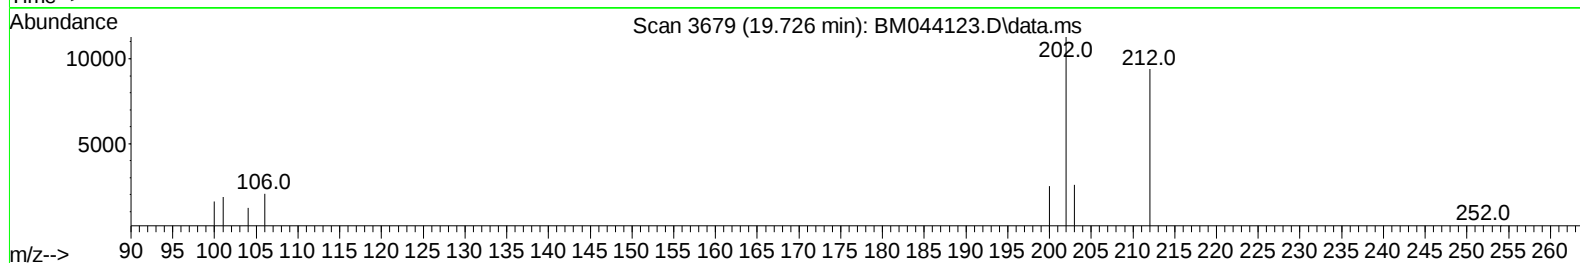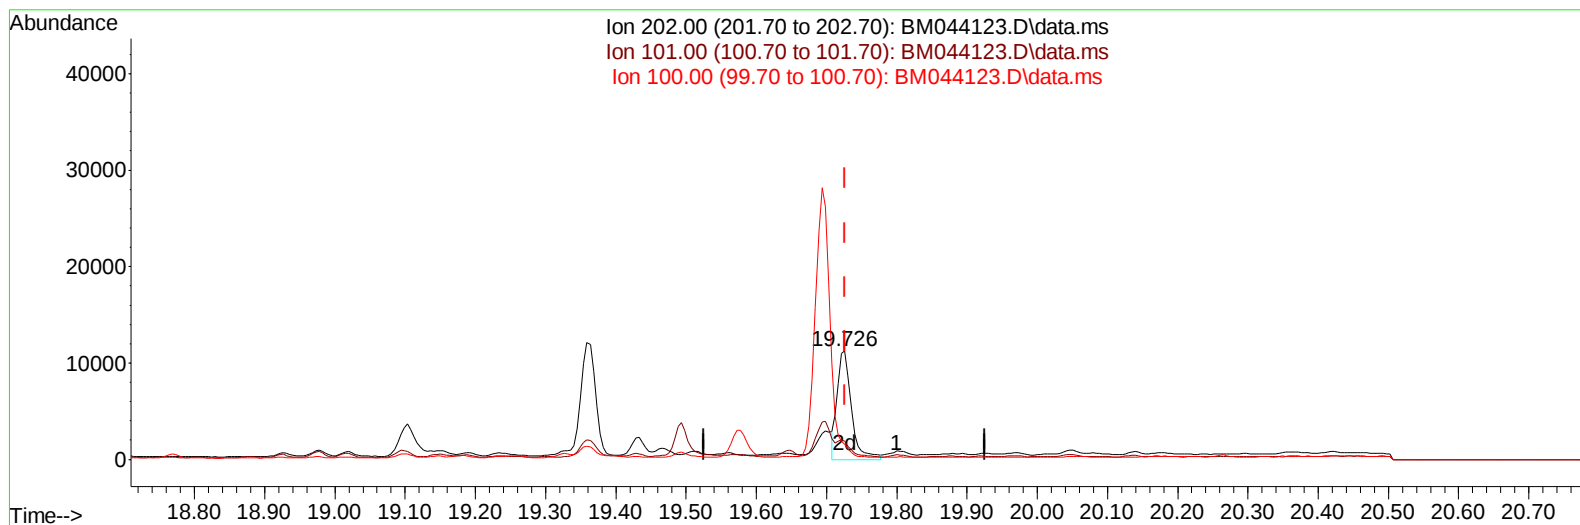

TIC: BM044123.D\data.ms

(20) Pyrene

19.726min (+ 0.000) 0.13 ng/ul m

response 15842

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.00	16.55
100.00	10.80	14.03#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

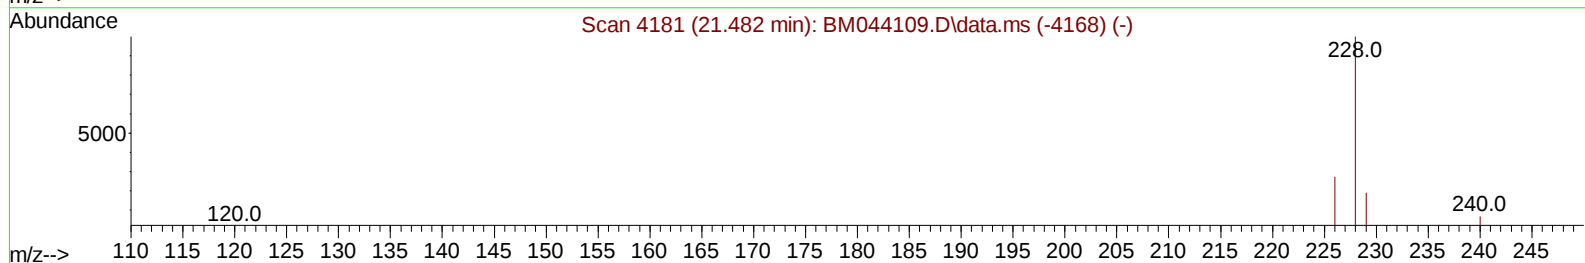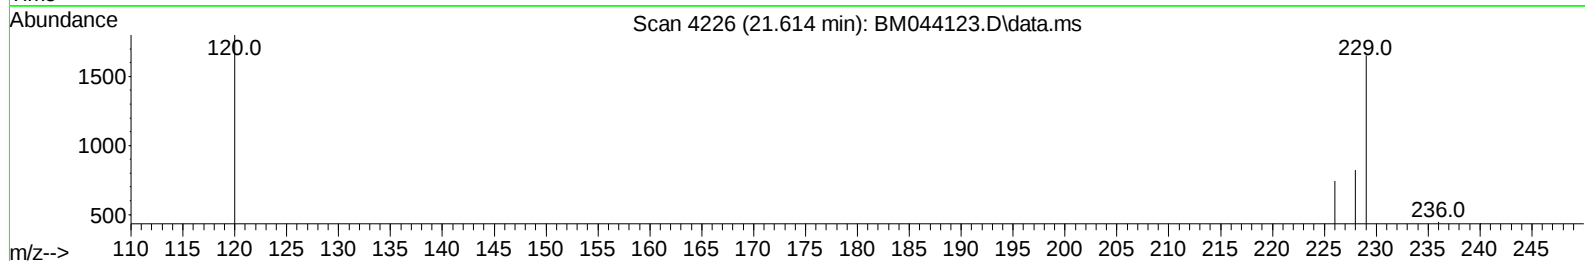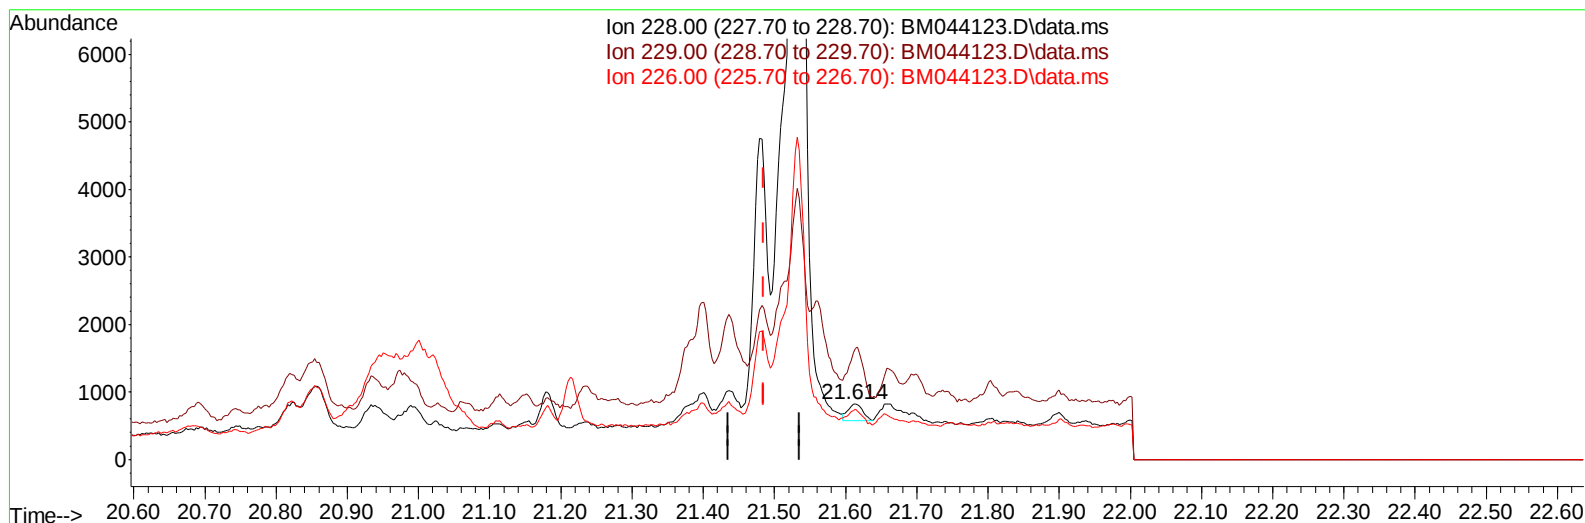

TIC: BM044123.D\data.ms

(21) Benzo(a)anthracene

21.614min (+ 0.129) 0.00 ng/u1

response 361

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.30	200.24#
226.00	27.60	90.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

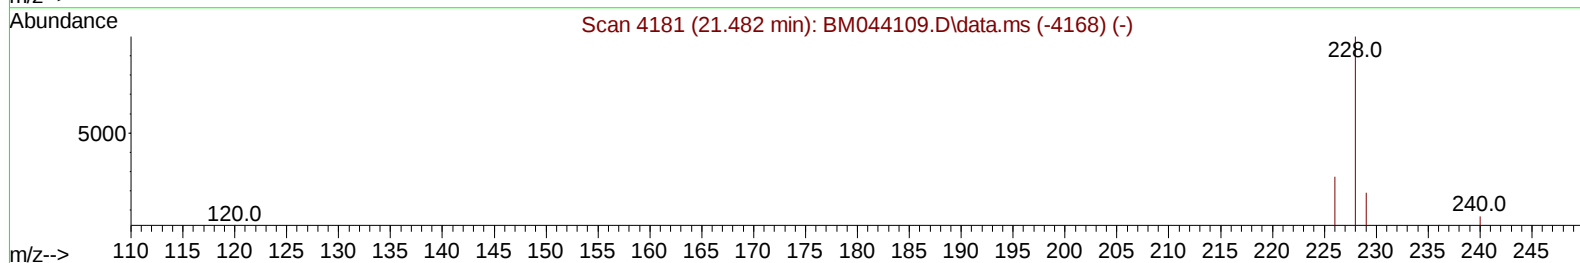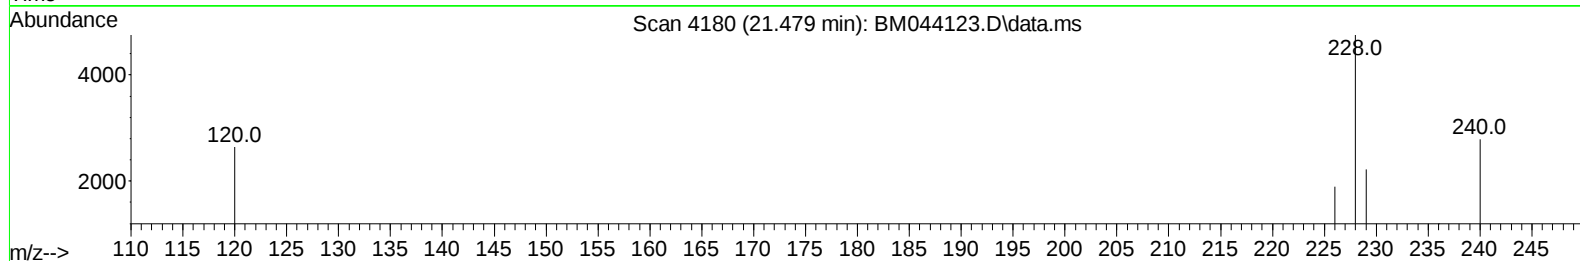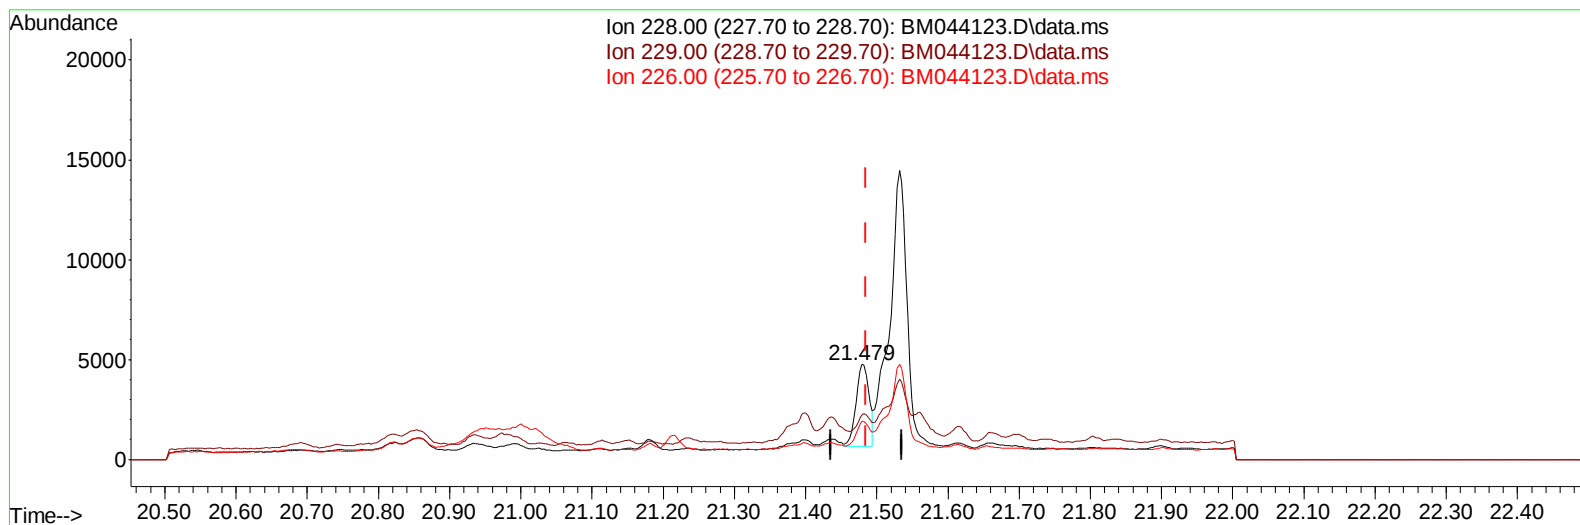

TIC: BM044123.D\data.ms

(21) Benzo(a)anthracene

21.479min (-0.006) 0.05 ng/u1 m

response 5293

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.30	46.63#
226.00	27.60	39.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

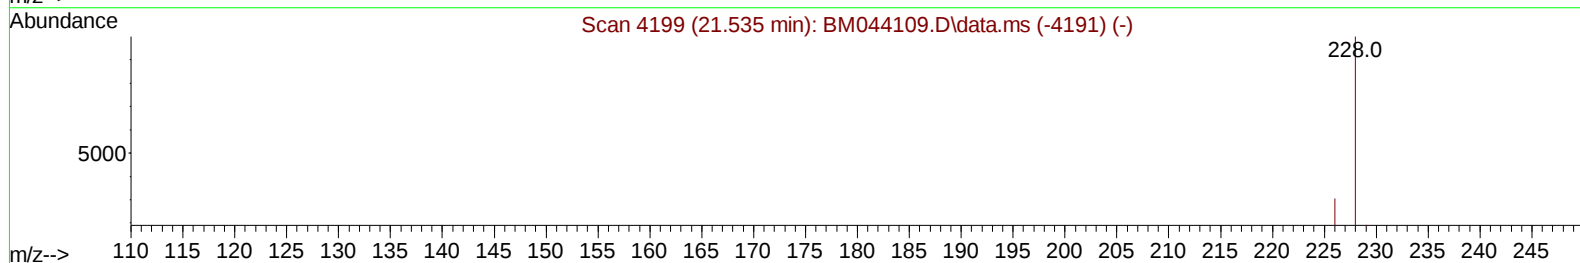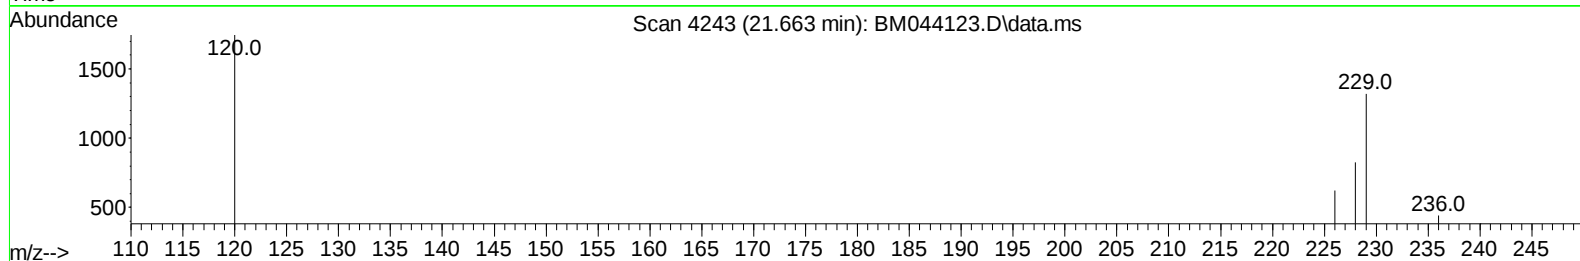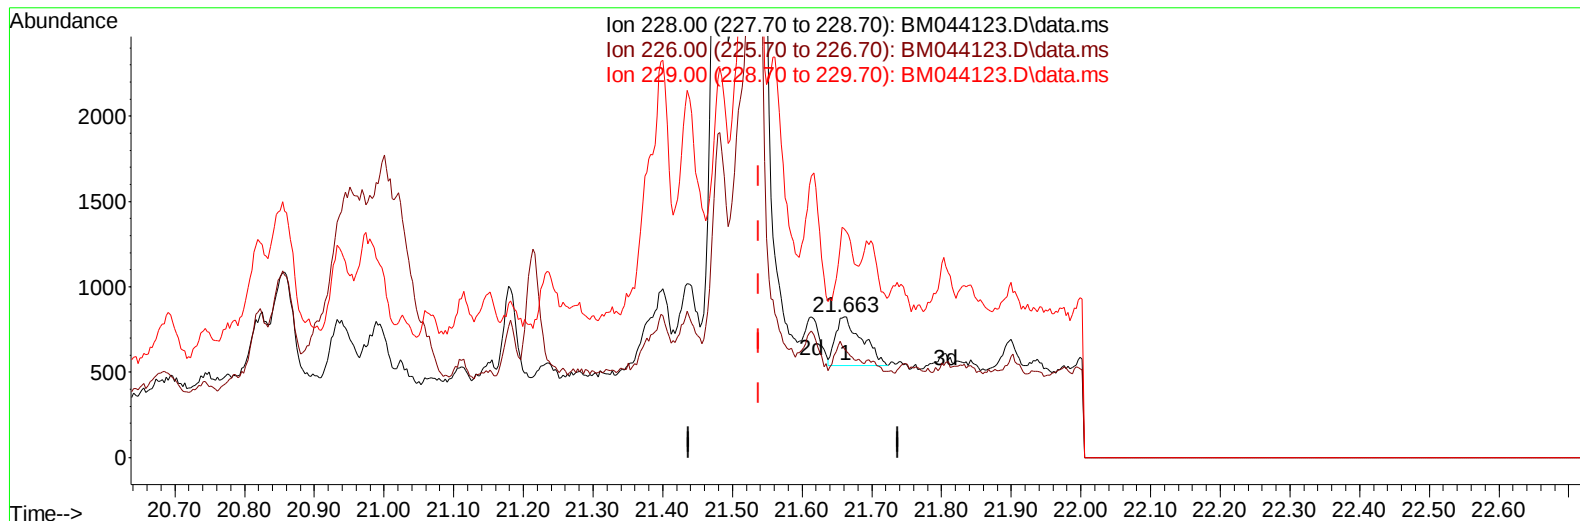

TIC: BM044123.D\data.ms

(22) Chrysene

21.663min (+ 0.126) 0.01 ng/u1

response 739

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.20	75.49#
229.00	19.70	160.44#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

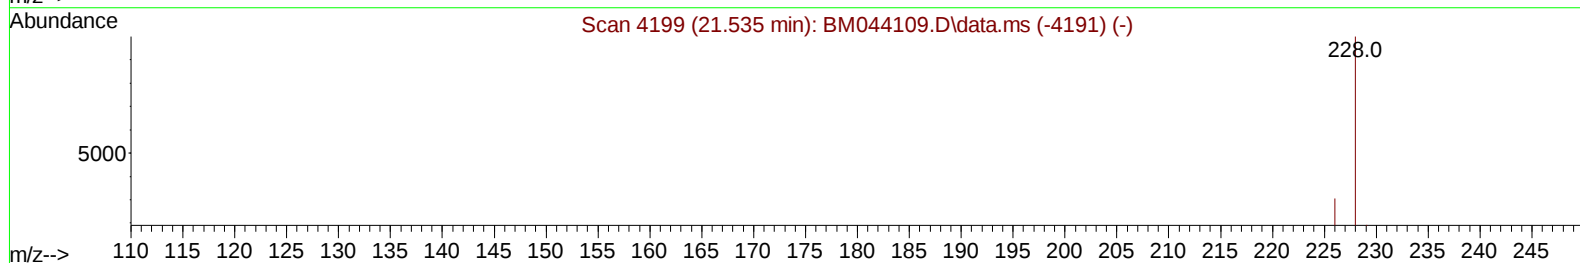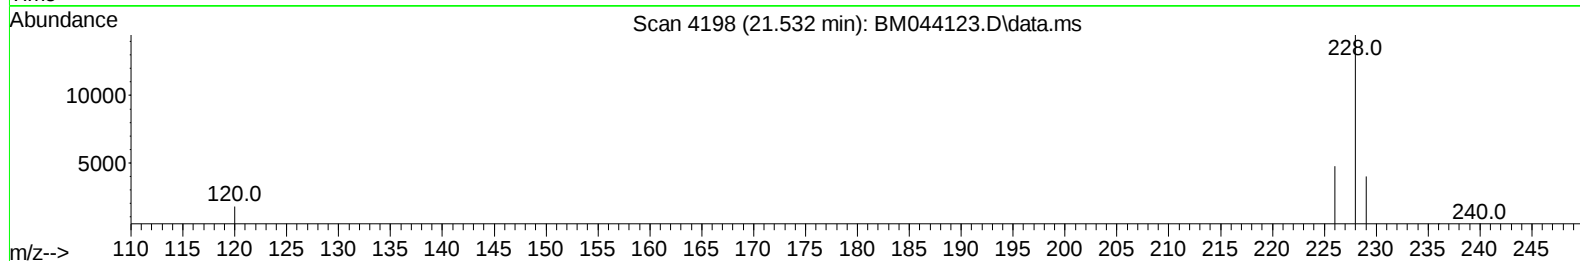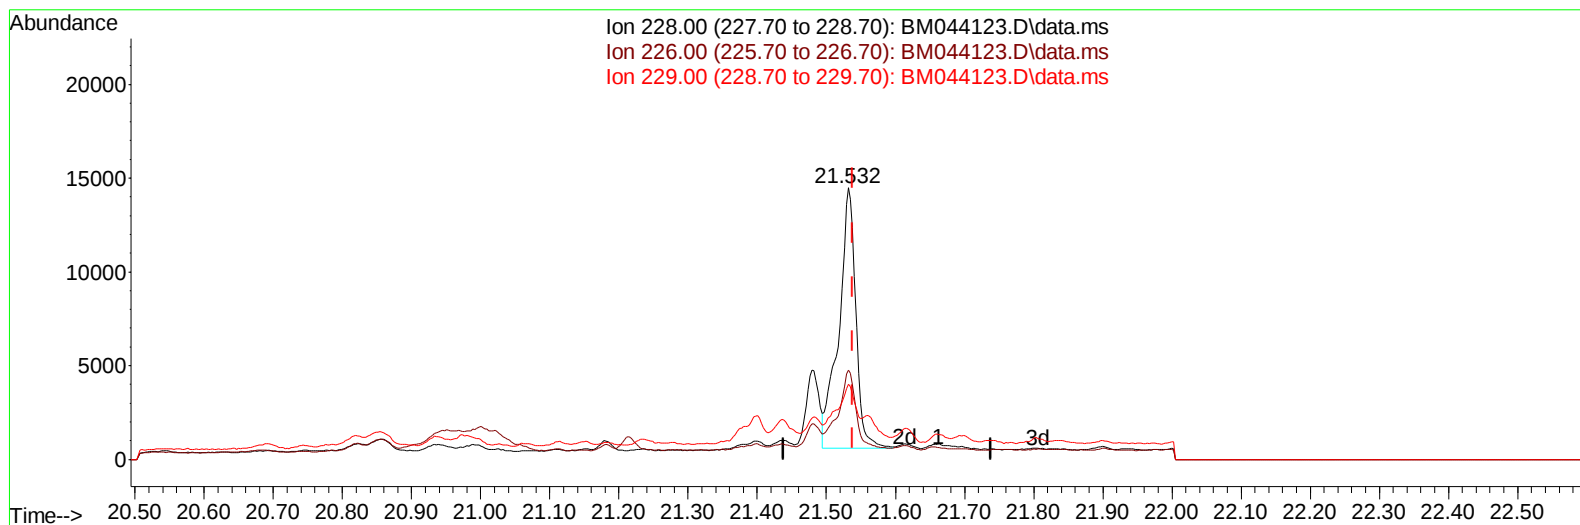

TIC: BM044123.D\data.ms

(22) Chrysene

21.532min (-0.006) 0.19 ng/u1 m

response 23782

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.20	32.99
229.00	19.70	27.73#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

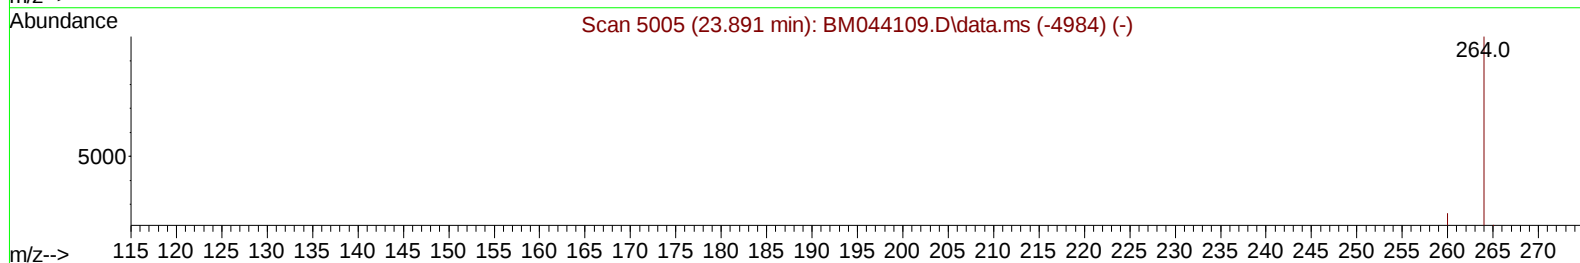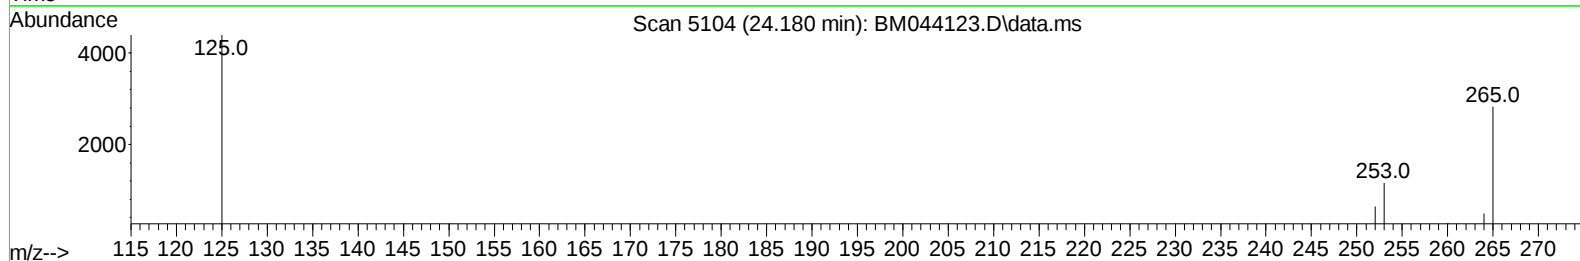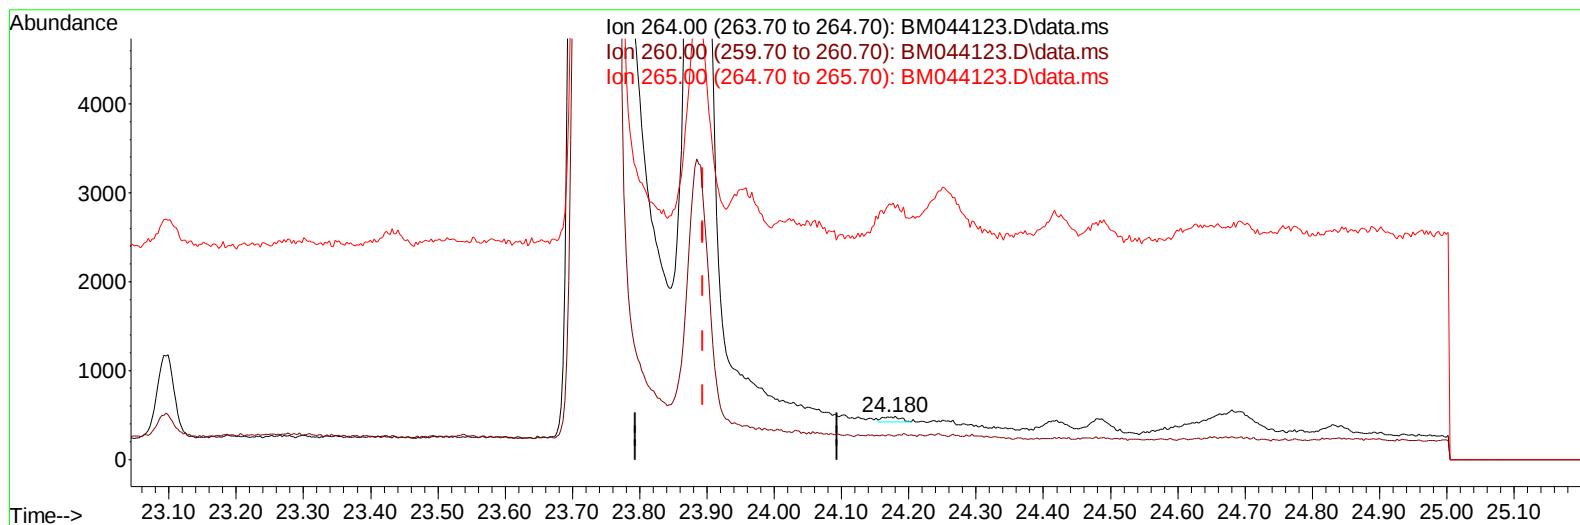

TIC: BM044123.D\data.ms

(23) Perylene-d12 (I)

24.180min (+ 0.287) 0.40 ng/u1

response 119

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.00	54.75#
265.00	45.40	584.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

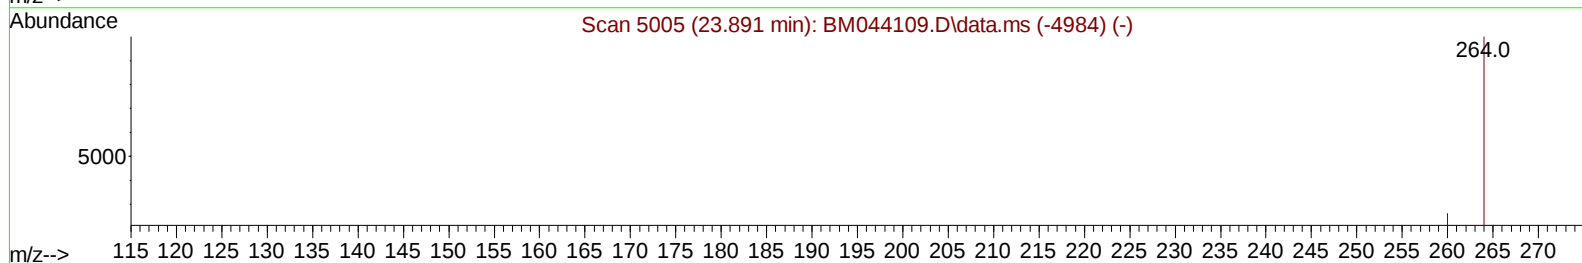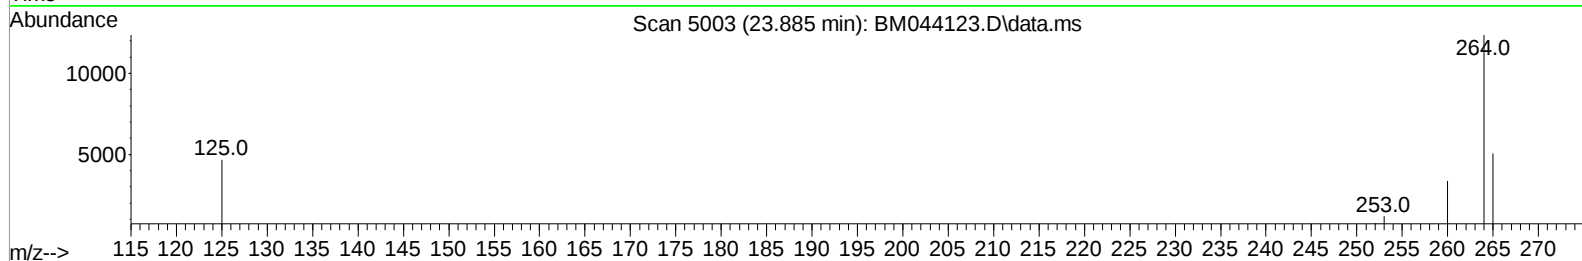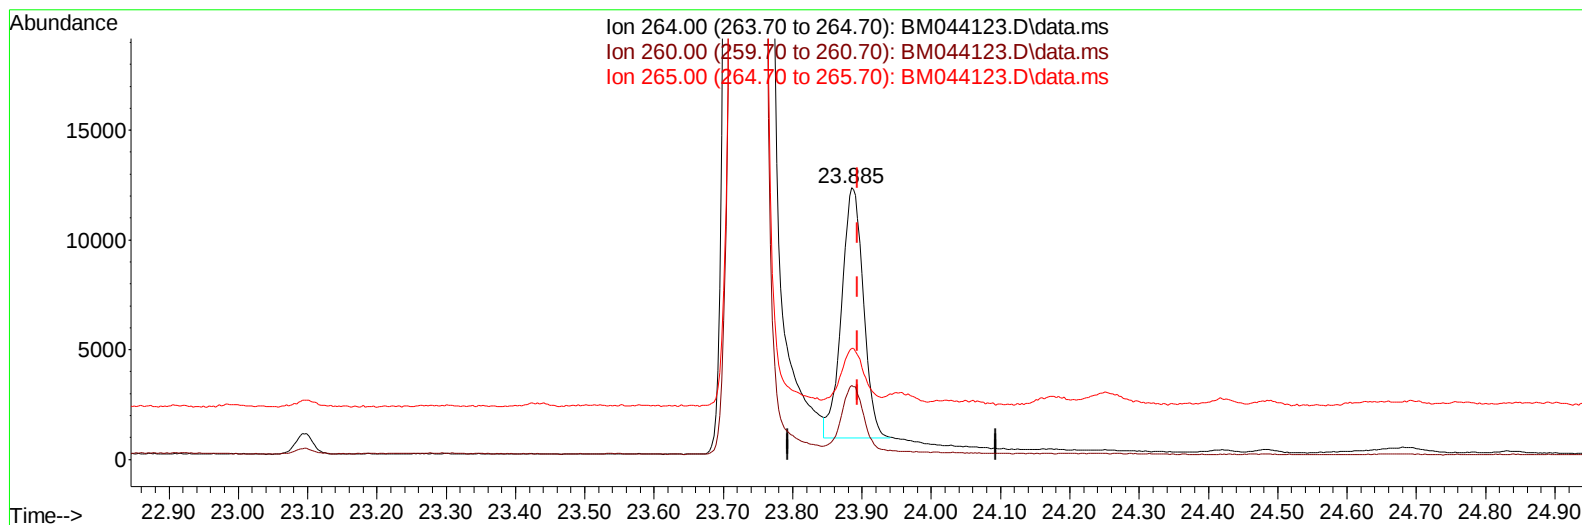

TIC: BM044123.D\data.ms

(23) Perylene-d12 (I)

23.885min (-0.009) 0.40 ng/ul m

response 24978

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.00	27.33
265.00	45.40	40.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

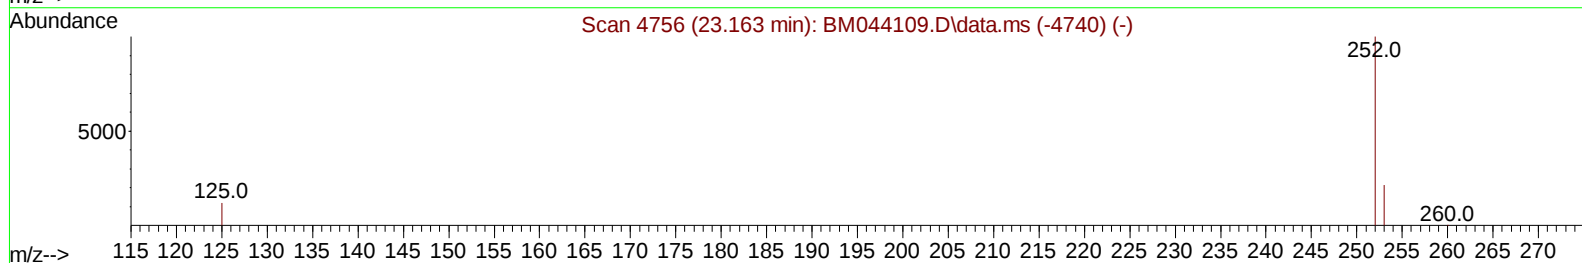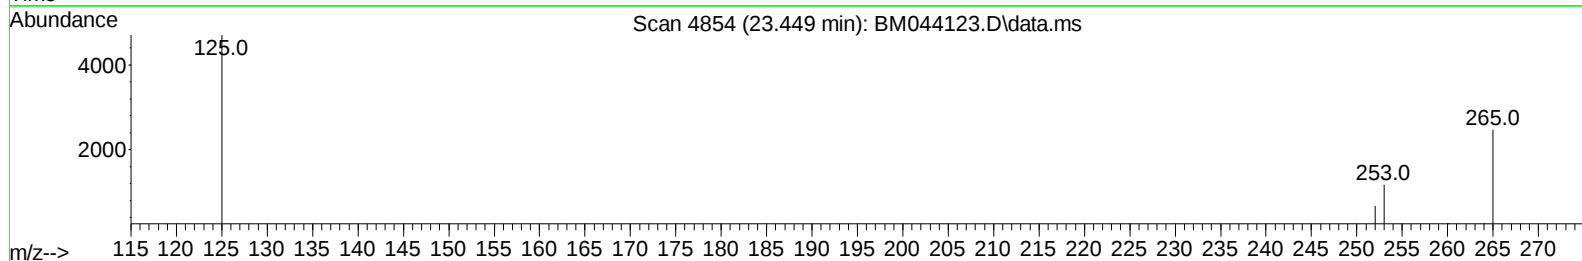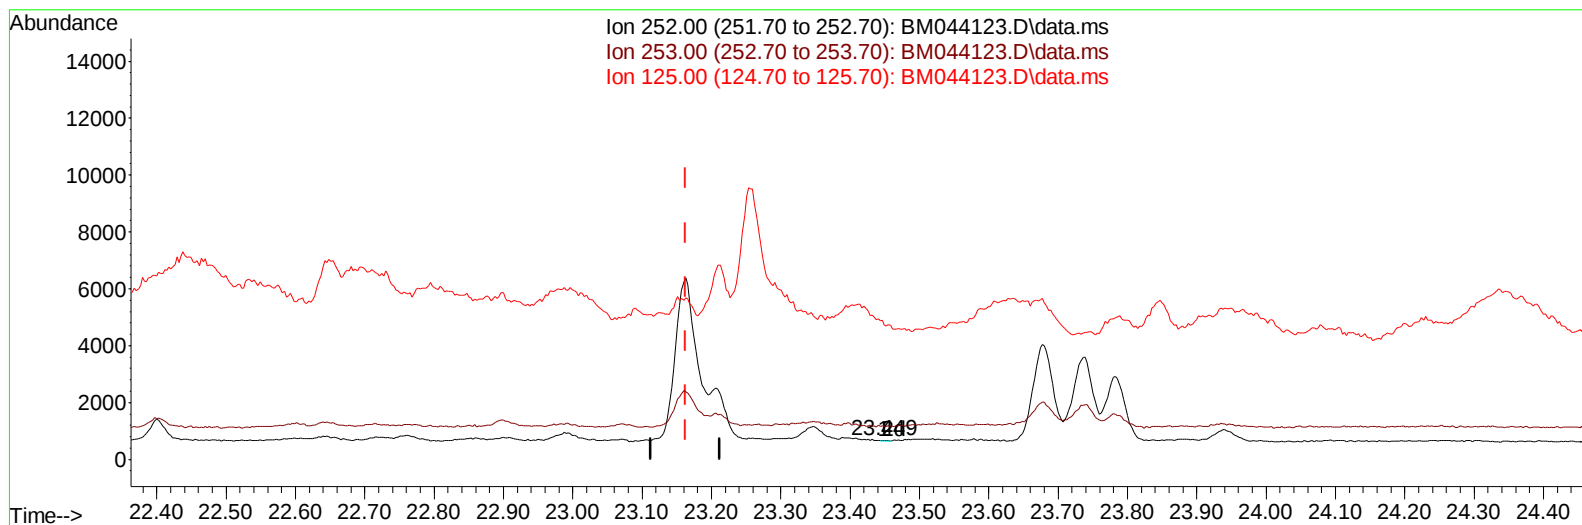

TIC: BM044123.D\data.ms

(24) Benzo(b)fluoranthene

23.449min (+ 0.287) 0.00 ng/u1

response 17

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.00	172.97#
125.00	14.10	695.13#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

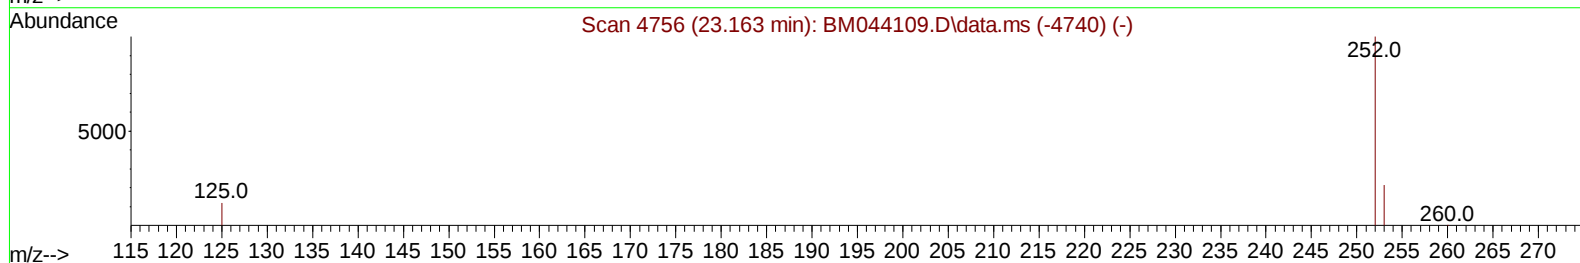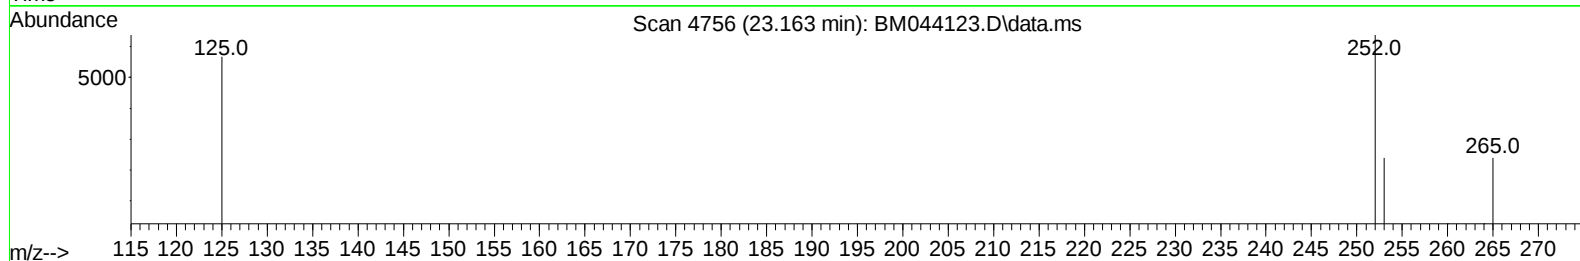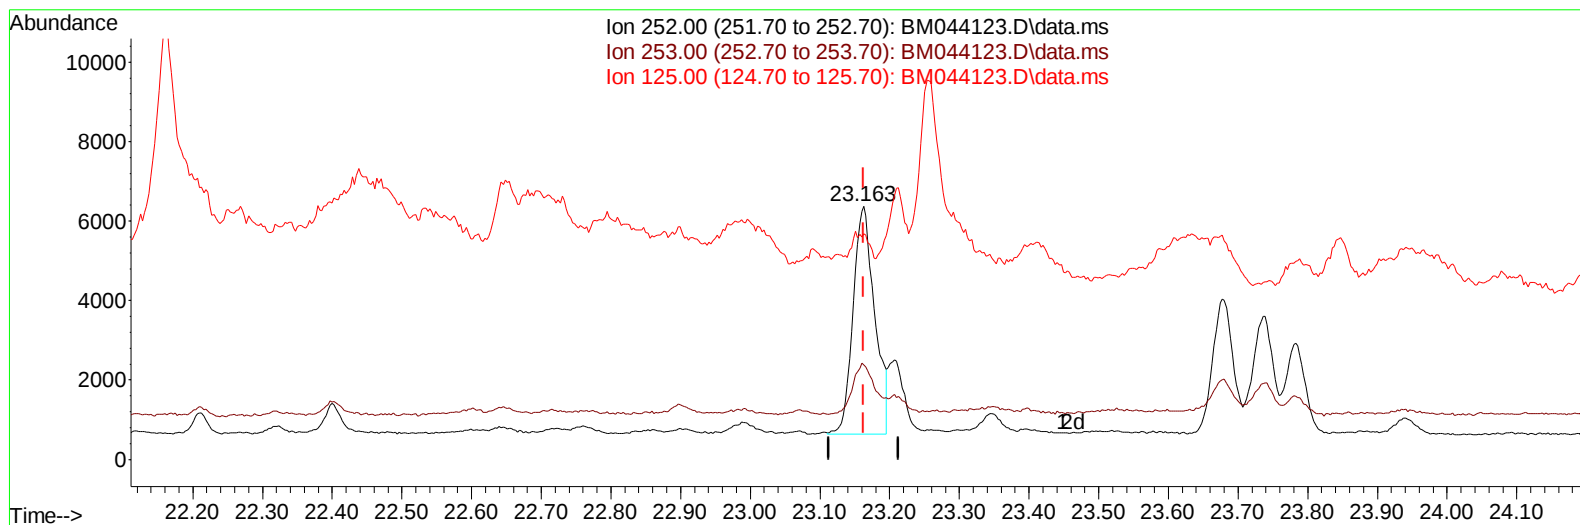

TIC: BM044123.D\data.ms

(24) Benzo(b)fluoranthene

23.163min (+ 0.000) 0.12 ng/u1 m

response 12412

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.00	37.43
125.00	14.10	89.06#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

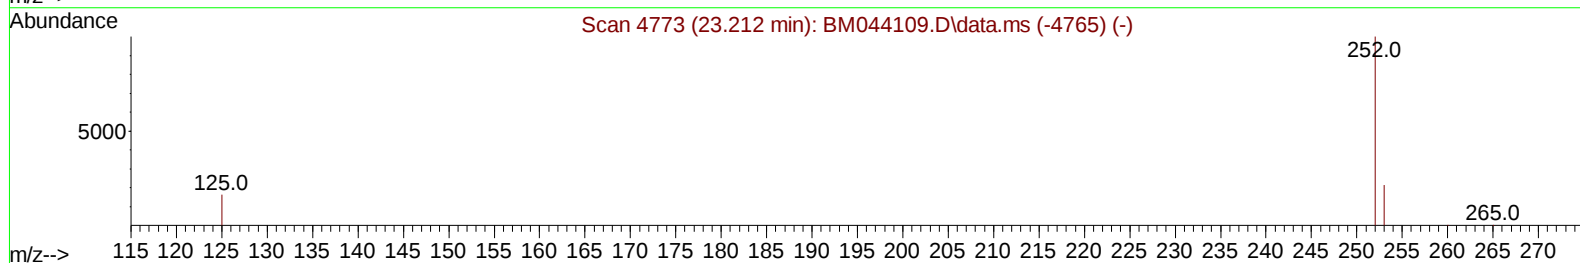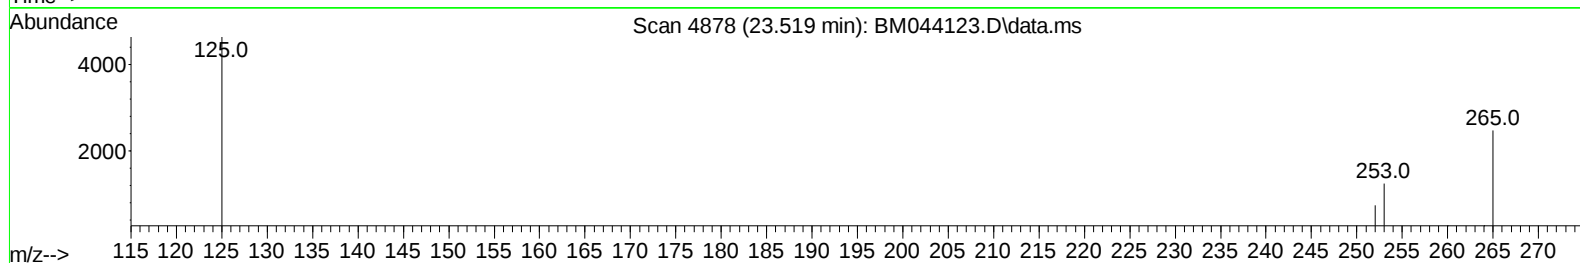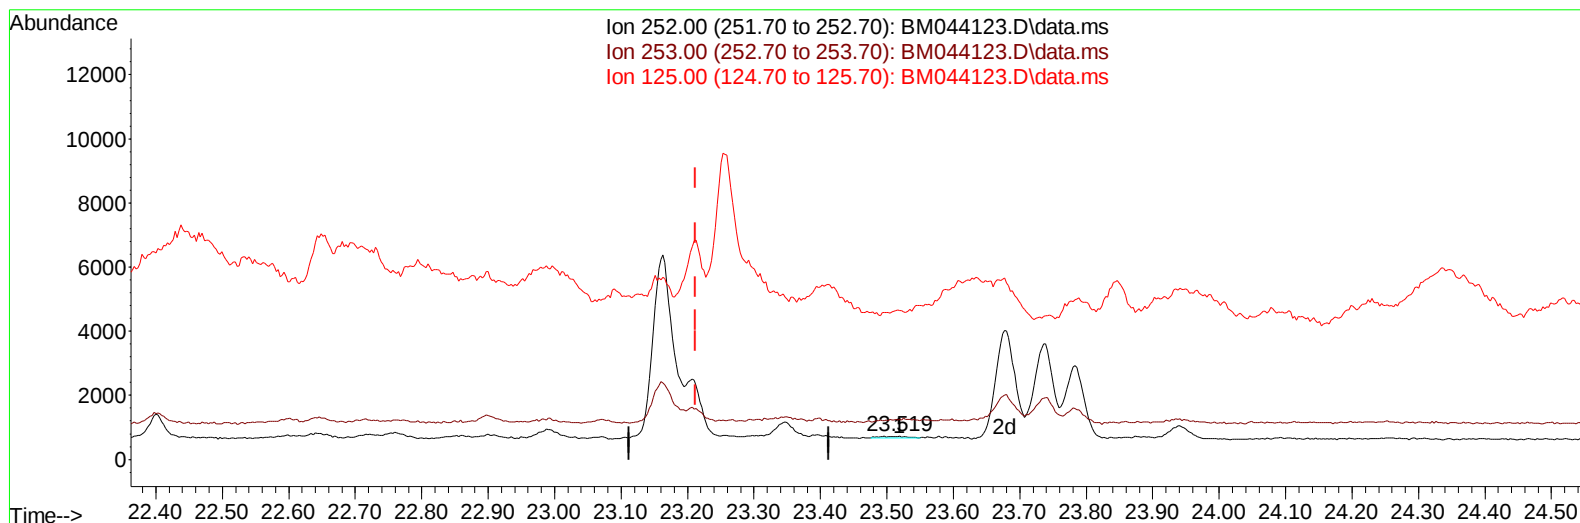

TIC: BM044123.D\data.ms

(25) Benzo(k)fluoranthene

23.519min (+ 0.307) 0.00 ng/u1

response 140

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	170.31#
125.00	15.40	634.47#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

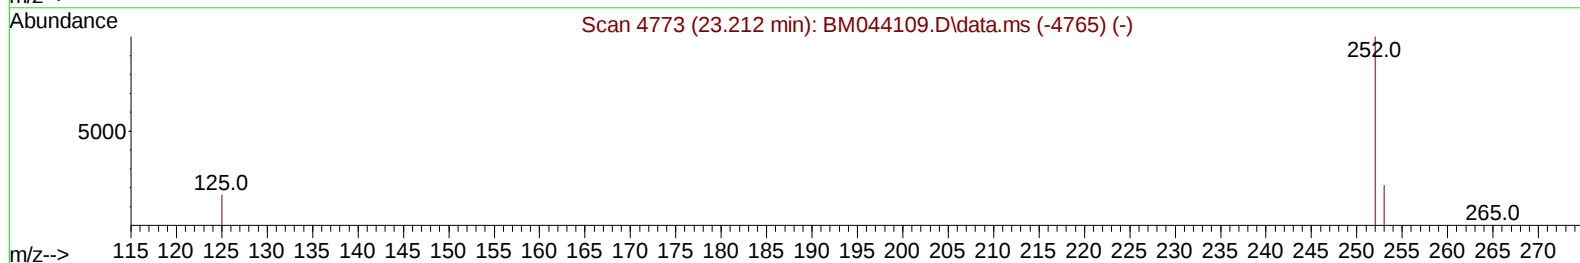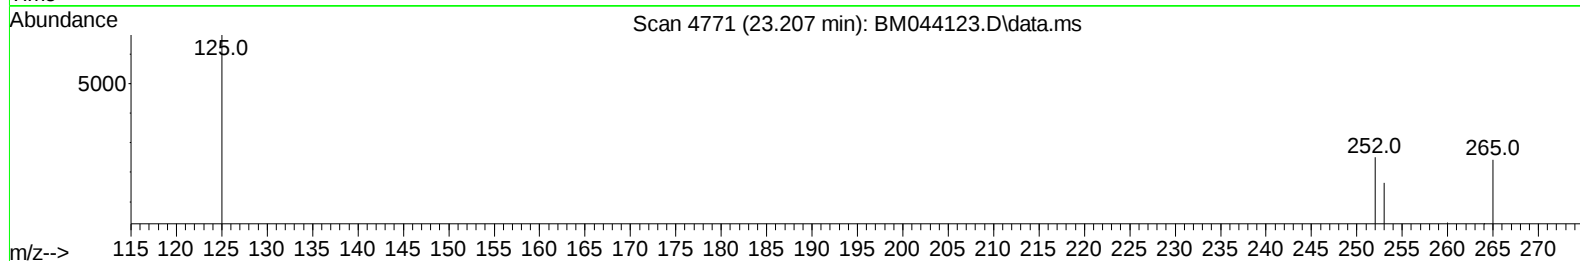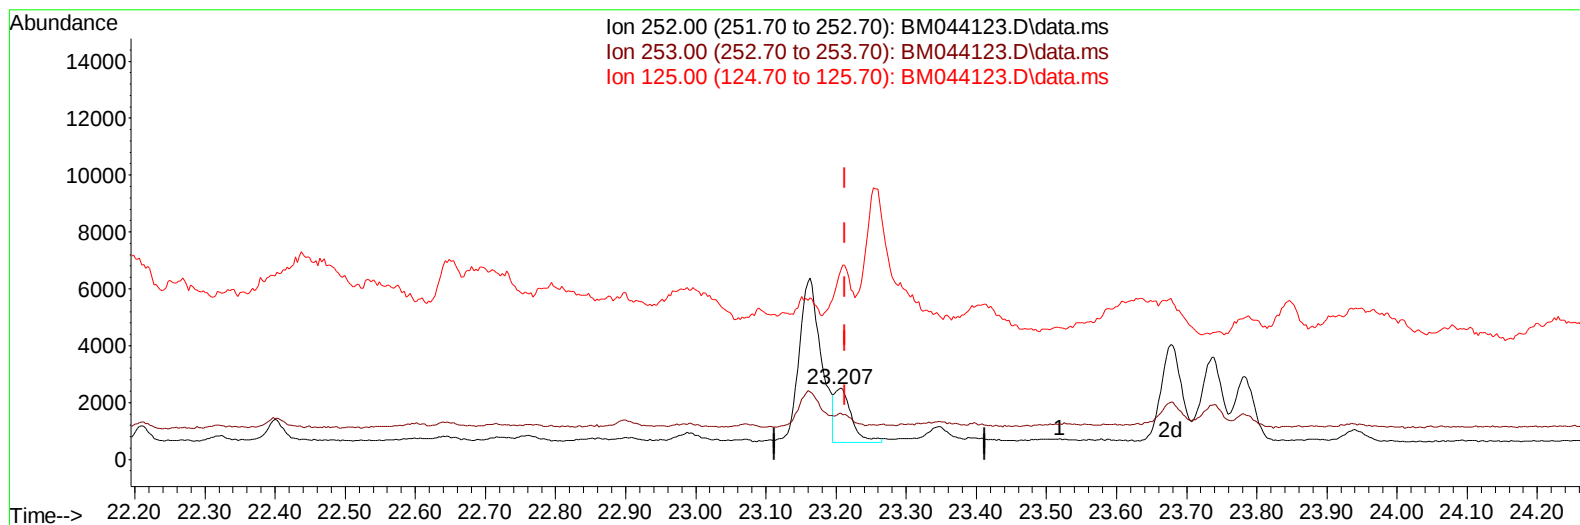

TIC: BM044123.D\data.ms

(25) Benzo(k)fluoranthene

23.207min (-0.006) 0.03 ng/u1 m

response 3215

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	65.31#
125.00	15.40	265.63#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

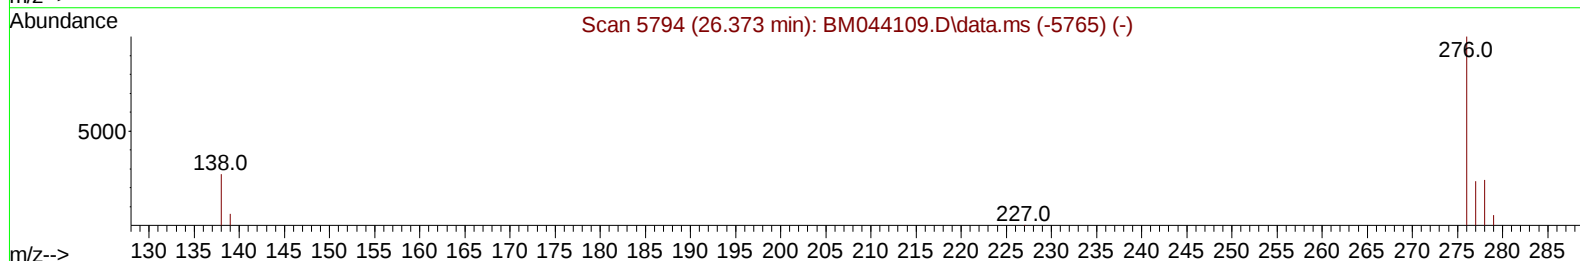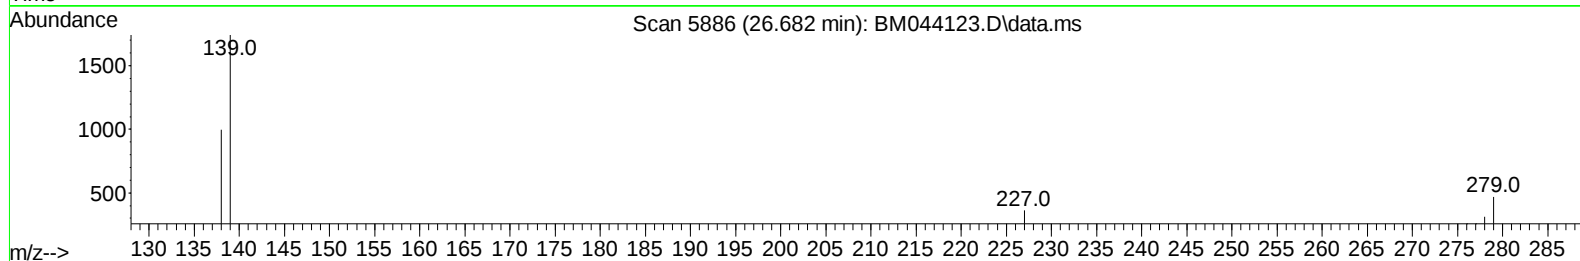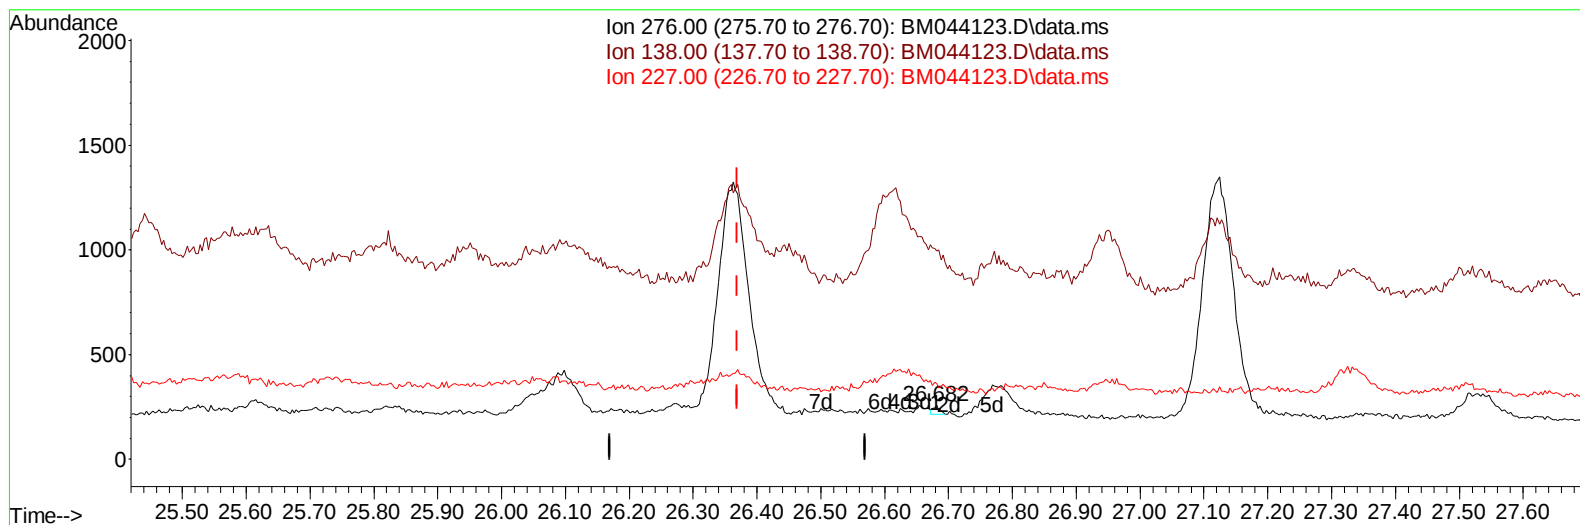

TIC: BM044123.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

26.682min (+ 0.312) 0.00 ng/u1

response	31
Ion	Exp% Act%
276.00	100.00 100.00
138.00	31.50 0.00#
227.00	0.10 0.00#
0.00	0.00 0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044123.D
 Acq On : 16 Feb 2024 04:51
 Operator : MA/JU
 Sample : P1305-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
 Supervised By :mohammad ahmed 02/19/2024

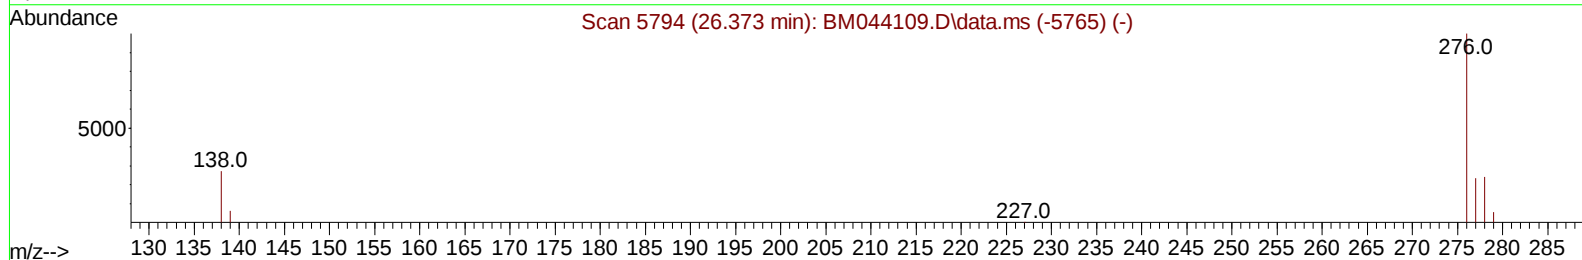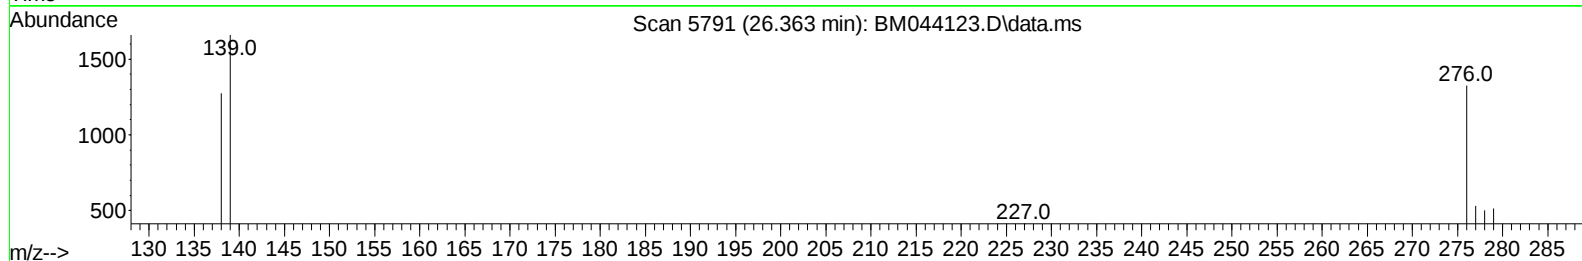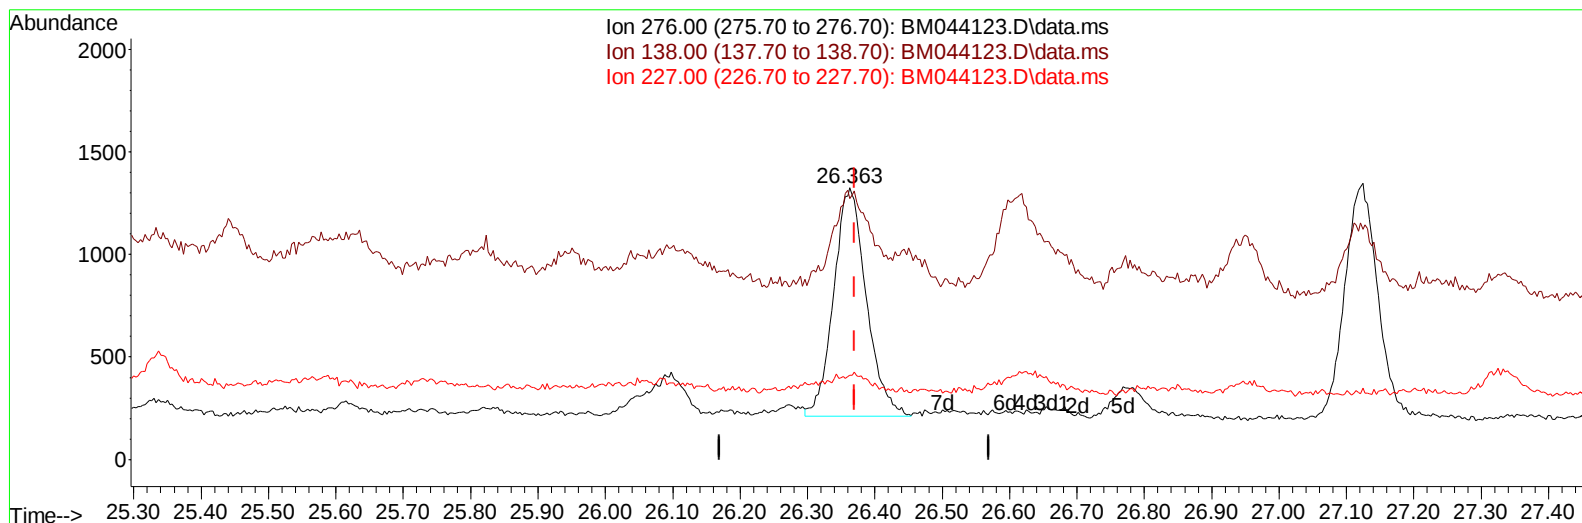

TIC: BM044123.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

26.363min (-0.007) 0.03 ng/ul m

response 3762

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	31.50	0.00#
227.00	0.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

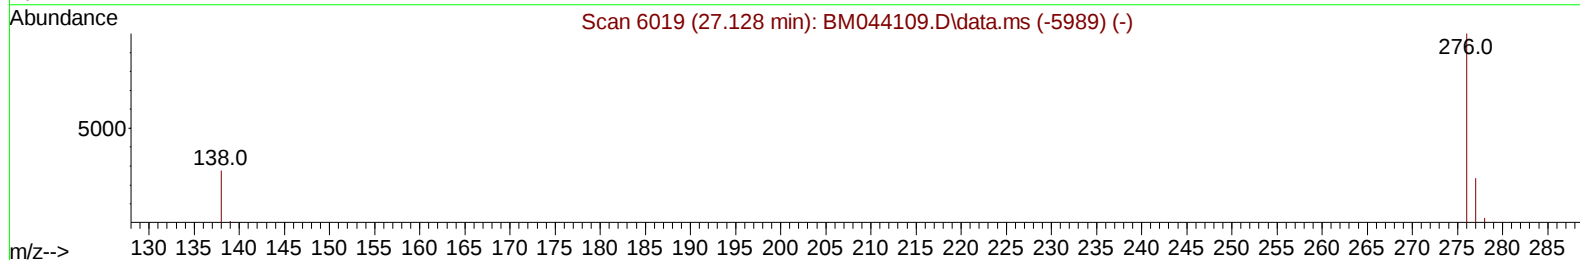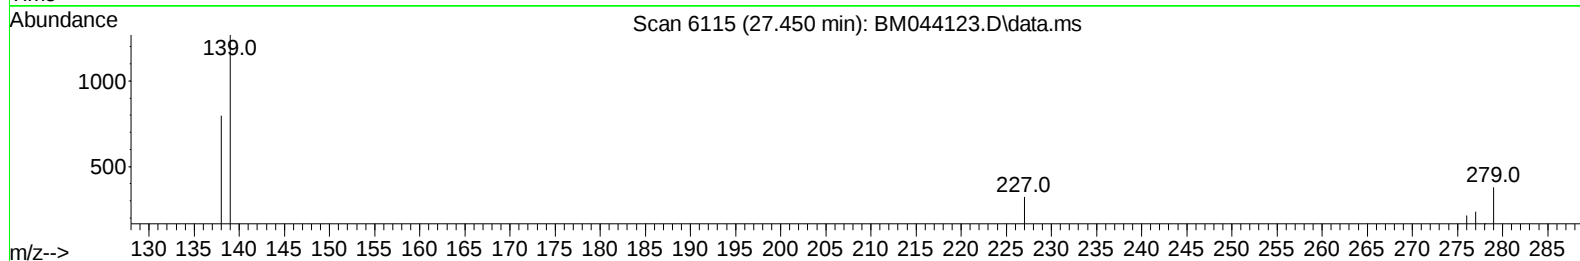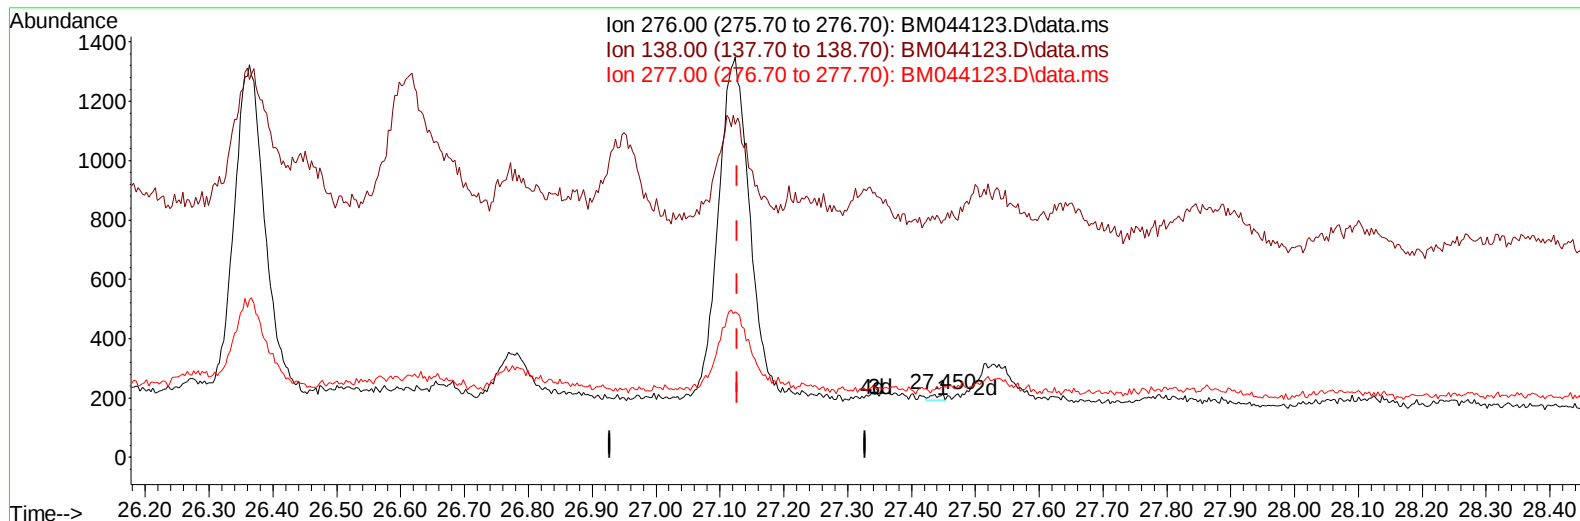

TIC: BM044123.D\data.ms

(29) Benzo(g,h,i)perylene

27.450min (+ 0.322) 0.00 ng/u1

response 23

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	28.40	373.36#
277.00	23.80	109.81#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044123.D
 Acq On : 16 Feb 2024 04:51
 Operator : MA/JU
 Sample : P1305-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
 Supervised By :mohammad ahmed 02/19/2024

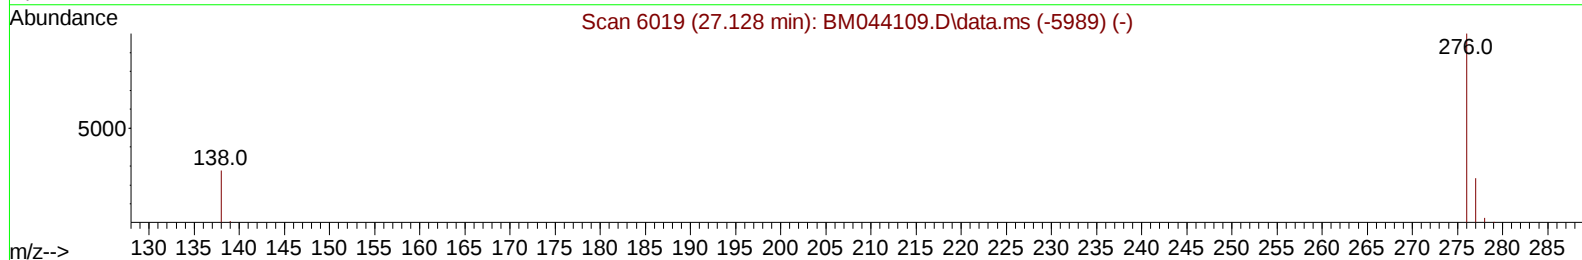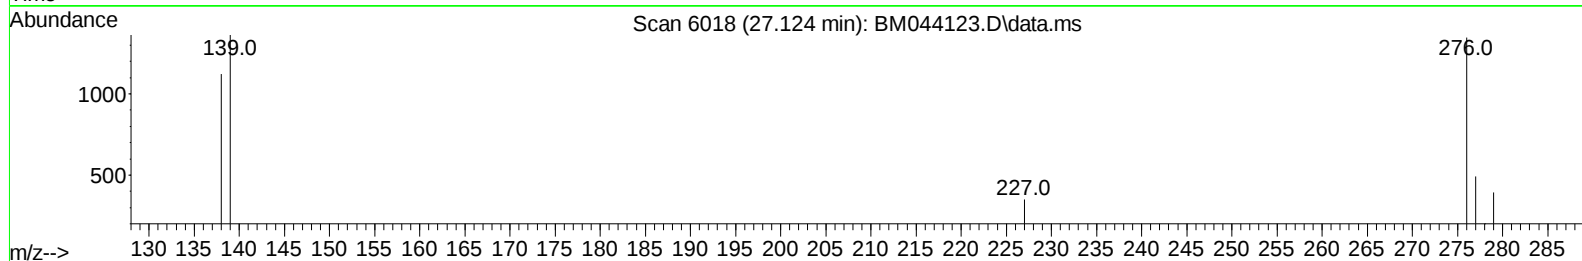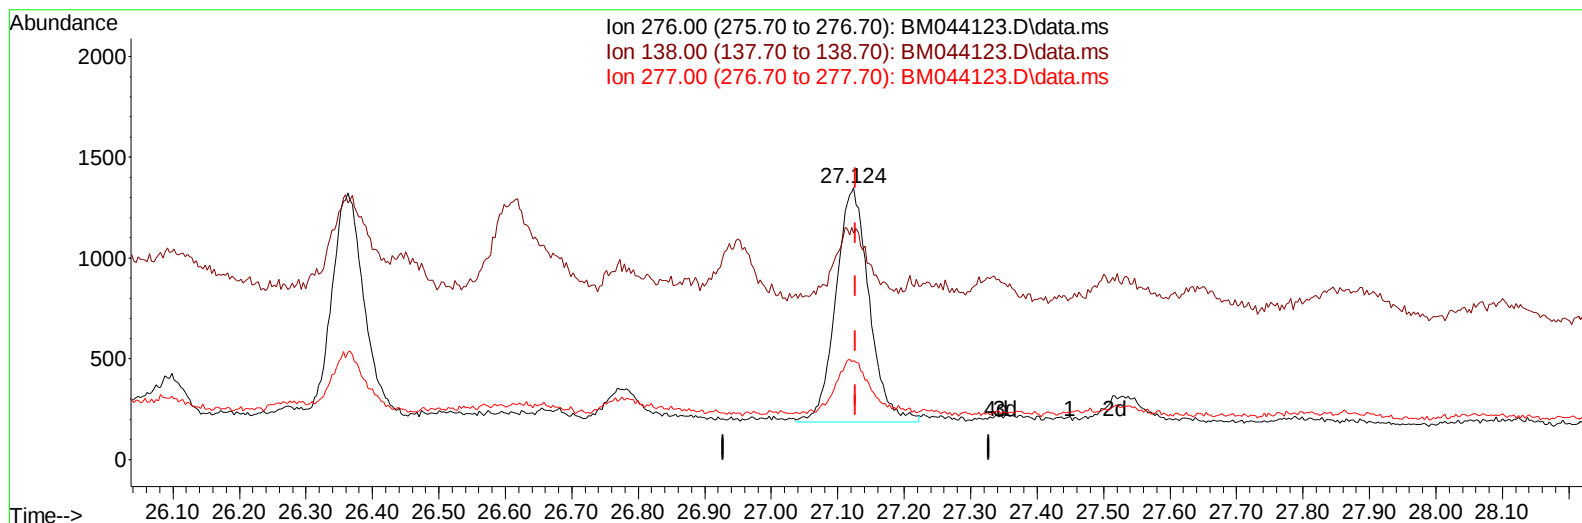

TIC: BM044123.D\data.ms

(29) Benzo(g,h,i)perylene

27.124min (-0.003) 0.04 ng/ul m

response 4067

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	28.40	83.31#
277.00	23.80	36.42#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044123.D
 Acq On : 16 Feb 2024 04:51
 Operator : MA/JU
 Sample : P1305-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FP2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/17/2024
 Supervised By :mohammad ahmed 02/19/2024

Quant Time: Feb 17 03:21:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.905	152		9410	0.400	ng/ul	0.00
4) Naphthalene-d8	10.704	136		32392	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164		18487	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.296	188		39101m	0.400	ng/ul	0.00
17) Chrysene-d12	21.497	240		25180m	0.400	ng/ul	0.00
23) Perylene-d12	23.885	264		24978m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.352	96		62282	4.674	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152		14530	0.320	ng/ul	0.00
18) Fluoranthene-d10	19.331	212		29269m	0.390	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.754	128		8425	0.088	ng/ul	97
7) 2-Methylnaphthalene	12.365	142		13650	0.230	ng/ul	100
8) 1-Methylnaphthalene	12.585	142		6186	0.103	ng/ul	100
12) Fluorene	15.597	166		3461	0.042	ng/ul#	89
14) Pentachlorophenol	16.942	266		505	0.036	ng/ul	87
15) Phenanthrene	17.339	178		48449	0.391	ng/ul	100
19) Fluoranthene	19.359	202		16888m	0.147	ng/ul	
20) Pyrene	19.726	202		15842m	0.131	ng/ul	
21) Benzo(a)anthracene	21.479	228		5293m	0.046	ng/ul	
22) Chrysene	21.532	228		23782m	0.191	ng/ul	
24) Benzo(b)fluoranthene	23.163	252		12412m	0.120	ng/ul	
25) Benzo(k)fluoranthene	23.207	252		3215m	0.029	ng/ul	
27) Indeno(1,2,3-cd)pyrene	26.363	276		3762m	0.031	ng/ul	
29) Benzo(g,h,i)perylene	27.124	276		4067m	0.038	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044123.D
Acq On : 16 Feb 2024 04:51
Operator : MA/JU
Sample : P1305-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP2

Manual IntegrationsAPPROVED

Quant Time: Feb 17 03:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

