




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

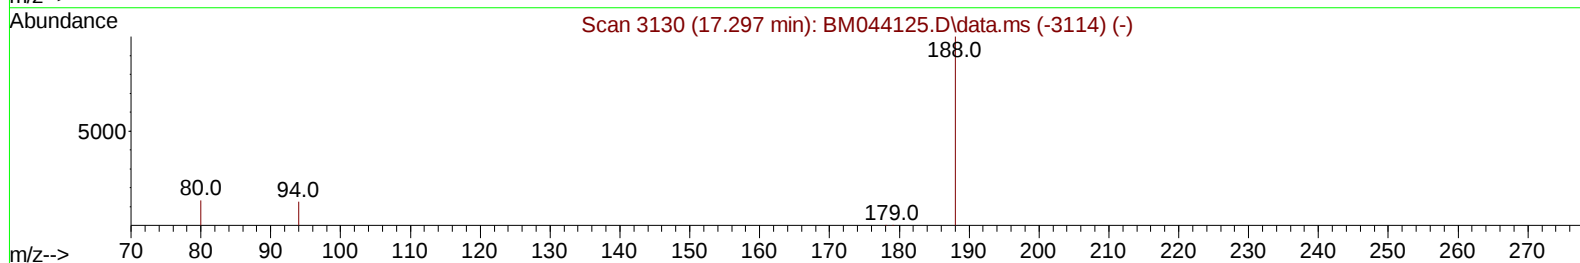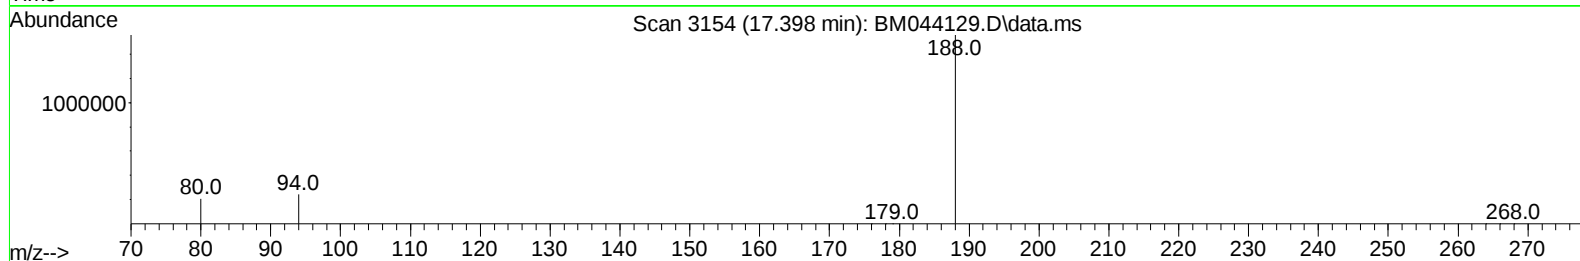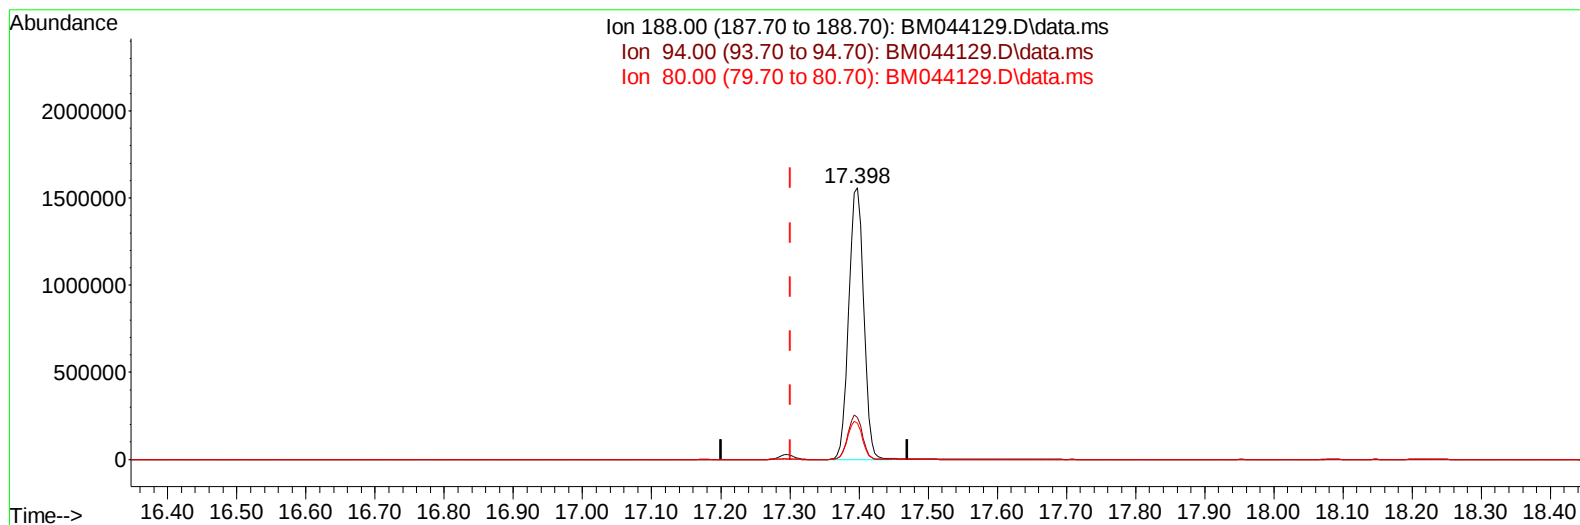

TIC: BM044129.D\data.ms

(13) Phenanthrene-d10 (I)

17.398min (+ 0.097) 0.40 ng/u1

response 2332770

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	15.49#
80.00	13.40	13.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

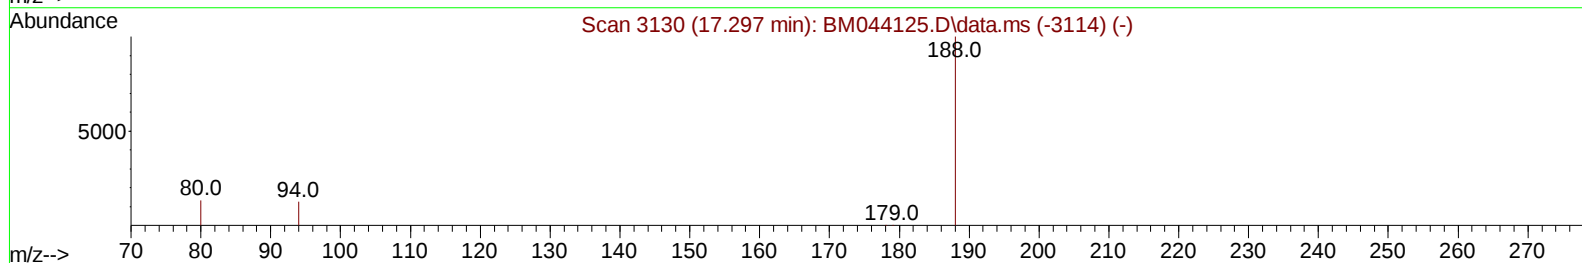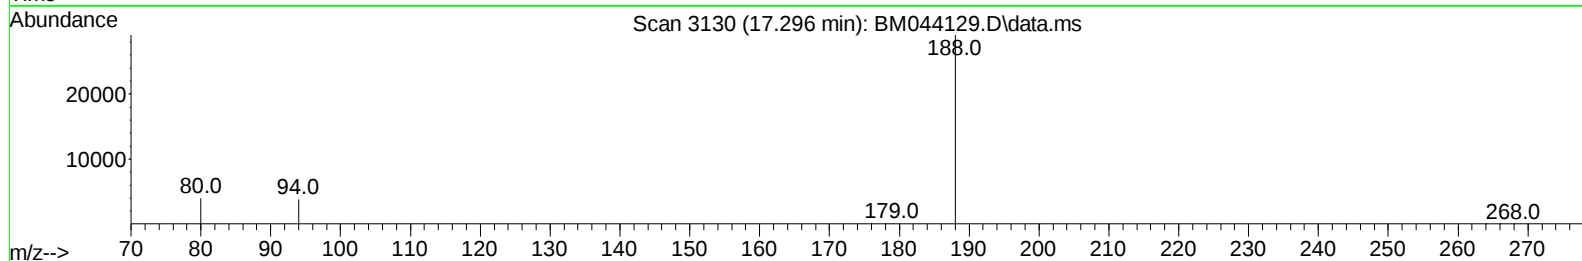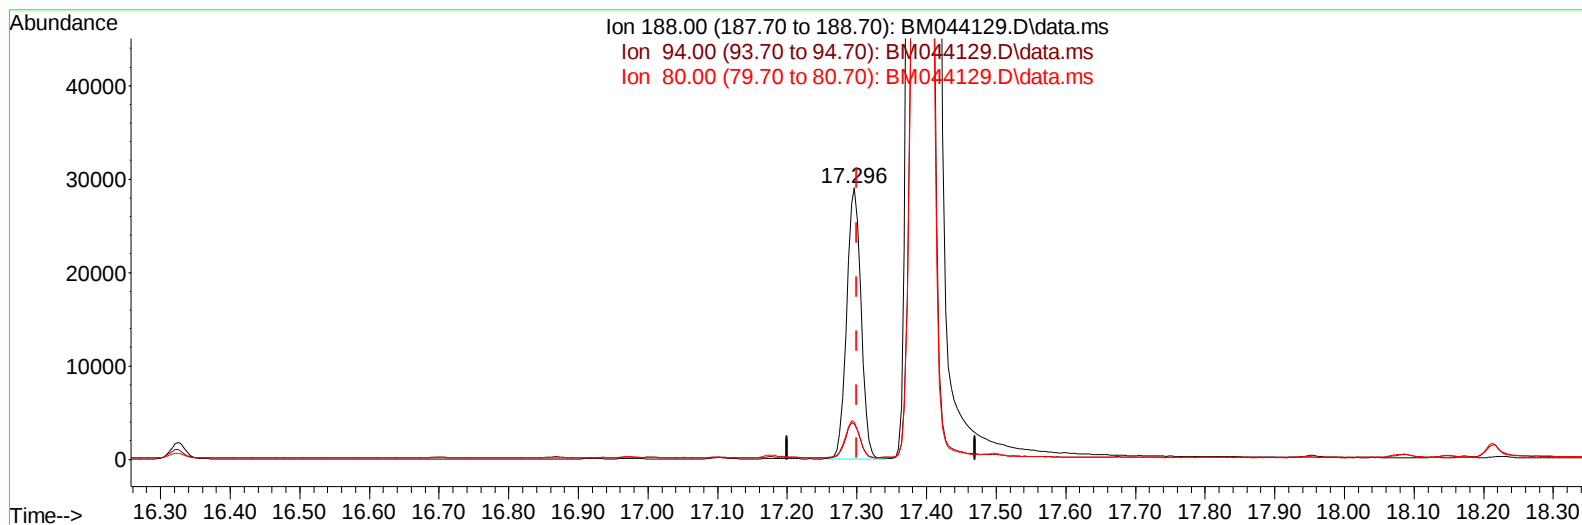

TIC: BM044129.D\data.ms

(13) Phenanthrene-d10 (I)

17.296min (-0.004) 0.40 ng/ul m

response 41385

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	13.16
80.00	13.40	13.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

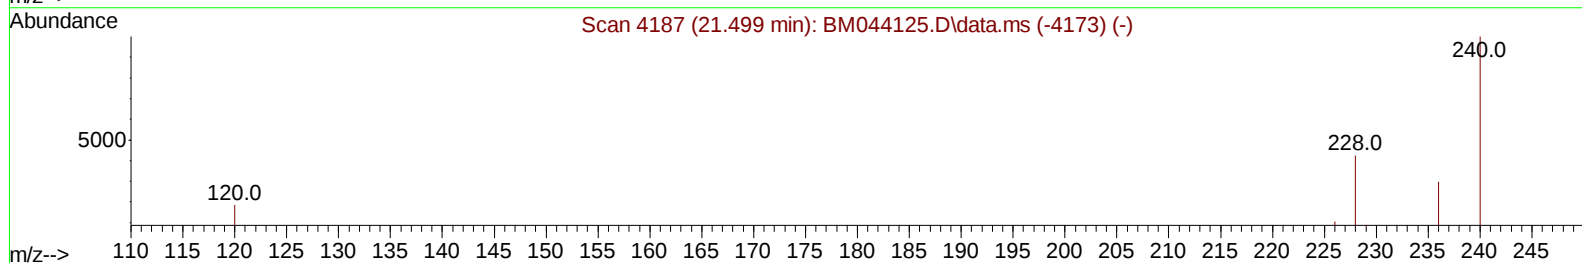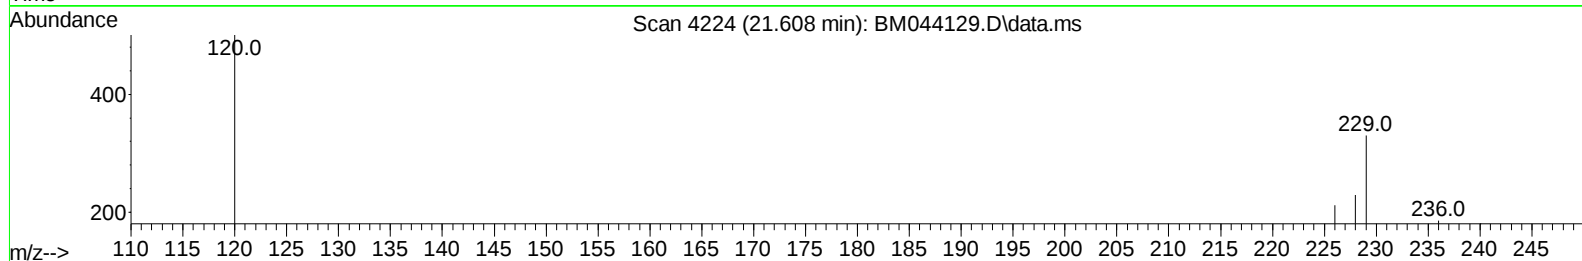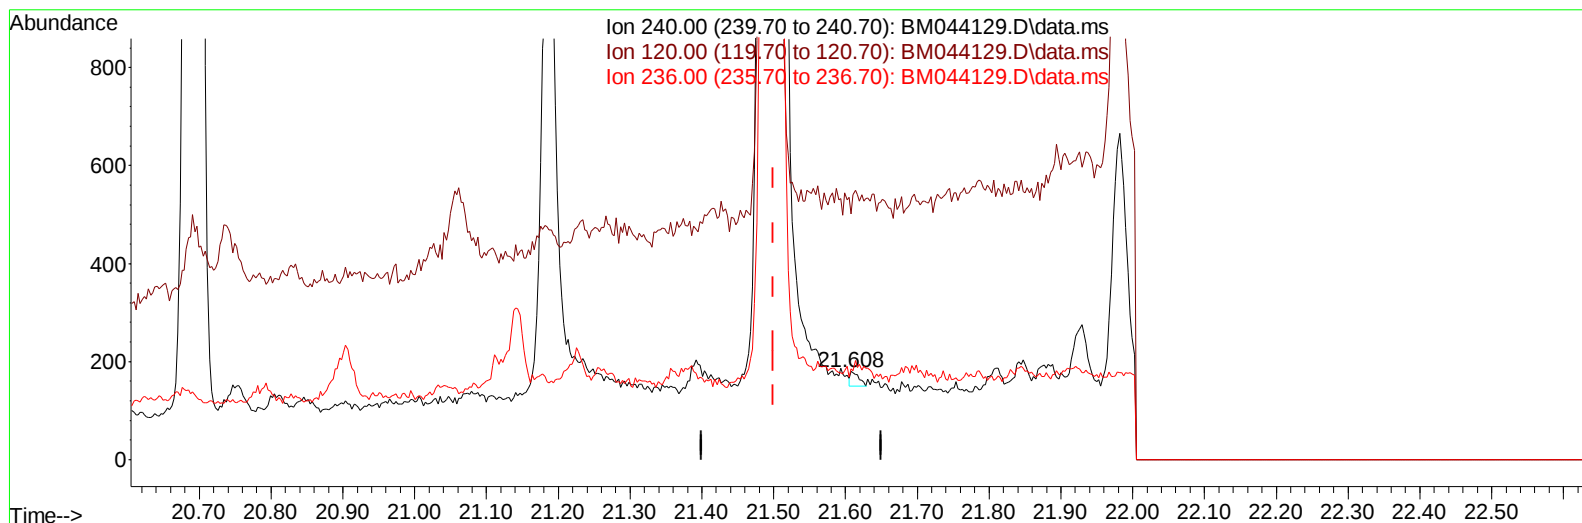

TIC: BM044129.D\data.ms

(17) Chrysene-d12

21.608min (+ 0.108) 0.40 ng/u1

response 24

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.50	278.33#
236.00	30.60	102.78#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

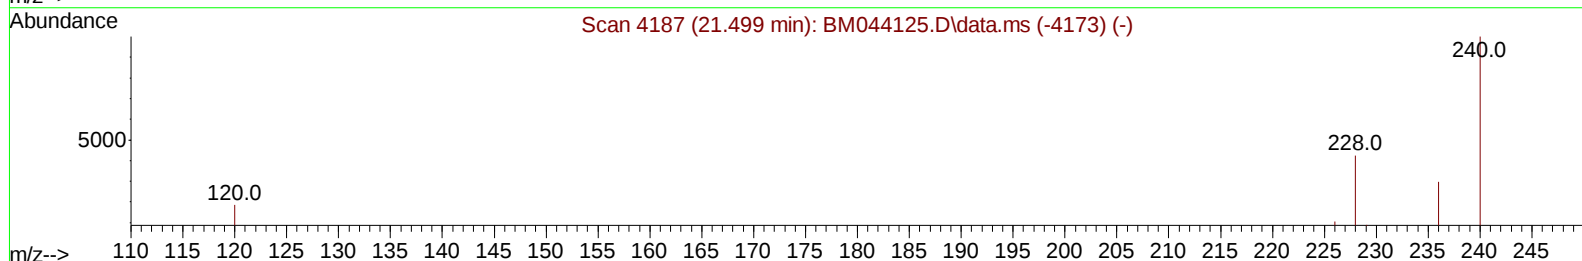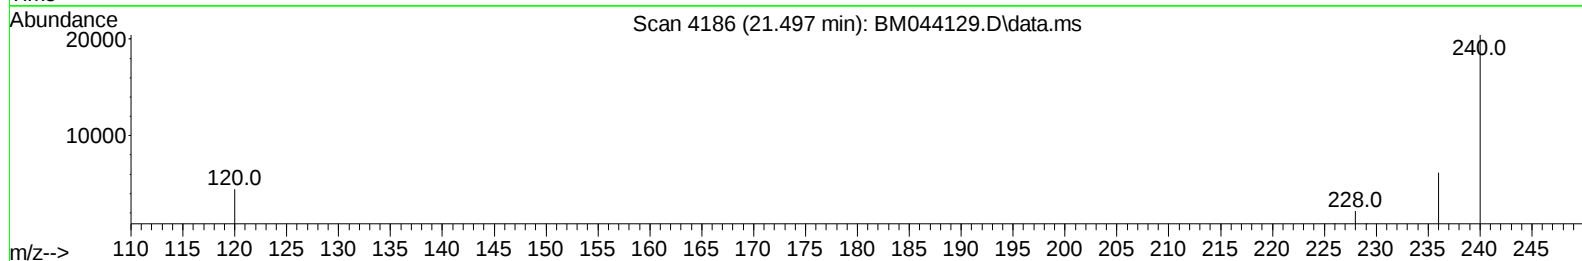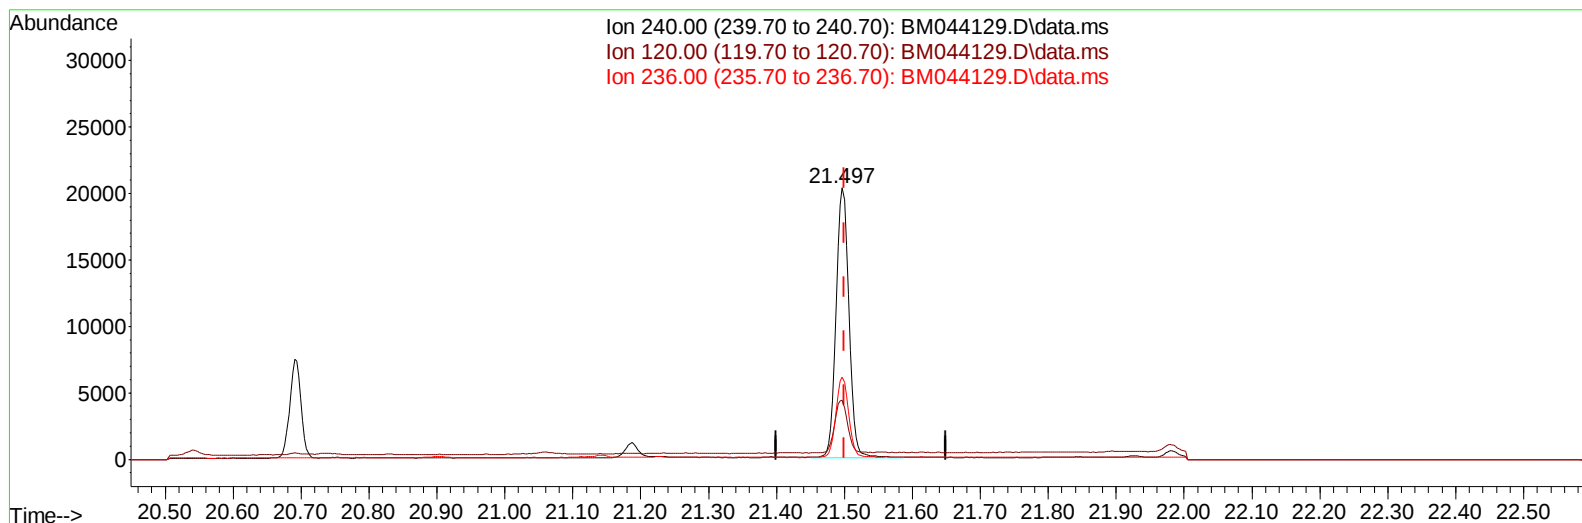

TIC: BM044129.D\data.ms

(17) Chrysene-d12

21.497min (-0.003) 0.40 ng/ul m

response 26590

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.50	21.78
236.00	30.60	30.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

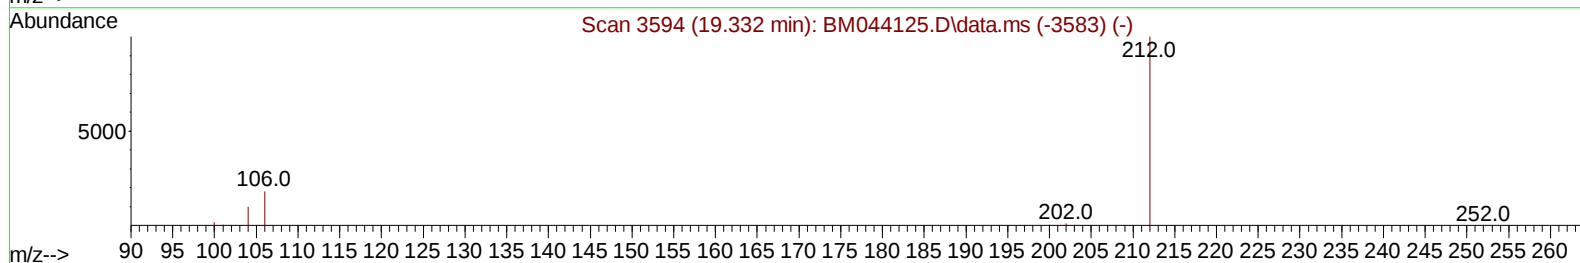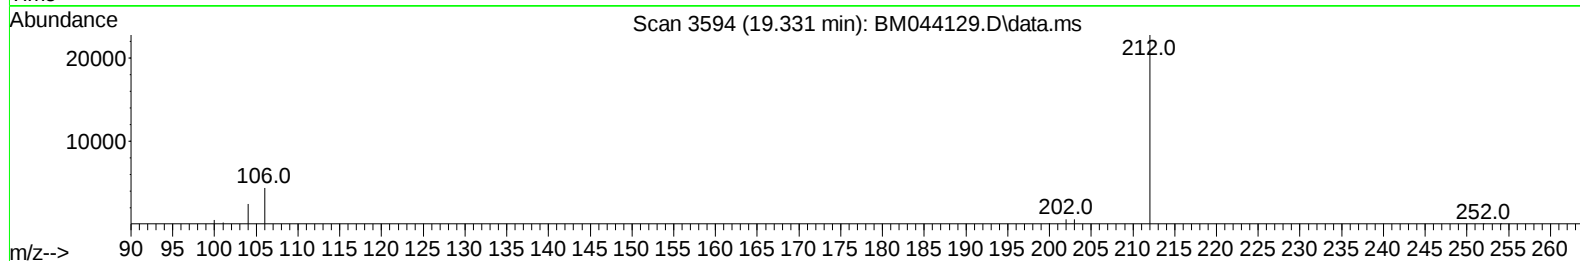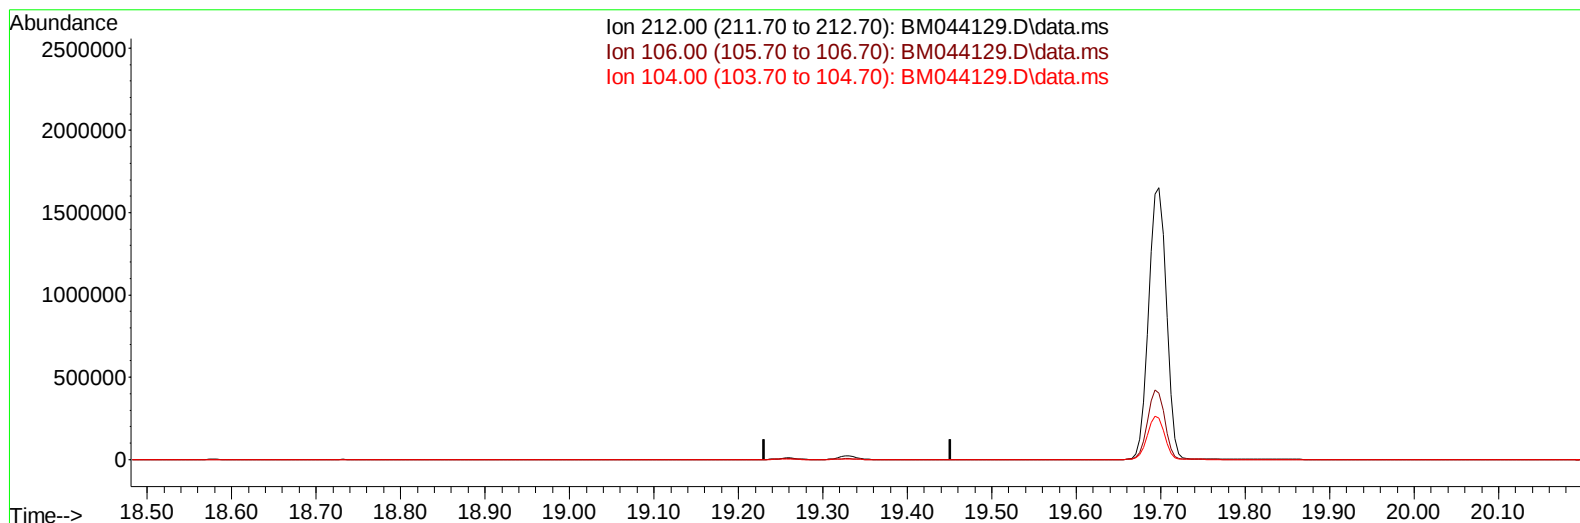

TIC: BM044129.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.331min (-19.331) 0.00 ng/u1

response 0

Ion	Exp%	Act%
212.00	100.00	0.00
106.00	18.40	0.00#
104.00	10.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

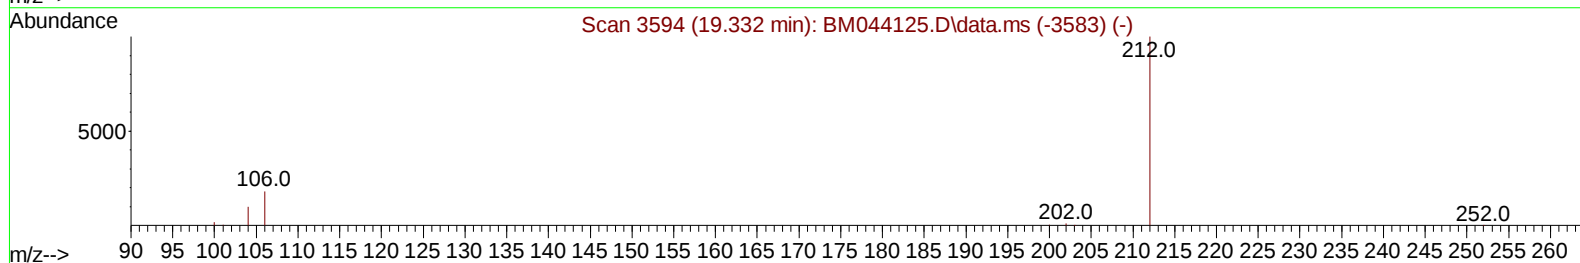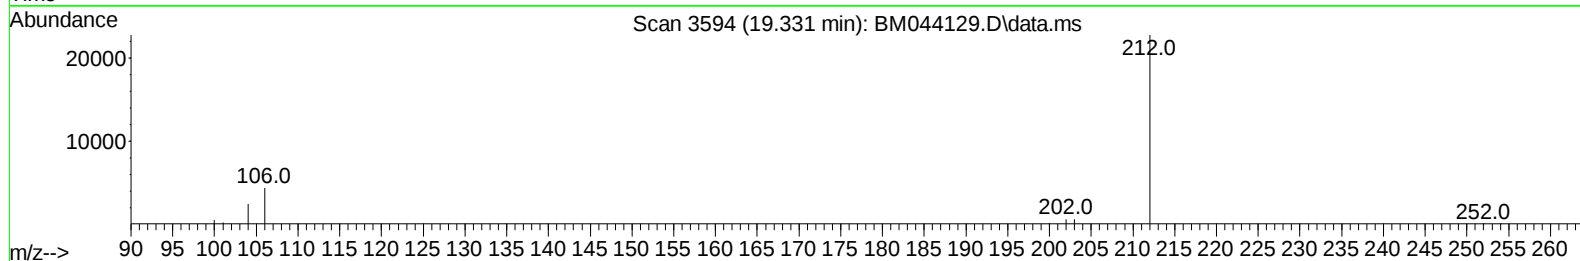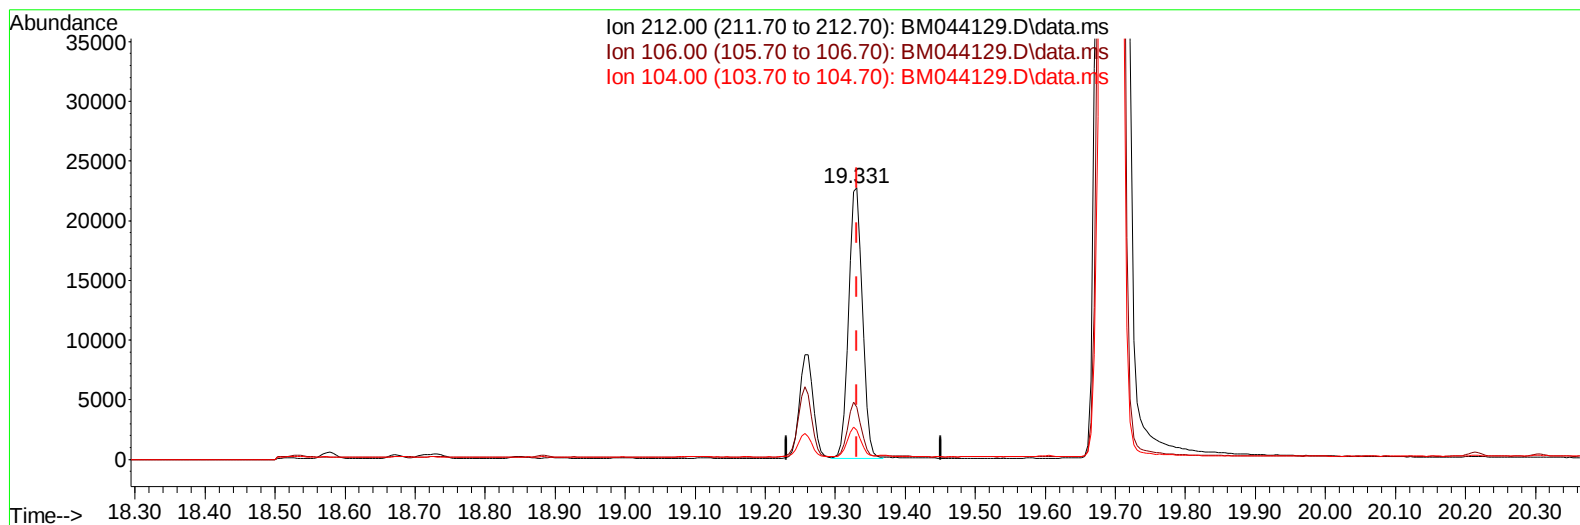

TIC: BM044129.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.331min (+ 0.000) 0.39 ng/ul m

response 30653

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	18.40	0.00#
104.00	10.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

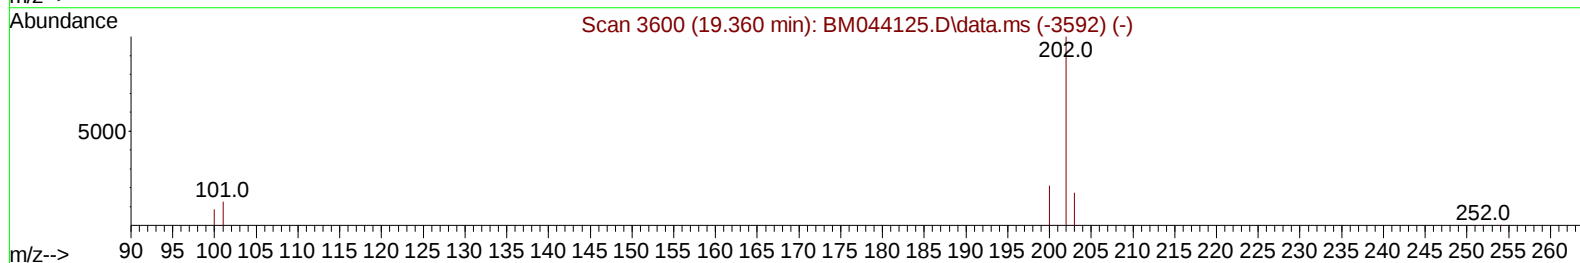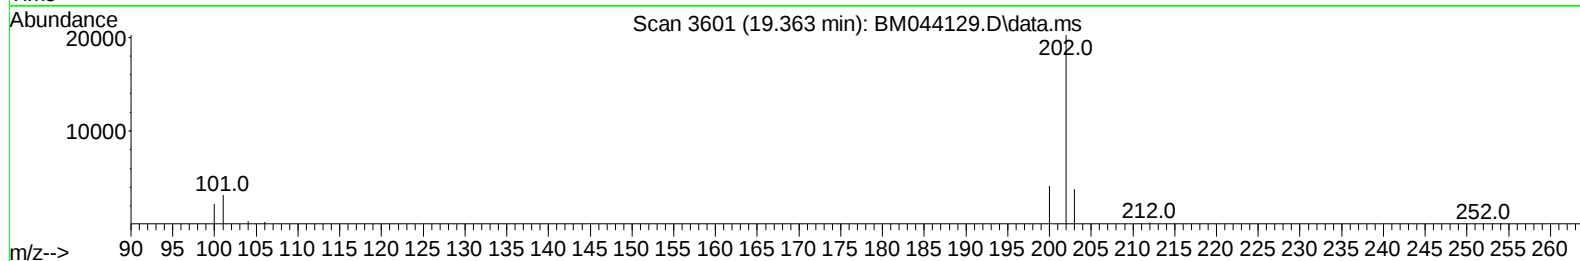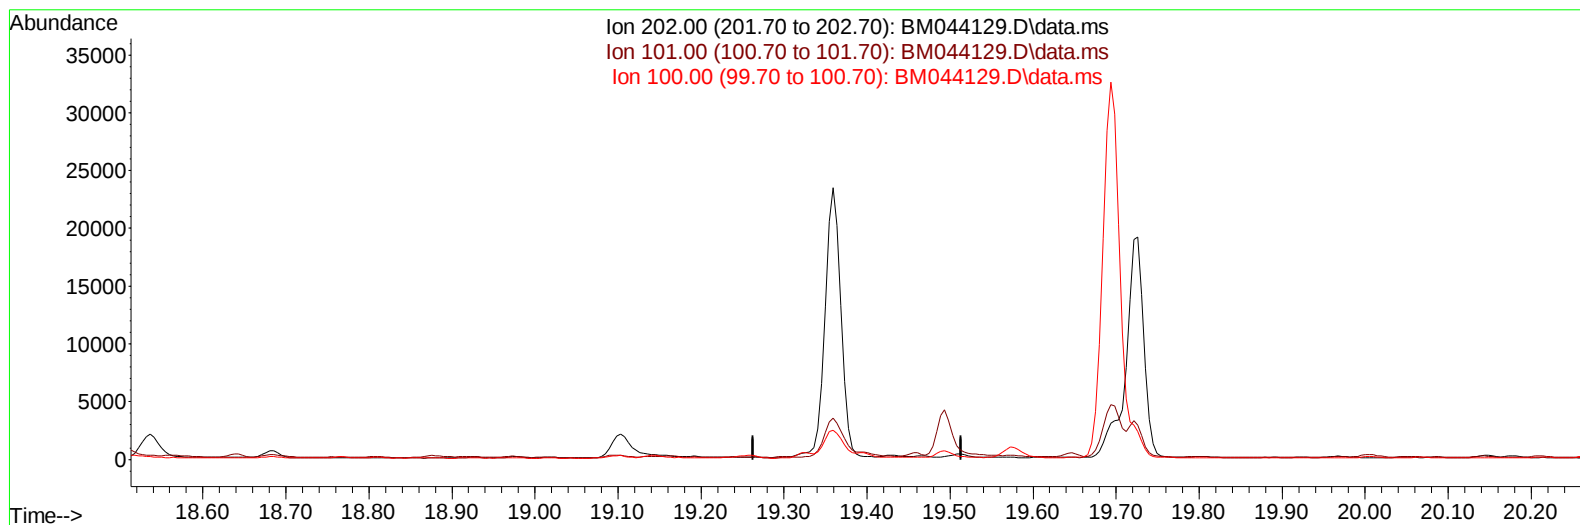

TIC: BM044129.D\data.ms

(19) Fluoranthene (C)

19.363min (-19.363) 0.00 ng/u1

response 0

Ion	Exp%	Act%
202.00	100.00	0.00
101.00	12.20	0.00#
100.00	8.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

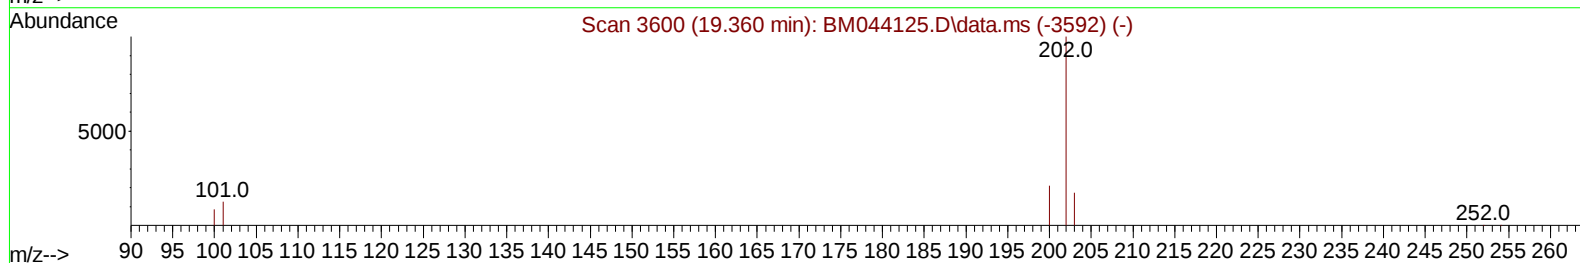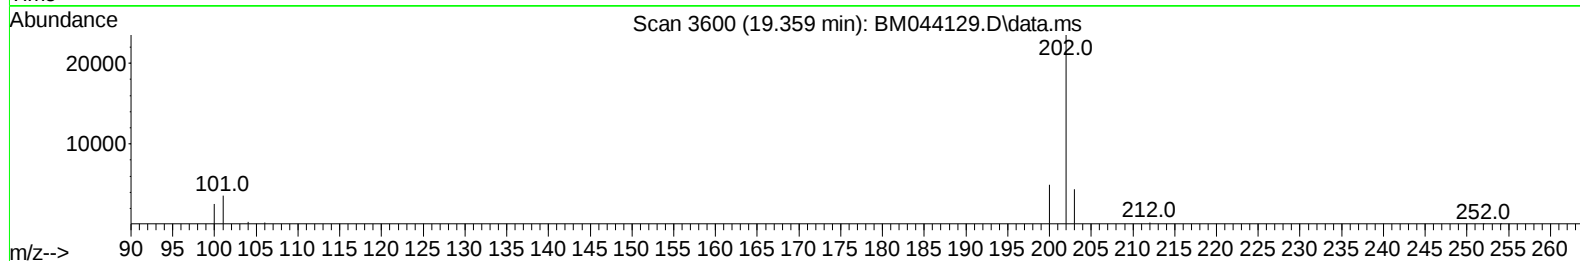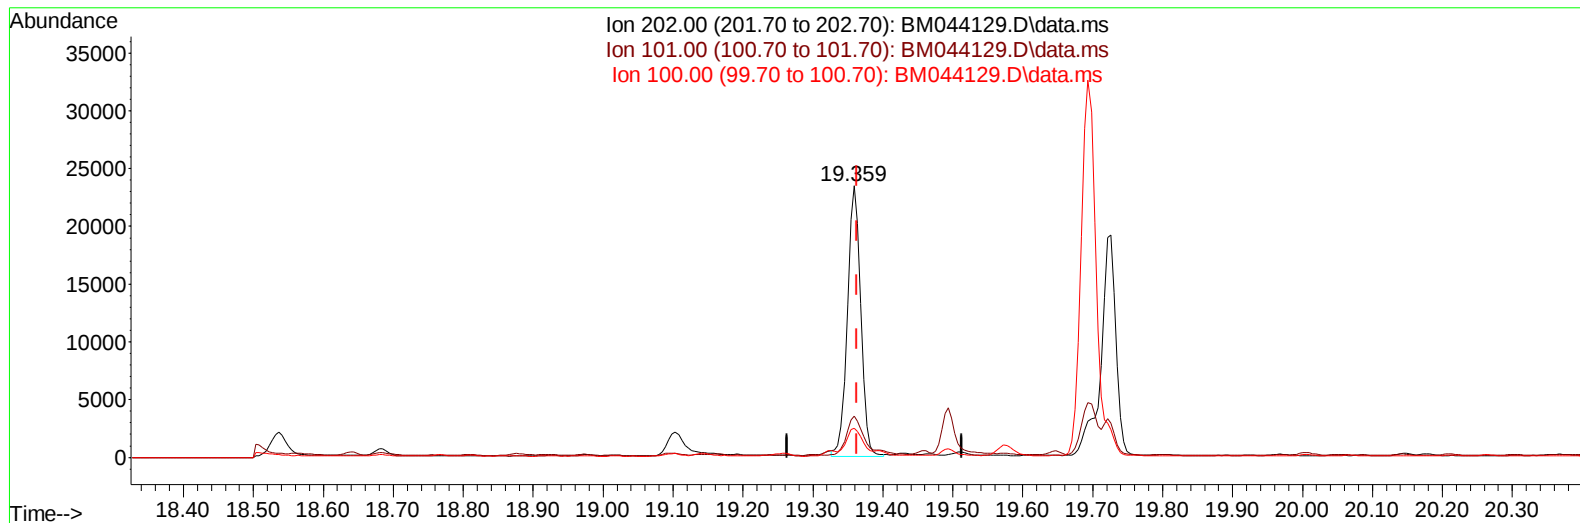

TIC: BM044129.D\data.ms

(19) Fluoranthene (C)

19.359min (-0.005) 0.26 ng/ul m

response 31190

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.20	15.18#
100.00	8.70	10.81#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

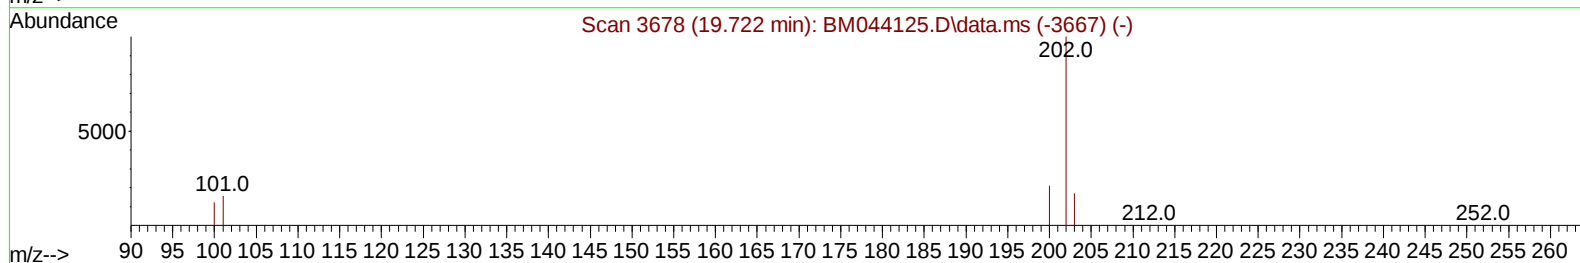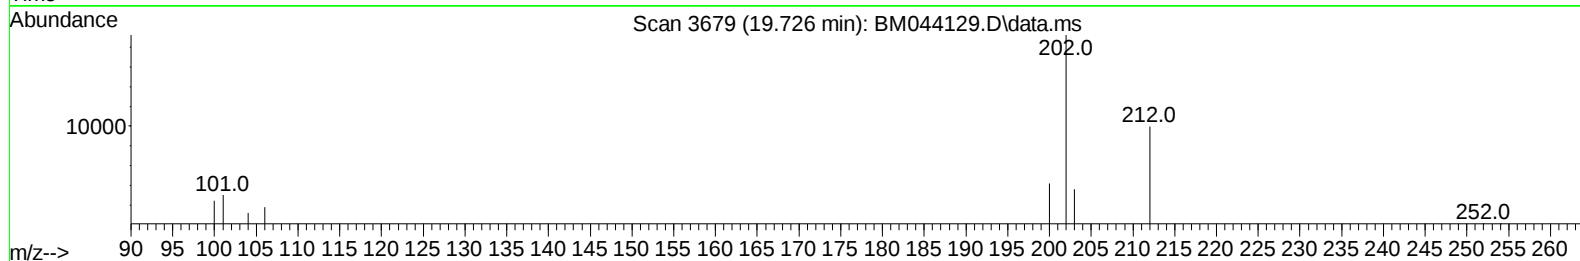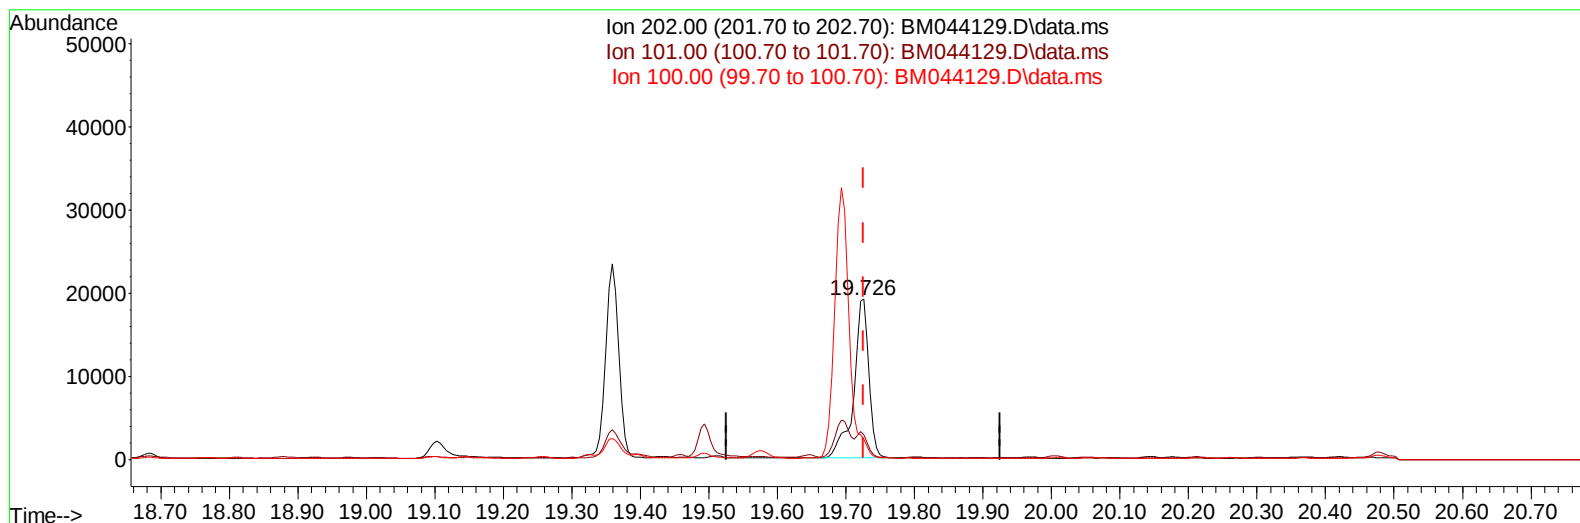

TIC: BM044129.D\data.ms

(20) Pyrene

19.726min (+ 0.000) 0.23 ng/u1

response 29069

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.00	15.49
100.00	10.80	12.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

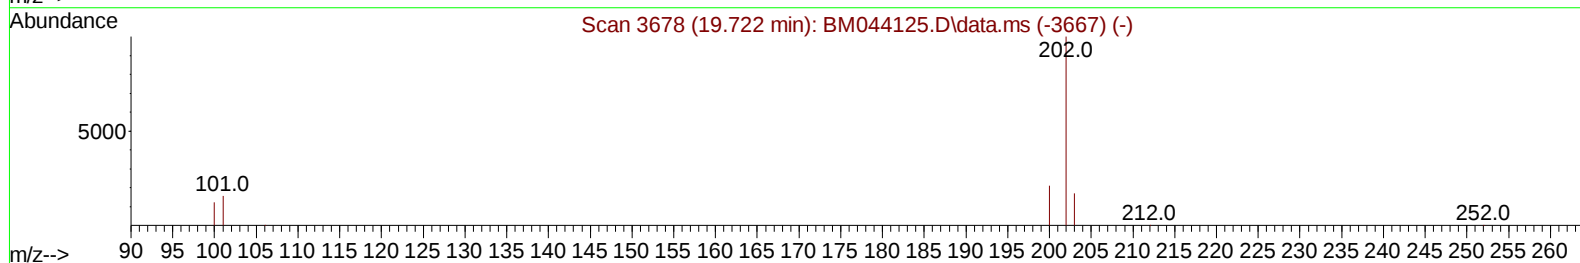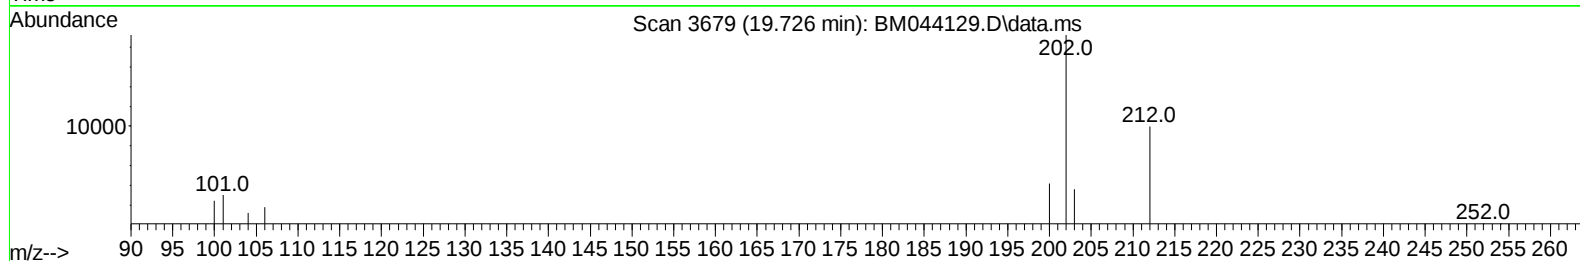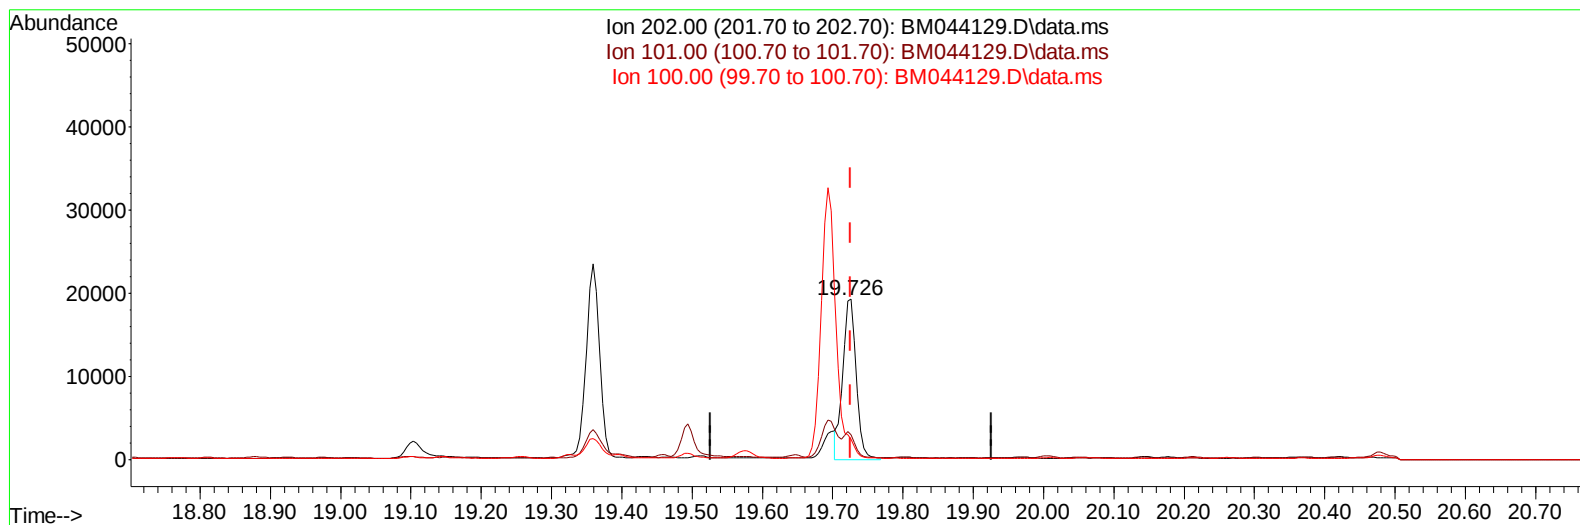

TIC: BM044129.D\data.ms

(20) Pyrene

19.726min (+ 0.000) 0.20 ng/ul m

response 25903

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.00	15.49
100.00	10.80	12.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

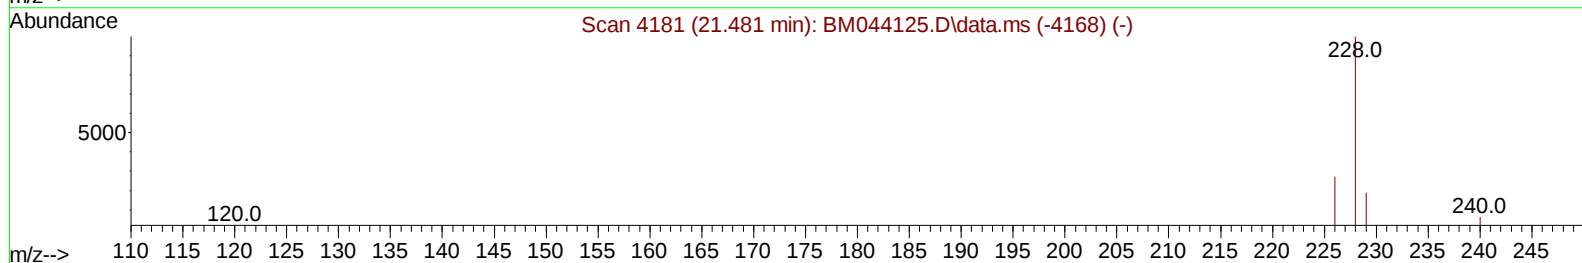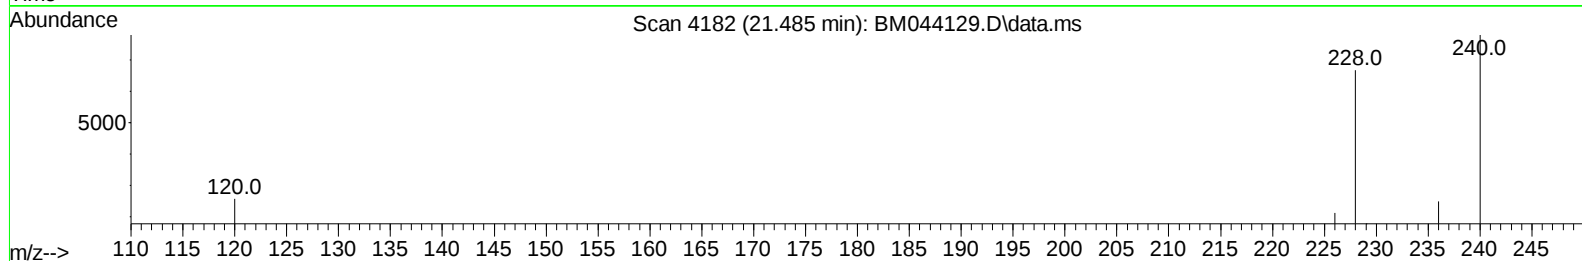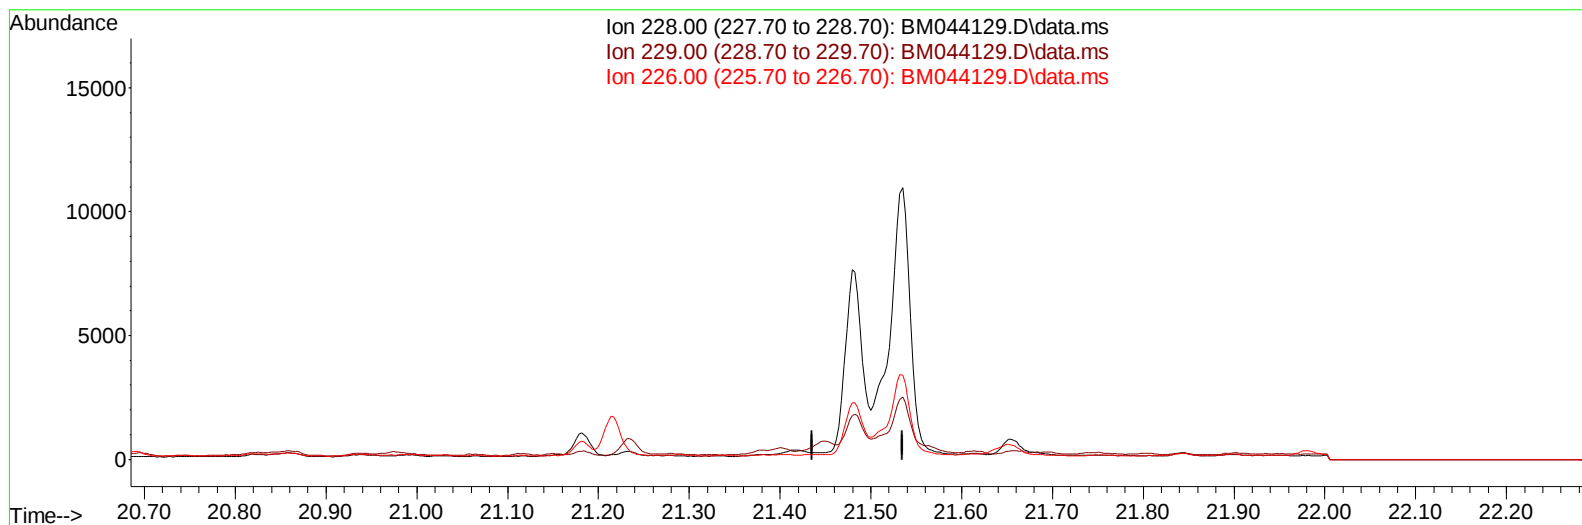

TIC: BM044129.D\data.ms

(21) Benzo(a)anthracene

21.485min (-21.485) 0.00 ng/u1

response 0

Ion	Exp%	Act%
228.00	100.00	0.00
229.00	19.30	0.00#
226.00	27.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

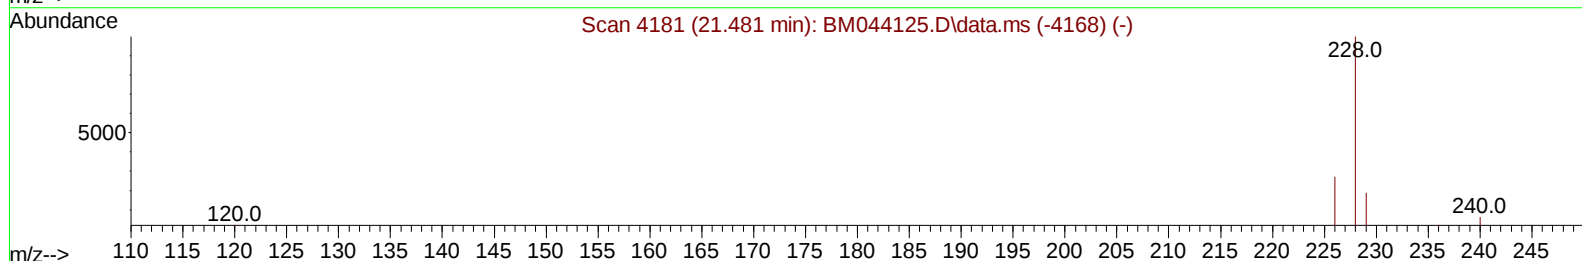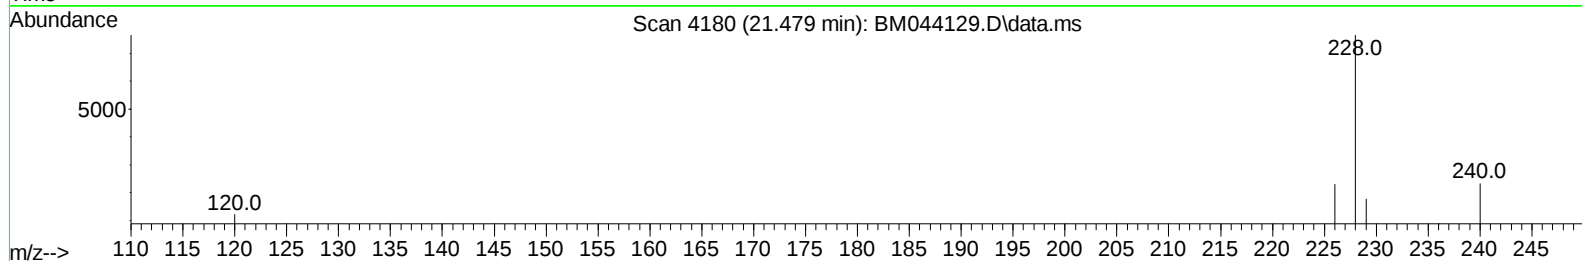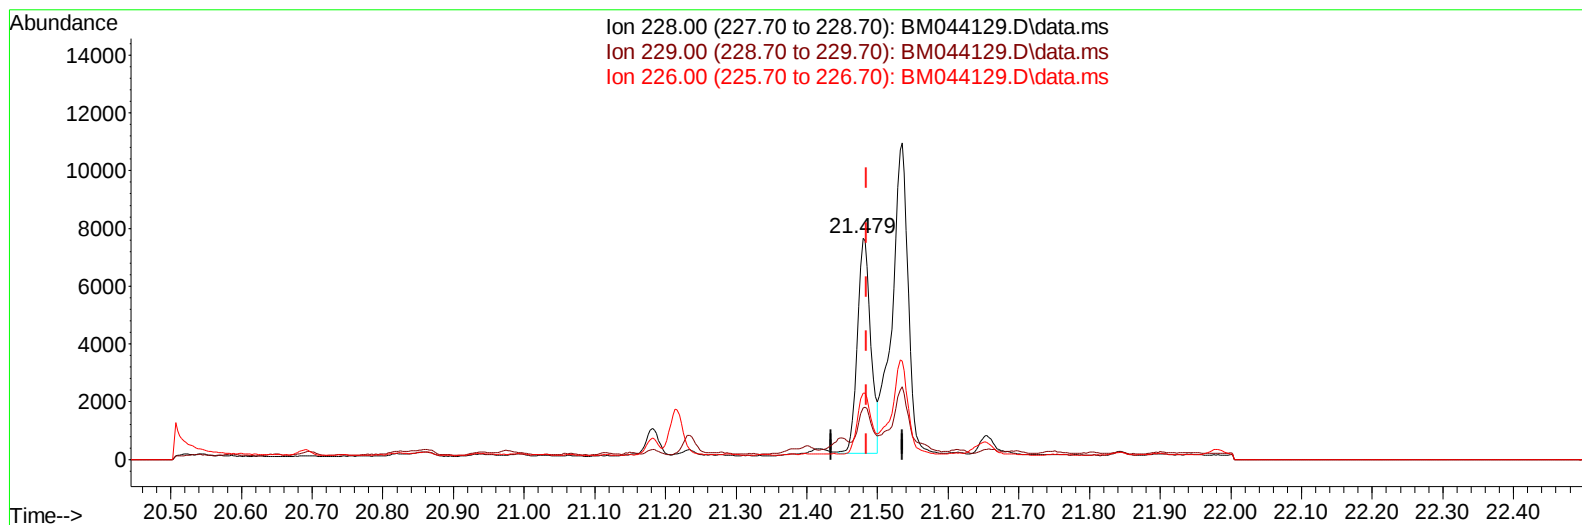

TIC: BM044129.D\data.ms

(21) Benzo(a)anthracene

21.479min (-0.006) 0.08 ng/ul m

response 9825

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.30	23.29#
226.00	27.60	30.01
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

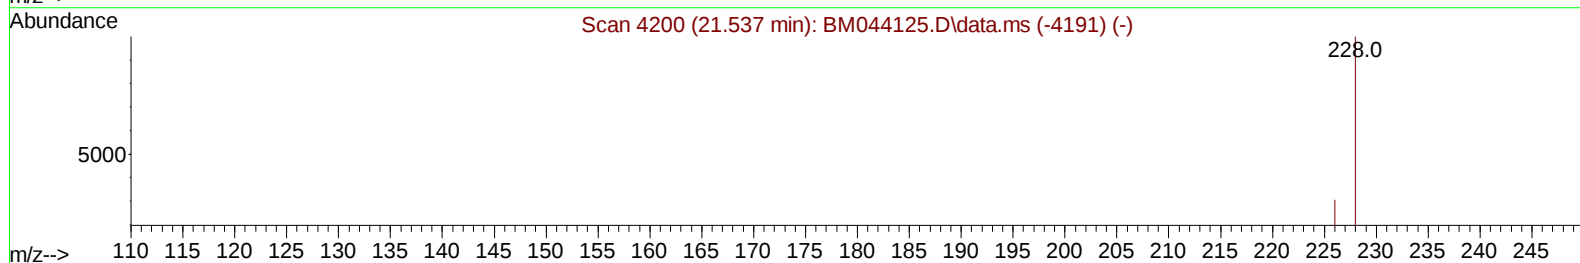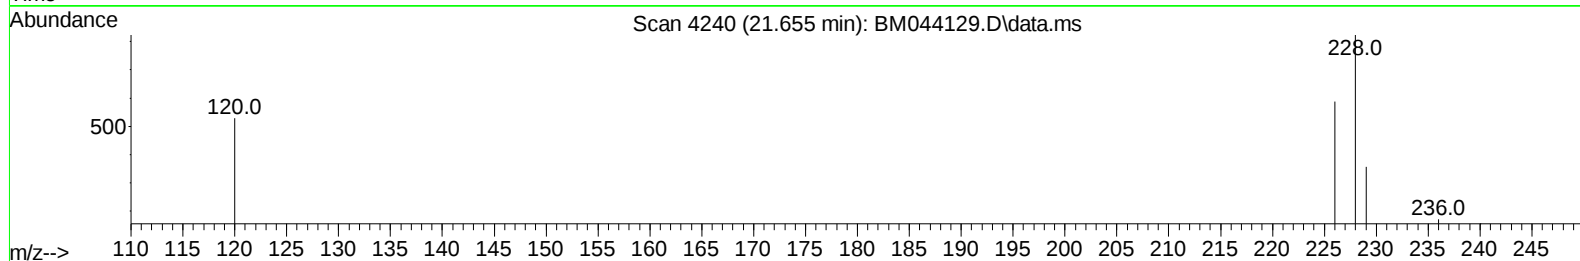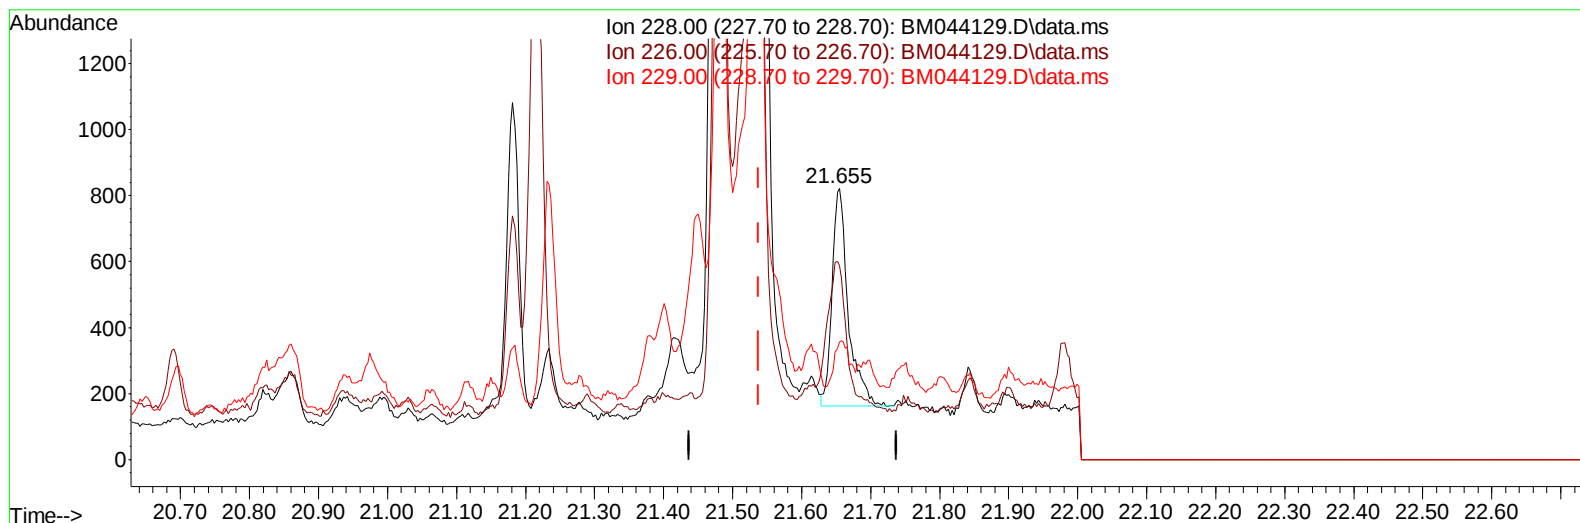

TIC: BM044129.D\data.ms

(22) Chrysene

21.655min (+ 0.117) 0.01 ng/u1

response 1067

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.20	71.32#
229.00	19.70	43.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

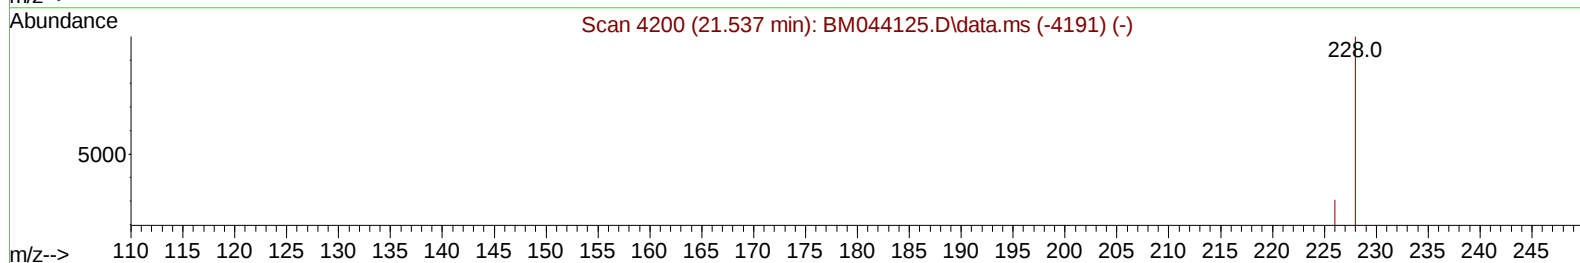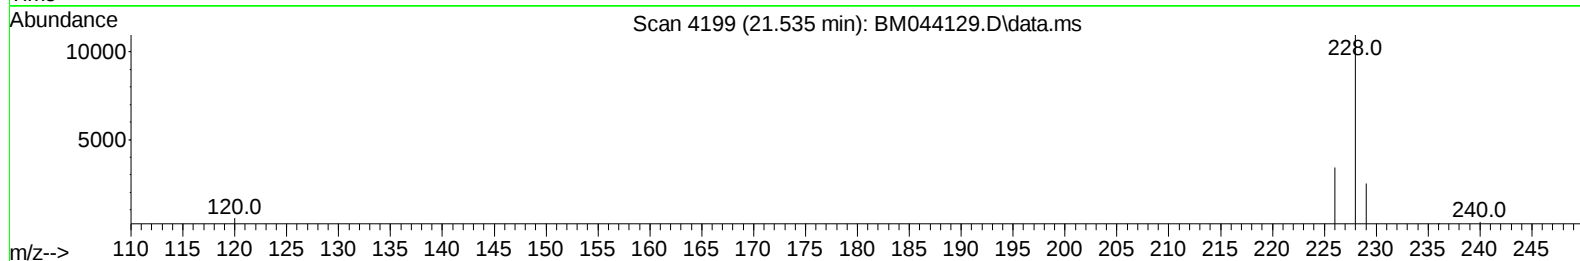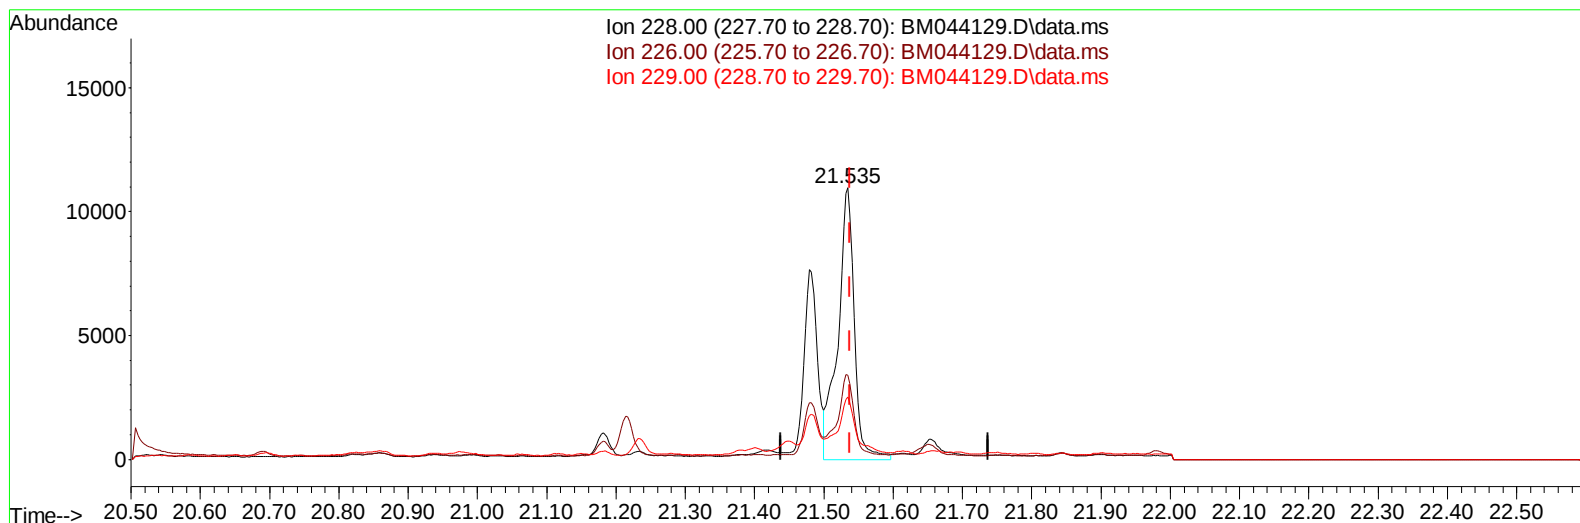

TIC: BM044129.D\data.ms

(22) Chrysene

21.535min (-0.003) 0.14 ng/ul m

response 18130

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.20	31.10
229.00	19.70	22.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

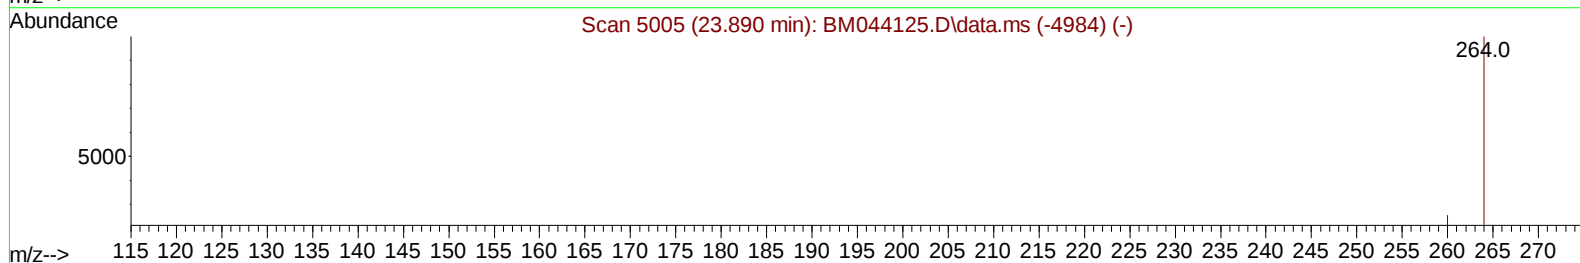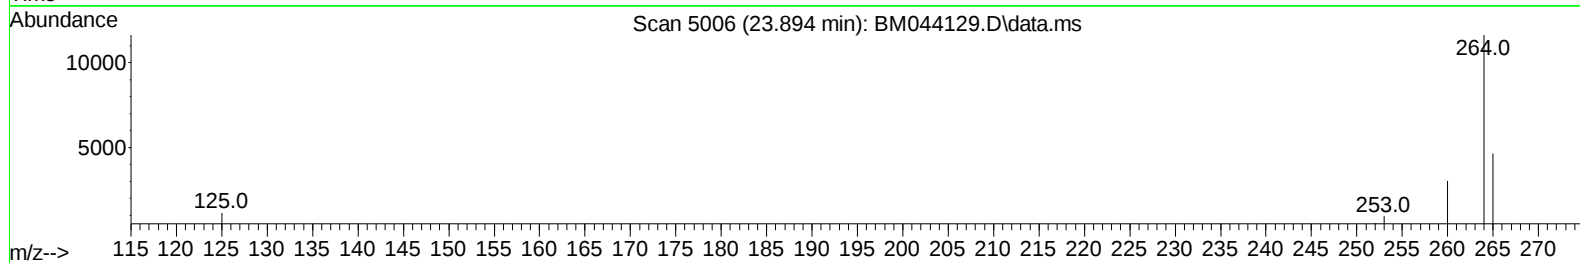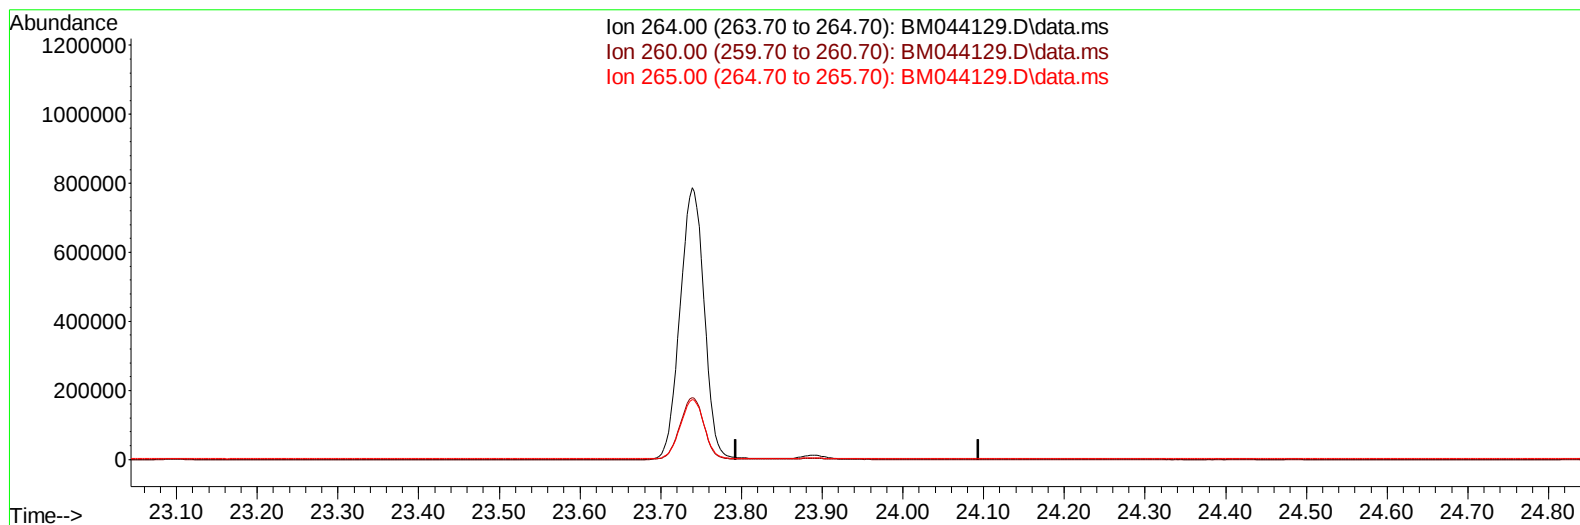

TIC: BM044129.D\data.ms

(23) Perylene-d12 (I)

23.894min (-23.894) 0.00 ng/u1

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.00	0.00#
265.00	45.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

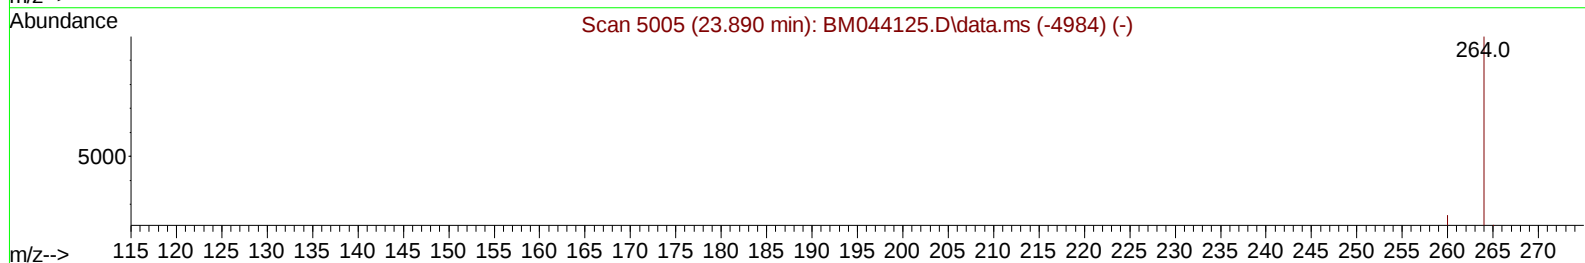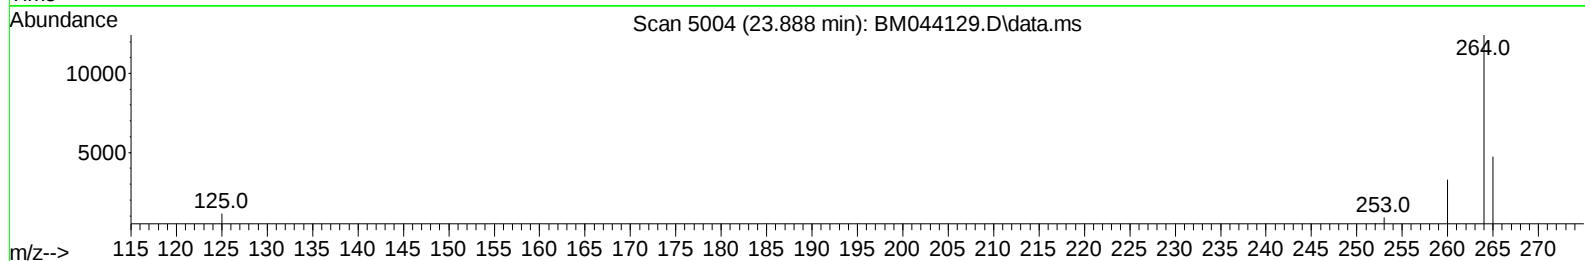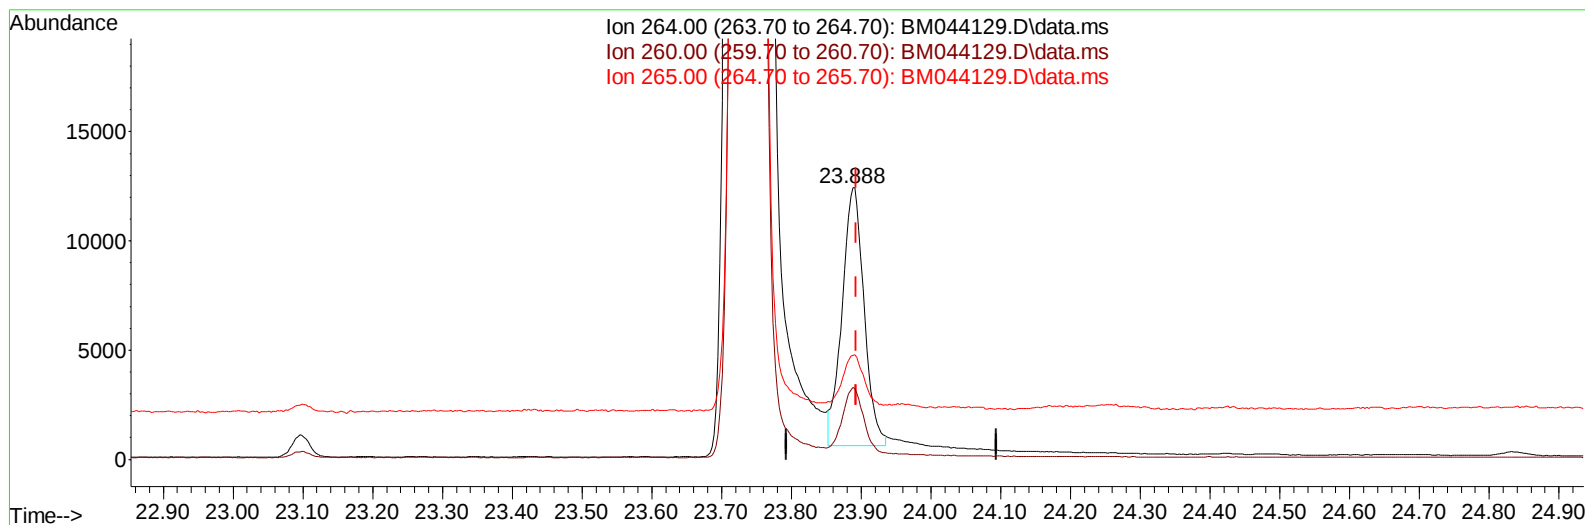

TIC: BM044129.D\data.ms

(23) Perylene-d12 (I)

23.888min (-0.006) 0.40 ng/ul m

response 25917

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.00	26.56
265.00	45.40	38.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

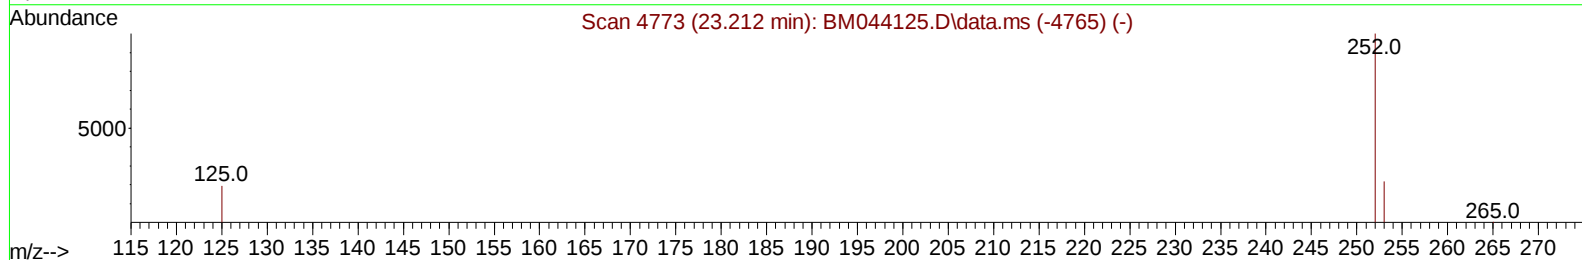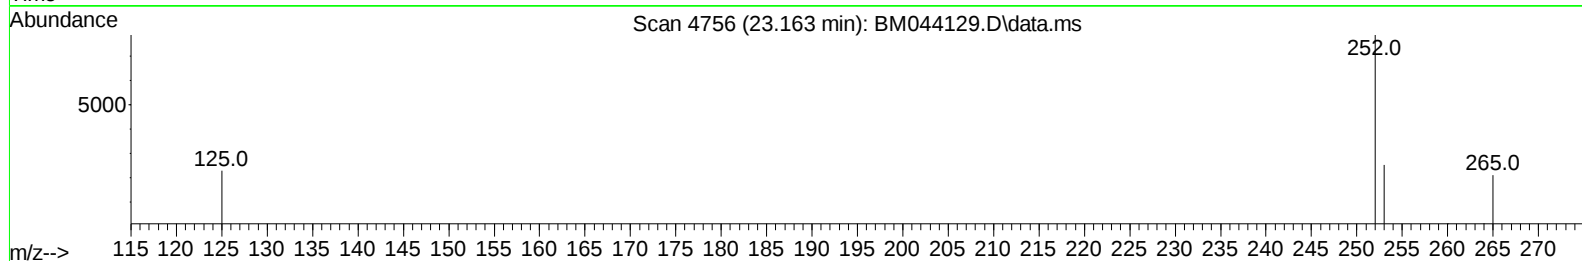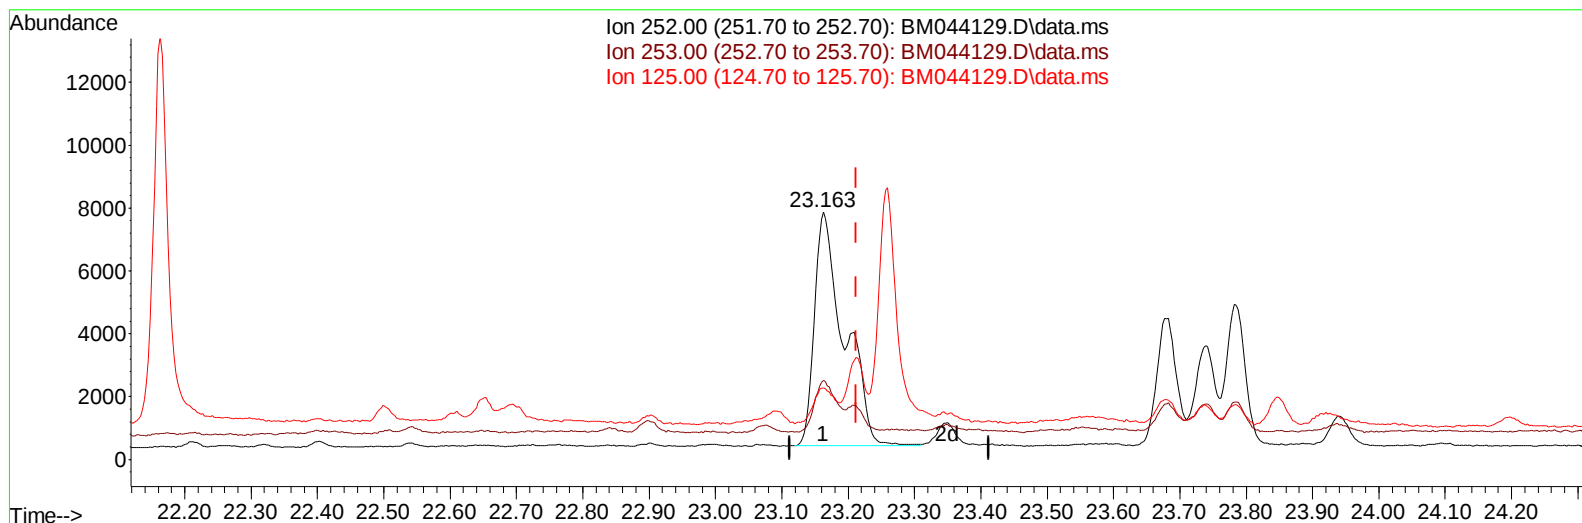

TIC: BM044129.D\data.ms

(25) Benzo(k)fluoranthene

23.163min (-0.050) 0.20 ng/u1

response 23266

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	32.01#
125.00	15.40	28.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

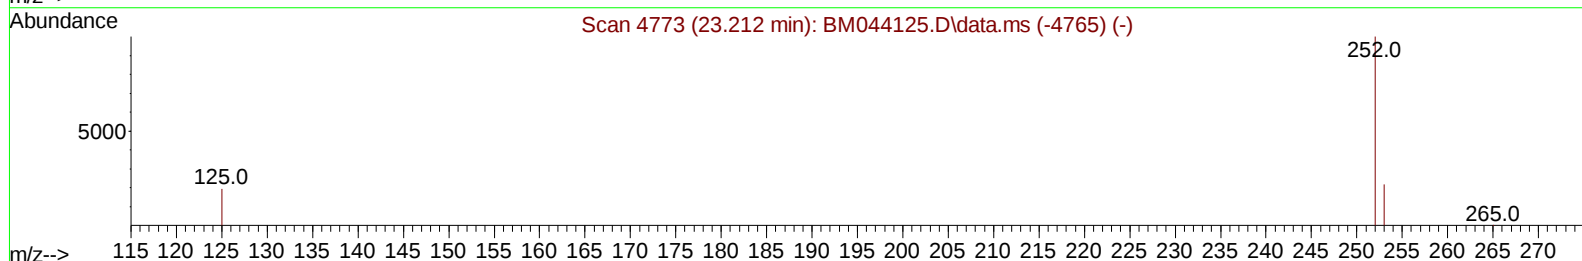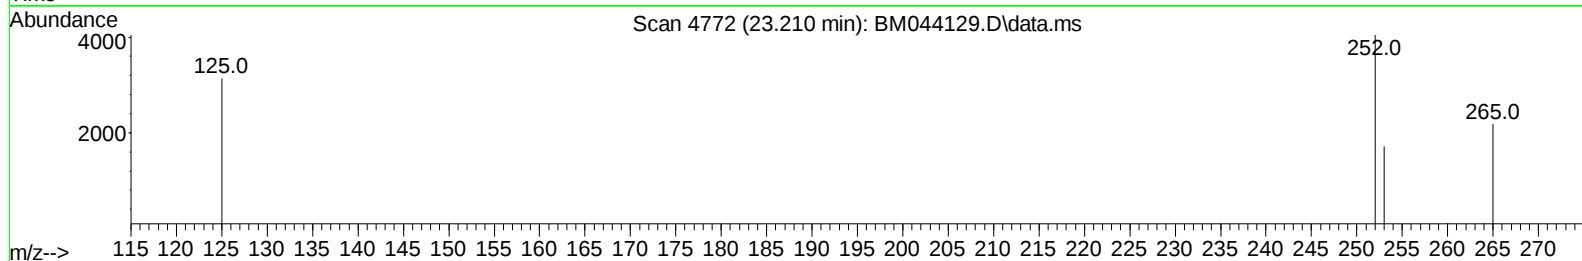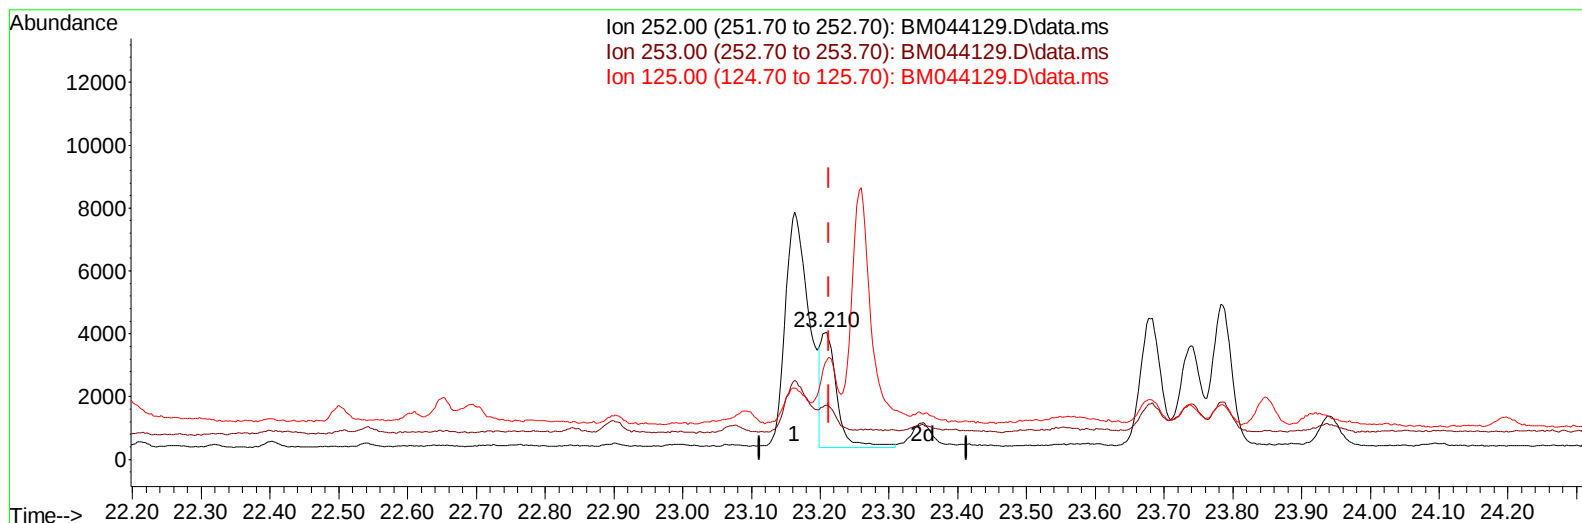

TIC: BM044129.D\data.ms

(25) Benzo(k)fluoranthene

23.210min (-0.003) 0.05 ng/u1 m

response 6052

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	42.39#
125.00	15.40	77.62#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044129.D
 Acq On : 16 Feb 2024 09:05
 Operator : MA/JU
 Sample : P1305-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FP5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/17/2024
 Supervised By :mohammad ahmed 02/19/2024

Quant Time: Feb 16 22:38:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.900	152		11055	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136		37713	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164		19786	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.296	188		41385m	0.400	ng/ul	0.00
17) Chrysene-d12	21.497	240		26590m	0.400	ng/ul	0.00
23) Perylene-d12	23.888	264		25917m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.352	96		75579	4.828	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152		16999	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.331	212		30653m	0.386	ng/ul	0.00
Target Compounds							
						Qvalue	
5) Naphthalene	10.748	128		4651	0.041	ng/ul#	93
7) 2-Methylnaphthalene	12.365	142		4002	0.058	ng/ul	98
8) 1-Methylnaphthalene	12.585	142		1975	0.028	ng/ul	98
14) Pentachlorophenol	16.942	266		441	0.030	ng/ul	96
15) Phenanthrene	17.339	178		19522	0.149	ng/ul	99
19) Fluoranthene	19.359	202		31190m	0.257	ng/ul	
20) Pyrene	19.726	202		25903m	0.203	ng/ul	
21) Benzo(a)anthracene	21.479	228		9825m	0.081	ng/ul	
22) Chrysene	21.535	228		18130m	0.138	ng/ul	
24) Benzo(b)fluoranthene	23.163	252		17663	0.165	ng/ul#	78
25) Benzo(k)fluoranthene	23.210	252		6052m	0.052	ng/ul	
26) Benzo(a)pyrene	23.783	252		8364	0.084	ng/ul#	71
27) Indeno(1,2,3-cd)pyrene	26.363	276		6432	0.051	ng/ul#	97
29) Benzo(g,h,i)perylene	27.128	276		6693	0.060	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044129.D
Acq On : 16 Feb 2024 09:05
Operator : MA/JU
Sample : P1305-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FP5

Manual IntegrationsAPPROVED

Quant Time: Feb 16 22:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

