




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044169.D
Acq On : 17 Feb 2024 10:30
Operator : MA/JU
Sample : PB159059BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK059

Manual IntegrationsAPPROVED

Quant Time: Feb 18 23:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/19/2024
Supervised By :mohammad ahmed 02/19/2024

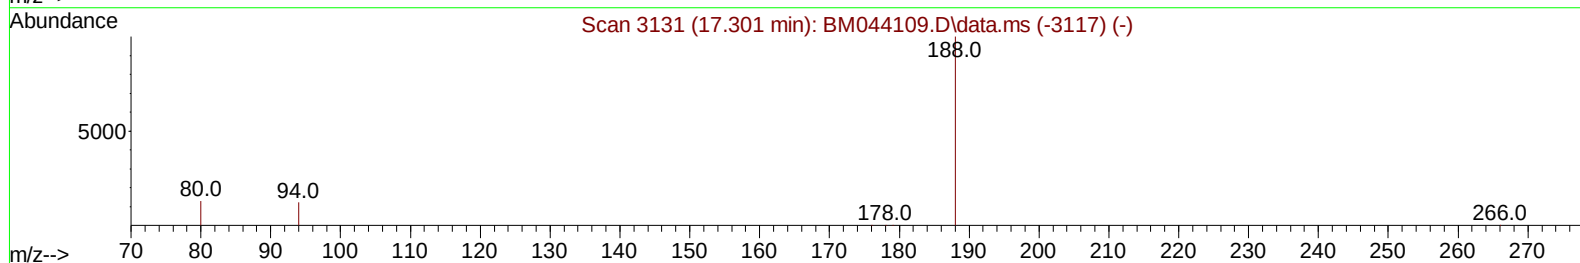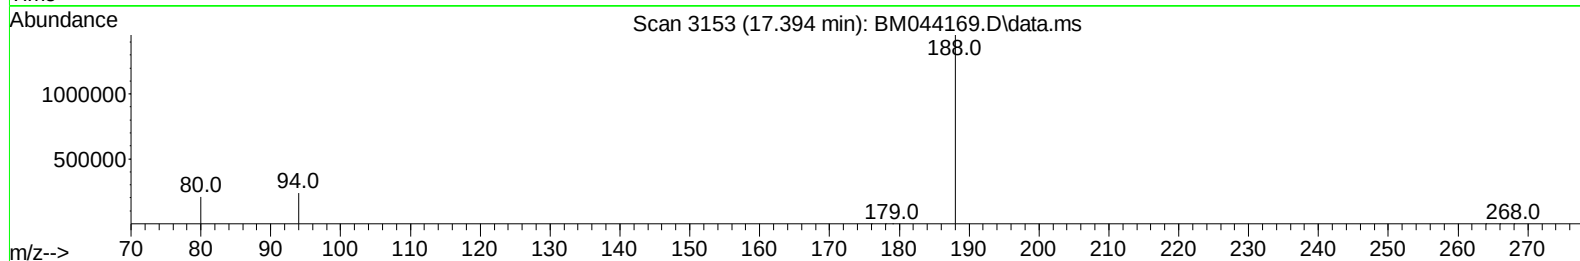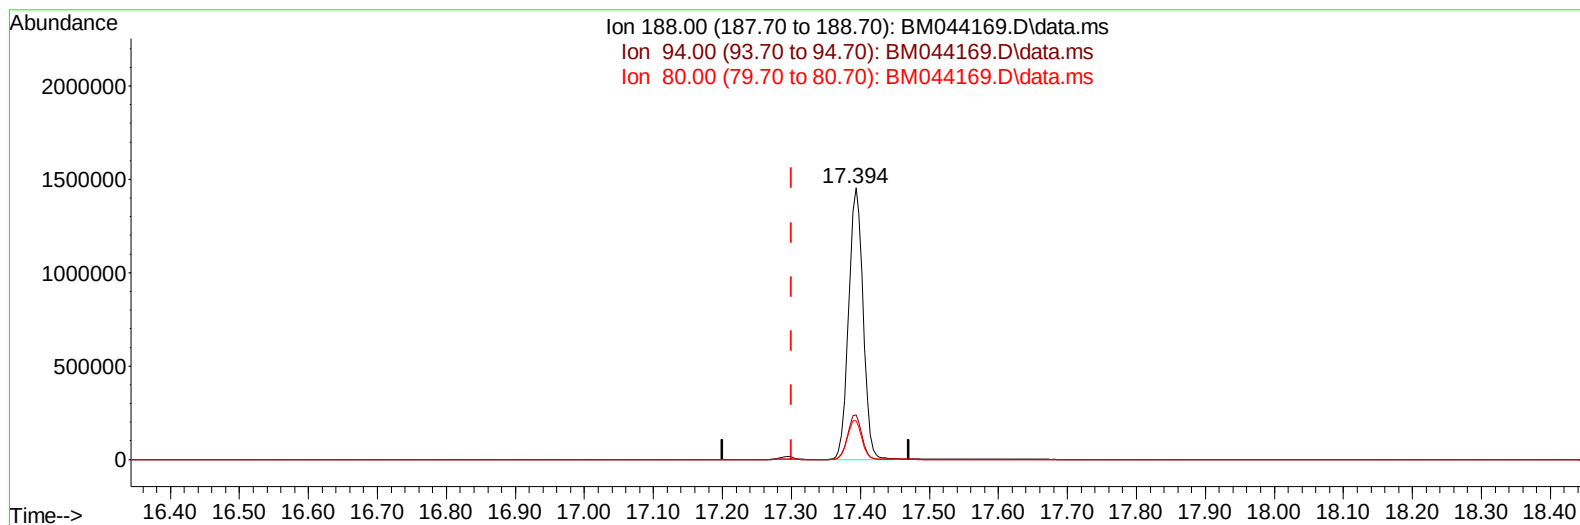

TIC: BM044169.D\data.ms

(13) Phenanthrene-d10 (I)

17.394min (+ 0.093) 0.40 ng/u1

response 2132722

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	16.33#
80.00	13.40	14.32
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044169.D
Acq On : 17 Feb 2024 10:30
Operator : MA/JU
Sample : PB159059BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK059

Manual IntegrationsAPPROVED

Quant Time: Feb 18 23:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/19/2024
Supervised By :mohammad ahmed 02/19/2024

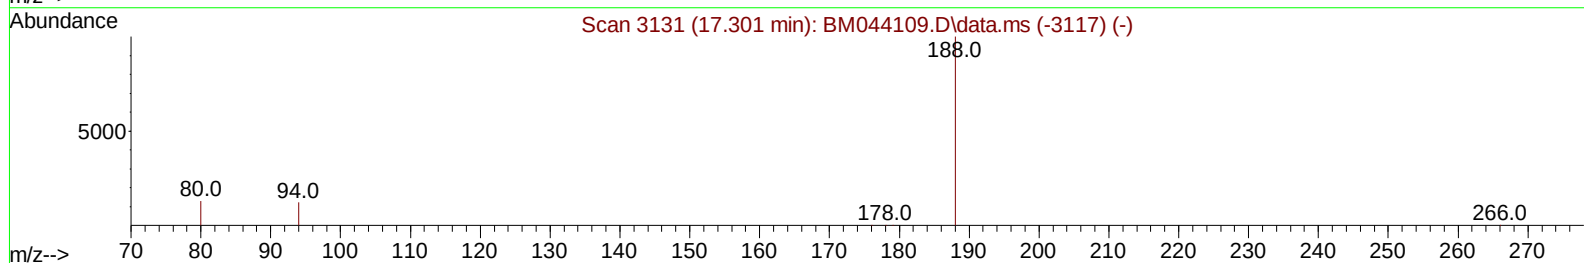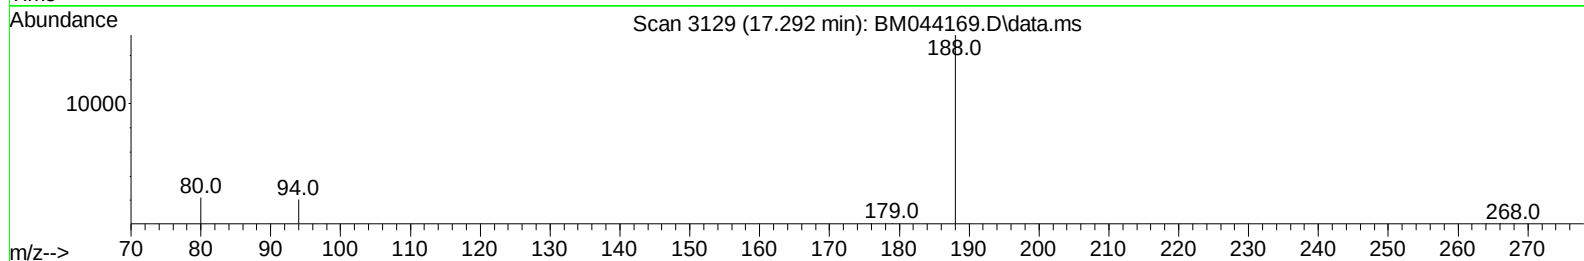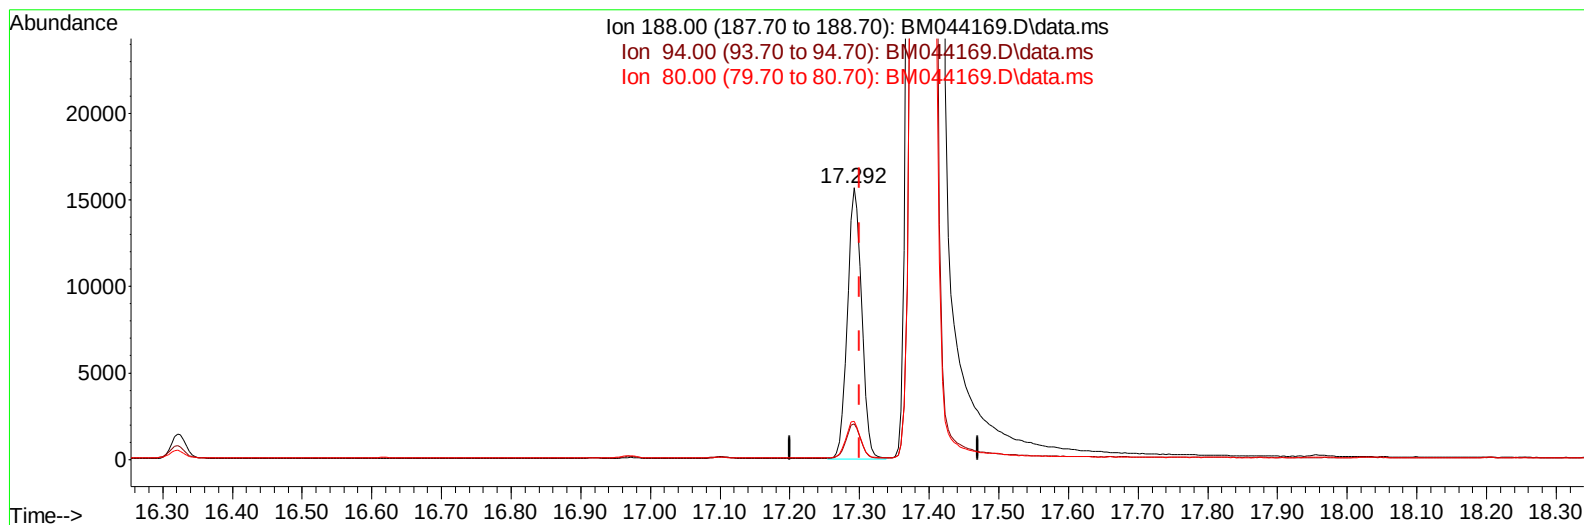

TIC: BM044169.D\data.ms

(13) Phenanthrene-d10 (I)

17.292min (-0.008) 0.40 ng/ul m

response 22218

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	13.13
80.00	13.40	14.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044169.D
Acq On : 17 Feb 2024 10:30
Operator : MA/JU
Sample : PB159059BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK059

Manual IntegrationsAPPROVED

Quant Time: Feb 18 23:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/19/2024
Supervised By :mohammad ahmed 02/19/2024

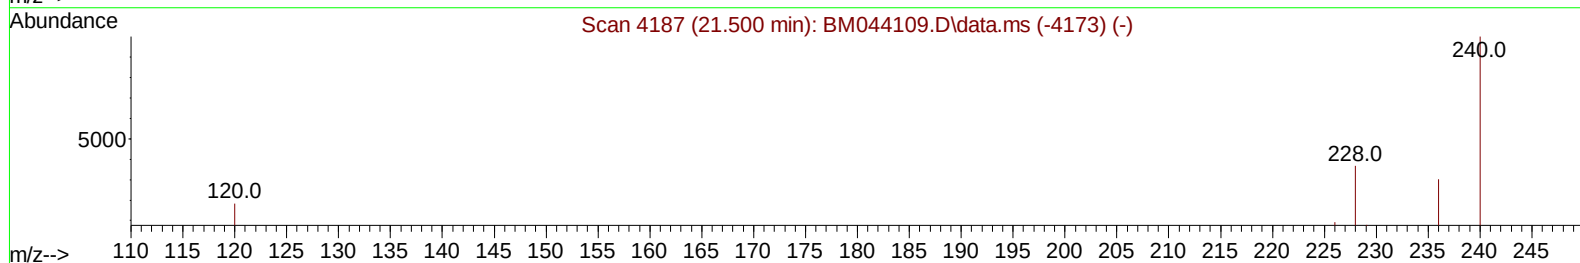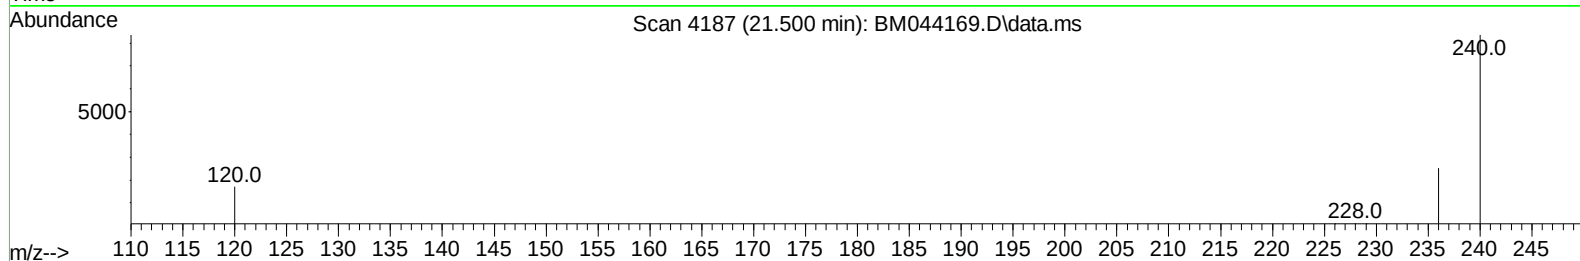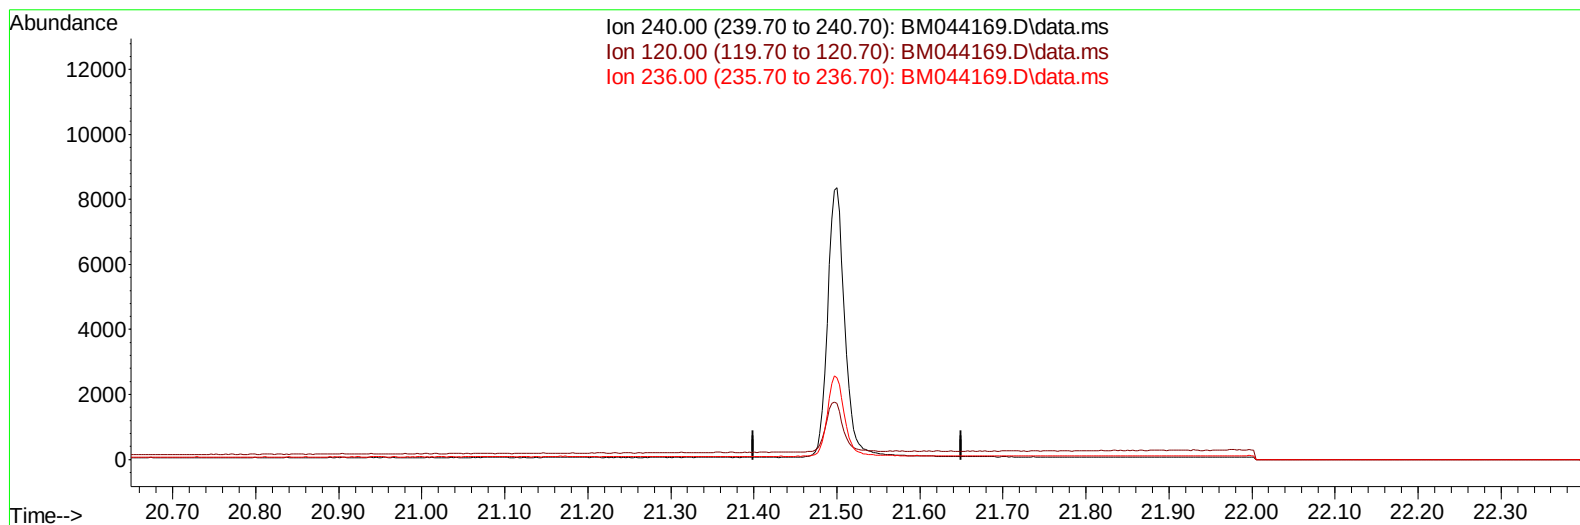

TIC: BM044169.D\data.ms

(17) Chrysene-d12

21.500min (-21.500) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.50	0.00#
236.00	30.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044169.D
Acq On : 17 Feb 2024 10:30
Operator : MA/JU
Sample : PB159059BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK059

Manual IntegrationsAPPROVED

Quant Time: Feb 18 23:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/19/2024
Supervised By :mohammad ahmed 02/19/2024

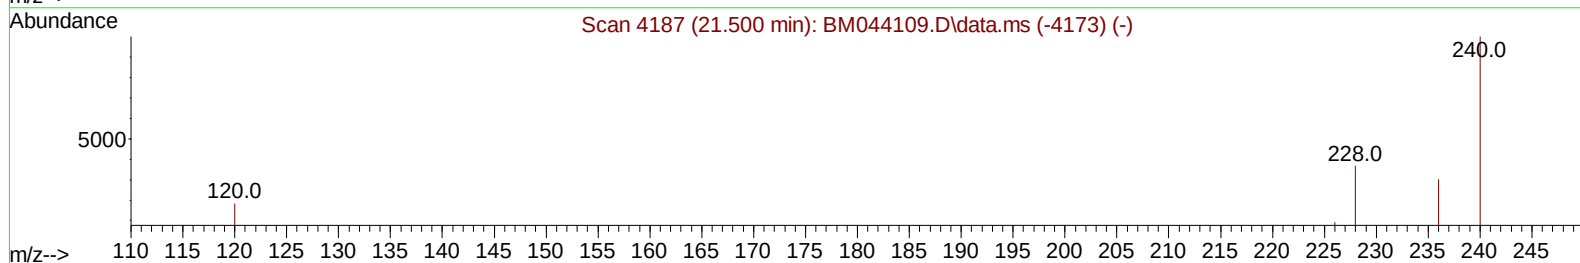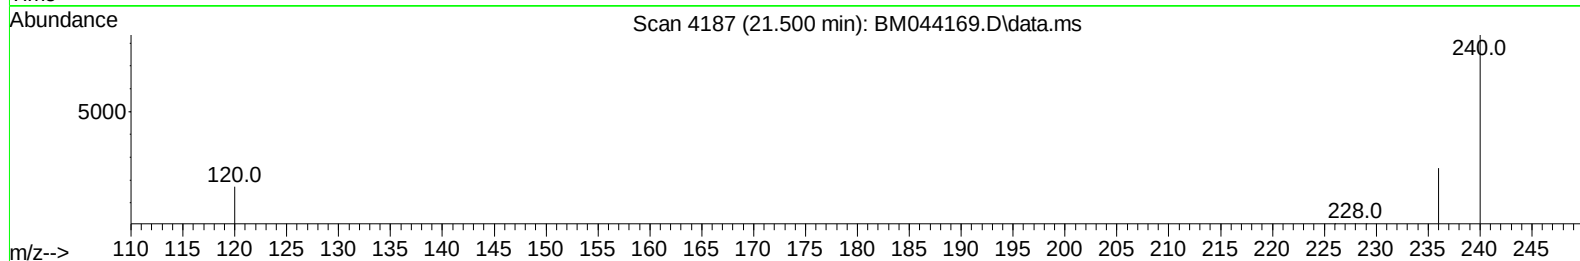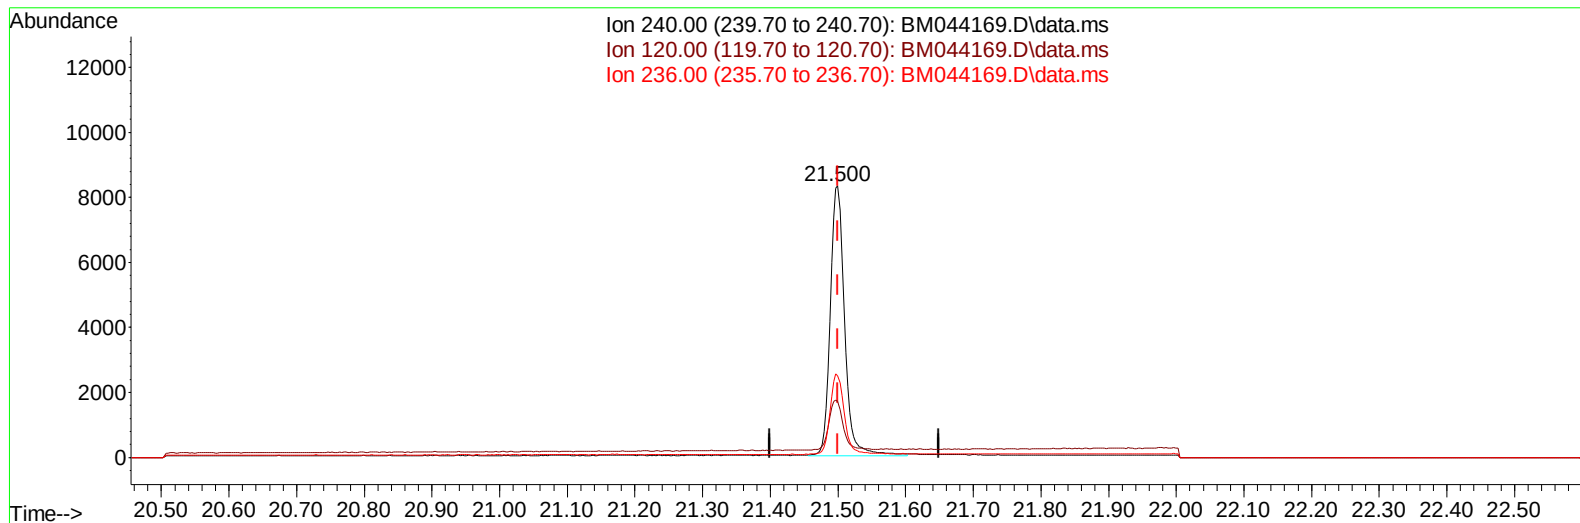

TIC: BM044169.D\data.ms

(17) Chrysene-d12

21.500min (+ 0.000) 0.40 ng/ul m

response 12105

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.50	20.62
236.00	30.60	30.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044169.D
 Acq On : 17 Feb 2024 10:30
 Operator : MA/JU
 Sample : PB159059BL
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK059

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/19/2024
 Supervised By :mohammad ahmed 02/19/2024

Quant Time: Feb 18 23:56:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	6201	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	20350	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	10812	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	22218m	0.400	ng/ul	0.00
17) Chrysene-d12	21.500	240	12105m	0.400	ng/ul	0.00
23) Perylene-d12	23.885	264	16521	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	71103	8.097	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	13291	0.466	ng/ul	0.00
18) Fluoranthene-d10	19.326	212	22901	0.634	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044169.D
Acq On : 17 Feb 2024 10:30
Operator : MA/JU
Sample : PB159059BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK059

Manual IntegrationsAPPROVED

Quant Time: Feb 18 23:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/19/2024
Supervised By :mohammad ahmed 02/19/2024

