

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044111.D
 Acq On : 15 Feb 2024 21:35
 Operator : MA/JU
 Sample : P1329-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FL7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/17/2024
 Supervised By :mohammad ahmed 02/19/2024

Quant Time: Feb 17 02:23:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	8155	0.400	ng/u1	0.00
4) Naphthalene-d8	10.699	136	25707	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.543	164	13152	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.297	188	27290m	0.400	ng/u1	0.00
17) Chrysene-d12	21.499	240	16185m	0.400	ng/u1	0.00
23) Perylene-d12	23.887	264	15408m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	64124	5.553	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.294	152	11949	0.332	ng/u1	0.00
18) Fluoranthene-d10	19.332	212	21488m	0.445	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.938	266	300	0.031	ng/u1	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044111.D
Acq On : 15 Feb 2024 21:35
Operator : MA/JU
Sample : P1329-08
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0FL7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024


Quant Time: Feb 17 02:23:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

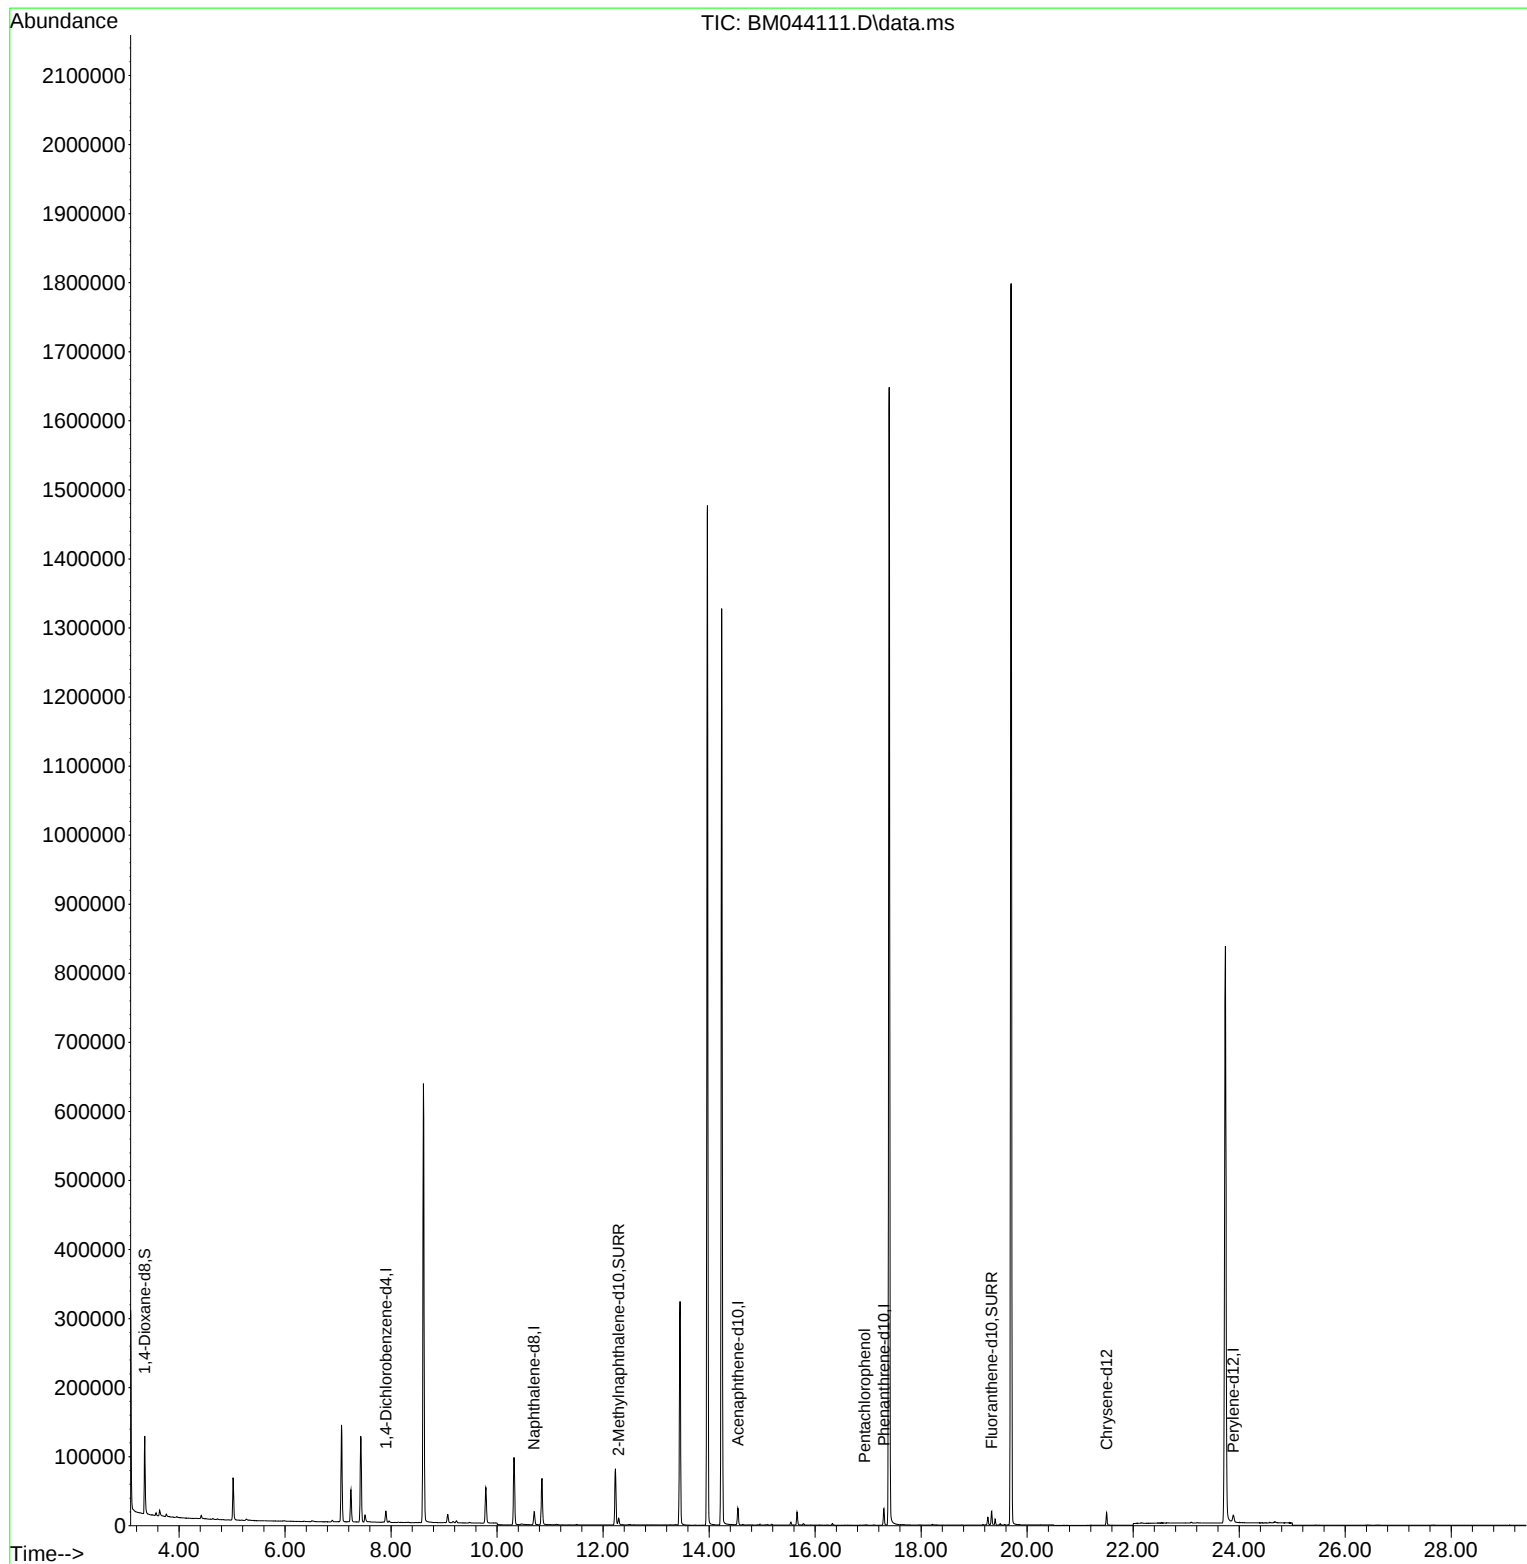

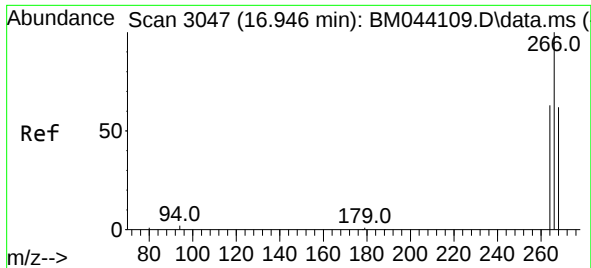

#14
Pentachlorophenol
Concen: 0.031 ng/ul
RT: 16.938 min Scan# 3045
Delta R.T. -0.008 min
Lab File: BM044111.D
Acq: 15 Feb 2024 21:35

Instrument :
BNA_M
ClientSampleId :
C0FL7

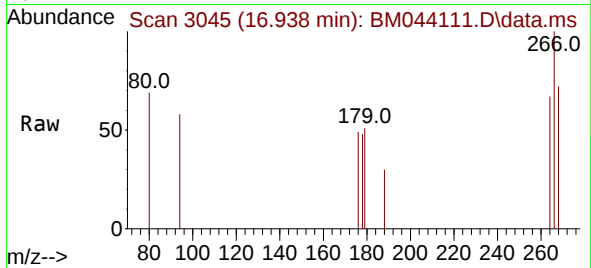

Tgt Ion:266 Resp: 300
Ion Ratio Lower Upper
266 100
264 70.7 49.4 74.0
268 66.0 52.1 78.1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

