

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044132.D
 Acq On : 16 Feb 2024 10:55
 Operator : MA/JU
 Sample : P1305-07
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FP9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/17/2024
 Supervised By :mohammad ahmed 02/19/2024

Quant Time: Feb 16 22:38:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	8795	0.400	ng/u1	0.00
4) Naphthalene-d8	10.699	136	30291	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.542	164	16497	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.296	188	34469m	0.400	ng/u1	0.00
17) Chrysene-d12	21.497	240	22544m	0.400	ng/u1	0.00
23) Perylene-d12	23.888	264	25988	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	71576	5.747	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.294	152	16859	0.397	ng/u1	0.00
18) Fluoranthene-d10	19.331	212	32436	0.482	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.942	266	450	0.036	ng/u1	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044132.D
Acq On : 16 Feb 2024 10:55
Operator : MA/JU
Sample : P1305-07
Misc :
ALS Vial : 42 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0FP9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024


Quant Time: Feb 16 22:38:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

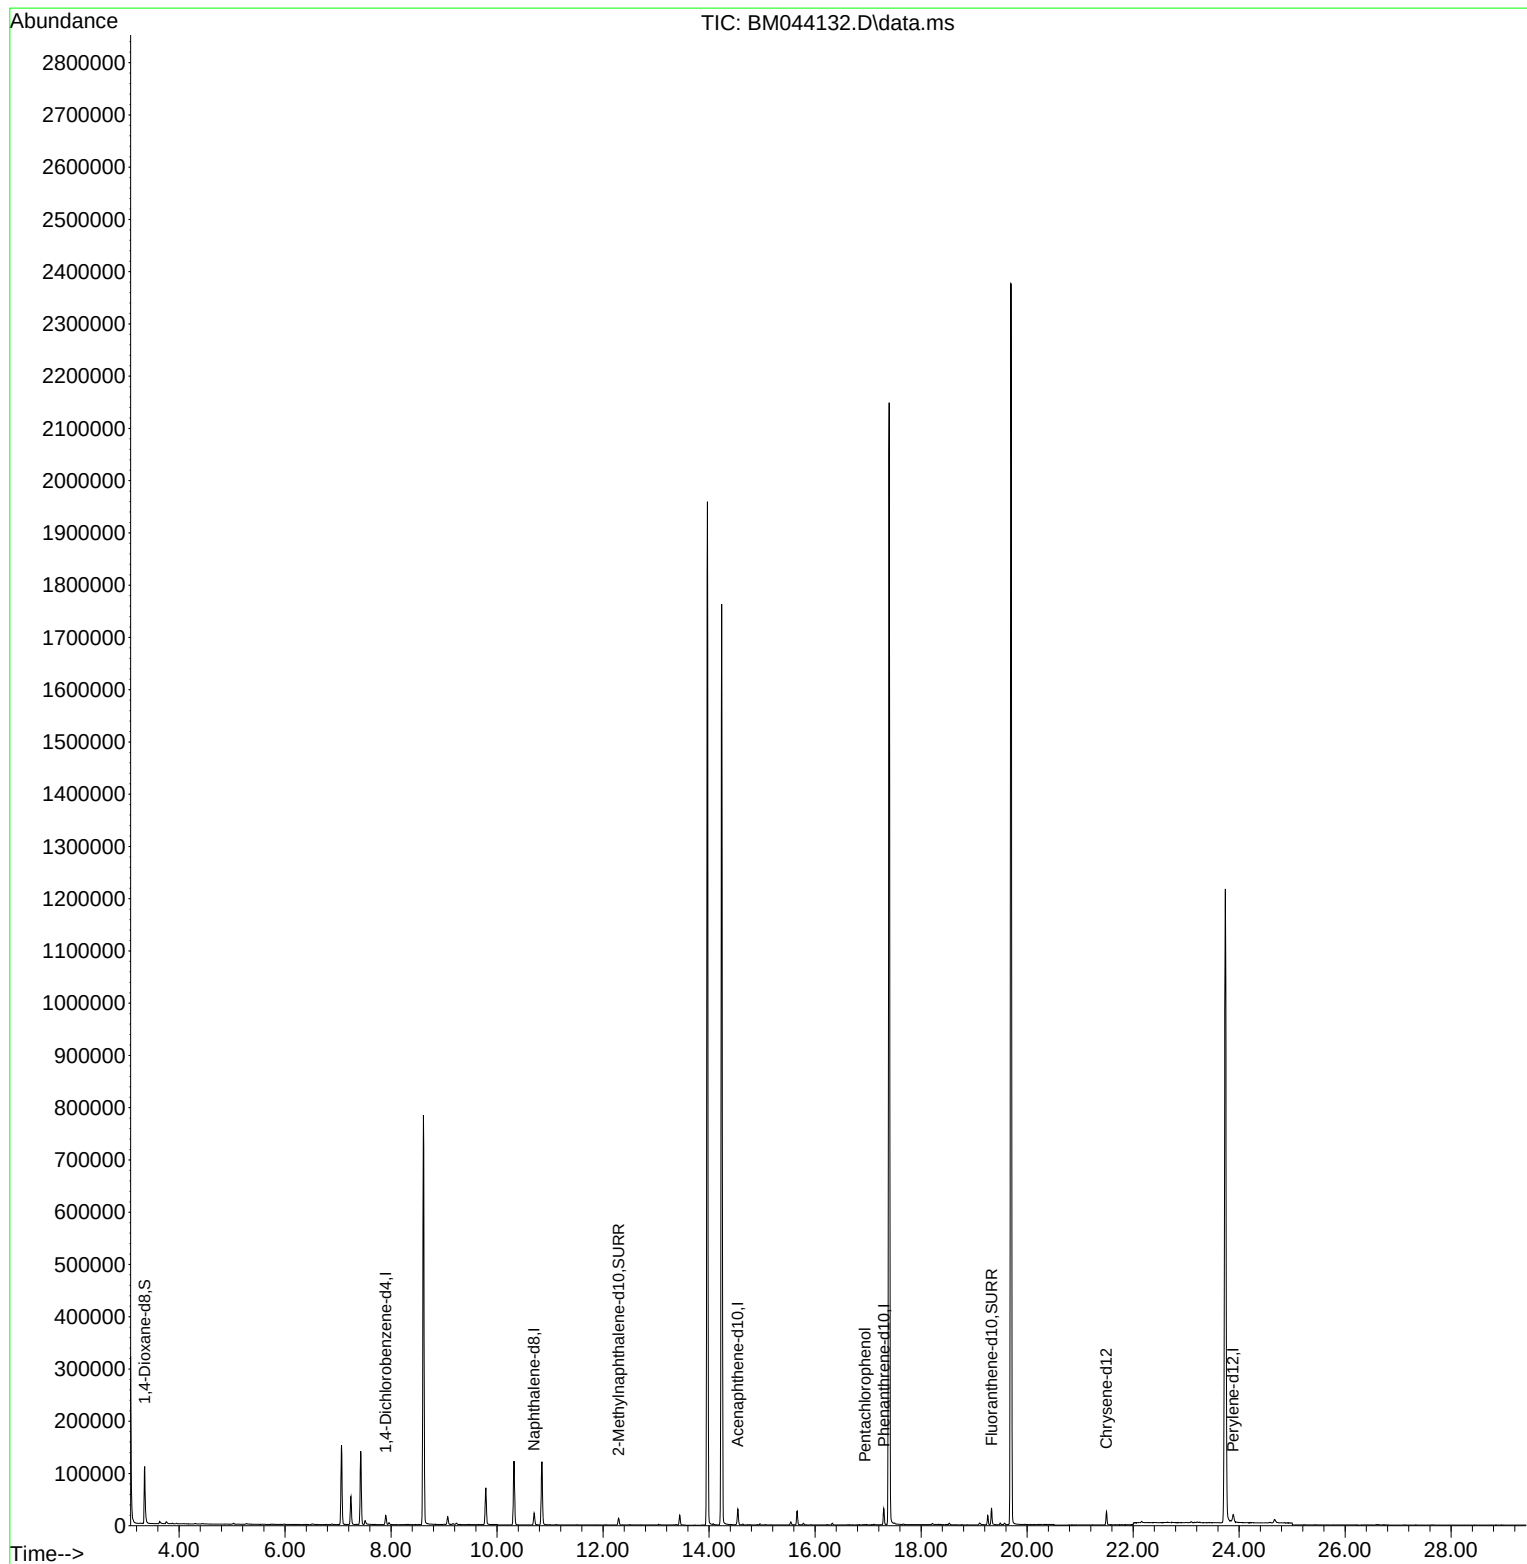

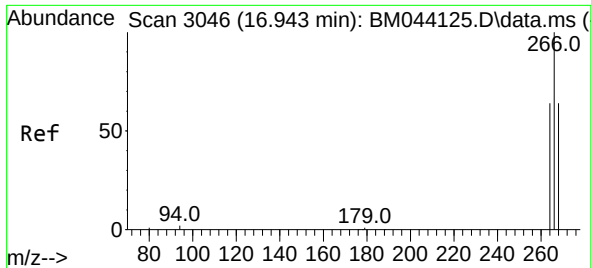

#14
 Pentachlorophenol
 Concen: 0.036 ng/ul
 RT: 16.942 min Scan# 3046
 Delta R.T. -0.004 min
 Lab File: BM044132.D
 Acq: 16 Feb 2024 10:55

Instrument :
 BNA_M
 ClientSampleId :
 C0FP9

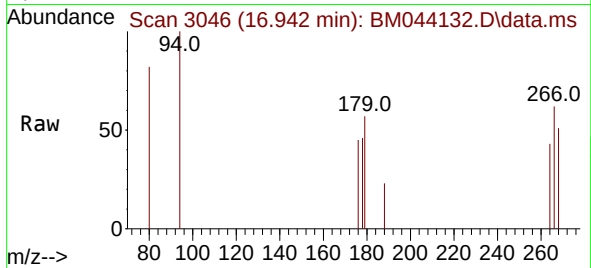

Tgt Ion:	266	Resp:	450
Ion	Ratio	Lower	Upper
266	100		
264	63.6	49.4	74.0
268	56.7	52.1	78.1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/17/2024
 Supervised By :mohammad ahmed 02/19/2024

