

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044155.D
 Acq On : 17 Feb 2024 01:27
 Operator : MA/JU
 Sample : P1402-08
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/17/2024
 Supervised By :mohammad ahmed 02/19/2024

Quant Time: Feb 17 02:08:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	8026	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	26185	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	13616	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	28169m	0.400	ng/ul	0.00
17) Chrysene-d12	21.494	240	16217m	0.400	ng/ul	0.00
23) Perylene-d12	23.885	264	19530	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	42009	3.696	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	13987	0.381	ng/ul	0.00
18) Fluoranthene-d10	19.326	212	30110	0.622	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.386	88	132531	11.666	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044155.D
Acq On : 17 Feb 2024 01:27
Operator : MA/JU
Sample : P1402-08
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC3


Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

Quant Time: Feb 17 02:08:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

02/17/2024
Supervised By :mohammad
ahmed


02/19/2024

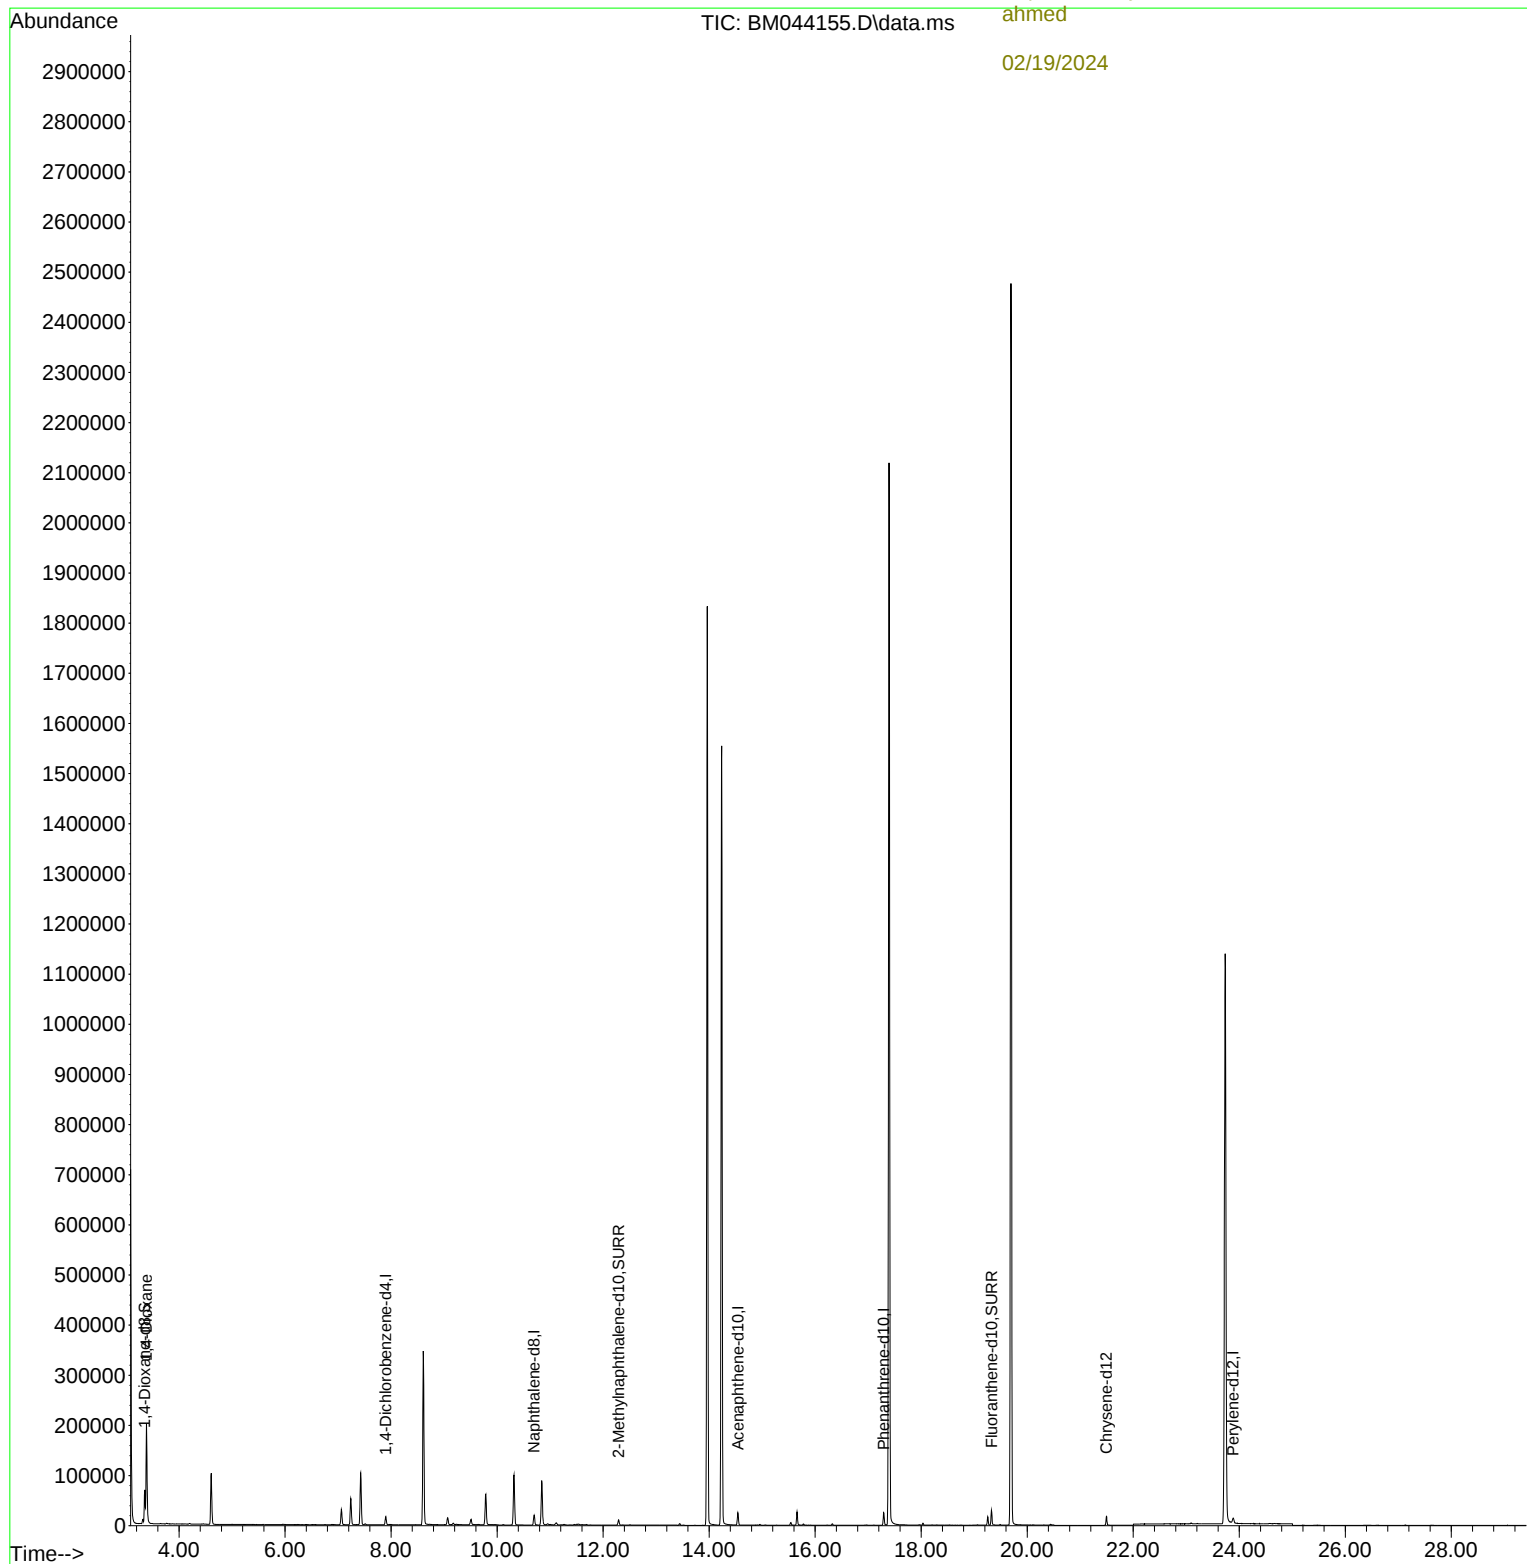

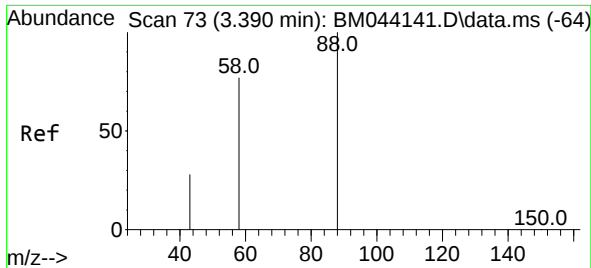

#2
1,4-Dioxane
Concen: 11.666 ng/ul
RT: 3.386 min Scan# 71
Delta R.T. -0.004 min
Lab File: BM044155.D
Acq: 17 Feb 2024 01:27



Instrument :
BNA_M
ClientSampleId :
C0AC3

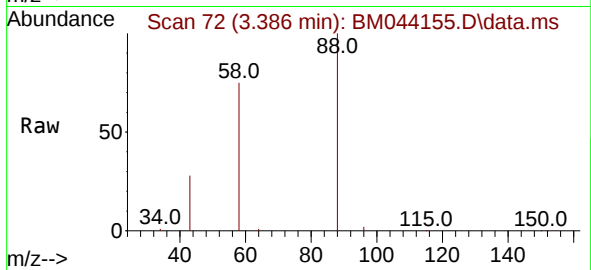

Tgt Ion: 88 Resp: 13253
Ion Ratio Lower Upper
88 100
43 28.3 32.2 48.2
58 74.9 40.6 60.8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/17/2024
Supervised By :mohammad ahmed 02/19/2024

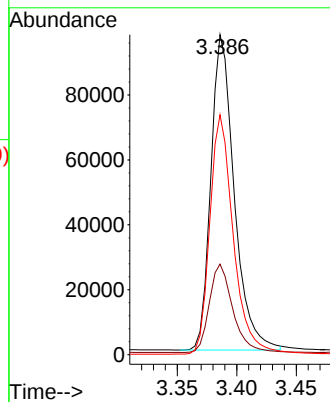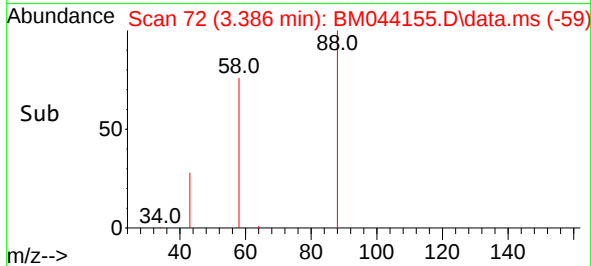

02/17/2024
Supervised By :mohammad
ahmed

02/19/2024